

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
 Data File : PL071352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2021 14:23
 Operator : AR\AJ
 Sample : M4953-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:55:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.499	5652751	14979490	12.035	11.937
28)	SA Decachlor...	10.328	11.391	2113754	3507817	2.919	2.524
Target Compounds							
10)	B gamma-Chl...	7.281	0.000	153690	0	0.242	N.D. #
14)	MA Endrin	8.008f	8.878	422756	1568269	0.748	1.169 #
15)	B Endosulfa...	0.000	9.149f	0	2042646	N.D.	1.516 #
17)	MA 4,4'-DDT	0.000	9.382f	0	3008805	N.D.	2.163 #
23)	Chlordane-1	5.897	0.000	255017	0	15.167	N.D. #
25)	Chlordane-3	7.281	0.000	153690	0	2.478	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
Data File : PL071352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2021 14:23
Operator : AR\AJ
Sample : M4953-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:55:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

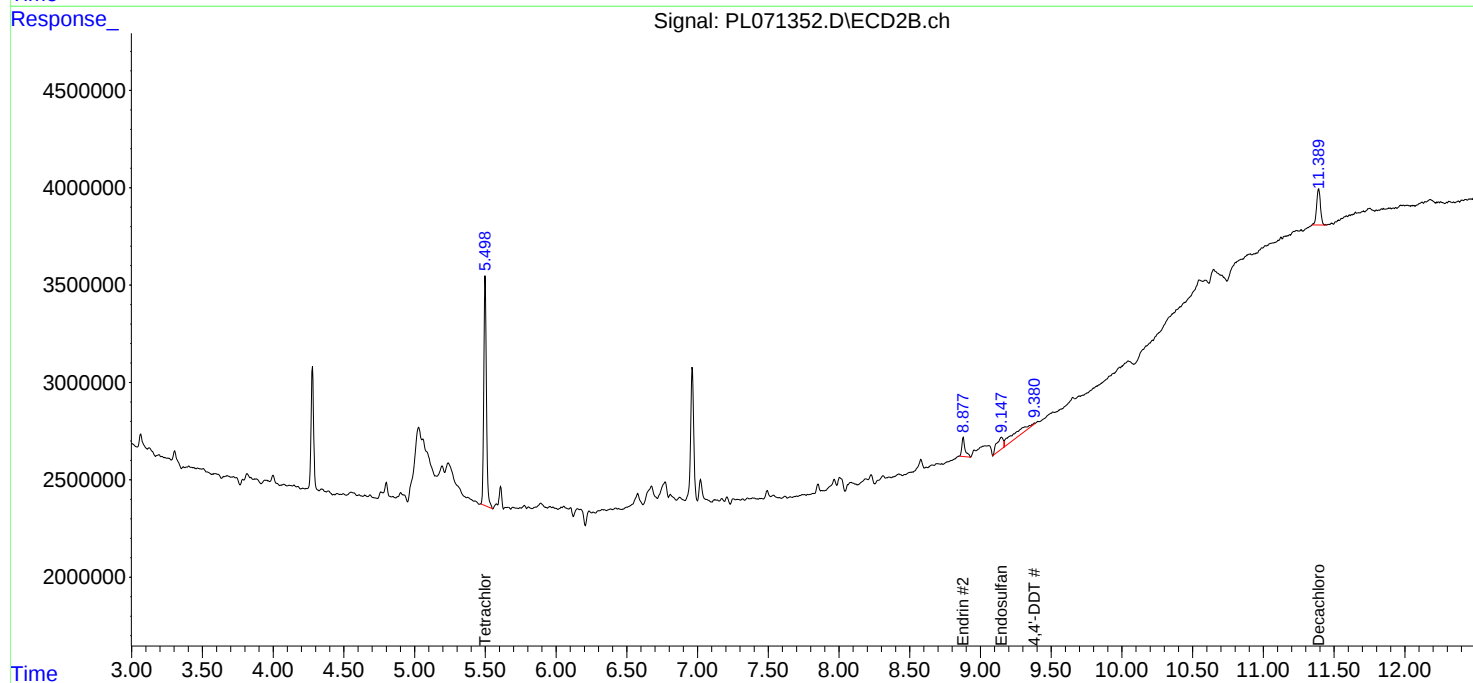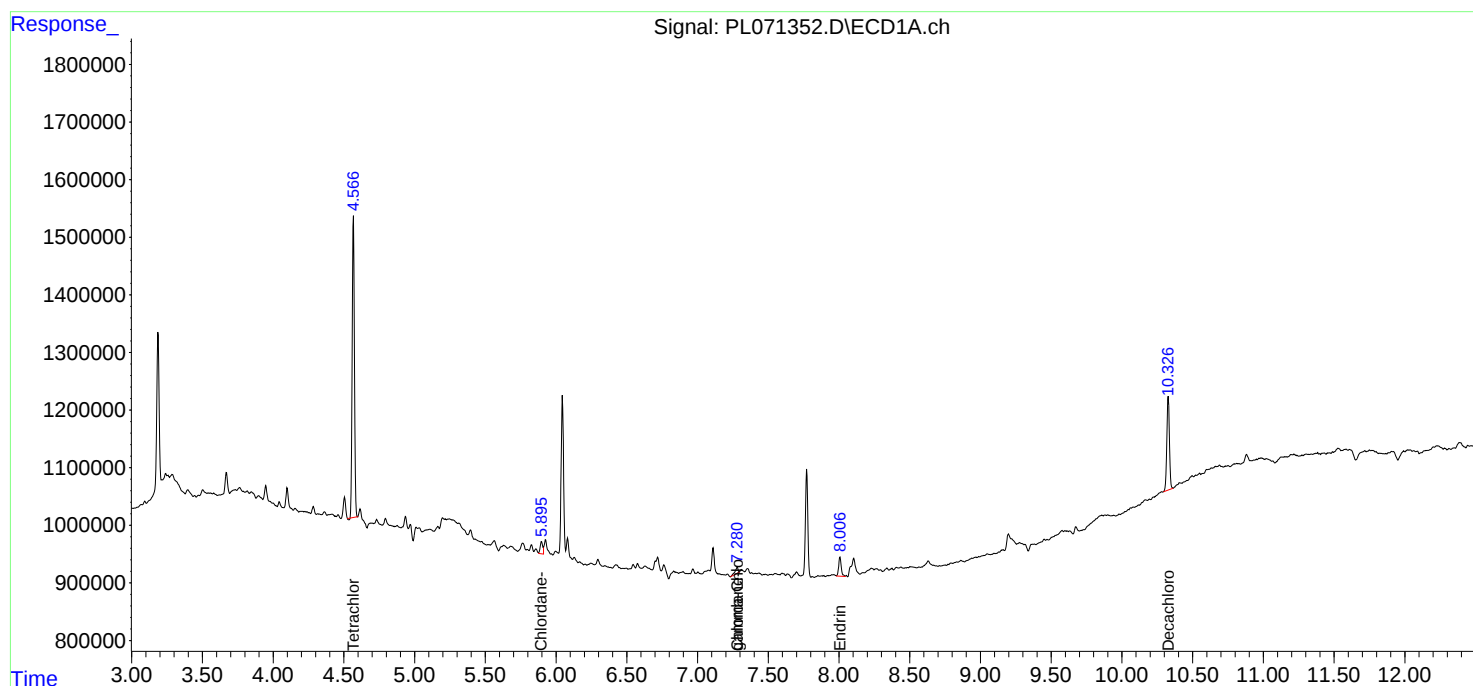


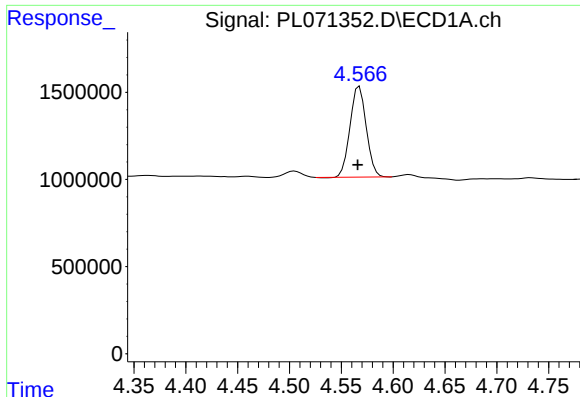

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.001 min
Response: 5652751
Conc: 12.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

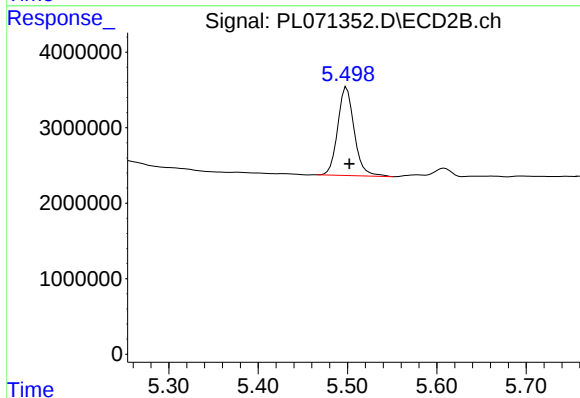


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 14979490
Conc: 11.94 ng/ml

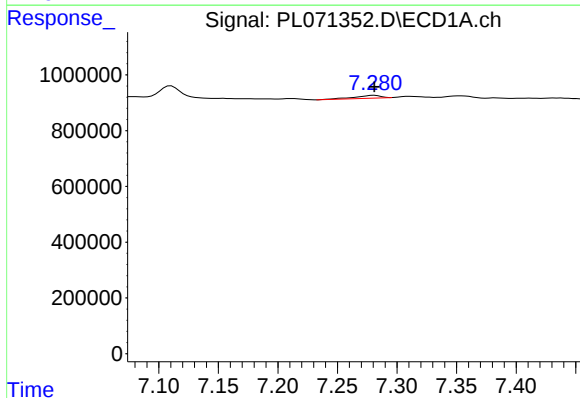


#10 gamma-Chlordane

R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 153690
Conc: 0.24 ng/ml

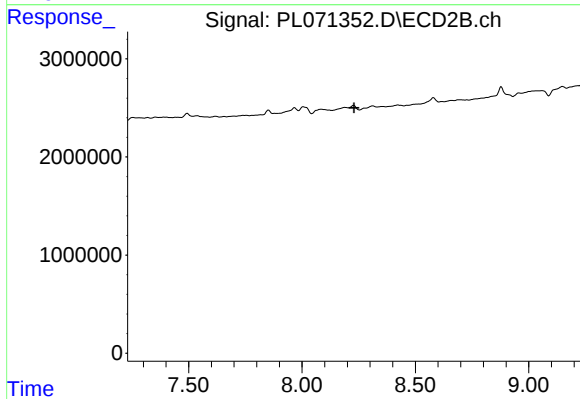

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

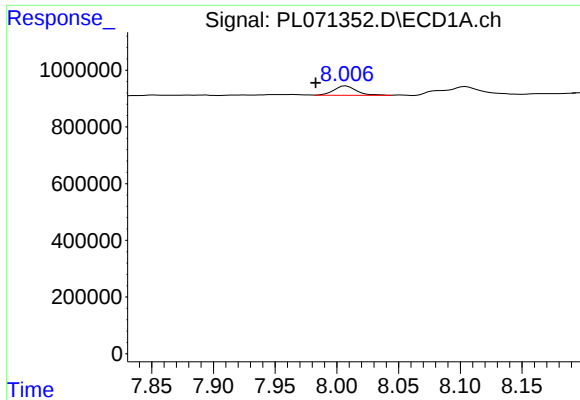

#14 Endrin


R.T.: 8.008 min
Delta R.T.: 0.025 min
Response: 422756
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

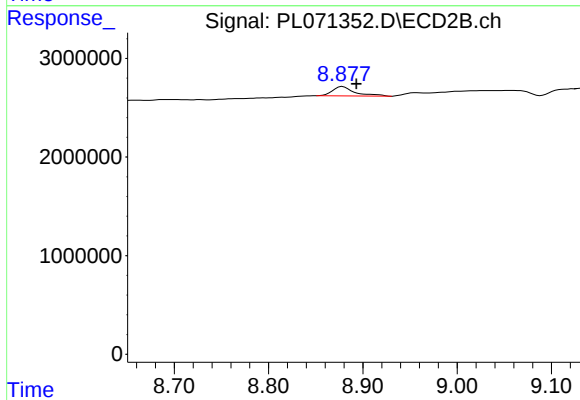


#14 Endrin

R.T.: 8.878 min
Delta R.T.: -0.015 min
Response: 1568269
Conc: 1.17 ng/ml

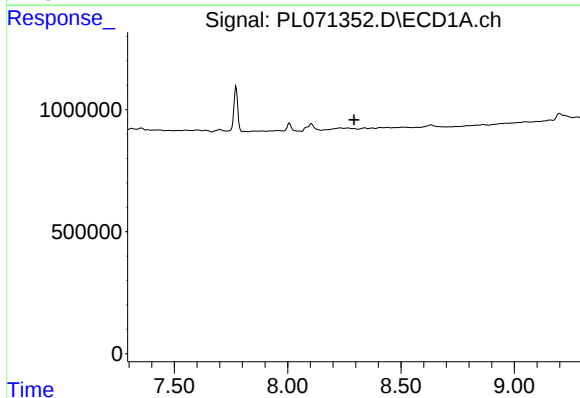


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.293 min
Response: 0
Conc: N.D.

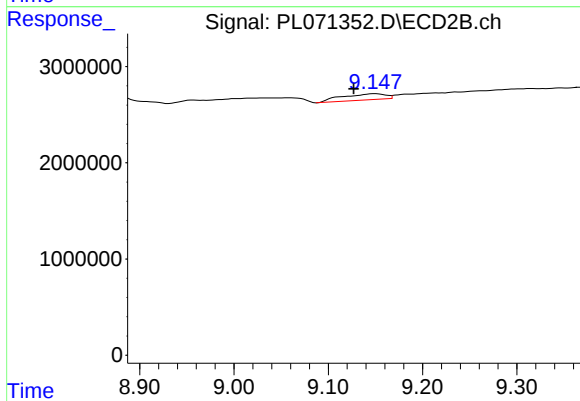

#15 Endosulfan II


R.T.: 9.149 min
Delta R.T.: 0.022 min
Response: 2042646
Conc: 1.52 ng/ml

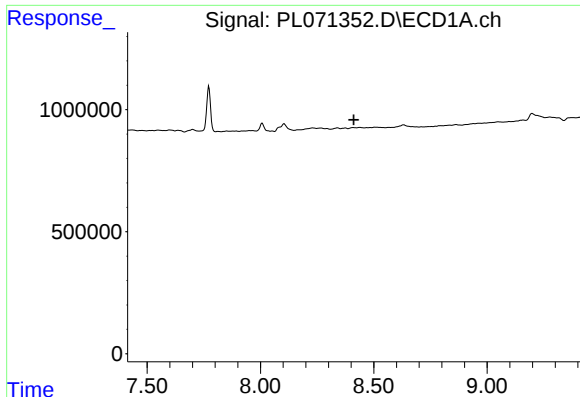

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

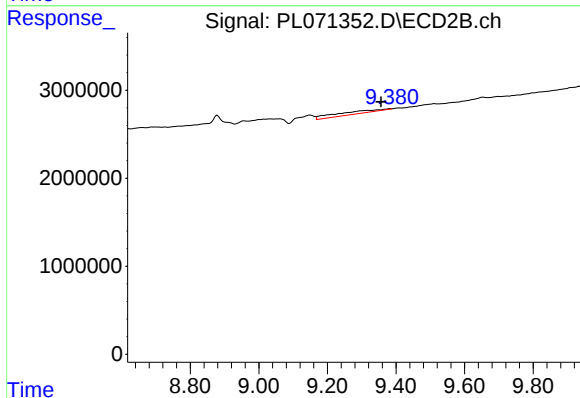


#17 4,4'-DDT

R.T.: 9.382 min
Delta R.T.: 0.026 min
Response: 3008805
Conc: 2.16 ng/ml

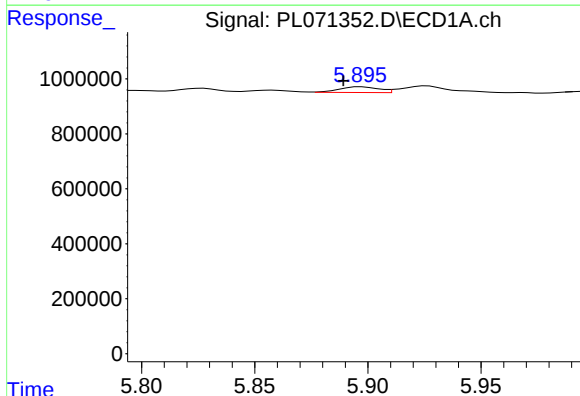


#23 Chlordane-1

R.T.: 5.897 min
Delta R.T.: 0.008 min
Response: 255017
Conc: 15.17 ng/ml

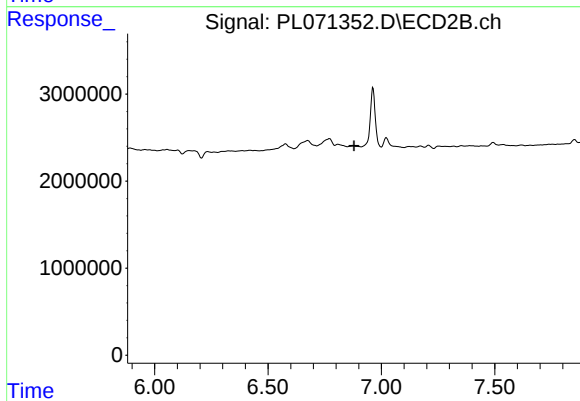

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 6.880 min
Response: 0
Conc: N.D.

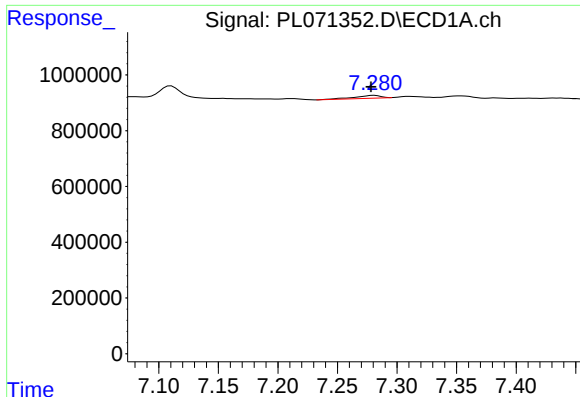

#25 Chlordane-3


R.T.: 7.281 min
Delta R.T.: 0.003 min
Response: 153690
Conc: 2.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

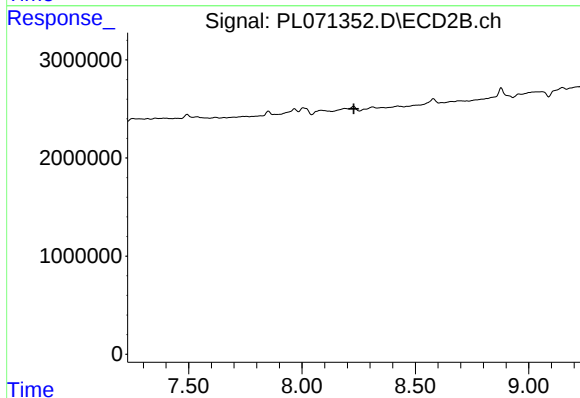


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

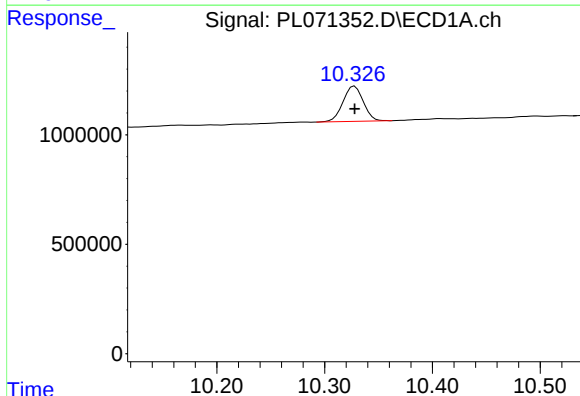

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 2113754
Conc: 2.92 ng/ml

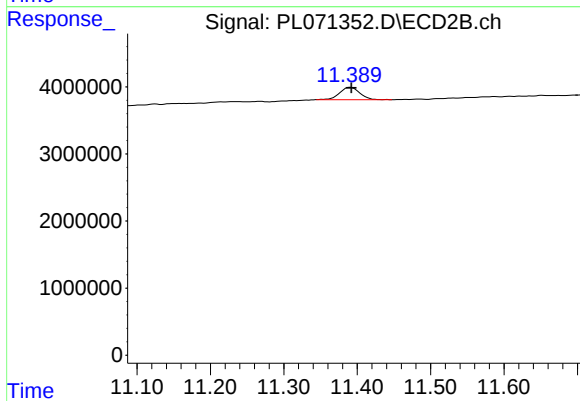

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: -0.001 min
Response: 3507817
Conc: 2.52 ng/ml