

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
 Data File : PL071358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2021 21:06
 Operator : AR\AJ
 Sample : M4967-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:42:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.562	5.499	10818765	26962010	23.034	21.485
28)	SA Decachlor...	10.323	11.388	12086418	20056707	16.692	14.429
Target Compounds							
12)	B 4,4'-DDE	7.560	8.497	329903	665760	0.583	0.432 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
Data File : PL071358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2021 21:06
Operator : AR\AJ
Sample : M4967-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:42:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

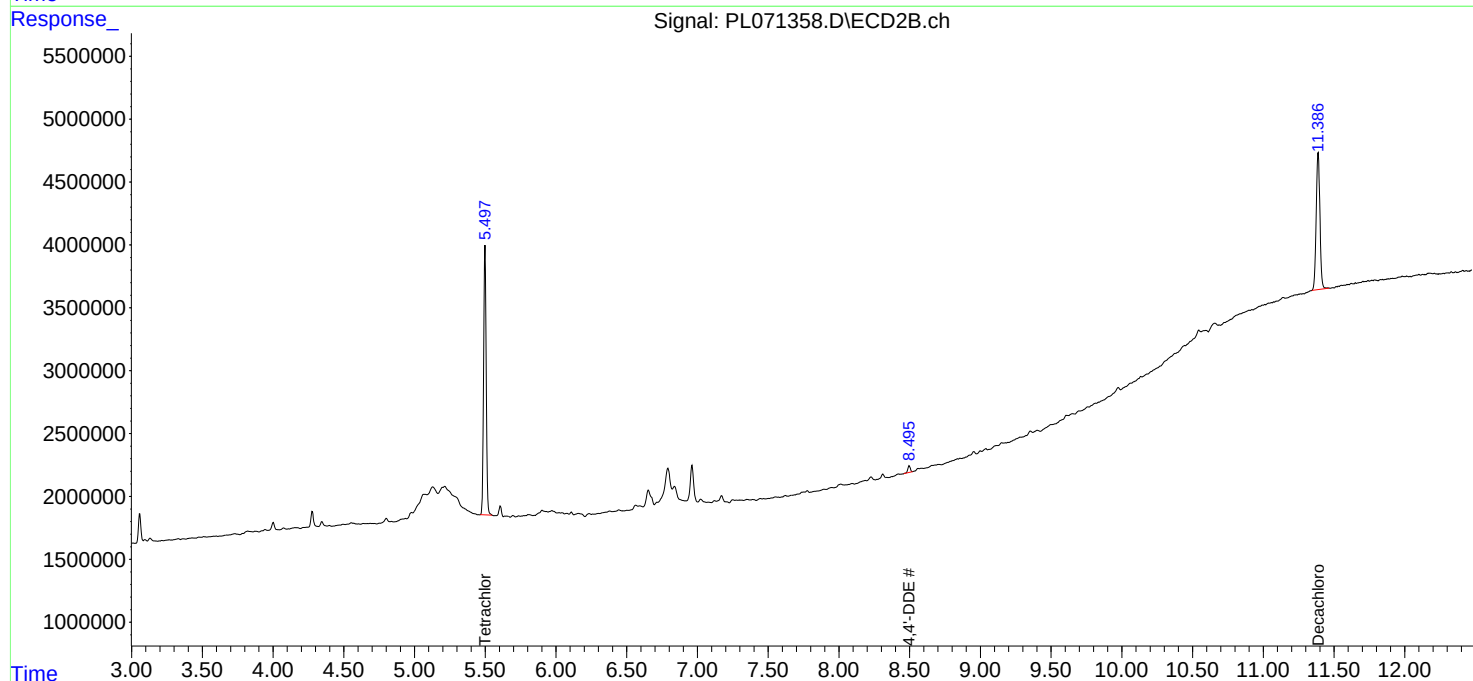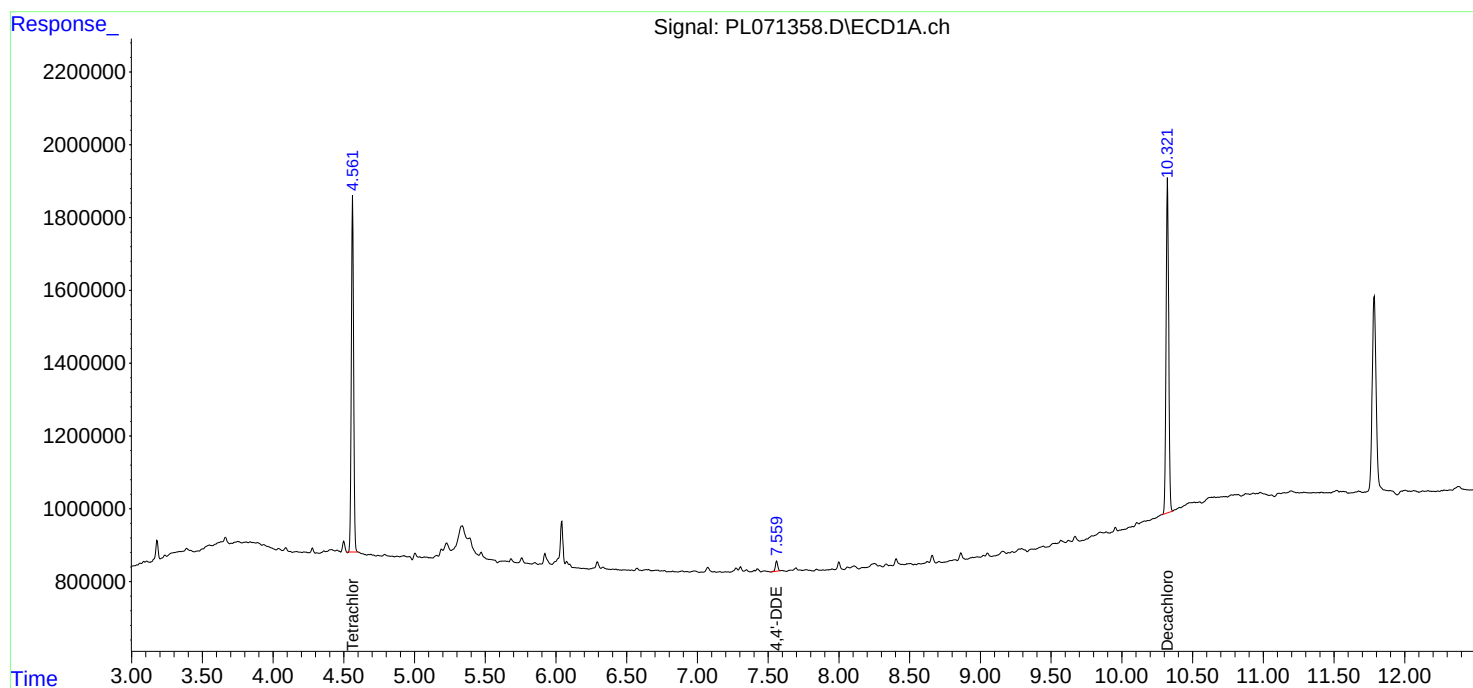


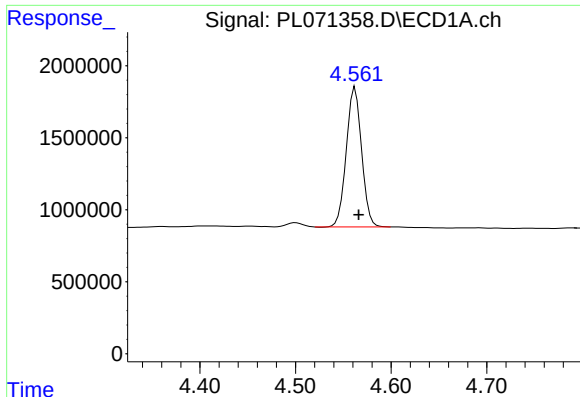

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: -0.004 min
Response: 10818765
Conc: 23.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7S

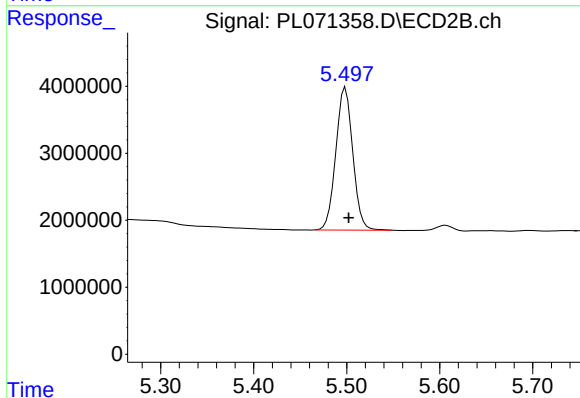


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 26962010
Conc: 21.48 ng/ml

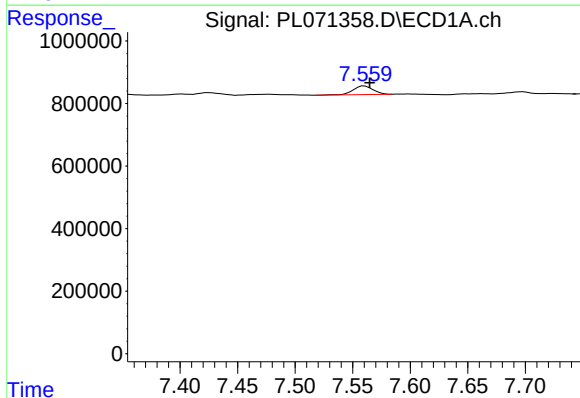


#12 4,4'-DDE

R.T.: 7.560 min
Delta R.T.: -0.005 min
Response: 329903
Conc: 0.58 ng/ml

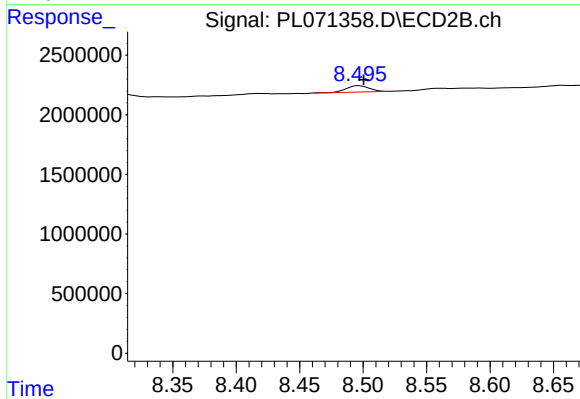

#12 4,4'-DDE


R.T.: 8.497 min
Delta R.T.: -0.003 min
Response: 665760
Conc: 0.43 ng/ml

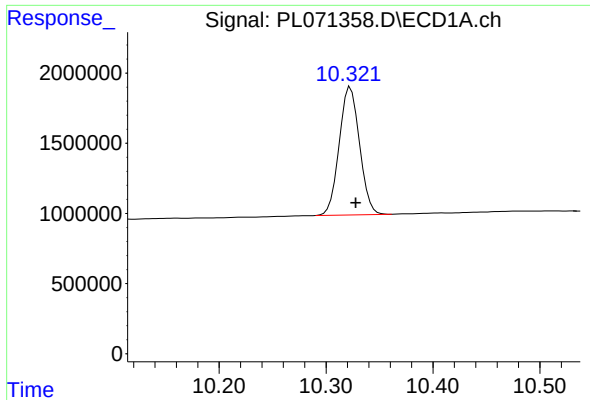

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.005 min
Response: 12086418
Conc: 16.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7S

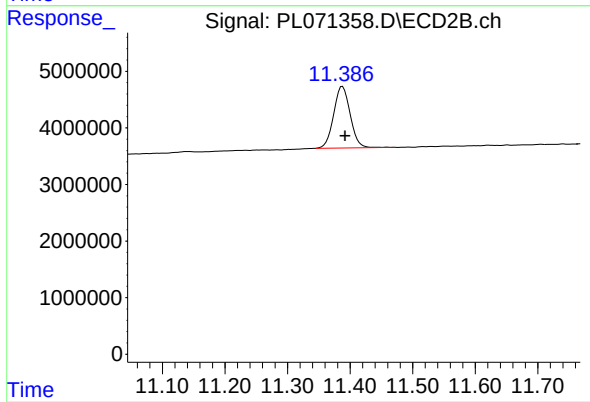

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.004 min
Response: 20056707
Conc: 14.43 ng/ml