

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120922\
 Data File : PL079663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2022 17:32
 Operator : AR\AJ
 Sample : N5912-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FMC-TOTE-1207

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/12/2022
 Supervised By : Ankita Jodhani 12/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:00:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.315	2.568	4173560	12327918	1.847m	4.529m#
2) SA Decachlor...	8.761	7.630	7982147	5132680	4.110	2.185 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120922\
Data File : PL079663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2022 17:32
Operator : AR\AJ
Sample : N5912-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FMC-TOTE-1207


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/12/2022
Supervised By : Ankita Jodhani 12/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:00:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

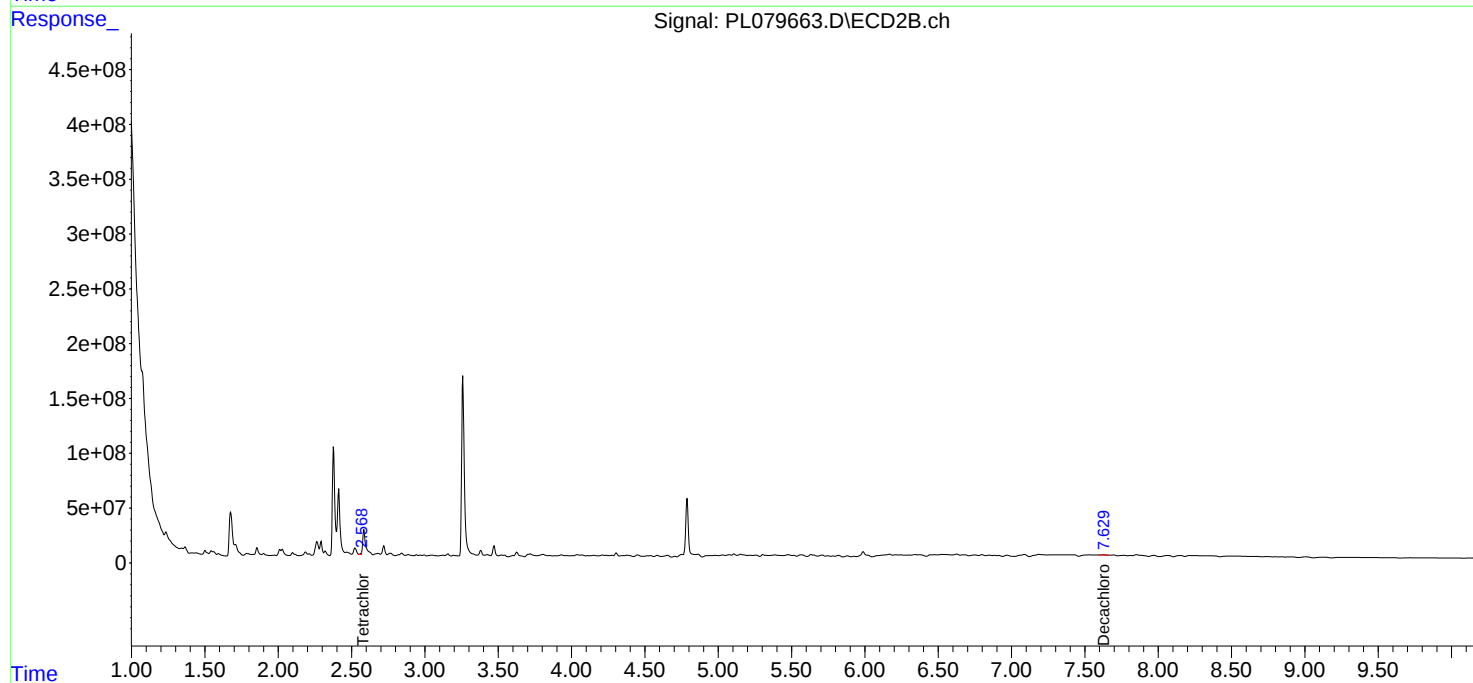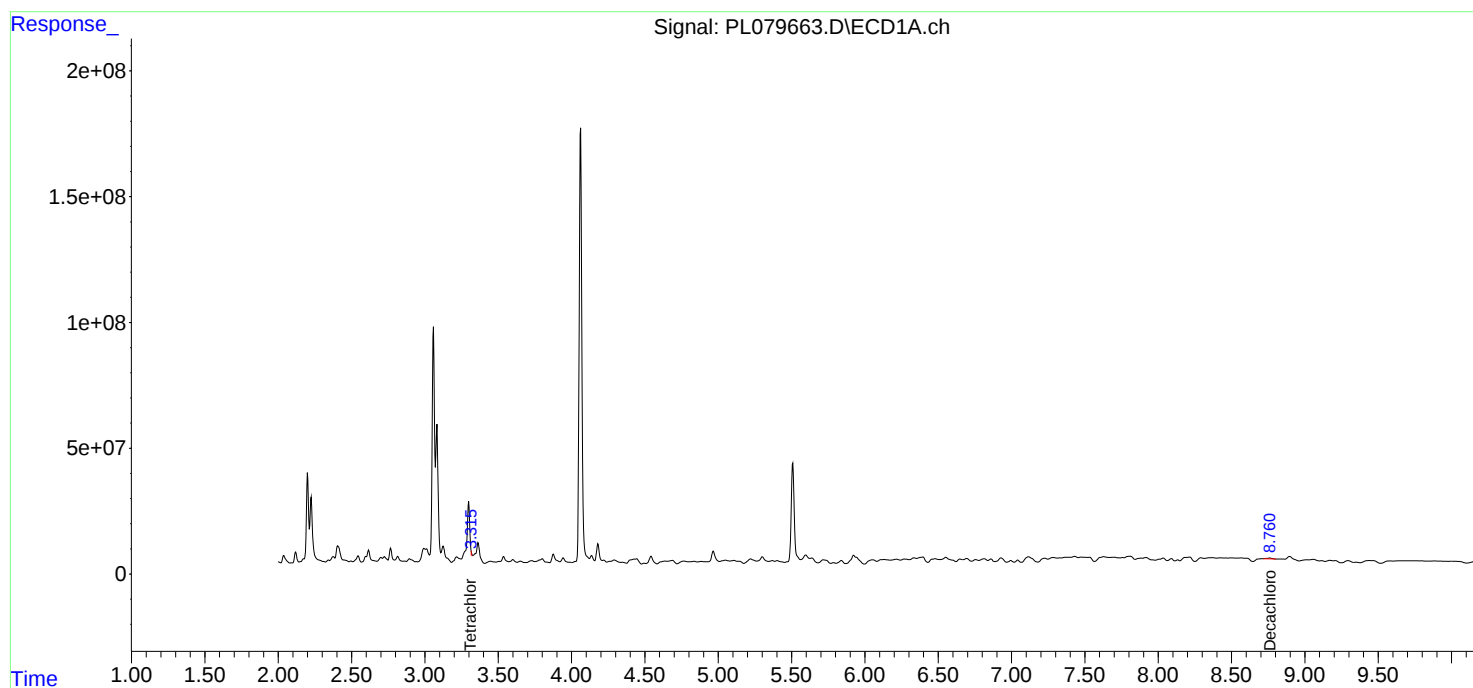

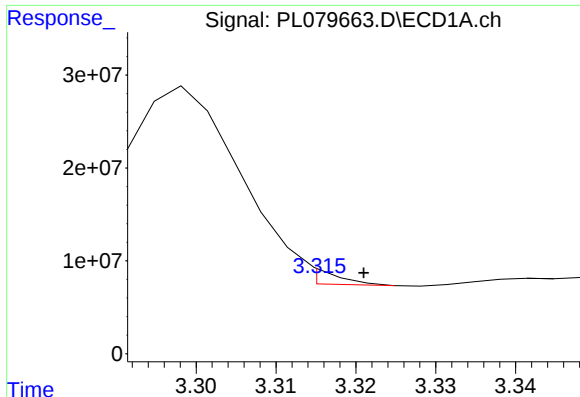


#1 Tetrachloro-m-xylene

R.T.: 3.315 min
Delta R.T.: -0.006 min
Response: 4173560
Conc: 1.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
FMC-TOTE-1207


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2022
Supervised By :Ankita Jodhani 12/12/2022

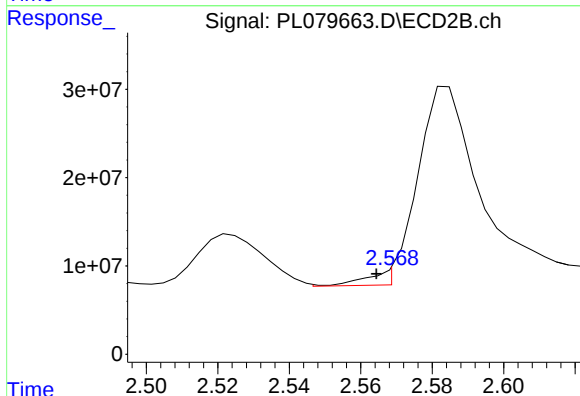


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: 0.004 min
Response: 12327918
Conc: 4.53 ng/ml m

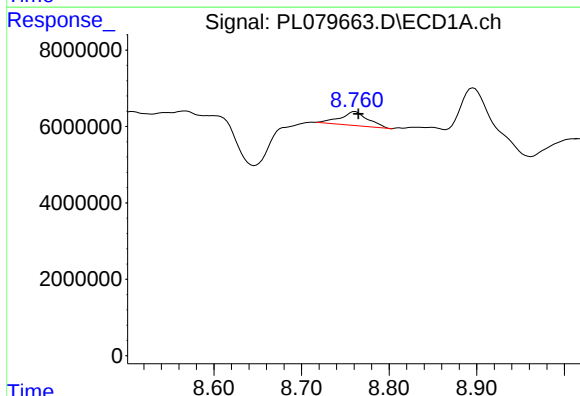

#28 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: -0.004 min
Response: 7982147
Conc: 4.11 ng/ml

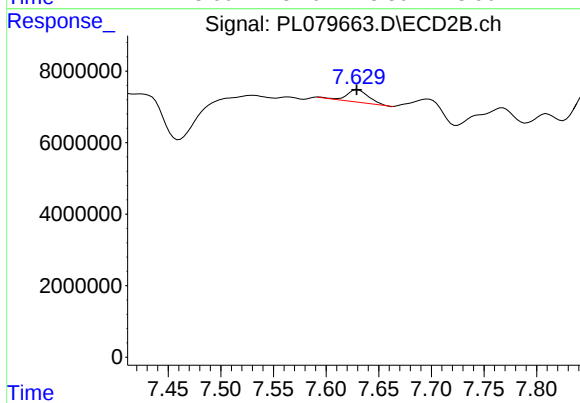

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 5132680
Conc: 2.18 ng/ml