

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120922\
 Data File : PL079664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2022 17:45
 Operator : AR\AJ
 Sample : N5947-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NYE-WATER-1208

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/12/2022
 Supervised By : Ankita Jodhani 12/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:00:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.564	43272771	52359334	19.155	19.235m
2)	SA Decachlor...	8.764	7.631	25153780	28632051	12.952	12.188

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120922\
Data File : PL079664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2022 17:45
Operator : AR\AJ
Sample : N5947-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NYE-WATER-1208


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/12/2022
Supervised By : Ankita Jodhani 12/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:00:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

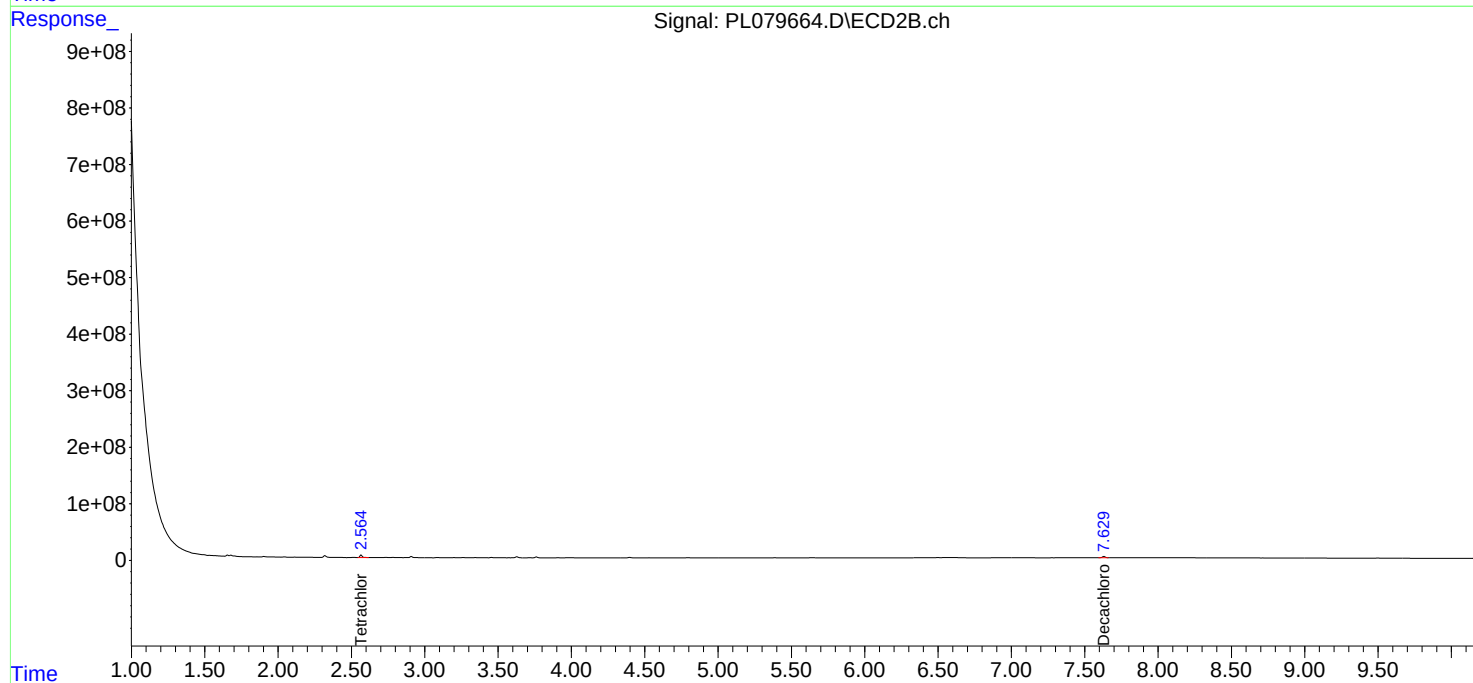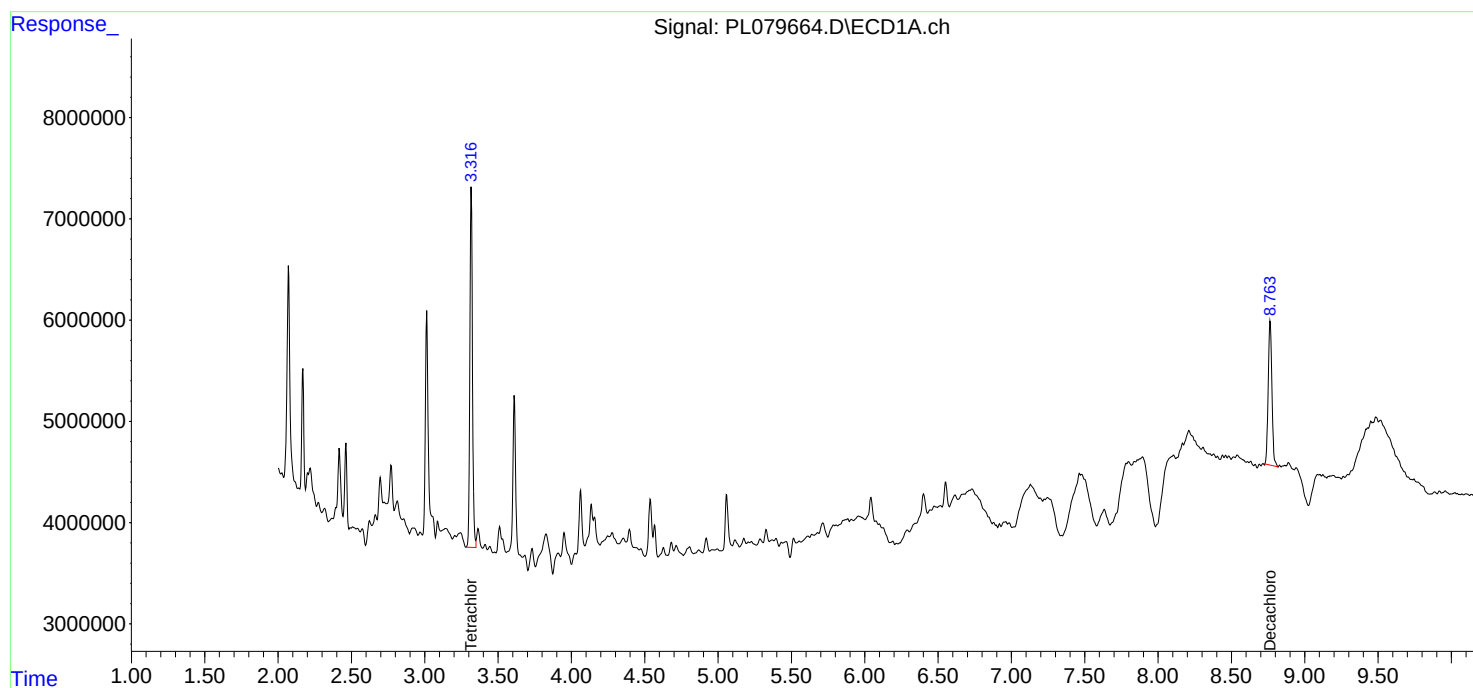

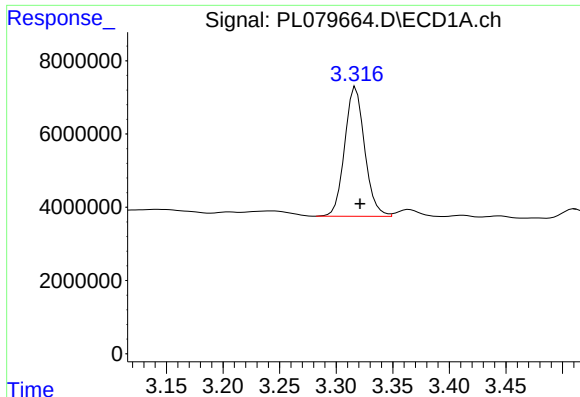


#1 Tetrachloro-m-xylene

R.T.: 3.317 min
Delta R.T.: -0.004 min
Response: 43272771
Conc: 19.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
NYE-WATER-1208


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2022
Supervised By :Ankita Jodhani 12/12/2022

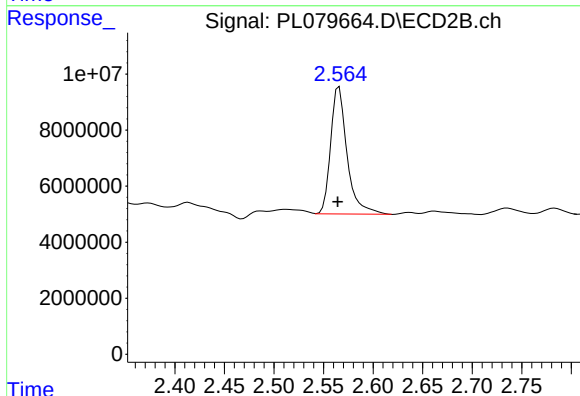


#1 Tetrachloro-m-xylene

R.T.: 2.564 min
Delta R.T.: 0.000 min
Response: 52359334
Conc: 19.24 ng/ml m

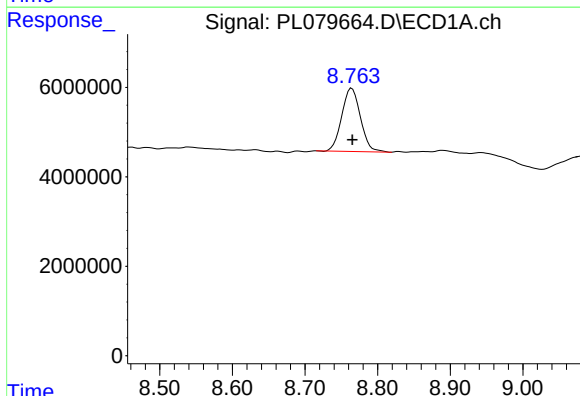

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 25153780
Conc: 12.95 ng/ml

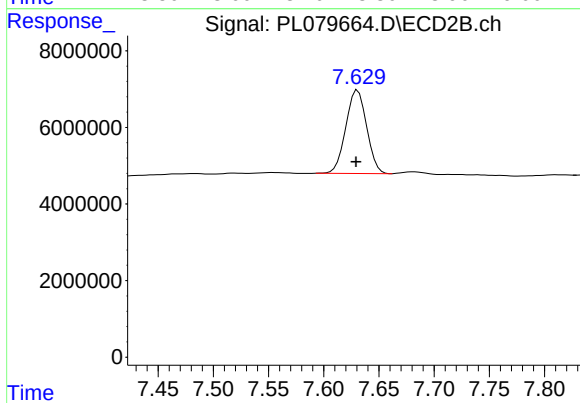

#28 Decachlorobiphenyl

R.T.: 7.631 min
Delta R.T.: 0.002 min
Response: 28632051
Conc: 12.19 ng/ml