

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120924\
 Data File : PL093333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2024 13:31
 Operator : AR\AJ
 Sample : PB165473BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB165473BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/10/2024
 Supervised By : Ankita Jodhani 12/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:24:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.776	49238744	51916245	18.946	18.001
28) SA Decachlor...	9.065	7.917	38555910	58435178	22.177m	20.457

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120924\
Data File : PL093333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2024 13:31
Operator : AR\AJ
Sample : PB165473BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB165473BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/10/2024
Supervised By : Ankita Jodhani 12/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:24:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

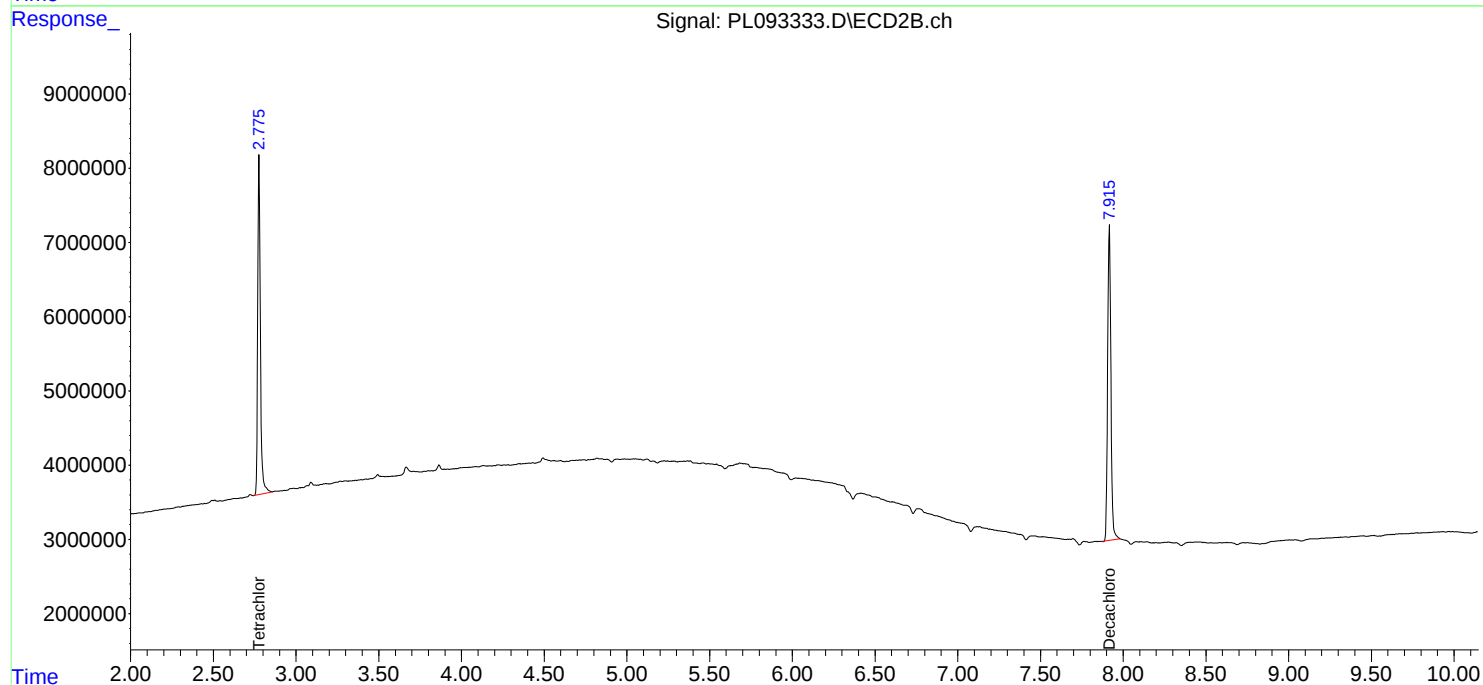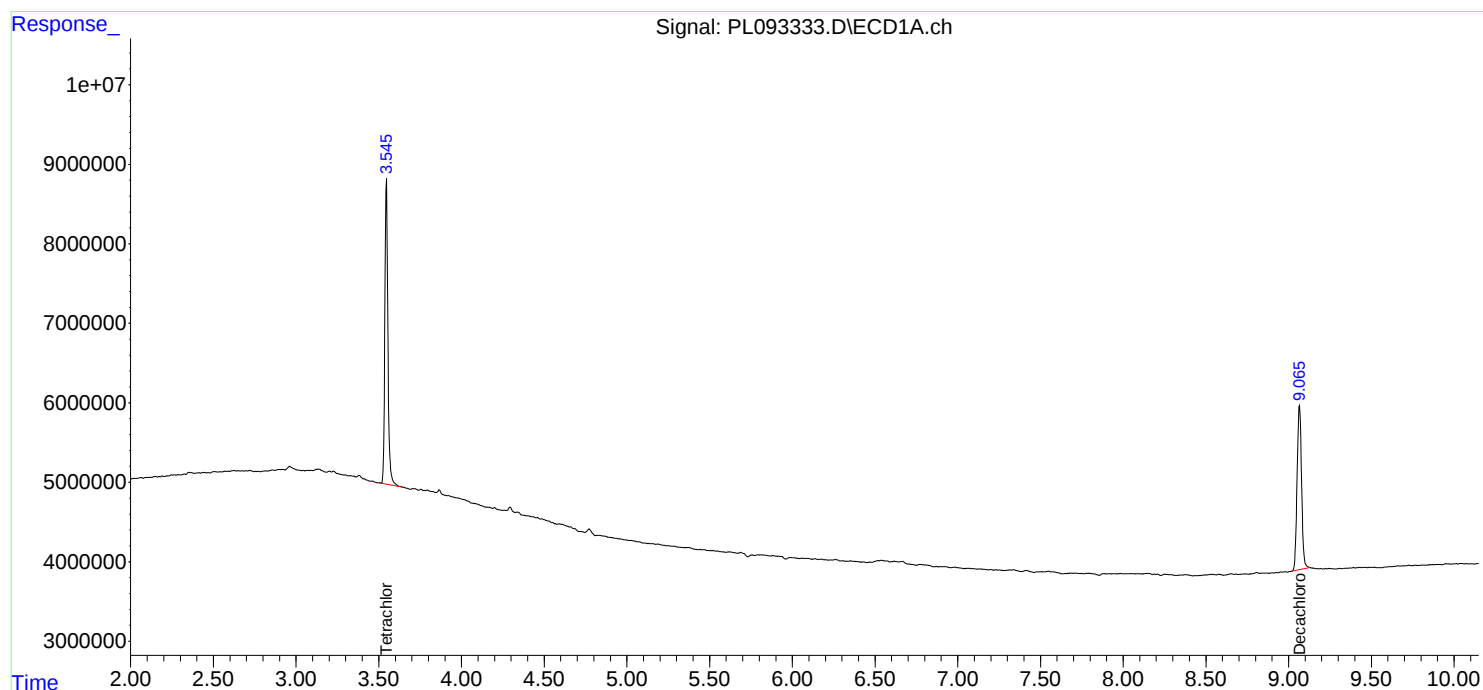

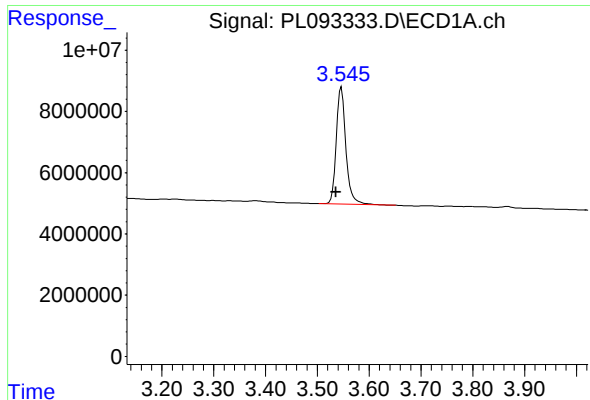


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.010 min
Response: 49238744
Conc: 18.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB165473BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/10/2024
Supervised By :Ankita Jodhani 12/10/2024

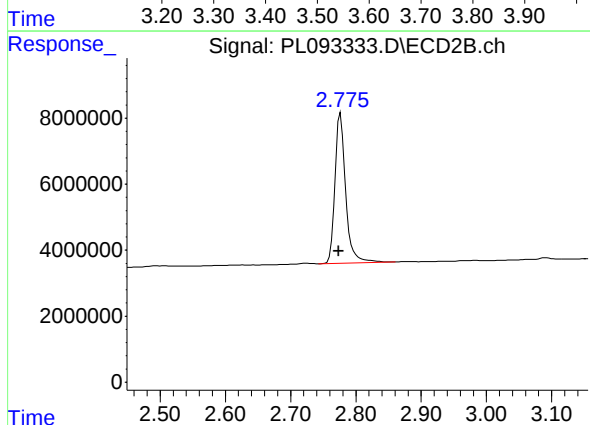


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.003 min
Response: 51916245
Conc: 18.00 ng/ml

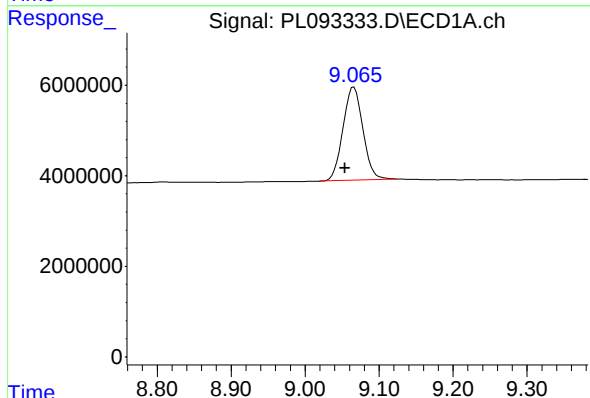

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.010 min
Response: 38555910
Conc: 22.18 ng/ml m

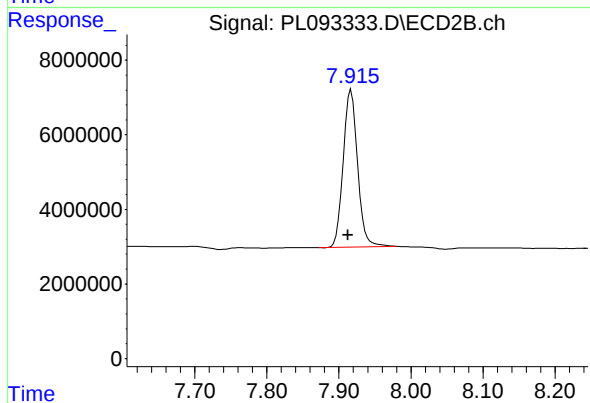

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.005 min
Response: 58435178
Conc: 20.46 ng/ml