

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120924\
 Data File : PL093339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2024 15:16
 Operator : AR\AJ
 Sample : P5176-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-12062024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/10/2024
 Supervised By :Ankita Jodhani 12/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:29:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.775	2709504	6101103	1.043m	2.115 #
28) SA Decachlor...	9.053	7.913	2421852	3817231	1.393m	1.336

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120924\
Data File : PL093339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2024 15:16
Operator : AR\AJ
Sample : P5176-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-02-12062024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/10/2024
Supervised By : Ankita Jodhani 12/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time : Dec 10 00:29:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

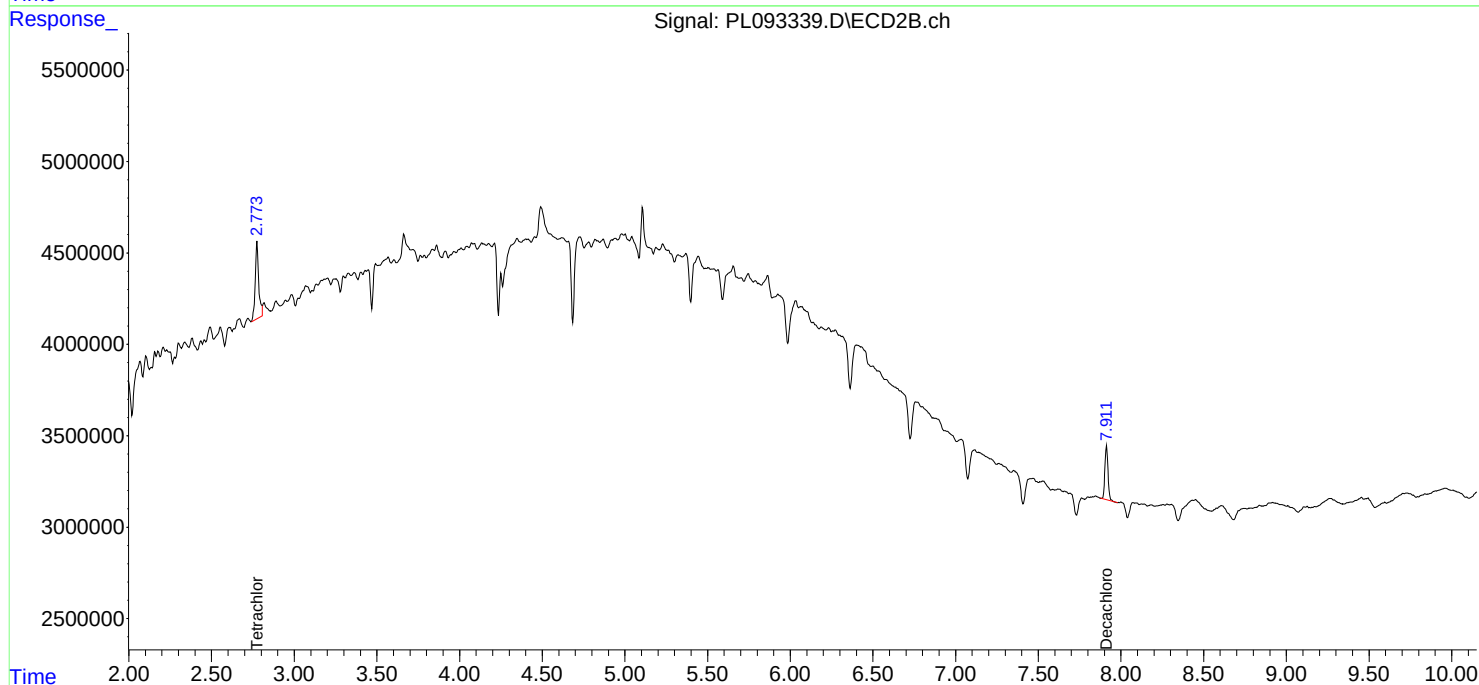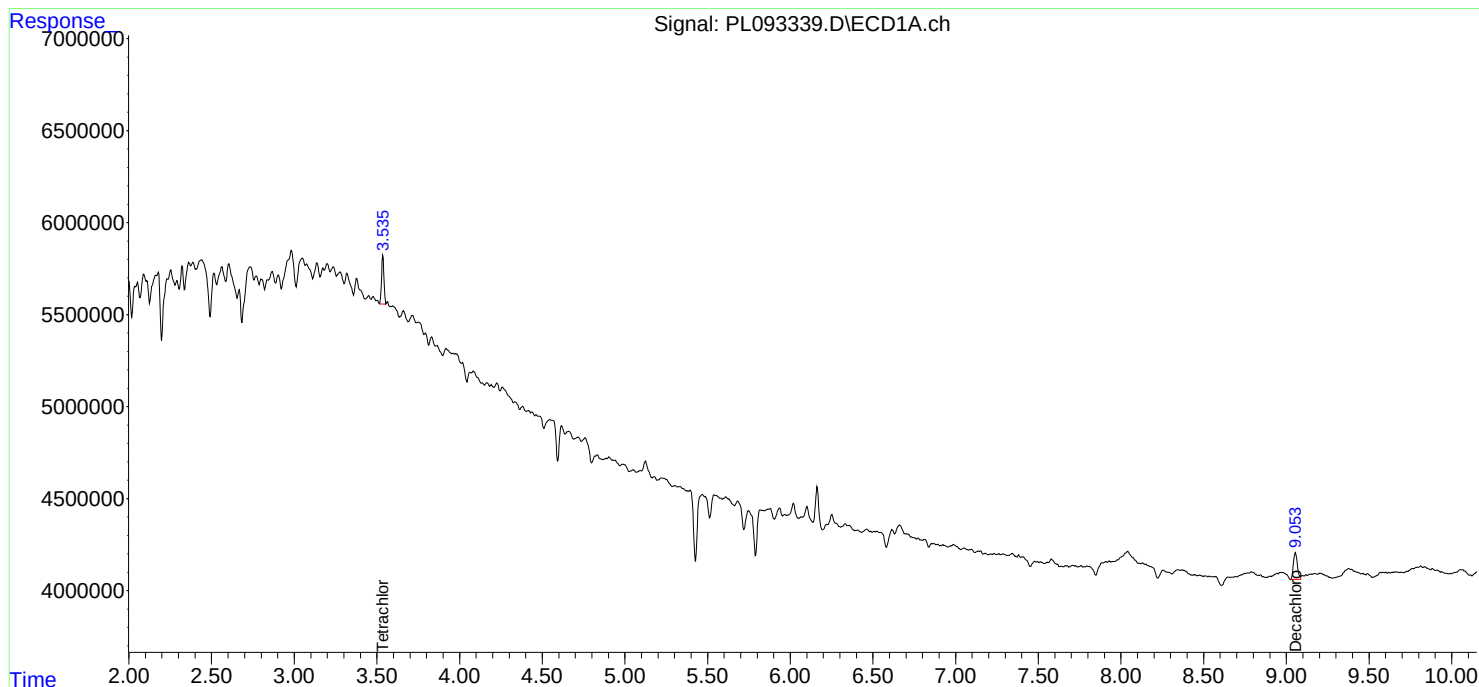

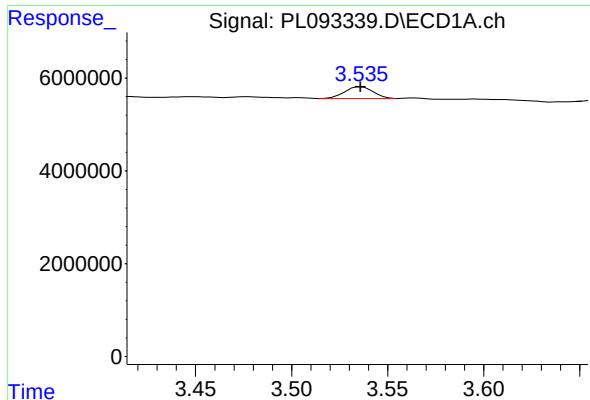


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 2709504
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-12062024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/10/2024
Supervised By :Ankita Jodhani 12/10/2024

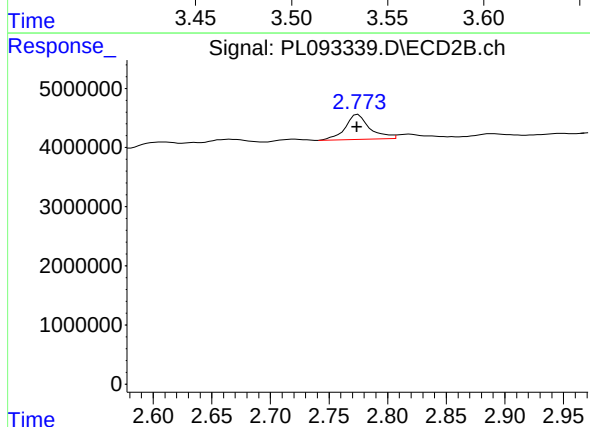


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.001 min
Response: 6101103
Conc: 2.12 ng/ml

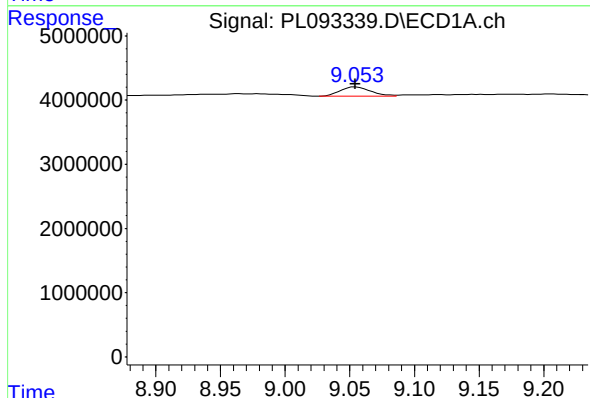

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 2421852
Conc: 1.39 ng/ml m

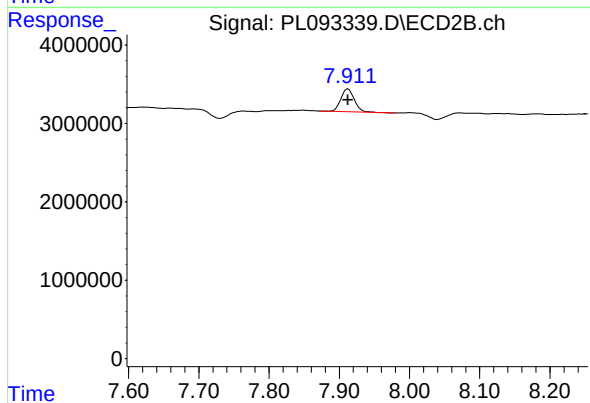

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 3817231
Conc: 1.34 ng/ml