

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
 Data File : PL097805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2025 11:38
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 12:14:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 12:09:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	2.799	284.0E6	491.7E6	75.366	75.068
28)	SA Decachlor...	8.956	7.947	213.6E6	368.5E6	75.168	75.079
Target Compounds							
23)	Chlordane-1	4.649	3.803	175.1E6	200.1E6	753.749	752.441
24)	Chlordane-2	5.172	4.380	188.4E6	221.5E6	790.871	746.294
25)	Chlordane-3	5.875	5.012	671.6E6	671.4E6	753.262	749.376
26)	Chlordane-4	5.959	5.075	791.6E6	628.4E6	753.099	758.729
27)	Chlordane-5	6.794	5.967	135.8E6	247.1E6	752.399	753.363



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
Data File : PL097805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2025 11:38
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 12:14:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 12:09:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

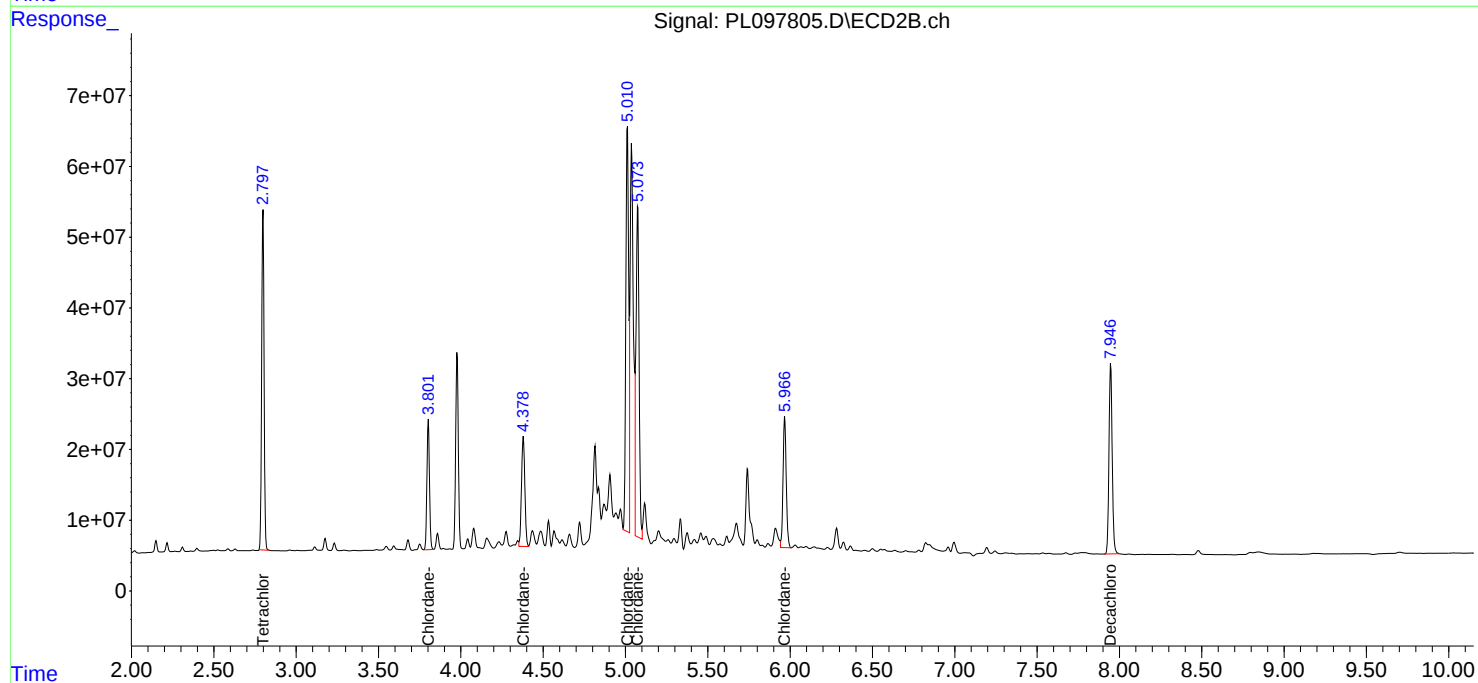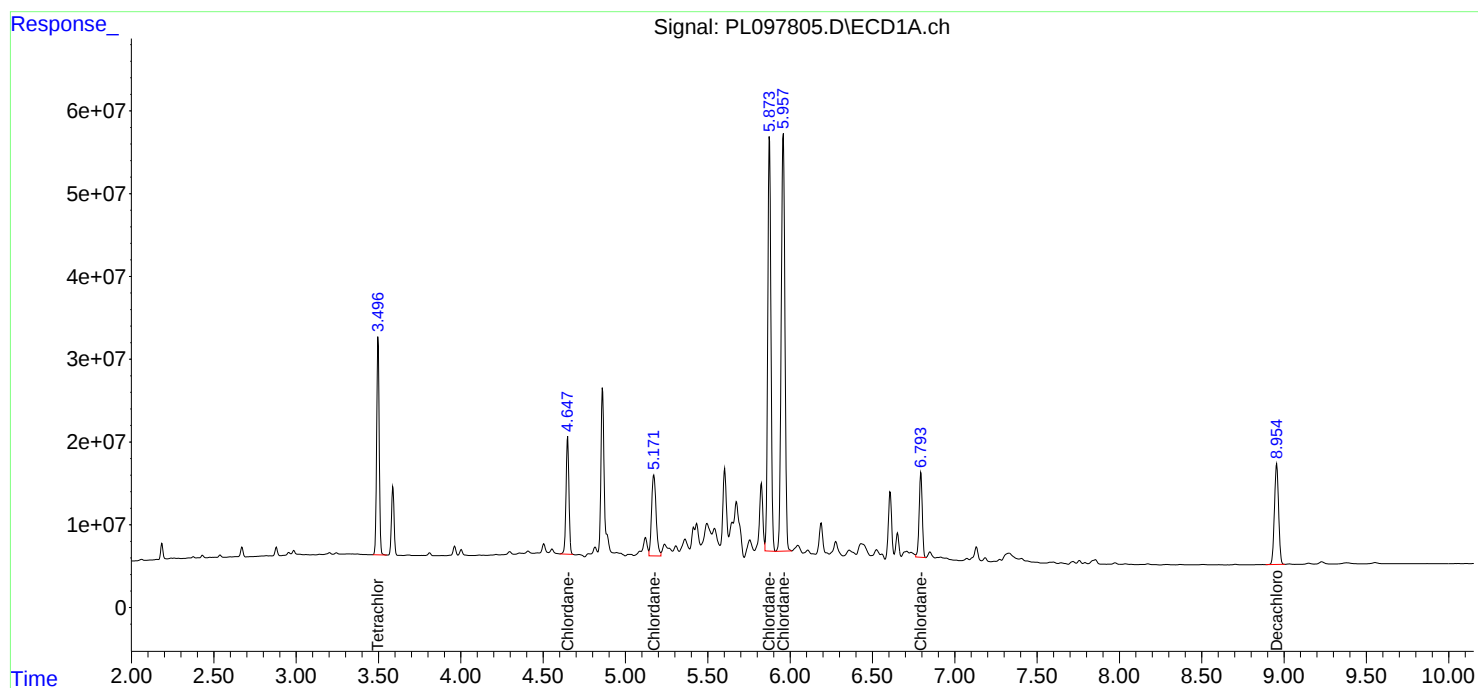


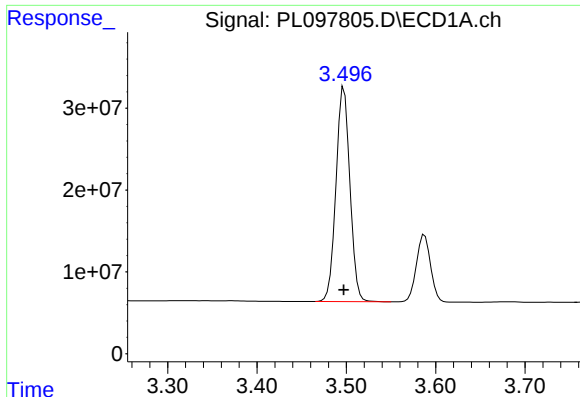

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 284008312
Conc: 75.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

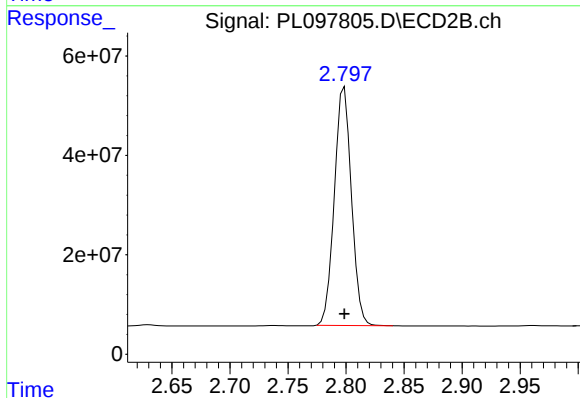


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: 0.000 min
Response: 491718638
Conc: 75.07 ng/ml

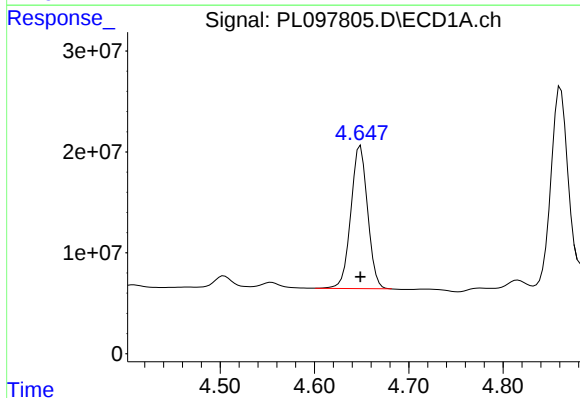


#23 Chlordane-1

R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 175122417
Conc: 753.75 ng/ml

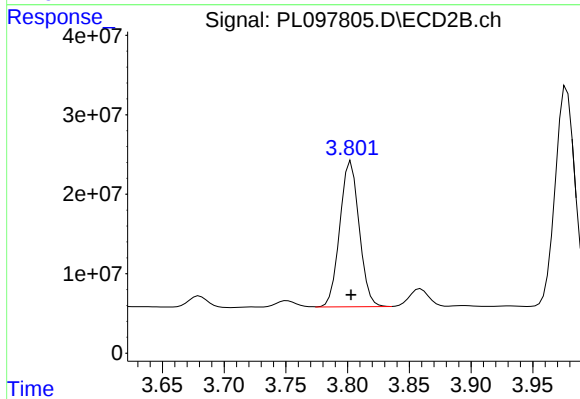

#23 Chlordane-1


R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 200067373
Conc: 752.44 ng/ml

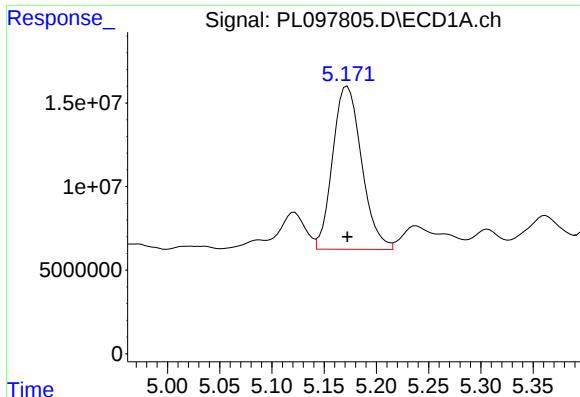

#24 Chlordane-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 188372407
Conc: 790.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

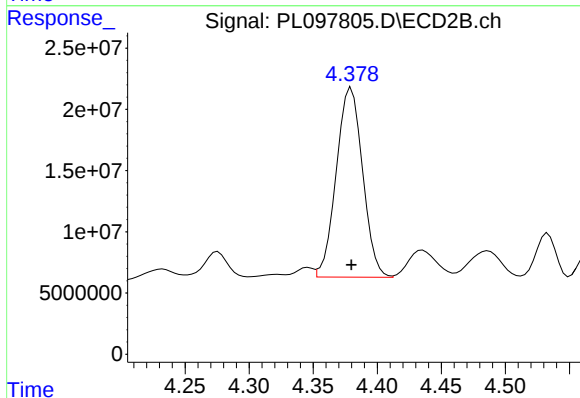


#24 Chlordane-2

R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 221501663
Conc: 746.29 ng/ml

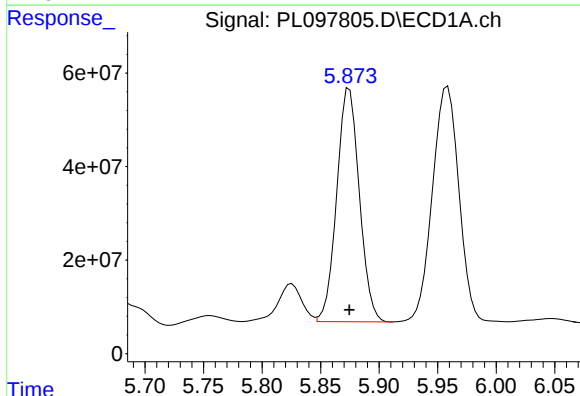


#25 Chlordane-3

R.T.: 5.875 min
Delta R.T.: 0.000 min
Response: 671633266
Conc: 753.26 ng/ml

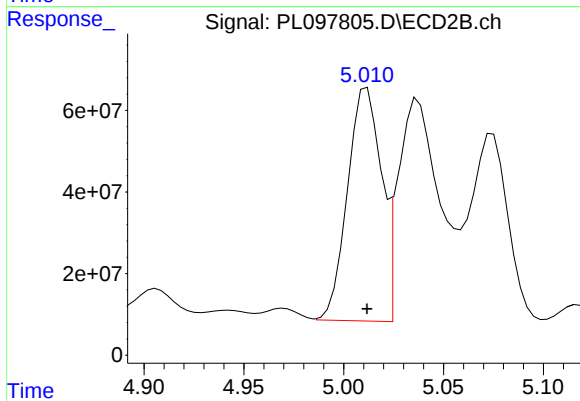

#25 Chlordane-3


R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 671353338
Conc: 749.38 ng/ml

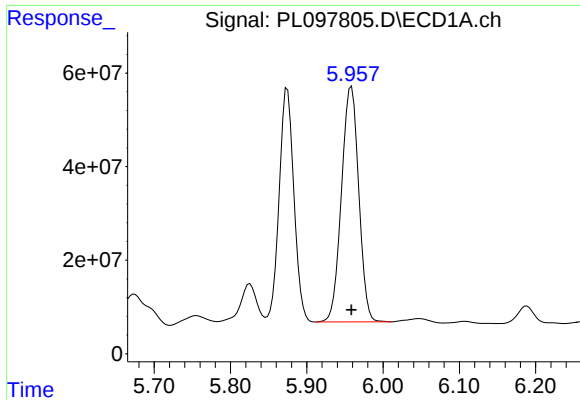

#26 Chlordane-4


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 791645501
Conc: 753.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

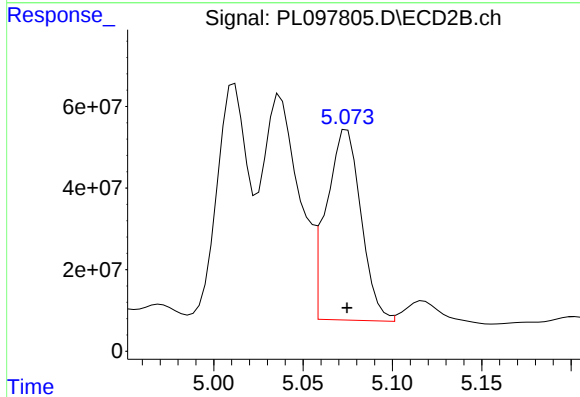


#26 Chlordane-4

R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 628418229
Conc: 758.73 ng/ml

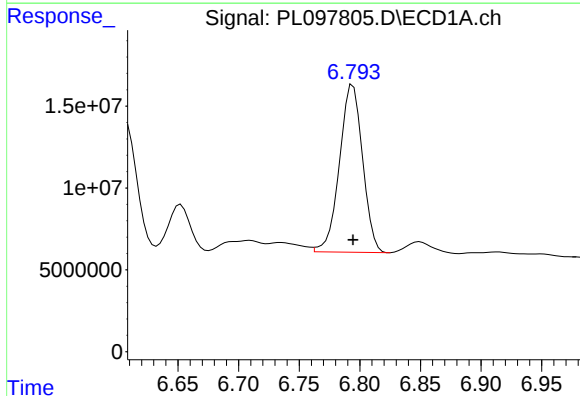


#27 Chlordane-5

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 135795581
Conc: 752.40 ng/ml

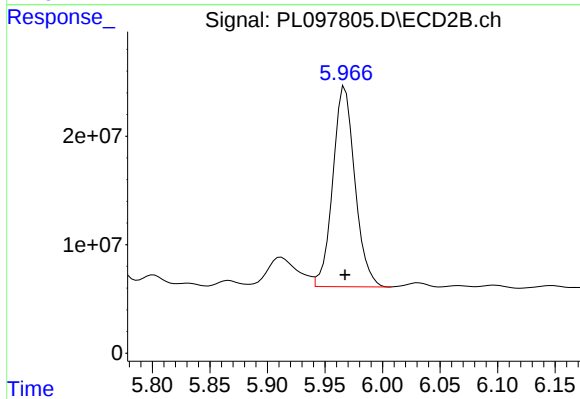

#27 Chlordane-5


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 247053474
Conc: 753.36 ng/ml

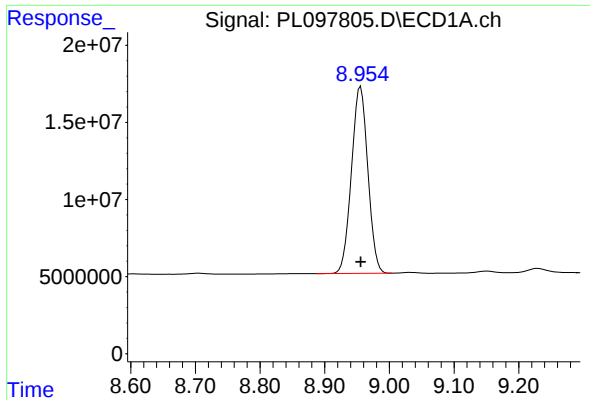

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.000 min
Response: 213565357
Conc: 75.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

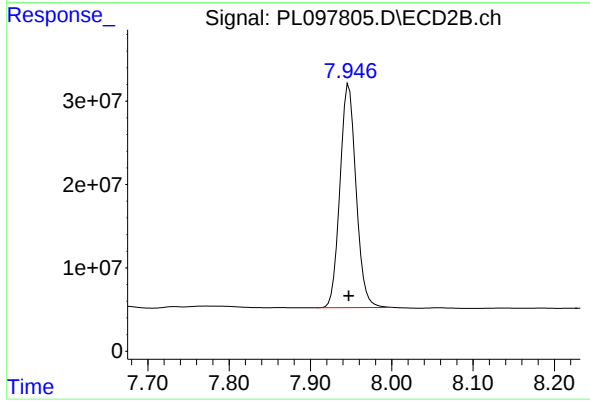

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 368489745
Conc: 75.08 ng/ml