

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
 Data File : PL097817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2025 16:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:06:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.499	2.798	113.1E6	158.1E6	22.414	22.634
28)	SA Decachlor...	8.960	7.949	94547053	161.1E6	24.884	24.498
Target Compounds							
8)	B Heptachlo...	0.000	4.788f	0	33183258	N.D.	3.685 #
14)	MA Endrin	0.000	5.679	0	6394680	N.D.	0.765 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
Data File : PL097817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2025 16:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:06:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

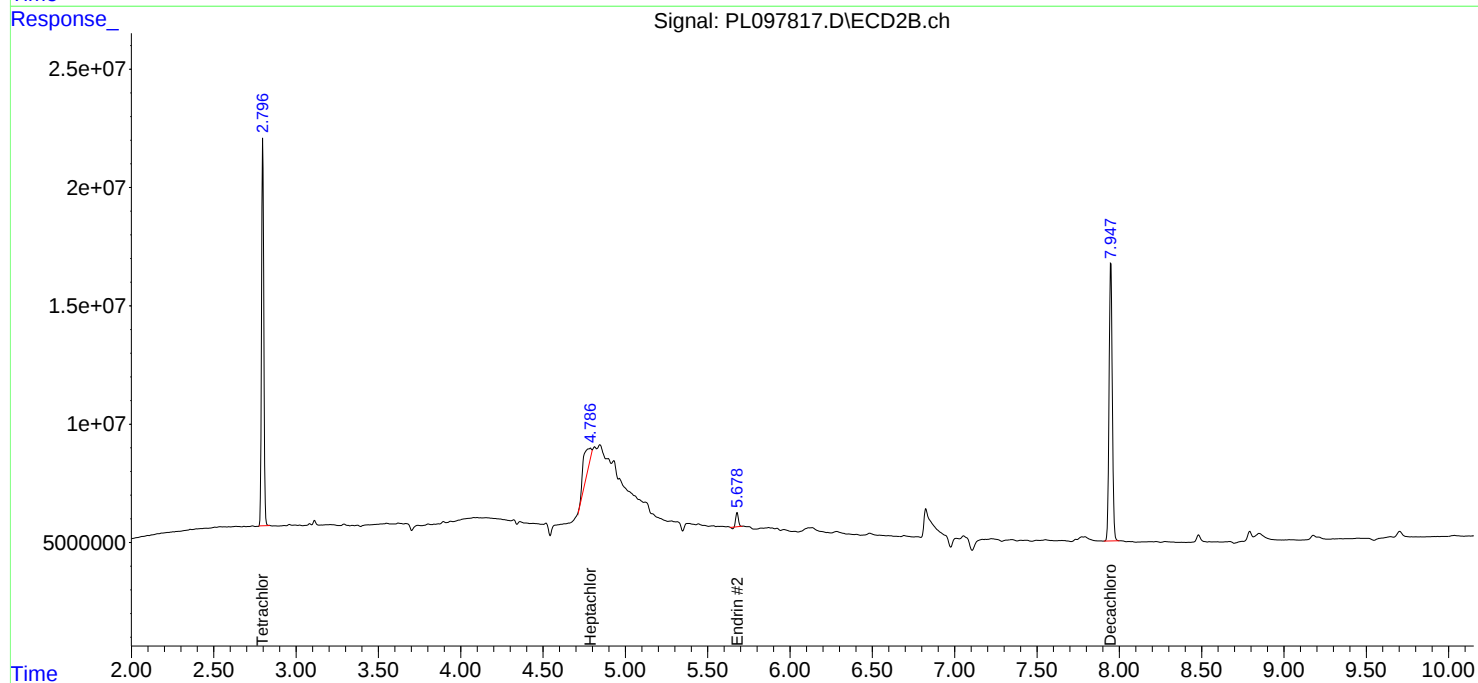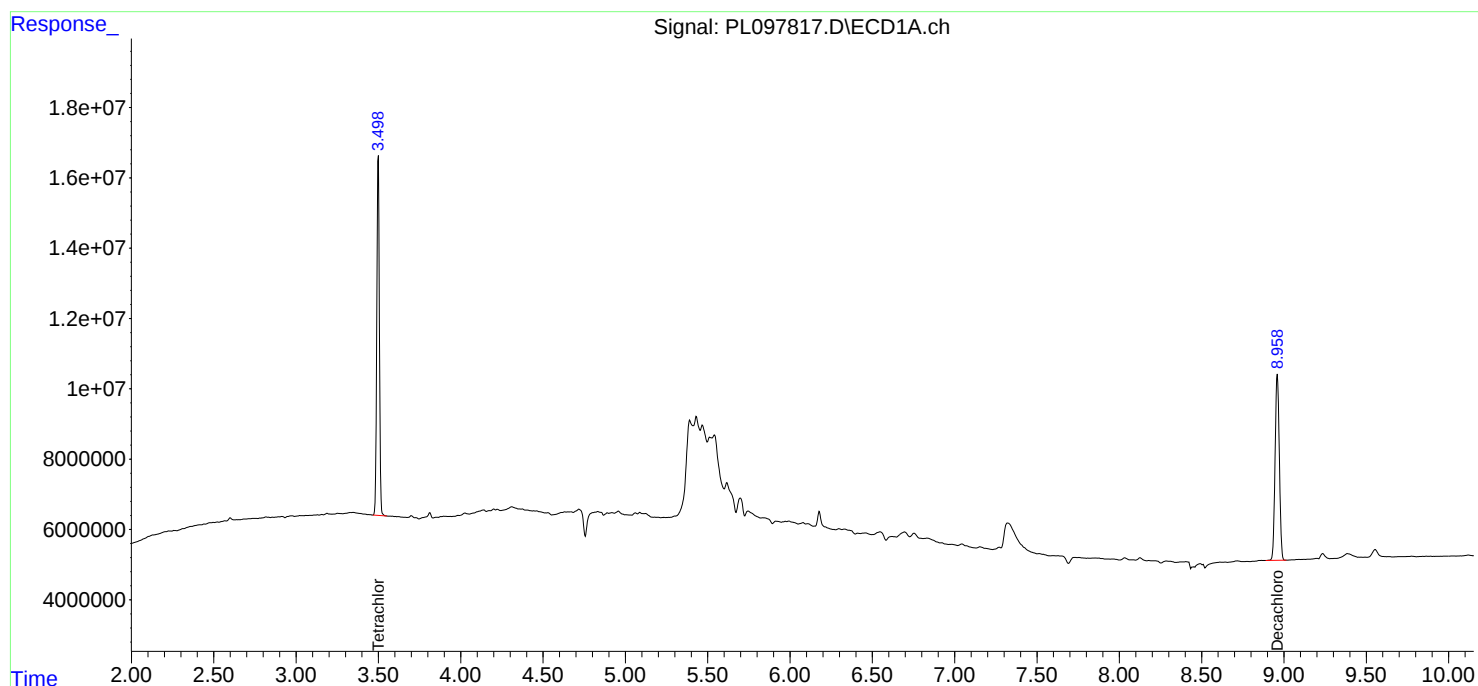


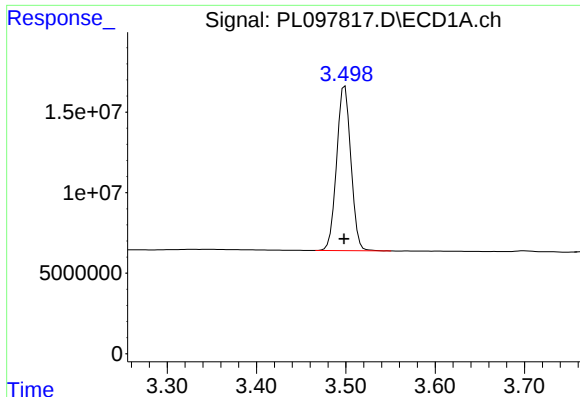

#1 Tetrachloro-m-xylene


R.T.: 3.499 min
Delta R.T.: 0.000 min
Response: 113124745
Conc: 22.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

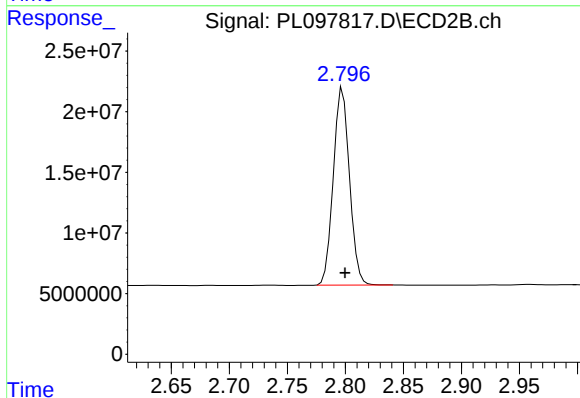


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: -0.002 min
Response: 158103833
Conc: 22.63 ng/ml

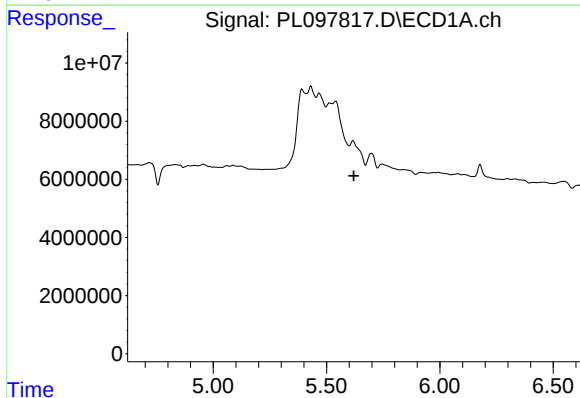


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.620 min
Response: 0
Conc: N.D.

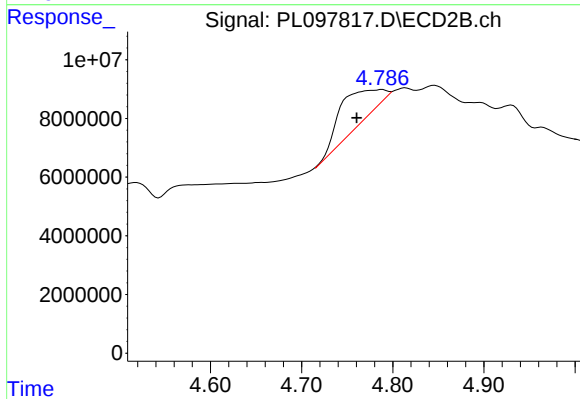

#8 Heptachlor epoxide


R.T.: 4.788 min
Delta R.T.: 0.028 min
Response: 33183258
Conc: 3.69 ng/ml

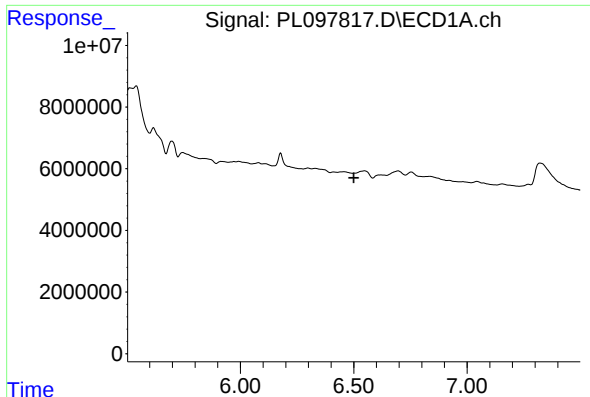

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

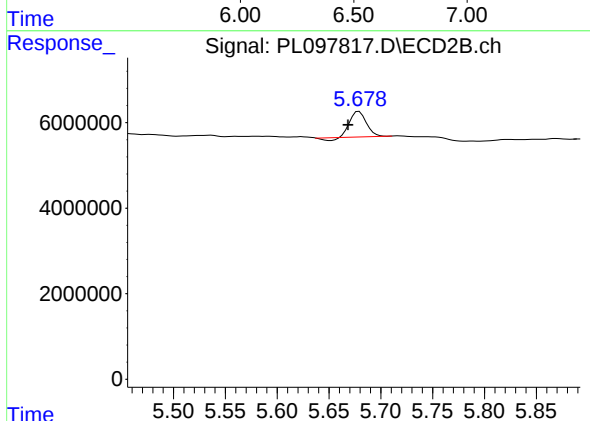


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.010 min
Response: 6394680
Conc: 0.77 ng/ml

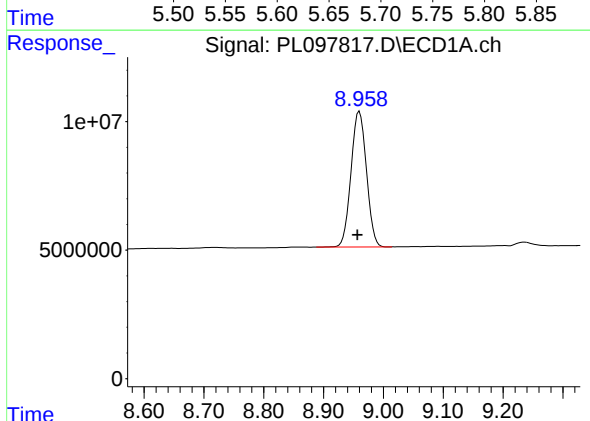

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: 0.003 min
Response: 94547053
Conc: 24.88 ng/ml

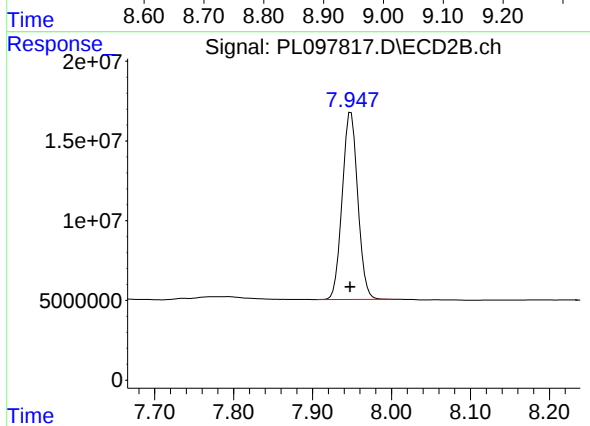

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.001 min
Response: 161101515
Conc: 24.50 ng/ml