

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
 Data File : PL097804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2025 11:25
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 12:11:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 12:09:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	2.799	378.5E6	663.3E6	100.693	101.303
28)	SA Decachlor...	8.955	7.947	279.5E6	484.9E6	98.477	98.851
Target Compounds							
23)	Chlordane-1	4.648	3.802	233.0E6	269.8E6	1005.201	1016.506
24)	Chlordane-2	5.172	4.379	230.9E6	296.4E6	996.782	996.291
25)	Chlordane-3	5.874	5.011	903.1E6	906.5E6	1015.023	1011.411
26)	Chlordane-4	5.958	5.074	1058.4E6	830.5E6	1008.905	1008.603
27)	Chlordane-5	6.794	5.966	181.1E6	333.9E6	1005.010	1020.429



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
Data File : PL097804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2025 11:25
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 12:11:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 12:09:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

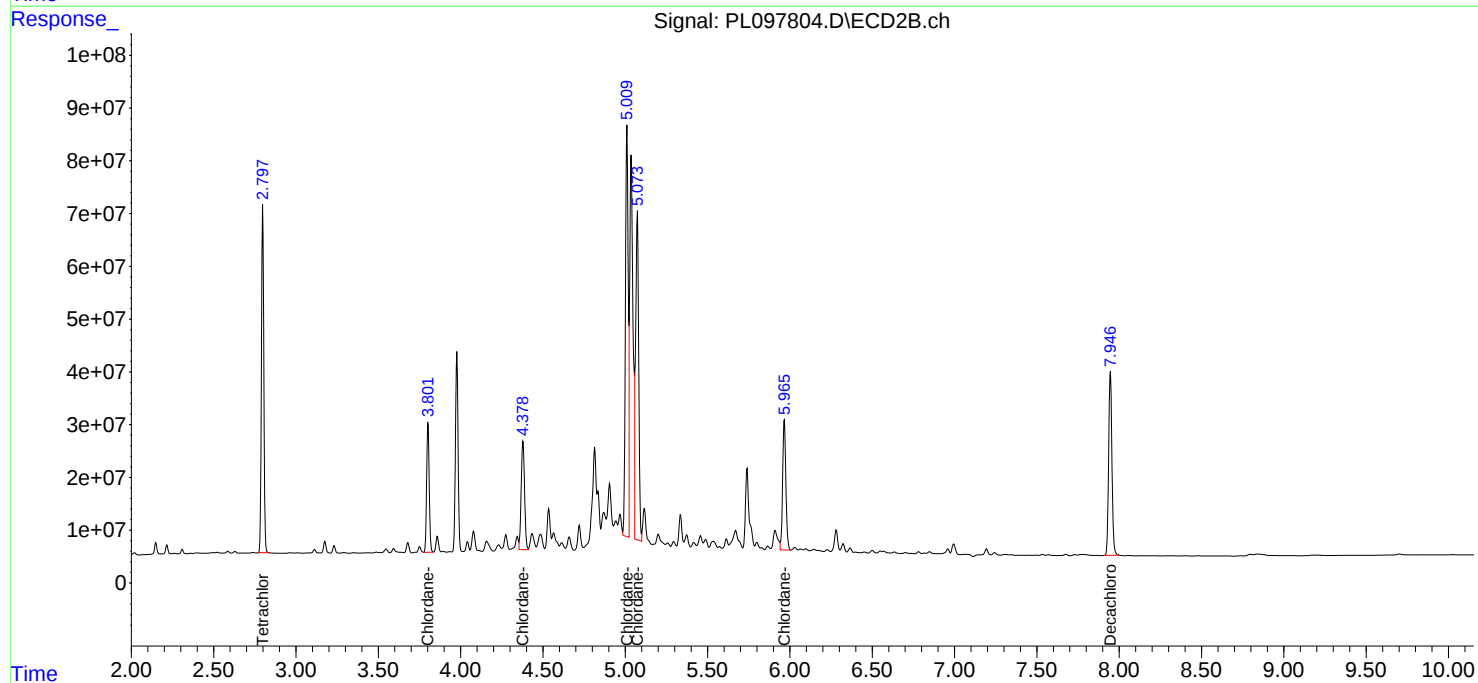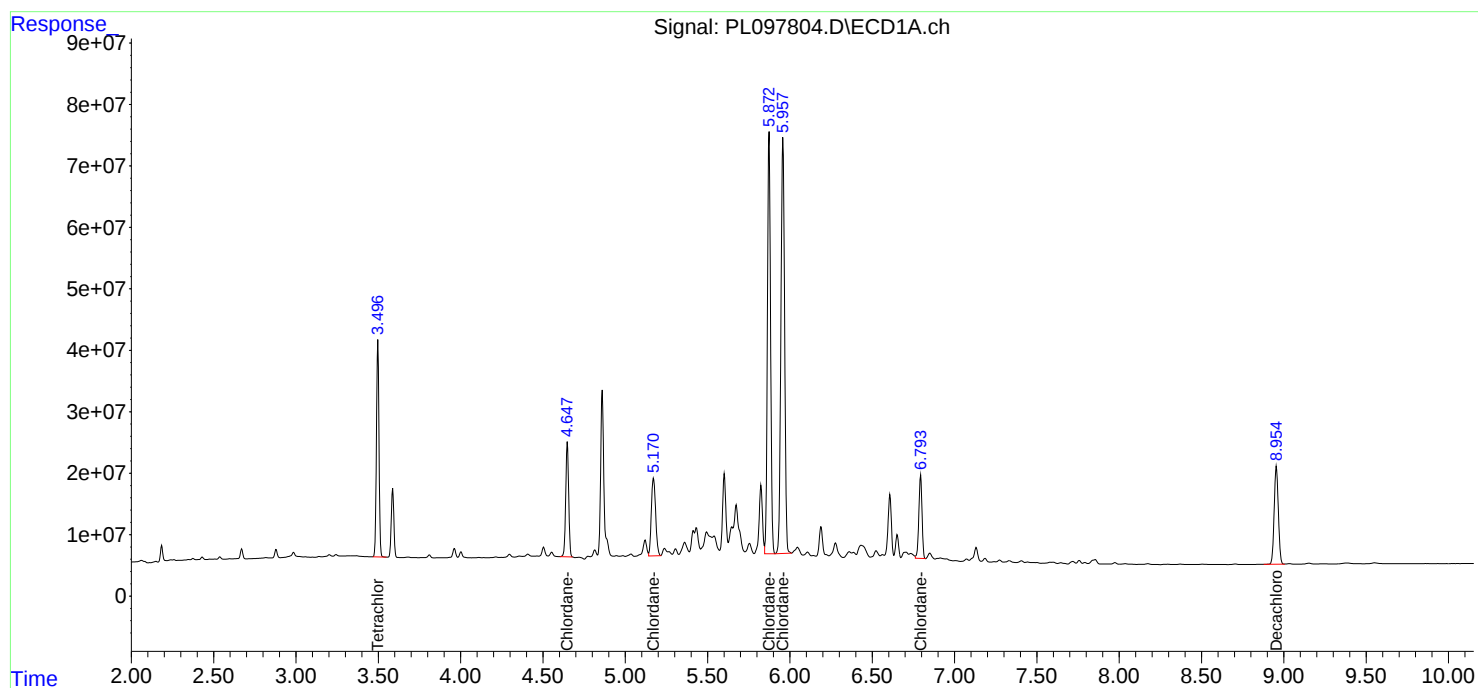


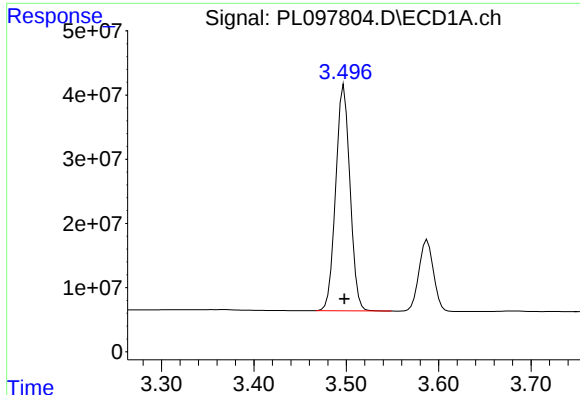

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 378520821
Conc: 100.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

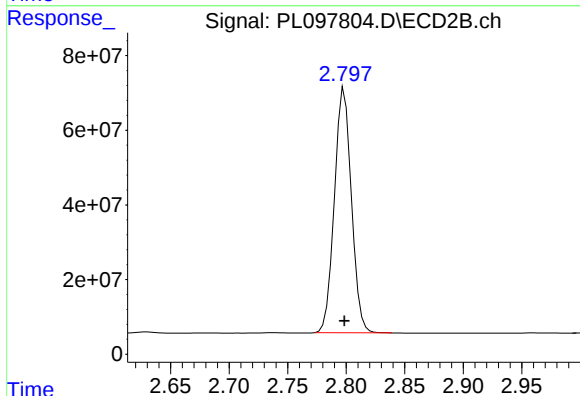


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: 0.000 min
Response: 663271739
Conc: 101.30 ng/ml

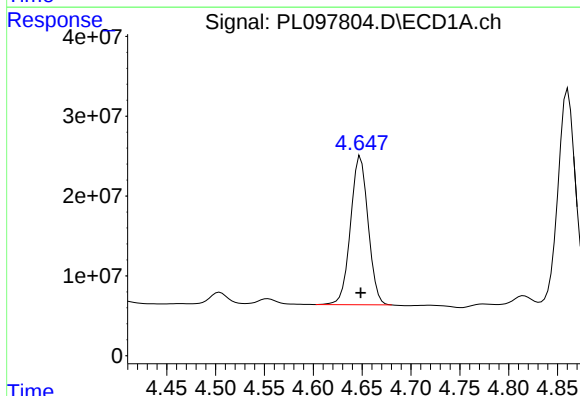


#23 Chlordane-1

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 232959658
Conc: 1005.20 ng/ml

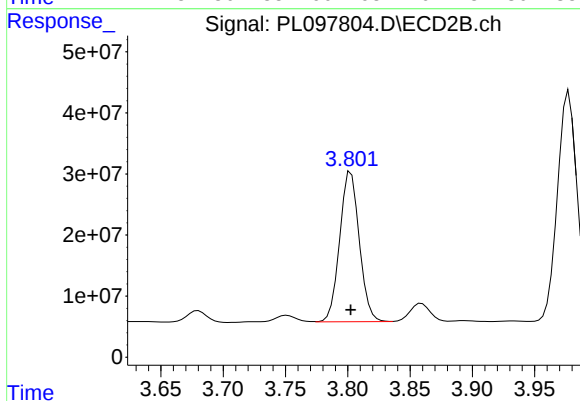

#23 Chlordane-1


R.T.: 3.802 min
Delta R.T.: 0.000 min
Response: 269839682
Conc: 1016.51 ng/ml

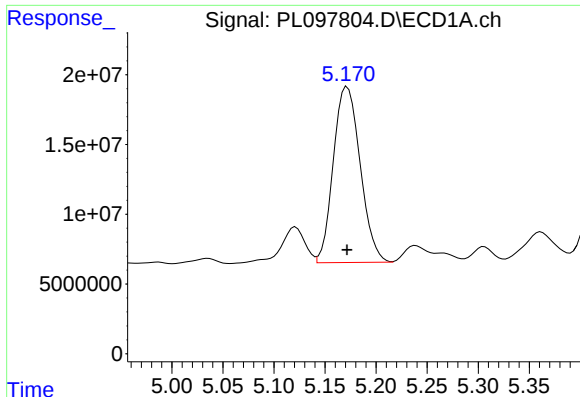

#24 Chlordane-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 230947957
Conc: 996.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

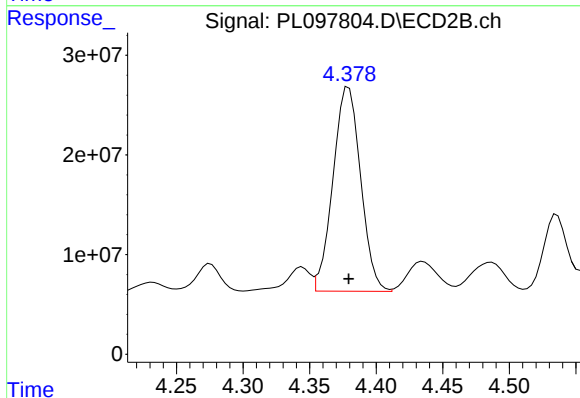


#24 Chlordane-2

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 296431879
Conc: 996.29 ng/ml

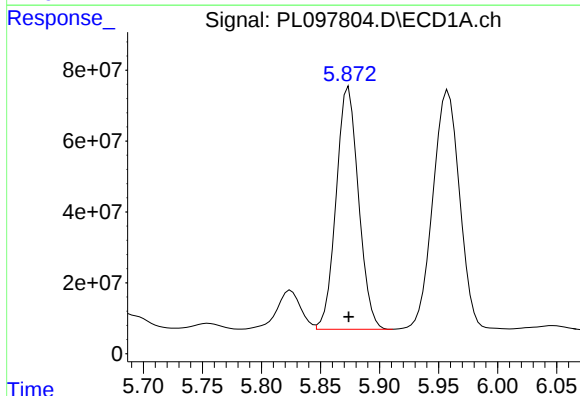


#25 Chlordane-3

R.T.: 5.874 min
Delta R.T.: 0.000 min
Response: 903060873
Conc: 1015.02 ng/ml

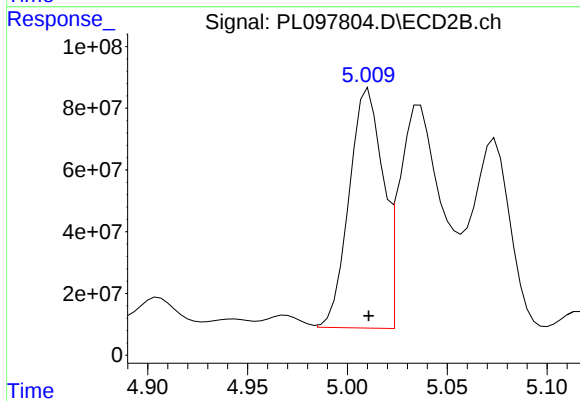

#25 Chlordane-3


R.T.: 5.011 min
Delta R.T.: 0.000 min
Response: 906483214
Conc: 1011.41 ng/ml

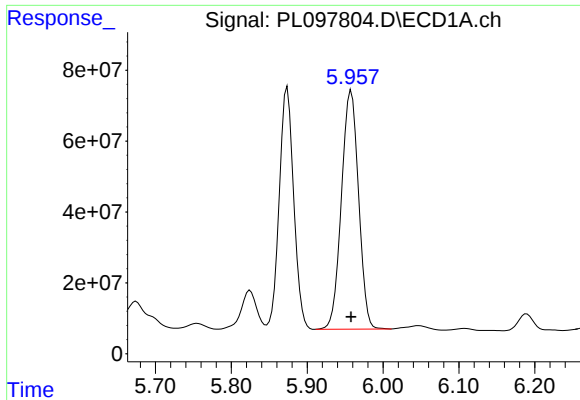

#26 Chlordane-4


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 1058353191
Conc: 1008.91 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

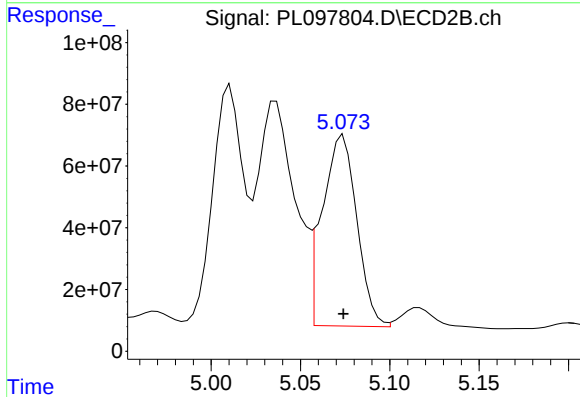


#26 Chlordane-4

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 830515690
Conc: 1008.60 ng/ml

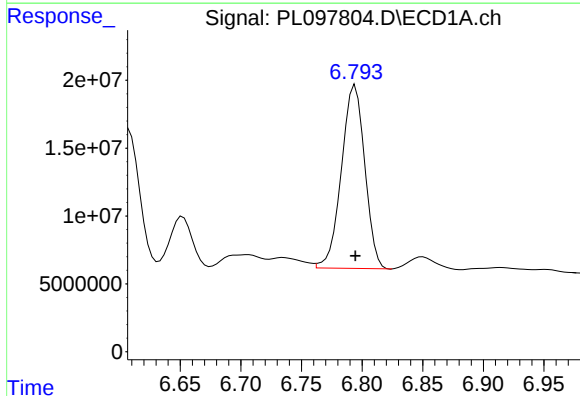


#27 Chlordane-5

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 181097704
Conc: 1005.01 ng/ml

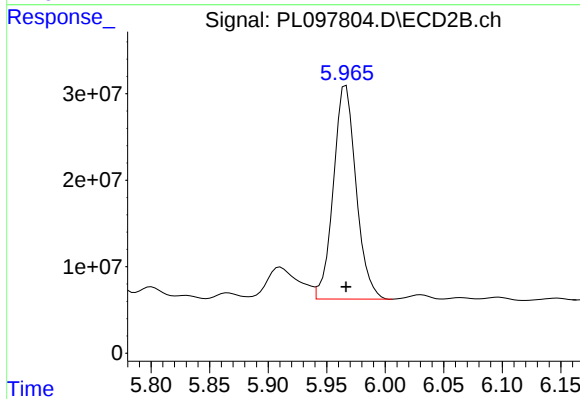

#27 Chlordane-5


R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 333883457
Conc: 1020.43 ng/ml

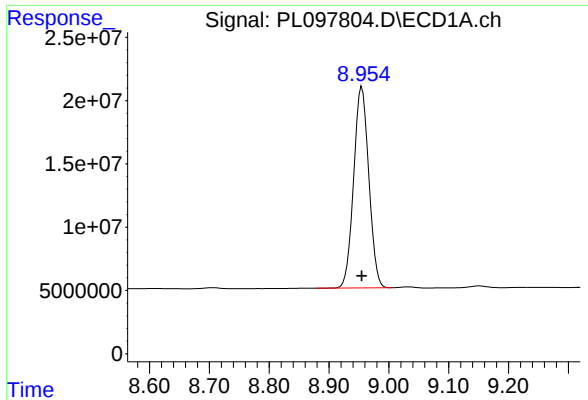

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: 0.000 min
Response: 279478919
Conc: 98.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

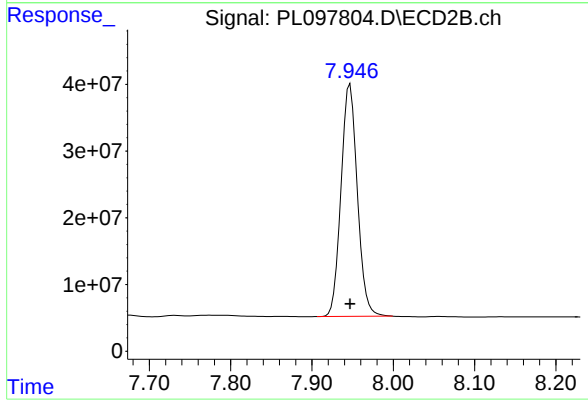

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 484905257
Conc: 98.85 ng/ml