

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
 Data File : PL097806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2025 11:52
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 12:09:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 12:09:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	2.799	186.7E6	323.1E6	50.000	50.000
28)	SA Decachlor...	8.956	7.947	144.1E6	248.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.649	3.803	115.3E6	130.5E6	500.000	500.000
24)	Chlordane-2	5.172	4.380	116.2E6	149.3E6	500.000	500.000
25)	Chlordane-3	5.874	5.012	438.2E6	443.0E6	500.000	500.000
26)	Chlordane-4	5.958	5.075	519.8E6	408.2E6	500.000	500.000
27)	Chlordane-5	6.794	5.967	89646038	160.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
Data File : PL097806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2025 11:52
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 12:09:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 12:09:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

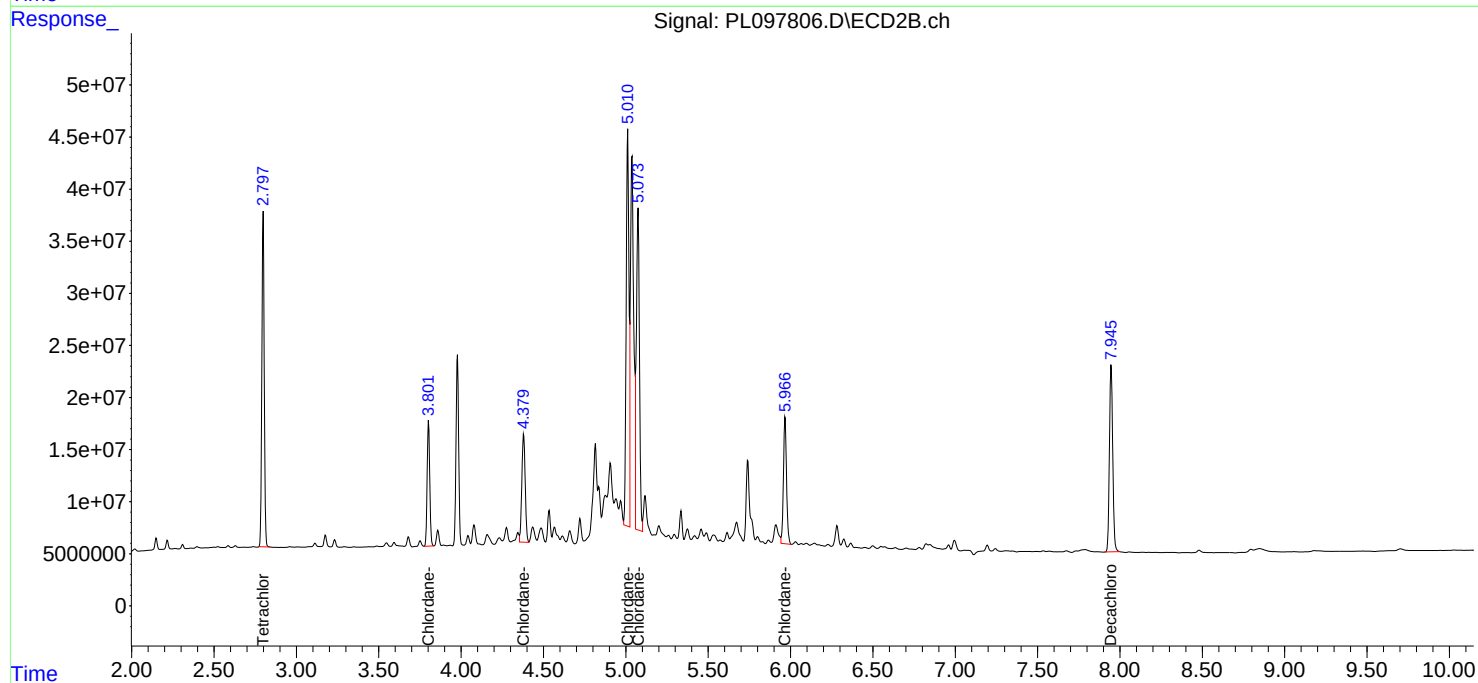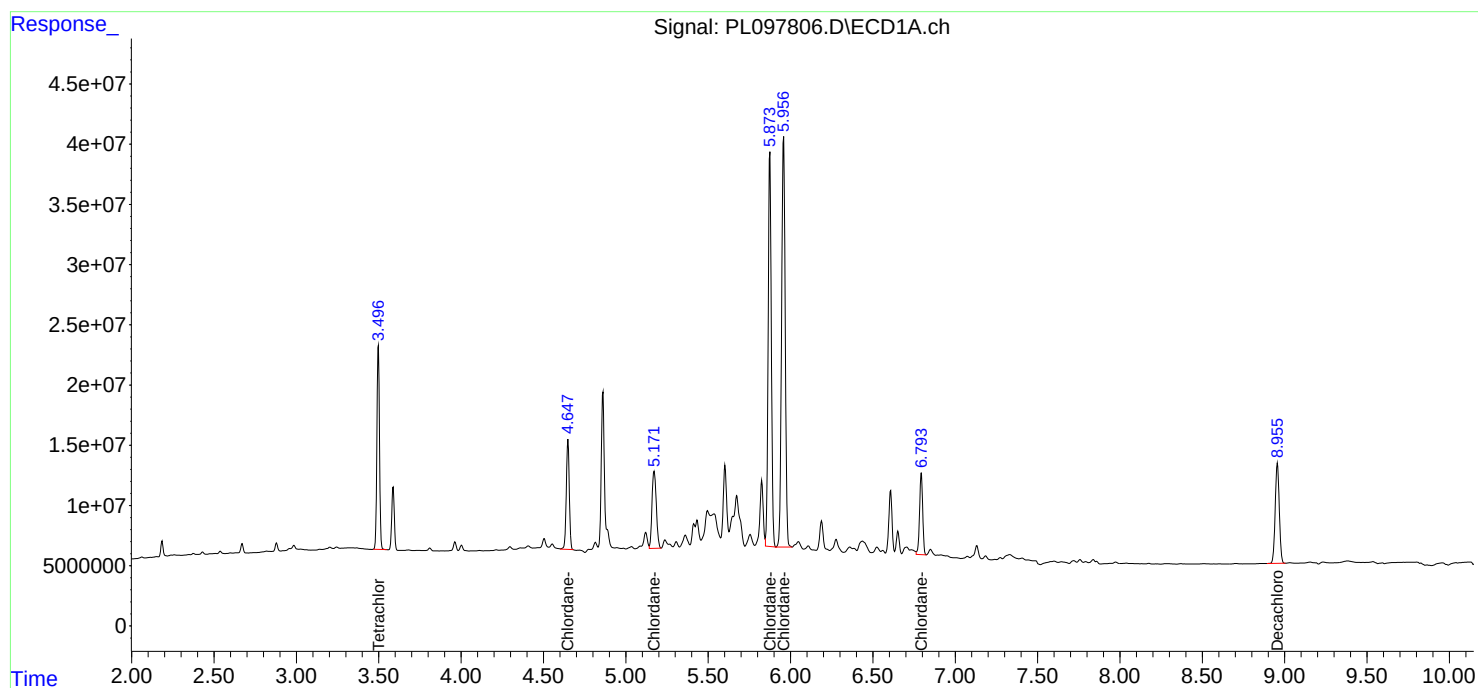


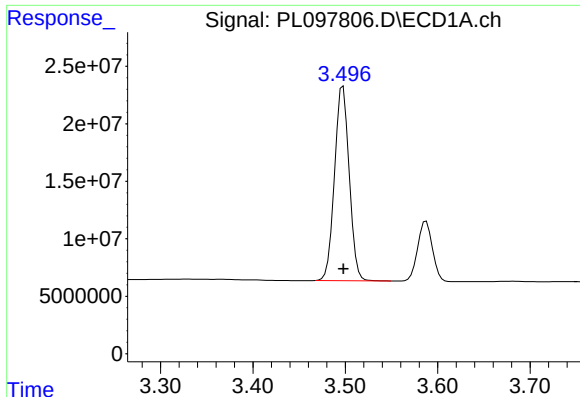

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 186656352
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

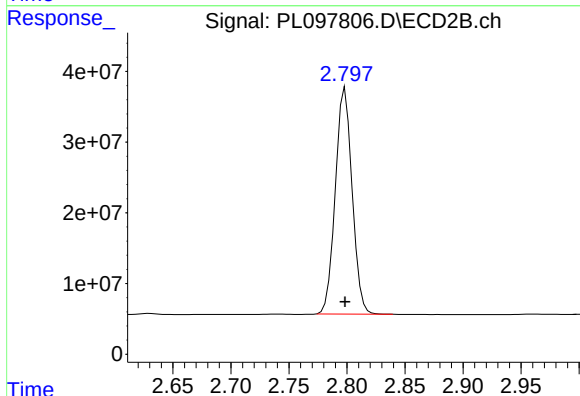


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: 0.000 min
Response: 323103351
Conc: 50.00 ng/ml

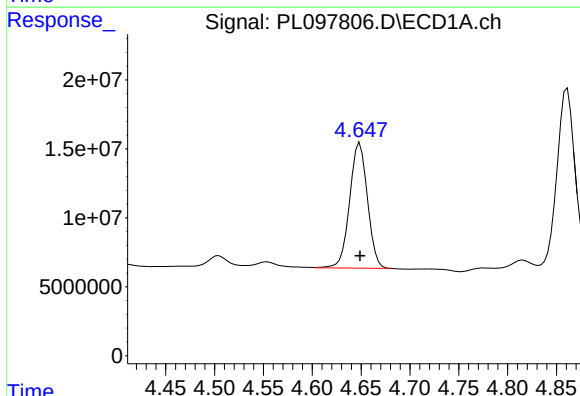


#23 Chlordane-1

R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 115274575
Conc: 500.00 ng/ml

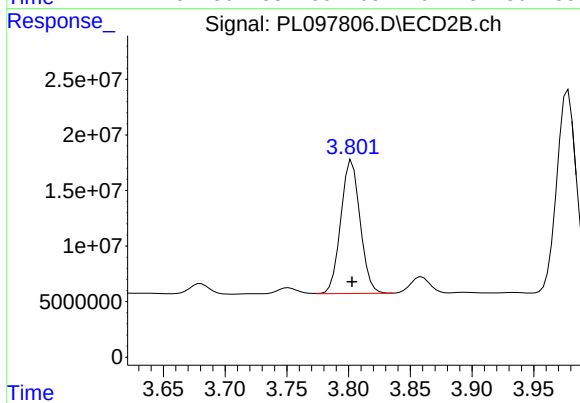

#23 Chlordane-1


R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 130538314
Conc: 500.00 ng/ml

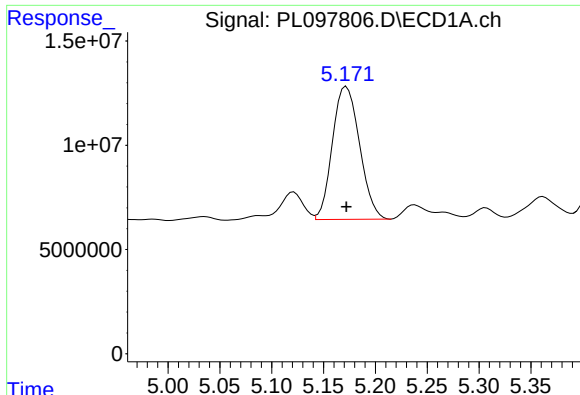

#24 Chlordane-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 116219671
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

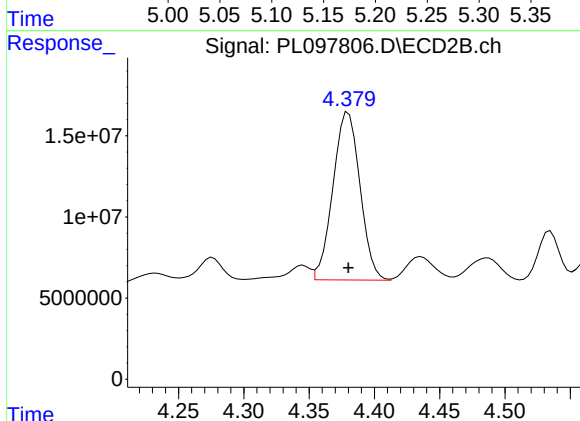


#24 Chlordane-2

R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 149319412
Conc: 500.00 ng/ml

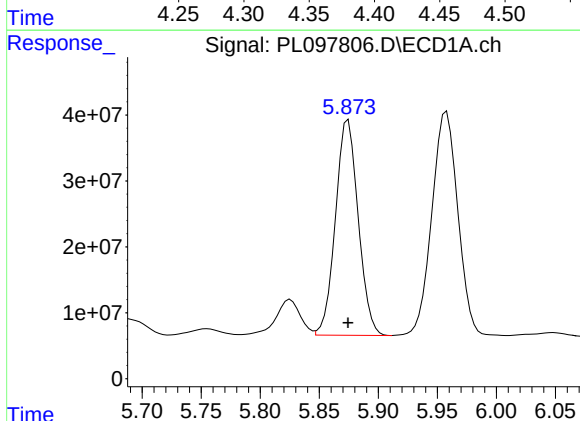


#25 Chlordane-3

R.T.: 5.874 min
Delta R.T.: 0.000 min
Response: 438164178
Conc: 500.00 ng/ml

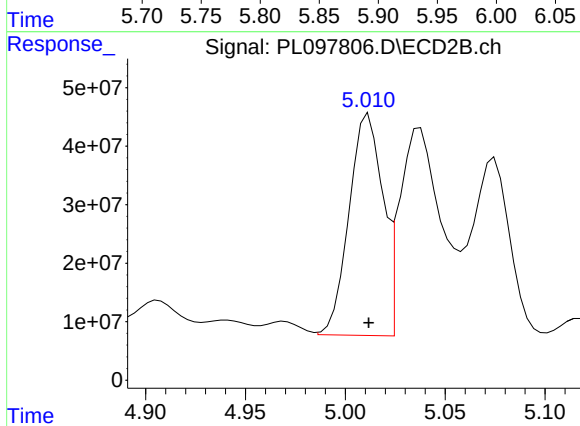

#25 Chlordane-3


R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 443014018
Conc: 500.00 ng/ml

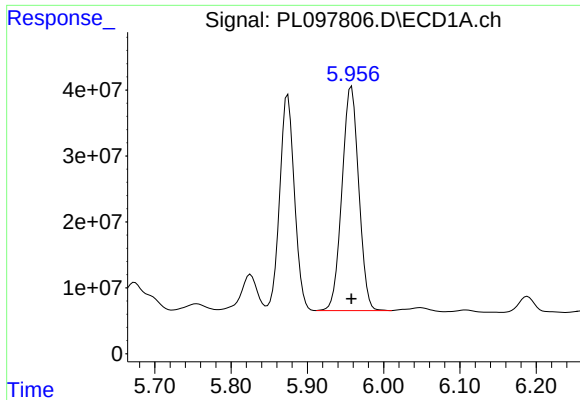

#26 Chlordane-4


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 519834850
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

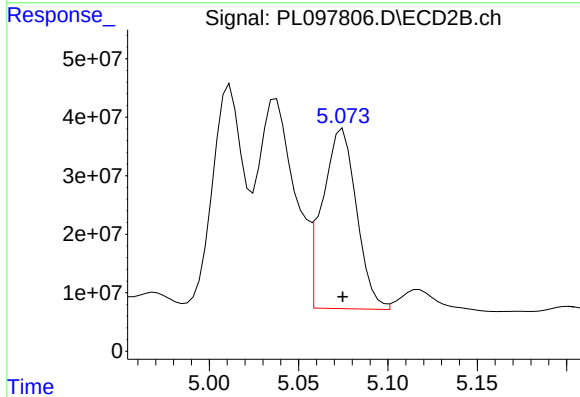


#26 Chlordane-4

R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 408174189
Conc: 500.00 ng/ml

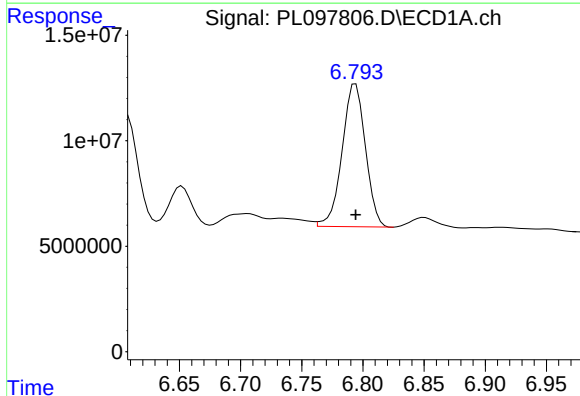


#27 Chlordane-5

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 89646038
Conc: 500.00 ng/ml

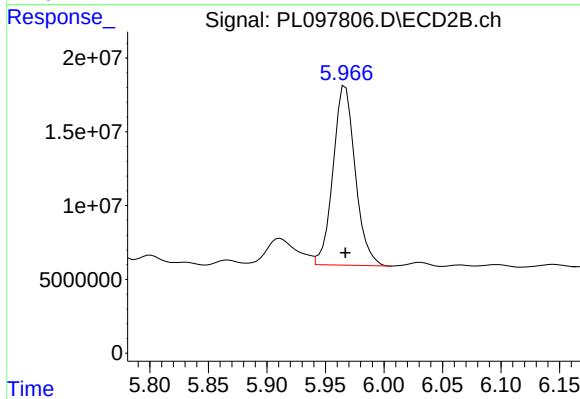

#27 Chlordane-5


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 160257299
Conc: 500.00 ng/ml

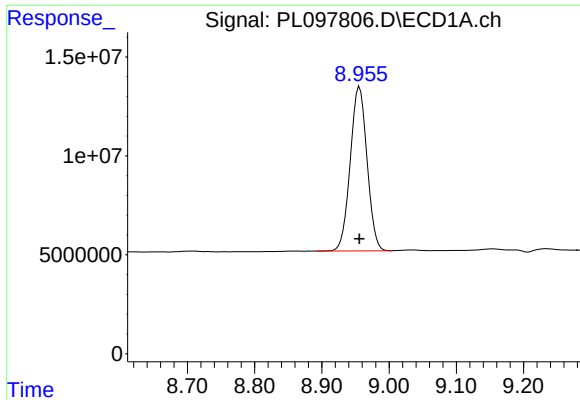

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.000 min
Response: 144062330
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

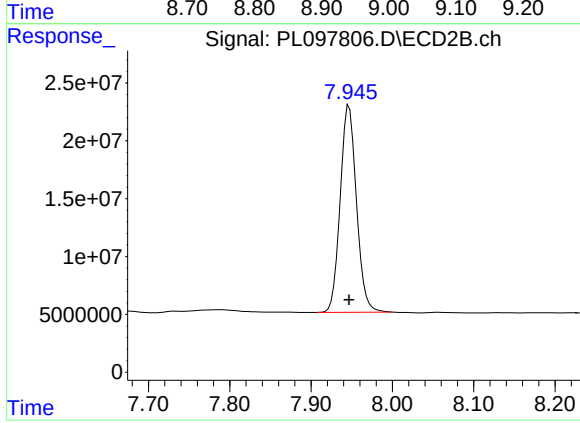

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 248091253
Conc: 50.00 ng/ml