

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
 Data File : PL097815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2025 13:54
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL120925CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:13:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:13:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	2.798	189.7E6	334.8E6	49.543	51.563
28)	SA Decachlor...	8.956	7.947	145.7E6	254.8E6	48.915	49.328
Target Compounds							
23)	Chlordane-1	4.649	3.802	117.6E6	134.5E6	500.417	508.150
24)	Chlordane-2	5.172	4.380	119.0E6	153.2E6	492.575	498.380
25)	Chlordane-3	5.874	5.011	445.9E6	453.7E6	505.369	519.659
26)	Chlordane-4	5.957	5.075	528.7E6	417.4E6	499.268	517.084
27)	Chlordane-5	6.794	5.967	91478525	165.0E6	503.000	501.464



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120925\
Data File : PL097815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2025 13:54
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL120925CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:13:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:13:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

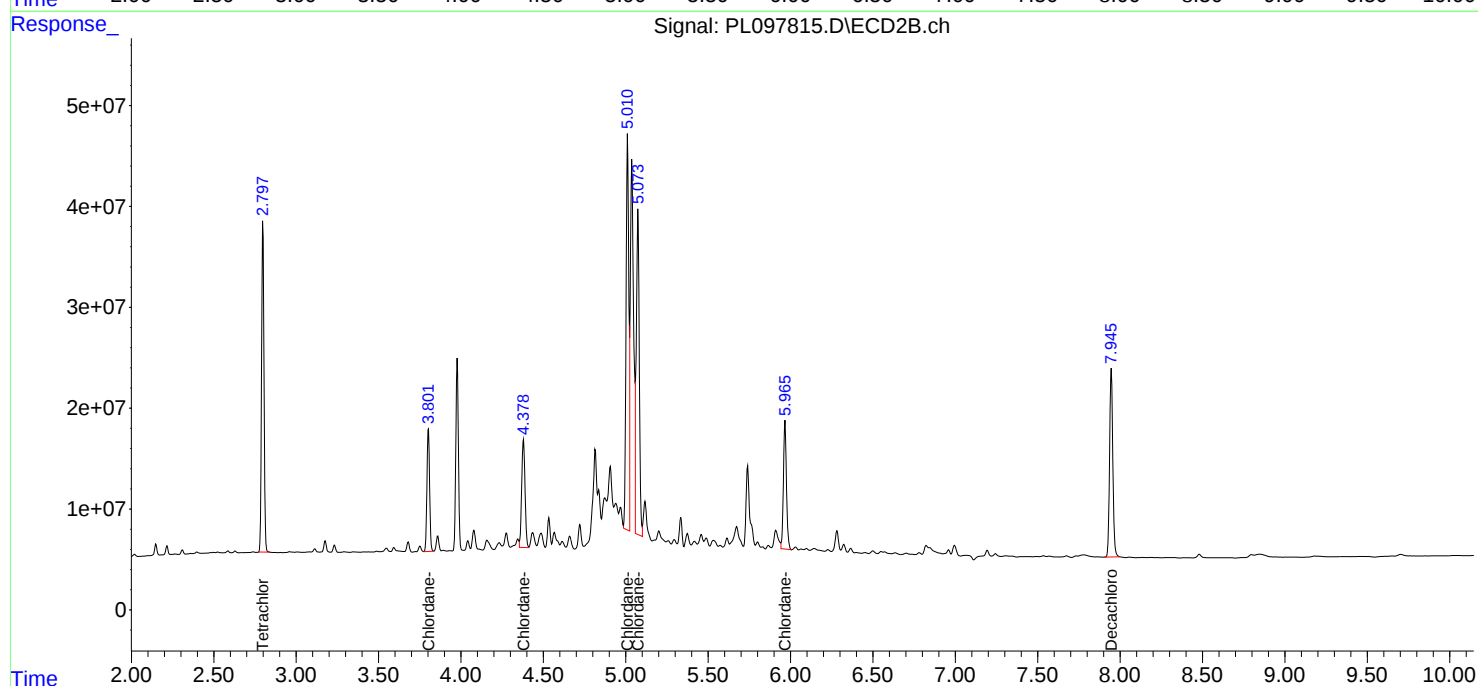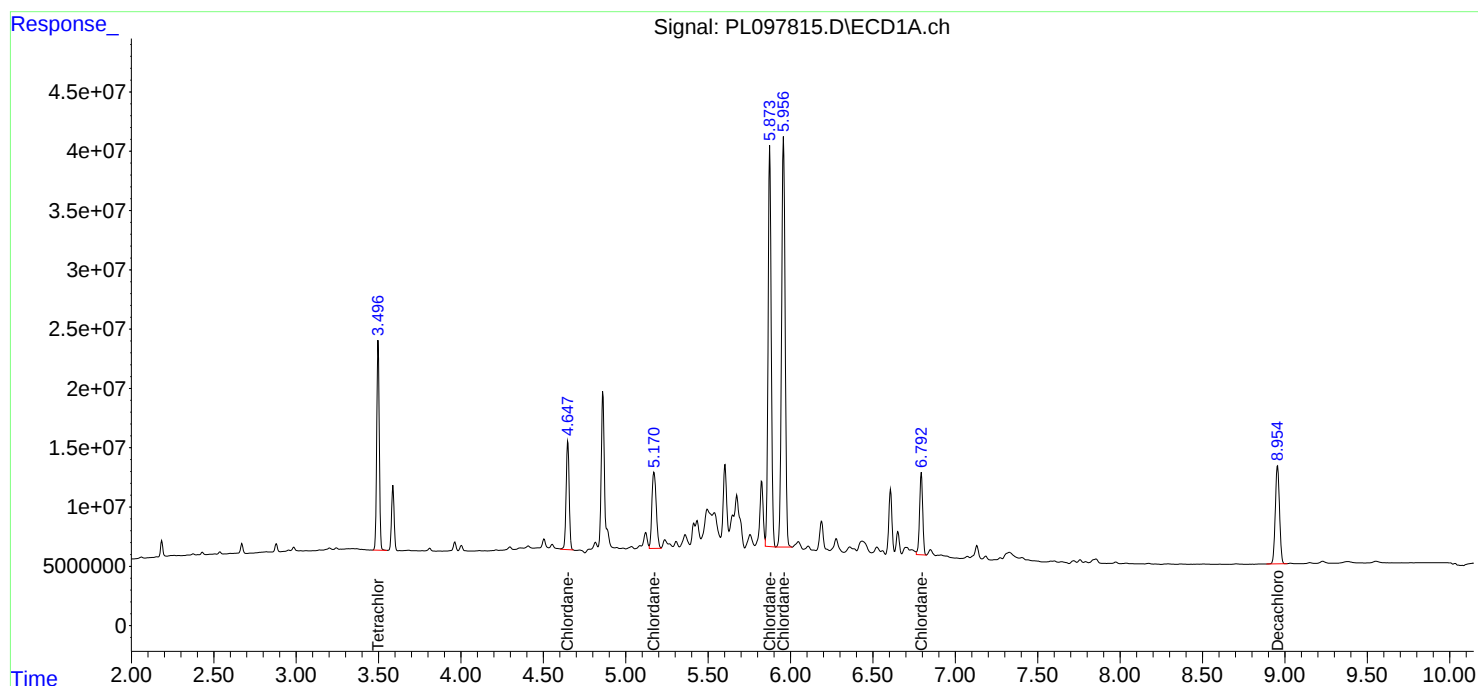


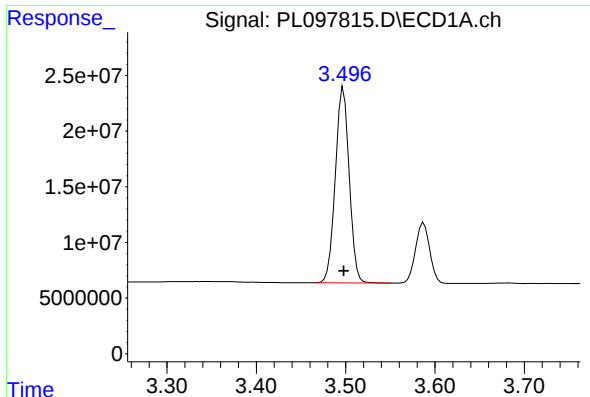

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 189671078
Conc: 49.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120925CHLOR

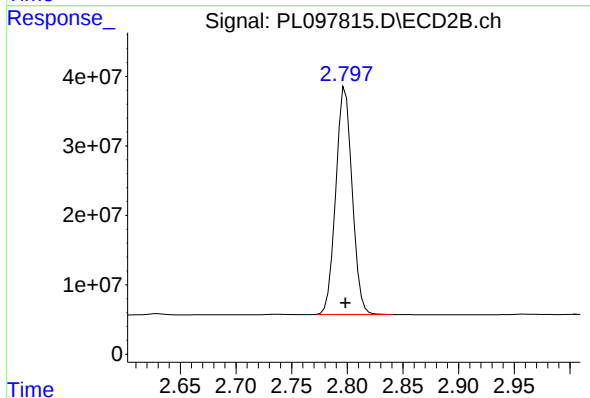


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: 0.000 min
Response: 334833124
Conc: 51.56 ng/ml

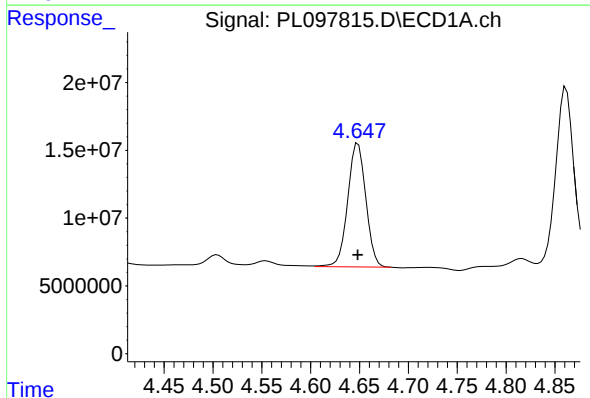


#23 Chlordane-1

R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 117570428
Conc: 500.42 ng/ml

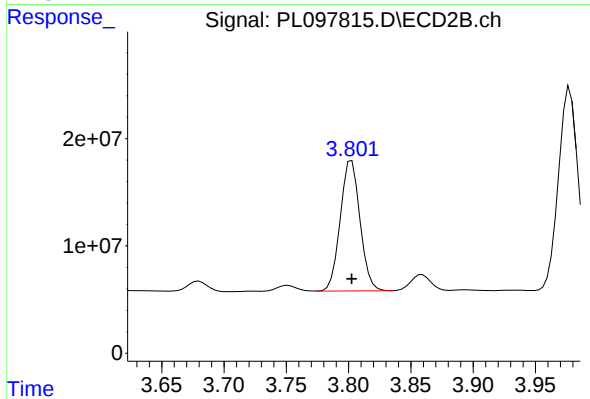

#23 Chlordane-1


R.T.: 3.802 min
Delta R.T.: 0.000 min
Response: 134471108
Conc: 508.15 ng/ml

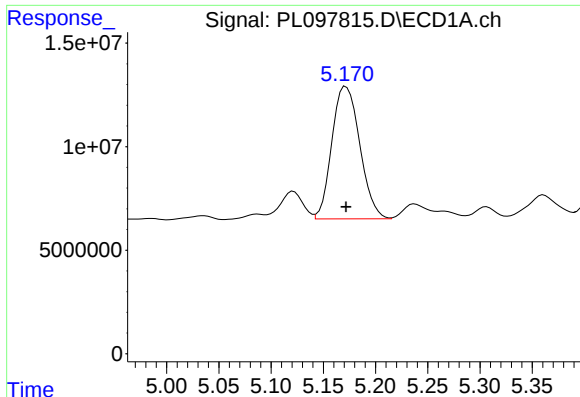

#24 Chlordane-2


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 119002123
Conc: 492.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120925CHLOR

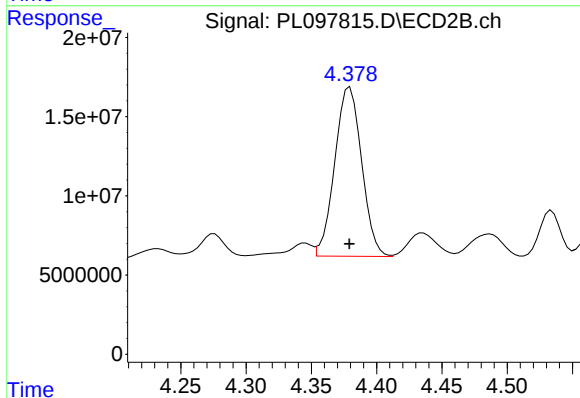


#24 Chlordane-2

R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 153191355
Conc: 498.38 ng/ml

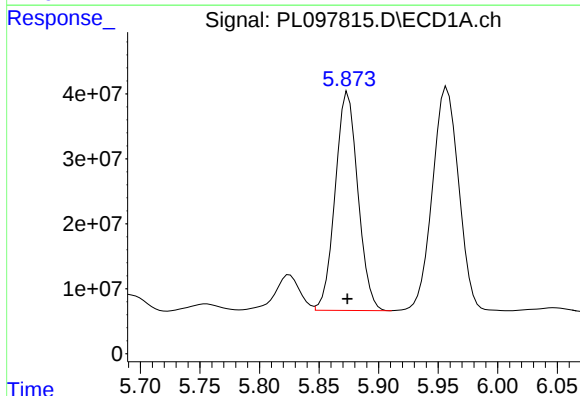


#25 Chlordane-3

R.T.: 5.874 min
Delta R.T.: 0.000 min
Response: 445914960
Conc: 505.37 ng/ml

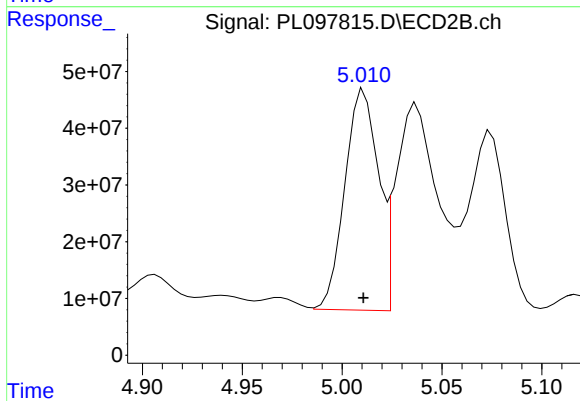

#25 Chlordane-3


R.T.: 5.011 min
Delta R.T.: 0.000 min
Response: 453733156
Conc: 519.66 ng/ml

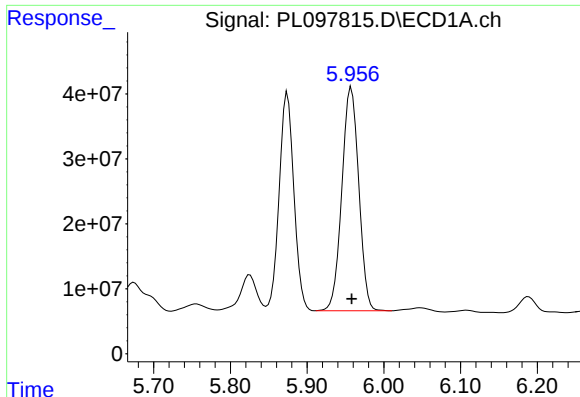

#26 Chlordane-4


R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 528683237
Conc: 499.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120925CHLOR

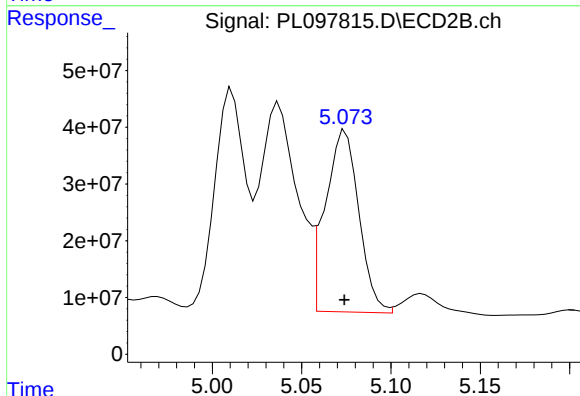


#26 Chlordane-4

R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 417441079
Conc: 517.08 ng/ml

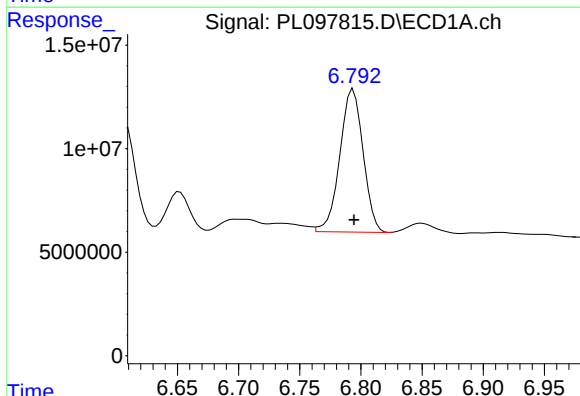


#27 Chlordane-5

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 91478525
Conc: 503.00 ng/ml

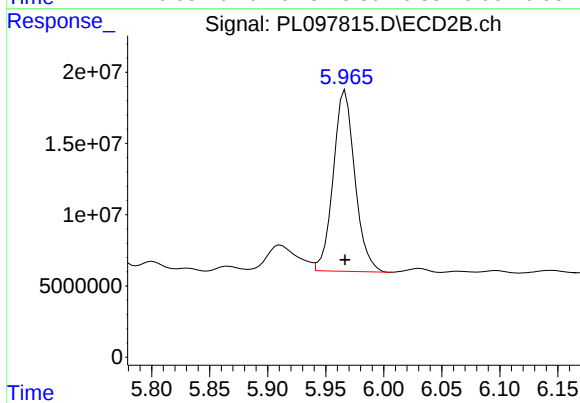

#27 Chlordane-5


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 164966182
Conc: 501.46 ng/ml

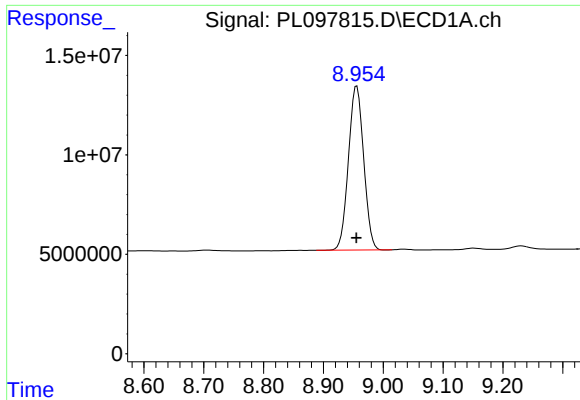

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.000 min
Response: 145685281
Conc: 48.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120925CHLOR

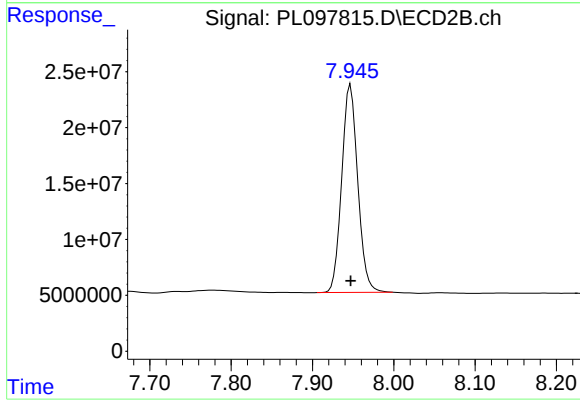

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 254777787
Conc: 49.33 ng/ml