

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121018\
 Data File : PL042917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2018 16:12
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 00:47:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	135.3E6	68830150	22.069	23.223
28)	SA Decachlor...	8.201	9.228	138.7E6	58457099	21.242	22.410
Target Compounds							
2)	A alpha-BHC	3.897	0.000	4004134	0	0.424	N.D. #
6)	B beta-BHC	4.397f	0.000	3056226	0	0.829	N.D. #
7)	B delta-BHC	0.000	5.155	0	2859504	N.D.	0.665 #
8)	B Heptachlo...	0.000	5.991	0	6910740	N.D.	1.822 #
10)	B gamma-Chl...	0.000	6.228	0	614195	N.D.	0.167 #
14)	MA Endrin	6.017	0.000	5278519	0	0.733	N.D. #
23)	Chlordane-1	4.361	5.155	883535	2859504	3.288	20.232 #
25)	Chlordane-3	0.000	6.228	0	614195	N.D.	1.251 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121018\
Data File : PL042917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2018 16:12
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 00:47:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

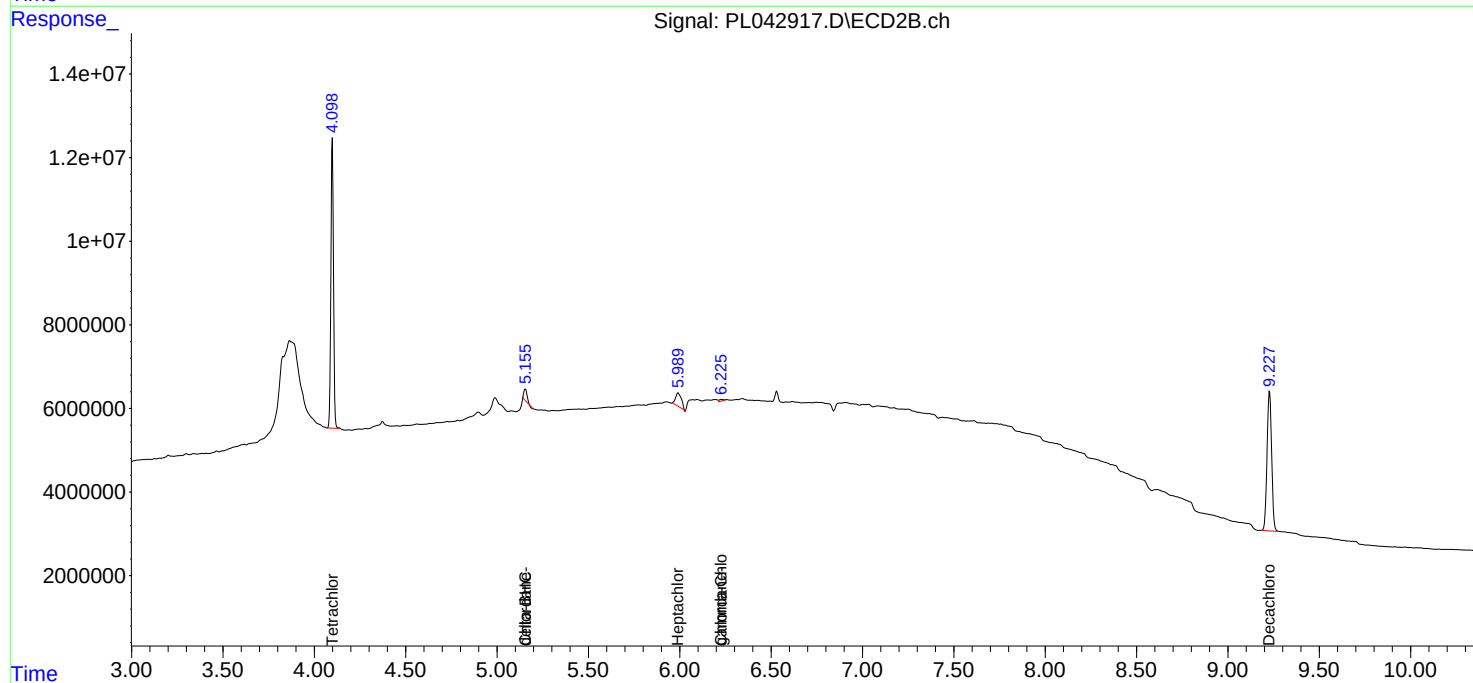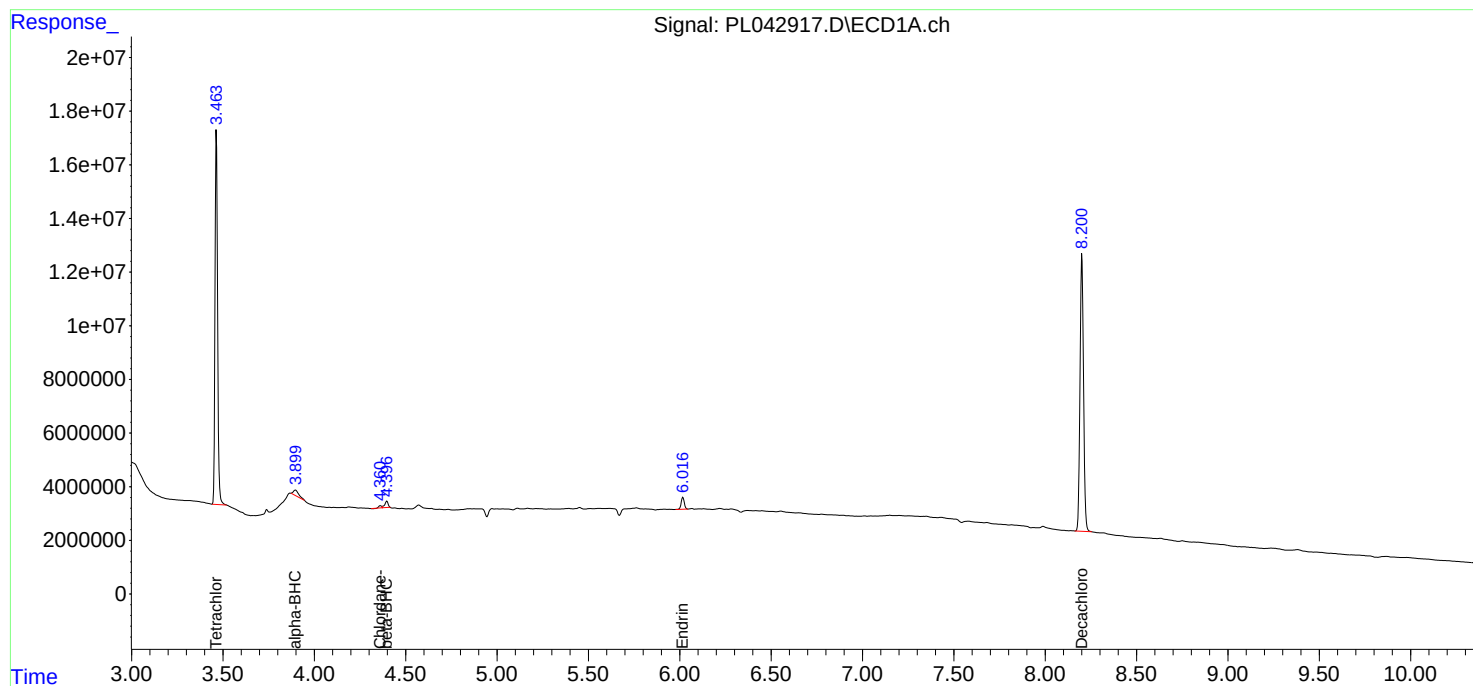


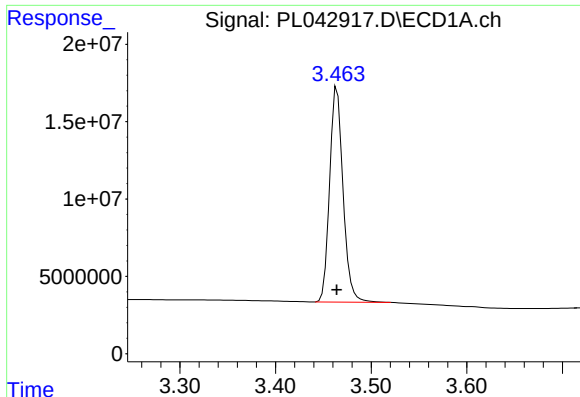

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 135349761
Conc: 22.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

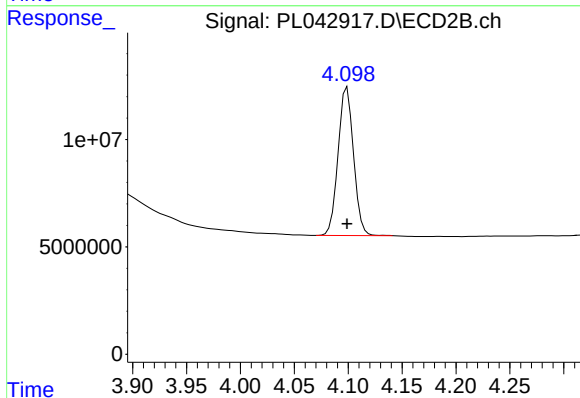


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 68830150
Conc: 23.22 ng/ml

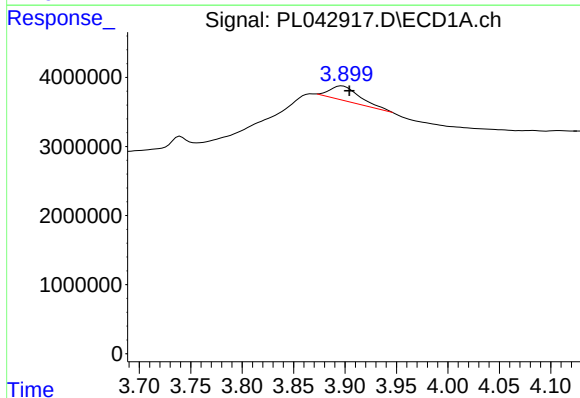


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: -0.007 min
Response: 4004134
Conc: 0.42 ng/ml

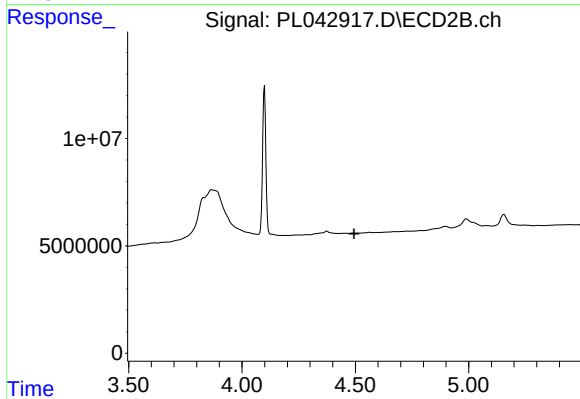

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

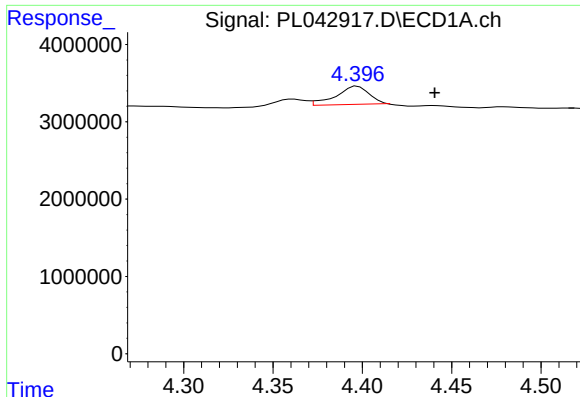

#6 beta-BHC


R.T.: 4.397 min
Delta R.T.: -0.043 min
Response: 3056226
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

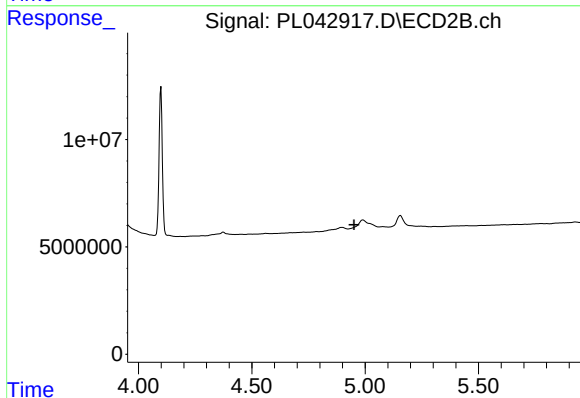


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

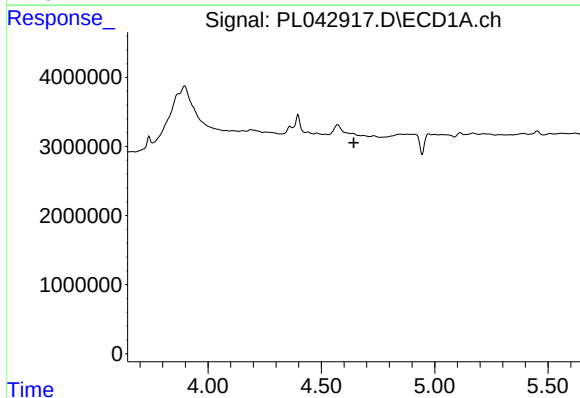


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

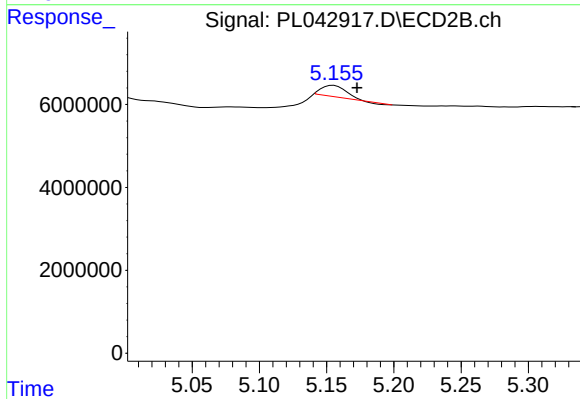

#7 delta-BHC


R.T.: 5.155 min
Delta R.T.: -0.017 min
Response: 2859504
Conc: 0.67 ng/ml

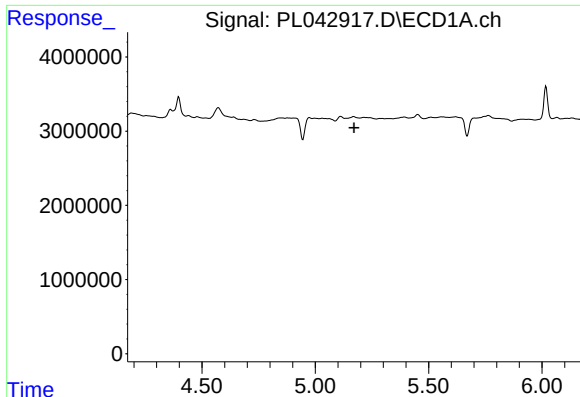

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

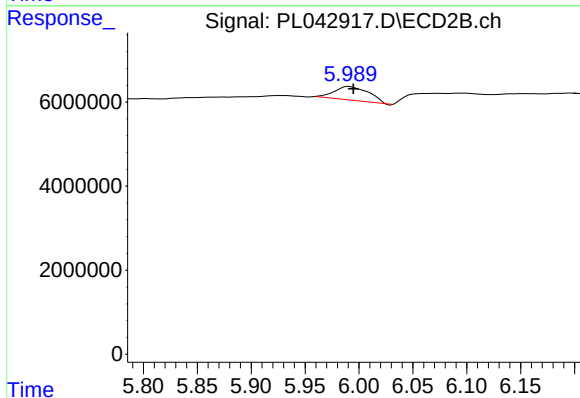


#8 Heptachlor epoxide

R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 6910740
Conc: 1.82 ng/ml

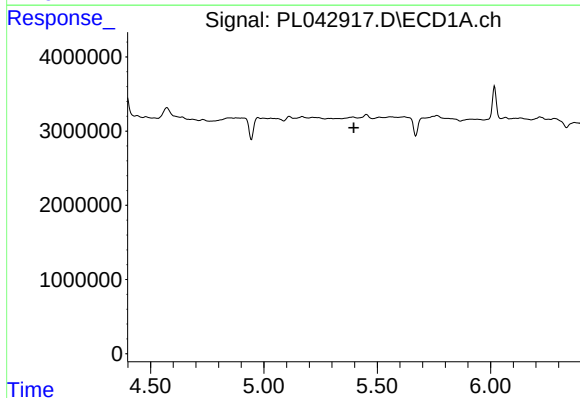


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

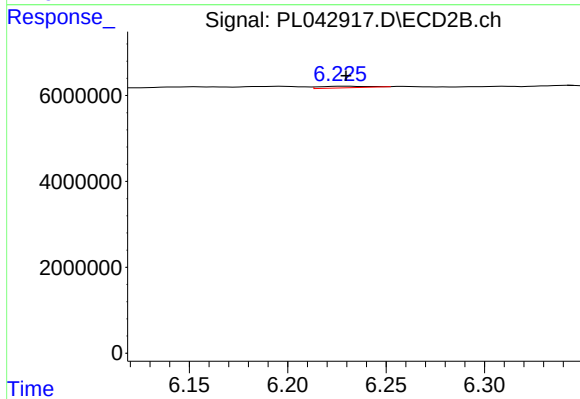

#10 gamma-Chlordane


R.T.: 6.228 min
Delta R.T.: -0.002 min
Response: 614195
Conc: 0.17 ng/ml

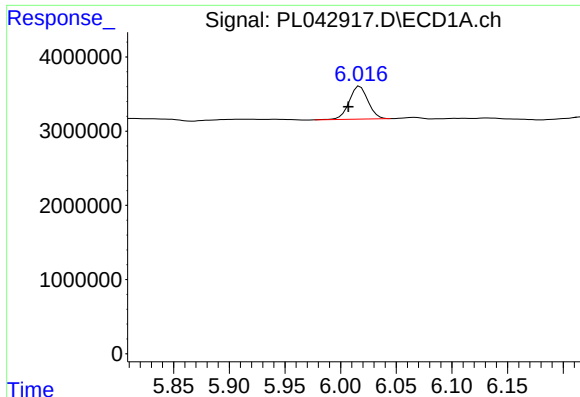

#14 Endrin


R.T.: 6.017 min
Delta R.T.: 0.010 min
Response: 5278519
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

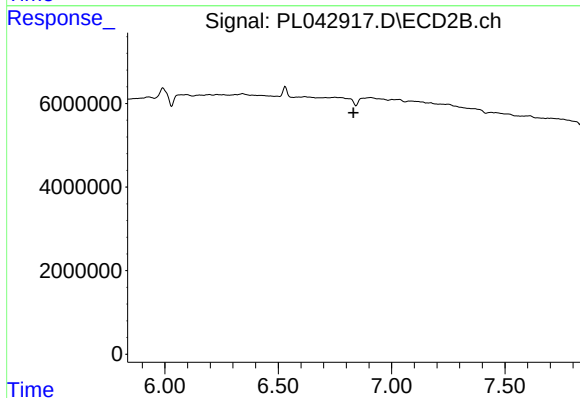


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

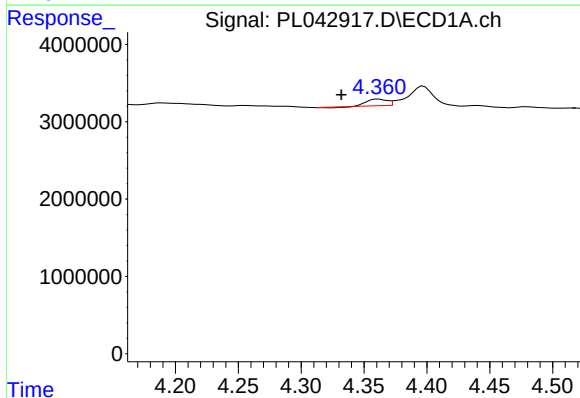


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.029 min
Response: 883535
Conc: 3.29 ng/ml

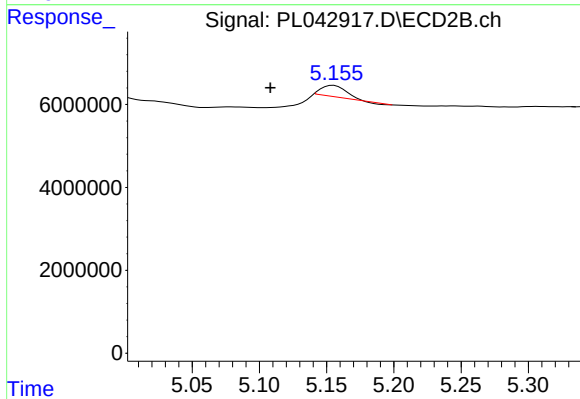

#23 Chlordane-1


R.T.: 5.155 min
Delta R.T.: 0.047 min
Response: 2859504
Conc: 20.23 ng/ml

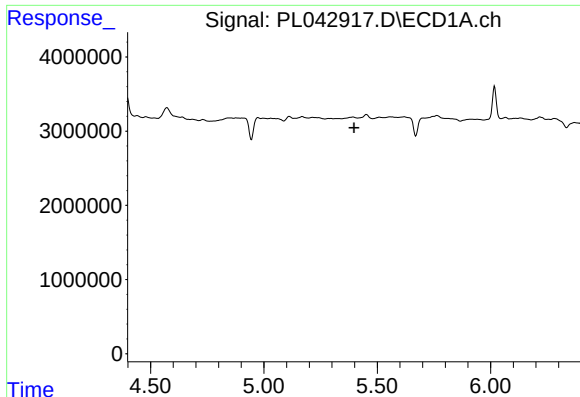

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

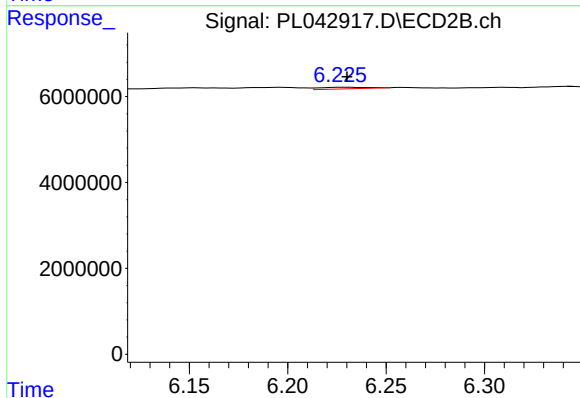


#25 Chlordane-3

R.T.: 6.228 min
Delta R.T.: -0.002 min
Response: 614195
Conc: 1.25 ng/ml

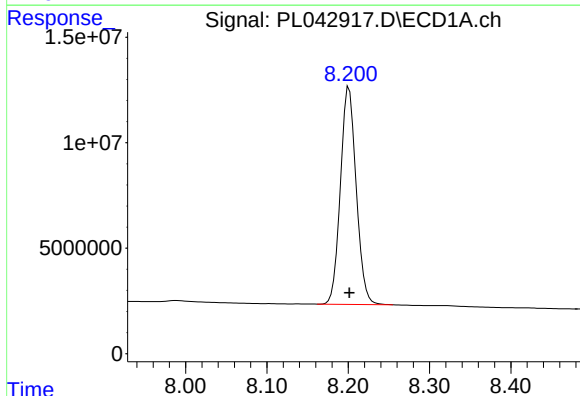

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 138712415
Conc: 21.24 ng/ml

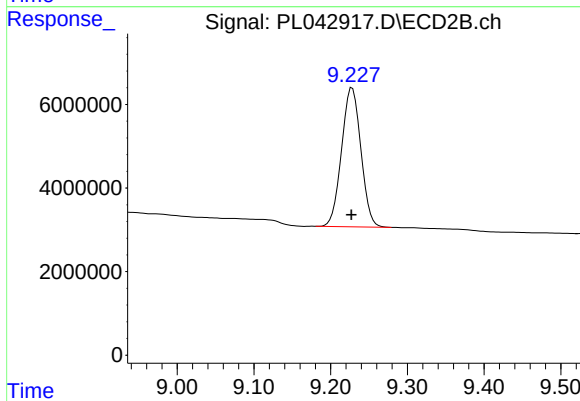

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.001 min
Response: 58457099
Conc: 22.41 ng/ml