

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121019\
 Data File : PL054899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2019 15:44
 Operator : SG\AJ
 Sample : K6174-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WATER-COMP

Manual Integrations
 APPROVED

Ankita
 12/11/2019 10:03:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 00:39:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.050	185.3E6	50892923	15.930m	19.944 #
28)	SA Decachlor...	8.318	9.149	188.2E6	48609337	19.656	20.276

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121019\
Data File : PL054899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2019 15:44
Operator : SG\AJ
Sample : K6174-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

Ankita
12/11/2019 10:03:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 00:39:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

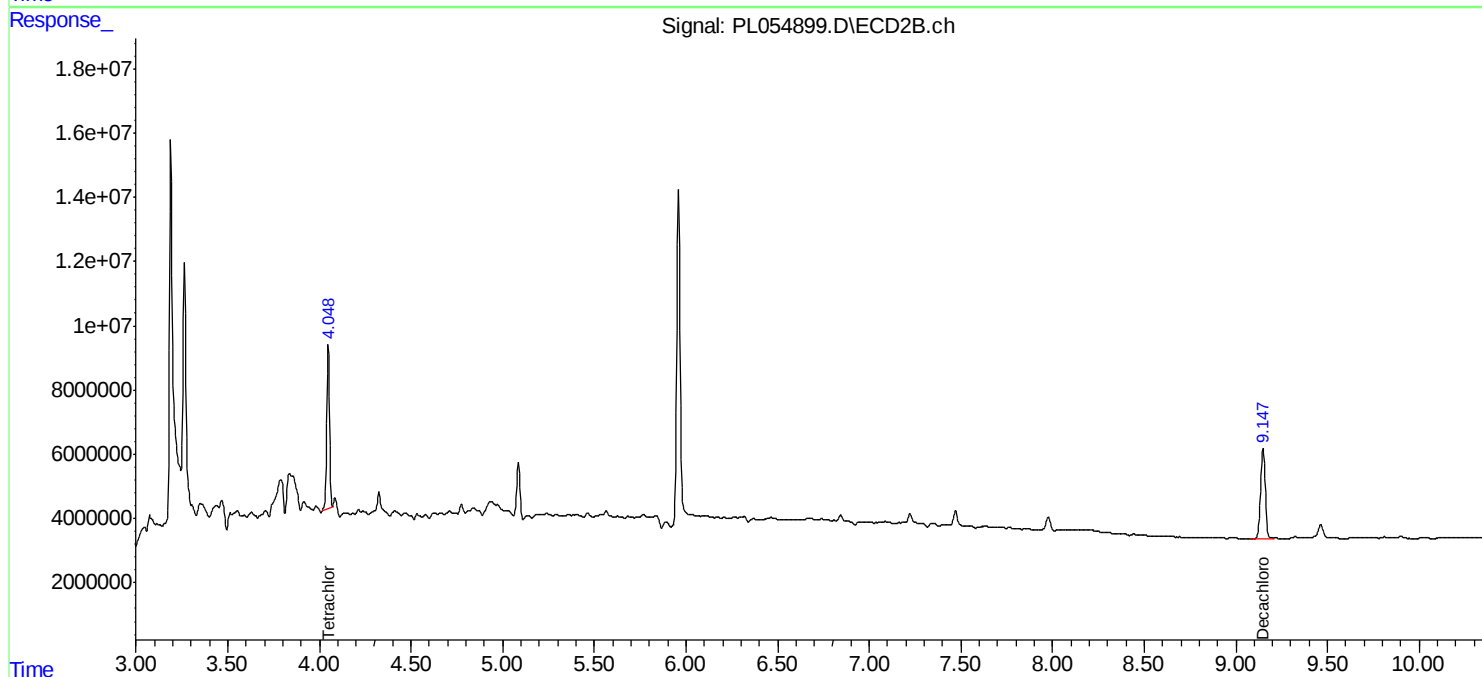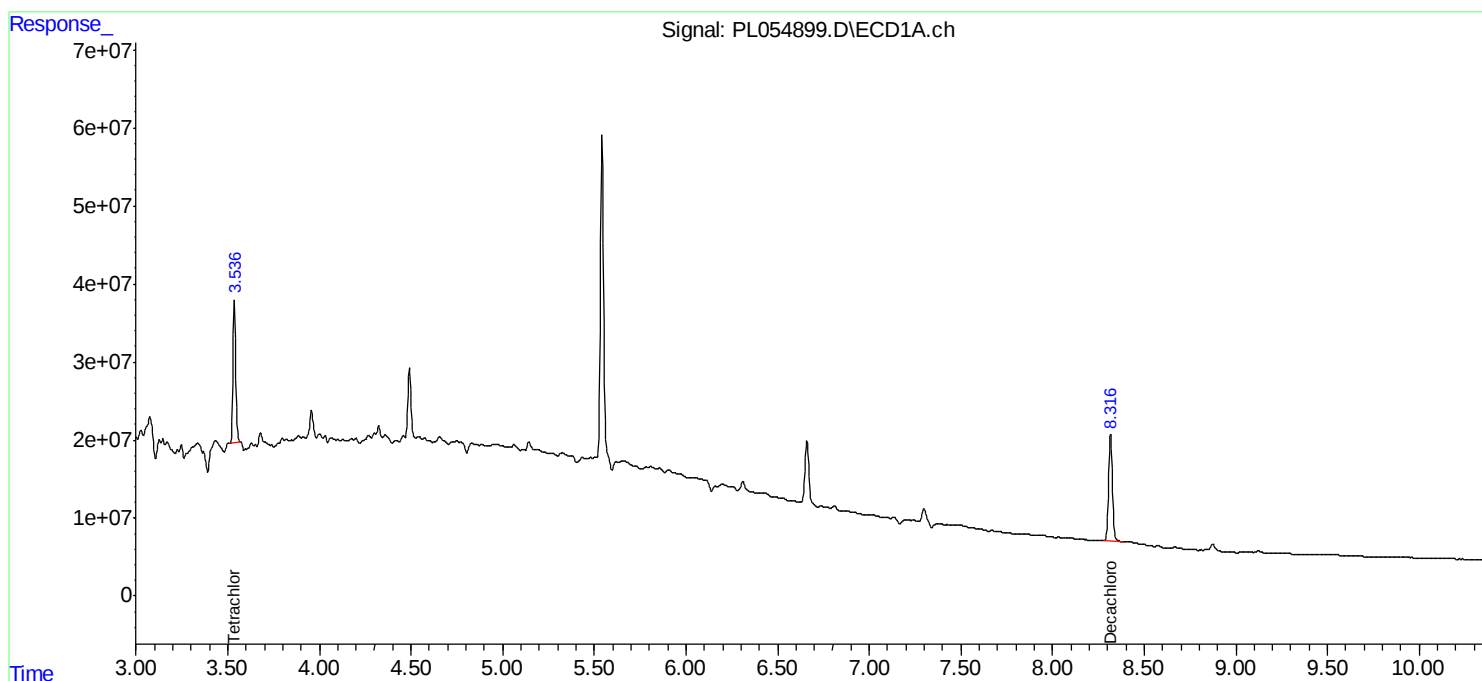

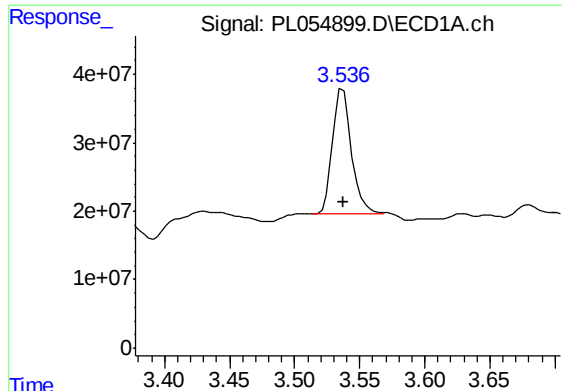


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 185326993
Conc: 15.93 ng/ml m

Instrument :
ECD_L
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

Ankita
12/11/2019 10:03:59 AM

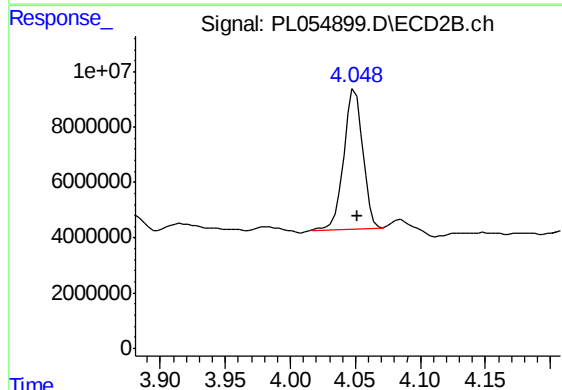


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 50892923
Conc: 19.94 ng/ml

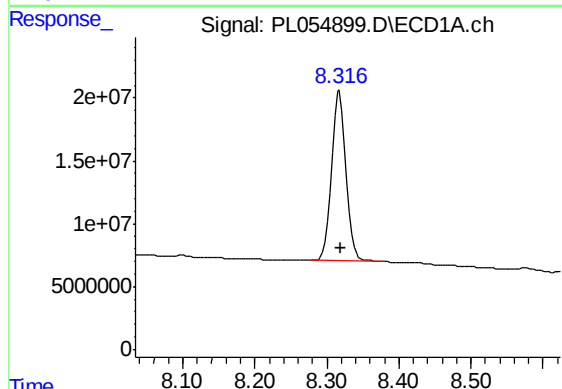

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.002 min
Response: 188232440
Conc: 19.66 ng/ml

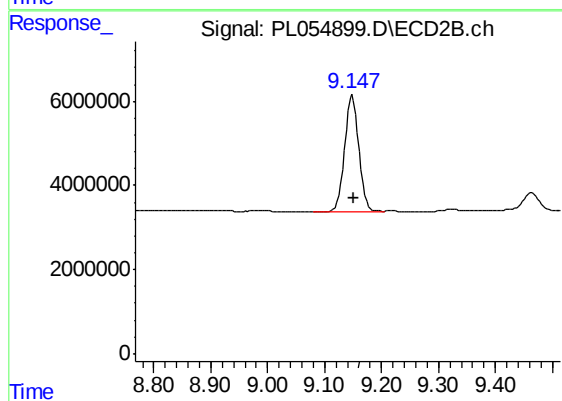

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.003 min
Response: 48609337
Conc: 20.28 ng/ml