

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
 Data File : PL071369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2021 09:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 22:24:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.502	11081048	27635536	23.592	22.022
28)	SA Decachlor...	10.329	11.395	15044080	24334750	20.776	17.507
Target Compounds							
2)	A alpha-BHC	5.253f	6.060f	494314	818232	0.756	0.442 #
7)	B delta-BHC	0.000	6.977f	0	1680395	N.D.	0.988 #
15)	B Endosulfa...	8.270f	0.000	181868	0	0.311	N.D. #
20)	A Methoxychlor	9.020	0.000	253308	0	0.701	N.D. #
27)	Chlordane-5	8.270f	0.000	181868	0	7.619	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
Data File : PL071369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2021 09:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 22:24:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

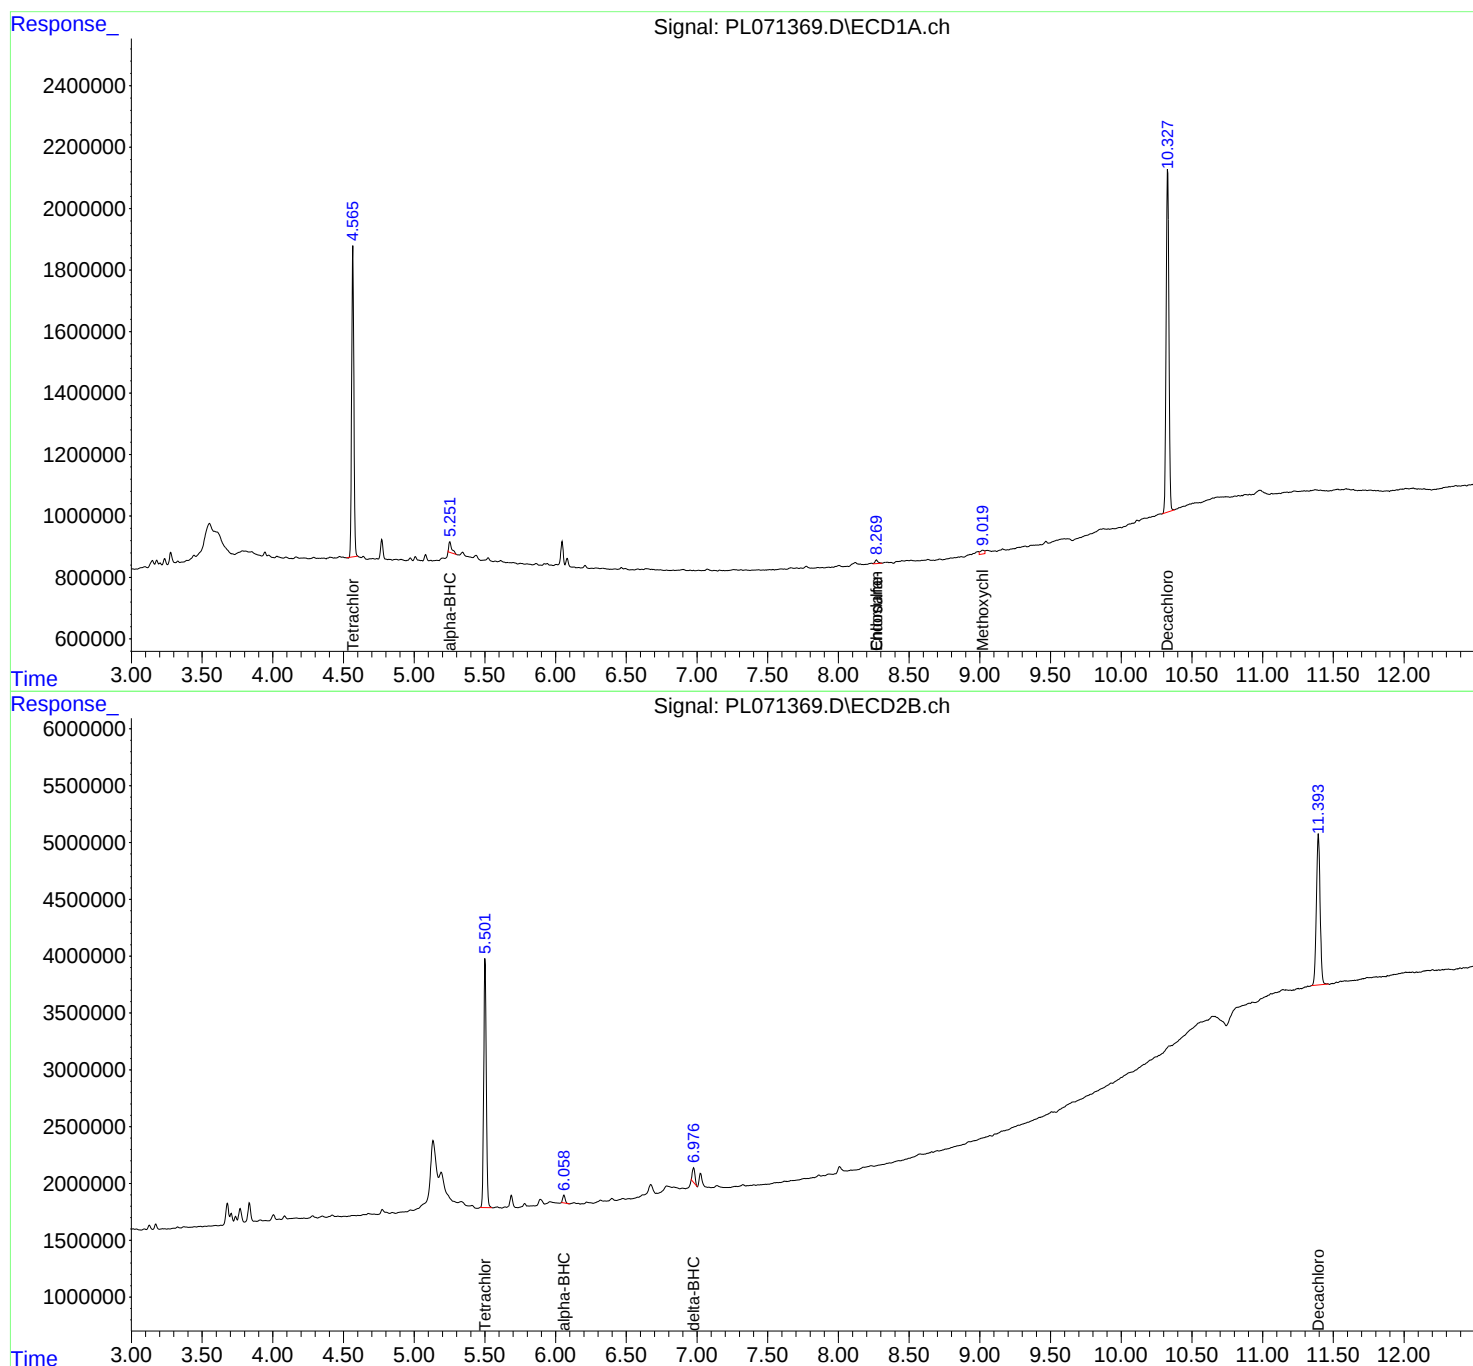


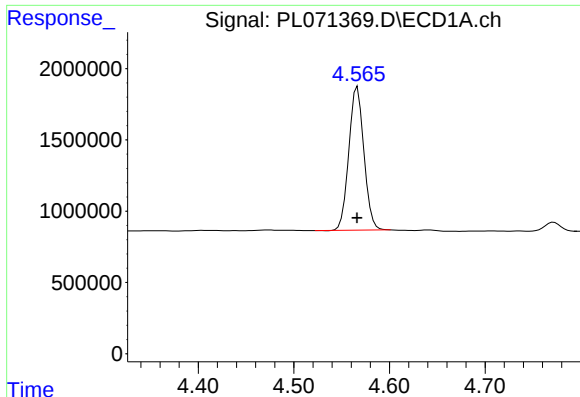

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: 0.000 min
Response: 11081048
Conc: 23.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

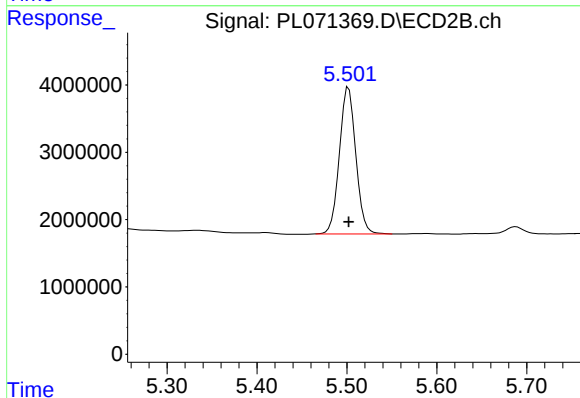


#1 Tetrachloro-m-xylene

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 27635536
Conc: 22.02 ng/ml

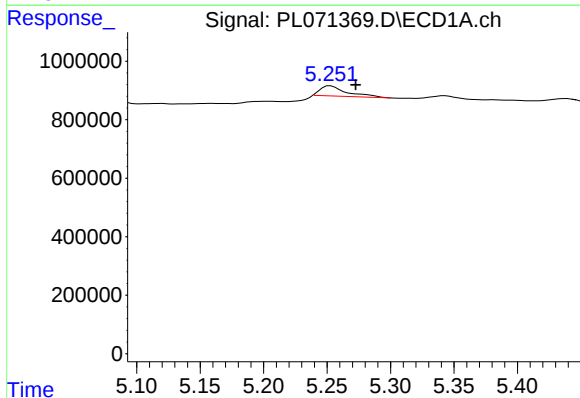


#2 alpha-BHC

R.T.: 5.253 min
Delta R.T.: -0.020 min
Response: 494314
Conc: 0.76 ng/ml

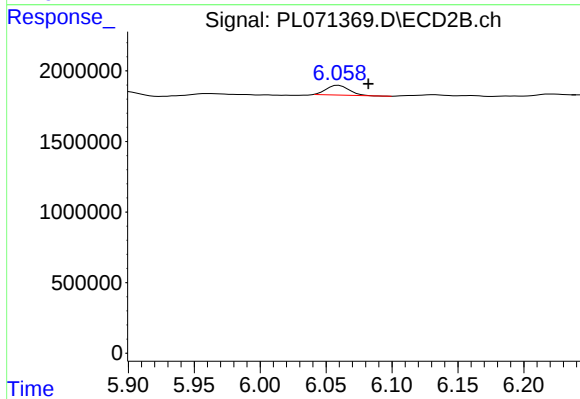

#2 alpha-BHC


R.T.: 6.060 min
Delta R.T.: -0.022 min
Response: 818232
Conc: 0.44 ng/ml

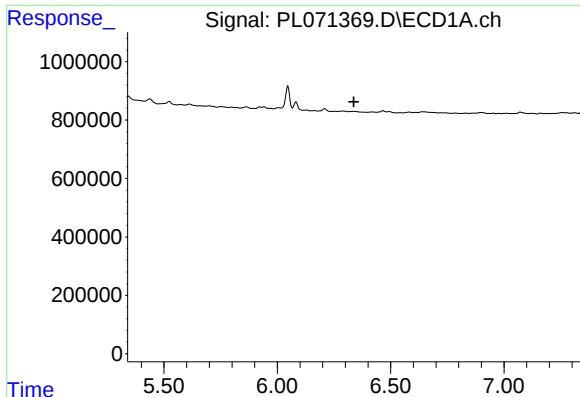

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

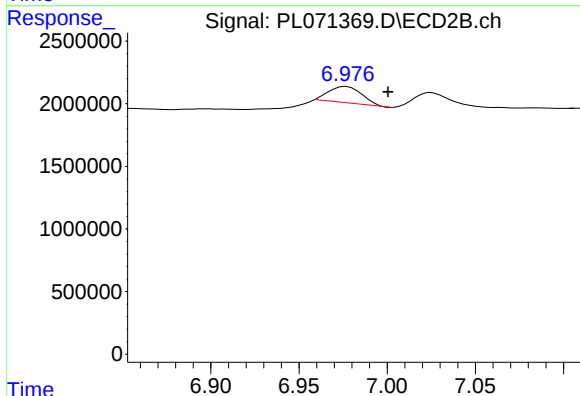


#7 delta-BHC

R.T.: 6.977 min
Delta R.T.: -0.023 min
Response: 1680395
Conc: 0.99 ng/ml

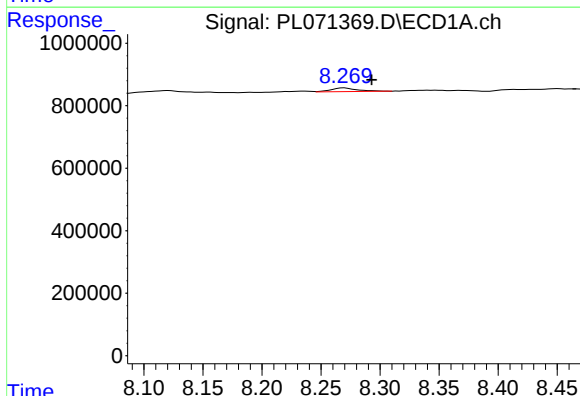


#15 Endosulfan II

R.T.: 8.270 min
Delta R.T.: -0.023 min
Response: 181868
Conc: 0.31 ng/ml

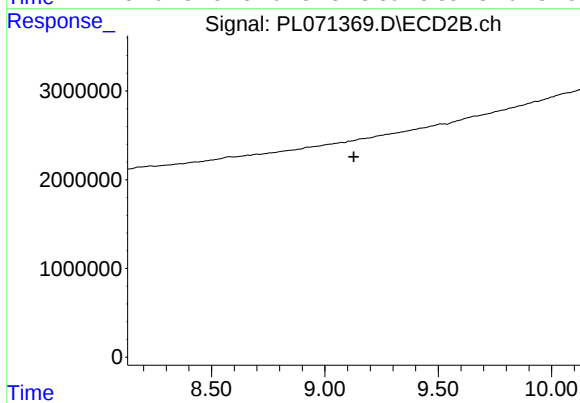

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.127 min
Response: 0
Conc: N.D.

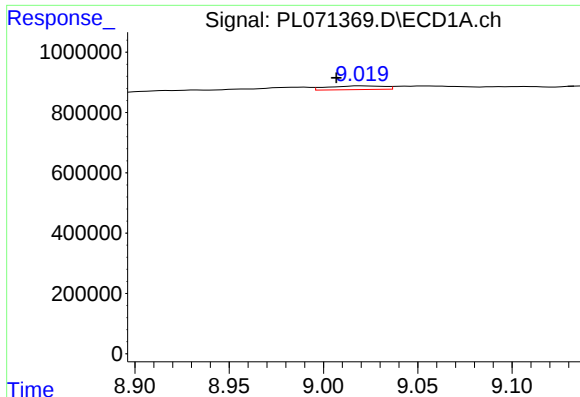

#20 Methoxychlor


R.T.: 9.020 min
Delta R.T.: 0.014 min
Response: 253308
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

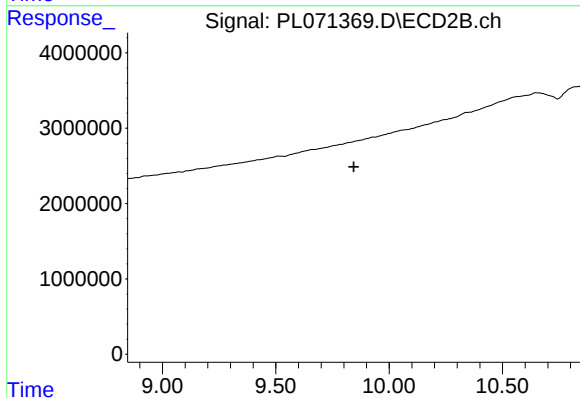


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

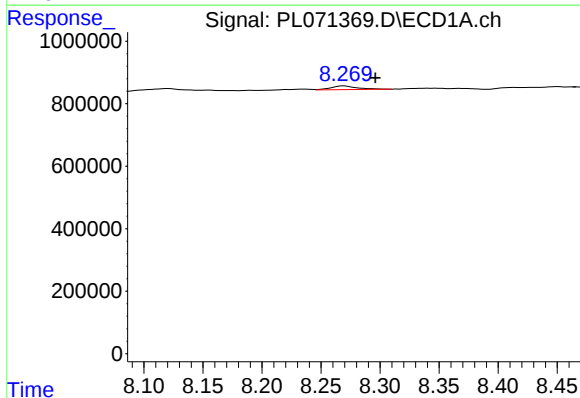


#27 Chlordane-5

R.T.: 8.270 min
Delta R.T.: -0.026 min
Response: 181868
Conc: 7.62 ng/ml

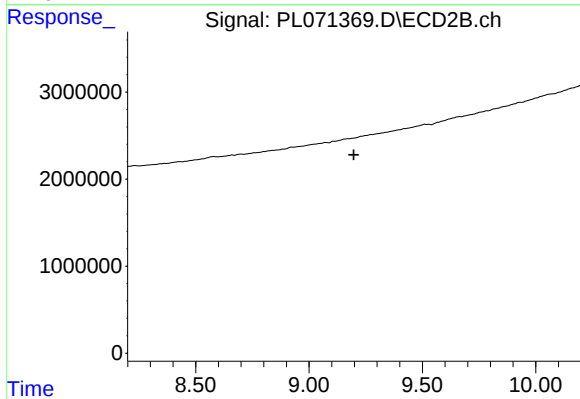

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

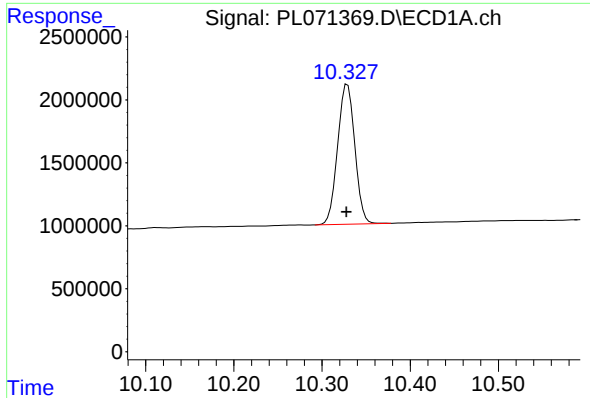

#28 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: 0.001 min
Response: 15044080
Conc: 20.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

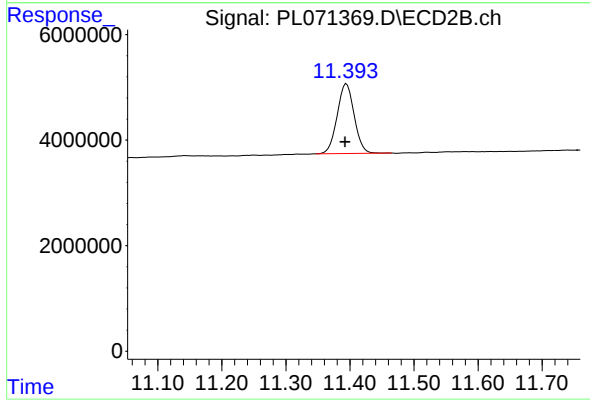

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.003 min
Response: 24334750
Conc: 17.51 ng/ml