

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
 Data File : PL071378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2021 17:18
 Operator : AR\AJ
 Sample : M4966-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 22:27:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.497	9312086	24372147	19.826	19.421
28)	SA Decachlor...	10.328	11.393	13559249	23693279	18.726	17.046
Target Compounds							
6)	B beta-BHC	0.000	6.758f	0	12023086	N.D.	13.661 #
7)	B delta-BHC	0.000	7.020f	0	3667193	N.D.	2.157 #
8)	B Heptachlo...	0.000	7.934f	0	2143829	N.D.	1.349 #
15)	B Endosulfa...	8.269f	9.153f	157352	590470	0.269	0.438 #
16)	A 4,4'-DDD	0.000	9.061f	0	858610	N.D.	0.740 #
18)	B Endrin al...	0.000	9.247f	0	43546	N.D.	0.042 #
23)	Chlordane-1	5.869f	6.902f	328599	669718	19.543	12.621 #
27)	Chlordane-5	8.269f	0.000	157352	0	6.592	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
Data File : PL071378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2021 17:18
Operator : AR\AJ
Sample : M4966-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 22:27:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

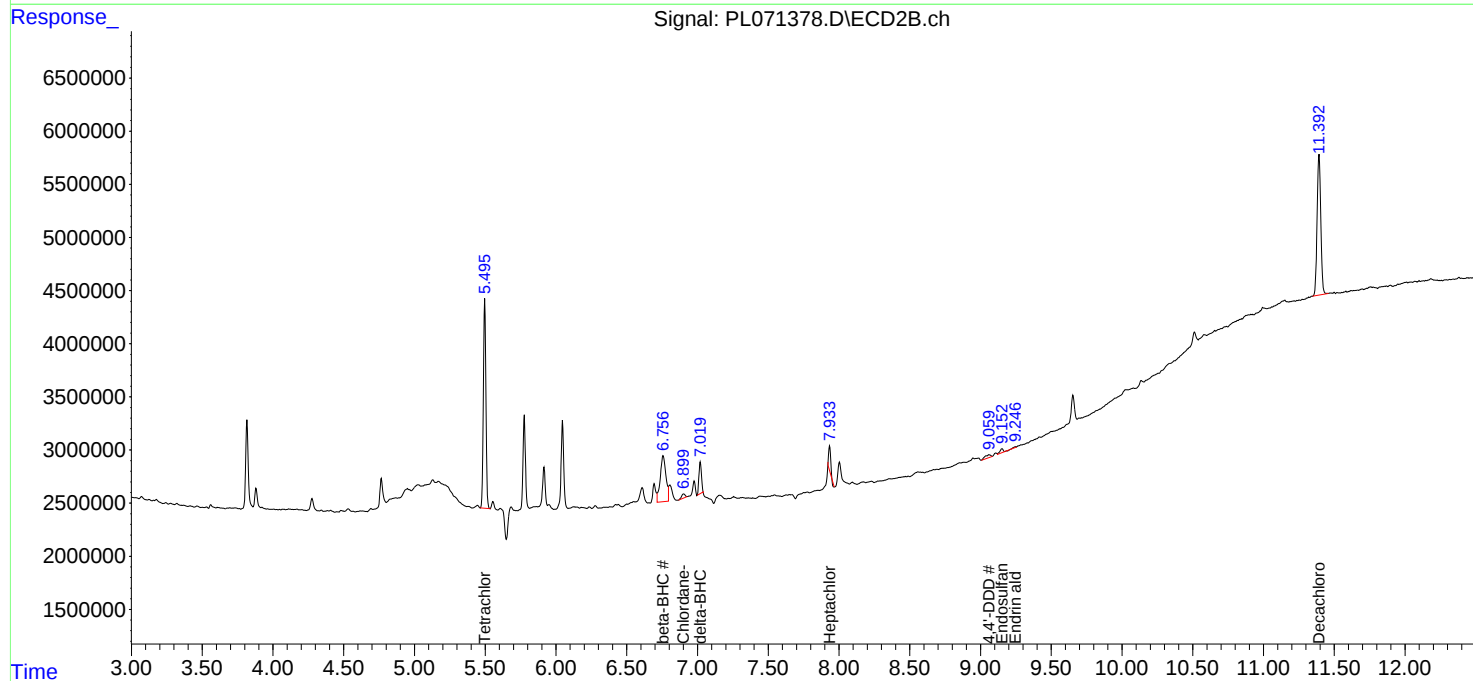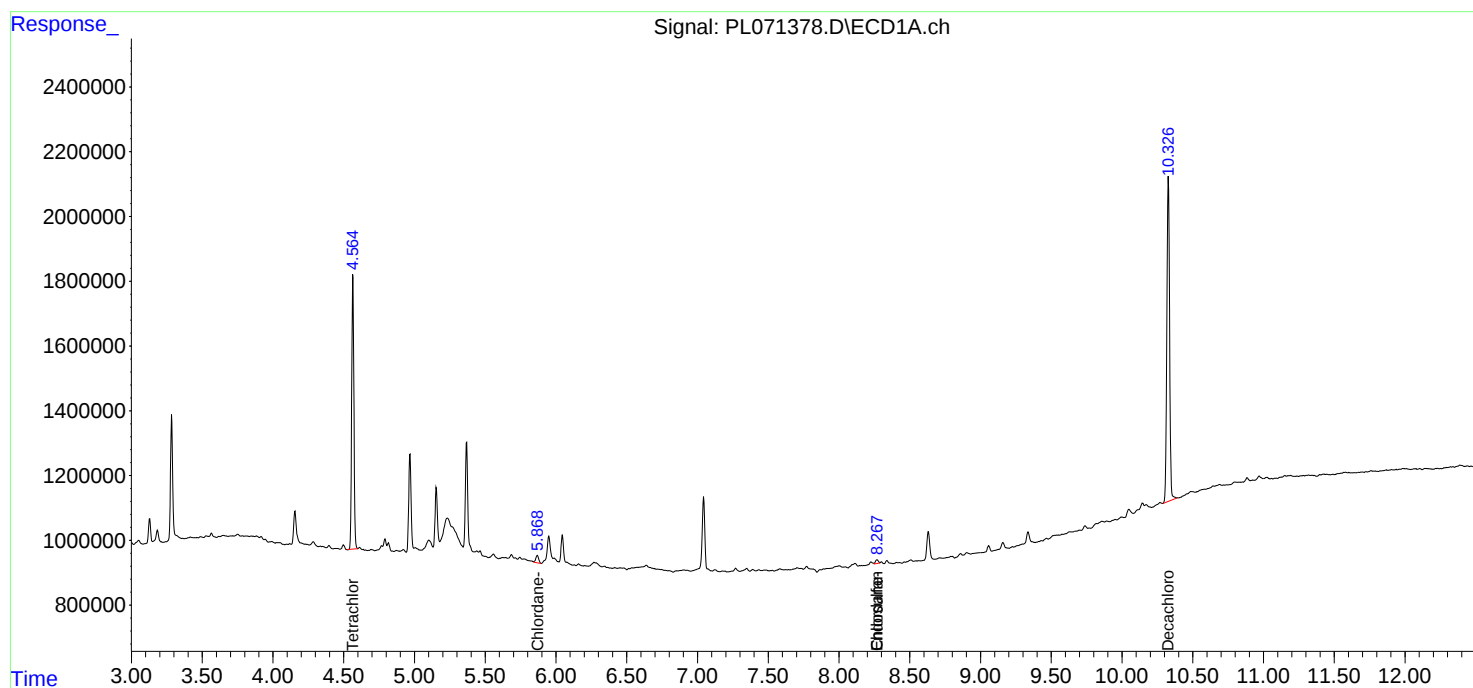


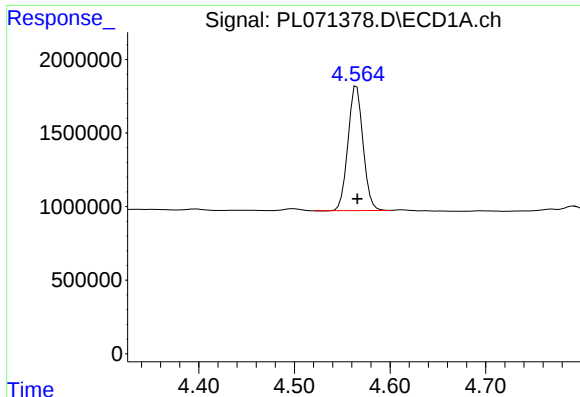

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: 0.000 min
Response: 9312086
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

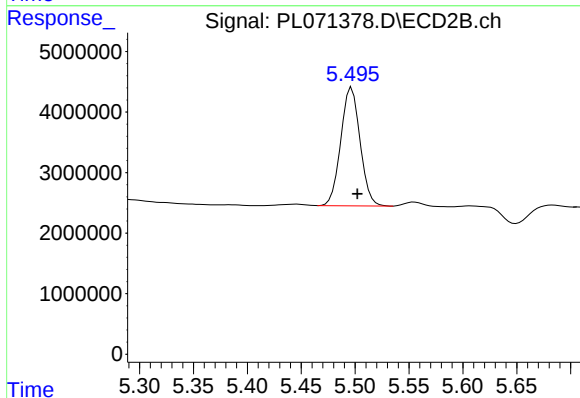


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.005 min
Response: 24372147
Conc: 19.42 ng/ml

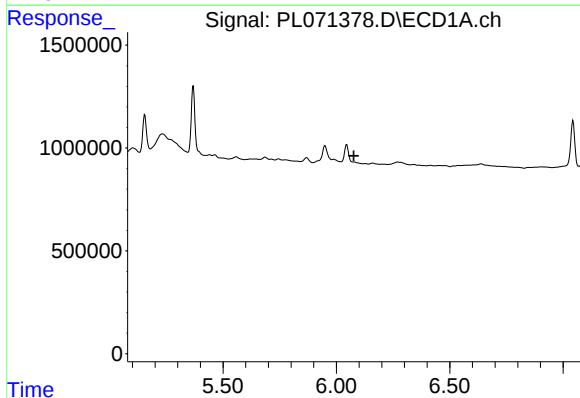


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

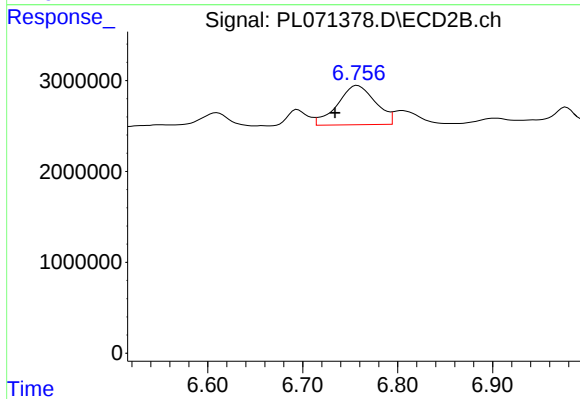

#6 beta-BHC


R.T.: 6.758 min
Delta R.T.: 0.024 min
Response: 12023086
Conc: 13.66 ng/ml

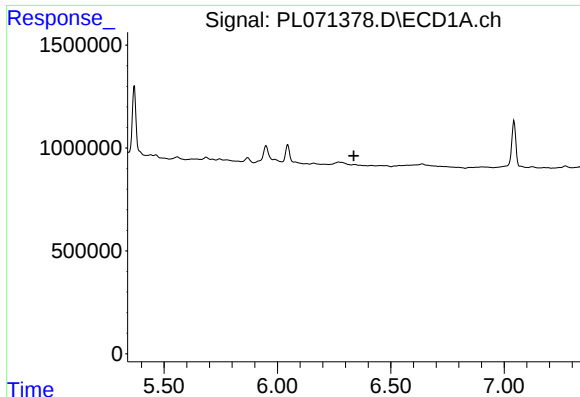

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

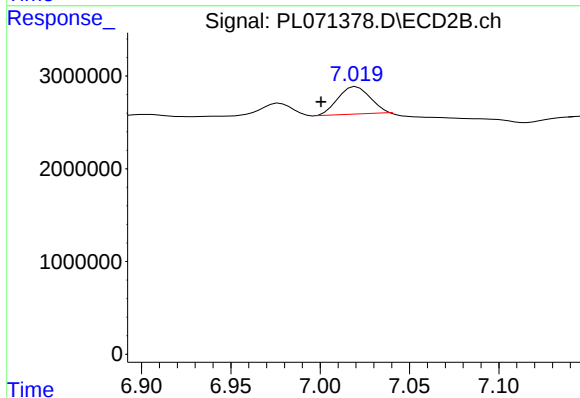


#7 delta-BHC

R.T.: 7.020 min
Delta R.T.: 0.020 min
Response: 3667193
Conc: 2.16 ng/ml

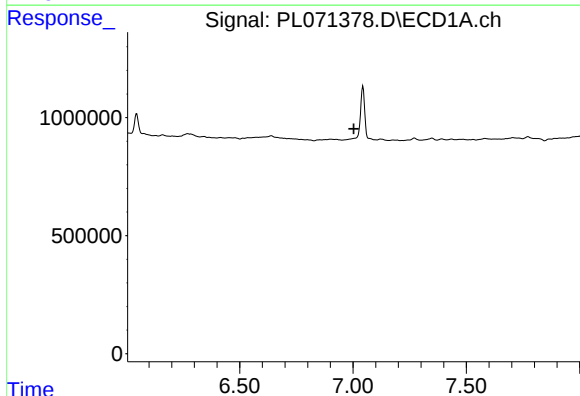


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.003 min
Response: 0
Conc: N.D.

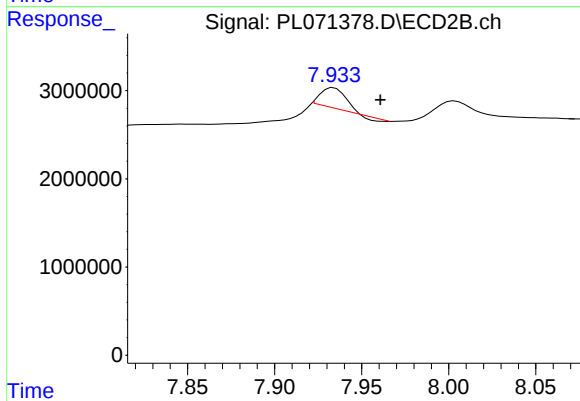

#8 Heptachlor epoxide


R.T.: 7.934 min
Delta R.T.: -0.027 min
Response: 2143829
Conc: 1.35 ng/ml

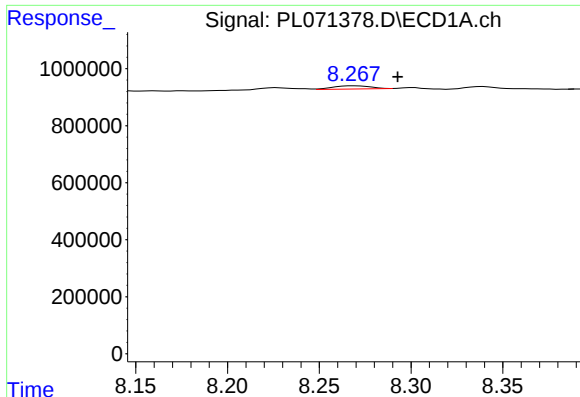

#15 Endosulfan II


R.T.: 8.269 min
Delta R.T.: -0.024 min
Response: 157352
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

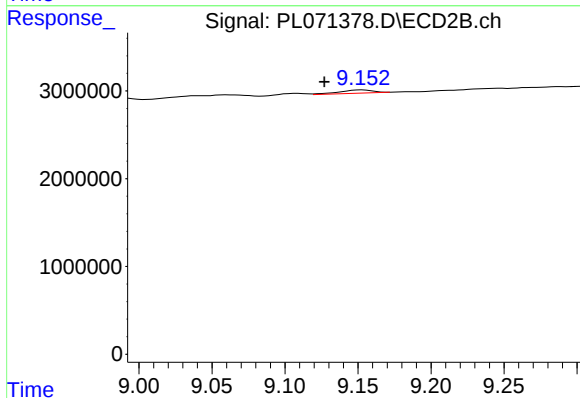


#15 Endosulfan II

R.T.: 9.153 min
Delta R.T.: 0.026 min
Response: 590470
Conc: 0.44 ng/ml

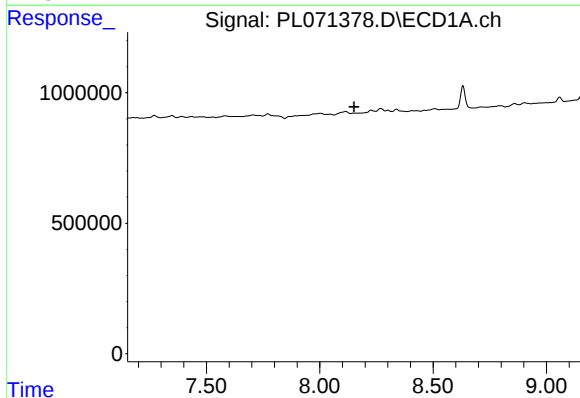


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

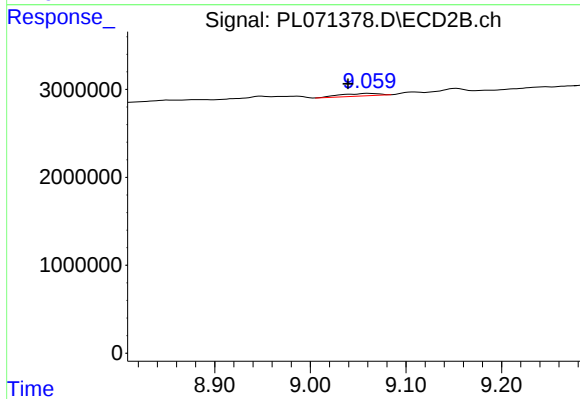

#16 4,4'-DDD


R.T.: 9.061 min
Delta R.T.: 0.021 min
Response: 858610
Conc: 0.74 ng/ml

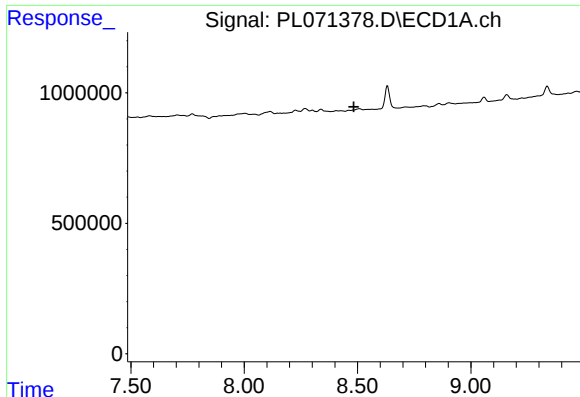

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

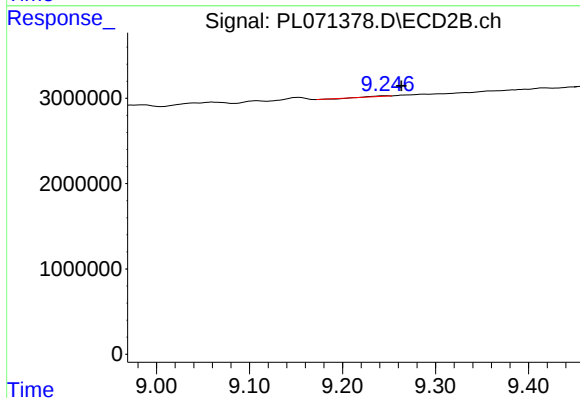


#18 Endrin aldehyde

R.T.: 9.247 min
Delta R.T.: -0.016 min
Response: 43546
Conc: 0.04 ng/ml

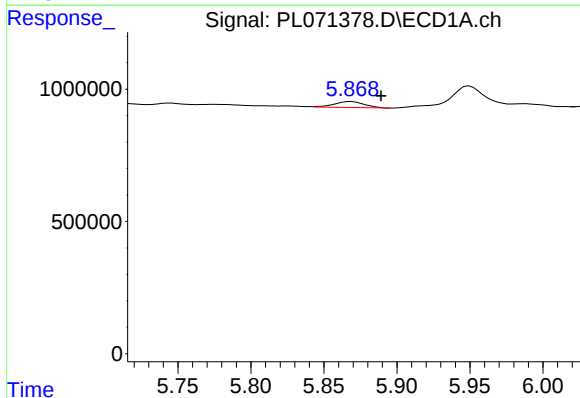


#23 Chlordane-1

R.T.: 5.869 min
Delta R.T.: -0.020 min
Response: 328599
Conc: 19.54 ng/ml

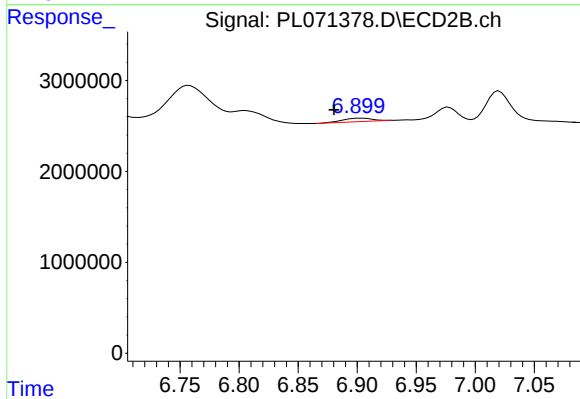

#23 Chlordane-1


R.T.: 6.902 min
Delta R.T.: 0.022 min
Response: 669718
Conc: 12.62 ng/ml

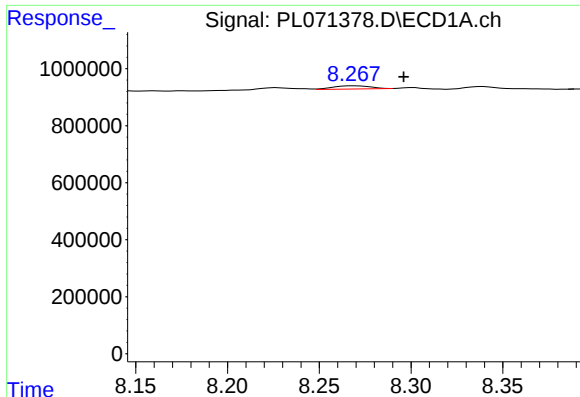

#27 Chlordane-5


R.T.: 8.269 min
Delta R.T.: -0.027 min
Response: 157352
Conc: 6.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

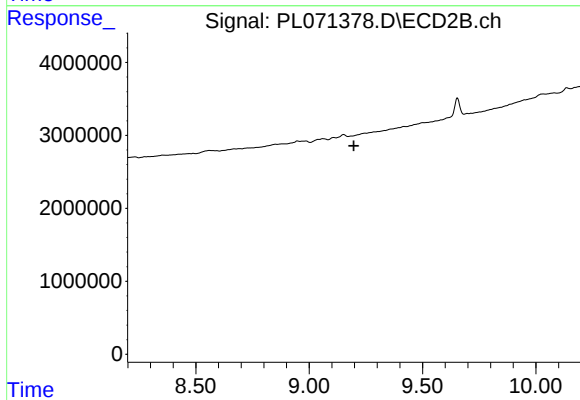


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

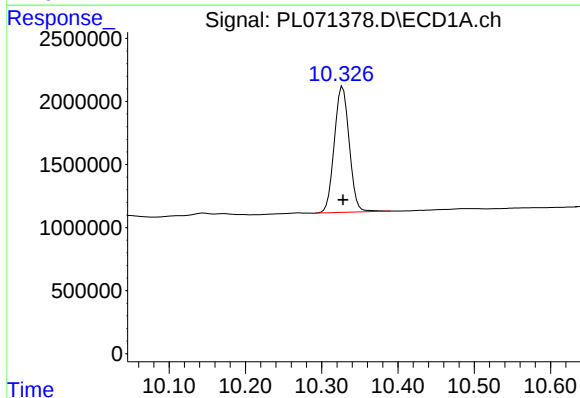

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 13559249
Conc: 18.73 ng/ml

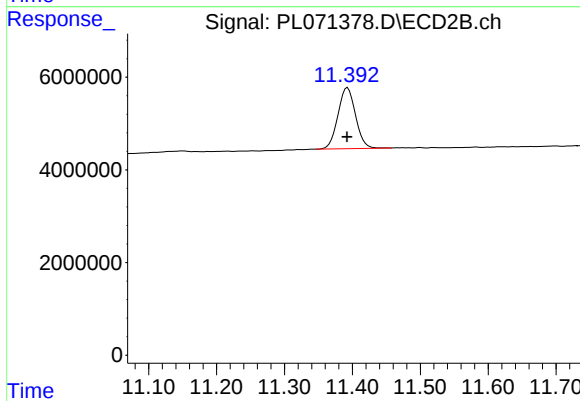

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.000 min
Response: 23693279
Conc: 17.05 ng/ml