

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
 Data File : PL071382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2021 18:24
 Operator : AR\AJ
 Sample : M4966-23
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 22:28:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.562	5.499	8496657	22670617	18.090	18.065
28)	SA Decachlor...	10.325	11.392	11835368	20155561	16.345	14.500
Target Compounds							
3)	MA gamma-BHC...	5.714f	0.000	580506	0	0.909	N.D. #
7)	B delta-BHC	0.000	7.021f	0	3362646	N.D.	1.978 #
8)	B Heptachlo...	0.000	7.934f	0	3069689	N.D.	1.932 #
15)	B Endosulfa...	8.268f	9.155f	300034	799796	0.514	0.594
16)	A 4,4'-DDD	0.000	9.065f	0	1277487	N.D.	1.101 #
20)	A Methoxychlor	9.009	0.000	62203	0	0.172	N.D. #
23)	Chlordane-1	5.863f	0.000	426287	0	25.353	N.D. #
27)	Chlordane-5	8.268f	0.000	300034	0	12.570	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
Data File : PL071382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2021 18:24
Operator : AR\AJ
Sample : M4966-23
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 22:28:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

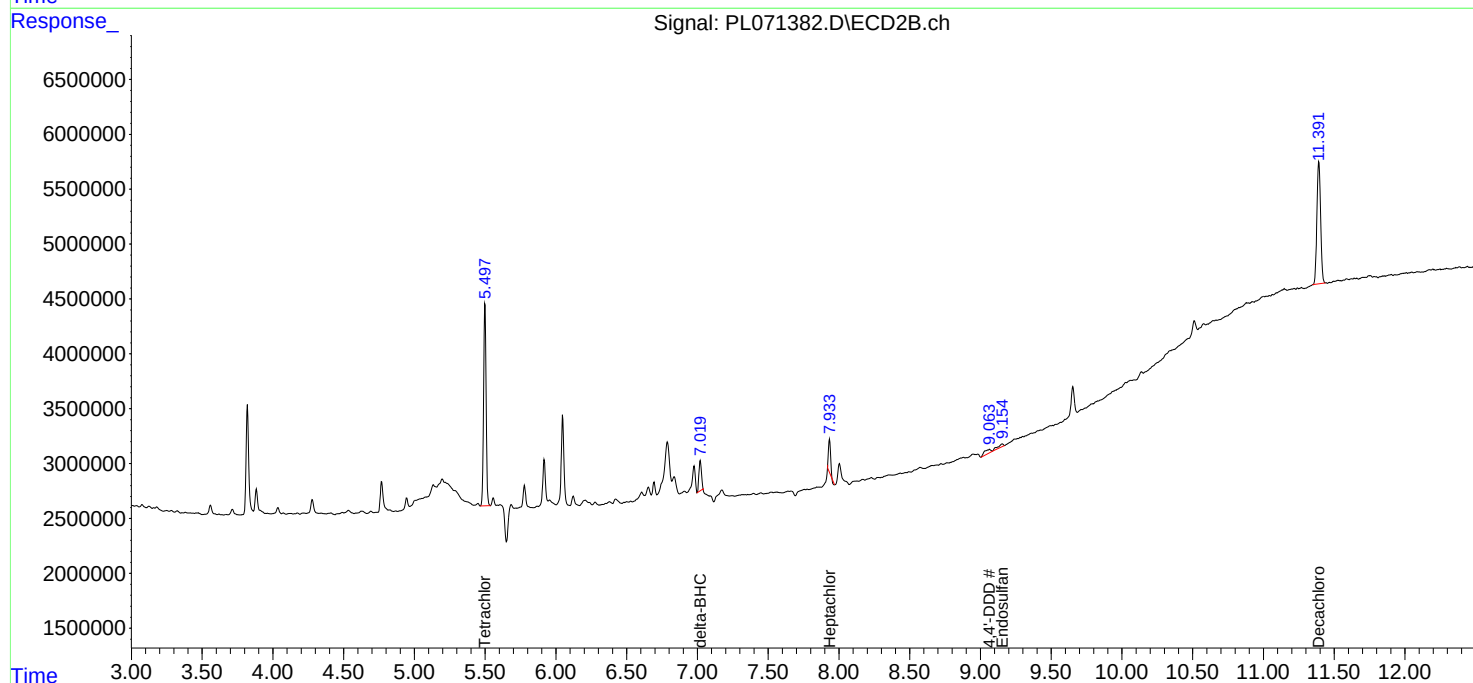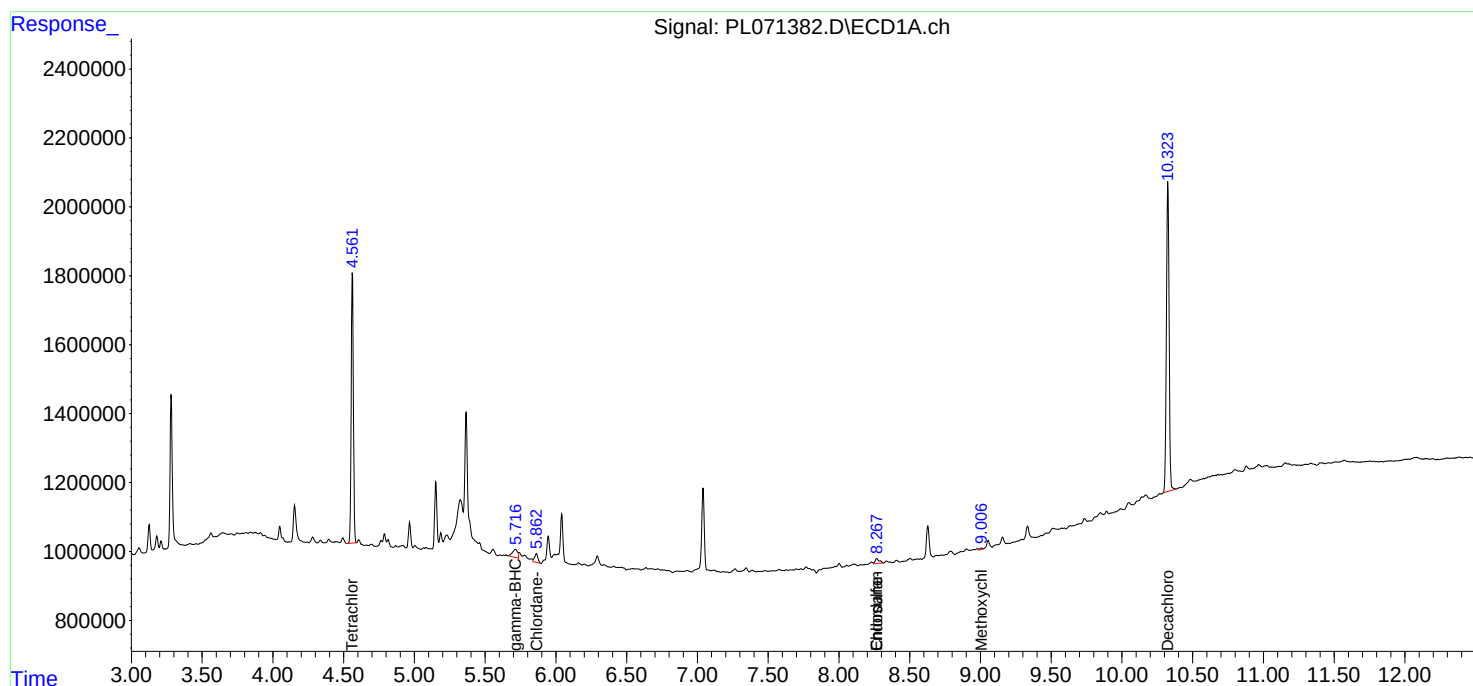


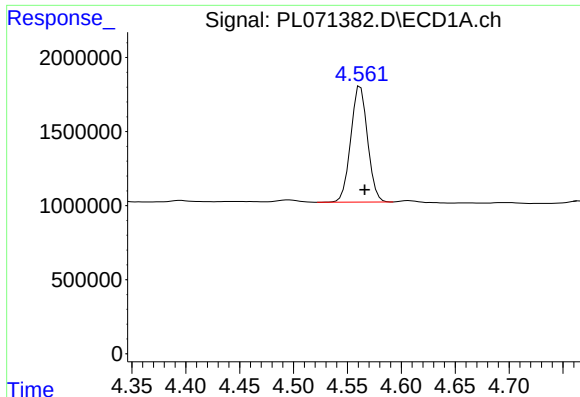

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: -0.004 min
Response: 8496657
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

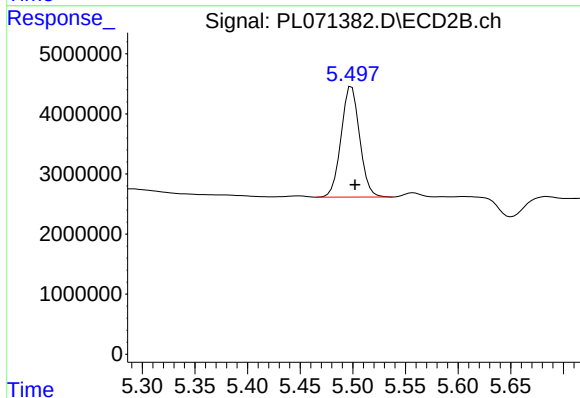


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 22670617
Conc: 18.07 ng/ml

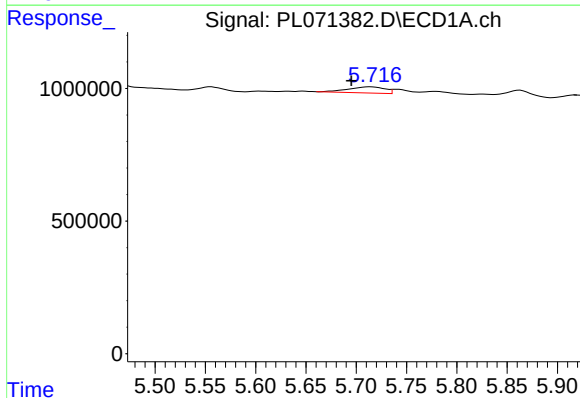


#3 gamma-BHC (Lindane)

R.T.: 5.714 min
Delta R.T.: 0.019 min
Response: 580506
Conc: 0.91 ng/ml

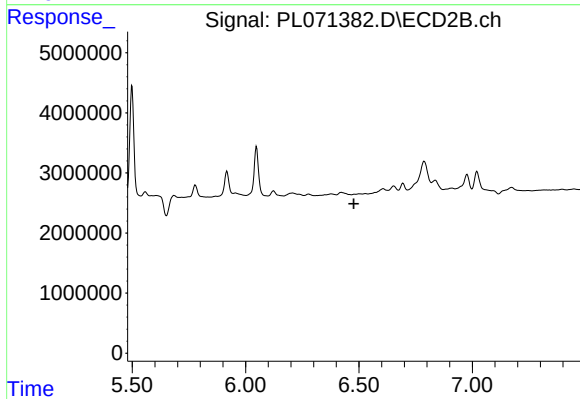

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

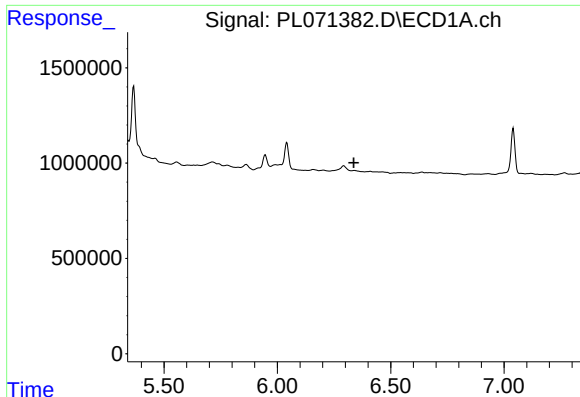

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

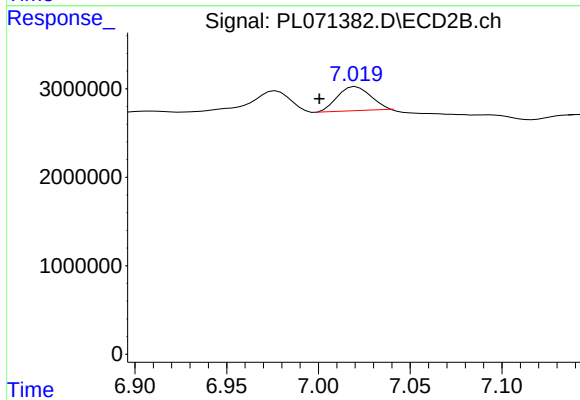


#7 delta-BHC

R.T.: 7.021 min
Delta R.T.: 0.020 min
Response: 3362646
Conc: 1.98 ng/ml

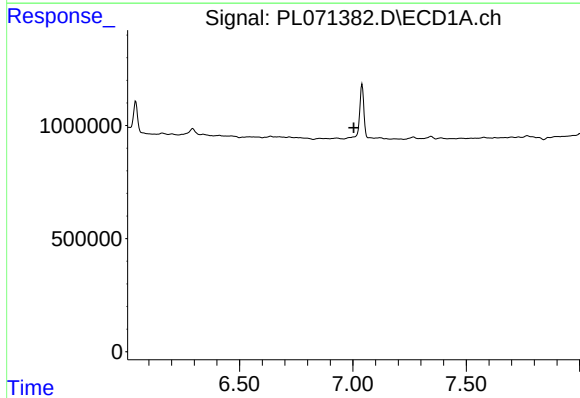


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.003 min
Response: 0
Conc: N.D.

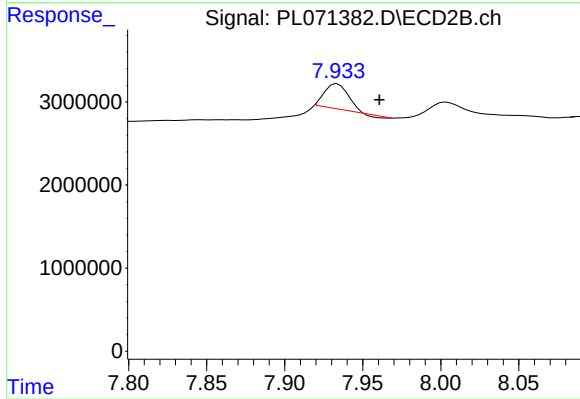

#8 Heptachlor epoxide


R.T.: 7.934 min
Delta R.T.: -0.027 min
Response: 3069689
Conc: 1.93 ng/ml

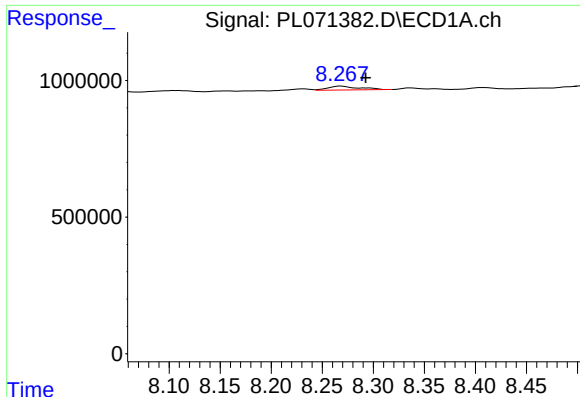

#15 Endosulfan II


R.T.: 8.268 min
Delta R.T.: -0.024 min
Response: 300034
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

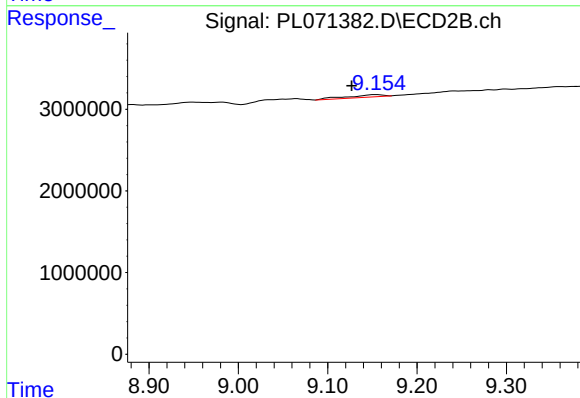


#15 Endosulfan II

R.T.: 9.155 min
Delta R.T.: 0.028 min
Response: 799796
Conc: 0.59 ng/ml

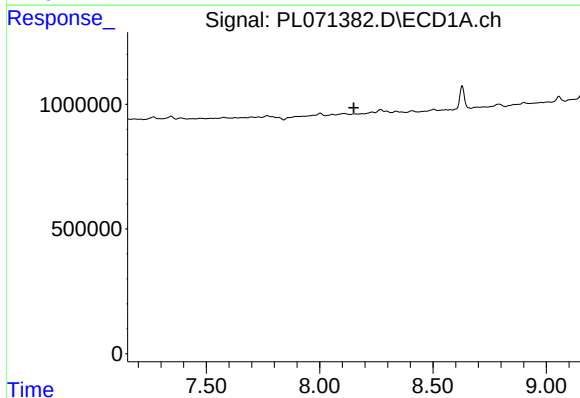


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

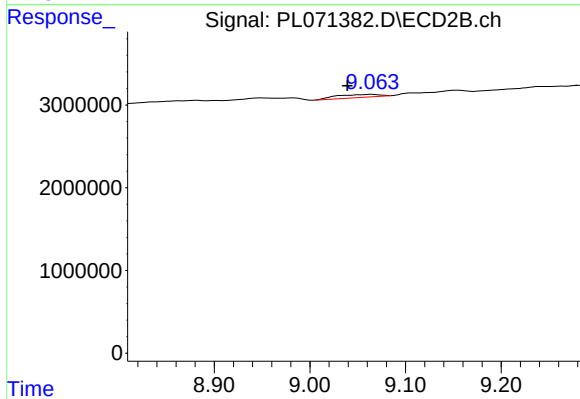

#16 4,4'-DDD


R.T.: 9.065 min
Delta R.T.: 0.026 min
Response: 1277487
Conc: 1.10 ng/ml

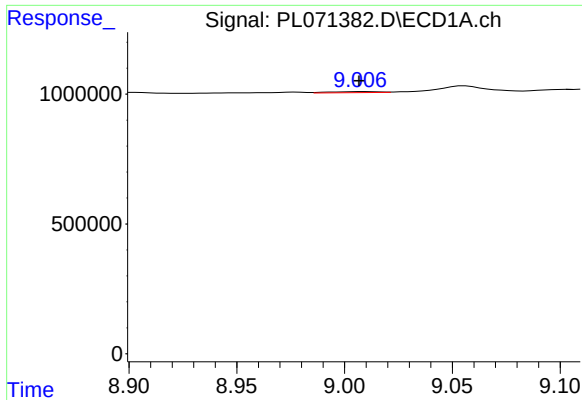

#20 Methoxychlor


R.T.: 9.009 min
Delta R.T.: 0.002 min
Response: 62203
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

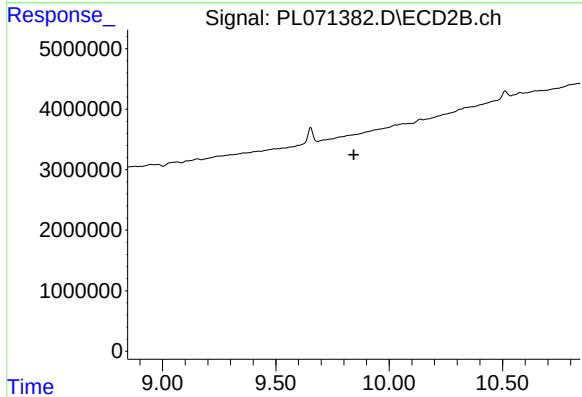


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

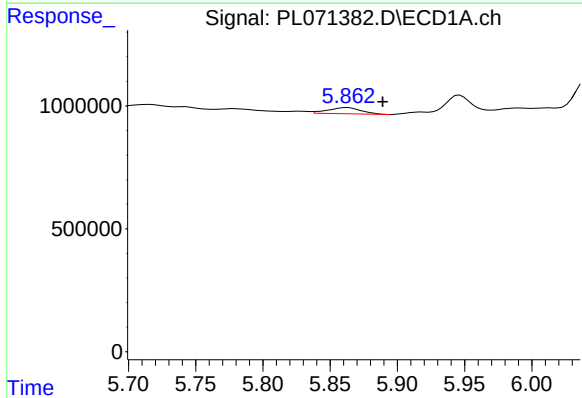


#23 Chlordane-1

R.T.: 5.863 min
Delta R.T.: -0.026 min
Response: 426287
Conc: 25.35 ng/ml

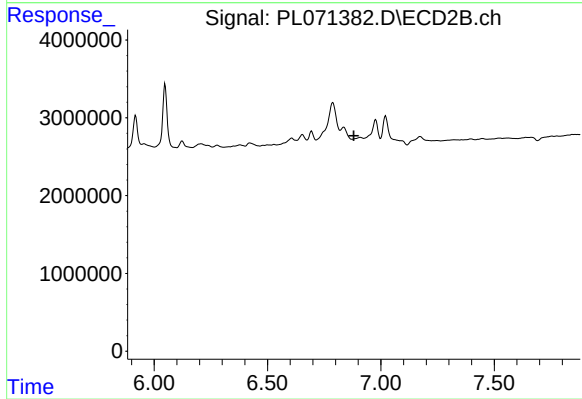

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.880 min
Response: 0
Conc: N.D.

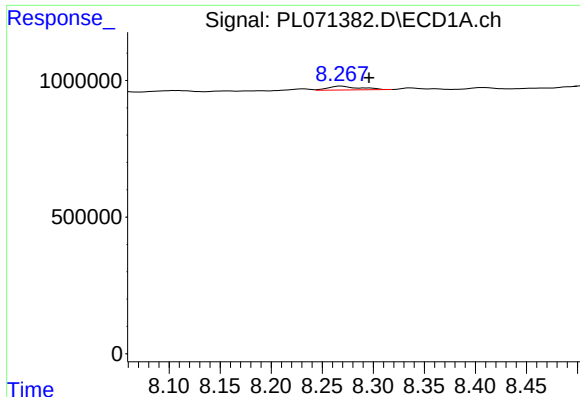

#27 Chlordane-5


R.T.: 8.268 min
Delta R.T.: -0.028 min
Response: 300034
Conc: 12.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

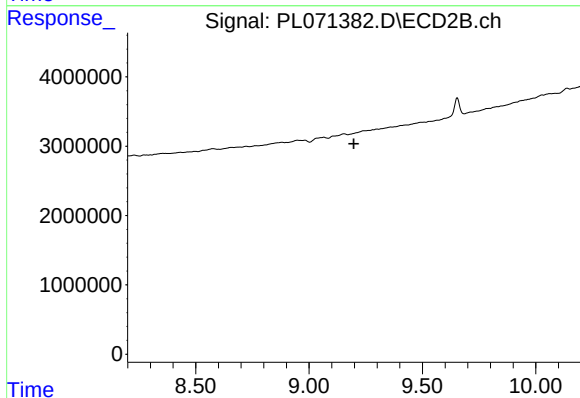


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

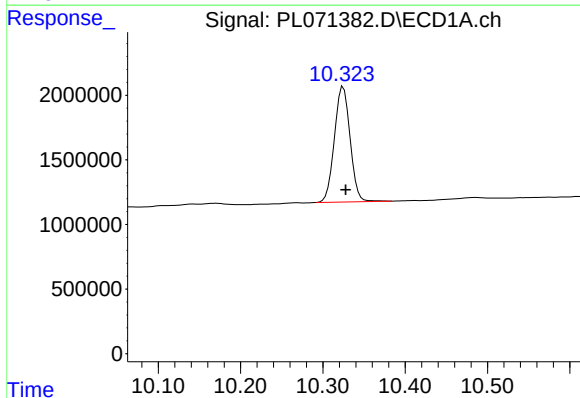

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: -0.003 min
Response: 11835368
Conc: 16.35 ng/ml

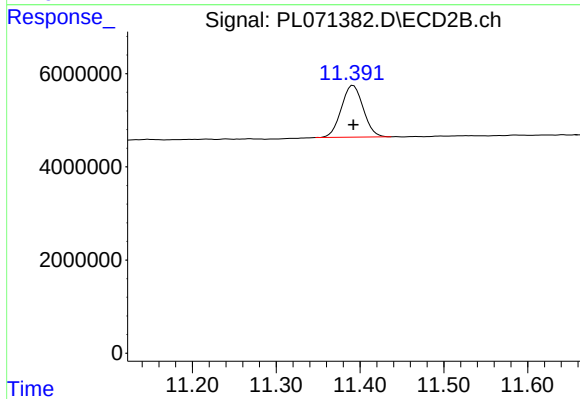

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 20155561
Conc: 14.50 ng/ml