

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
 Data File : PL071391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2021 22:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 22:30:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.561	5.498	10053717	27468752	21.405	21.889
28)	SA Decachlor...	10.322	11.388	14731933	25694763	20.345	18.485
Target Compounds							
2)	A alpha-BHC	0.000	6.056f	0	662044	N.D.	0.358 #
4)	MA Heptachlor	6.076f	0.000	15597	0	0.022	N.D. #
6)	B beta-BHC	6.076	0.000	15597	0	0.052	N.D. #
7)	B delta-BHC	0.000	7.018f	0	8228875	N.D.	4.840 #
13)	MA Dieldrin	7.693	0.000	302363	0	0.500	N.D. #
14)	MA Endrin	8.003f	0.000	380082	0	0.672	N.D. #
15)	B Endosulfa...	8.264f	9.150f	311538	384450	0.534	0.285 #
20)	A Methoxychlor	9.028f	0.000	402365	0	1.114	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121021\
Data File : PL071391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2021 22:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 22:30:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

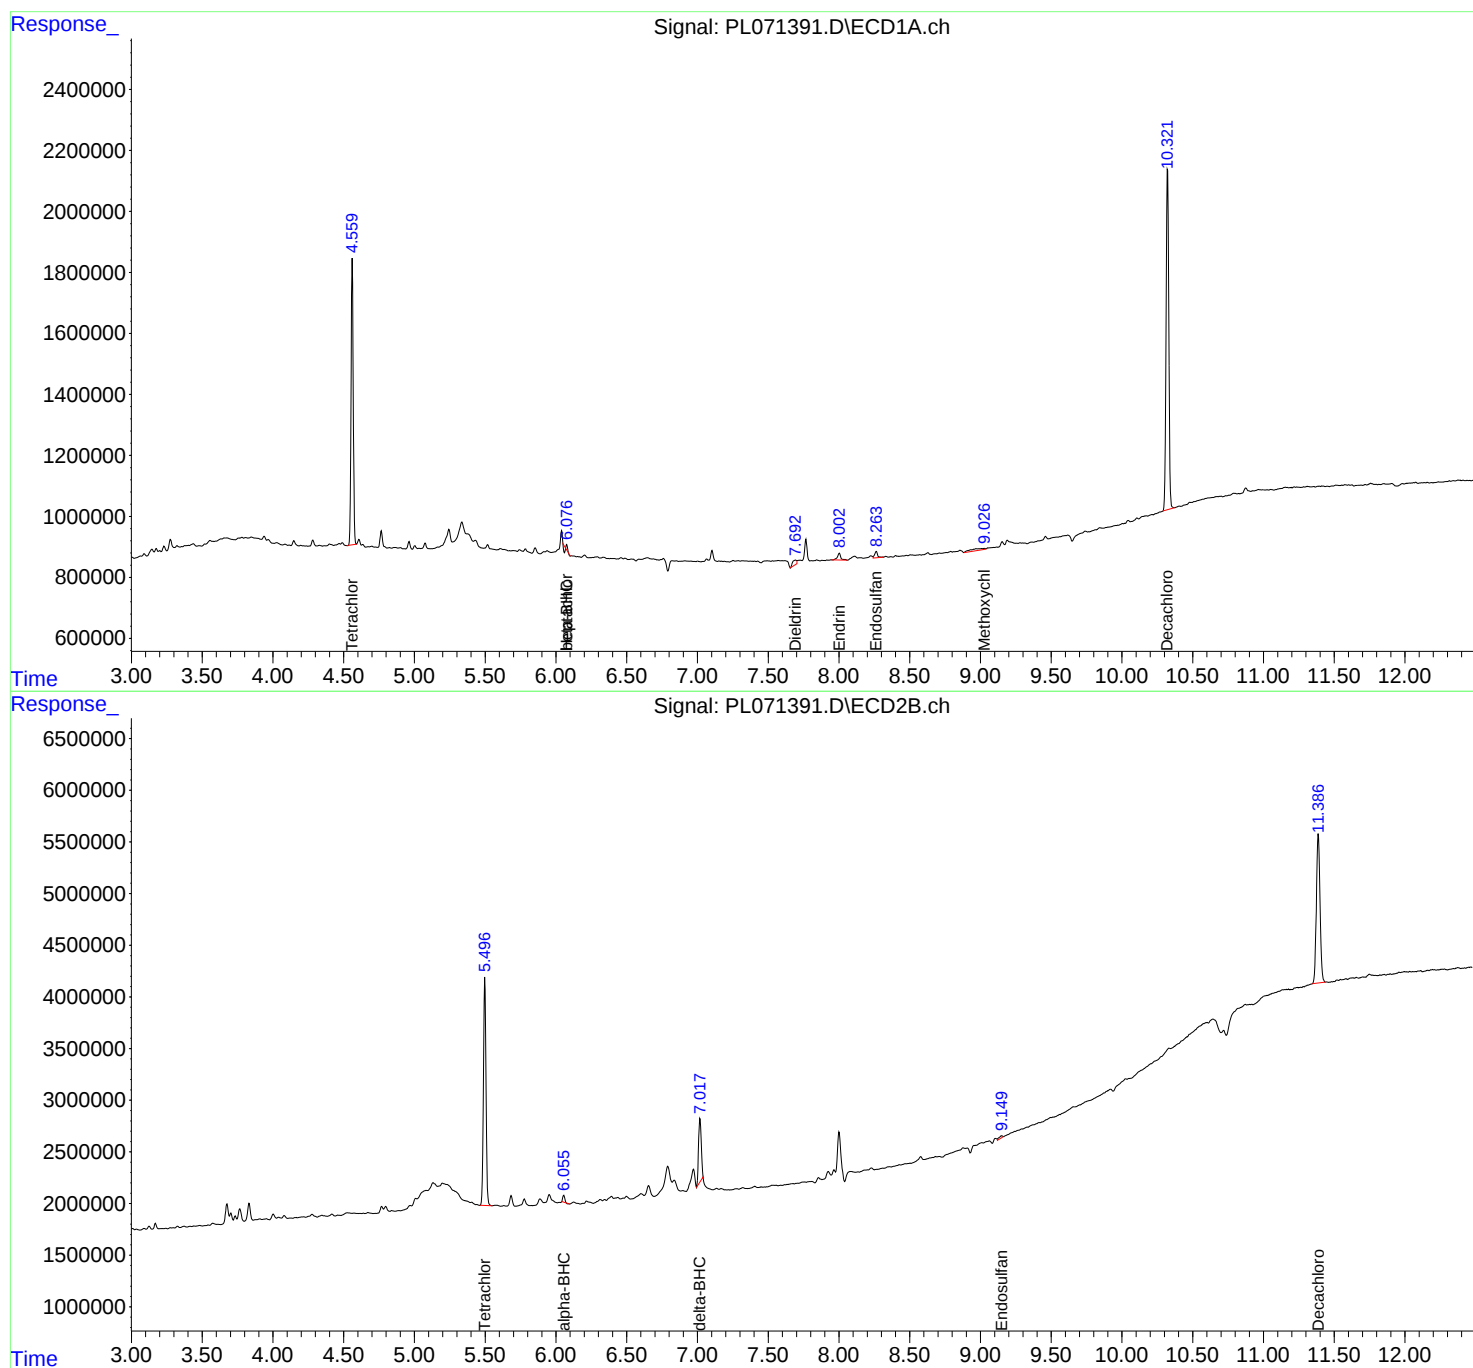


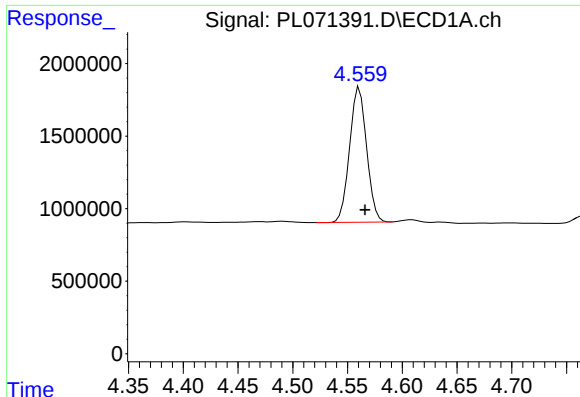

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: -0.005 min
Response: 10053717
Conc: 21.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

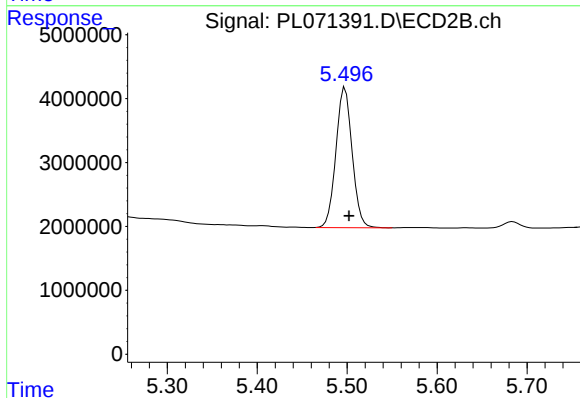


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: -0.004 min
Response: 27468752
Conc: 21.89 ng/ml

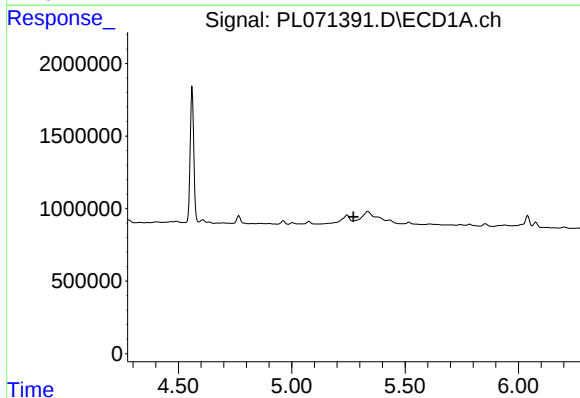


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

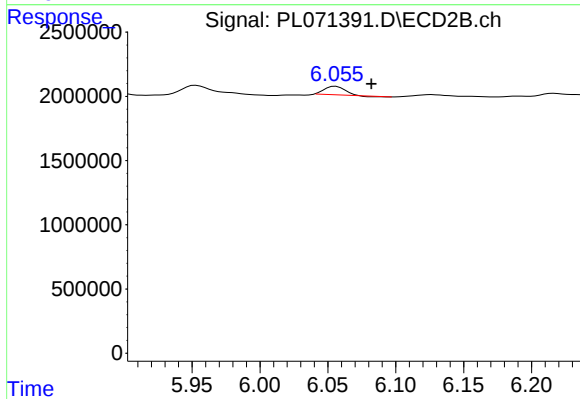

#2 alpha-BHC


R.T.: 6.056 min
Delta R.T.: -0.026 min
Response: 662044
Conc: 0.36 ng/ml

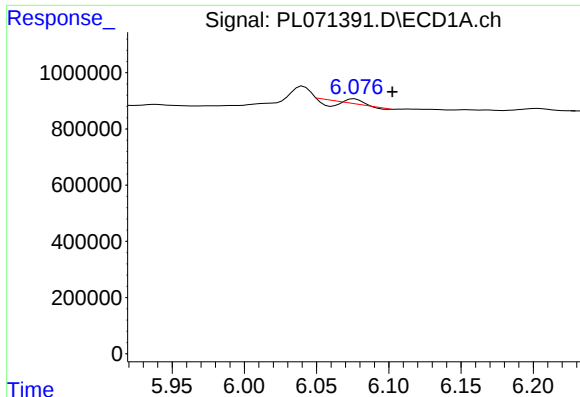

#4 Heptachlor


R.T.: 6.076 min
Delta R.T.: -0.026 min
Response: 15597
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

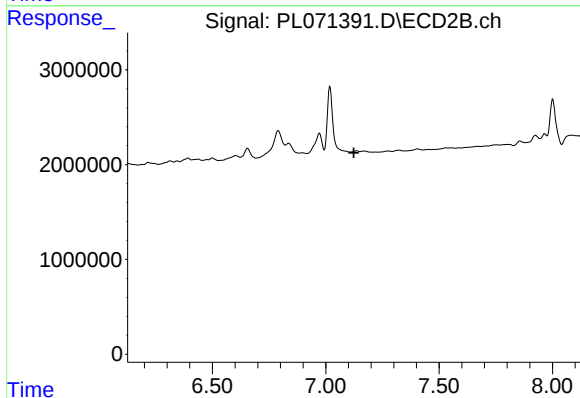


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.124 min
Response: 0
Conc: N.D.

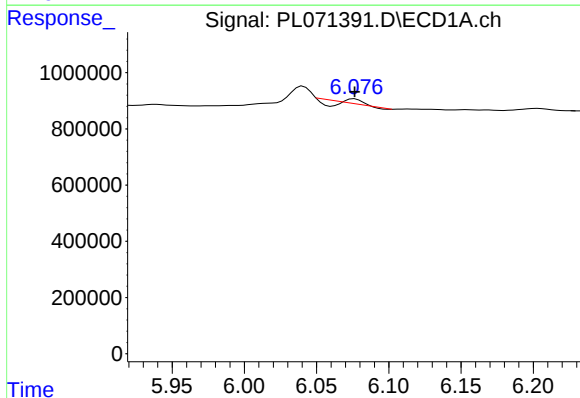


#6 beta-BHC

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 15597
Conc: 0.05 ng/ml

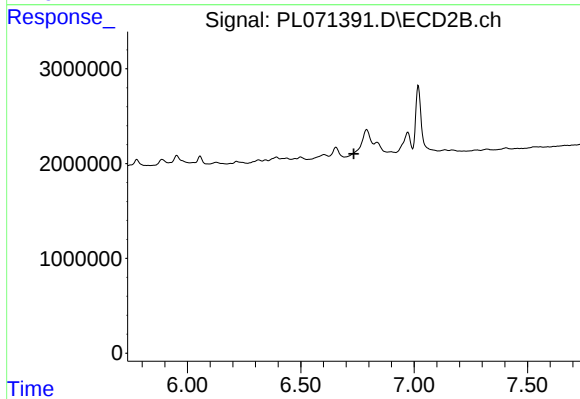

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

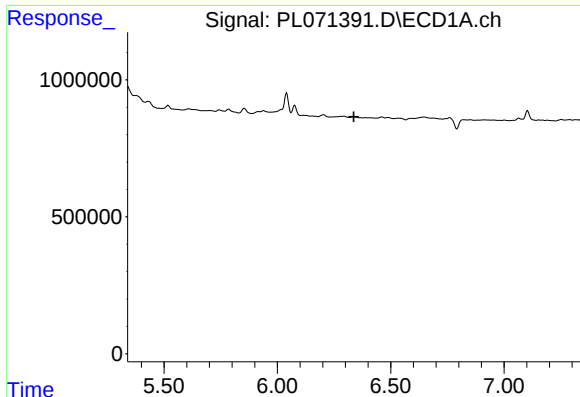

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

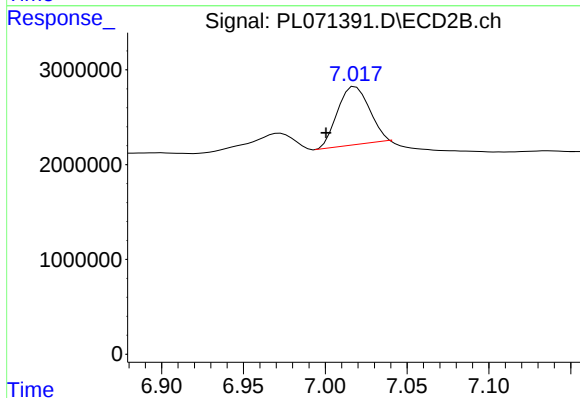


#7 delta-BHC

R.T.: 7.018 min
Delta R.T.: 0.018 min
Response: 8228875
Conc: 4.84 ng/ml

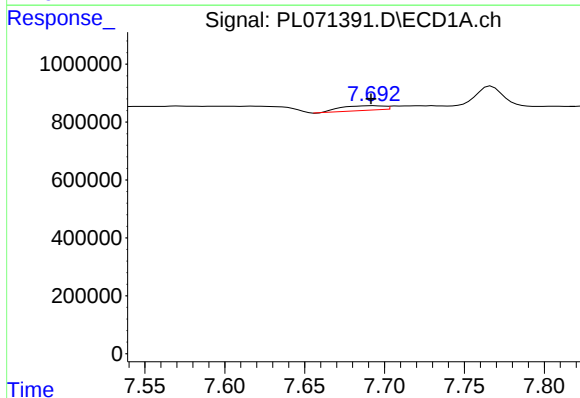


#13 Dieldrin

R.T.: 7.693 min
Delta R.T.: 0.001 min
Response: 302363
Conc: 0.50 ng/ml

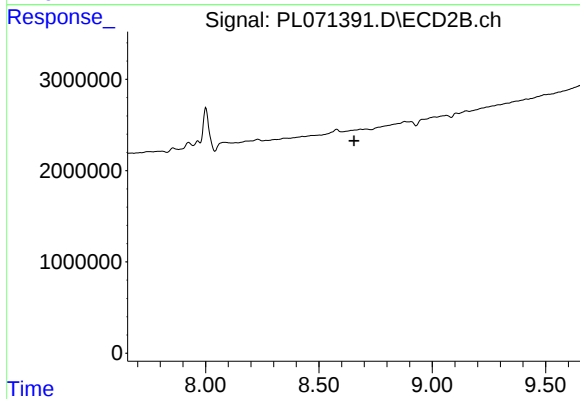

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

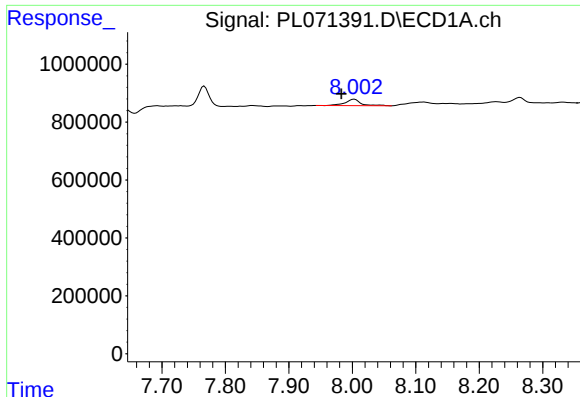

#14 Endrin


R.T.: 8.003 min
Delta R.T.: 0.020 min
Response: 380082
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

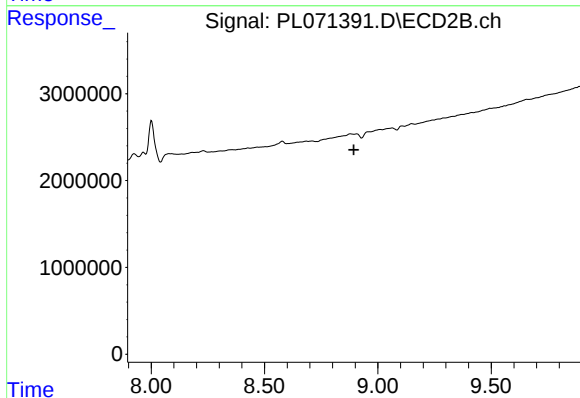


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

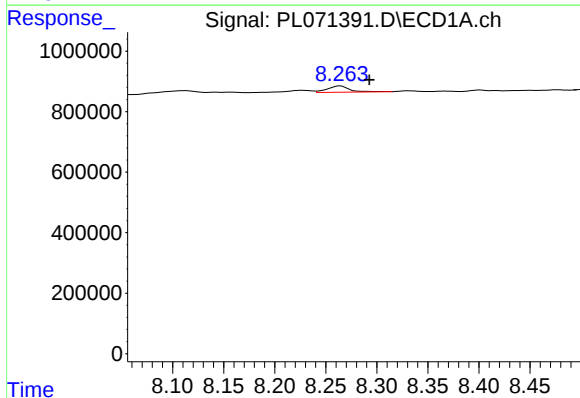


#15 Endosulfan II

R.T.: 8.264 min
Delta R.T.: -0.029 min
Response: 311538
Conc: 0.53 ng/ml

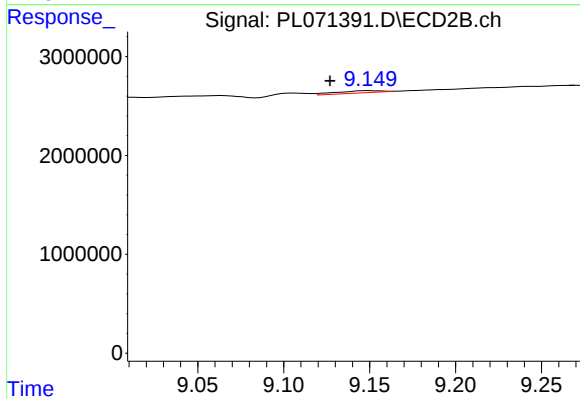

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.023 min
Response: 384450
Conc: 0.29 ng/ml

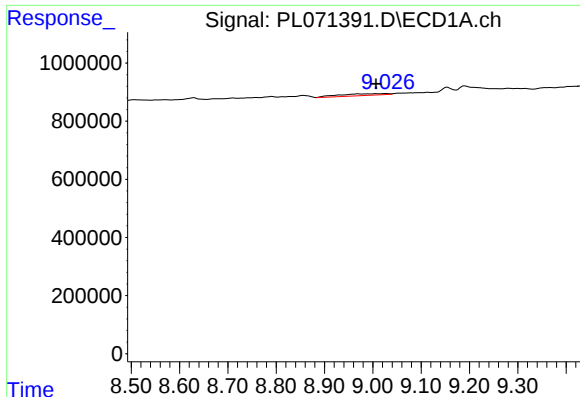

#20 Methoxychlor


R.T.: 9.028 min
Delta R.T.: 0.021 min
Response: 402365
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

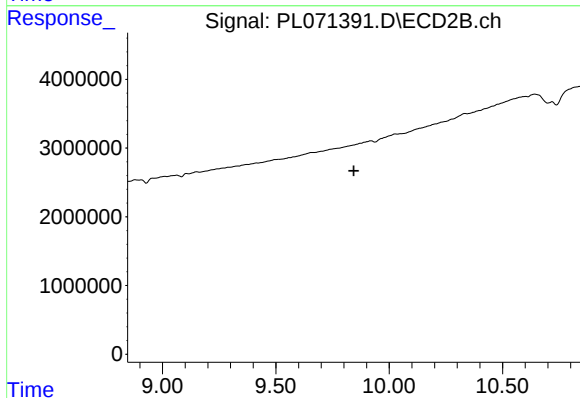


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

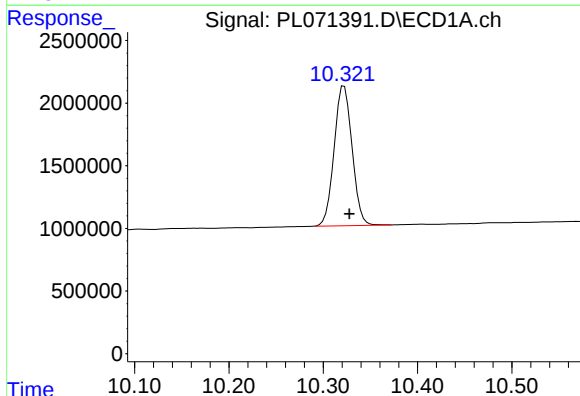

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: -0.006 min
Response: 14731933
Conc: 20.35 ng/ml

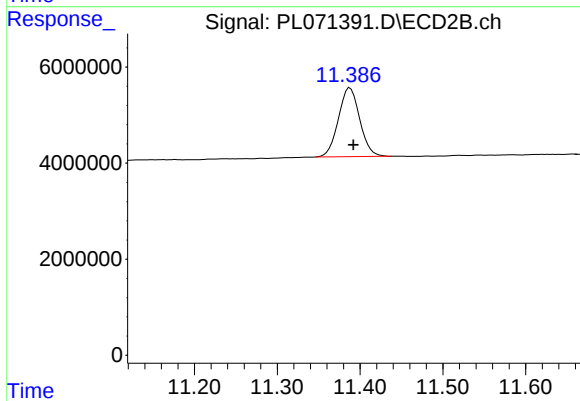

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.004 min
Response: 25694763
Conc: 18.49 ng/ml