

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
 Data File : PL097820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 09:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 02:40:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5) MB	Aldrin	5.178f	0.000	64007301	0	8.835	N.D. #
8) B	Heptachlo...	5.620	0.000	164.9E6	0	24.791	N.D. #
13) MA	Dieldrin	0.000	5.381	0	123.4E6	N.D.	13.169 #
14) MA	Endrin	0.000	5.680	0	39272770	N.D.	4.699 #
15) B	Endosulfa...	0.000	5.966	0	10414454	N.D.	1.258 #
16) A	4,4'-DDD	6.630	0.000	10024329	0	2.164	N.D. #
23)	Chlordane-1	4.664	0.000	1767428	0	7.523	N.D. #
24)	Chlordane-2	5.178	4.375	64007301	39203261	264.940	127.541 #
27)	Chlordane-5	0.000	5.966	0	10414454	N.D.	31.658 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
Data File : PL097820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 09:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 02:40:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

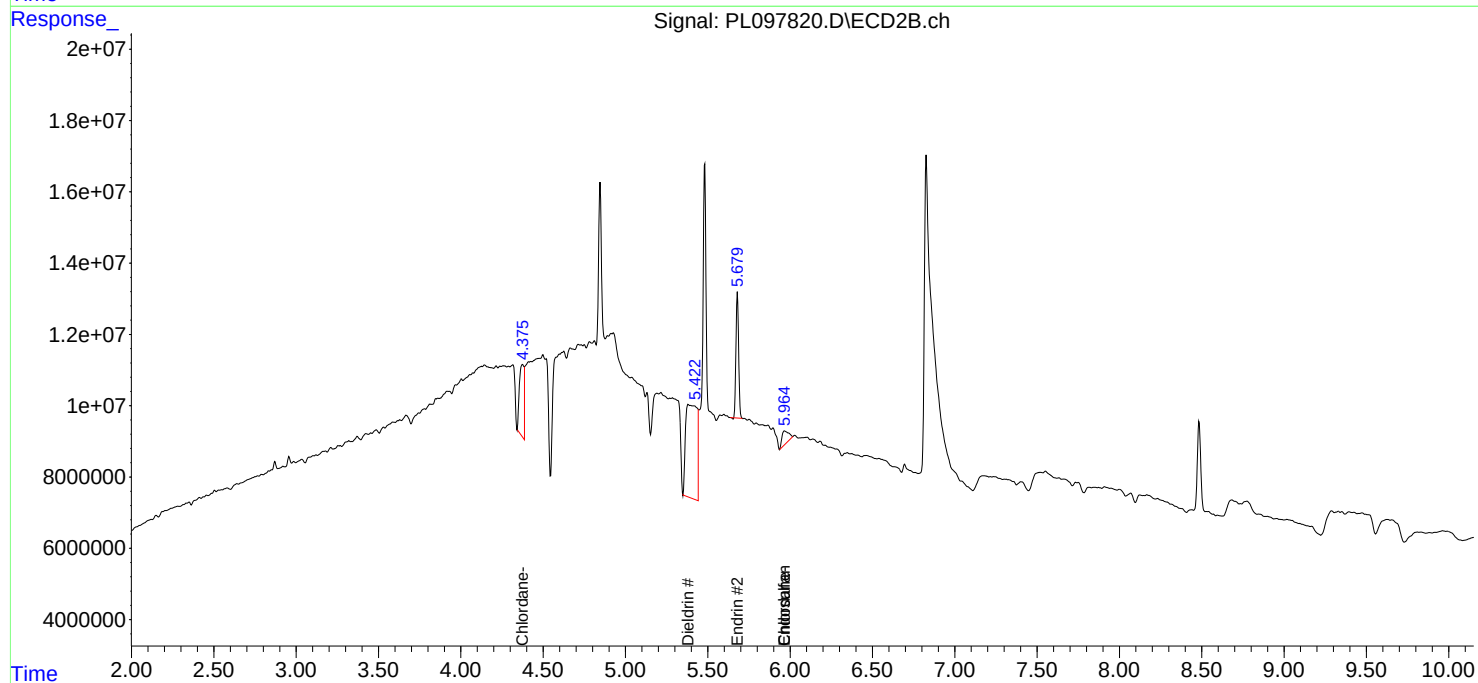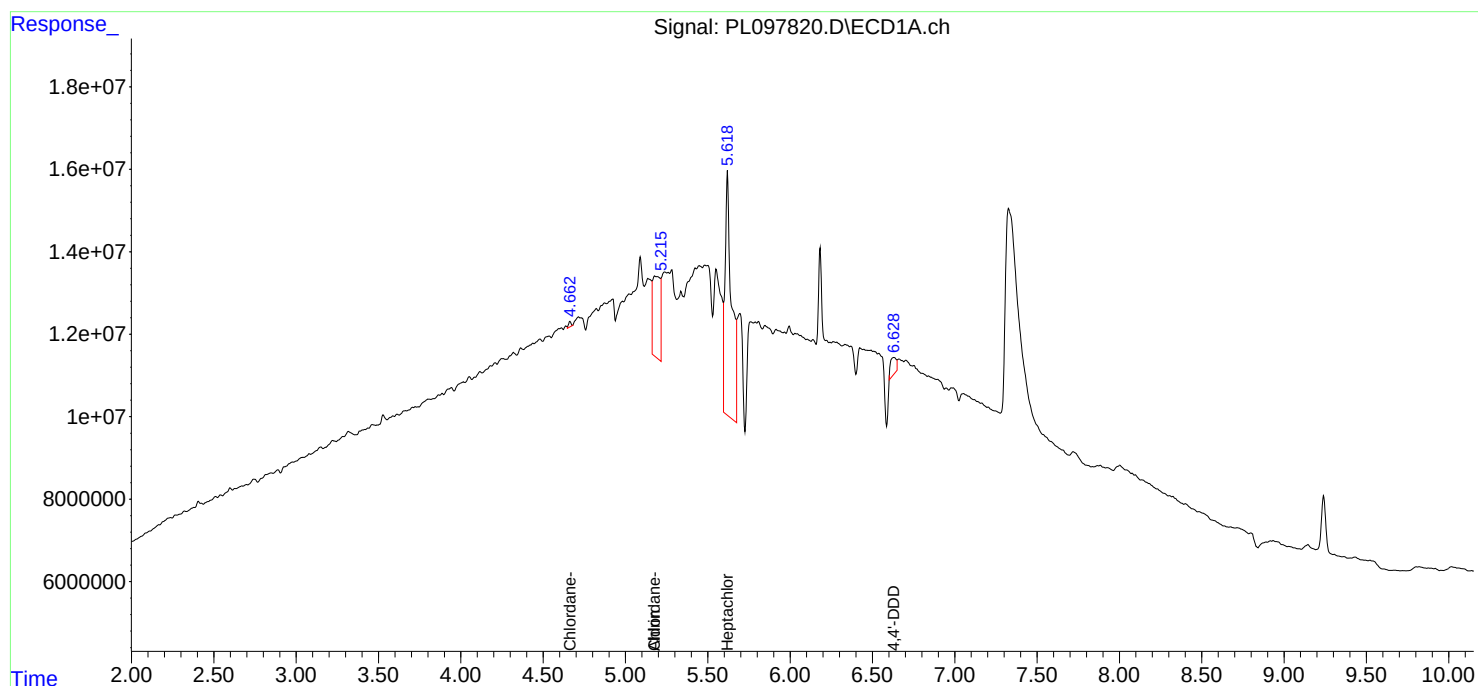


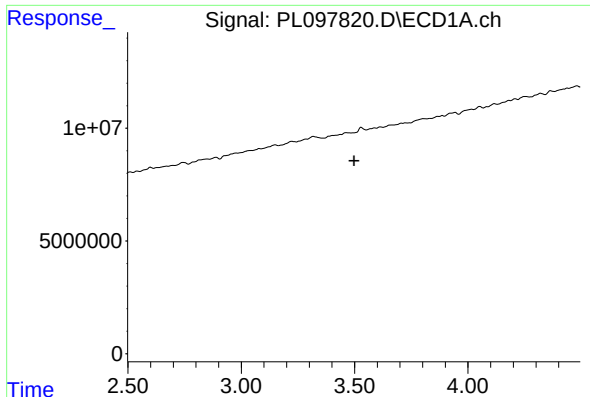

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.498 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

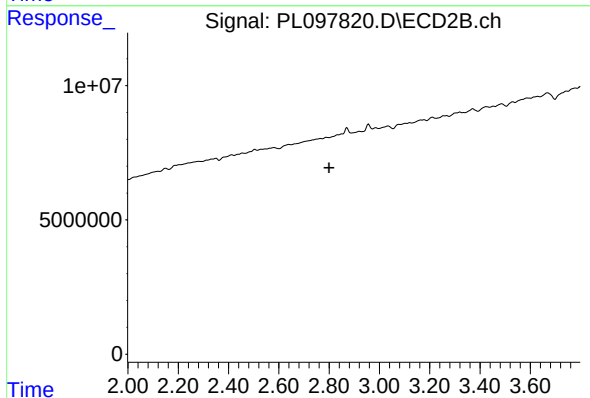


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.800 min
Response: 0
Conc: N.D.

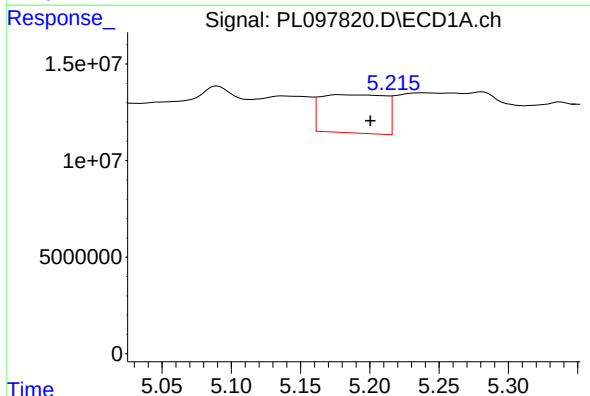


#5 Aldrin

R.T.: 5.178 min
Delta R.T.: -0.023 min
Response: 64007301
Conc: 8.84 ng/ml

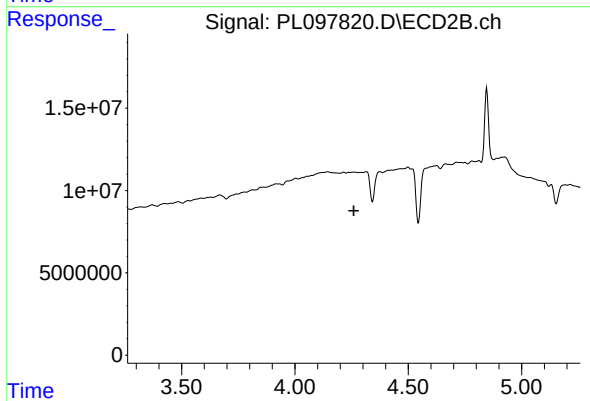

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.260 min
Response: 0
Conc: N.D.

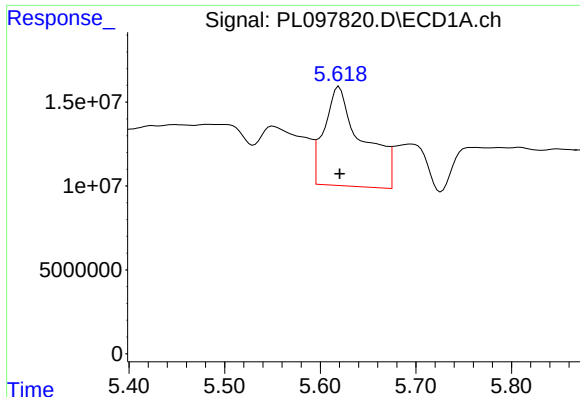

#8 Heptachlor epoxide


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 164937893
Conc: 24.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

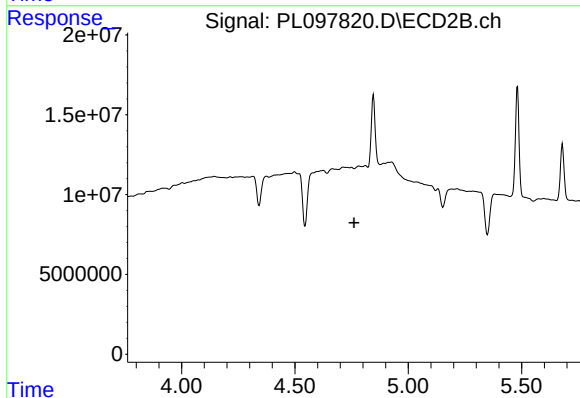


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.761 min
Response: 0
Conc: N.D.

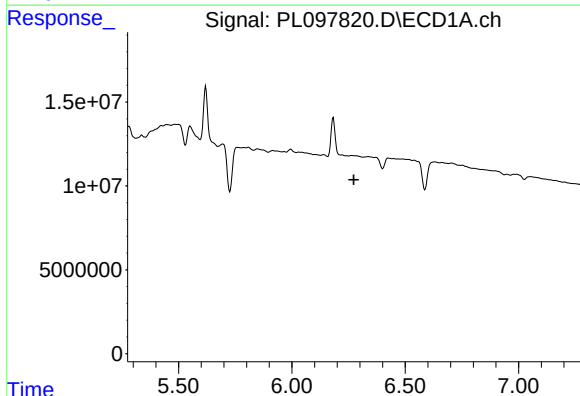


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.273 min
Response: 0
Conc: N.D.

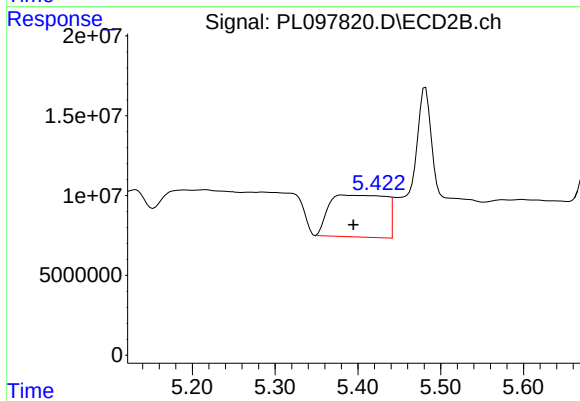

#13 Dieldrin


R.T.: 5.381 min
Delta R.T.: -0.014 min
Response: 123398959
Conc: 13.17 ng/ml

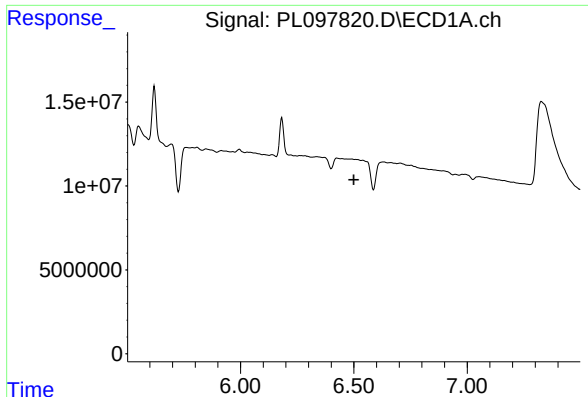

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

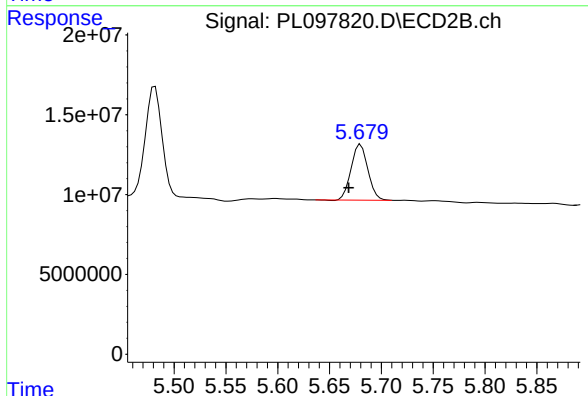


#14 Endrin

R.T.: 5.680 min
Delta R.T.: 0.012 min
Response: 39272770
Conc: 4.70 ng/ml

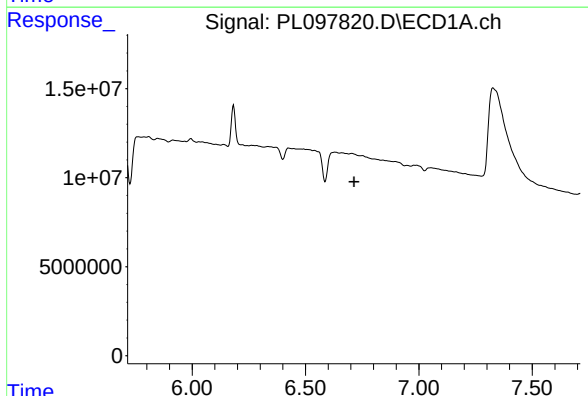


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.714 min
Response: 0
Conc: N.D.

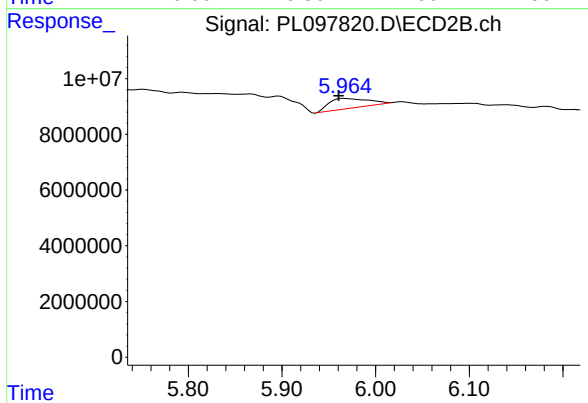

#15 Endosulfan II


R.T.: 5.966 min
Delta R.T.: 0.005 min
Response: 10414454
Conc: 1.26 ng/ml

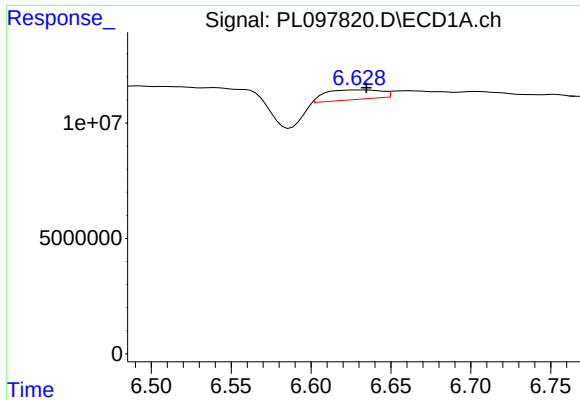

#16 4,4'-DDD


R.T.: 6.630 min
Delta R.T.: -0.005 min
Response: 10024329
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

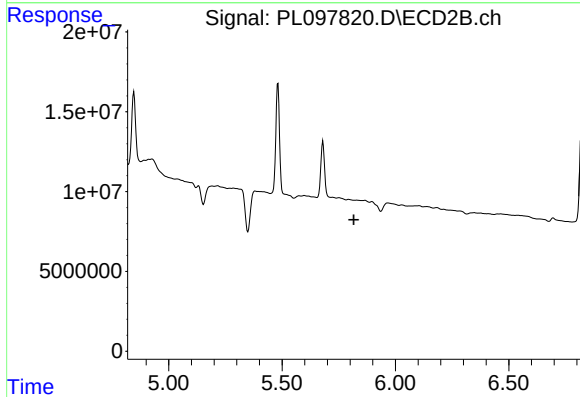


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.817 min
Response: 0
Conc: N.D.

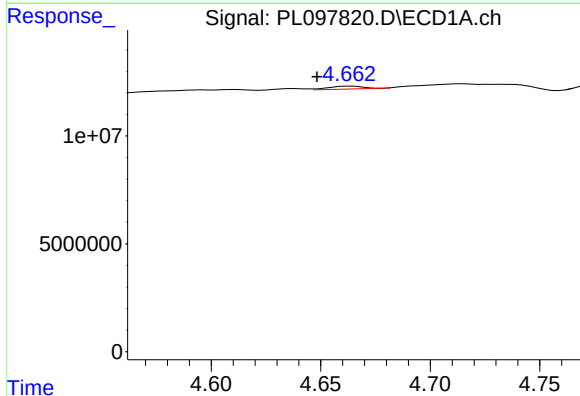


#23 Chlordane-1

R.T.: 4.664 min
Delta R.T.: 0.015 min
Response: 1767428
Conc: 7.52 ng/ml

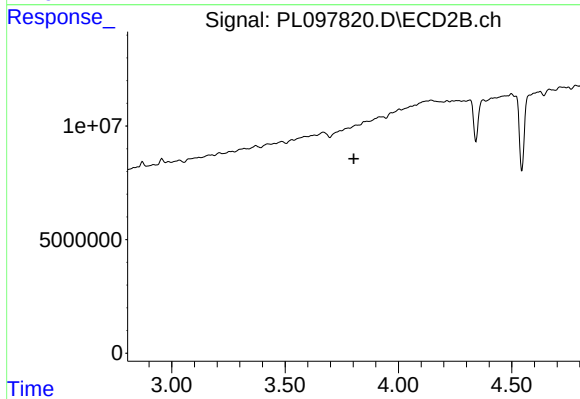

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 3.802 min
Response: 0
Conc: N.D.

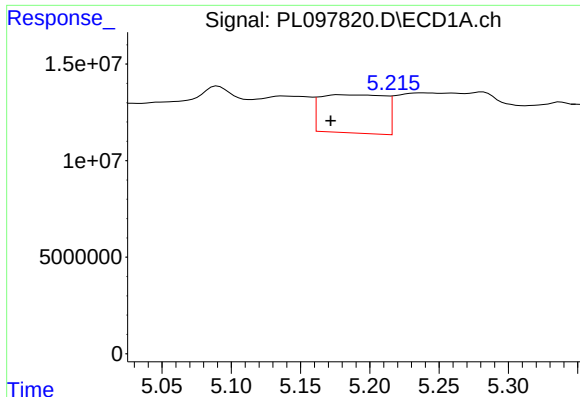

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.006 min
Response: 64007301
Conc: 264.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

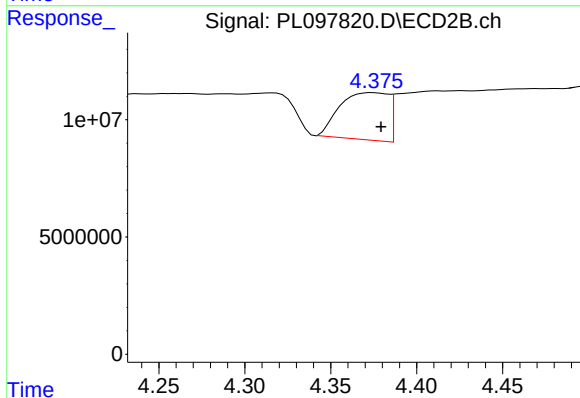


#24 Chlordane-2

R.T.: 4.375 min
Delta R.T.: -0.005 min
Response: 39203261
Conc: 127.54 ng/ml

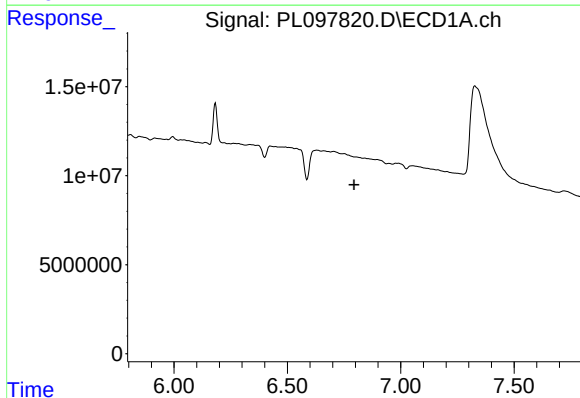


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

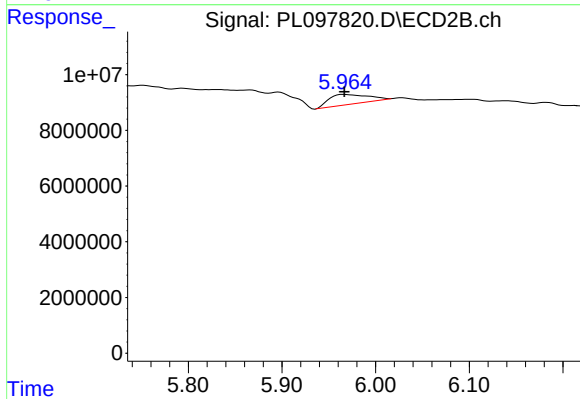

#27 Chlordane-5

R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 10414454
Conc: 31.66 ng/ml

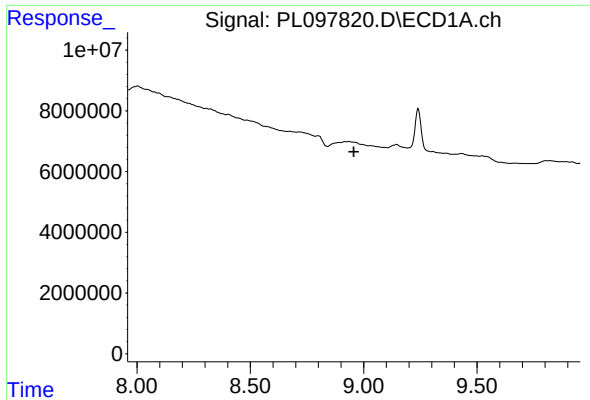

#28 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T. : 8.957 min

Response: 0

Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

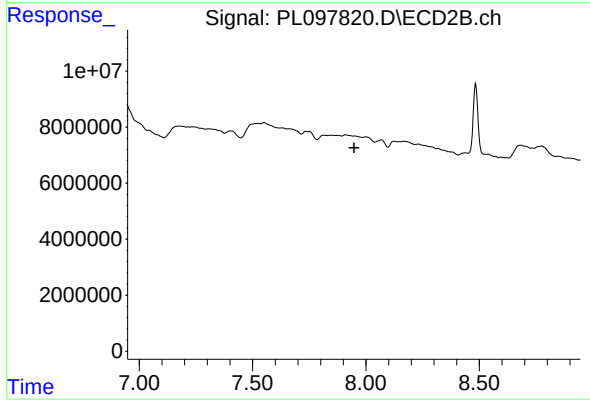

#28 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 7.948 min

Response: 0

Conc: N.D.