

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
 Data File : PL097821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 09:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 02:40:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.499	2.800	124.8E6	170.5E6	24.736	24.414
28)	SA Decachlor...	8.964	7.951	99343746	163.0E6	26.147	24.788
Target Compounds							
8)	B Heptachlo...	5.617	0.000	11862577	0	1.783	N.D. #
9)	A Endosulfan I	0.000	5.107f	0	44578283	N.D.	4.375 #
14)	MA Endrin	0.000	5.681	0	6577541	N.D.	0.787 #
15)	B Endosulfa...	6.709	0.000	3996023	0	0.782	N.D. #
18)	B Endrin al...	0.000	6.141	0	7942974	N.D.	1.244 #
26)	Chlordane-4	0.000	5.107f	0	44578283	N.D.	55.219 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
Data File : PL097821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 09:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 02:40:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

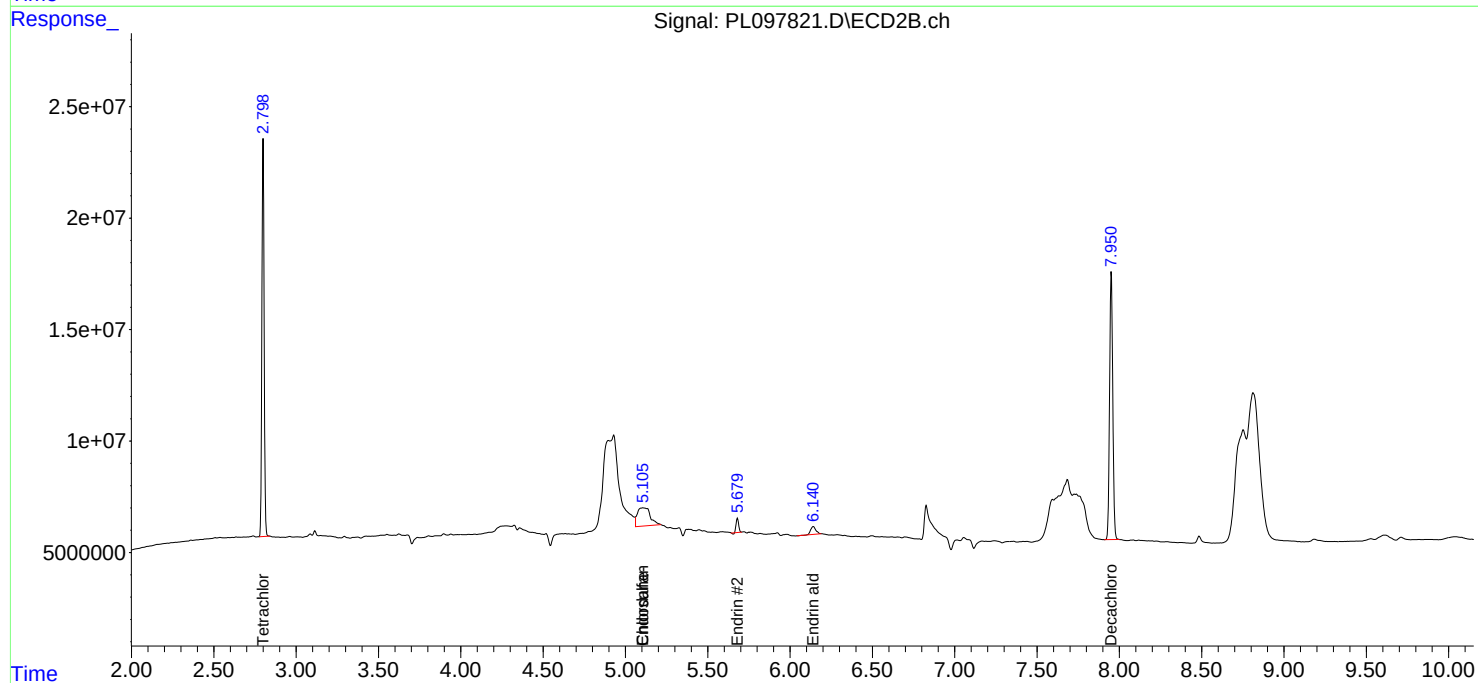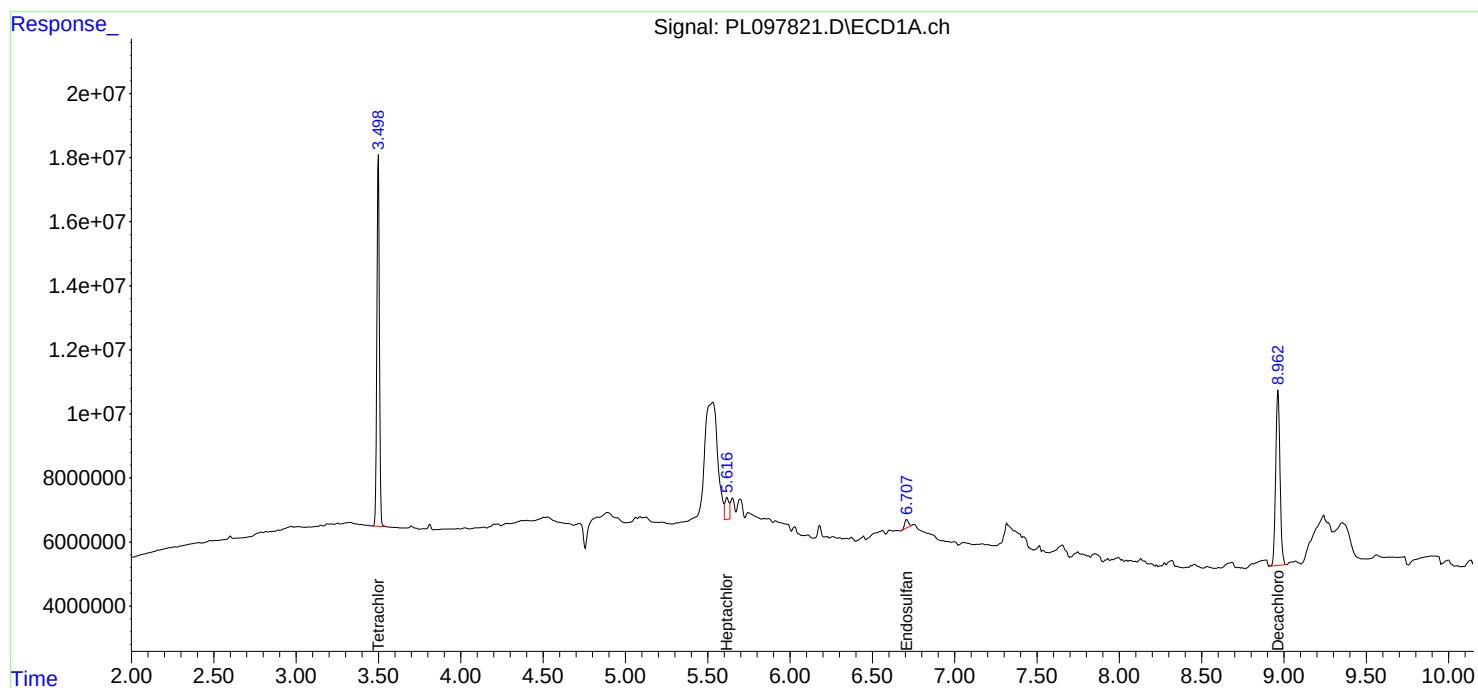


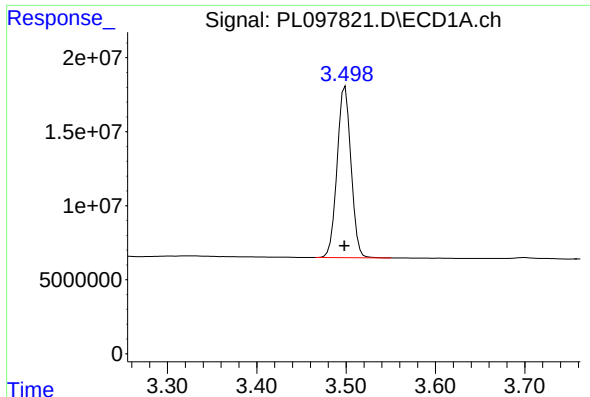

#1 Tetrachloro-m-xylene


R.T.: 3.499 min
Delta R.T.: 0.000 min
Response: 124842696
Conc: 24.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

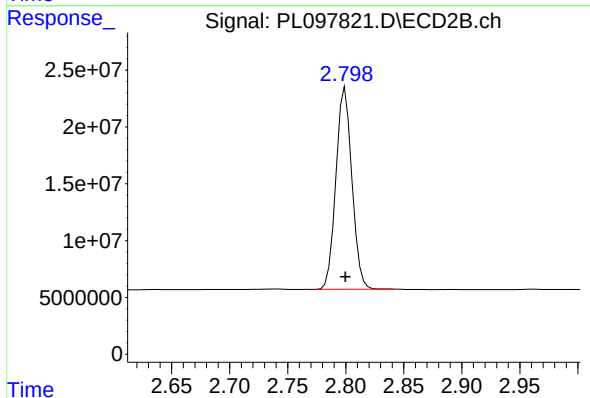


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 170539342
Conc: 24.41 ng/ml

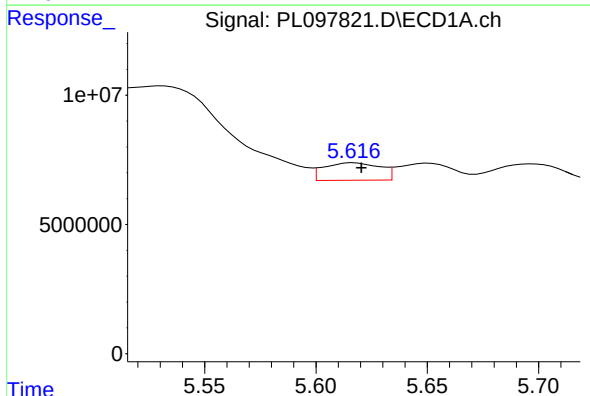


#8 Heptachlor epoxide

R.T.: 5.617 min
Delta R.T.: -0.003 min
Response: 11862577
Conc: 1.78 ng/ml

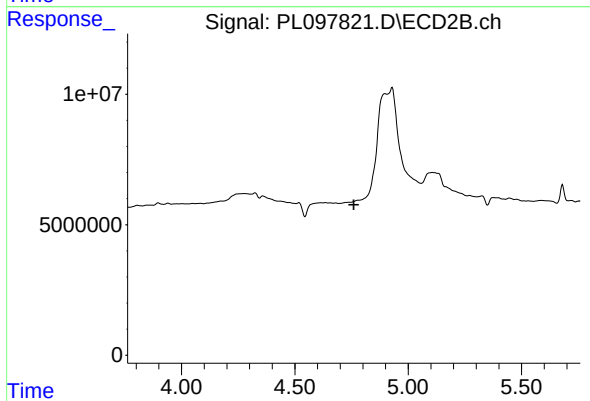

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.761 min
Response: 0
Conc: N.D.

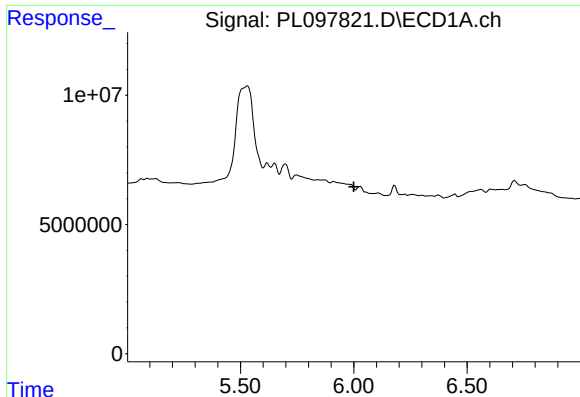

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.001 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

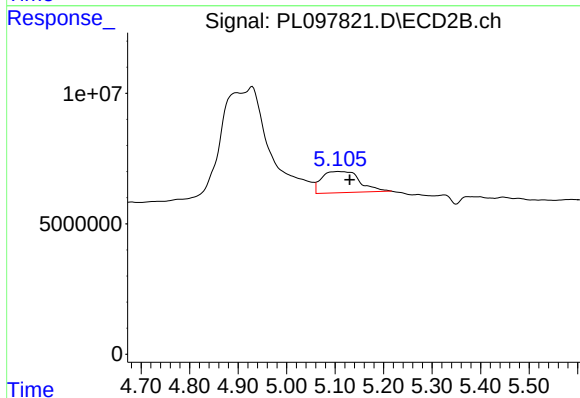


#9 Endosulfan I

R.T.: 5.107 min
Delta R.T.: -0.024 min
Response: 44578283
Conc: 4.38 ng/ml

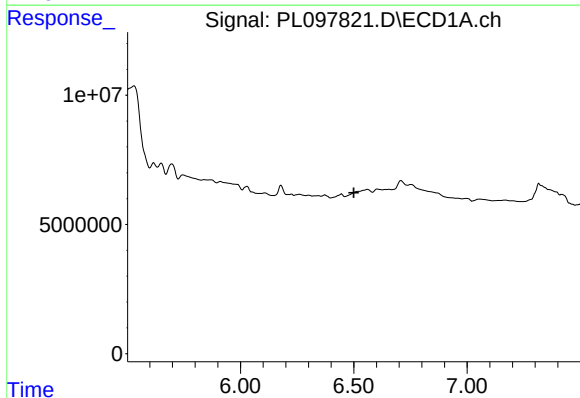


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.500 min
Response: 0
Conc: N.D.

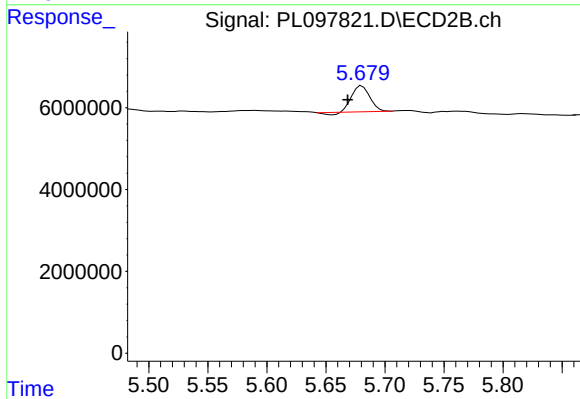

#14 Endrin


R.T.: 5.681 min
Delta R.T.: 0.012 min
Response: 6577541
Conc: 0.79 ng/ml

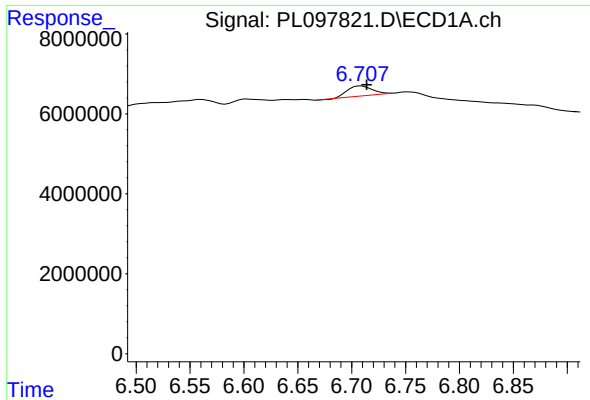

#15 Endosulfan II


R.T.: 6.709 min
Delta R.T.: -0.006 min
Response: 3996023
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

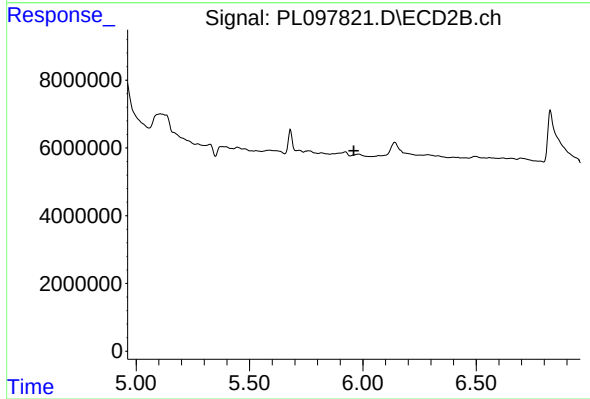


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.961 min
Response: 0
Conc: N.D.

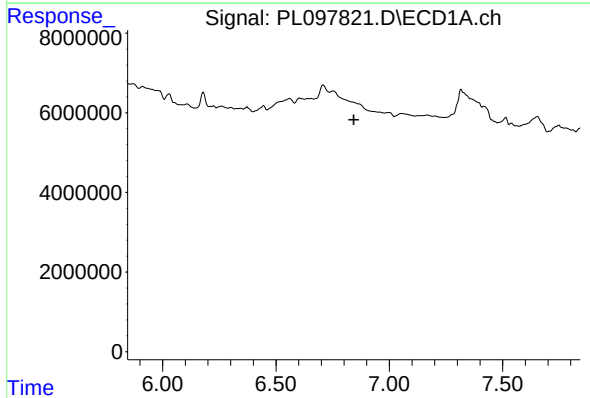


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

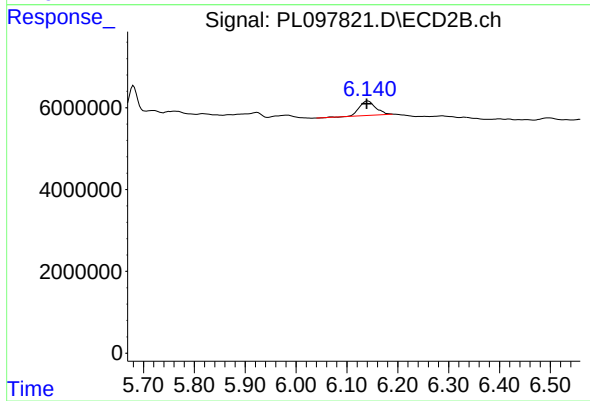

#18 Endrin aldehyde


R.T.: 6.141 min
Delta R.T.: 0.002 min
Response: 7942974
Conc: 1.24 ng/ml

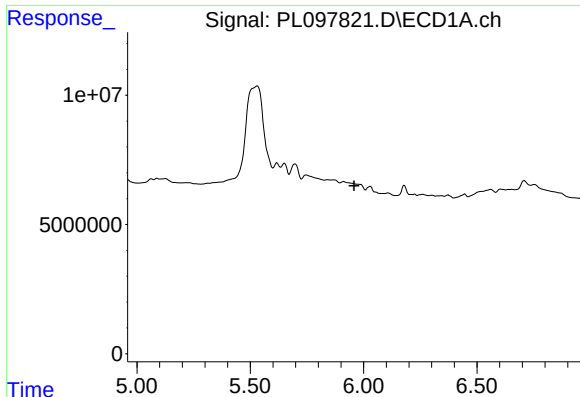

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

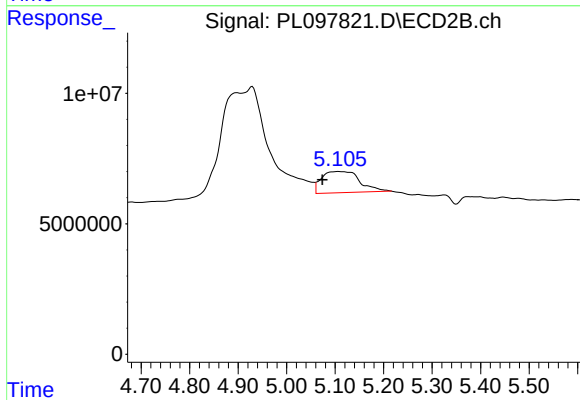


#26 Chlordane-4

R.T.: 5.107 min
Delta R.T.: 0.033 min
Response: 44578283
Conc: 55.22 ng/ml

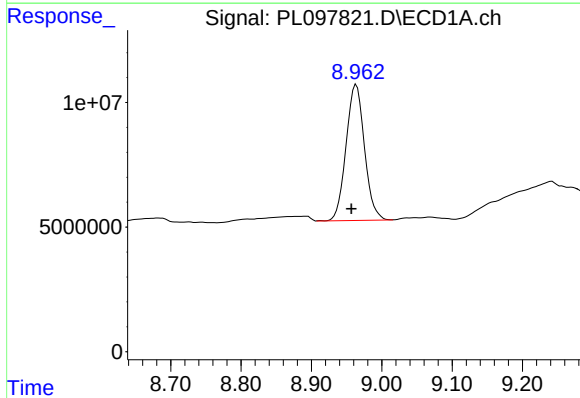

#28 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: 0.007 min
Response: 99343746
Conc: 26.15 ng/ml

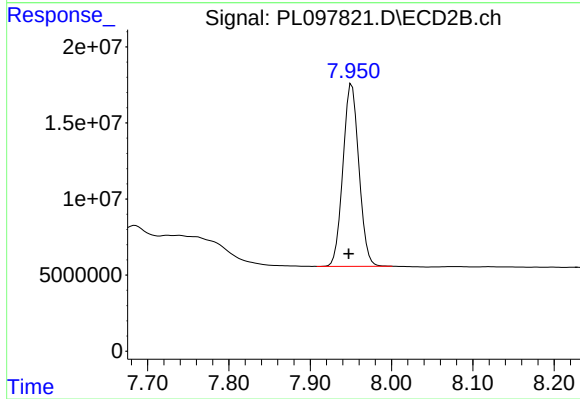

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.004 min
Response: 163007849
Conc: 24.79 ng/ml