

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
 Data File : PL097828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 18:15
 Operator : AR\AJ
 Sample : Q3826-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 02:42:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	2.800	115.9E6	158.4E6	22.972	22.677
28)	SA Decachlor...	8.962	7.951	63250202	113.6E6	16.647	17.270
Target Compounds							
3)	MA gamma-BHC...	0.000	3.638	0	10299239	N.D.	0.958 #
8)	B Heptachlo...	5.615	0.000	5567195	0	0.837	N.D. #
9)	A Endosulfan I	0.000	5.153f	0	62277434	N.D.	6.113 #
11)	B alpha-Chl...	0.000	5.092f	0	38383233	N.D.	3.743 #
12)	B 4,4'-DDE	6.132	5.266	134665	18409160	0.023	2.089 #
13)	MA Dieldrin	0.000	5.399	0	49441073	N.D.	5.276 #
14)	MA Endrin	0.000	5.678	0	6094641	N.D.	0.729 #
15)	B Endosulfa...	0.000	5.967	0	16103751	N.D.	1.946 #
17)	MA 4,4'-DDT	6.950	6.068	17639929	27548208	3.682	3.591
18)	B Endrin al...	0.000	6.147	0	10173507	N.D.	1.593 #
20)	A Methoxychlor	0.000	6.670f	0	33483180	N.D.	8.012 #
23)	Chlordane-1	0.000	3.807	0	17442852	N.D.	65.914 #
26)	Chlordane-4	0.000	5.092f	0	38383233	N.D.	47.545 #
27)	Chlordane-5	0.000	5.967	0	16103751	N.D.	48.952 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
Data File : PL097828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 18:15
Operator : AR\AJ
Sample : Q3826-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 02:42:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

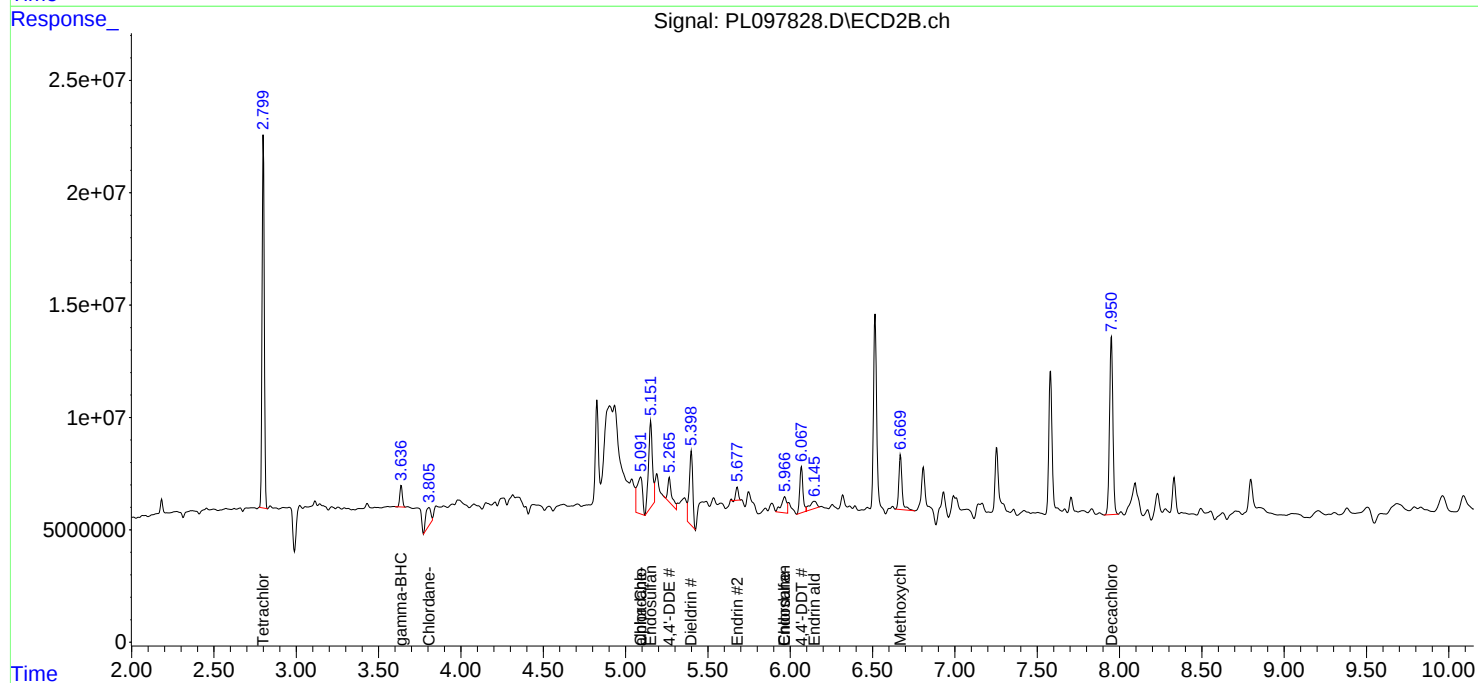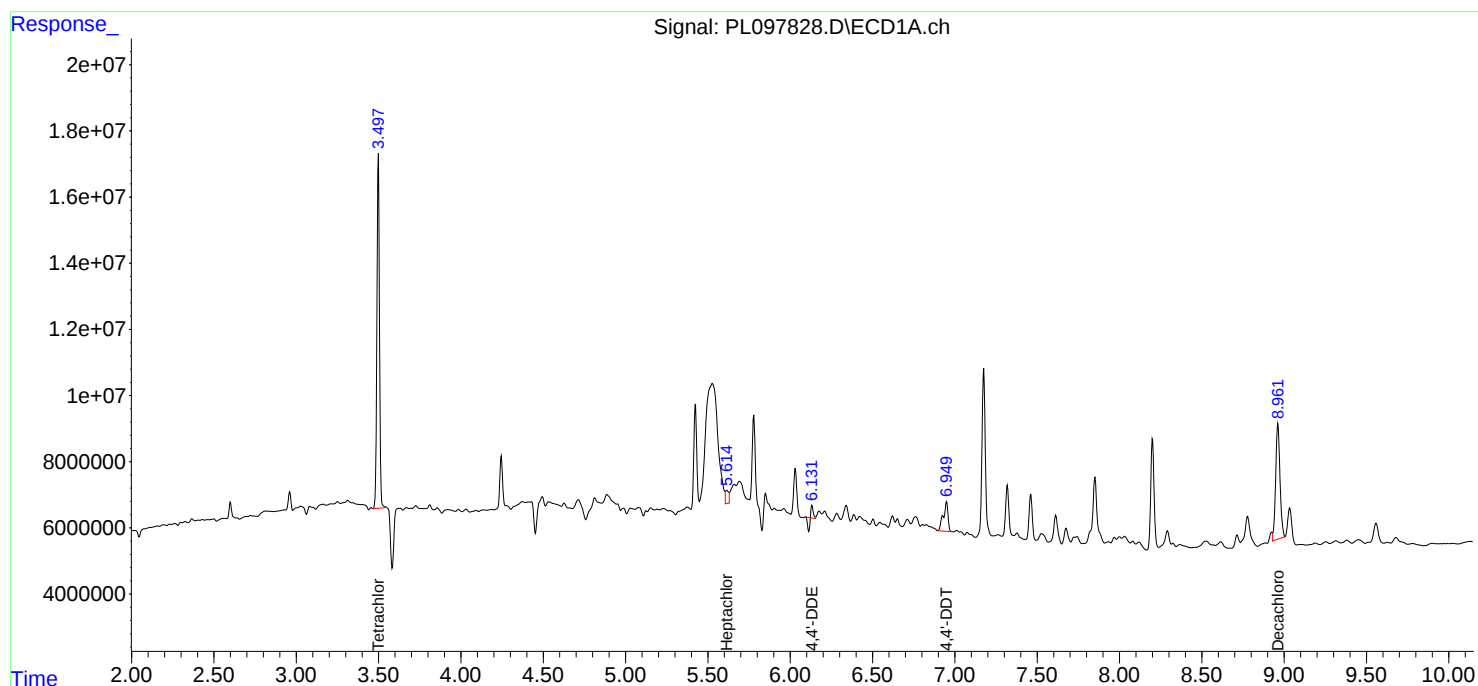


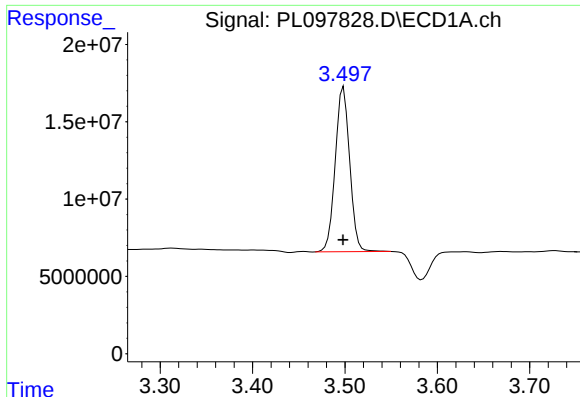

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 115939175
Conc: 22.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14

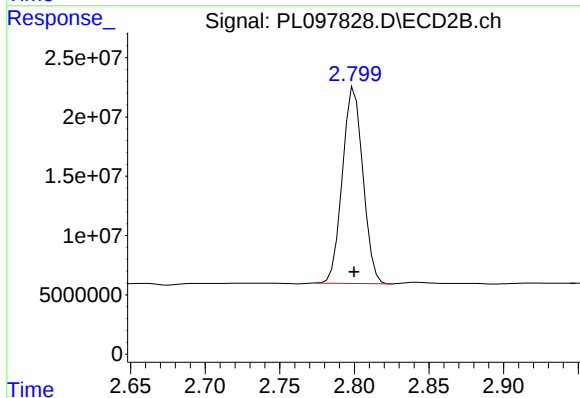


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 158402340
Conc: 22.68 ng/ml

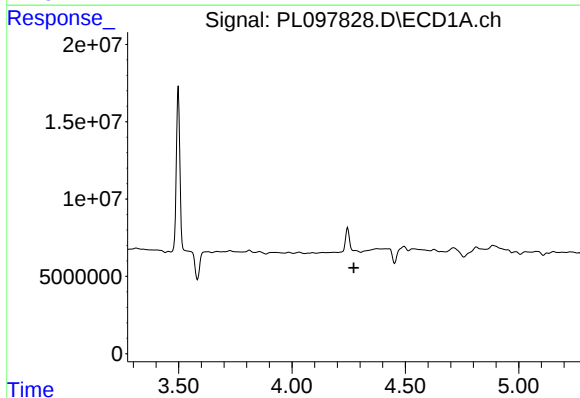


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

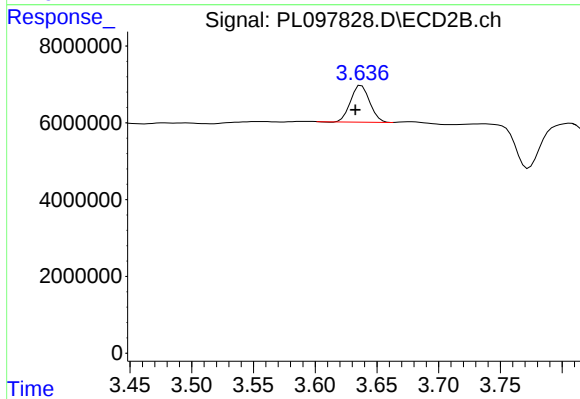

#3 gamma-BHC (Lindane)


R.T.: 3.638 min
Delta R.T.: 0.005 min
Response: 10299239
Conc: 0.96 ng/ml

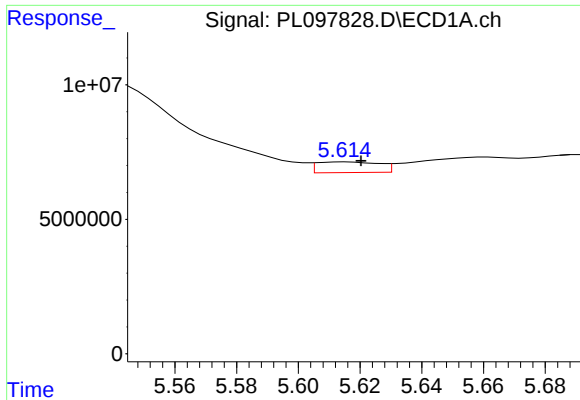

#8 Heptachlor epoxide


R.T.: 5.615 min
Delta R.T.: -0.005 min
Response: 5567195
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14

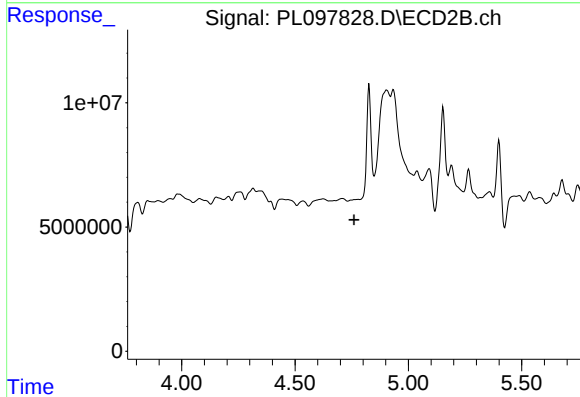


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.761 min
Response: 0
Conc: N.D.

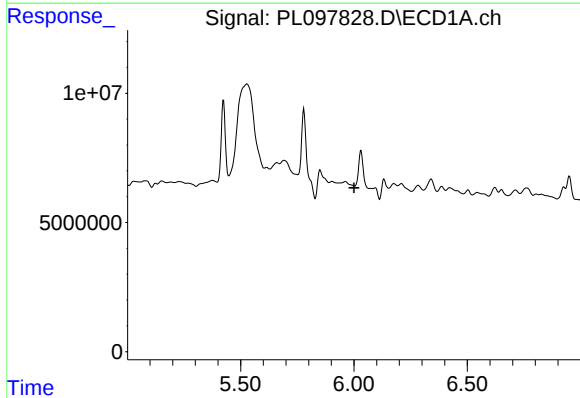


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.001 min
Response: 0
Conc: N.D.

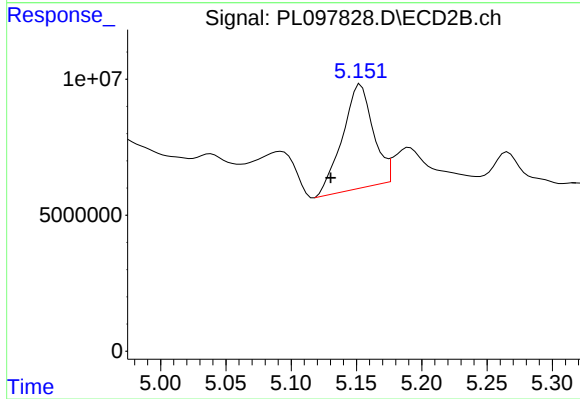

#9 Endosulfan I


R.T.: 5.153 min
Delta R.T.: 0.023 min
Response: 62277434
Conc: 6.11 ng/ml

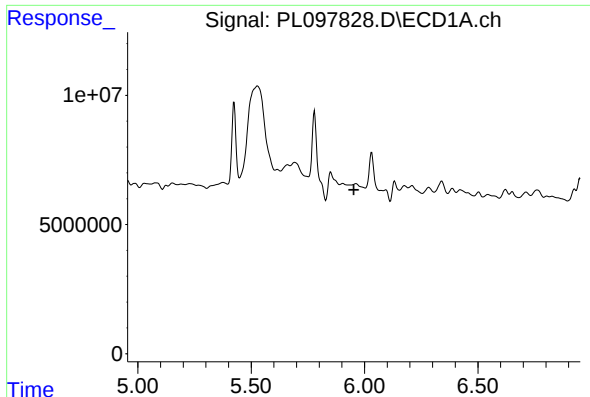

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14

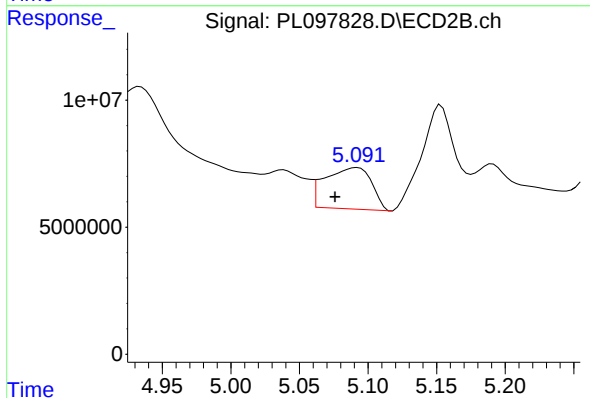


#11 alpha-Chlordane

R.T.: 5.092 min
Delta R.T.: 0.016 min
Response: 38383233
Conc: 3.74 ng/ml

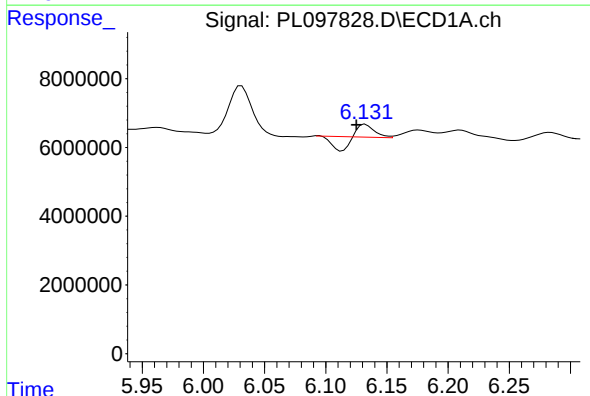


#12 4,4'-DDE

R.T.: 6.132 min
Delta R.T.: 0.007 min
Response: 134665
Conc: 0.02 ng/ml

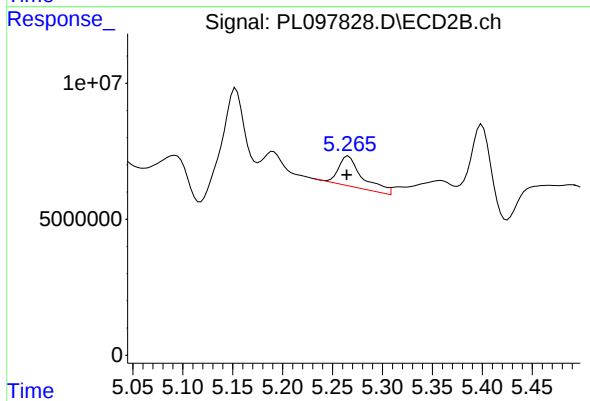

#12 4,4'-DDE


R.T.: 5.266 min
Delta R.T.: 0.002 min
Response: 18409160
Conc: 2.09 ng/ml

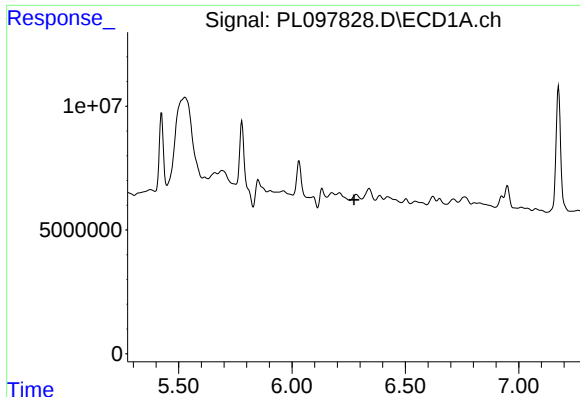

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14

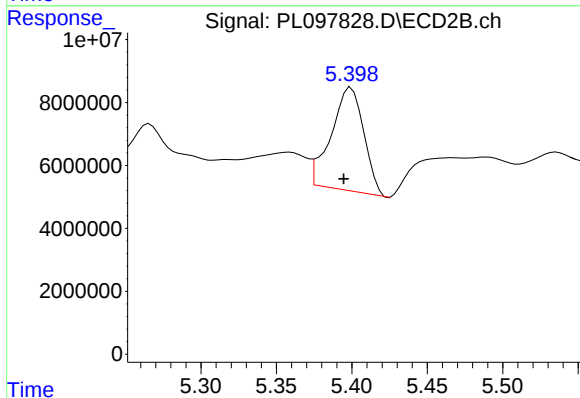


#13 Dieldrin

R.T.: 5.399 min
Delta R.T.: 0.005 min
Response: 49441073
Conc: 5.28 ng/ml

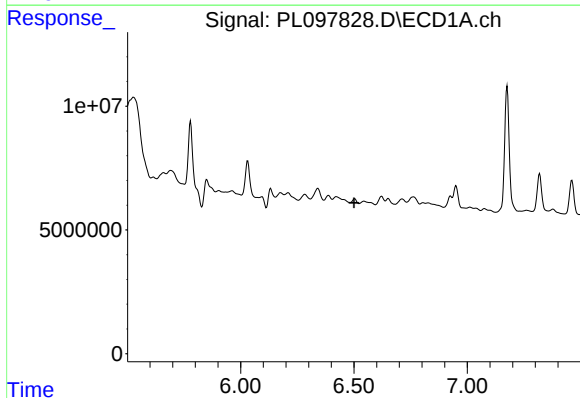


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.500 min
Response: 0
Conc: N.D.

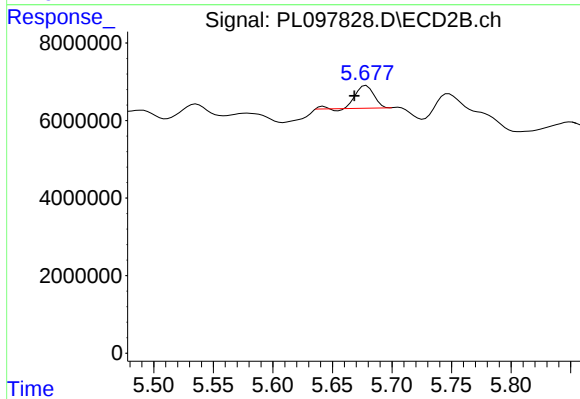

#14 Endrin


R.T.: 5.678 min
Delta R.T.: 0.010 min
Response: 6094641
Conc: 0.73 ng/ml

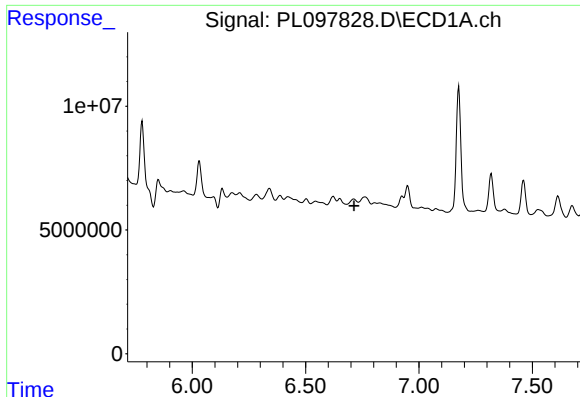

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14

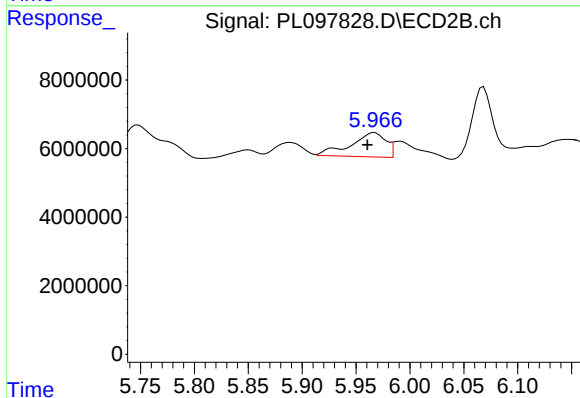


#15 Endosulfan II

R.T.: 5.967 min
Delta R.T.: 0.007 min
Response: 16103751
Conc: 1.95 ng/ml

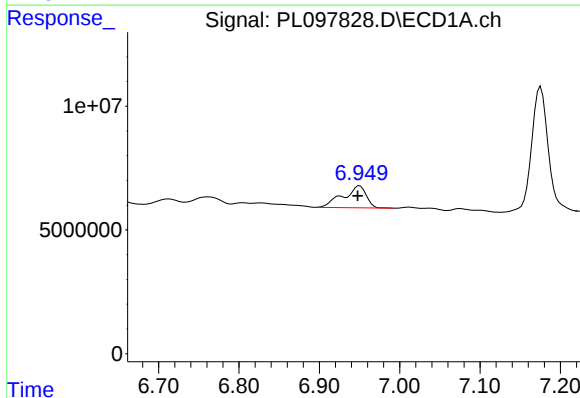


#17 4,4'-DDT

R.T.: 6.950 min
Delta R.T.: 0.002 min
Response: 17639929
Conc: 3.68 ng/ml

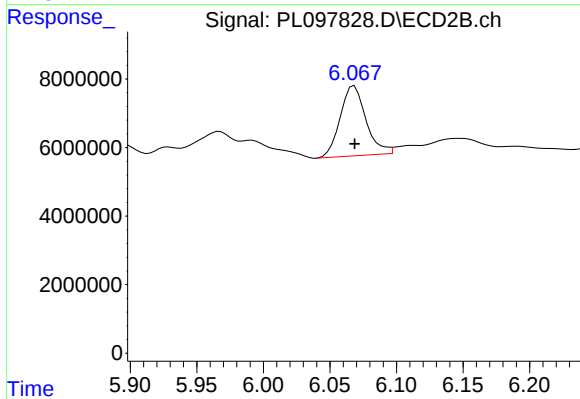

#17 4,4'-DDT


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 27548208
Conc: 3.59 ng/ml

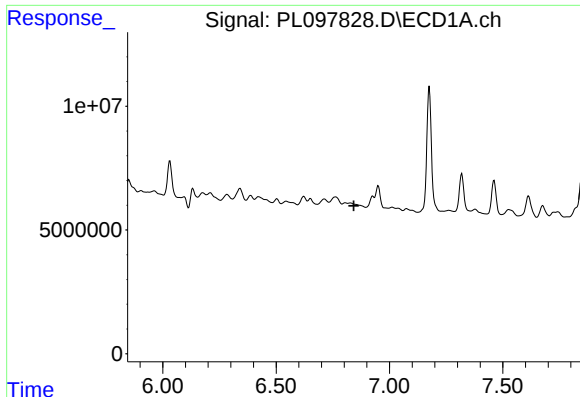

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14

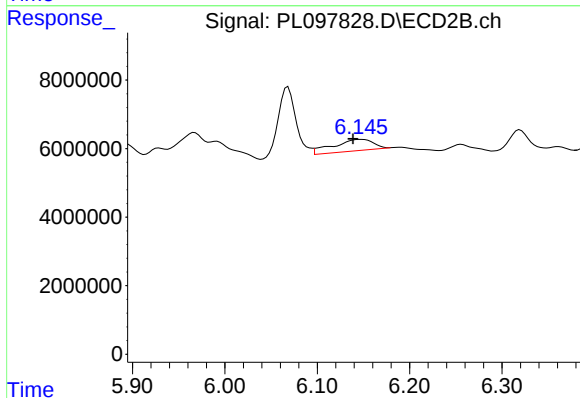


#18 Endrin aldehyde

R.T.: 6.147 min
Delta R.T.: 0.008 min
Response: 10173507
Conc: 1.59 ng/ml

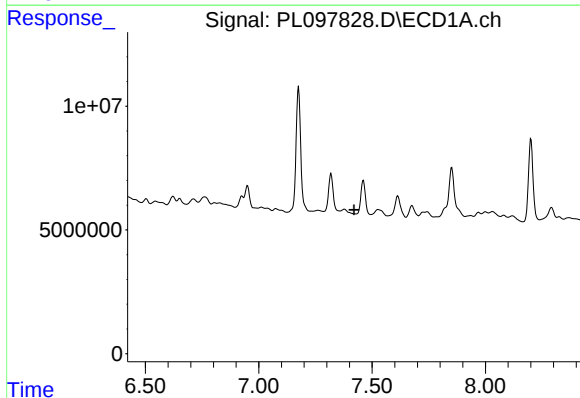


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.421 min
Response: 0
Conc: N.D.

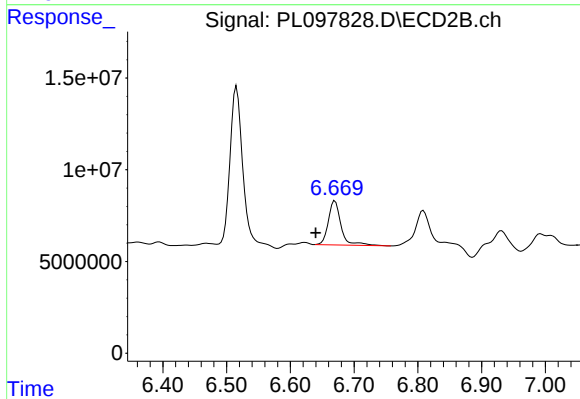

#20 Methoxychlor


R.T.: 6.670 min
Delta R.T.: 0.030 min
Response: 33483180
Conc: 8.01 ng/ml

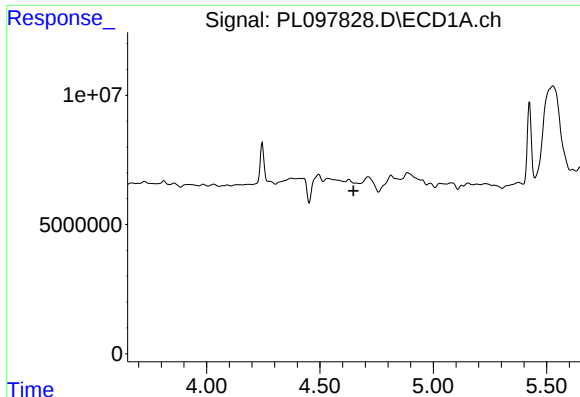

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14

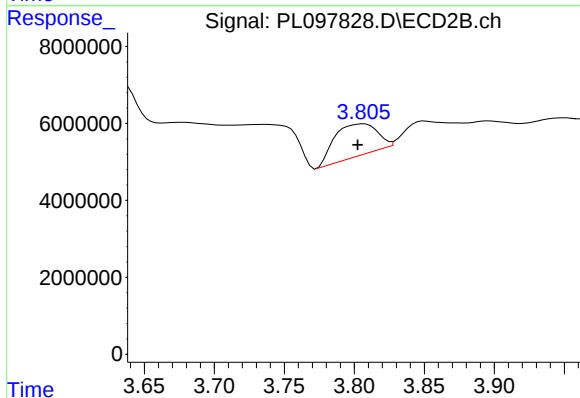


#23 Chlordane-1

R.T.: 3.807 min
Delta R.T.: 0.004 min
Response: 17442852
Conc: 65.91 ng/ml

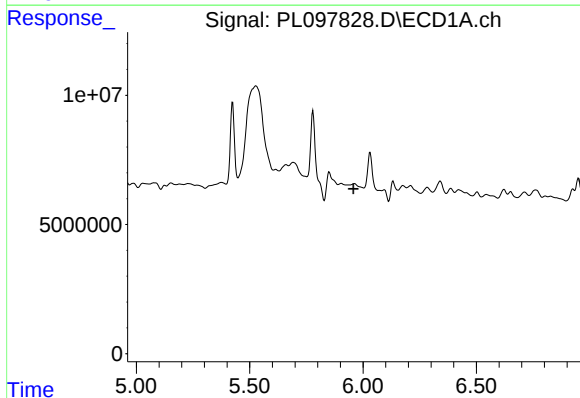


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.958 min
Response: 0
Conc: N.D.

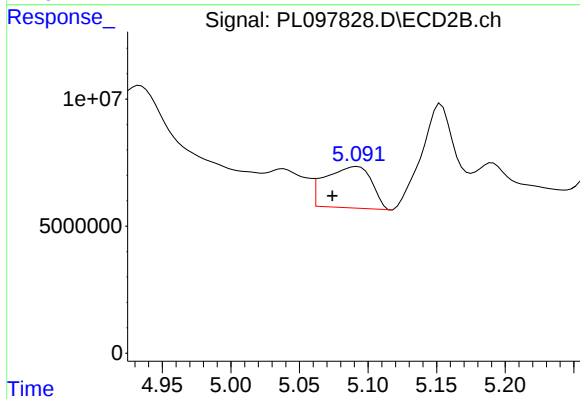

#26 Chlordane-4


R.T.: 5.092 min
Delta R.T.: 0.018 min
Response: 38383233
Conc: 47.55 ng/ml

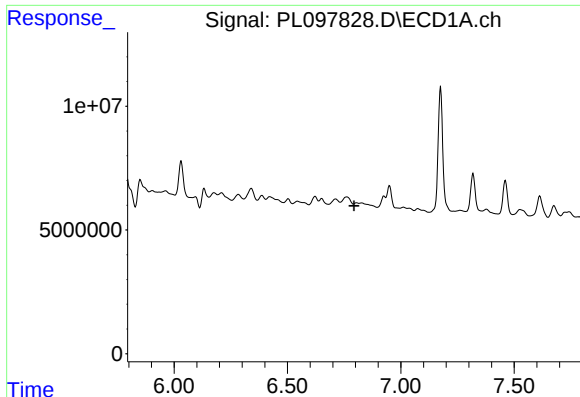

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14

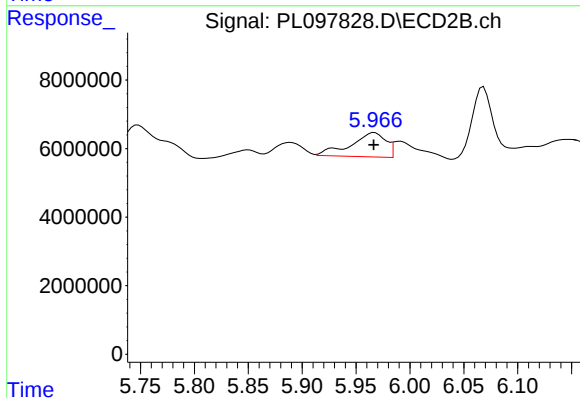


#27 Chlordane-5

R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 16103751
Conc: 48.95 ng/ml

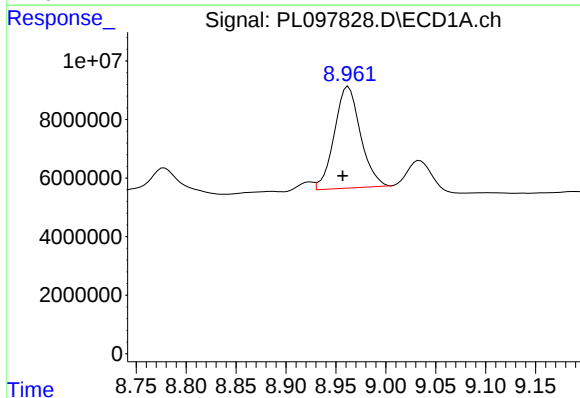

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.006 min
Response: 63250202
Conc: 16.65 ng/ml

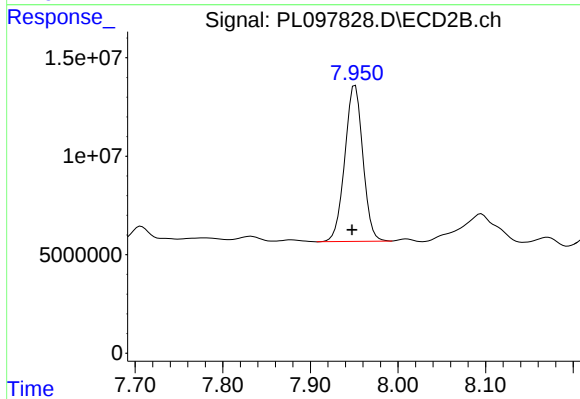

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.004 min
Response: 113570411
Conc: 17.27 ng/ml