

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
 Data File : PL097829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 18:29
 Operator : AR\AJ
 Sample : Q3826-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 02:43:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	2.800	116.5E6	157.2E6	23.079	22.504
28)	SA Decachlor...	8.961	7.950	58396633	107.5E6	15.370	16.347
Target Compounds							
9)	A Endosulfan I	6.030f	5.151f	4553146	16531367	0.773	1.623 #
10)	B gamma-Chl...	5.850f	0.000	191874	0	0.030	N.D. #
11)	B alpha-Chl...	0.000	5.093f	0	14913892	N.D.	1.454 #
13)	MA Dieldrin	0.000	5.399	0	16226477	N.D.	1.732 #
14)	MA Endrin	0.000	5.679	0	14408817	N.D.	1.724 #
15)	B Endosulfa...	6.710	5.965	17330026	9143938	3.391	1.105 #
17)	MA 4,4'-DDT	0.000	6.067	0	8792270	N.D.	1.146 #
18)	B Endrin al...	0.000	6.144	0	7685188	N.D.	1.204 #
20)	A Methoxychlor	0.000	6.670f	0	5391774	N.D.	1.290 #
25)	Chlordane-3	5.850f	0.000	191874	0	0.217	N.D. #
26)	Chlordane-4	0.000	5.093f	0	14913892	N.D.	18.474 #
27)	Chlordane-5	6.772f	5.965	3167059	9143938	17.414	27.796 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
Data File : PL097829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 18:29
Operator : AR\AJ
Sample : Q3826-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 02:43:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

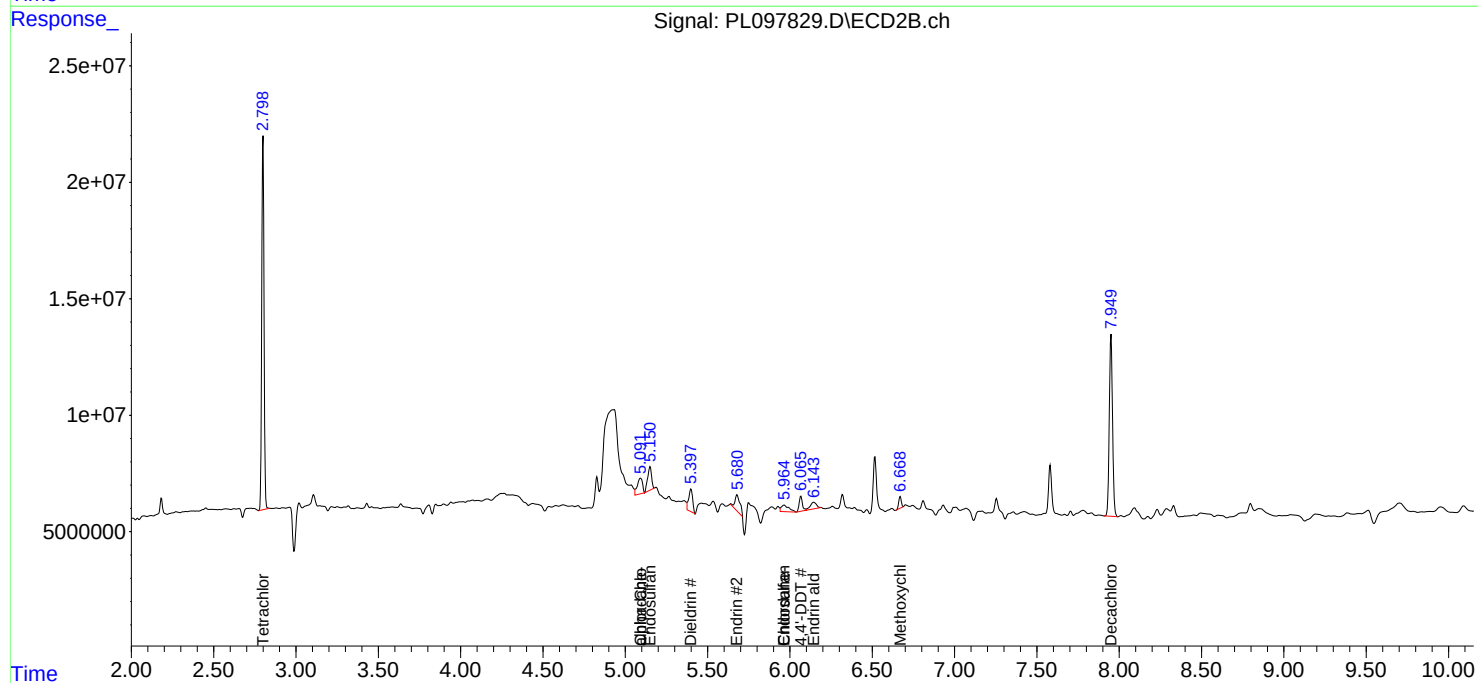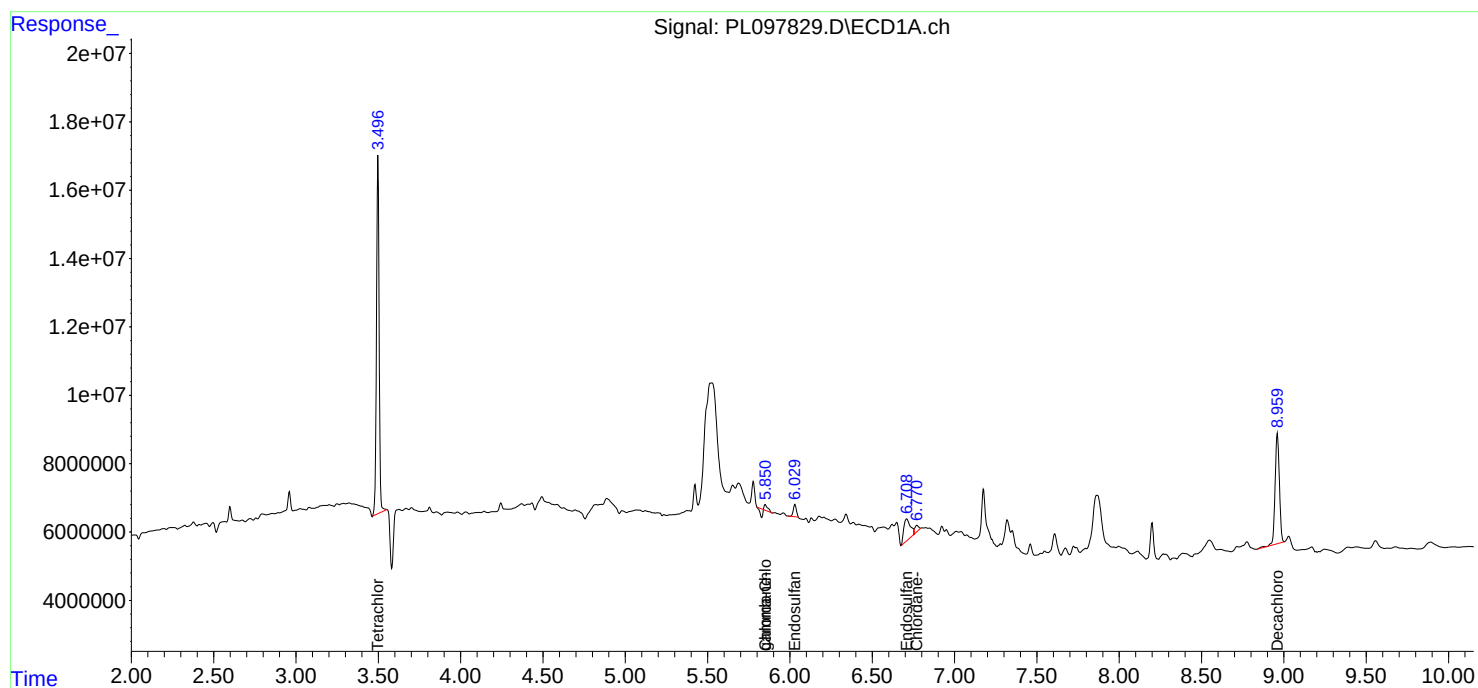


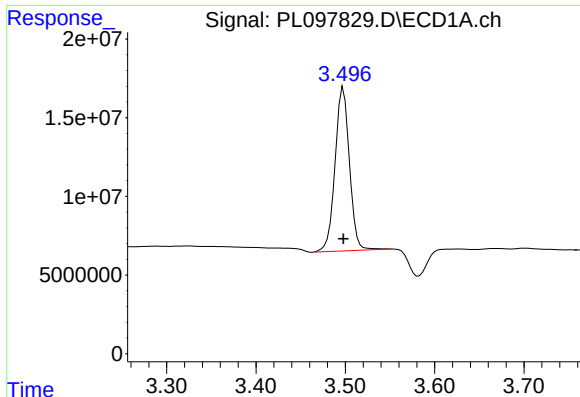

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 116476463
Conc: 23.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

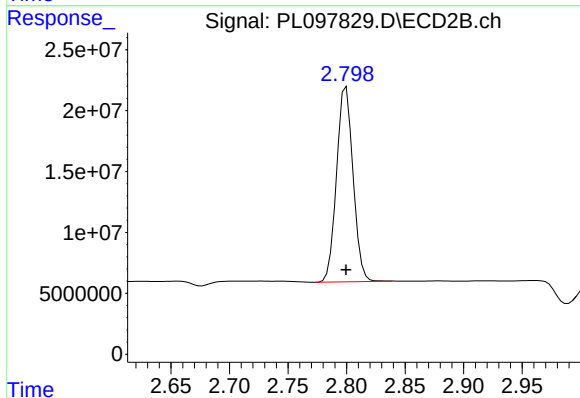


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 157193753
Conc: 22.50 ng/ml

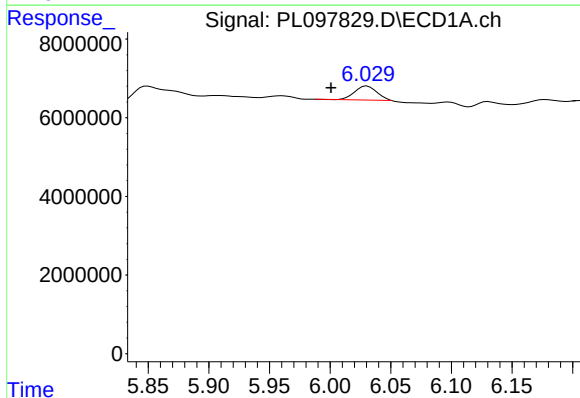


#9 Endosulfan I

R.T.: 6.030 min
Delta R.T.: 0.030 min
Response: 4553146
Conc: 0.77 ng/ml

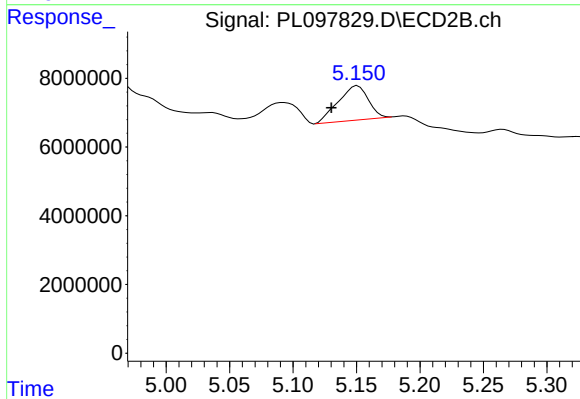

#9 Endosulfan I


R.T.: 5.151 min
Delta R.T.: 0.021 min
Response: 16531367
Conc: 1.62 ng/ml

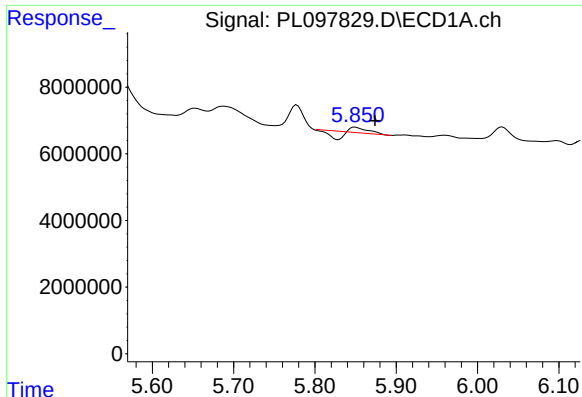

#10 gamma-Chlordane


R.T.: 5.850 min
Delta R.T.: -0.024 min
Response: 191874
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

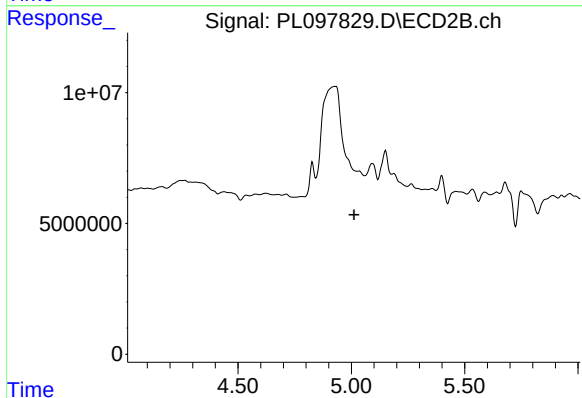


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

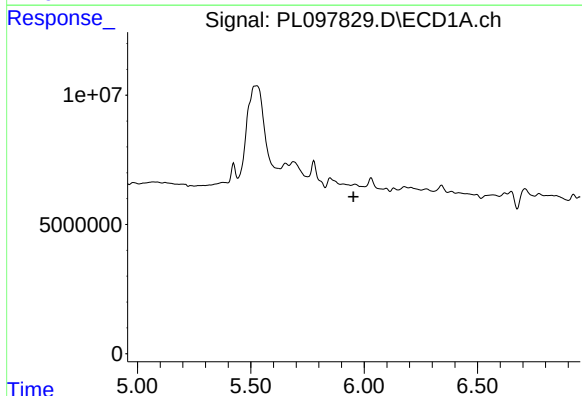


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.953 min
Response: 0
Conc: N.D.

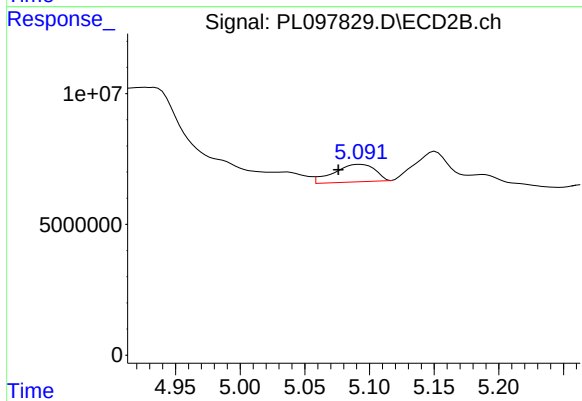

#11 alpha-Chlordane


R.T.: 5.093 min
Delta R.T.: 0.017 min
Response: 14913892
Conc: 1.45 ng/ml

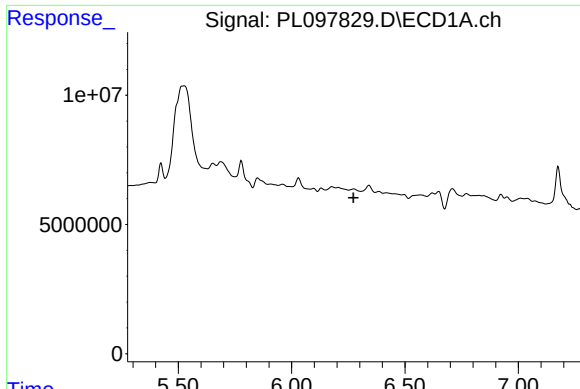

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

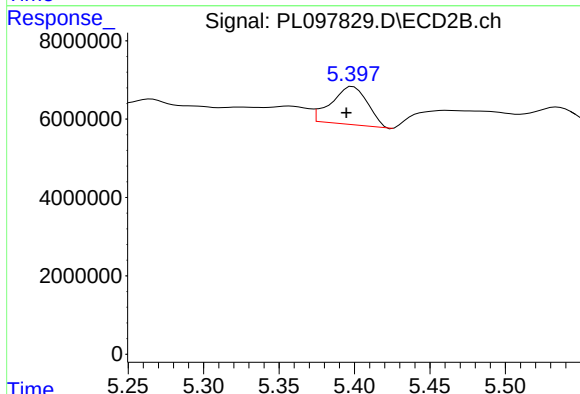


#13 Dieldrin

R.T.: 5.399 min
Delta R.T.: 0.004 min
Response: 16226477
Conc: 1.73 ng/ml

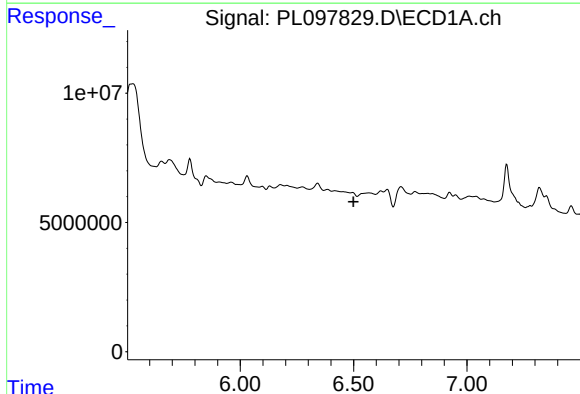


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.500 min
Response: 0
Conc: N.D.

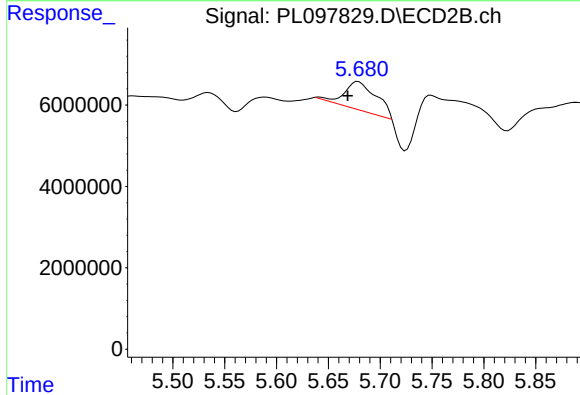

#14 Endrin


R.T.: 5.679 min
Delta R.T.: 0.010 min
Response: 14408817
Conc: 1.72 ng/ml

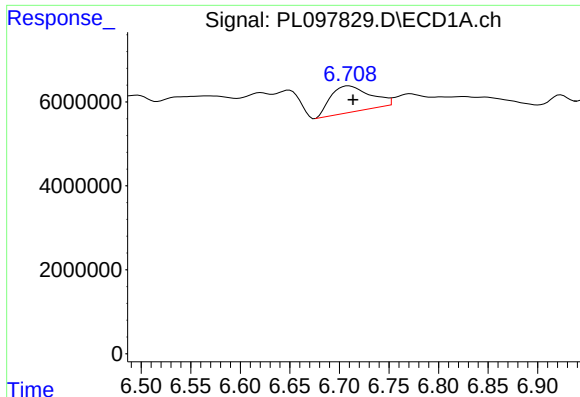

#15 Endosulfan II


R.T.: 6.710 min
Delta R.T.: -0.004 min
Response: 17330026
Conc: 3.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

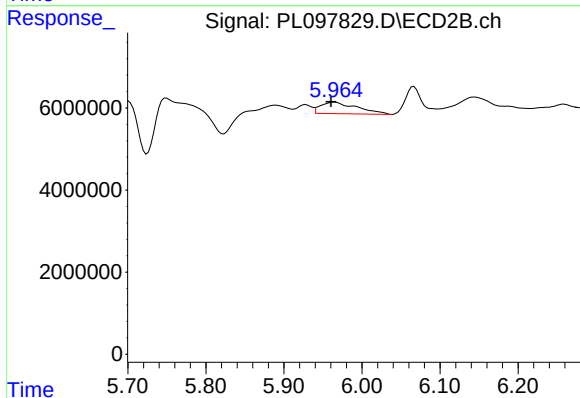


#15 Endosulfan II

R.T.: 5.965 min
Delta R.T.: 0.004 min
Response: 9143938
Conc: 1.10 ng/ml

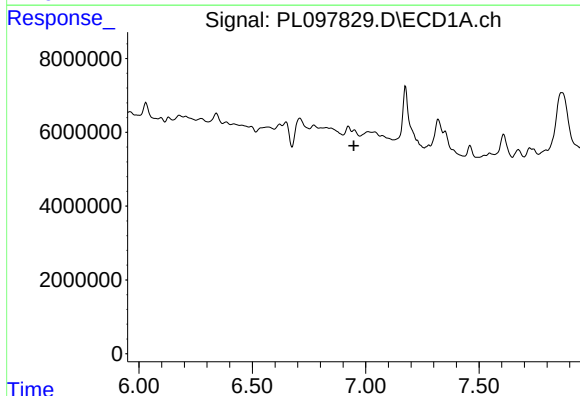


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.948 min
Response: 0
Conc: N.D.

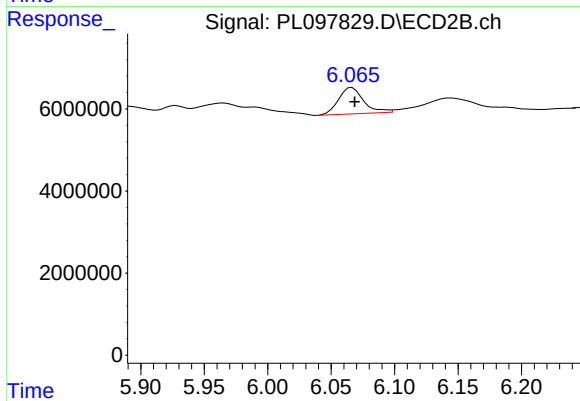

#17 4,4'-DDT


R.T.: 6.067 min
Delta R.T.: -0.002 min
Response: 8792270
Conc: 1.15 ng/ml

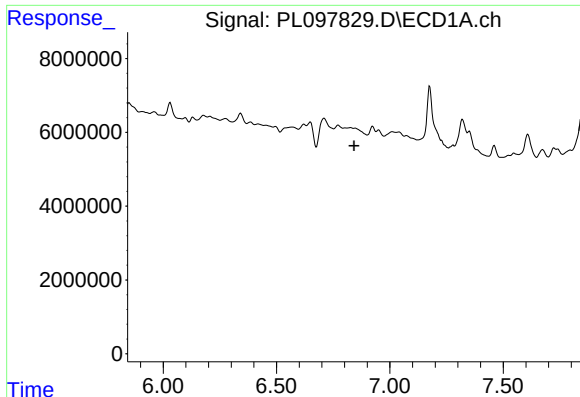

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

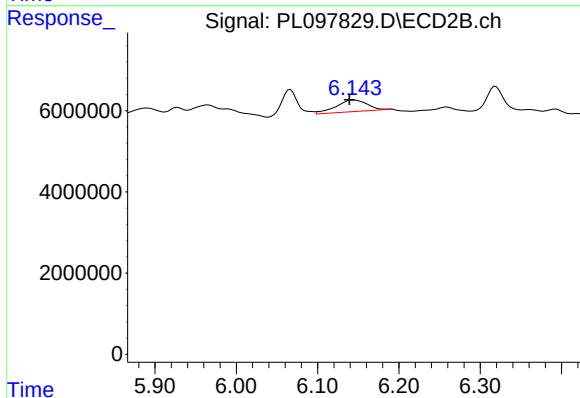


#18 Endrin aldehyde

R.T.: 6.144 min
Delta R.T.: 0.005 min
Response: 7685188
Conc: 1.20 ng/ml

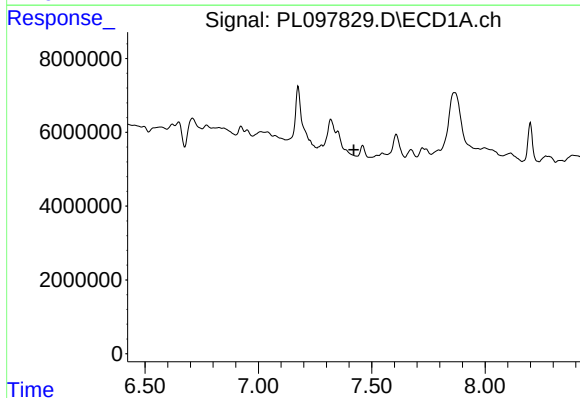


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.421 min
Response: 0
Conc: N.D.

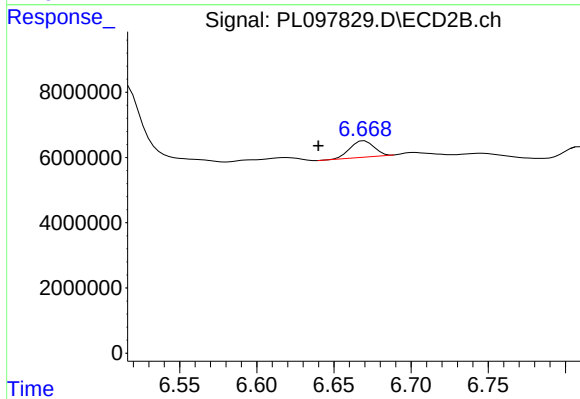

#20 Methoxychlor


R.T.: 6.670 min
Delta R.T.: 0.030 min
Response: 5391774
Conc: 1.29 ng/ml

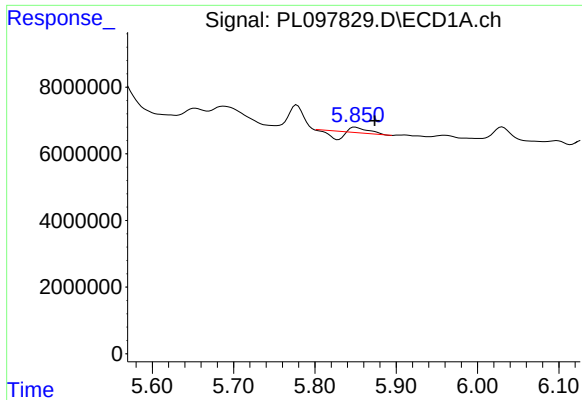

#25 Chlordane-3


R.T.: 5.850 min
Delta R.T.: -0.024 min
Response: 191874
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

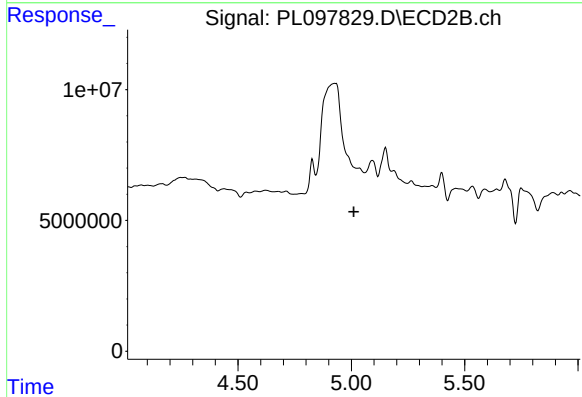


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.011 min
Response: 0
Conc: N.D.

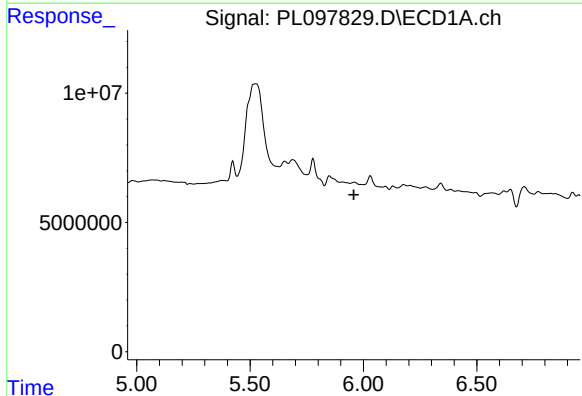


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.958 min
Response: 0
Conc: N.D.

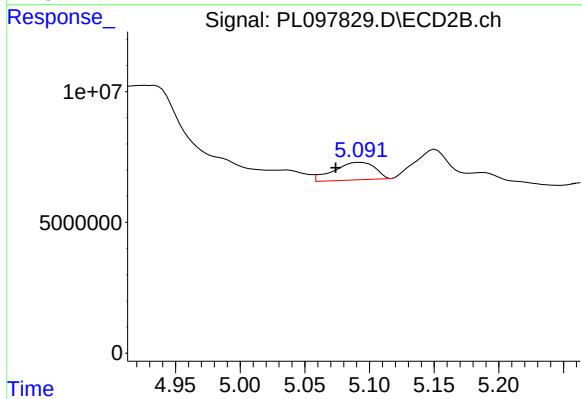

#26 Chlordane-4


R.T.: 5.093 min
Delta R.T.: 0.019 min
Response: 14913892
Conc: 18.47 ng/ml

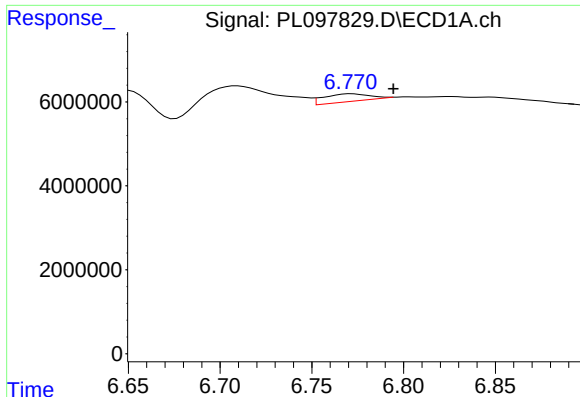

#27 Chlordane-5


R.T.: 6.772 min
Delta R.T.: -0.023 min
Response: 3167059
Conc: 17.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

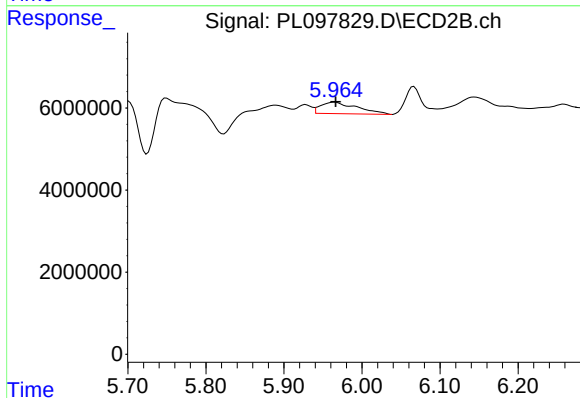


#27 Chlordane-5

R.T.: 5.965 min
Delta R.T.: -0.002 min
Response: 9143938
Conc: 27.80 ng/ml

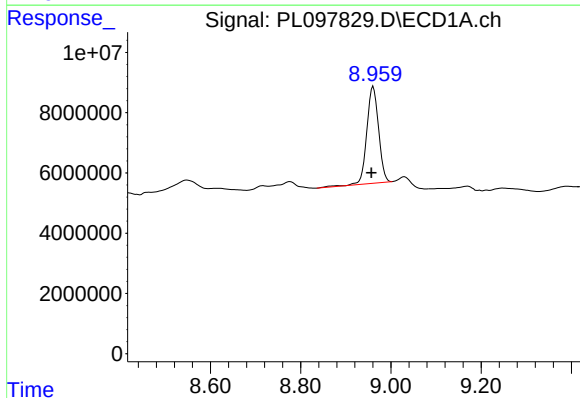

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: 0.004 min
Response: 58396633
Conc: 15.37 ng/ml

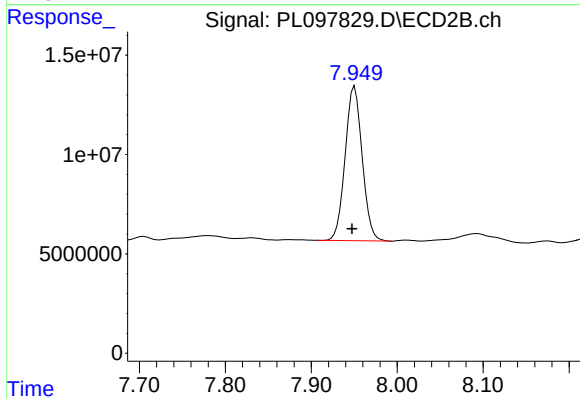

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.003 min
Response: 107500178
Conc: 16.35 ng/ml