

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
 Data File : PL097831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 18:56
 Operator : AR\AJ
 Sample : Q3826-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 02:43:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	2.800	74809561	103.9E6	14.823	14.871
2)	SA Decachlor...	8.960	7.950	37355233	67180678	9.832	10.216
Target Compounds							
3)	MA gamma-BHC...	0.000	3.637	0	14909406	N.D.	1.386 #
5)	MB Aldrin	0.000	4.260	0	9167888	N.D.	0.927 #
9)	A Endosulfan I	0.000	5.152f	0	67203153	N.D.	6.596 #
11)	B alpha-Chl...	0.000	5.092f	0	40302871	N.D.	3.930 #
13)	MA Dieldrin	0.000	5.399	0	62650243	N.D.	6.686 #
14)	MA Endrin	0.000	5.679	0	10955841	N.D.	1.311 #
15)	B Endosulfa...	0.000	5.967	0	15676951	N.D.	1.894 #
16)	A 4,4'-DDD	6.622	0.000	4675922	0	1.009	N.D. #
17)	MA 4,4'-DDT	0.000	6.065	0	5094409	N.D.	0.664 #
20)	A Methoxychlor	0.000	6.669f	0	35994916	N.D.	8.613 #
23)	Chlordane-1	4.625f	3.807	4246767	19002235	18.076	71.807 #
26)	Chlordane-4	0.000	5.092	0	40302871	N.D.	49.923 #
27)	Chlordane-5	0.000	5.967	0	15676951	N.D.	47.655 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121025\
Data File : PL097831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 18:56
Operator : AR\AJ
Sample : Q3826-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 02:43:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

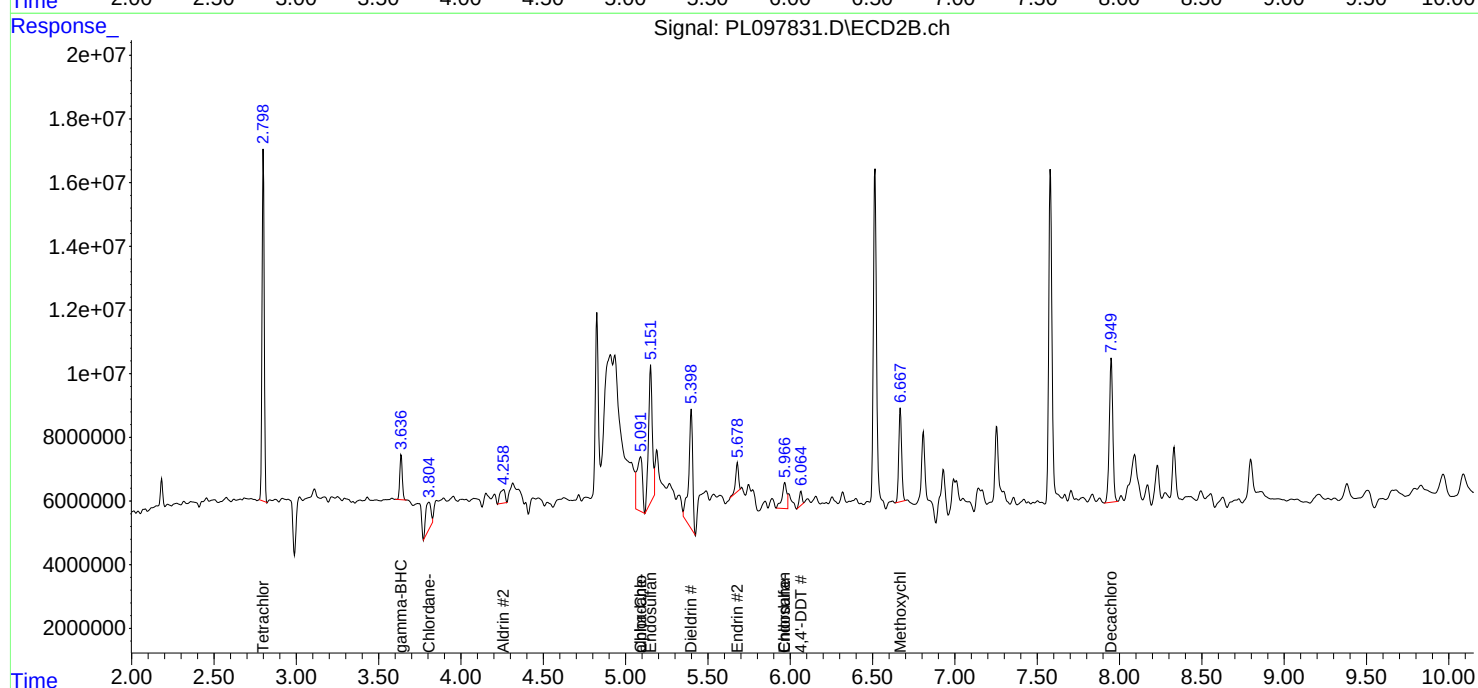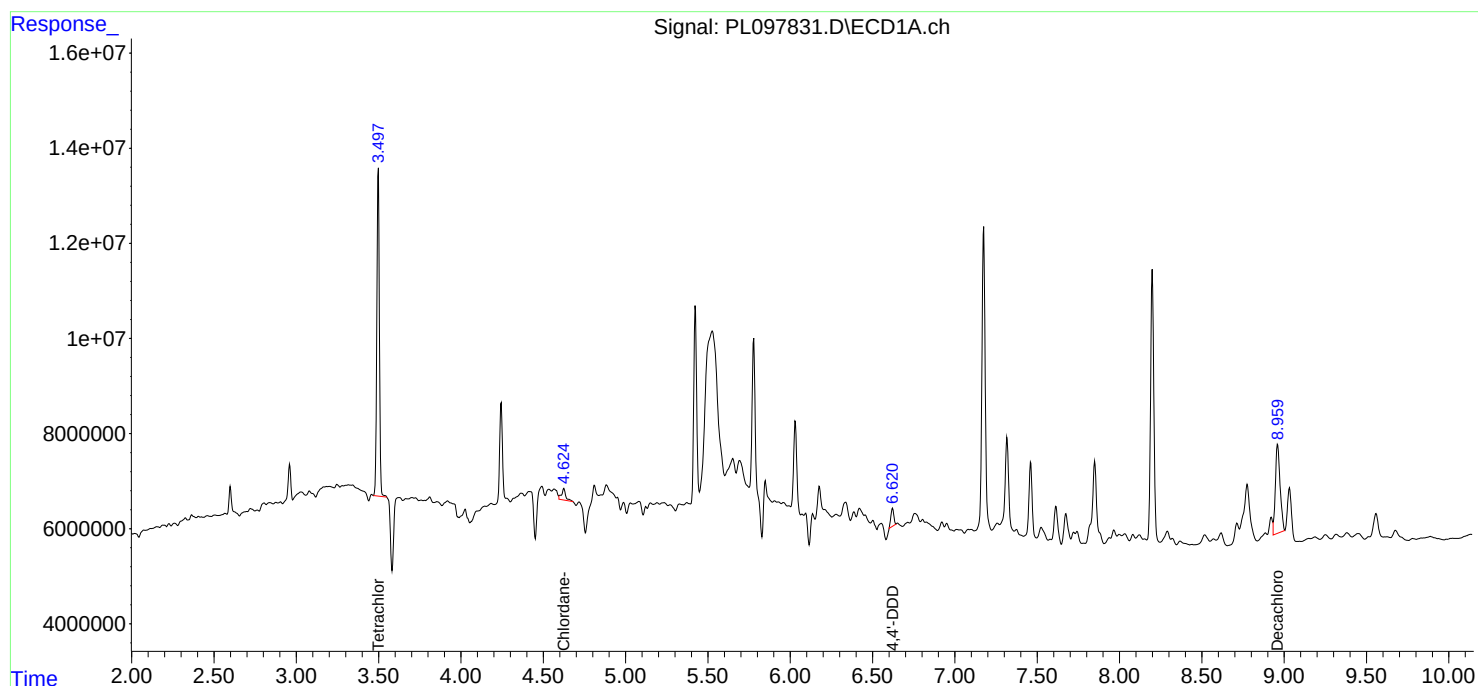


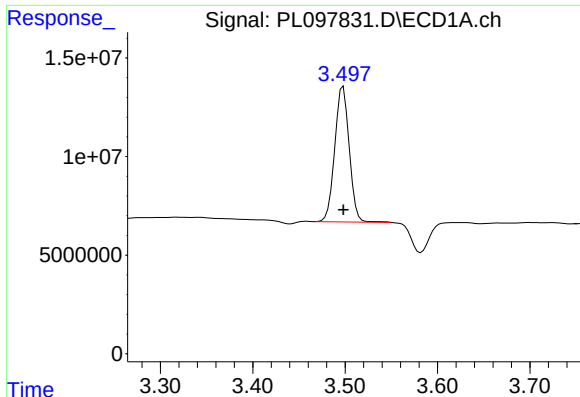

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 74809561
Conc: 14.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

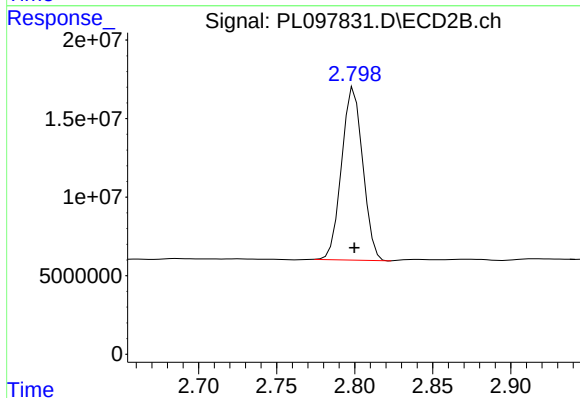


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 103876469
Conc: 14.87 ng/ml

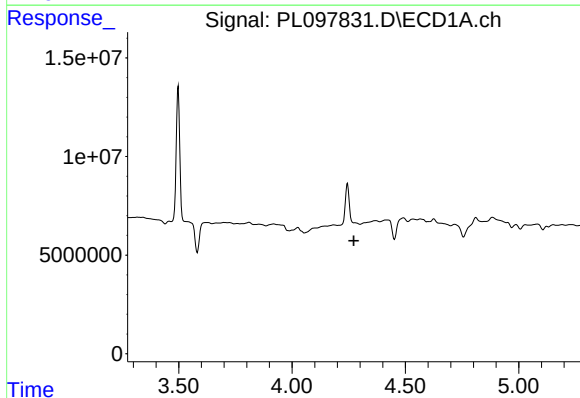


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

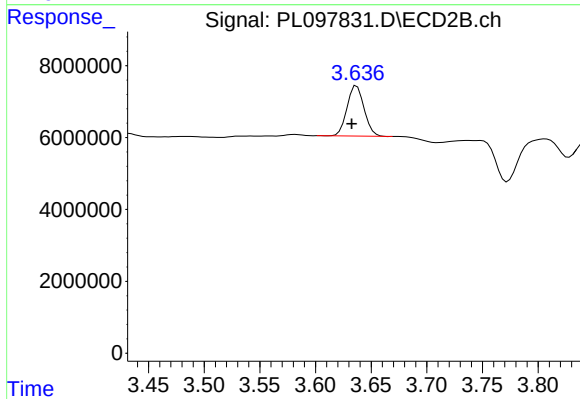

#3 gamma-BHC (Lindane)


R.T.: 3.637 min
Delta R.T.: 0.005 min
Response: 14909406
Conc: 1.39 ng/ml

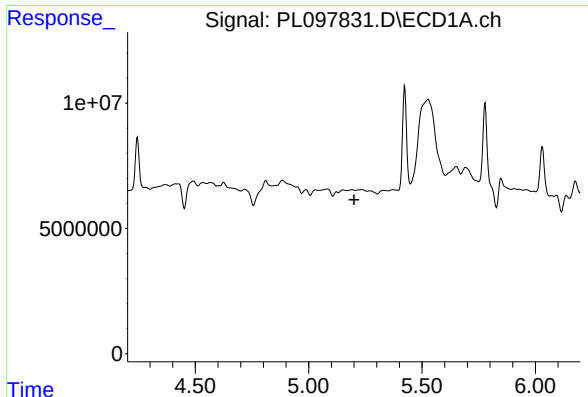

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

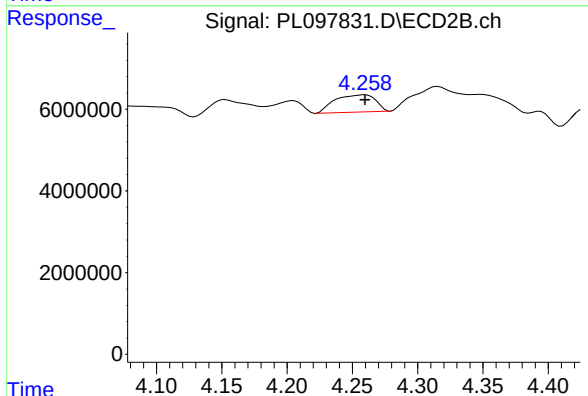


#5 Aldrin

R.T.: 4.260 min
Delta R.T.: 0.000 min
Response: 9167888
Conc: 0.93 ng/ml

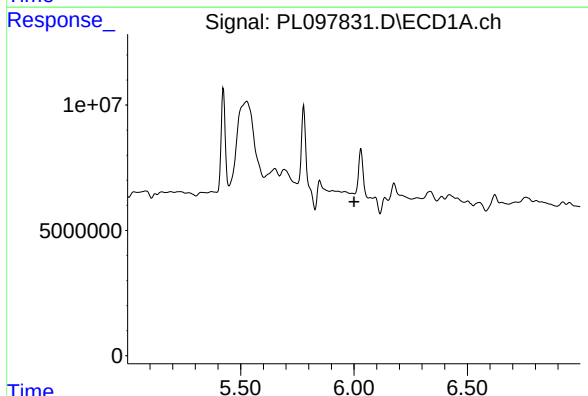


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.001 min
Response: 0
Conc: N.D.

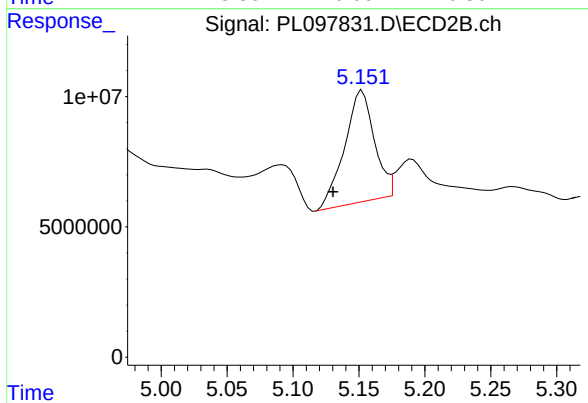

#9 Endosulfan I


R.T.: 5.152 min
Delta R.T.: 0.022 min
Response: 67203153
Conc: 6.60 ng/ml

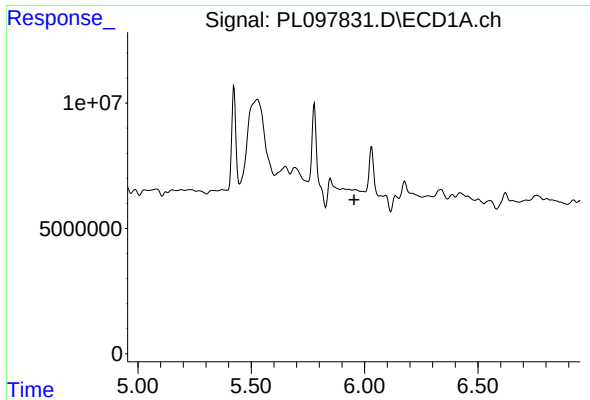

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

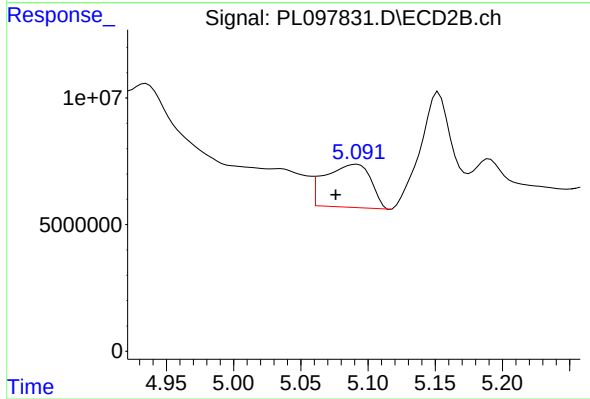


#11 alpha-Chlordane

R.T.: 5.092 min
Delta R.T.: 0.016 min
Response: 40302871
Conc: 3.93 ng/ml

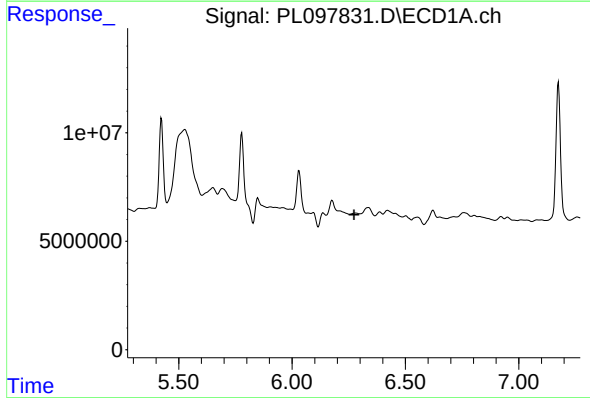


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.273 min
Response: 0
Conc: N.D.

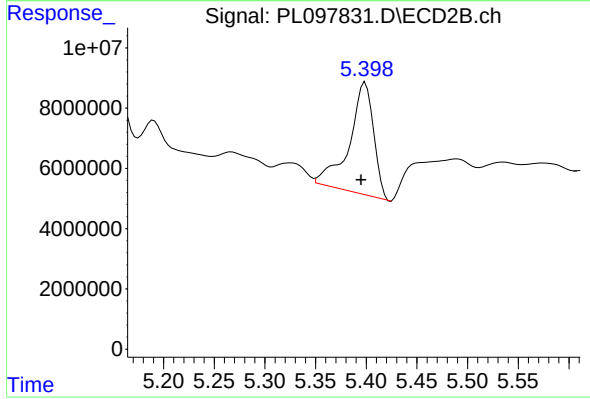

#13 Dieldrin


R.T.: 5.399 min
Delta R.T.: 0.004 min
Response: 62650243
Conc: 6.69 ng/ml

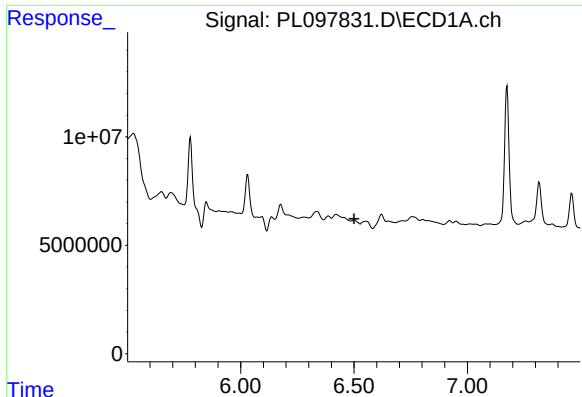

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

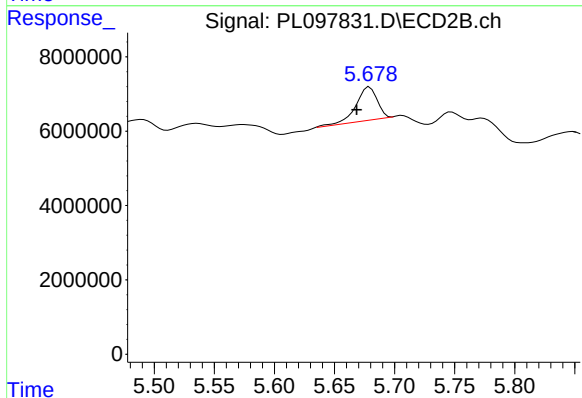


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.011 min
Response: 10955841
Conc: 1.31 ng/ml

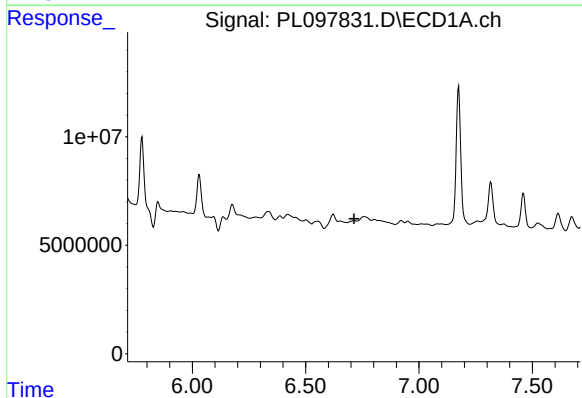


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.714 min
Response: 0
Conc: N.D.

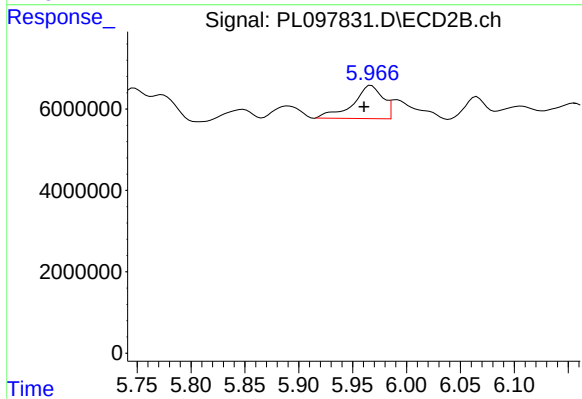

#15 Endosulfan II


R.T.: 5.967 min
Delta R.T.: 0.007 min
Response: 15676951
Conc: 1.89 ng/ml

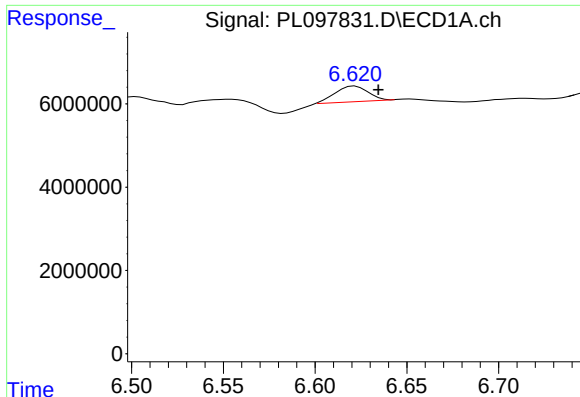

#16 4,4'-DDD


R.T.: 6.622 min
Delta R.T.: -0.013 min
Response: 4675922
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

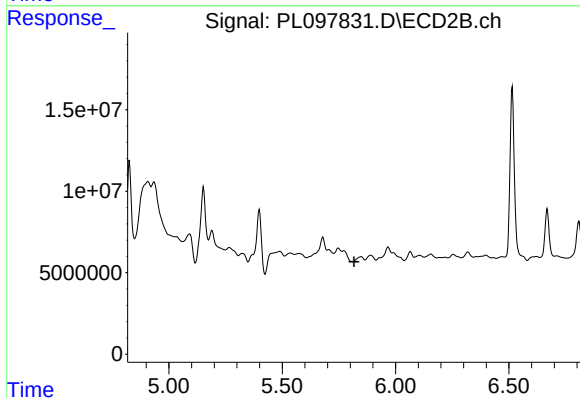


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.817 min
Response: 0
Conc: N.D.

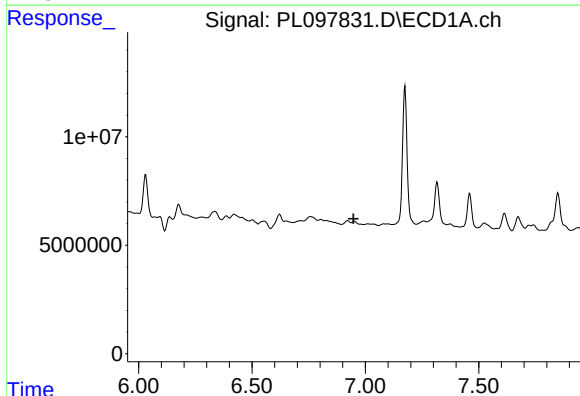


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.948 min
Response: 0
Conc: N.D.

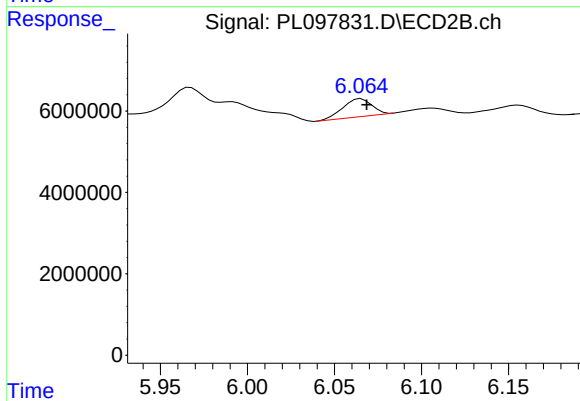

#17 4,4'-DDT


R.T.: 6.065 min
Delta R.T.: -0.003 min
Response: 5094409
Conc: 0.66 ng/ml

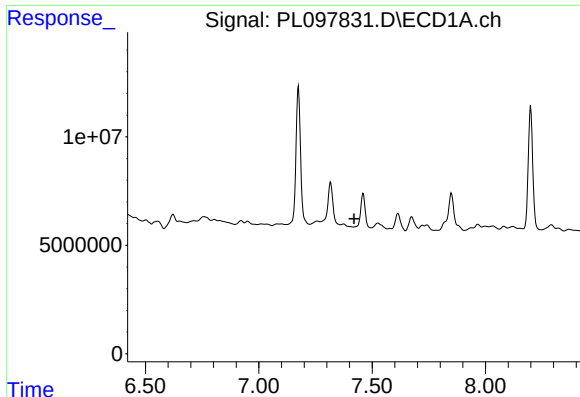

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

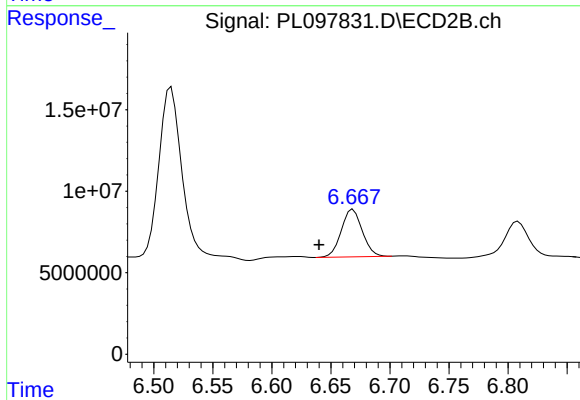


#20 Methoxychlor

R.T.: 6.669 min
Delta R.T.: 0.029 min
Response: 35994916
Conc: 8.61 ng/ml

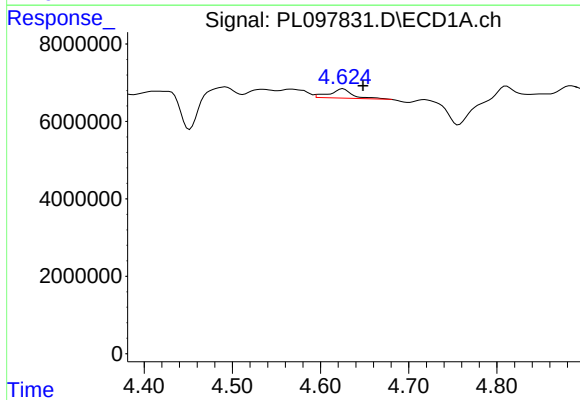


#23 Chlordane-1

R.T.: 4.625 min
Delta R.T.: -0.023 min
Response: 4246767
Conc: 18.08 ng/ml

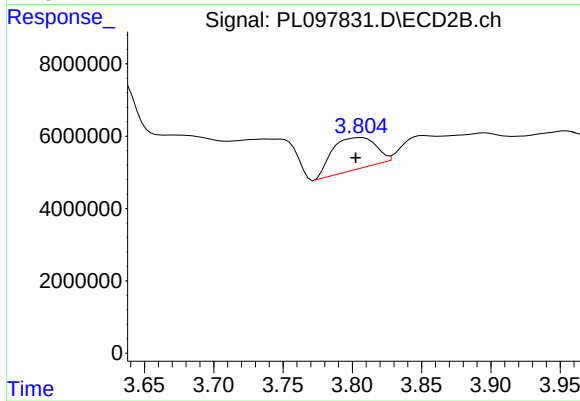

#23 Chlordane-1


R.T.: 3.807 min
Delta R.T.: 0.004 min
Response: 19002235
Conc: 71.81 ng/ml

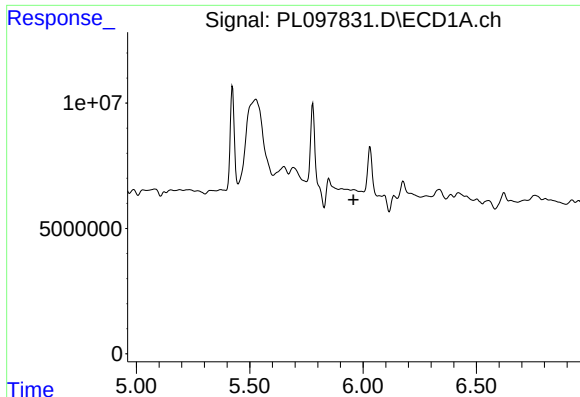

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

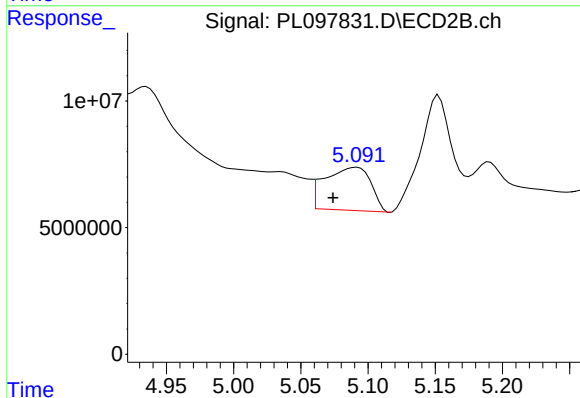


#26 Chlordane-4

R.T.: 5.092 min
Delta R.T.: 0.018 min
Response: 40302871
Conc: 49.92 ng/ml

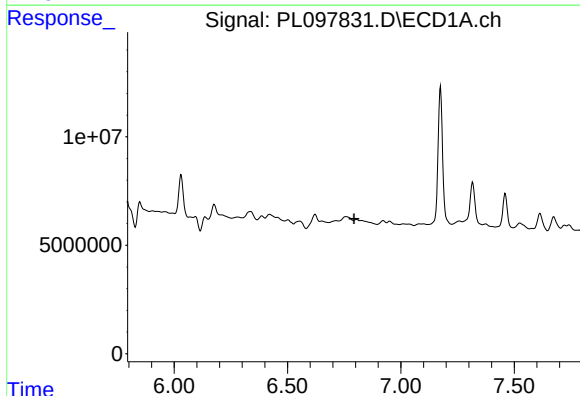


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

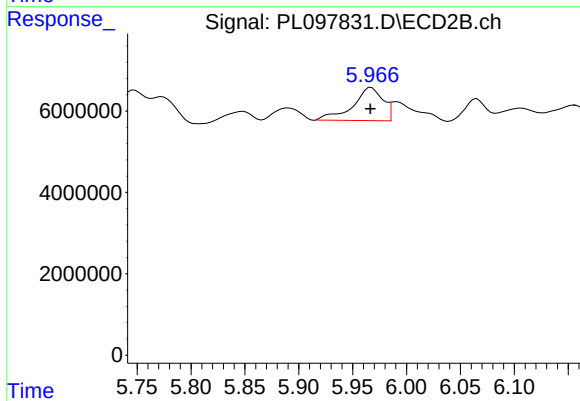

#27 Chlordane-5


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 15676951
Conc: 47.65 ng/ml

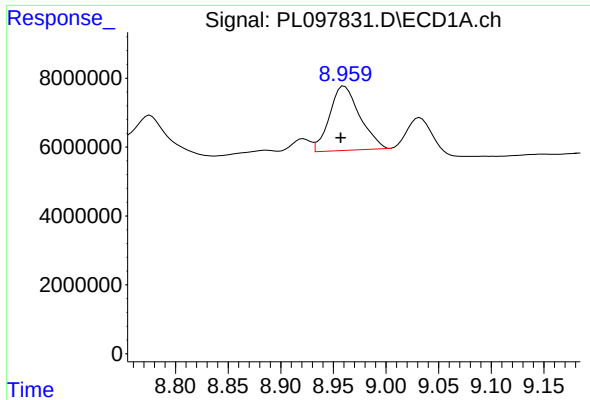

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: 0.004 min
Response: 37355233
Conc: 9.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

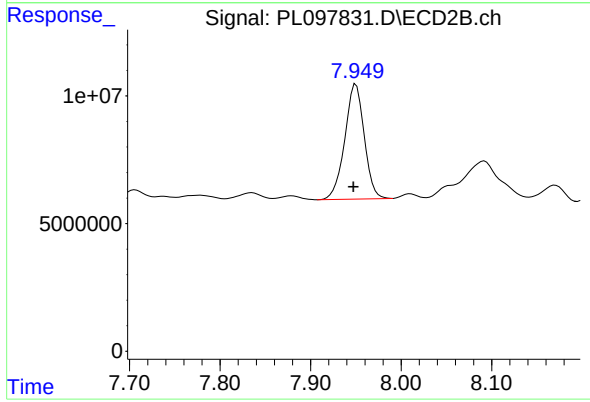

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.003 min
Response: 67180678
Conc: 10.22 ng/ml