

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
 Data File : PL042924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2018 09:49
 Operator : AJ\SJ
 Sample : J6269-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 10:15:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	55543490	27970370	9.057	9.437
28)	SA Decachlor...	8.202	9.228	76021572	29550044	11.642	11.328
Target Compounds							
2)	A alpha-BHC	0.000	4.456f	0	1379640	N.D.	0.305 #
6)	B beta-BHC	4.398f	0.000	8334743	0	2.260	N.D. #
7)	B delta-BHC	0.000	5.155	0	30783128	N.D.	7.163 #
8)	B Heptachlo...	0.000	5.989	0	37764540	N.D.	9.959 #
9)	A Endosulfan I	0.000	6.343	0	4202991	N.D.	1.238 #
10)	B gamma-Chl...	0.000	6.237	0	8040819	N.D.	2.189 #
11)	B alpha-Chl...	0.000	6.298	0	4897263	N.D.	1.362 #
13)	MA Dieldrin	5.708f	0.000	3411923	0	0.439	N.D. #
14)	MA Endrin	6.018	0.000	15873095	0	2.204	N.D. #
17)	MA 4,4'-DDT	6.369	0.000	1101203	0	0.185	N.D. #
20)	A Methoxychlor	6.874f	0.000	1381933	0	0.412	N.D. #
23)	Chlordane-1	4.398	5.155	8334743	30783128	31.018	217.806 #
24)	Chlordane-2	4.891	5.545	18940909	261721	65.990	1.825 #
25)	Chlordane-3	0.000	6.237	0	8040819	N.D.	16.374 #
26)	Chlordane-4	0.000	6.298	0	4897263	N.D.	8.580 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
Data File : PL042924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2018 09:49
Operator : AJ\SJ
Sample : J6269-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 10:15:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

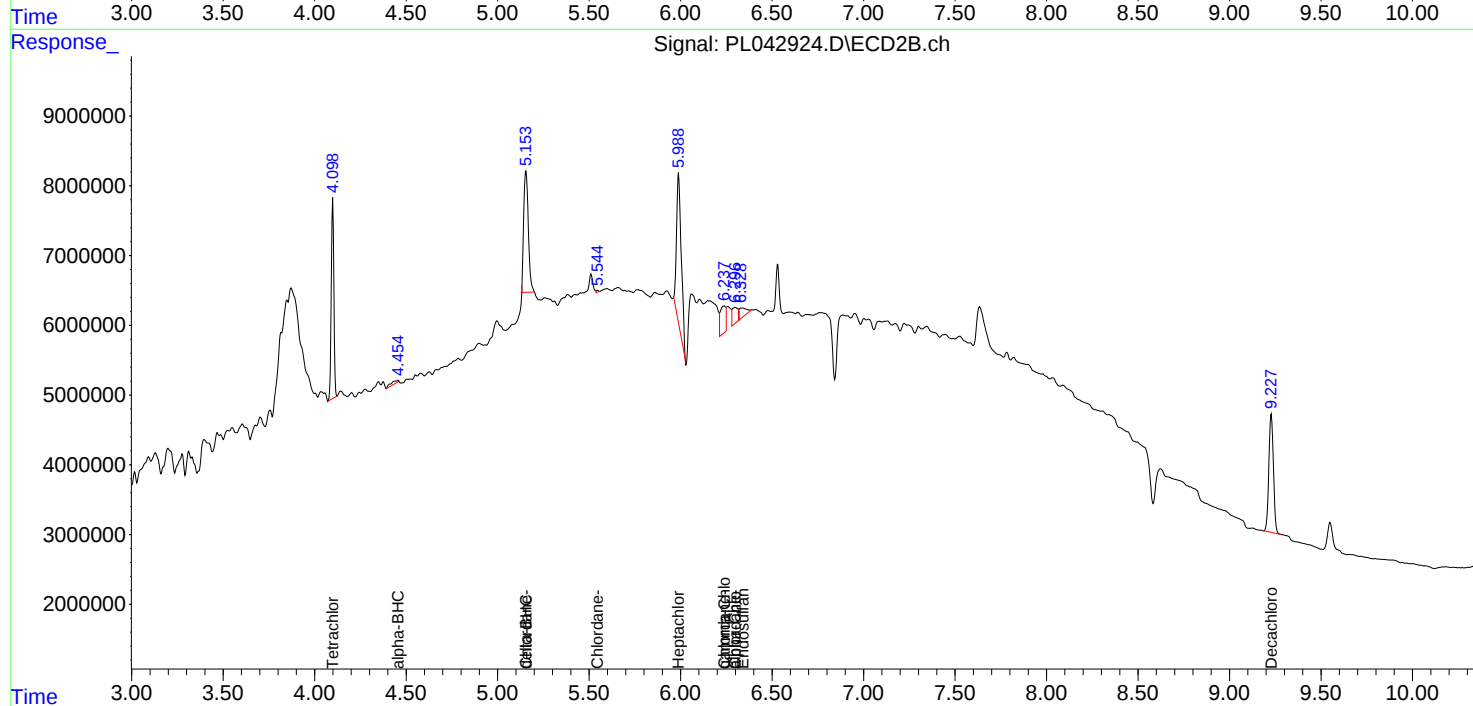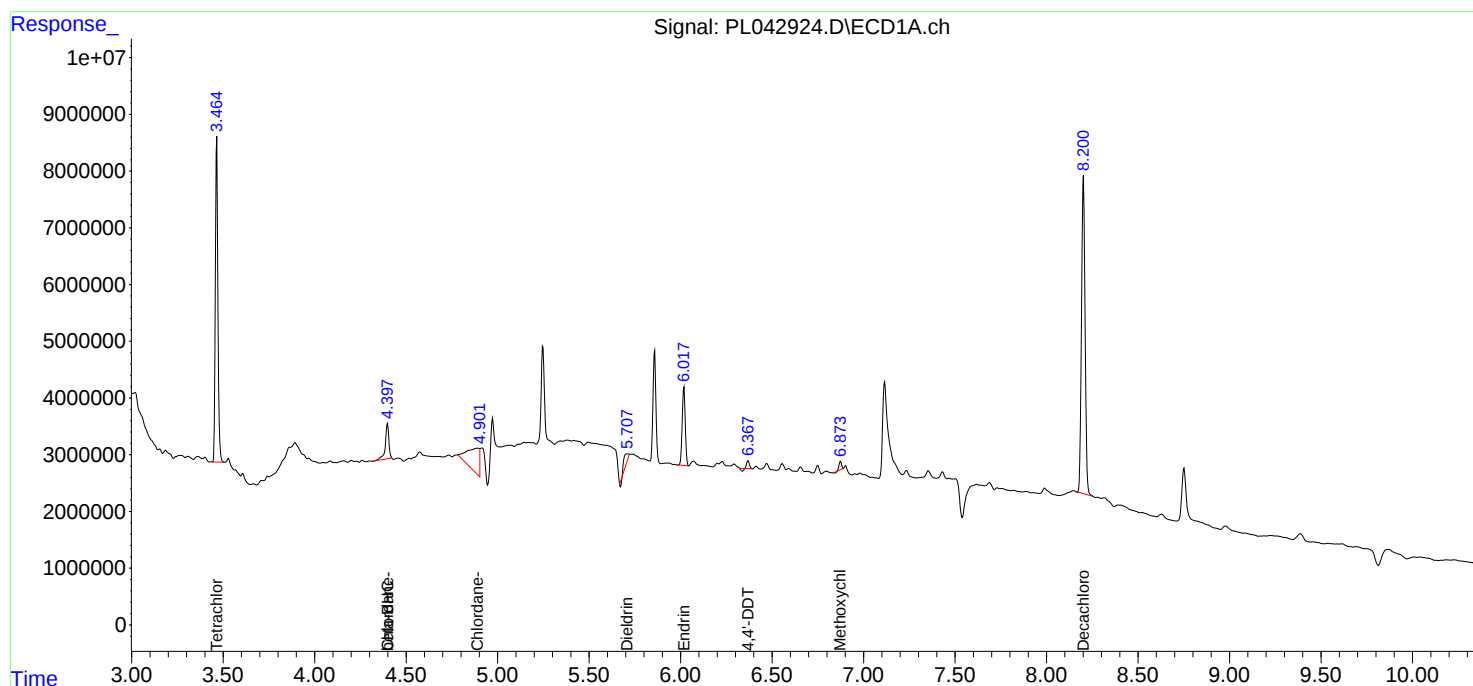


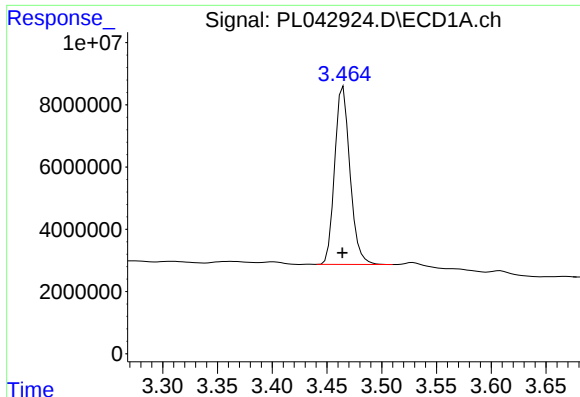

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 55543490
Conc: 9.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

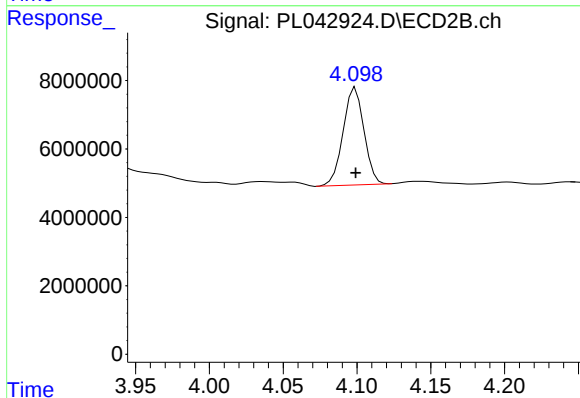


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 27970370
Conc: 9.44 ng/ml

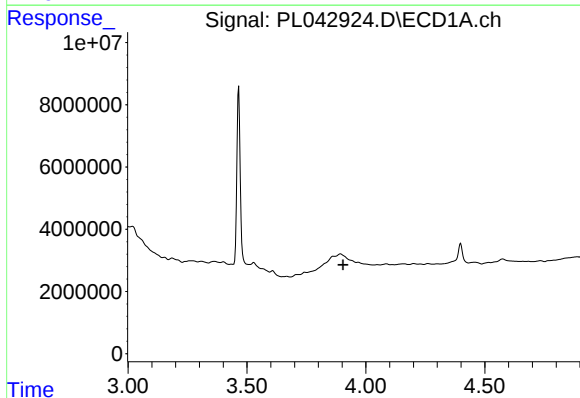


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.904 min
Response: 0
Conc: N.D.

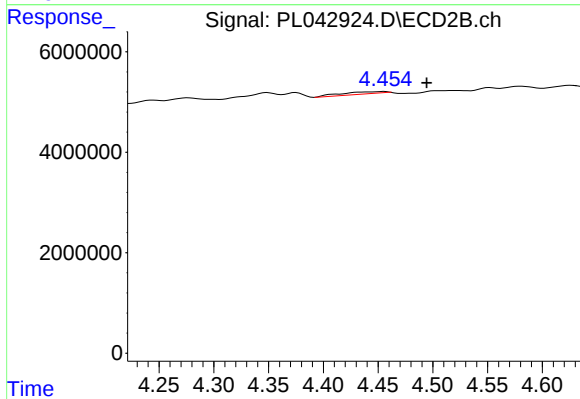

#2 alpha-BHC


R.T.: 4.456 min
Delta R.T.: -0.038 min
Response: 1379640
Conc: 0.30 ng/ml

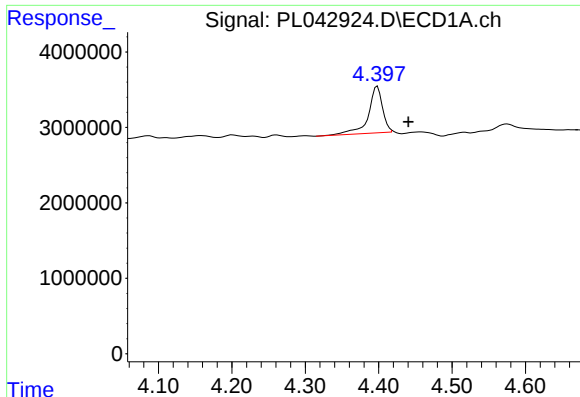

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.042 min
Response: 8334743
Conc: 2.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

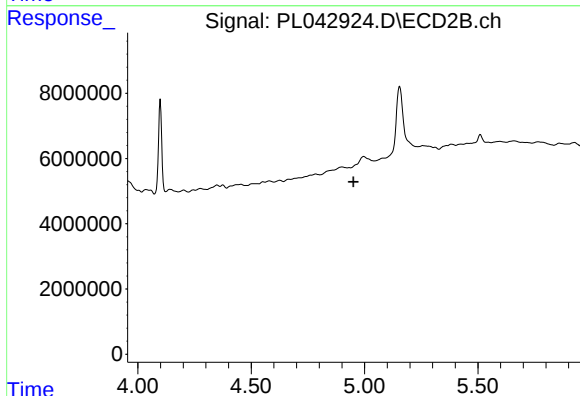


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

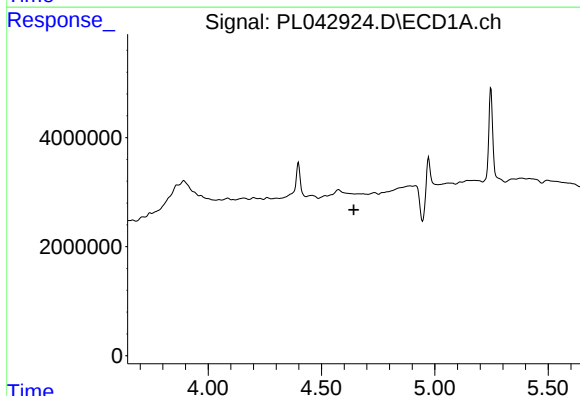


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

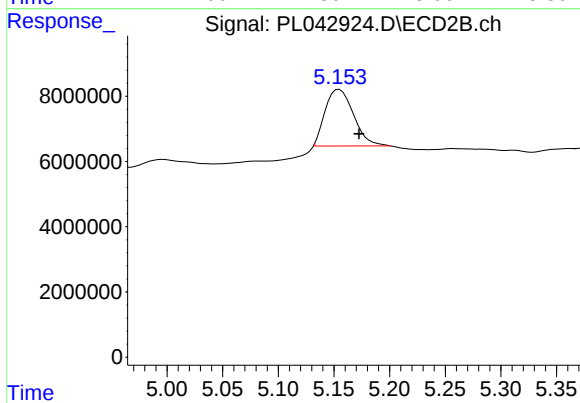

#7 delta-BHC


R.T.: 5.155 min
Delta R.T.: -0.018 min
Response: 30783128
Conc: 7.16 ng/ml

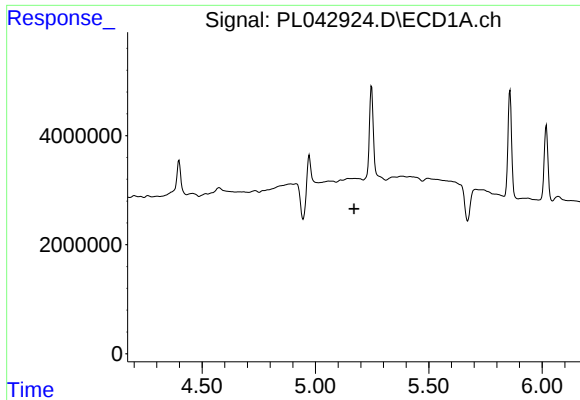

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

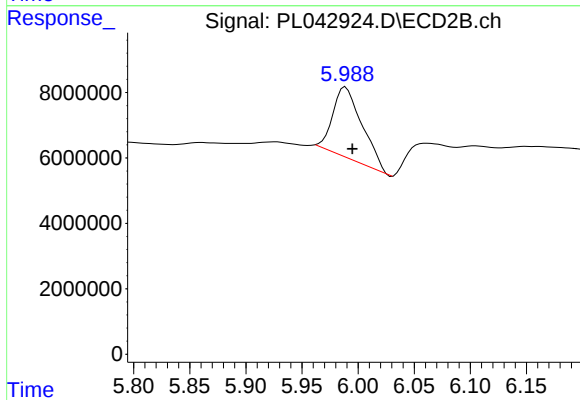


#8 Heptachlor epoxide

R.T.: 5.989 min
Delta R.T.: -0.006 min
Response: 37764540
Conc: 9.96 ng/ml

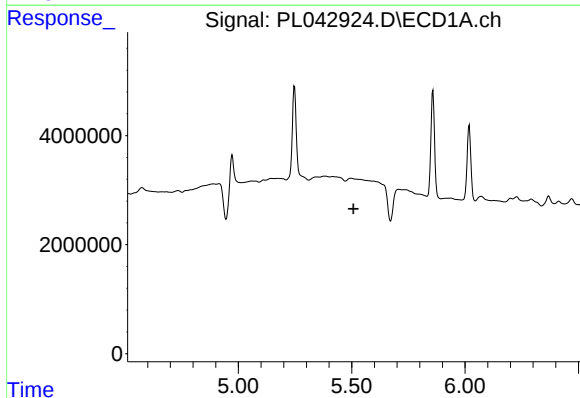


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

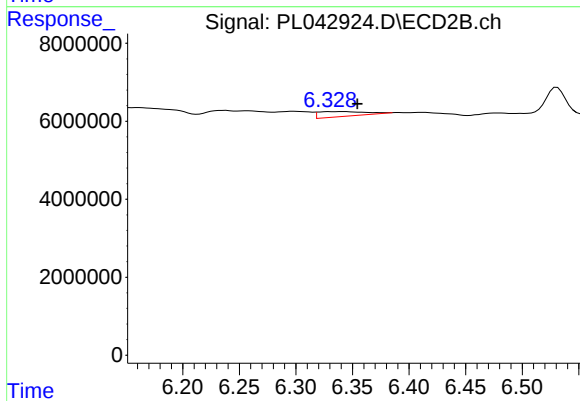

#9 Endosulfan I


R.T.: 6.343 min
Delta R.T.: -0.011 min
Response: 4202991
Conc: 1.24 ng/ml

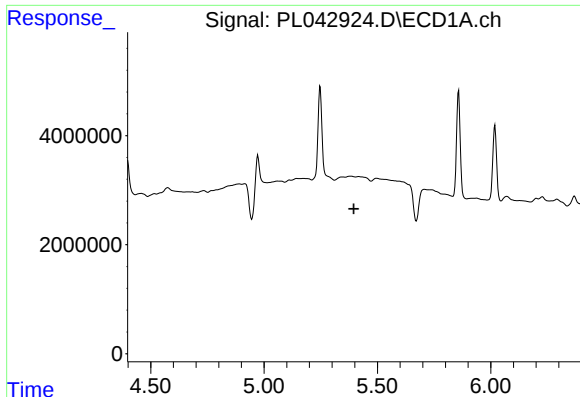

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

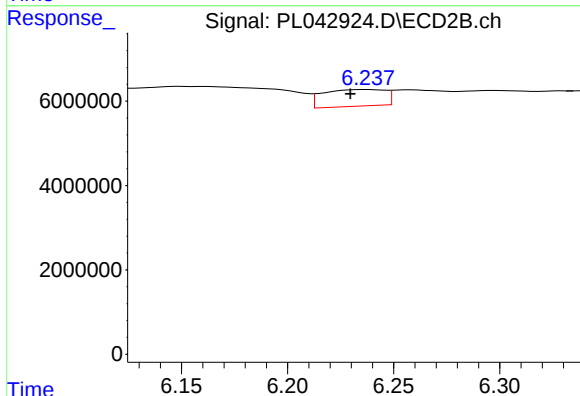


#10 gamma-Chlordane

R.T.: 6.237 min
Delta R.T.: 0.008 min
Response: 8040819
Conc: 2.19 ng/ml

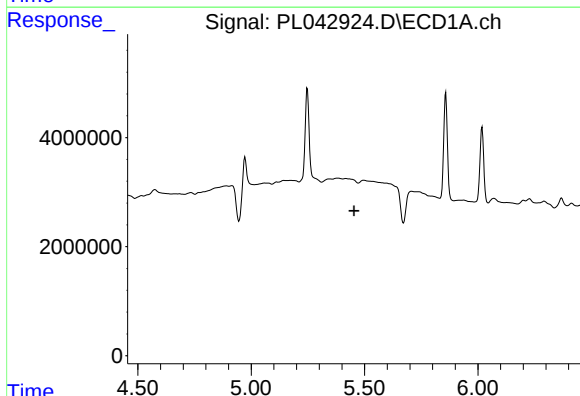


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

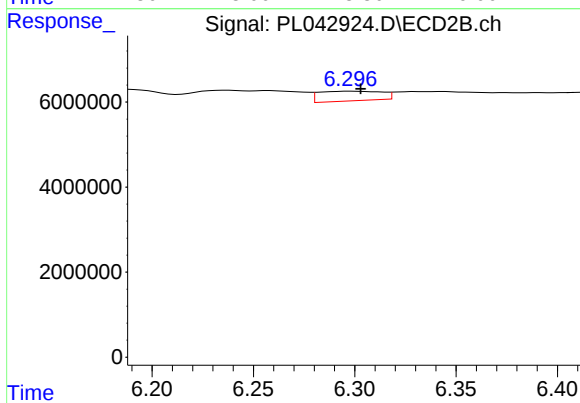

#11 alpha-Chlordane


R.T.: 6.298 min
Delta R.T.: -0.005 min
Response: 4897263
Conc: 1.36 ng/ml

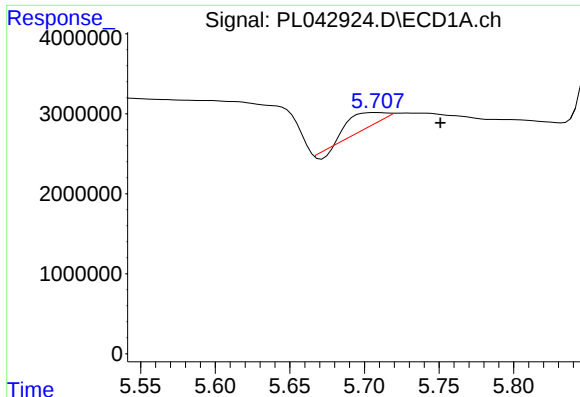

#13 Dieldrin


R.T.: 5.708 min
Delta R.T.: -0.043 min
Response: 3411923
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

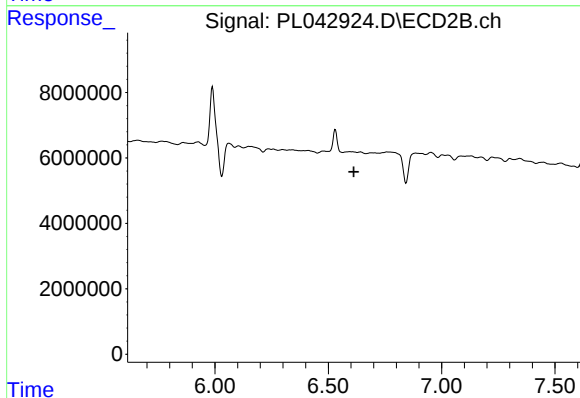


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

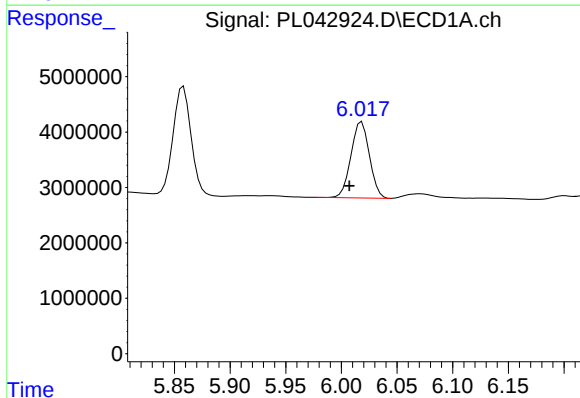


#14 Endrin

R.T.: 6.018 min
Delta R.T.: 0.011 min
Response: 15873095
Conc: 2.20 ng/ml

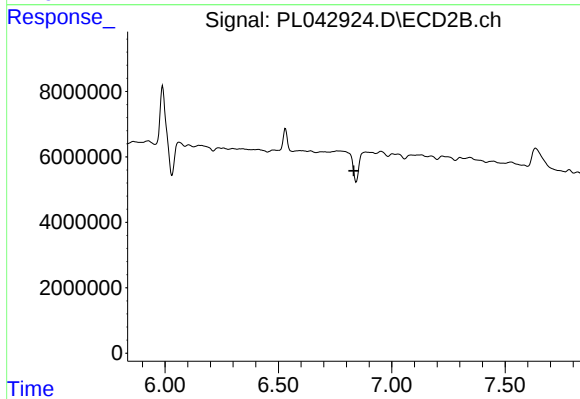

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

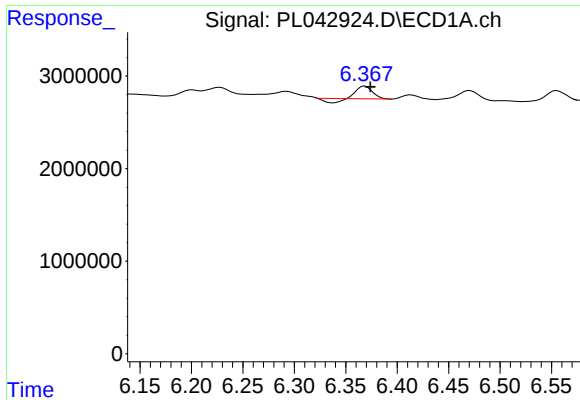

#17 4,4'-DDT


R.T.: 6.369 min
Delta R.T.: -0.005 min
Response: 1101203
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

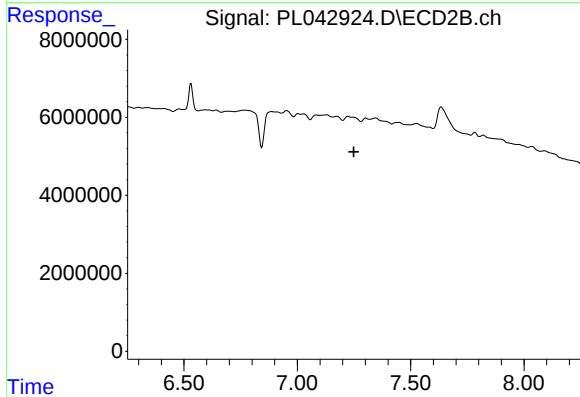


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

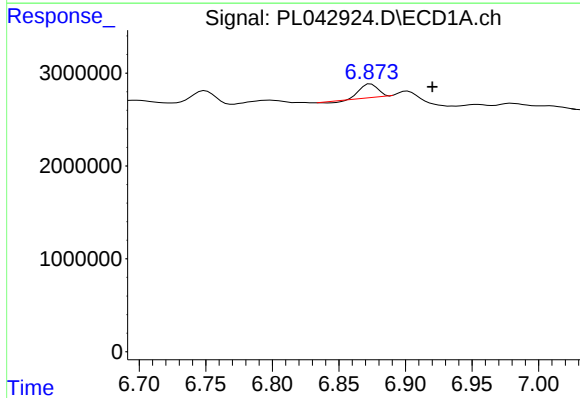


#20 Methoxychlor

R.T.: 6.874 min
Delta R.T.: -0.046 min
Response: 1381933
Conc: 0.41 ng/ml

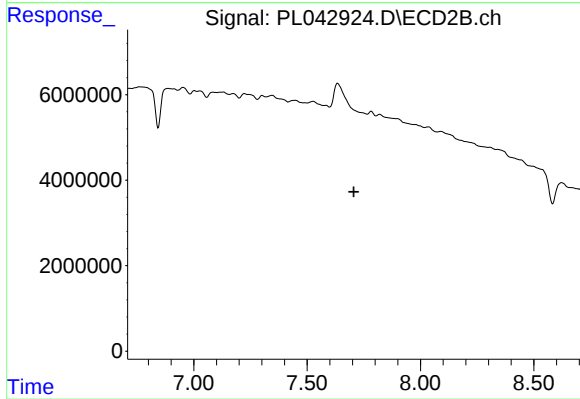

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.705 min
Response: 0
Conc: N.D.

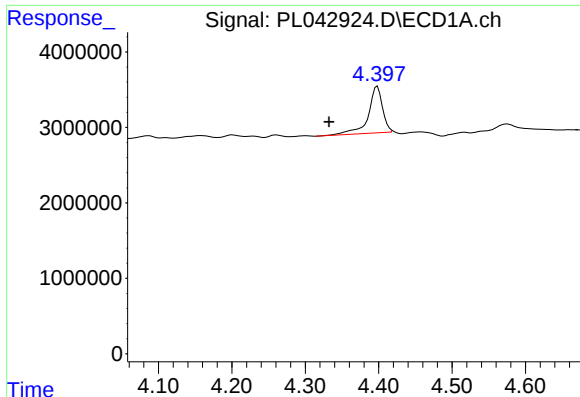

#23 Chlordane-1


R.T.: 4.398 min
Delta R.T.: 0.066 min
Response: 8334743
Conc: 31.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

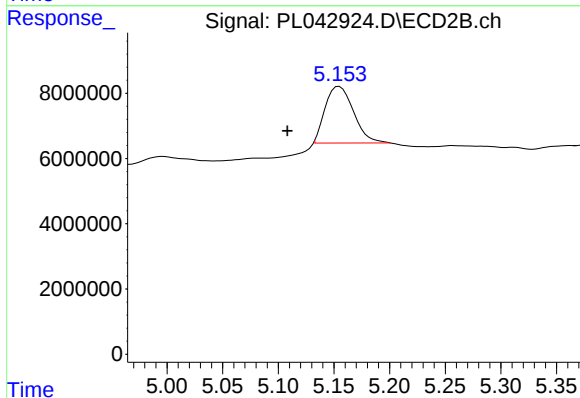


#23 Chlordane-1

R.T.: 5.155 min
Delta R.T.: 0.047 min
Response: 30783128
Conc: 217.81 ng/ml

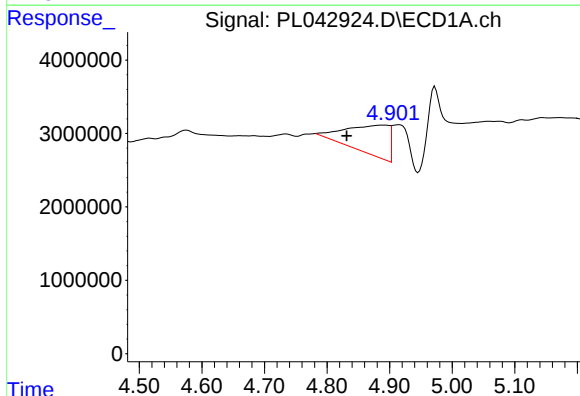


#24 Chlordane-2

R.T.: 4.891 min
Delta R.T.: 0.059 min
Response: 18940909
Conc: 65.99 ng/ml

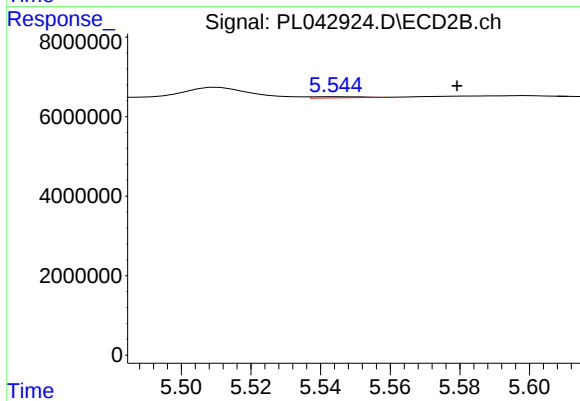

#24 Chlordane-2


R.T.: 5.545 min
Delta R.T.: -0.034 min
Response: 261721
Conc: 1.82 ng/ml

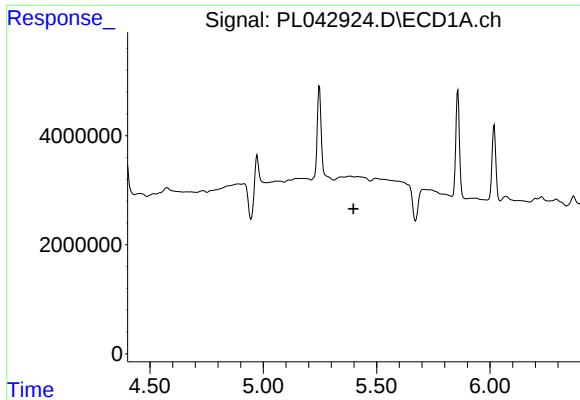

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

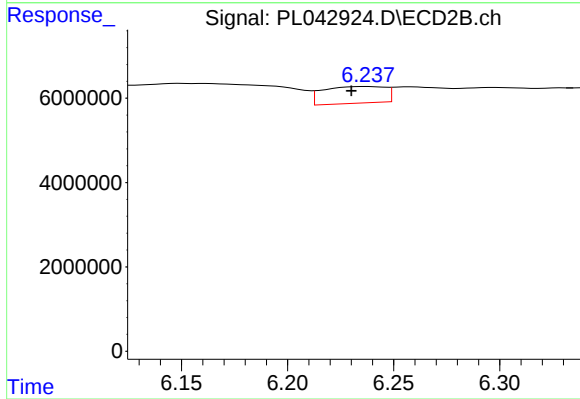


#25 Chlordane-3

R.T.: 6.237 min
Delta R.T.: 0.007 min
Response: 8040819
Conc: 16.37 ng/ml

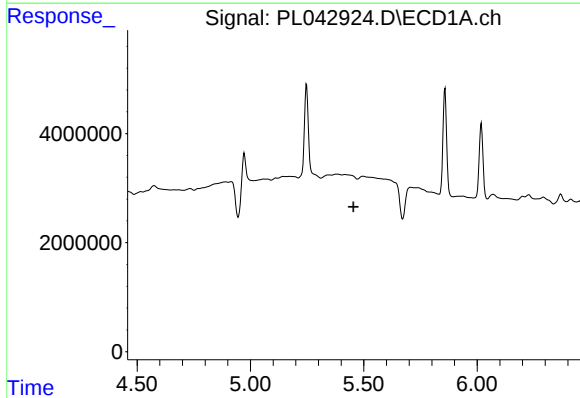


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

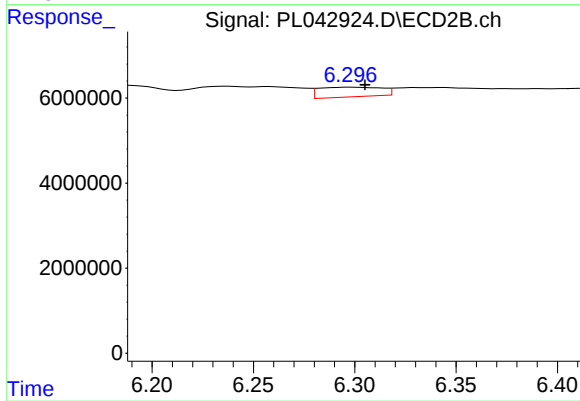

#26 Chlordane-4


R.T.: 6.298 min
Delta R.T.: -0.007 min
Response: 4897263
Conc: 8.58 ng/ml

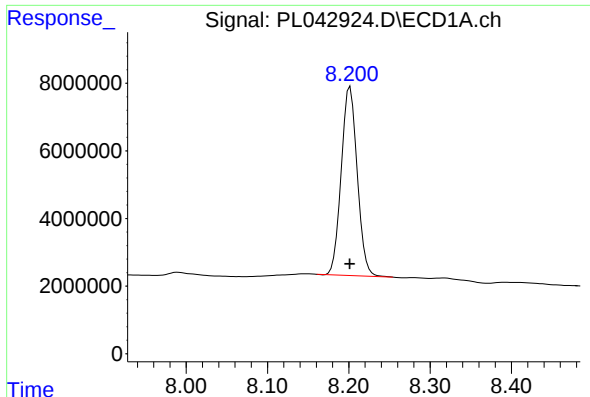

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 76021572
Conc: 11.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

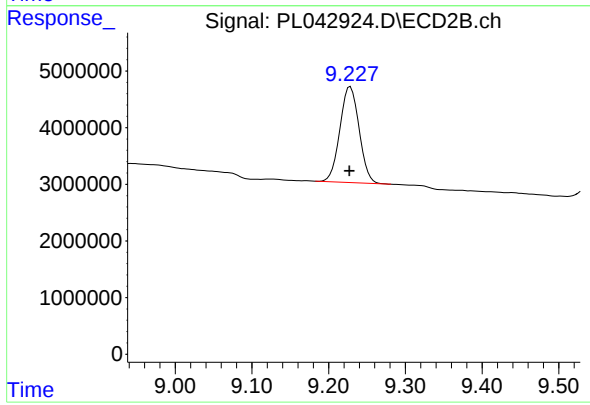

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.001 min
Response: 29550044
Conc: 11.33 ng/ml