

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
 Data File : PL042931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2018 11:27
 Operator : AJ\SJ
 Sample : J6337-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 11:51:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	77386581	39075253	12.618	13.184
28)	SA Decachlor...	8.201	9.228	40349959	15715612	6.179	6.025
Target Compounds							
6)	B beta-BHC	4.397f	0.000	4678634	0	1.268	N.D. #
7)	B delta-BHC	0.000	5.159	0	25055528	N.D.	5.830 #
8)	B Heptachlo...	0.000	5.991	0	15963149	N.D.	4.210 #
9)	A Endosulfan I	0.000	6.350	0	1036592	N.D.	0.305 #
10)	B gamma-Chl...	0.000	6.250	0	5539692	N.D.	1.508 #
11)	B alpha-Chl...	0.000	6.306	0	3503200	N.D.	0.974 #
12)	B 4,4'-DDE	5.620	6.458	3905065	5172093	0.564	1.427 #
13)	MA Dieldrin	5.820f	0.000	2545215	0	0.327	N.D. #
14)	MA Endrin	0.000	6.855	0	218008	N.D.	0.070 #
17)	MA 4,4'-DDT	6.373	0.000	1897826	0	0.319	N.D. #
23)	Chlordane-1	4.362	5.159	2349009	25055528	8.742	177.280 #
25)	Chlordane-3	0.000	6.250	0	5539692	N.D.	11.281 #
26)	Chlordane-4	0.000	6.306	0	3503200	N.D.	6.138 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
Data File : PL042931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2018 11:27
Operator : AJ\SJ
Sample : J6337-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 11:51:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

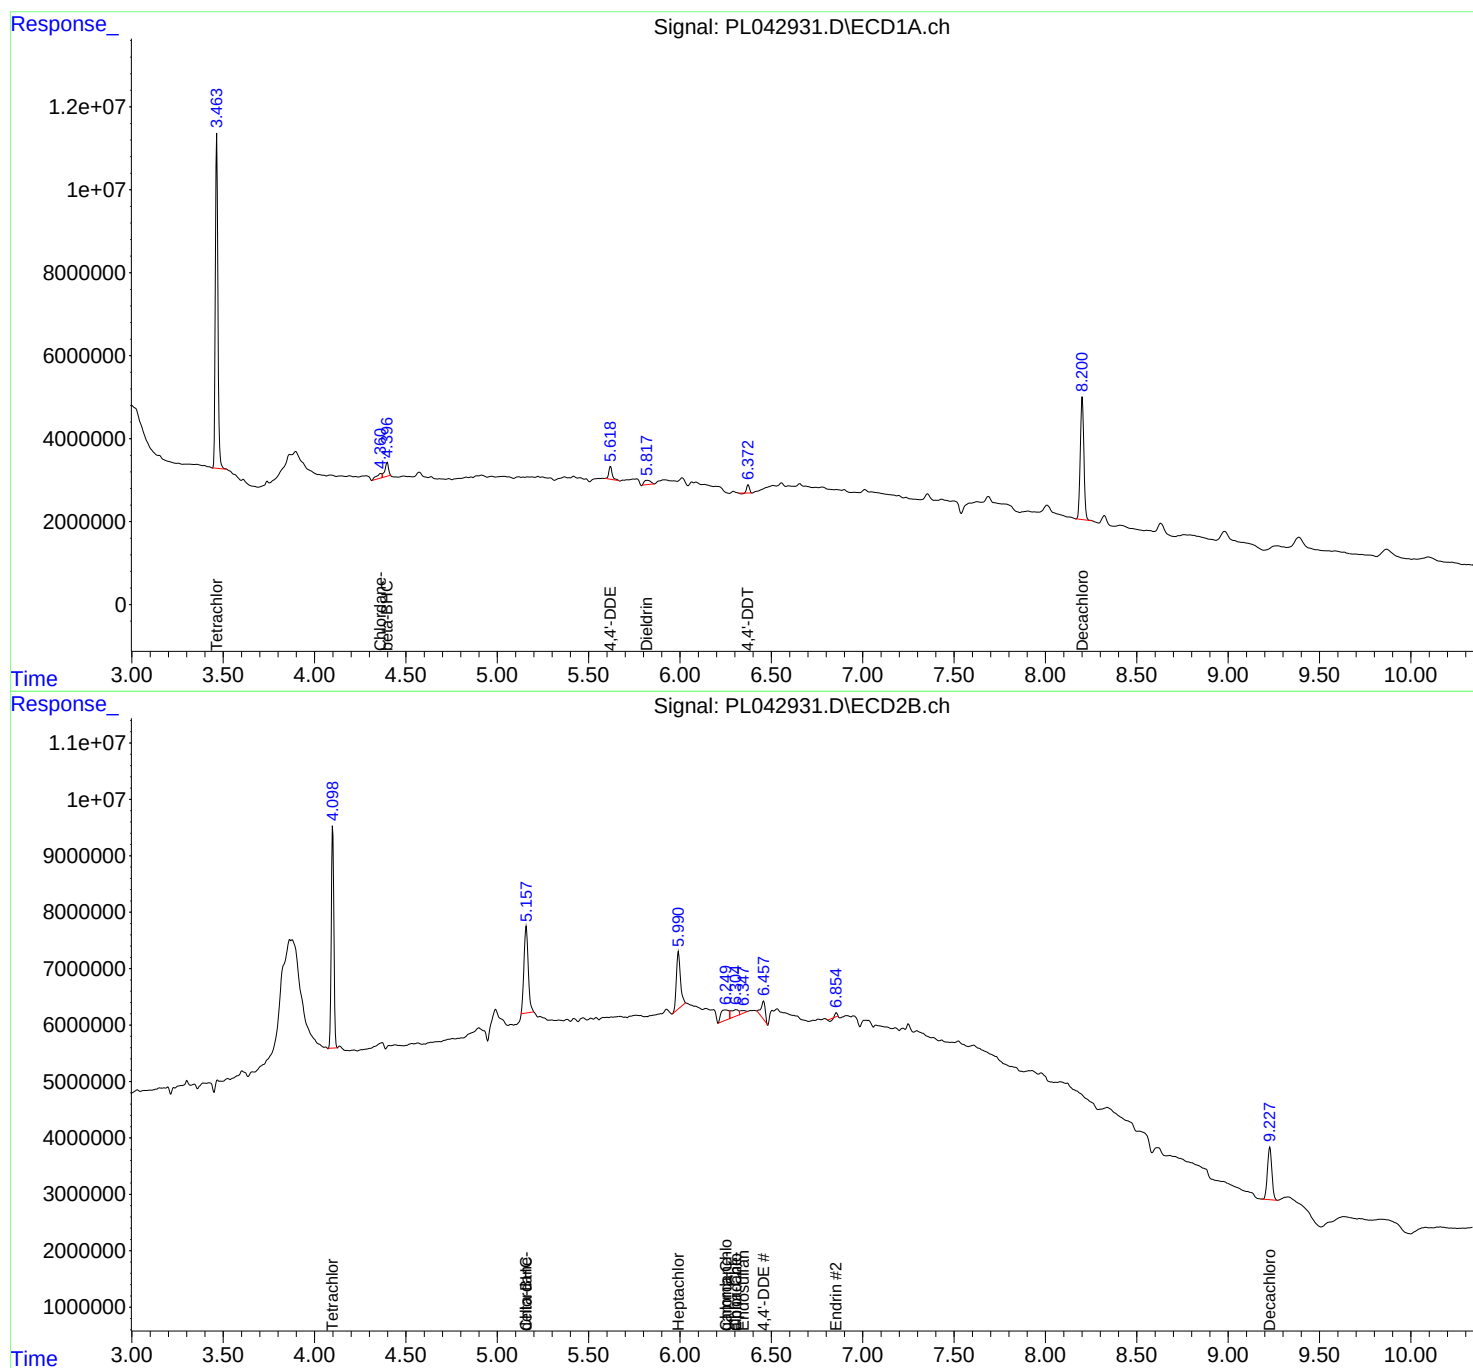


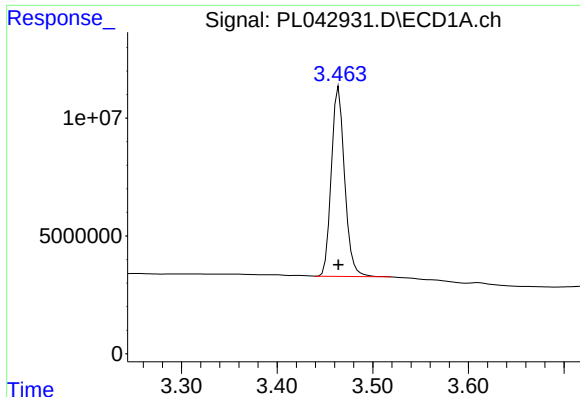

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 77386581
Conc: 12.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

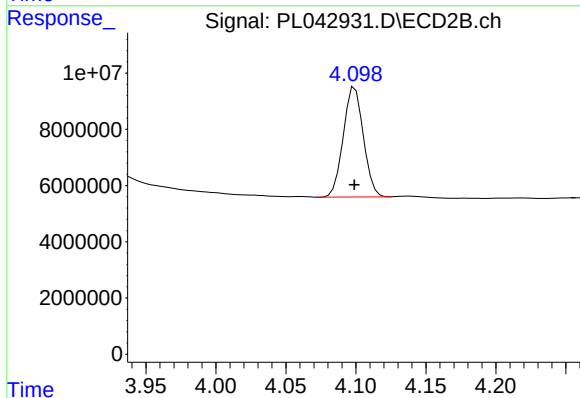


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 39075253
Conc: 13.18 ng/ml

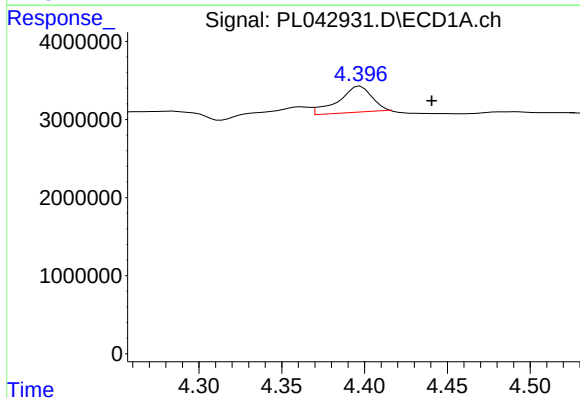


#6 beta-BHC

R.T.: 4.397 min
Delta R.T.: -0.043 min
Response: 4678634
Conc: 1.27 ng/ml

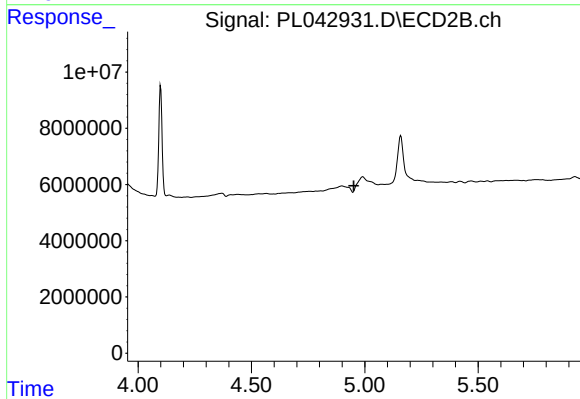

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

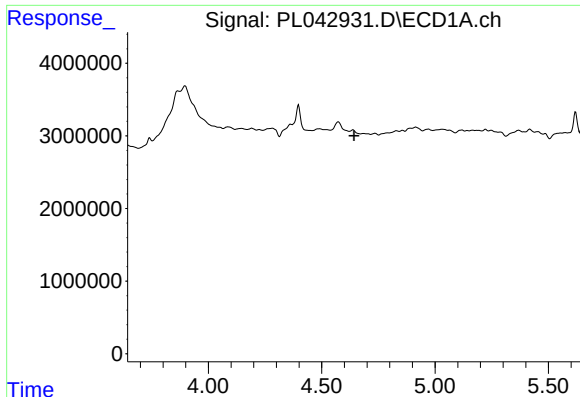

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

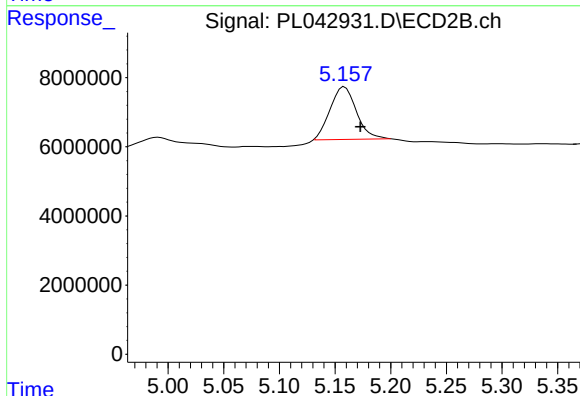


#7 delta-BHC

R.T.: 5.159 min
Delta R.T.: -0.014 min
Response: 2505528
Conc: 5.83 ng/ml

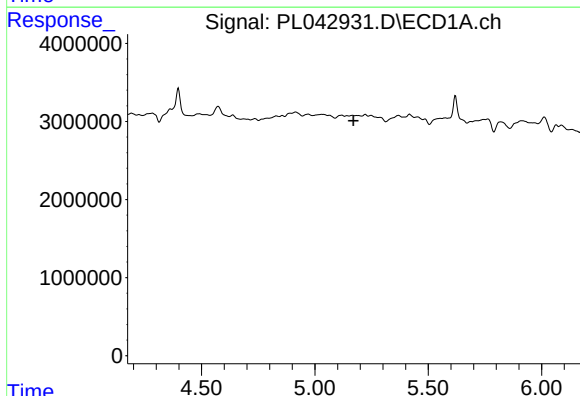


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

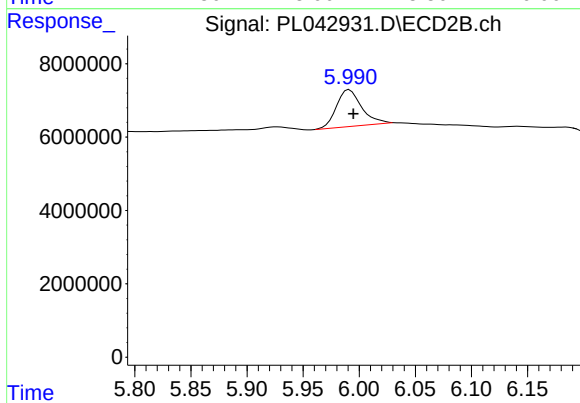

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 15963149
Conc: 4.21 ng/ml

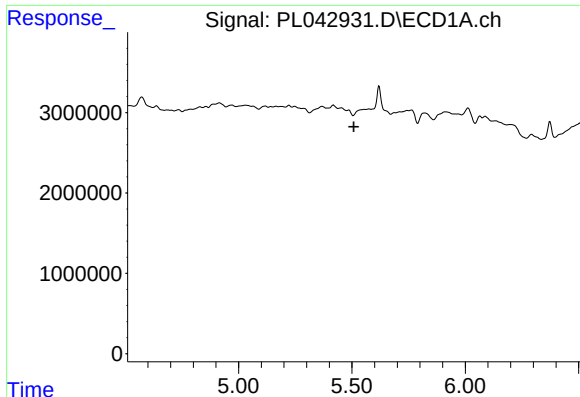

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

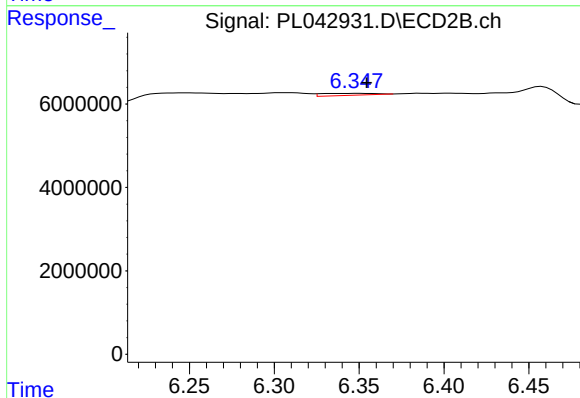


#9 Endosulfan I

R.T.: 6.350 min
Delta R.T.: -0.005 min
Response: 1036592
Conc: 0.31 ng/ml

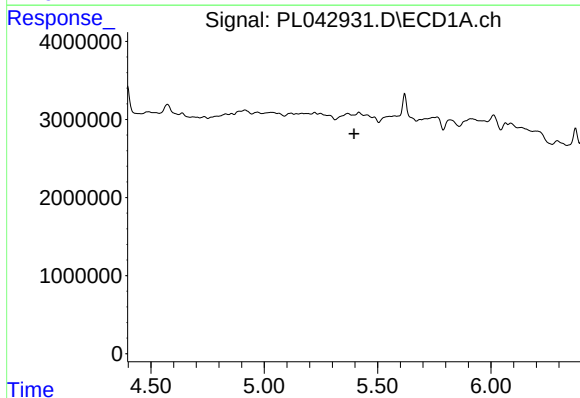


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

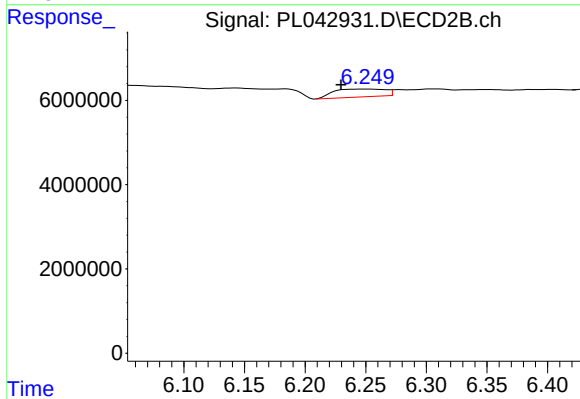

#10 gamma-Chlordane


R.T.: 6.250 min
Delta R.T.: 0.020 min
Response: 5539692
Conc: 1.51 ng/ml

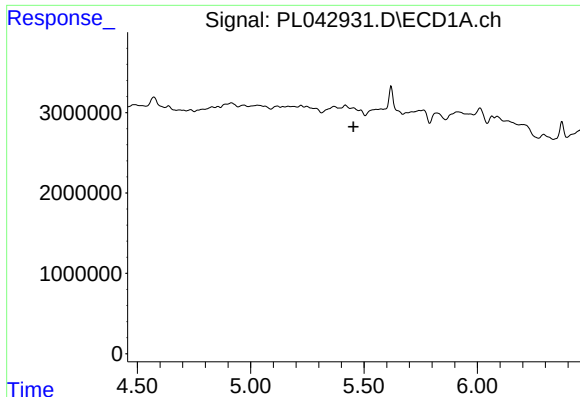

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

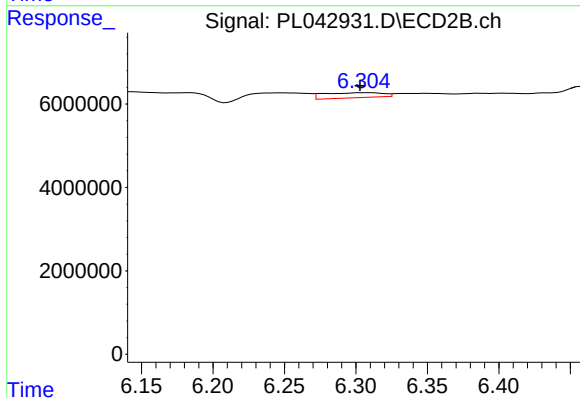


#11 alpha-Chlordane

R.T.: 6.306 min
Delta R.T.: 0.003 min
Response: 3503200
Conc: 0.97 ng/ml

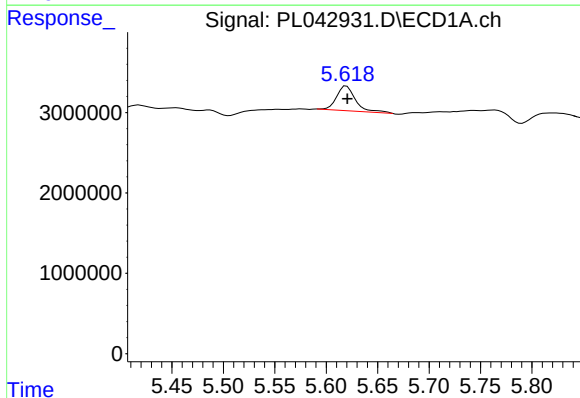


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 3905065
Conc: 0.56 ng/ml

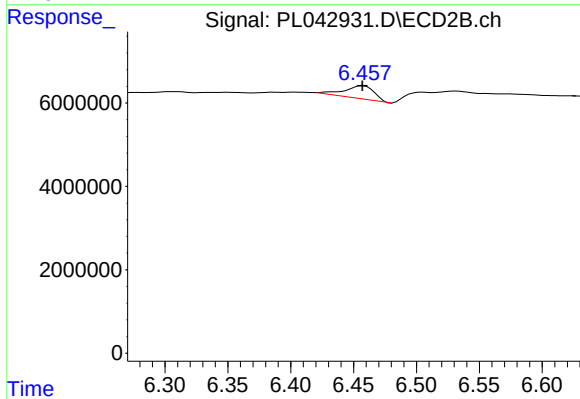

#12 4,4'-DDE


R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 5172093
Conc: 1.43 ng/ml

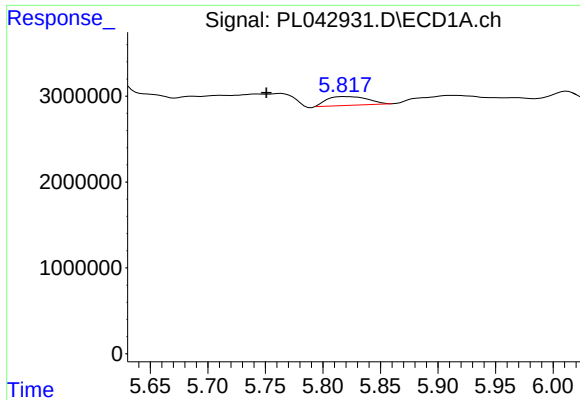

#13 Dieldrin


R.T.: 5.820 min
Delta R.T.: 0.069 min
Response: 2545215
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

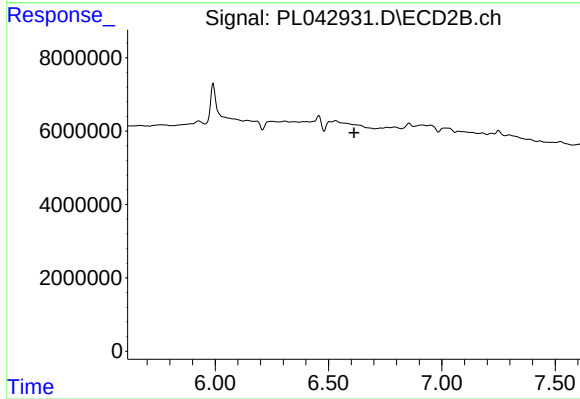


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

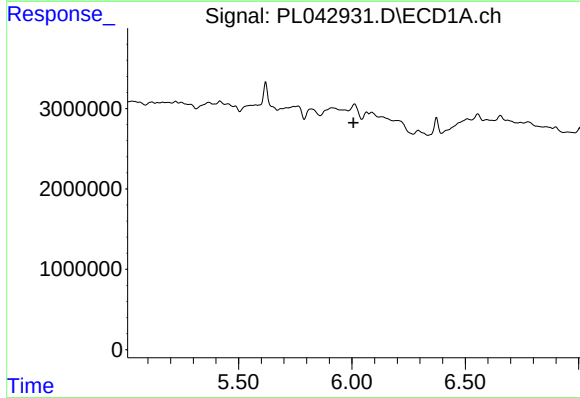


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.007 min
Response: 0
Conc: N.D.

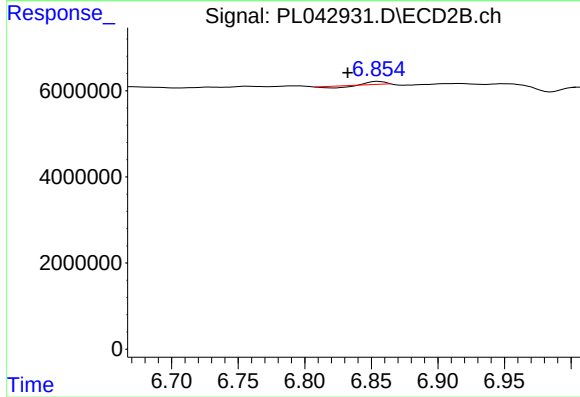

#14 Endrin


R.T.: 6.855 min
Delta R.T.: 0.023 min
Response: 218008
Conc: 0.07 ng/ml

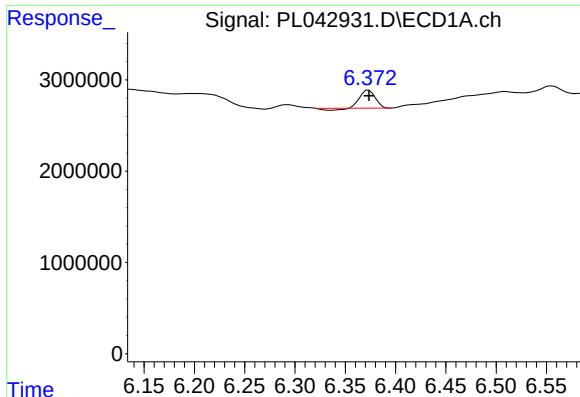

#17 4,4'-DDT


R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 1897826
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

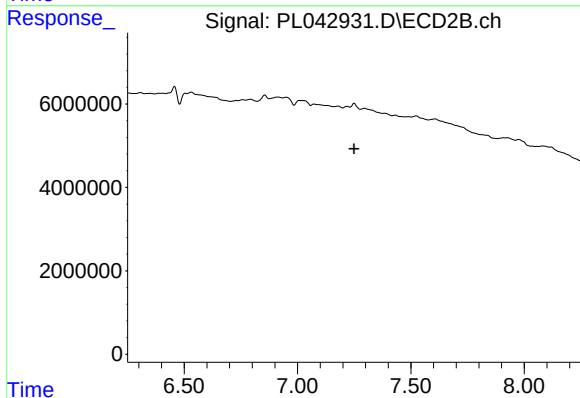


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

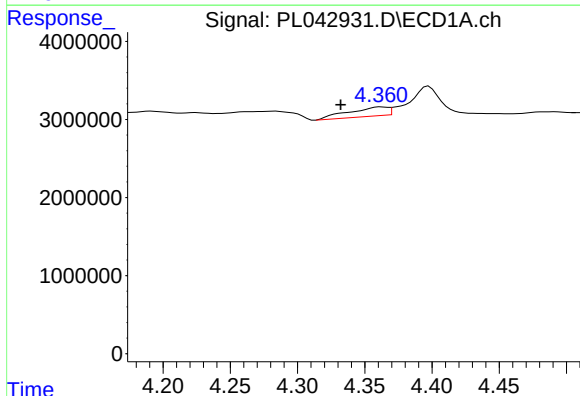


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 2349009
Conc: 8.74 ng/ml

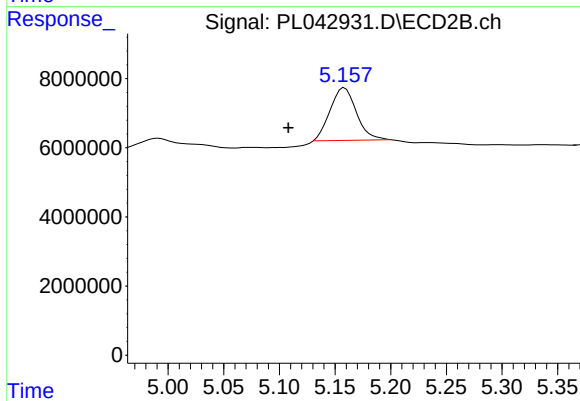

#23 Chlordane-1


R.T.: 5.159 min
Delta R.T.: 0.050 min
Response: 25055528
Conc: 177.28 ng/ml

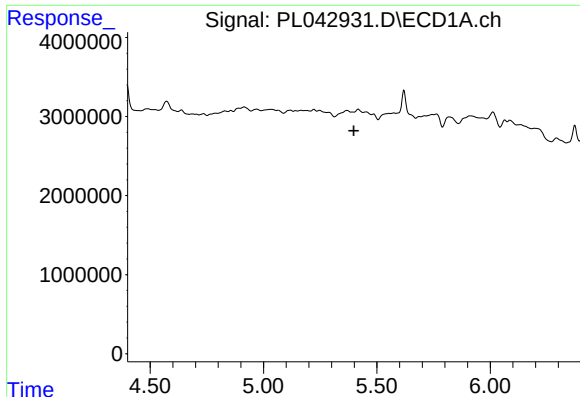

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

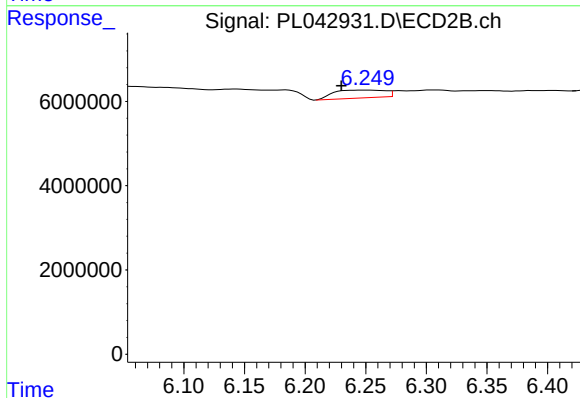


#25 Chlordane-3

R.T.: 6.250 min
Delta R.T.: 0.020 min
Response: 5539692
Conc: 11.28 ng/ml

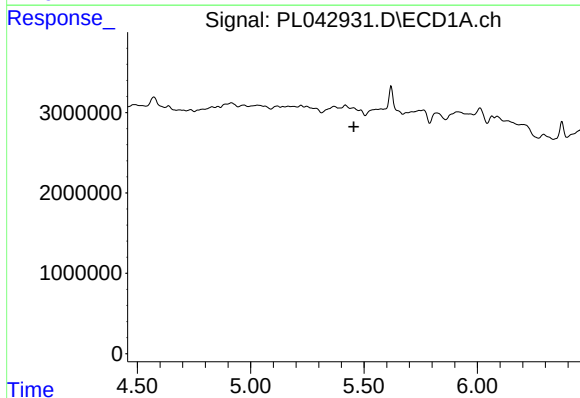


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

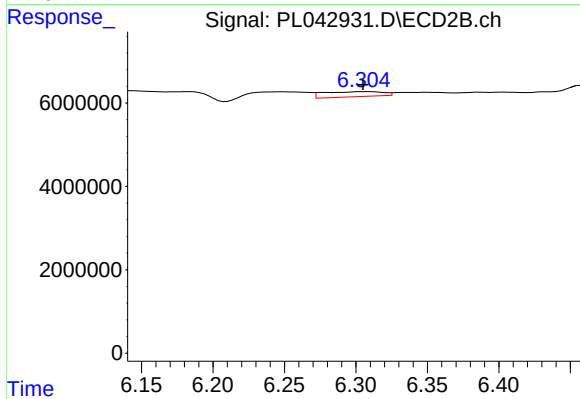

#26 Chlordane-4


R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 3503200
Conc: 6.14 ng/ml

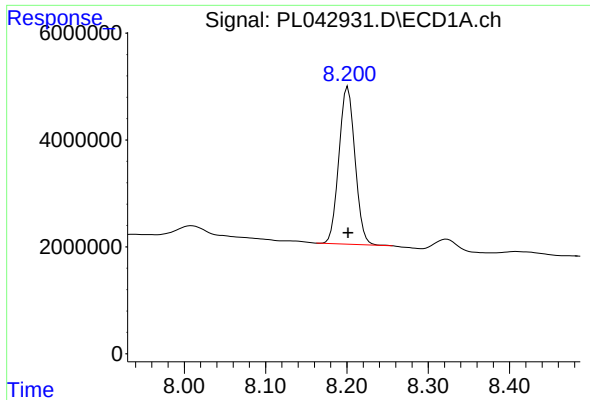

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 40349959
Conc: 6.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

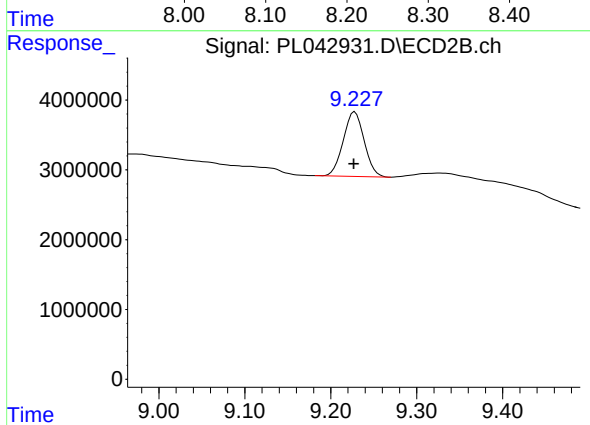

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.001 min
Response: 15715612
Conc: 6.02 ng/ml