

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
 Data File : PL042954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2018 17:34
 Operator : AJ\SJ
 Sample : PB115476BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:32:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	115.1E6	57352804	18.771	19.350
28)	SA Decachlor...	8.203	9.231	122.1E6	50608562	18.704	19.401
Target Compounds							
2)	A alpha-BHC	0.000	4.446f	0	463690	N.D.	0.103 #
6)	B beta-BHC	4.398f	0.000	7092120	0	1.923	N.D. #
7)	B delta-BHC	0.000	5.156	0	40090977	N.D.	9.329 #
8)	B Heptachlo...	0.000	5.990	0	28681739	N.D.	7.564 #
10)	B gamma-Chl...	0.000	6.251	0	2158905	N.D.	0.588 #
11)	B alpha-Chl...	0.000	6.251f	0	2158905	N.D.	0.600 #
13)	MA Dieldrin	5.701f	0.000	1592868	0	0.205	N.D. #
14)	MA Endrin	6.018	0.000	3173691	0	0.441	N.D. #
20)	A Methoxychlor	0.000	7.638f	0	7945436	N.D.	5.268 #
23)	Chlordane-1	4.363	5.156	1273571	40090977	4.740	283.663 #
25)	Chlordane-3	0.000	6.251	0	2158905	N.D.	4.396 #
26)	Chlordane-4	0.000	6.251	0	2158905	N.D.	3.783 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
Data File : PL042954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2018 17:34
Operator : AJ\SJ
Sample : PB115476BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:32:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

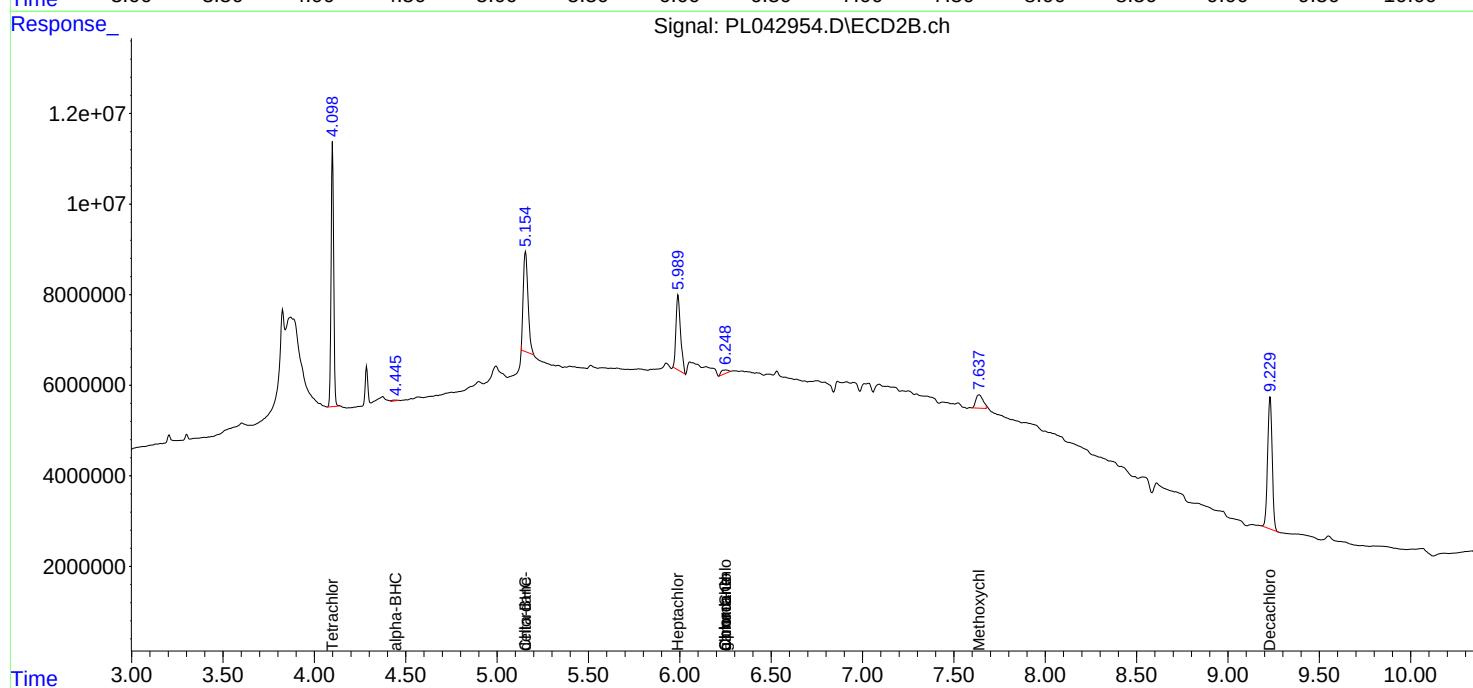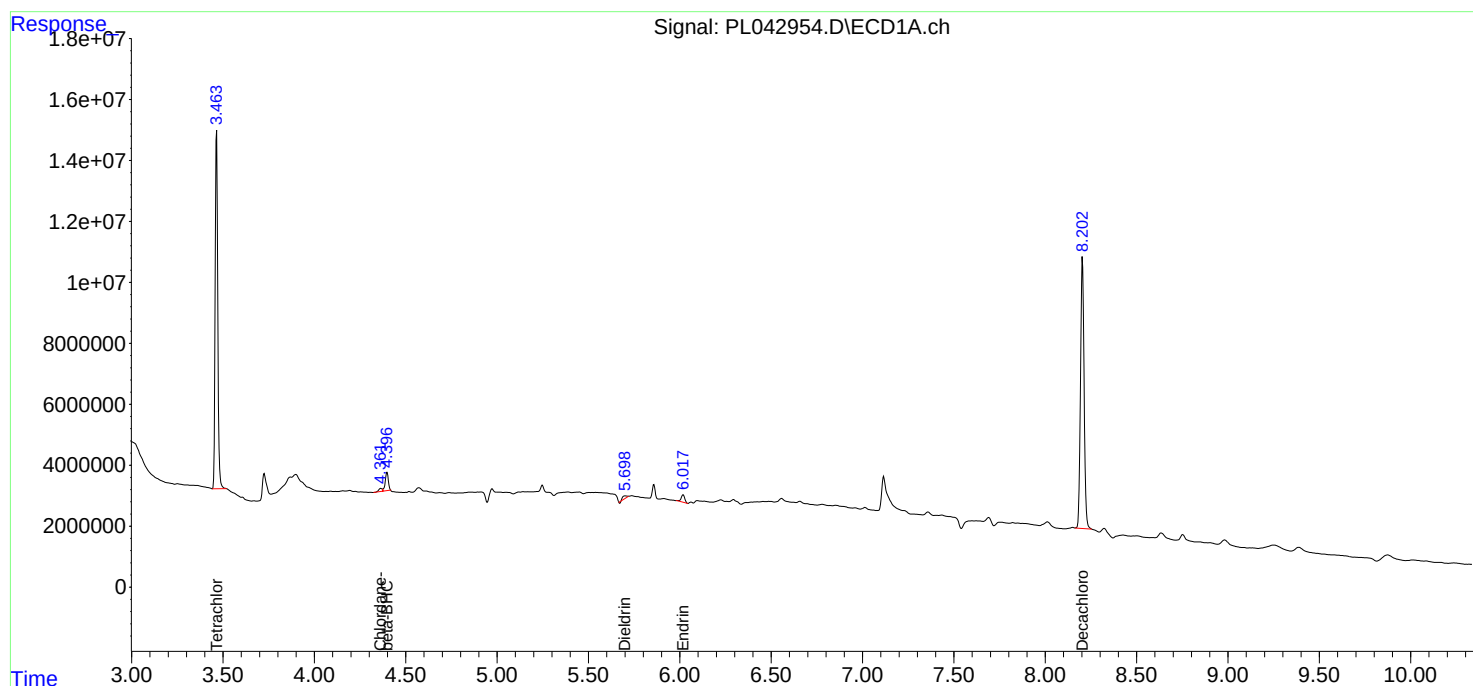


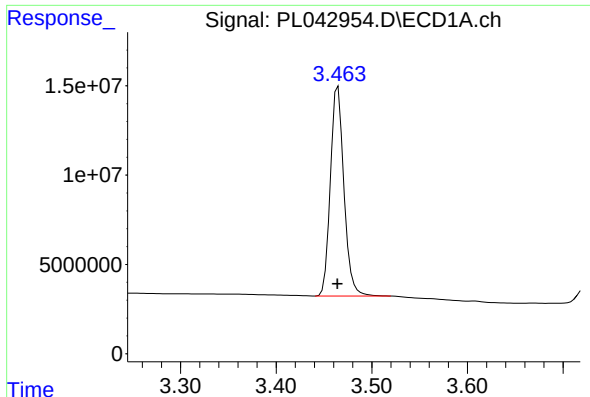

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 115122671
Conc: 18.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

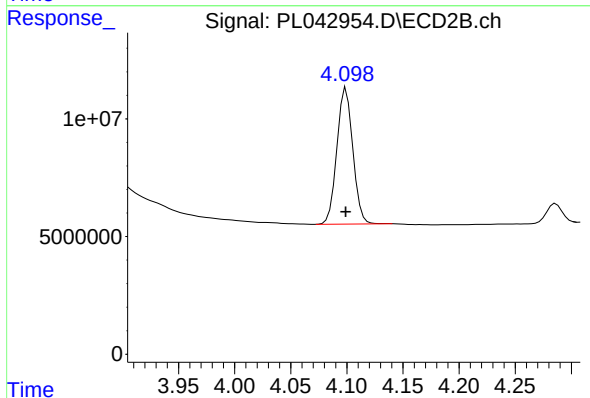


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 57352804
Conc: 19.35 ng/ml

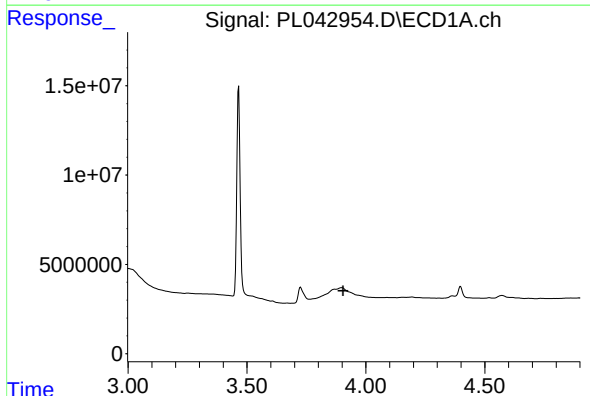


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.904 min
Response: 0
Conc: N.D.

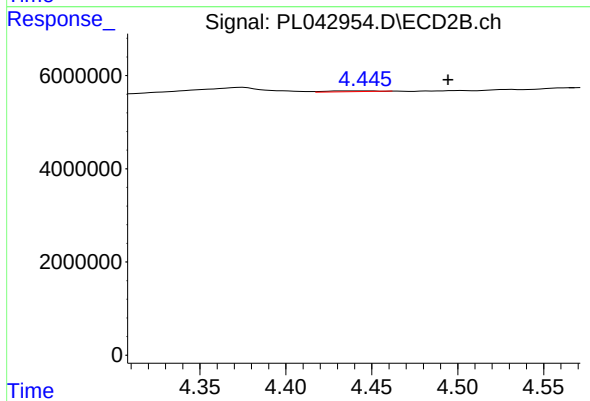

#2 alpha-BHC


R.T.: 4.446 min
Delta R.T.: -0.048 min
Response: 463690
Conc: 0.10 ng/ml

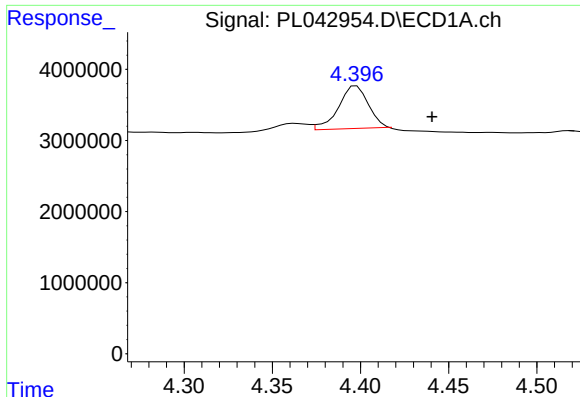

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 7092120
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

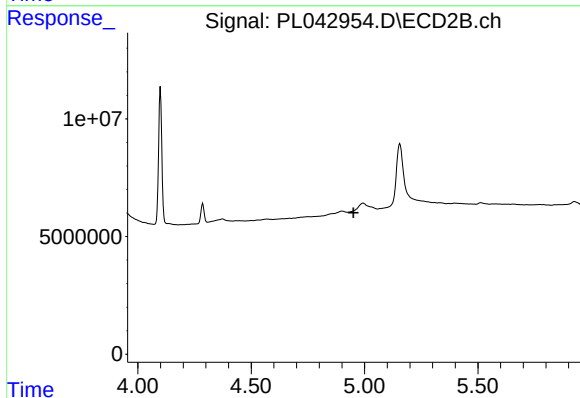


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

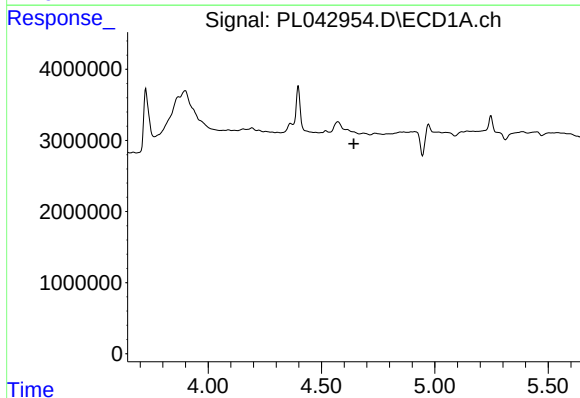


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

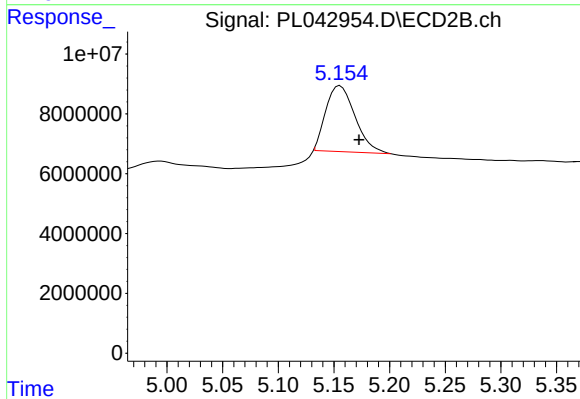

#7 delta-BHC


R.T.: 5.156 min
Delta R.T.: -0.017 min
Response: 40090977
Conc: 9.33 ng/ml

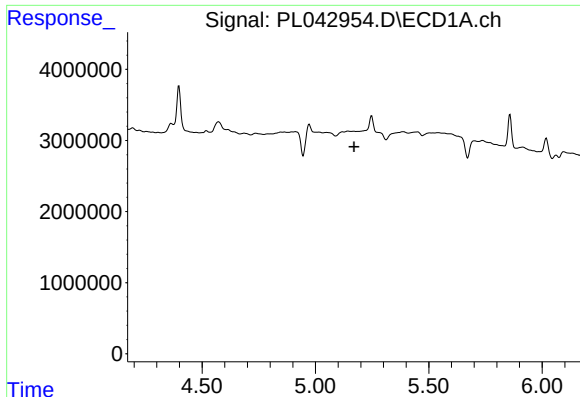

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

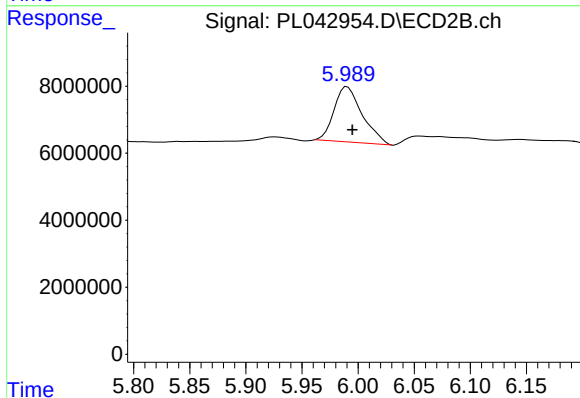


#8 Heptachlor epoxide

R.T.: 5.990 min
Delta R.T.: -0.004 min
Response: 28681739
Conc: 7.56 ng/ml

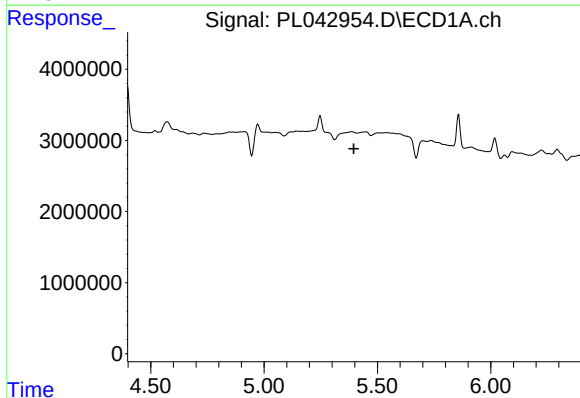


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

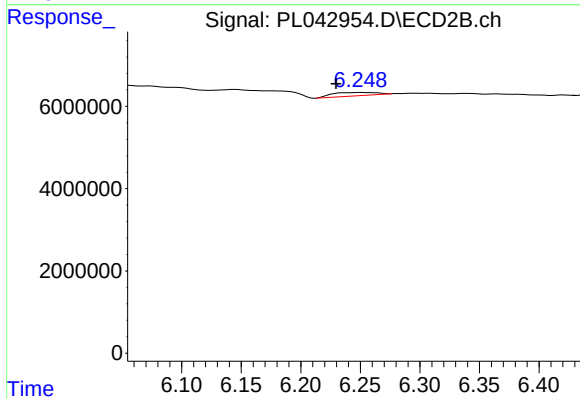

#10 gamma-Chlordane


R.T.: 6.251 min
Delta R.T.: 0.021 min
Response: 2158905
Conc: 0.59 ng/ml

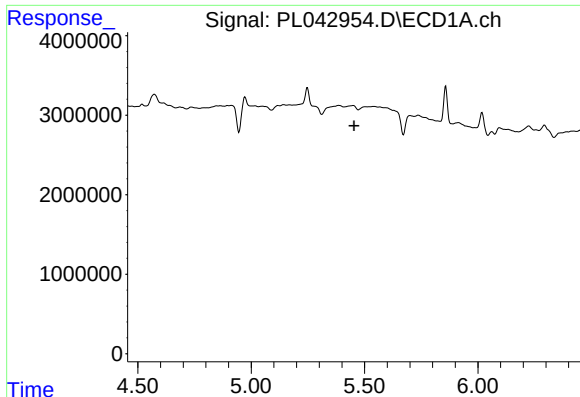

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

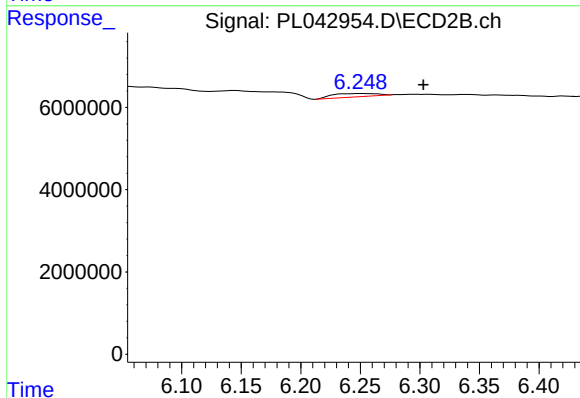


#11 alpha-Chlordane

R.T.: 6.251 min
Delta R.T.: -0.052 min
Response: 2158905
Conc: 0.60 ng/ml

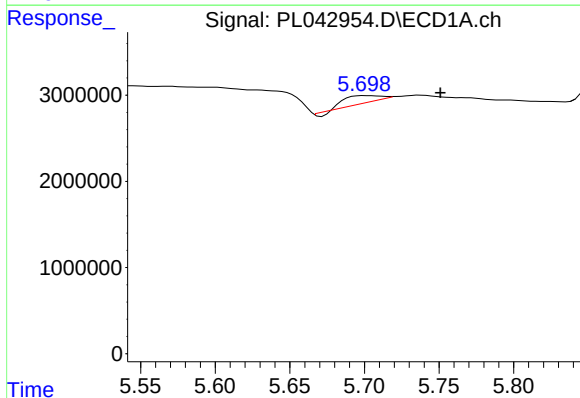


#13 Dieldrin

R.T.: 5.701 min
Delta R.T.: -0.050 min
Response: 1592868
Conc: 0.20 ng/ml

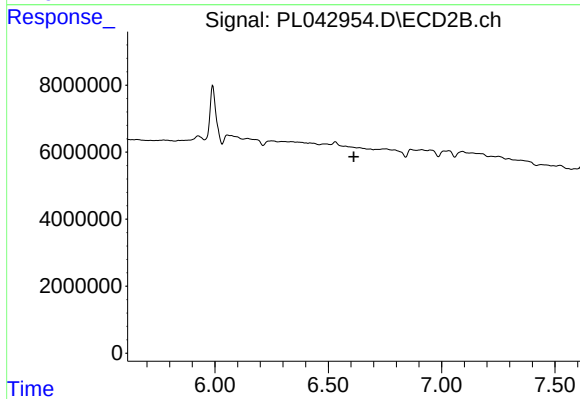

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

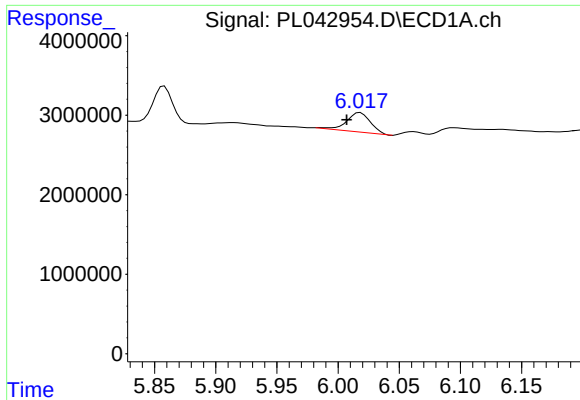

#14 Endrin


R.T.: 6.018 min
Delta R.T.: 0.011 min
Response: 3173691
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

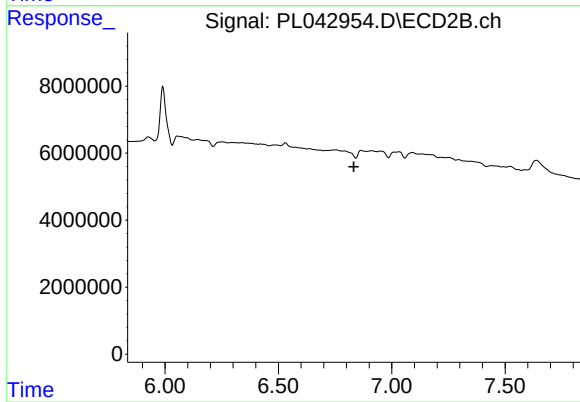


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

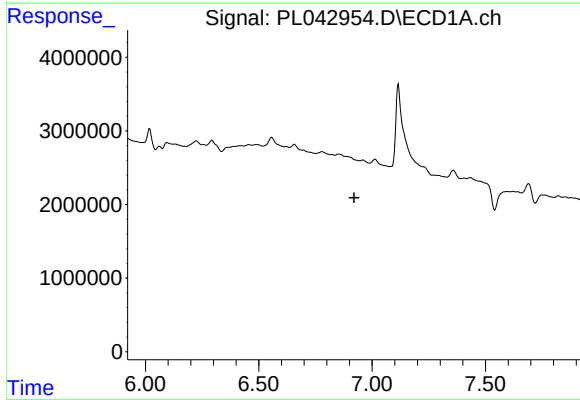


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.920 min
Response: 0
Conc: N.D.

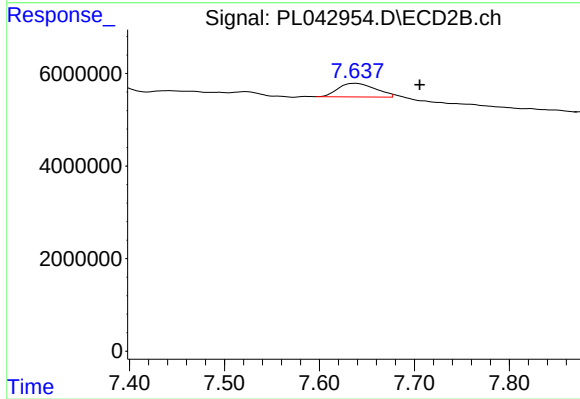

#20 Methoxychlor


R.T.: 7.638 min
Delta R.T.: -0.067 min
Response: 7945436
Conc: 5.27 ng/ml

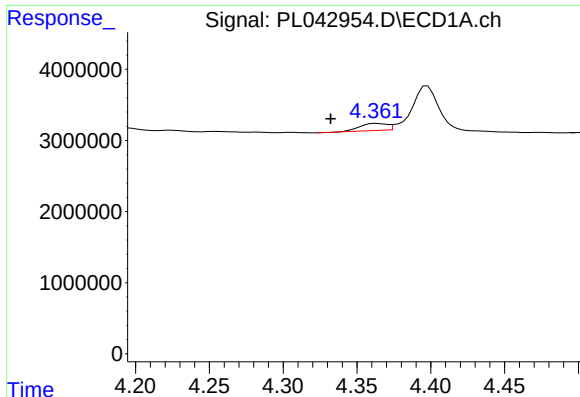

#23 Chlordane-1


R.T.: 4.363 min
Delta R.T.: 0.031 min
Response: 1273571
Conc: 4.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

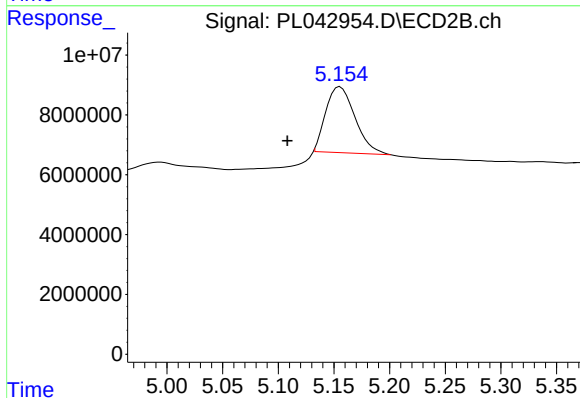


#23 Chlordane-1

R.T.: 5.156 min
Delta R.T.: 0.047 min
Response: 40090977
Conc: 283.66 ng/ml

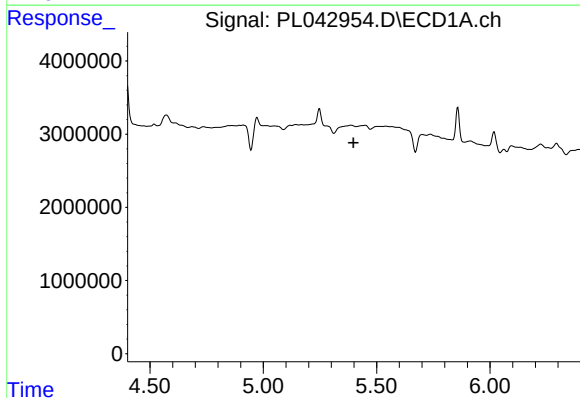


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

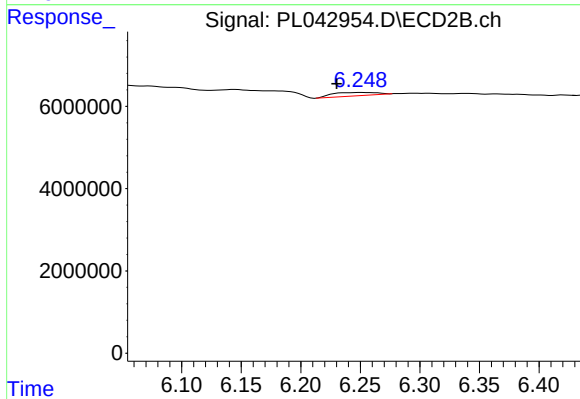

#25 Chlordane-3


R.T.: 6.251 min
Delta R.T.: 0.021 min
Response: 2158905
Conc: 4.40 ng/ml

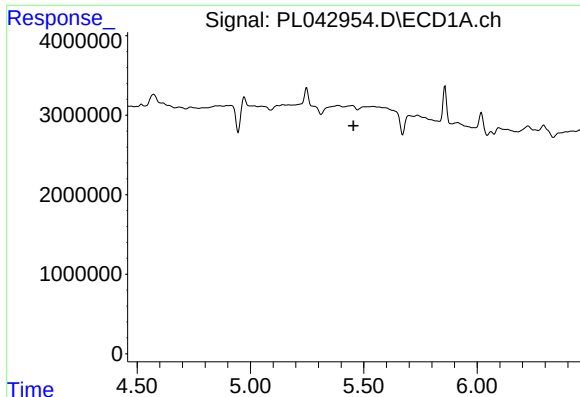

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

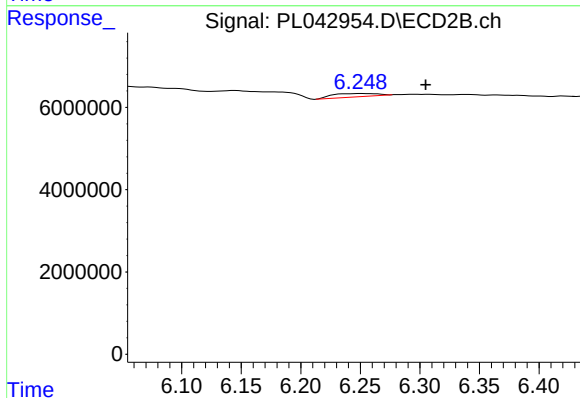


#26 Chlordane-4

R.T.: 6.251 min
Delta R.T.: -0.054 min
Response: 2158905
Conc: 3.78 ng/ml

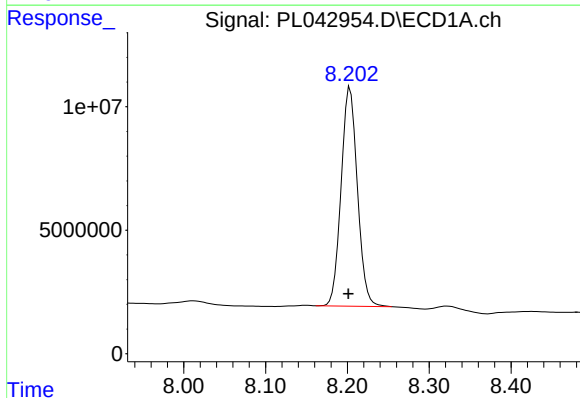

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.002 min
Response: 122139970
Conc: 18.70 ng/ml

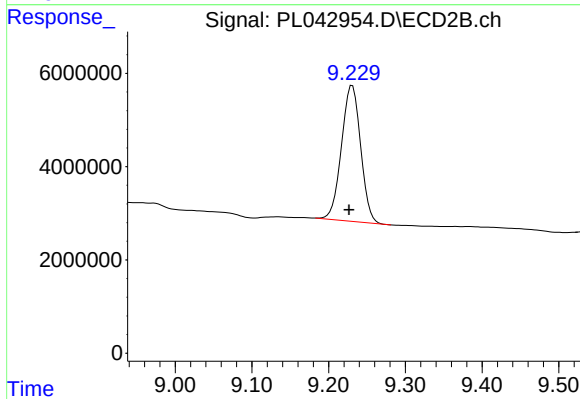

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.004 min
Response: 50608562
Conc: 19.40 ng/ml