

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
 Data File : PL042960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2018 18:59
 Operator : AJ\SJ
 Sample : J6275-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:32:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	107.4E6	53270647	17.508	17.973
28)	SA Decachlor...	8.203	9.230	107.9E6	43056093	16.522	16.506
Target Compounds							
6)	B beta-BHC	4.399f	0.000	6810395	0	1.846	N.D. #
7)	B delta-BHC	0.000	5.157	0	39979738	N.D.	9.303 #
8)	B Heptachlo...	0.000	5.990	0	24246934	N.D.	6.394 #
9)	A Endosulfan I	0.000	6.307f	0	691634	N.D.	0.204 #
10)	B gamma-Chl...	0.000	6.245	0	5341051	N.D.	1.454 #
11)	B alpha-Chl...	0.000	6.307	0	691634	N.D.	0.192 #
14)	MA Endrin	6.064f	0.000	1900676	0	0.264	N.D. #
15)	B Endosulfa...	6.217f	0.000	2437380	0	0.366	N.D. #
16)	A 4,4'-DDD	6.095f	0.000	684887	0	0.121	N.D. #
17)	MA 4,4'-DDT	6.372	0.000	1913438	0	0.322	N.D. #
23)	Chlordane-1	4.359	5.157	1870991	39979738	6.963	282.876 #
25)	Chlordane-3	0.000	6.245	0	5341051	N.D.	10.876 #
26)	Chlordane-4	0.000	6.307	0	691634	N.D.	1.212 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121118\
Data File : PL042960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2018 18:59
Operator : AJ\SJ
Sample : J6275-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:32:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

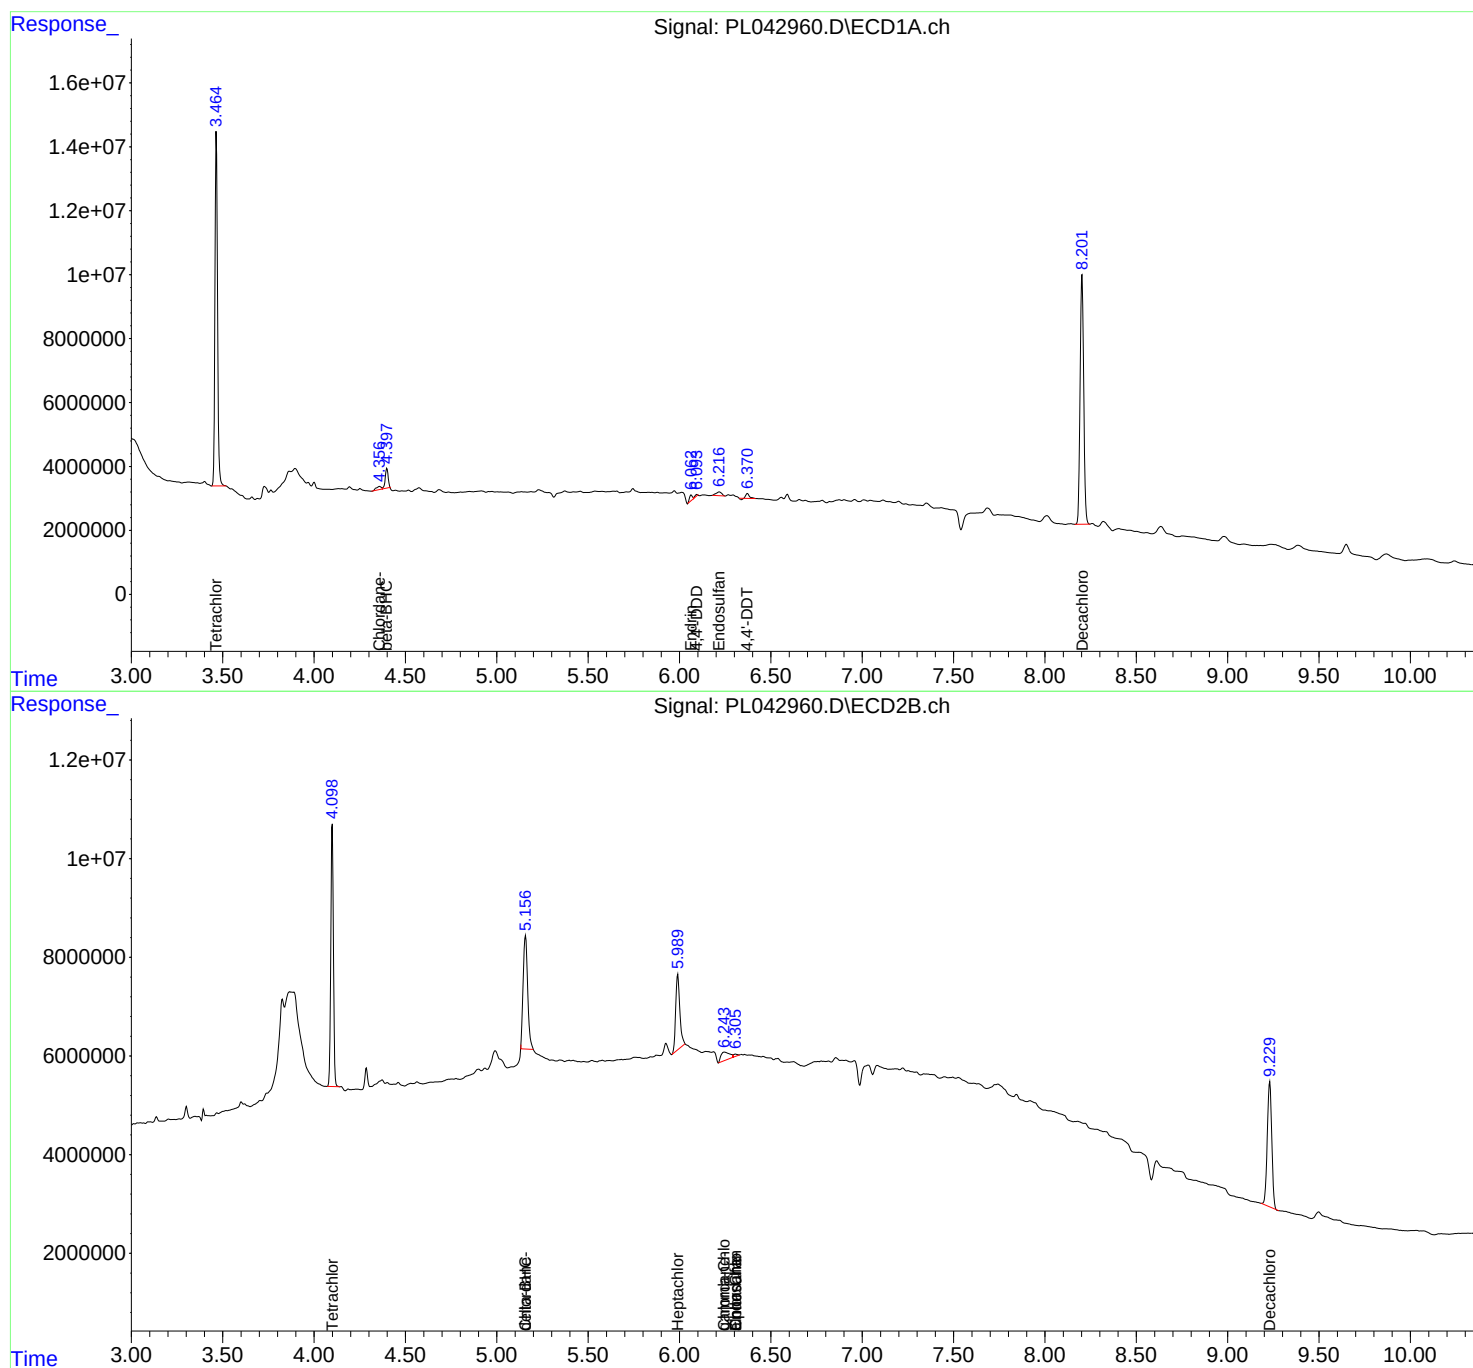


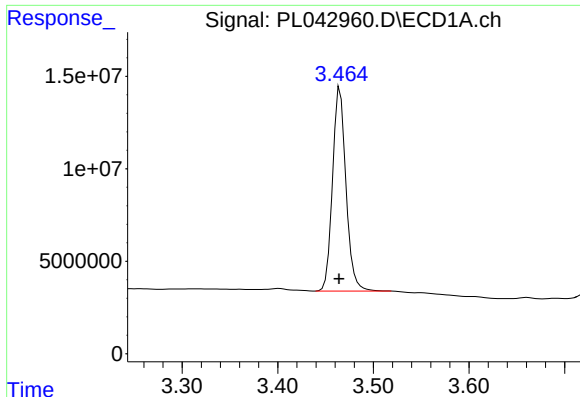

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 107373210
Conc: 17.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

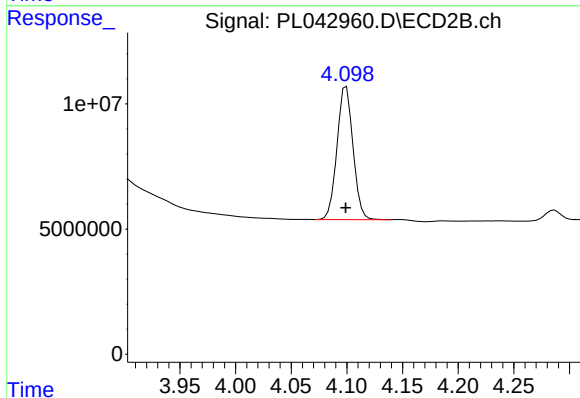


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 53270647
Conc: 17.97 ng/ml

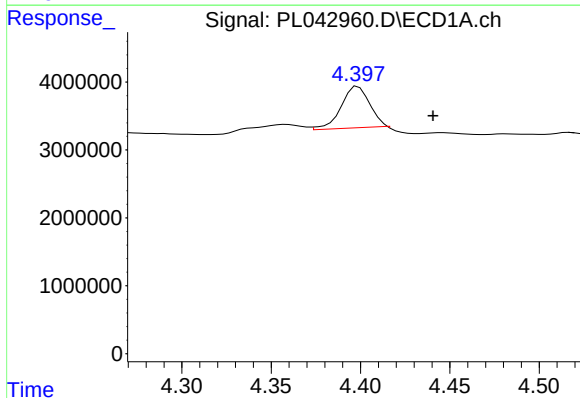


#6 beta-BHC

R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 6810395
Conc: 1.85 ng/ml

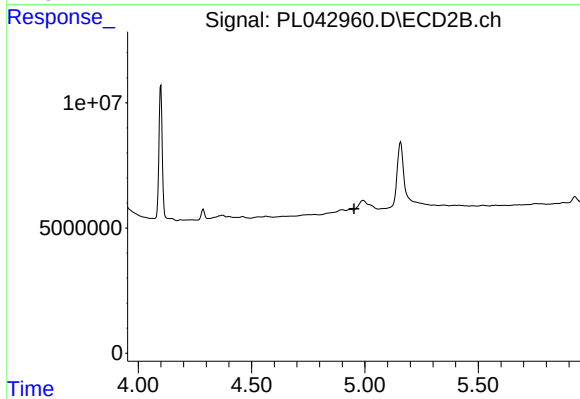

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.952 min
Response: 0
Conc: N.D.

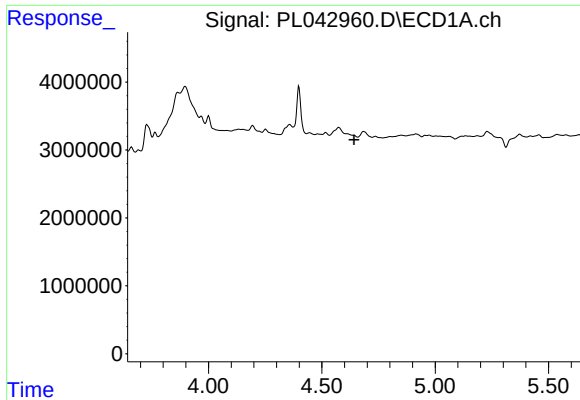

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

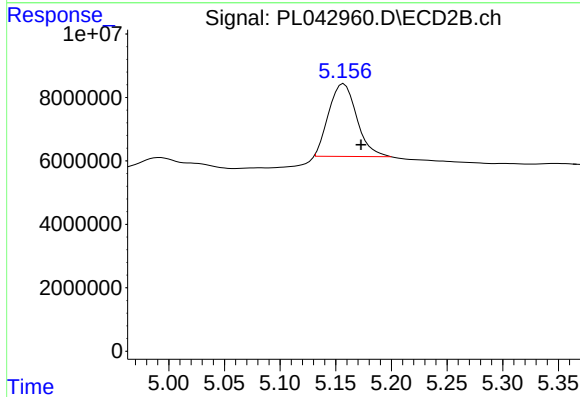


#7 delta-BHC

R.T.: 5.157 min
Delta R.T.: -0.015 min
Response: 39979738
Conc: 9.30 ng/ml

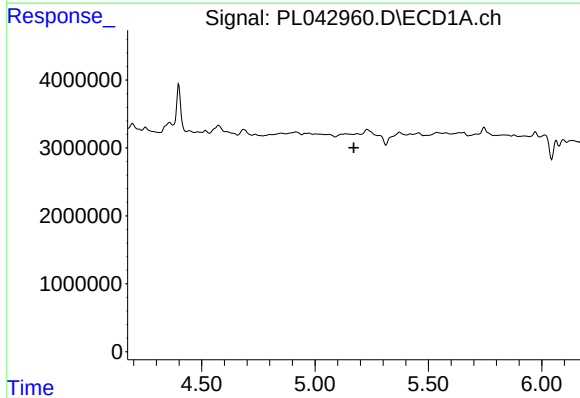


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

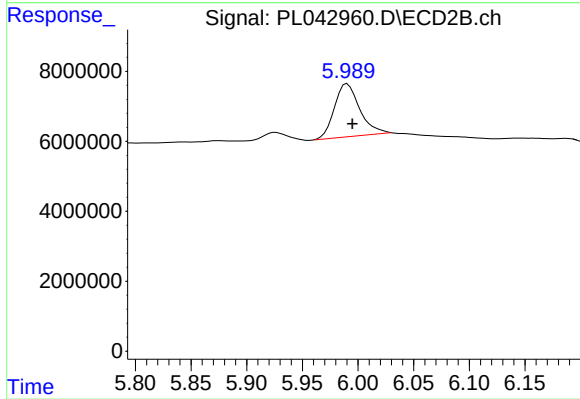

#8 Heptachlor epoxide


R.T.: 5.990 min
Delta R.T.: -0.004 min
Response: 24246934
Conc: 6.39 ng/ml

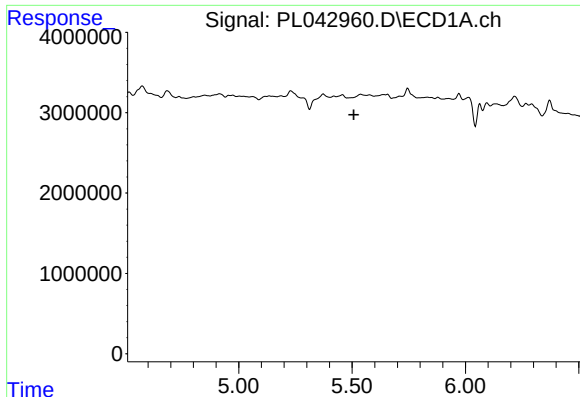

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

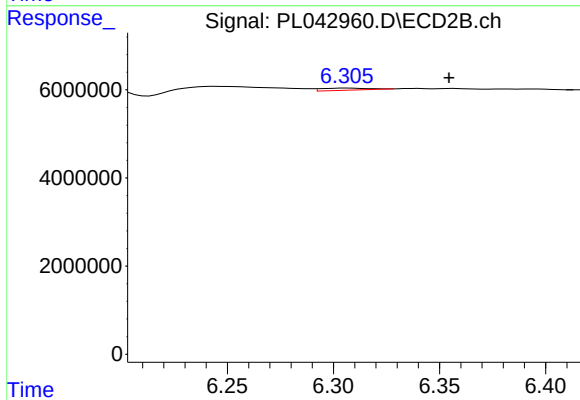


#9 Endosulfan I

R.T.: 6.307 min
Delta R.T.: -0.048 min
Response: 691634
Conc: 0.20 ng/ml

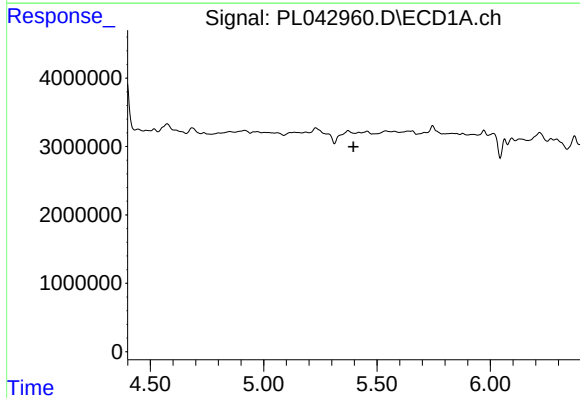


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

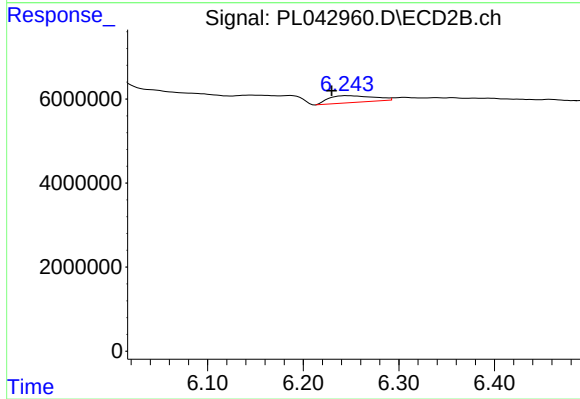

#10 gamma-Chlordane


R.T.: 6.245 min
Delta R.T.: 0.015 min
Response: 5341051
Conc: 1.45 ng/ml

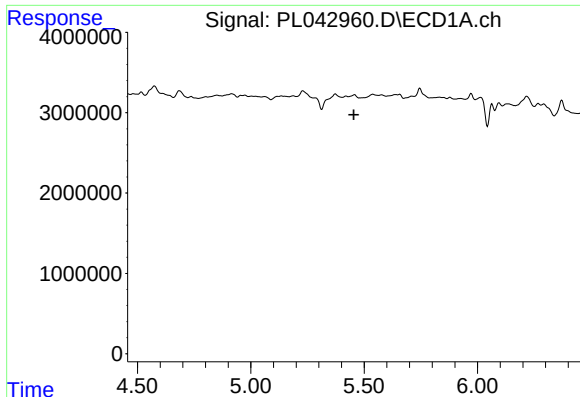

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

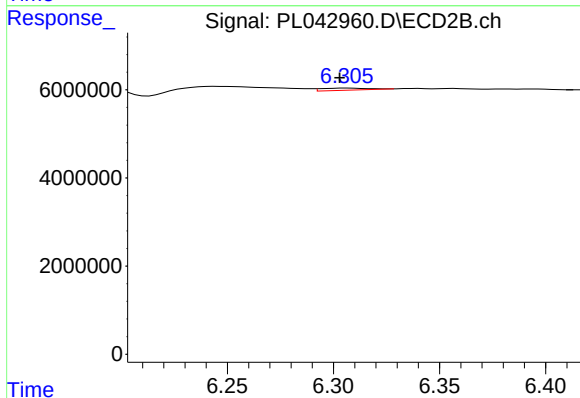


#11 alpha-Chlordane

R.T.: 6.307 min
Delta R.T.: 0.004 min
Response: 691634
Conc: 0.19 ng/ml

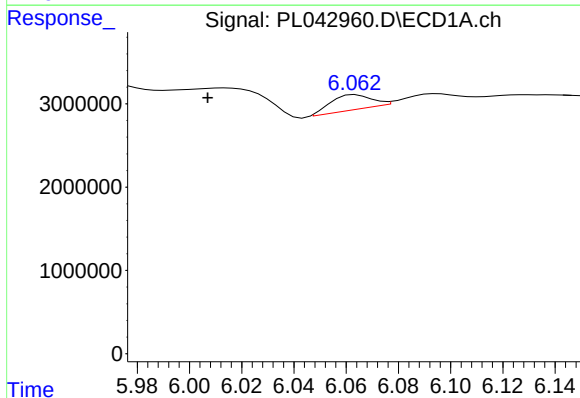


#14 Endrin

R.T.: 6.064 min
Delta R.T.: 0.057 min
Response: 1900676
Conc: 0.26 ng/ml

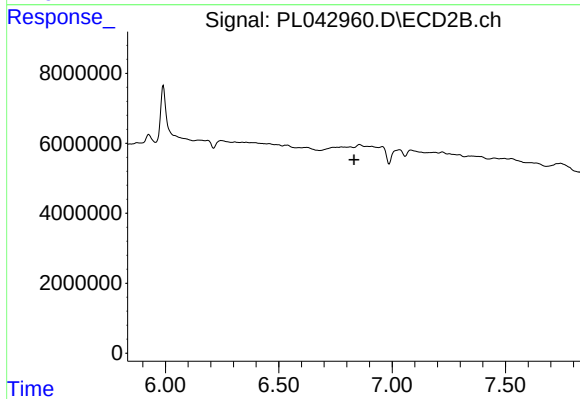

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.832 min
Response: 0
Conc: N.D.

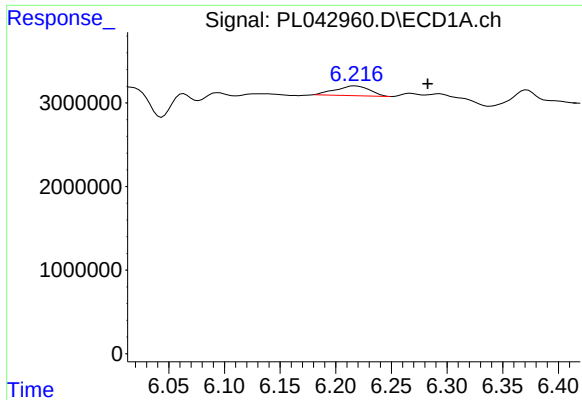

#15 Endosulfan II


R.T.: 6.217 min
Delta R.T.: -0.065 min
Response: 2437380
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

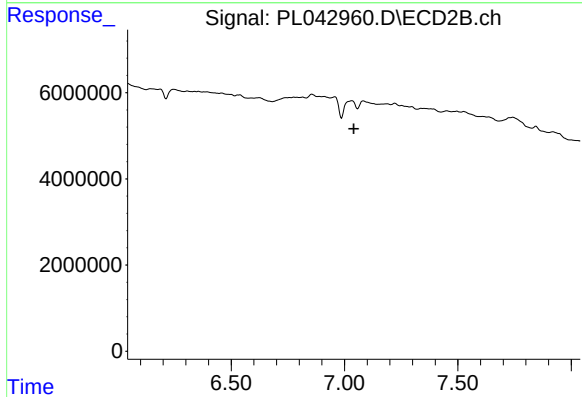


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

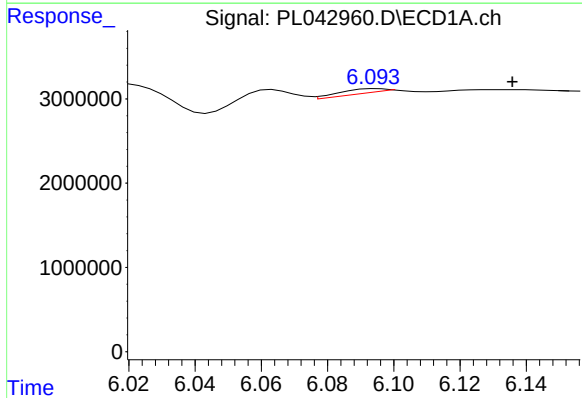


#16 4,4'-DDD

R.T.: 6.095 min
Delta R.T.: -0.041 min
Response: 684887
Conc: 0.12 ng/ml

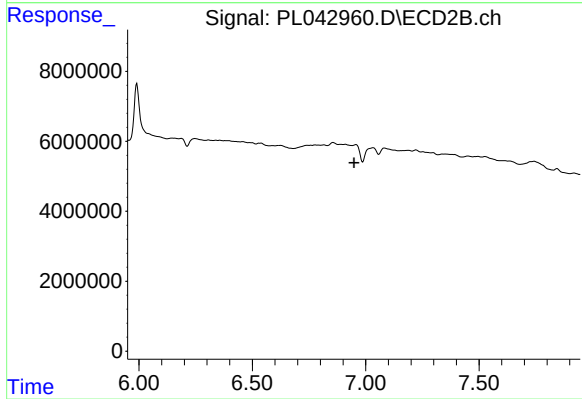

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

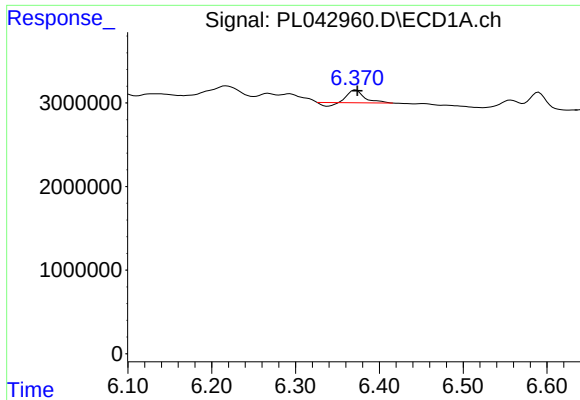

#17 4,4'-DDT


R.T.: 6.372 min
Delta R.T.: -0.002 min
Response: 1913438
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

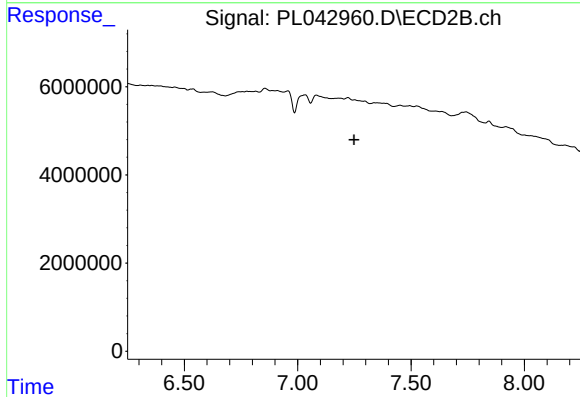


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

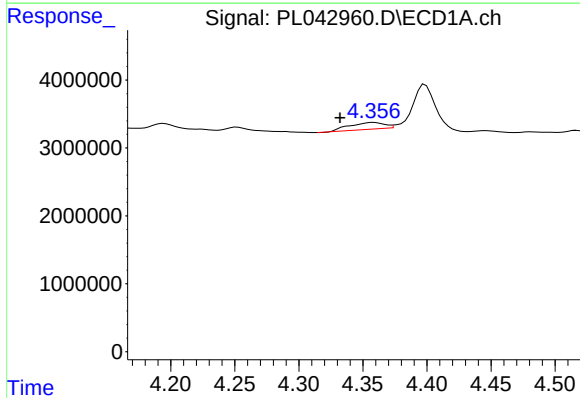


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.027 min
Response: 1870991
Conc: 6.96 ng/ml

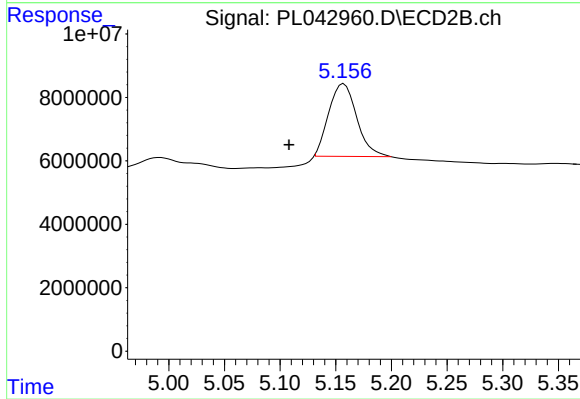

#23 Chlordane-1


R.T.: 5.157 min
Delta R.T.: 0.049 min
Response: 39979738
Conc: 282.88 ng/ml

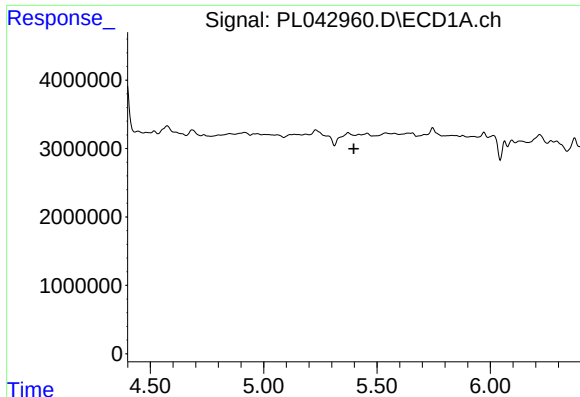

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

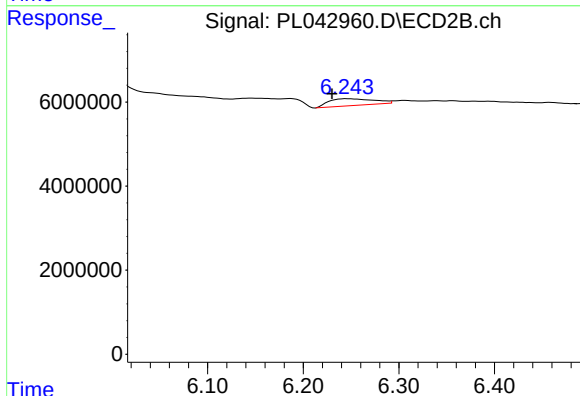


#25 Chlordane-3

R.T.: 6.245 min
Delta R.T.: 0.015 min
Response: 5341051
Conc: 10.88 ng/ml

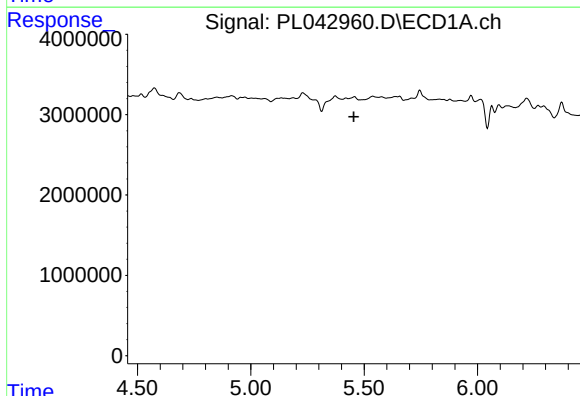


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

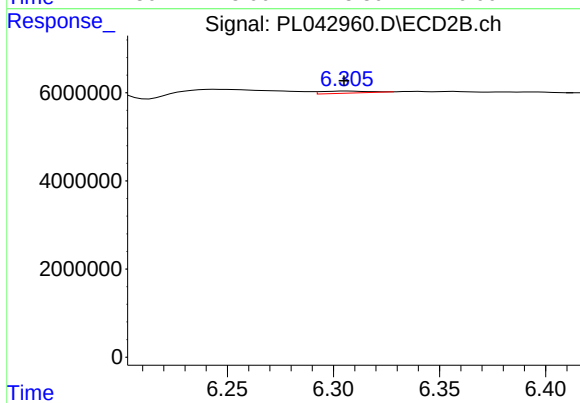

#26 Chlordane-4


R.T.: 6.307 min
Delta R.T.: 0.002 min
Response: 691634
Conc: 1.21 ng/ml

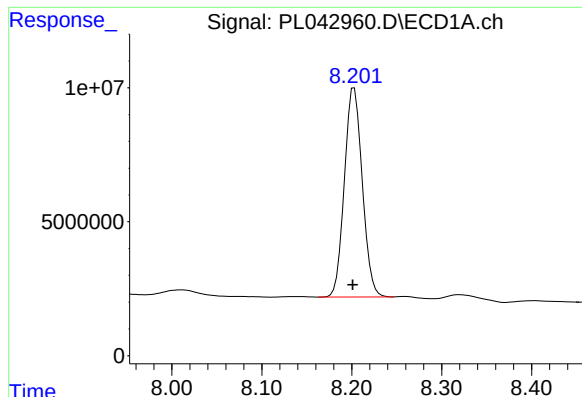

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.002 min
Response: 107885526
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

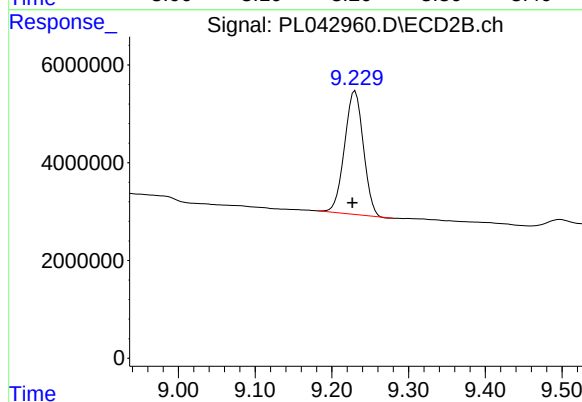

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.003 min
Response: 43056093
Conc: 16.51 ng/ml