

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121119\
 Data File : PL054936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 15:13
 Operator : SG\AJ
 Sample : K6204-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 K072-AB-WC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 03:57:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	4.049	196.2E6	50254081	16.861	19.694
28)	SA Decachlor...	8.320	9.148	158.0E6	41476677	16.499	17.300
Target Compounds							
6)	B beta-BHC	0.000	4.915f	0	7019134	N.D.	4.984 #
10)	B gamma-Chl...	5.499	6.162	9989234	2354998	0.659	0.894 #
11)	B alpha-Chl...	0.000	6.235	0	1606256	N.D.	0.612 #
12)	B 4,4'-DDE	5.721	6.390	29193817	7296854	2.194	2.948 #
14)	MA Endrin	6.113	0.000	6760289	0	0.531	N.D. #
17)	MA 4,4'-DDT	6.480	7.183	17762552	5247102	1.696	2.648 #
23)	Chlordane-1	4.421	0.000	5331256	0	13.509	N.D. #
25)	Chlordane-3	5.499	6.162	9989234	2354998	7.779	7.587
26)	Chlordane-4	0.000	6.235	0	1606256	N.D.	4.269 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121119\
Data File : PL054936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 15:13
Operator : SG\AJ
Sample : K6204-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 03:57:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

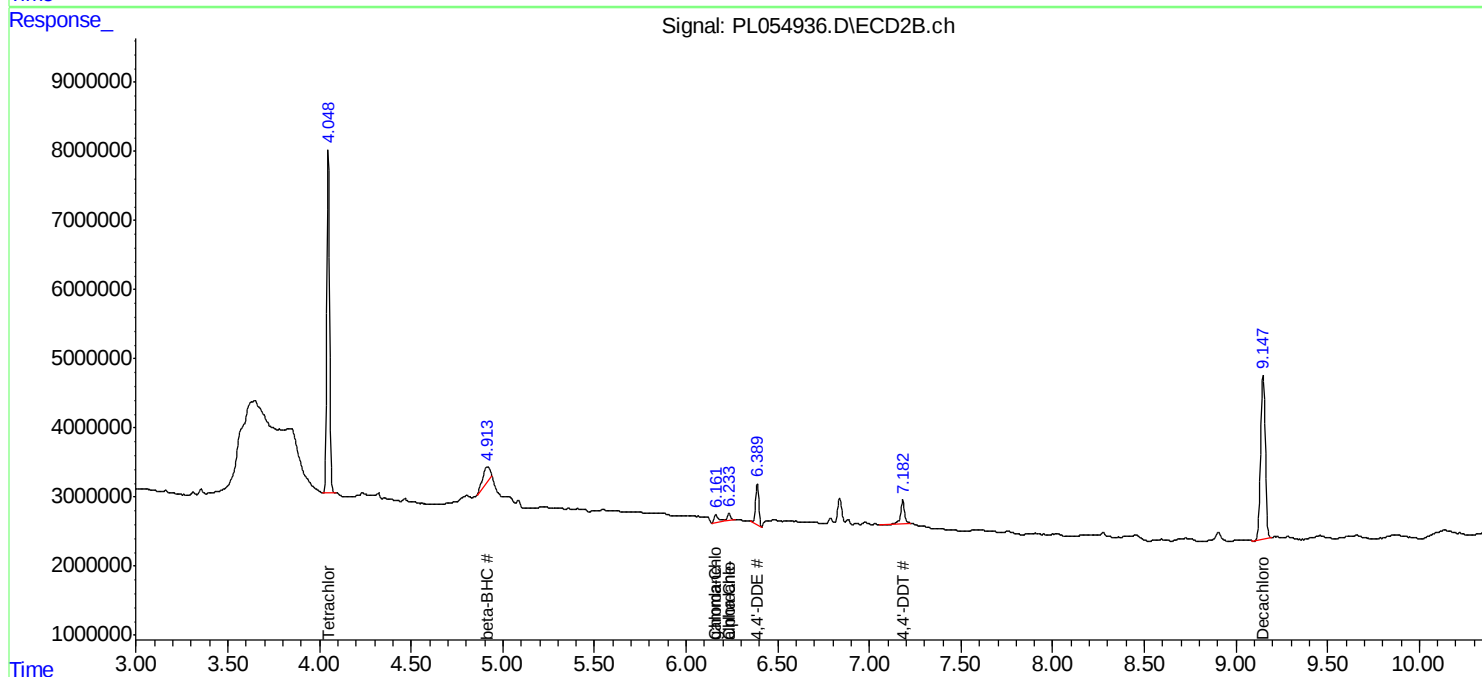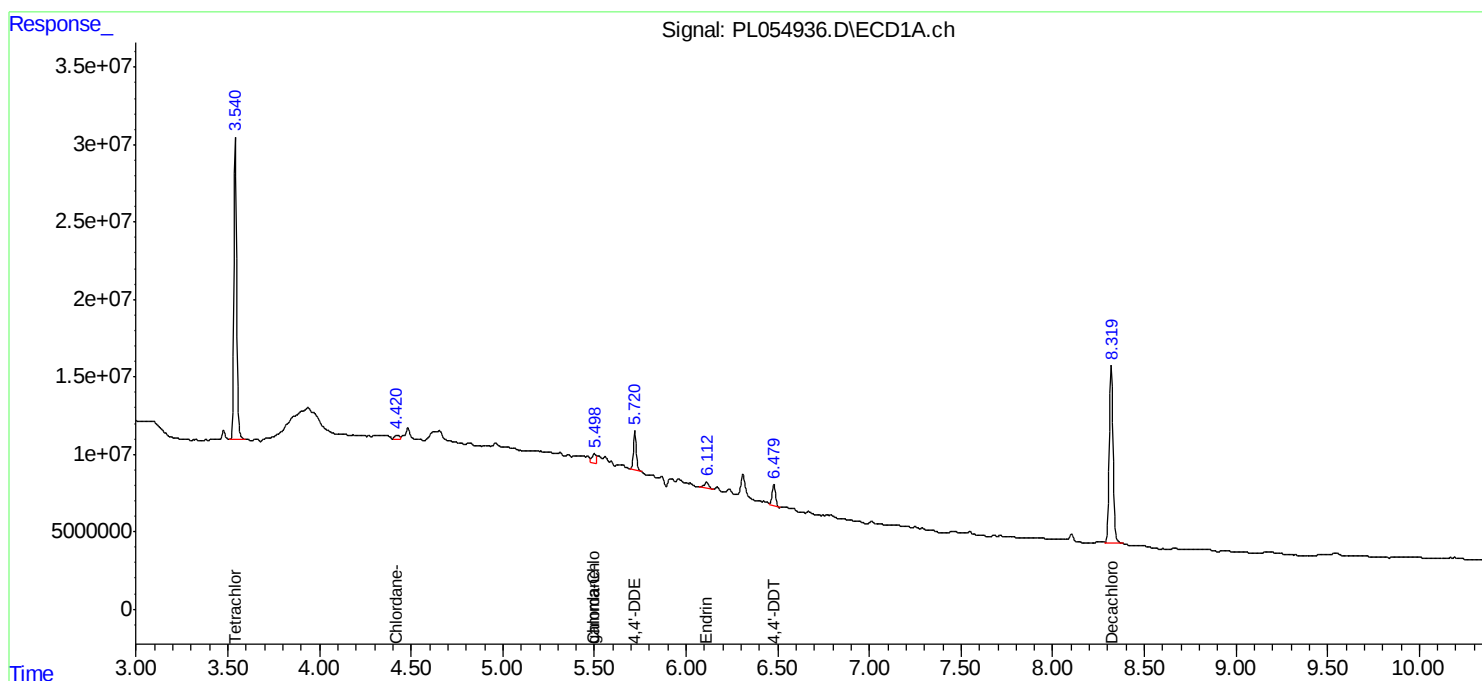


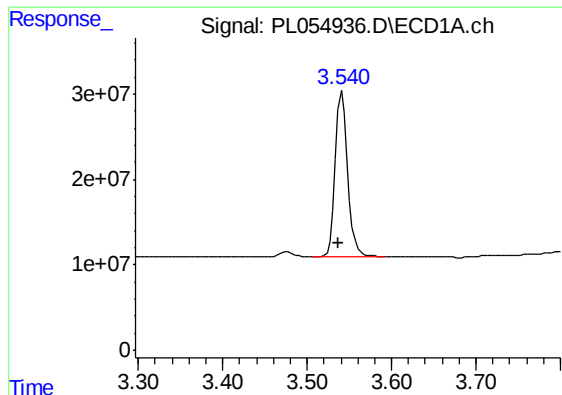

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.004 min
Response: 196168381
Conc: 16.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

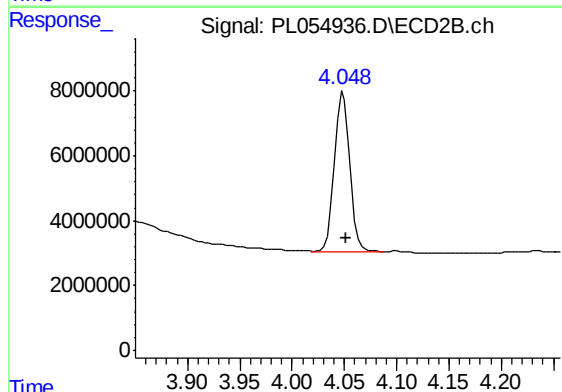


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 50254081
Conc: 19.69 ng/ml

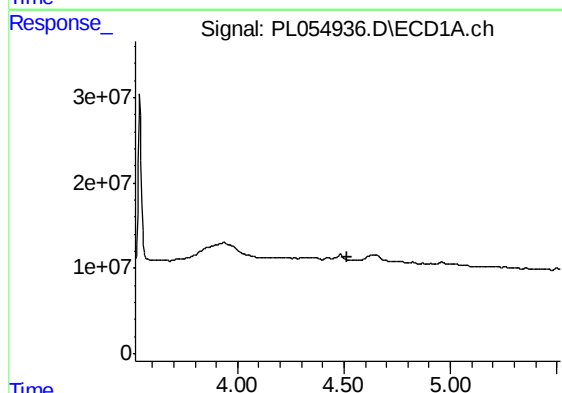


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.518 min
Response: 0
Conc: N.D.

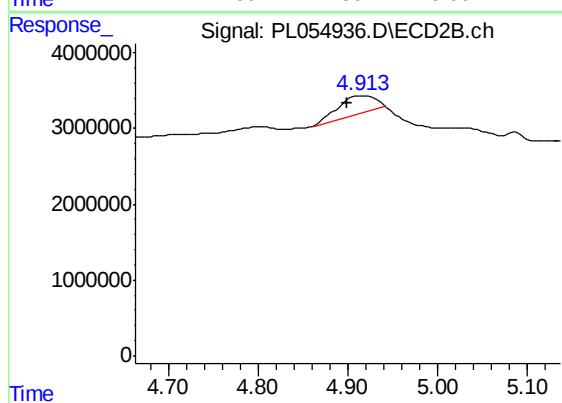

#6 beta-BHC


R.T.: 4.915 min
Delta R.T.: 0.016 min
Response: 7019134
Conc: 4.98 ng/ml

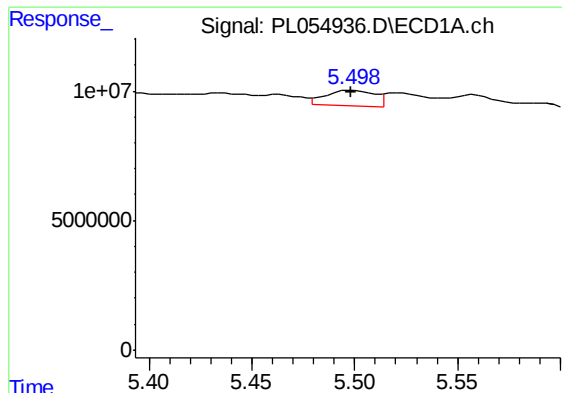

#10 gamma-Chlordane


R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 9989234
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

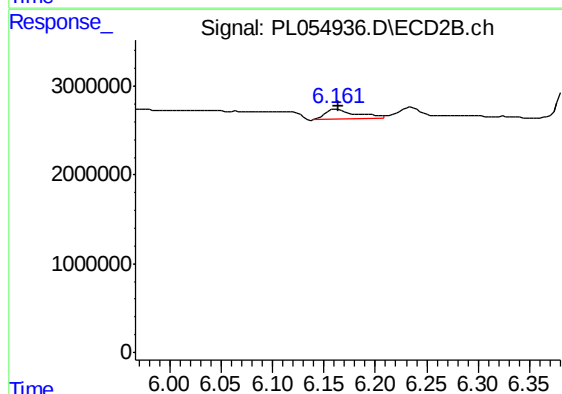


#10 gamma-Chlordane

R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 2354998
Conc: 0.89 ng/ml

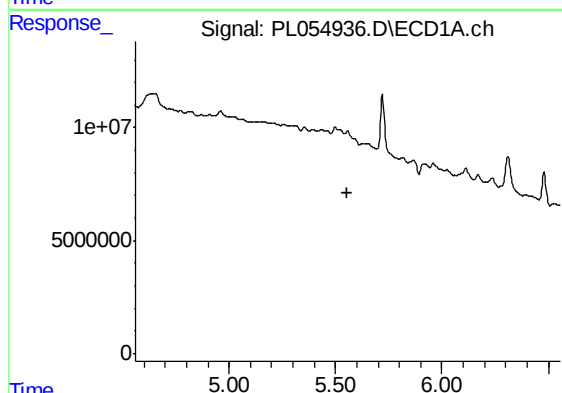


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.557 min
Response: 0
Conc: N.D.

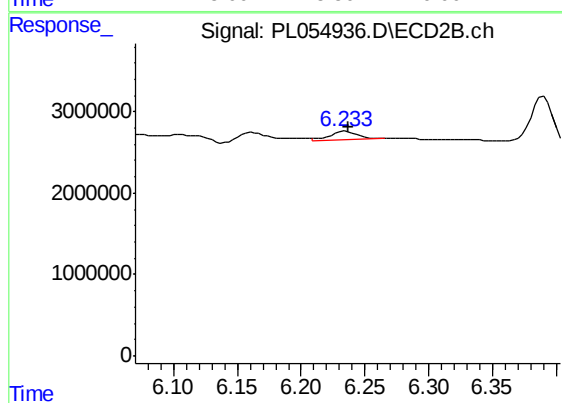

#11 alpha-Chlordane


R.T.: 6.235 min
Delta R.T.: -0.002 min
Response: 1606256
Conc: 0.61 ng/ml

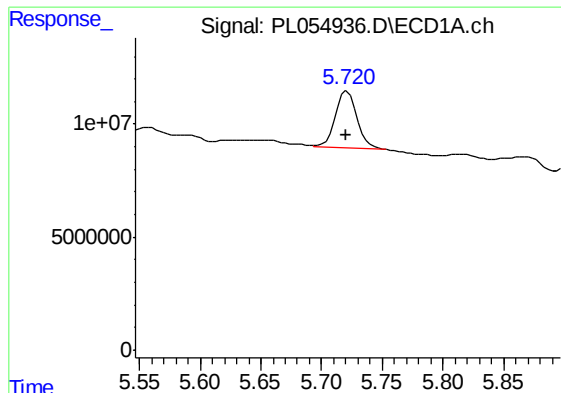

#12 4,4'-DDE


R.T.: 5.721 min
Delta R.T.: 0.001 min
Response: 29193817
Conc: 2.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

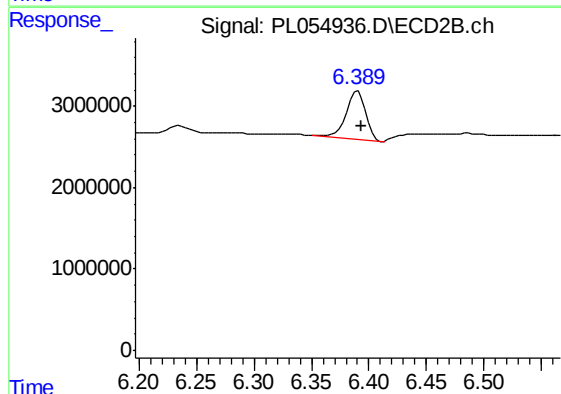


#12 4,4'-DDE

R.T.: 6.390 min
Delta R.T.: -0.003 min
Response: 7296854
Conc: 2.95 ng/ml

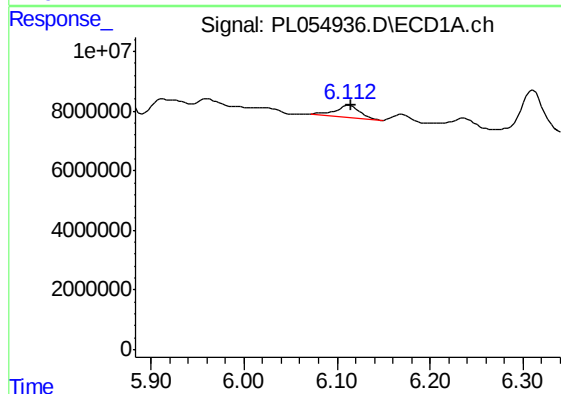


#14 Endrin

R.T.: 6.113 min
Delta R.T.: -0.002 min
Response: 6760289
Conc: 0.53 ng/ml

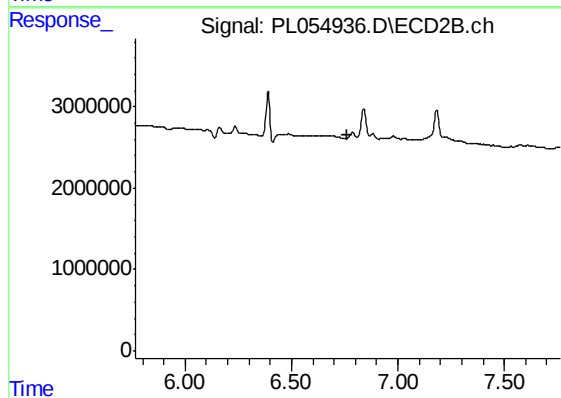

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

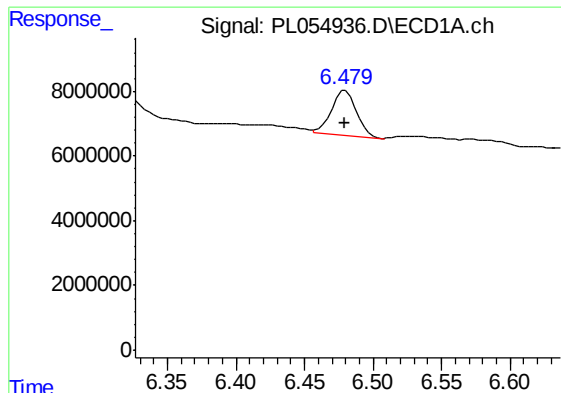

#17 4,4'-DDT


R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 17762552
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

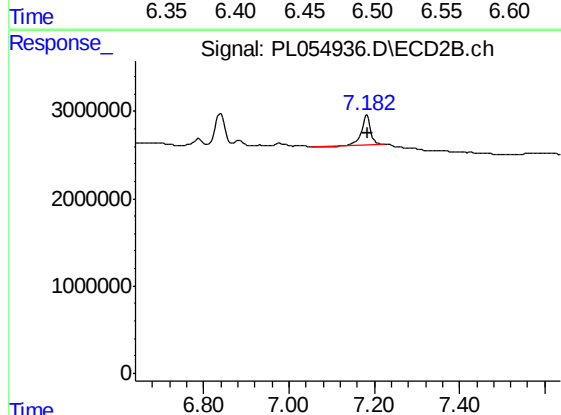


#17 4,4'-DDT

R.T.: 7.183 min
Delta R.T.: -0.002 min
Response: 5247102
Conc: 2.65 ng/ml

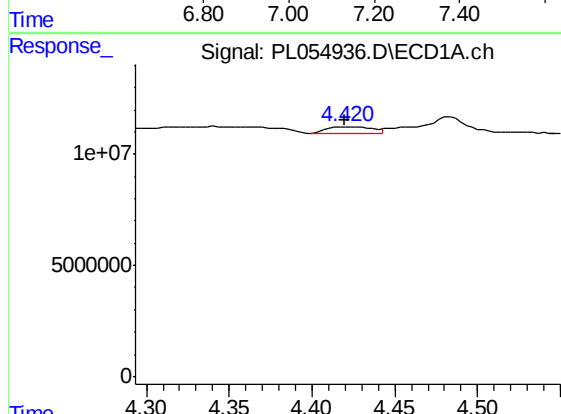


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.001 min
Response: 5331256
Conc: 13.51 ng/ml

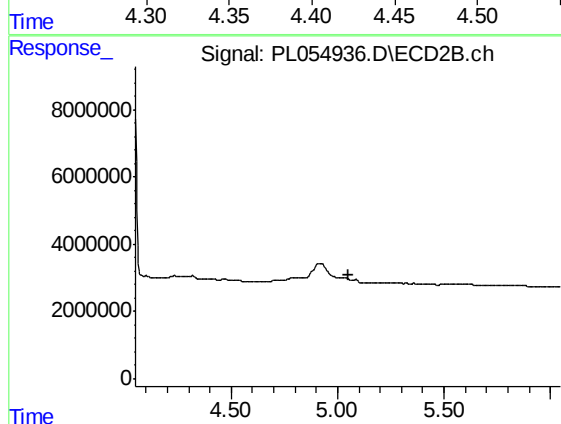

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

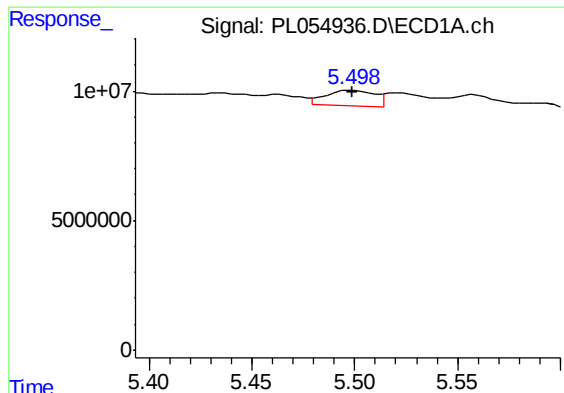

#25 Chlordane-3


R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 9989234
Conc: 7.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

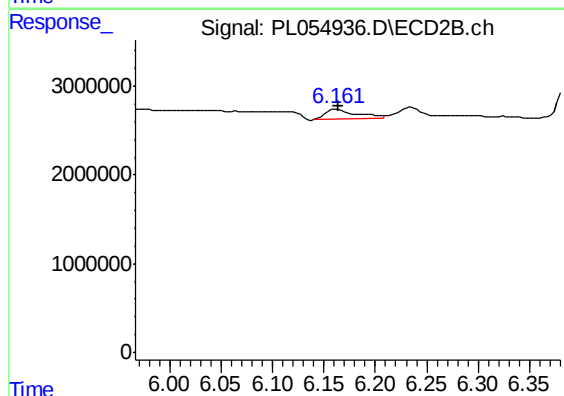


#25 Chlordane-3

R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 2354998
Conc: 7.59 ng/ml

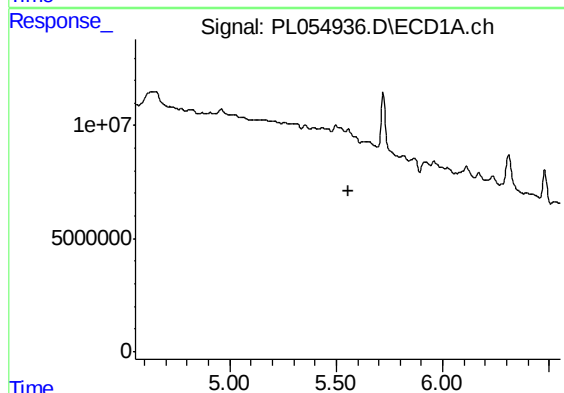


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.556 min
Response: 0
Conc: N.D.

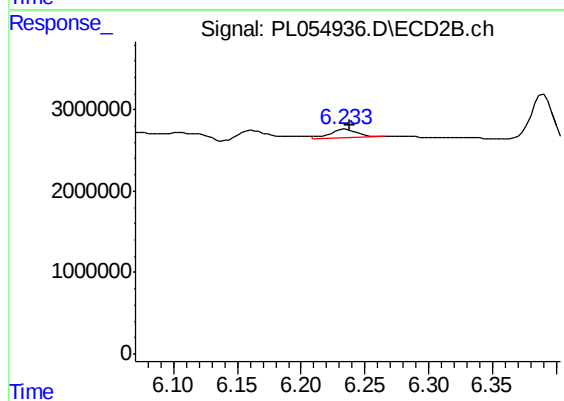

#26 Chlordane-4


R.T.: 6.235 min
Delta R.T.: -0.003 min
Response: 1606256
Conc: 4.27 ng/ml

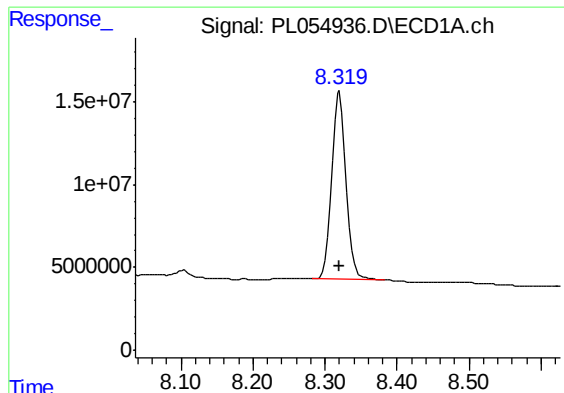

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 157998284
Conc: 16.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
K072-AB-WC-1

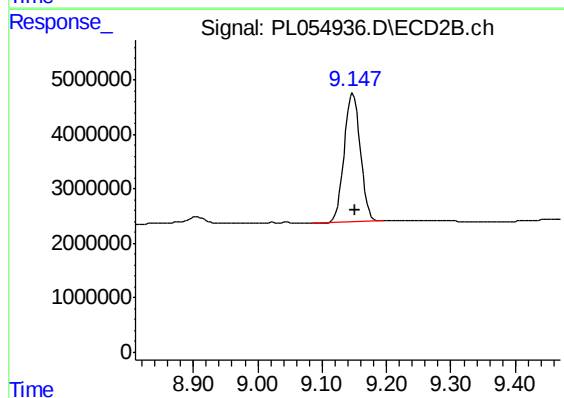

#28 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: -0.004 min
Response: 41476677
Conc: 17.30 ng/ml