

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121119\
 Data File : PL054940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 16:10
 Operator : SG\AJ
 Sample : K6247-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT3465

Manual Integrations
 APPROVED

Ankita
 12/12/2019 11:14:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 03:58:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.049	246.7E6	55550970	21.202	21.769
28)	SA Decachlor...	8.315	9.145	163.6E6	42592946	17.086	17.766
Target Compounds							
16)	A 4,4'-DDD	6.232	6.878	14049789	3507976	1.438m	1.827m#
17)	MA 4,4'-DDT	6.473	7.181	10053292	1263970	0.960	0.638 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121119\
Data File : PL054940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 16:10
Operator : SG\AJ
Sample : K6247-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
RT3465


Manual Integrations
APPROVED

Ankita
12/12/2019 11:14:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 03:58:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

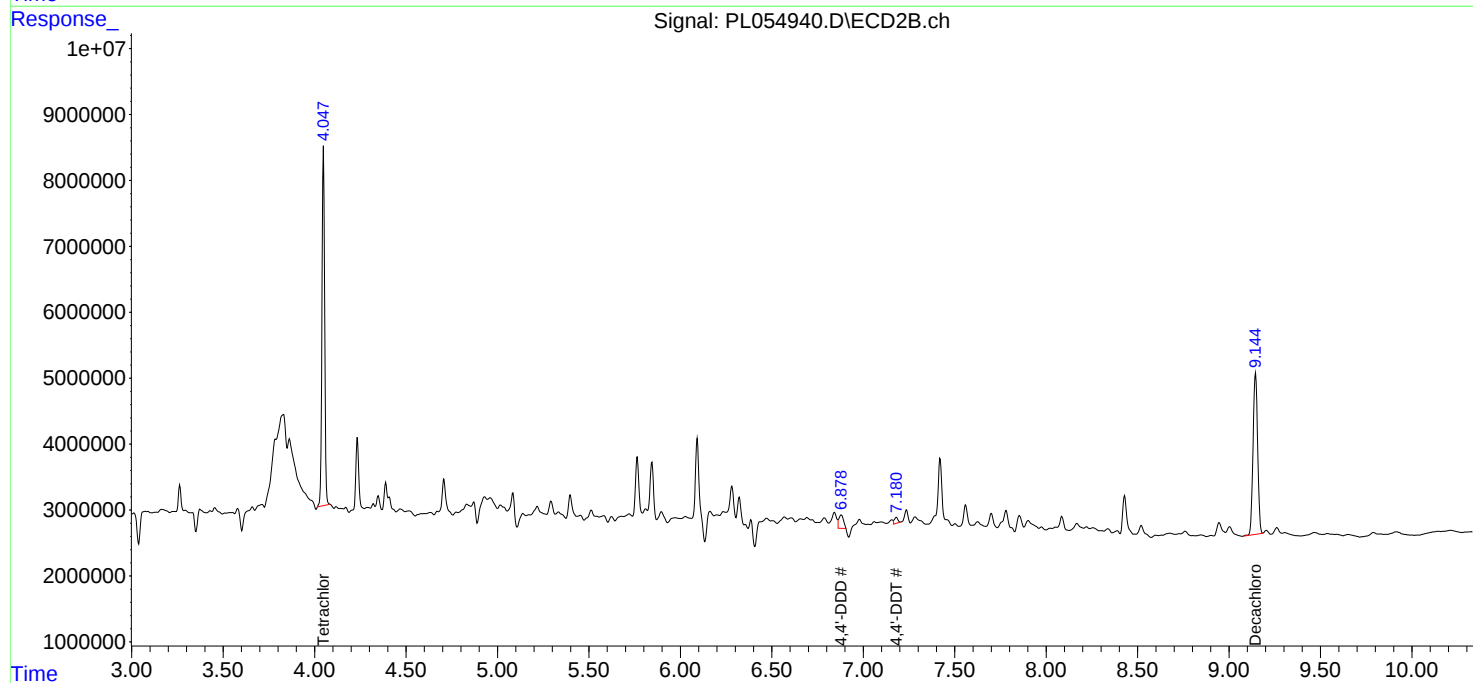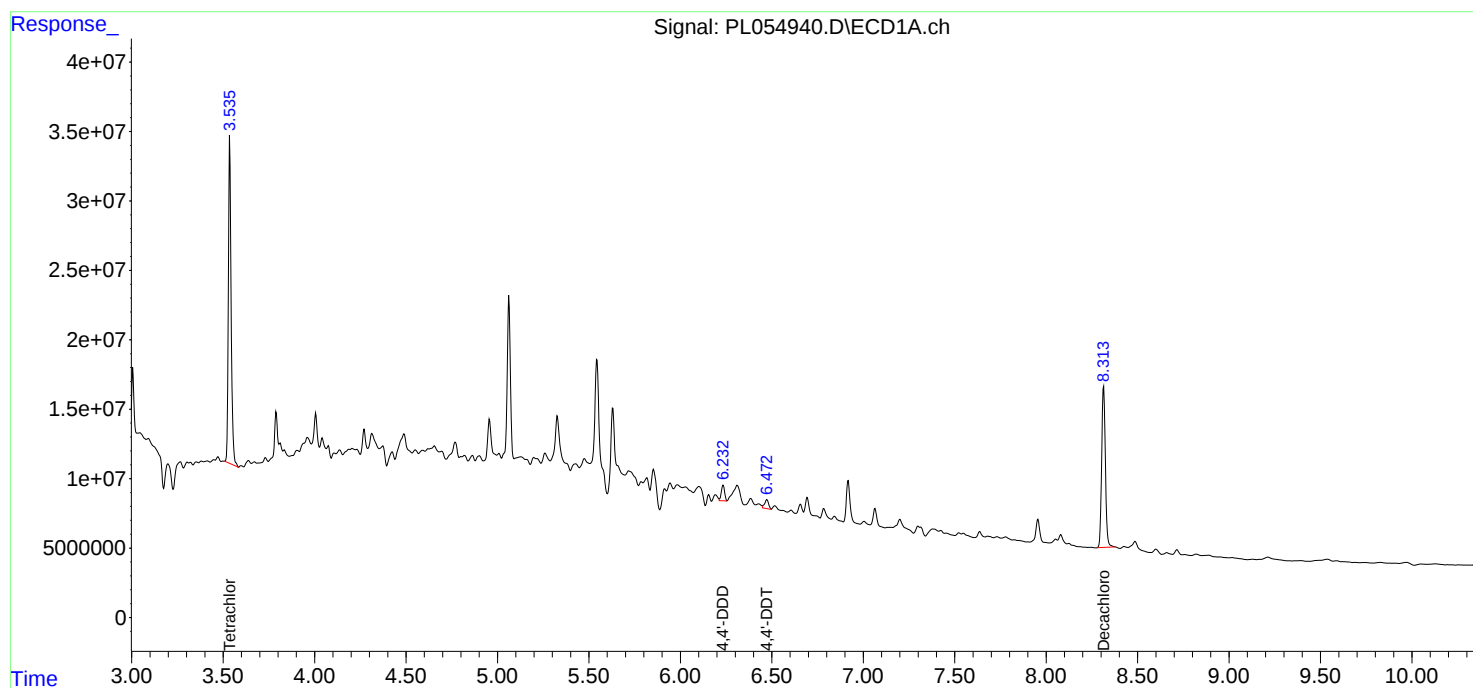

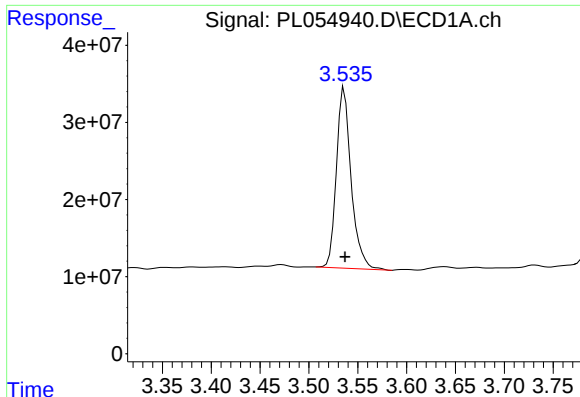


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 246665379
Conc: 21.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT3465


Manual Integrations
APPROVED

Ankita
12/12/2019 11:14:55 AM

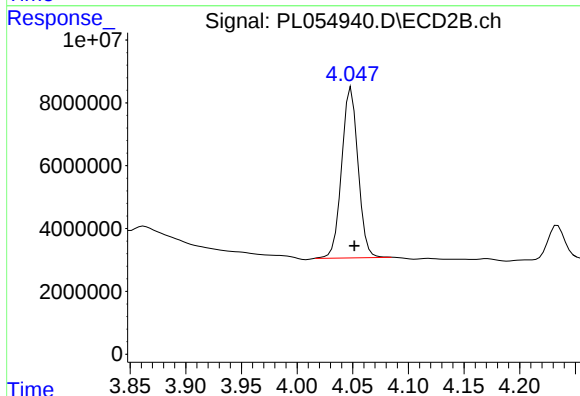


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.003 min
Response: 55550970
Conc: 21.77 ng/ml

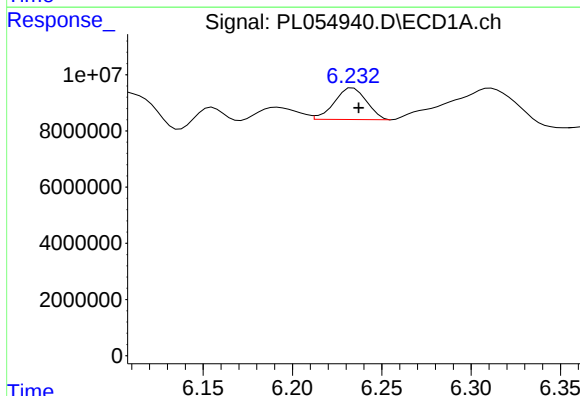


#16 4,4'-DDD

R.T.: 6.232 min
Delta R.T.: -0.005 min
Response: 14049789
Conc: 1.44 ng/ml m

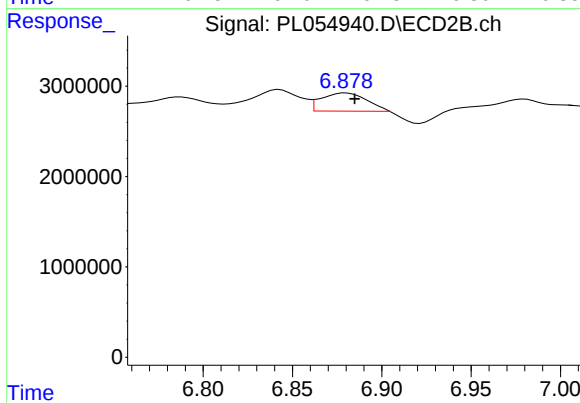

#16 4,4'-DDD

R.T.: 6.878 min
Delta R.T.: -0.006 min
Response: 3507976
Conc: 1.83 ng/ml m

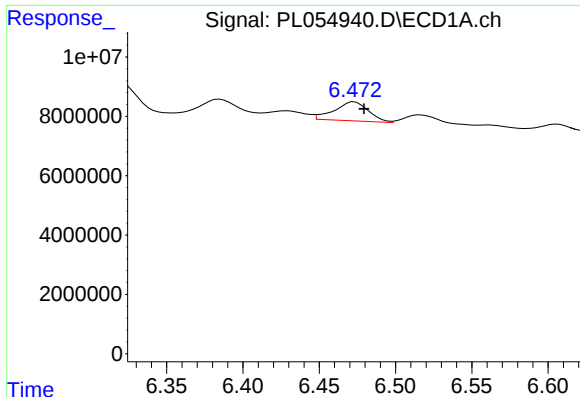


#17 4,4'-DDT

R.T.: 6.473 min
Delta R.T.: -0.006 min
Response: 10053292
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT3465


Manual Integrations
APPROVED

Ankita
12/12/2019 11:14:55 AM

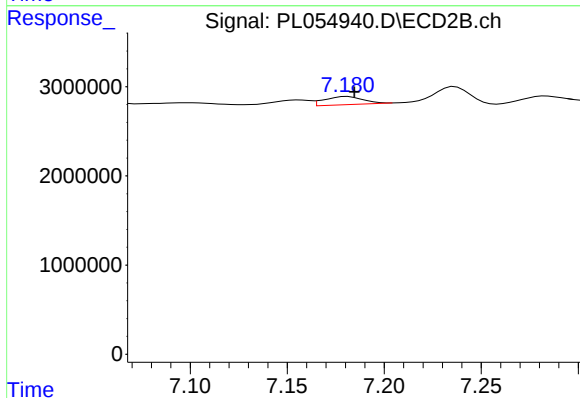


#17 4,4'-DDT

R.T.: 7.181 min
Delta R.T.: -0.004 min
Response: 1263970
Conc: 0.64 ng/ml

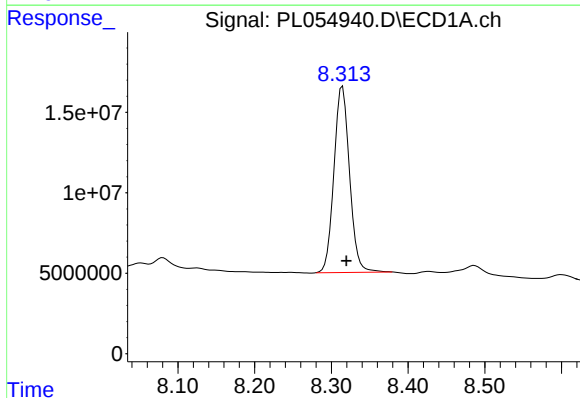

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.005 min
Response: 163613618
Conc: 17.09 ng/ml

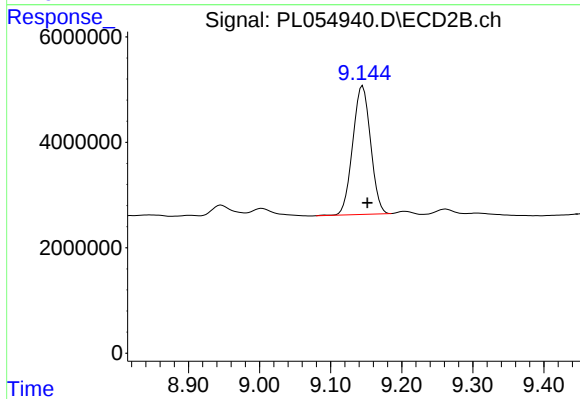

#28 Decachlorobiphenyl

R.T.: 9.145 min
Delta R.T.: -0.006 min
Response: 42592946
Conc: 17.77 ng/ml