

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
 Data File : PL063444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 09:17
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 09:50:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 09:46:51 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	154.8E6	242.9E6	73.518	72.268
28)	SA Decachlor...	8.127	8.990	143.5E6	189.7E6	68.627	70.576
Target Compounds							
23)	Chlordane-1	4.268	4.936	40966197	86667846	711.993	726.076
24)	Chlordane-2	4.764	5.403	44403208	87577810	695.079	660.733
25)	Chlordane-3	5.327	6.046	129.6E6	343.7E6	728.700	712.710
26)	Chlordane-4	5.384	6.121	109.1E6	403.8E6	731.745	704.656
27)	Chlordane-5	6.213	6.923	45818340	69984425	727.876	755.720



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
Data File : PL063444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 09:17
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 09:50:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 09:46:51 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

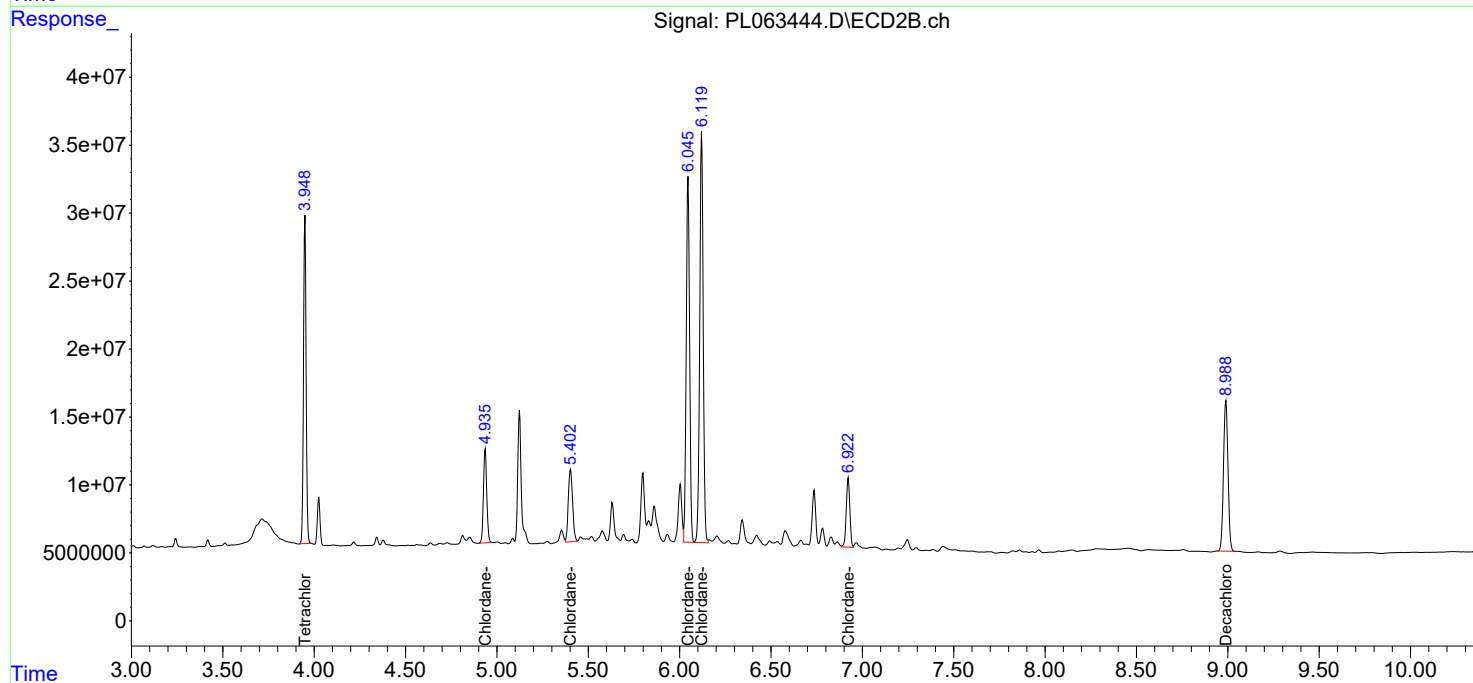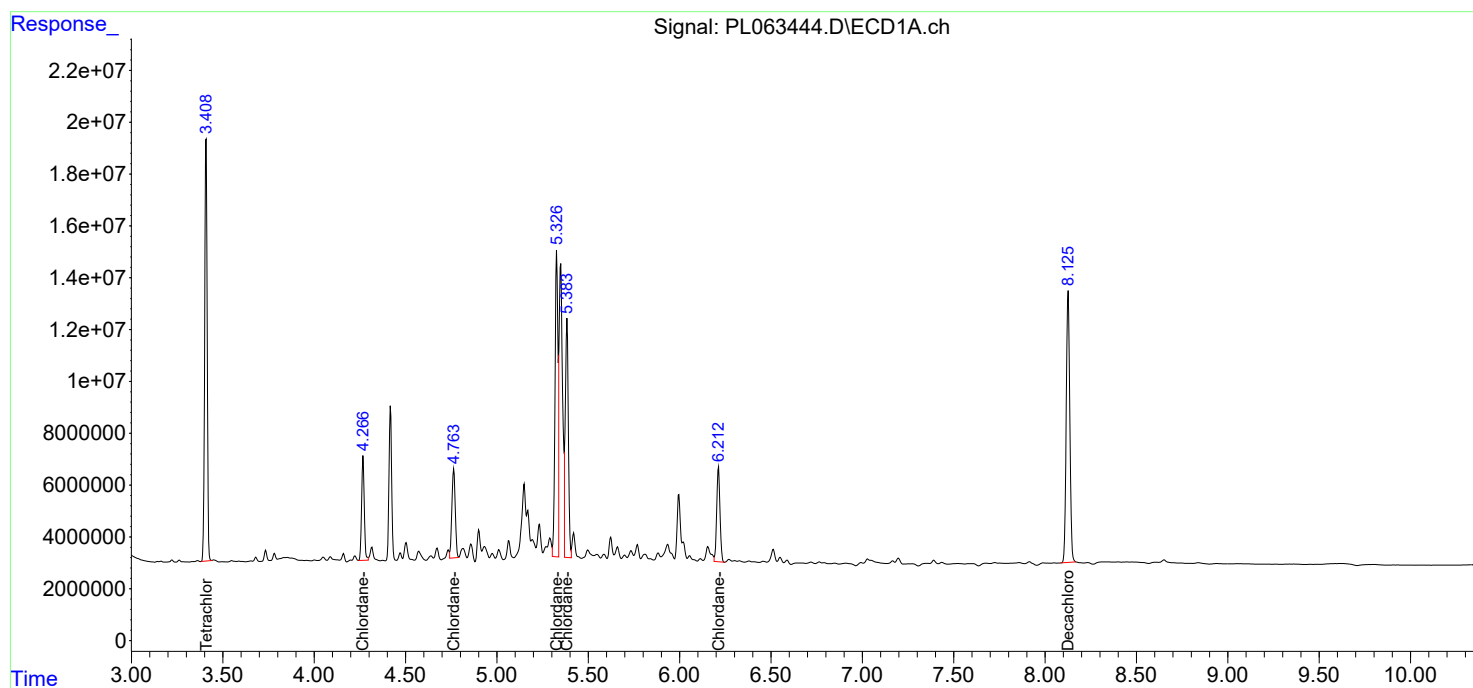


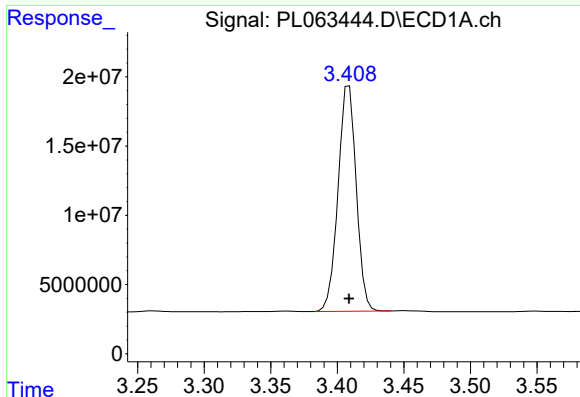

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 154758661
Conc: 73.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

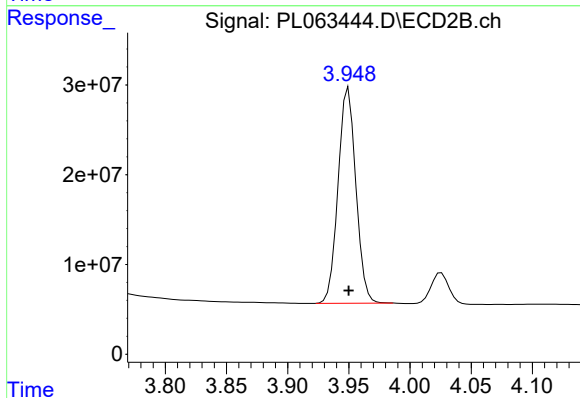


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 242946614
Conc: 72.27 ng/ml

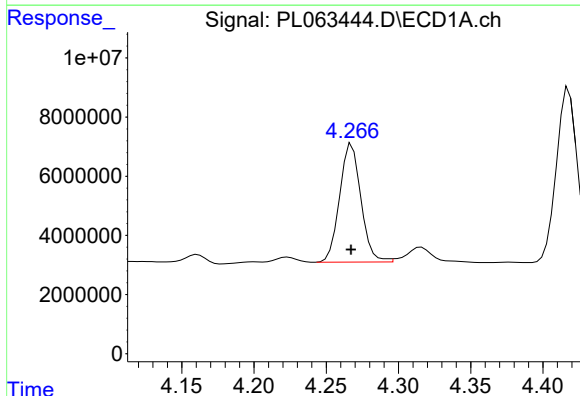


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 40966197
Conc: 711.99 ng/ml

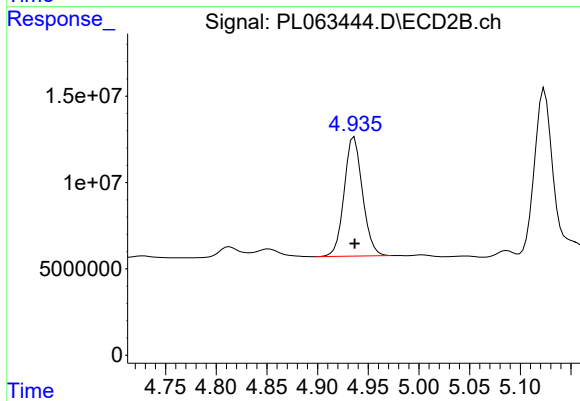

#23 Chlordane-1


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 86667846
Conc: 726.08 ng/ml

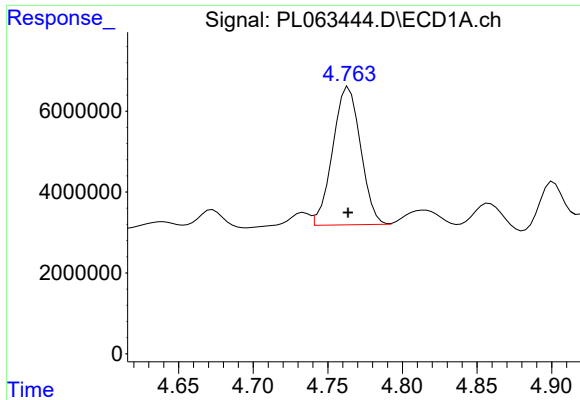

#24 Chlordane-2


R.T.: 4.764 min
Delta R.T.: 0.000 min
Response: 44403208
Conc: 695.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

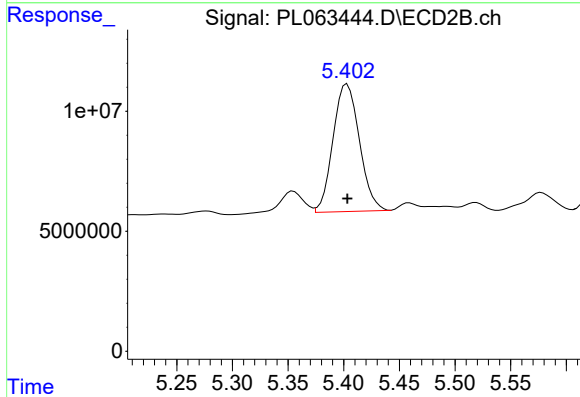


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 87577810
Conc: 660.73 ng/ml

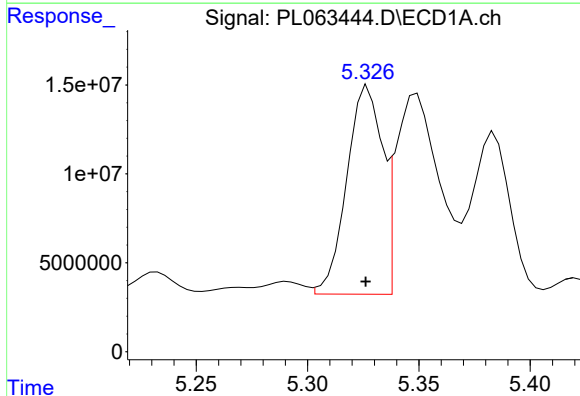


#25 Chlordane-3

R.T.: 5.327 min
Delta R.T.: 0.001 min
Response: 129576927
Conc: 728.70 ng/ml

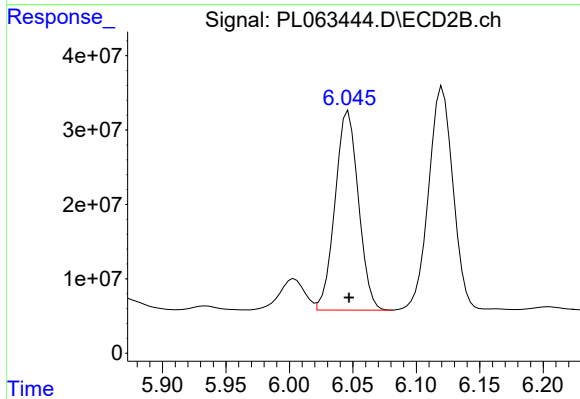

#25 Chlordane-3


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 343666587
Conc: 712.71 ng/ml

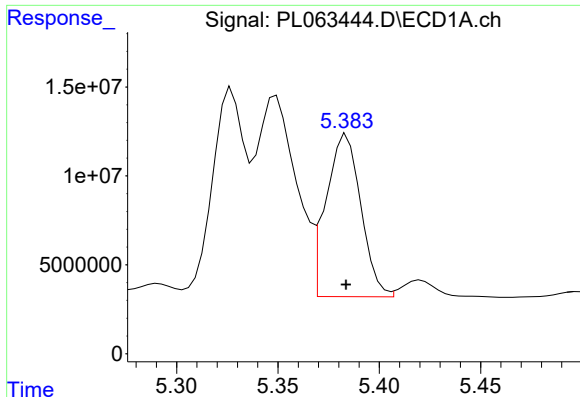

#26 Chlordane-4


R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 109148564
Conc: 731.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

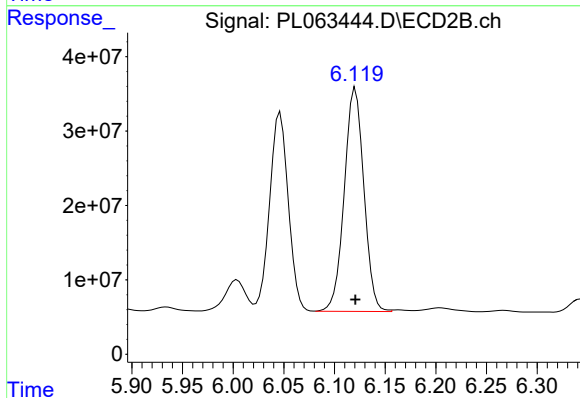


#26 Chlordane-4

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 403804996
Conc: 704.66 ng/ml

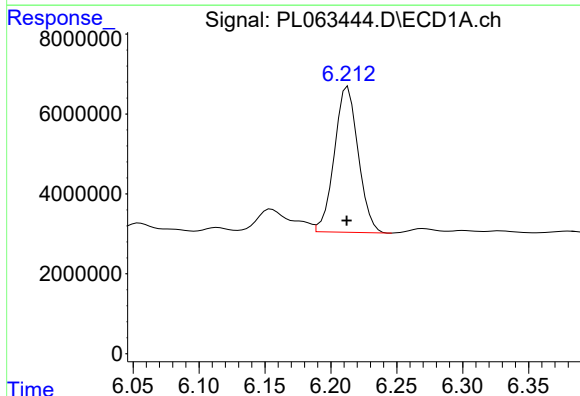


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.001 min
Response: 45818340
Conc: 727.88 ng/ml

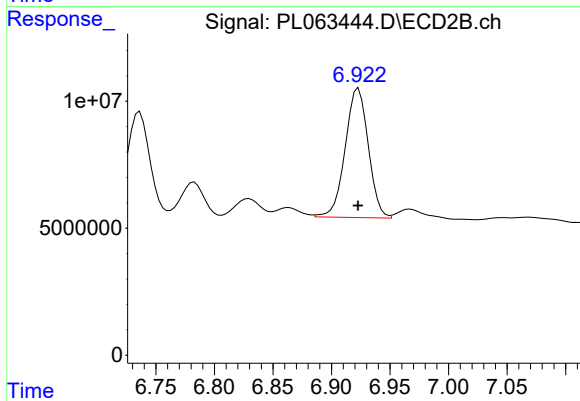

#27 Chlordane-5


R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 69984425
Conc: 755.72 ng/ml

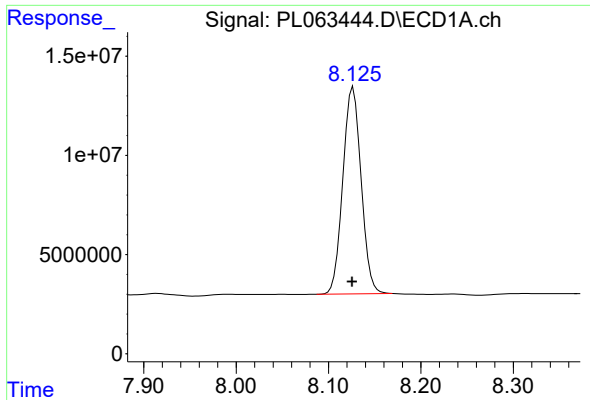

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 143489473
Conc: 68.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

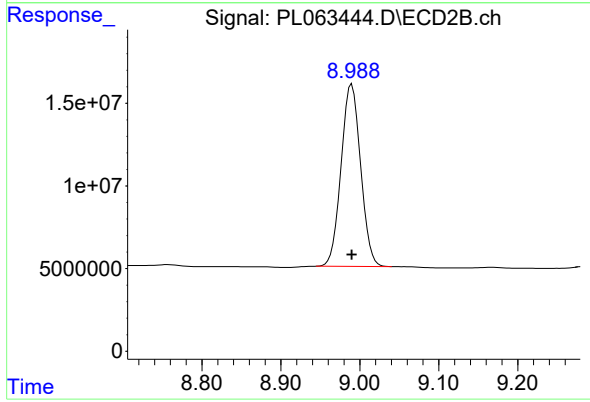

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 189680011
Conc: 70.58 ng/ml