

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
 Data File : PL063448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 10:14
 Operator : DD\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL121120

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 10:26:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 10:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.408	3.950	101.9E6	164.1E6	49.424	50.050
28)	SA Decachlor...	8.124	8.989	100.7E6	129.5E6	48.564	48.309
Target Compounds							
23)	Chlordane-1	4.267	4.936	27700449	58045507	506.707	505.897
24)	Chlordane-2	4.763	5.403	30937805	67266046	492.697	532.992
25)	Chlordane-3	5.326	6.046	84119647	238.1E6	485.518	516.682
26)	Chlordane-4	5.383	6.121	71976870	279.3E6	492.068	509.398
27)	Chlordane-5	6.211	6.923	29990161	44504909	481.066	490.405


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
Data File : PL063448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 10:14
Operator : DD\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL121120

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 10:26:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 10:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

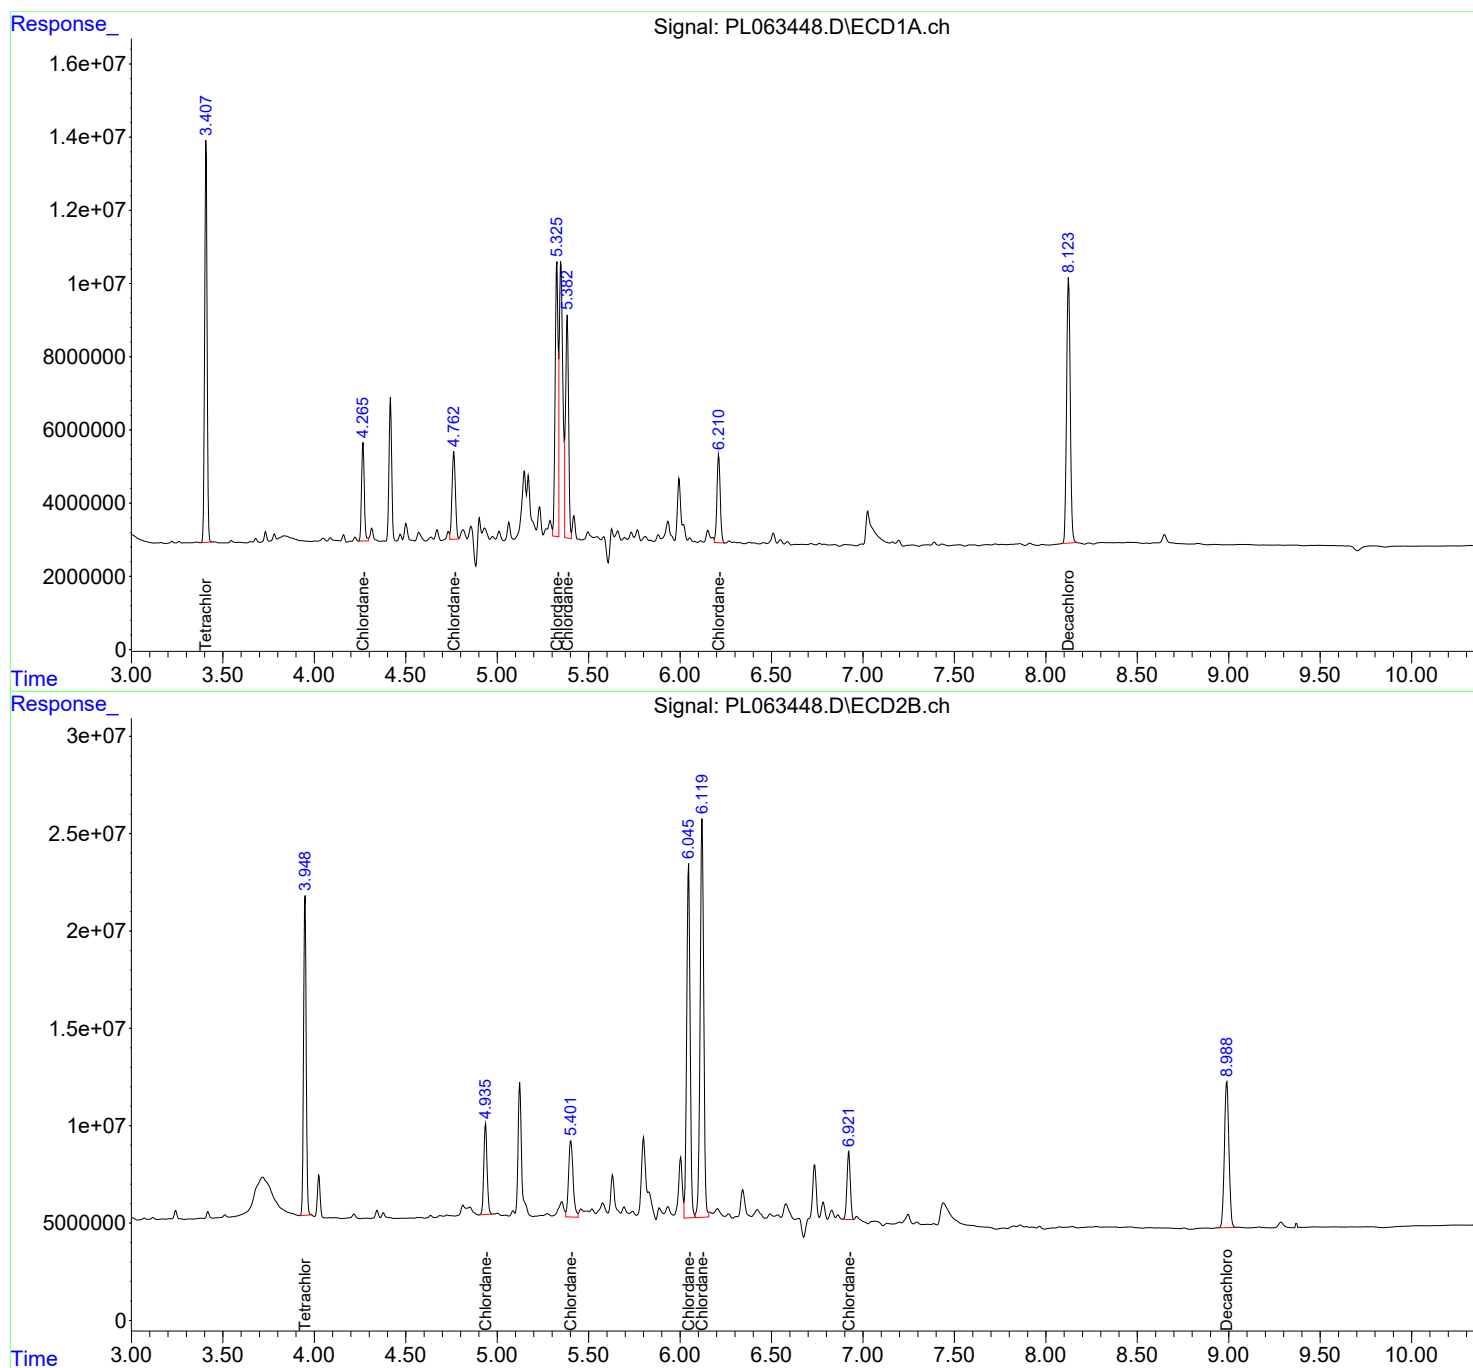


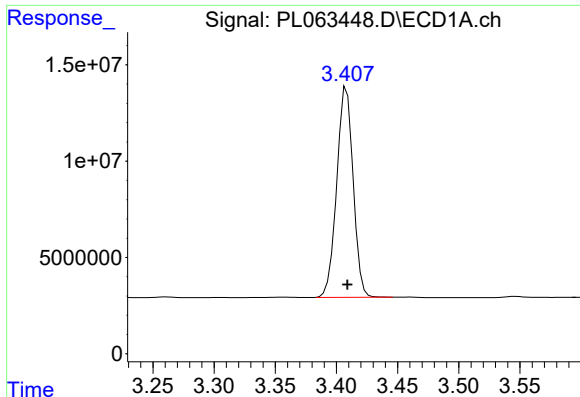

#1 Tetrachloro-m-xylene


R.T.: 3.408 min
Delta R.T.: 0.000 min
Response: 101900345
Conc: 49.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121120

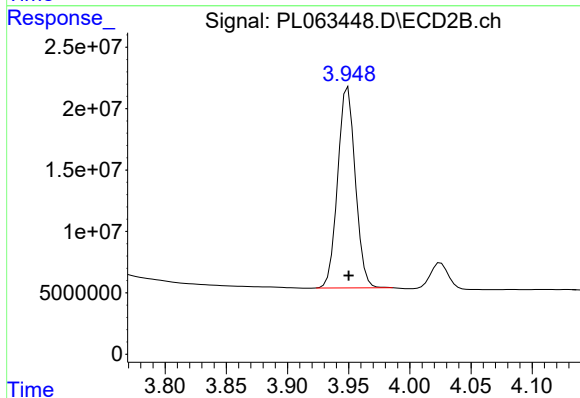


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 164091147
Conc: 50.05 ng/ml

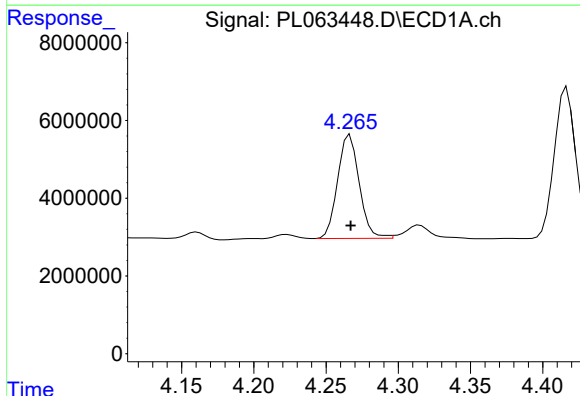


#23 Chlordane-1

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 27700449
Conc: 506.71 ng/ml

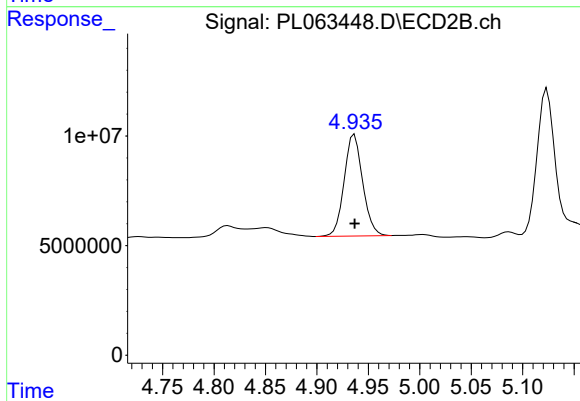

#23 Chlordane-1


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 58045507
Conc: 505.90 ng/ml

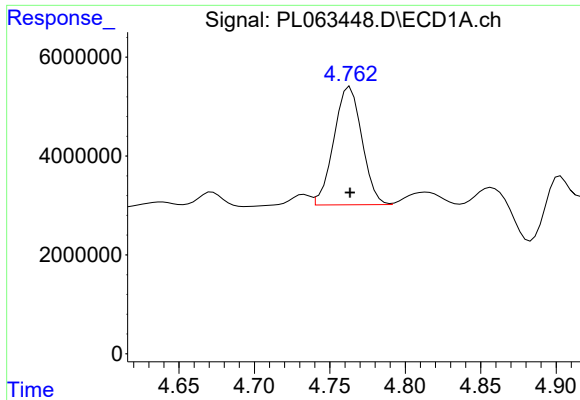

#24 Chlordane-2


R.T.: 4.763 min
Delta R.T.: 0.000 min
Response: 30937805
Conc: 492.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121120

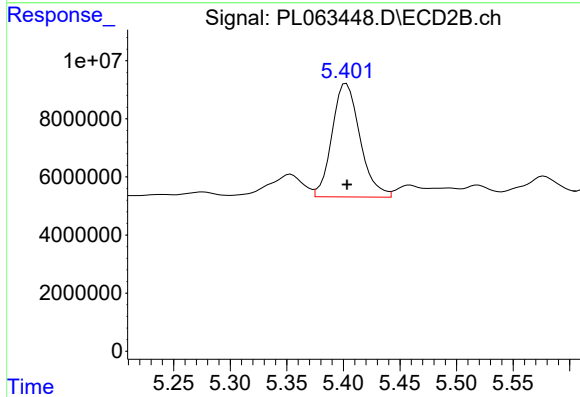


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 67266046
Conc: 532.99 ng/ml

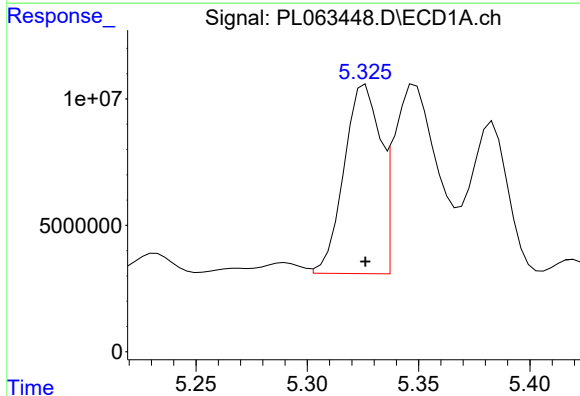


#25 Chlordane-3

R.T.: 5.326 min
Delta R.T.: 0.000 min
Response: 84119647
Conc: 485.52 ng/ml

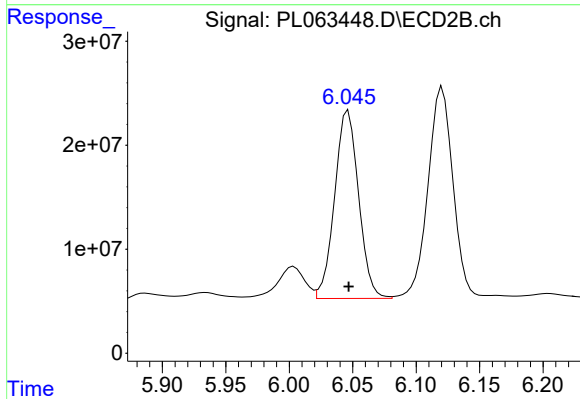

#25 Chlordane-3


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 238078252
Conc: 516.68 ng/ml

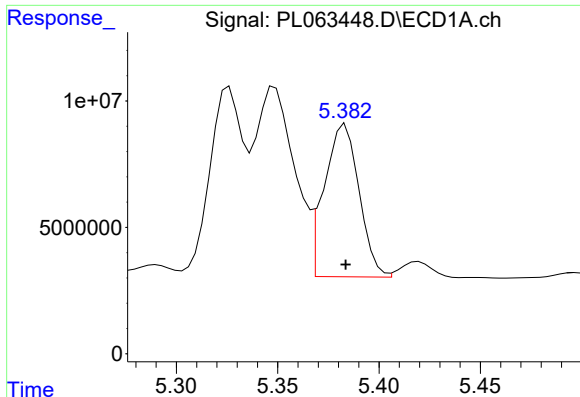

#26 Chlordane-4


R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 71976870
Conc: 492.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121120

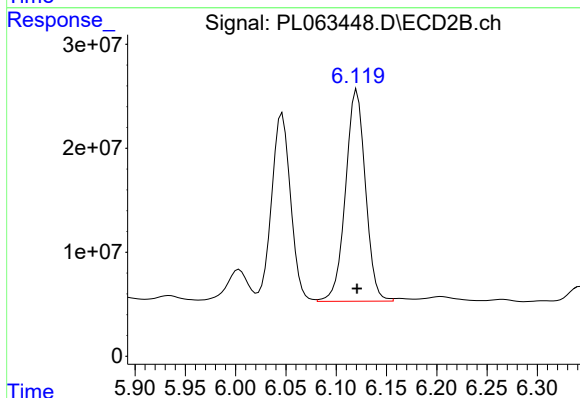


#26 Chlordane-4

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 279287661
Conc: 509.40 ng/ml

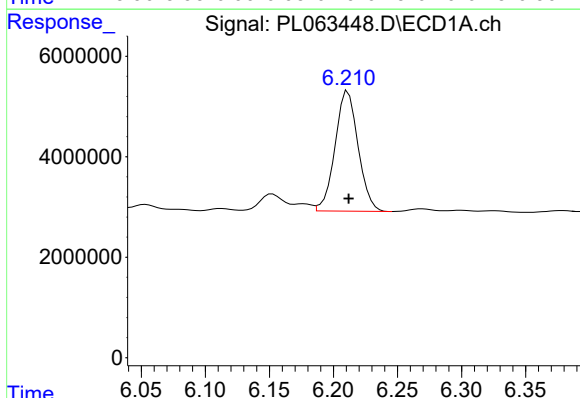


#27 Chlordane-5

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 29990161
Conc: 481.07 ng/ml

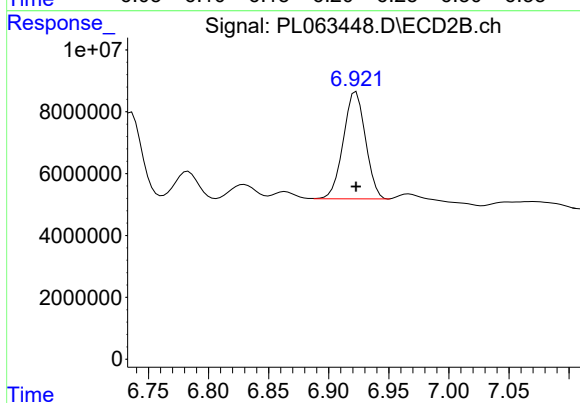

#27 Chlordane-5


R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 44504909
Conc: 490.41 ng/ml

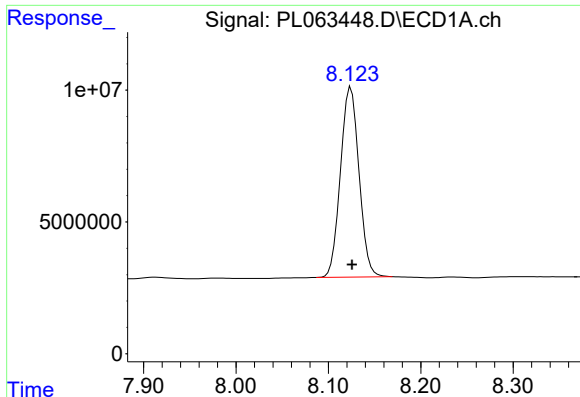

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 100652156
Conc: 48.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121120

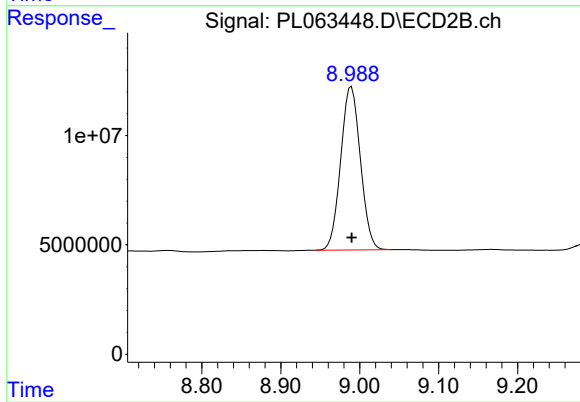

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 129531758
Conc: 48.31 ng/ml