

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
 Data File : PL063477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 17:40
 Operator : DD\AJ
 Sample : L4977-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 72-11976

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:57:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.949	23650287	41605005	13.898	13.275
28)	SA Decachlor...	8.124	8.988	28627091	37717815	14.215	14.977
Target Compounds							
10)	B gamma-Chl...	0.000	6.062	0	3735787	N.D.	1.053 #
14)	MA Endrin	0.000	6.671f	0	3546204	N.D.	1.212 #
23)	Chlordane-1	4.274	0.000	3579070	0	65.470	N.D. #
25)	Chlordane-3	0.000	6.062f	0	3735787	N.D.	8.107 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
Data File : PL063477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 17:40
Operator : DD\AJ
Sample : L4977-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
72-11976

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:57:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

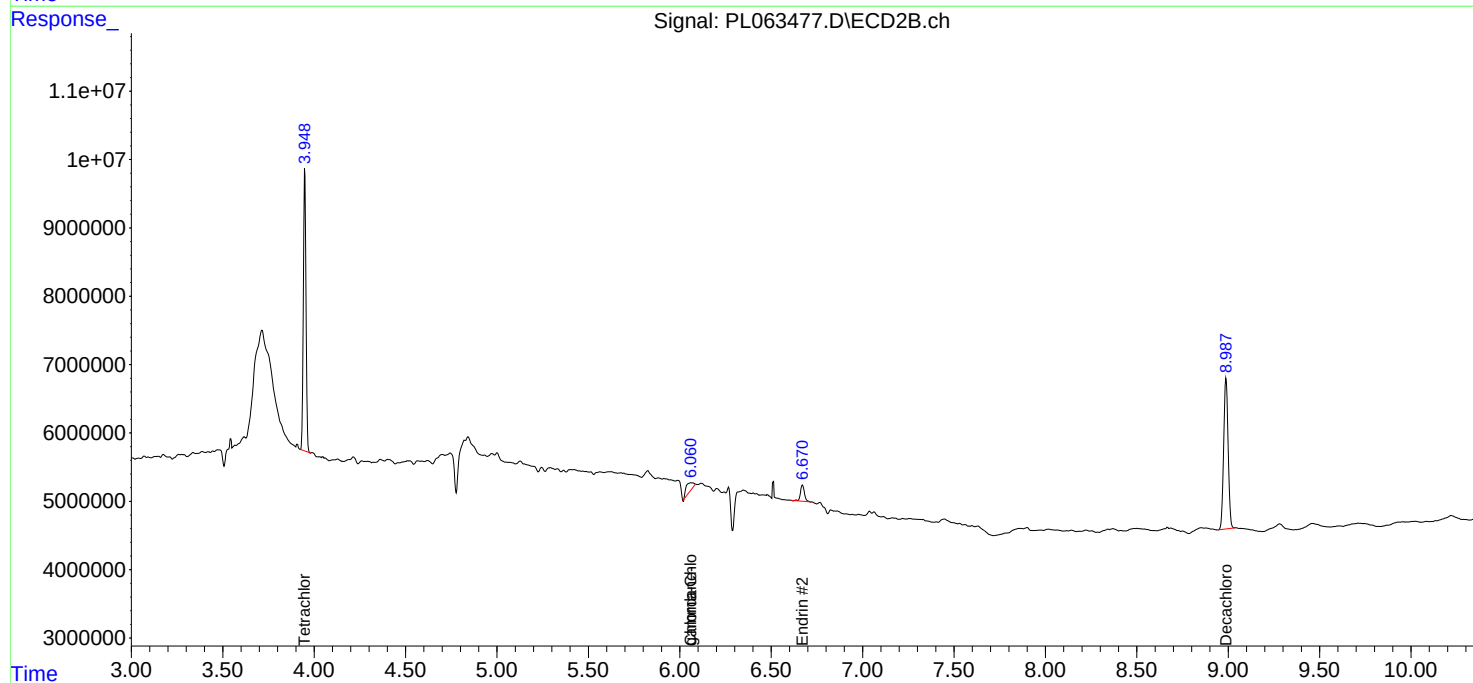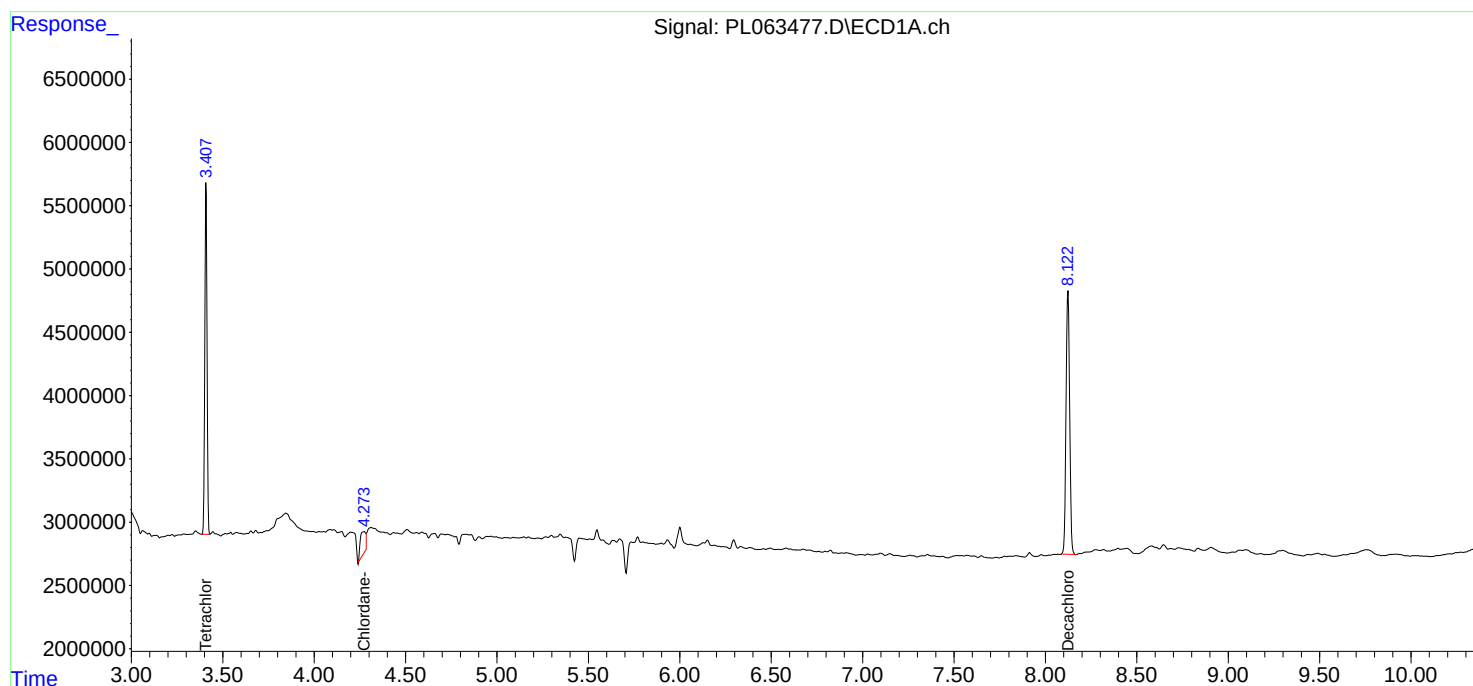


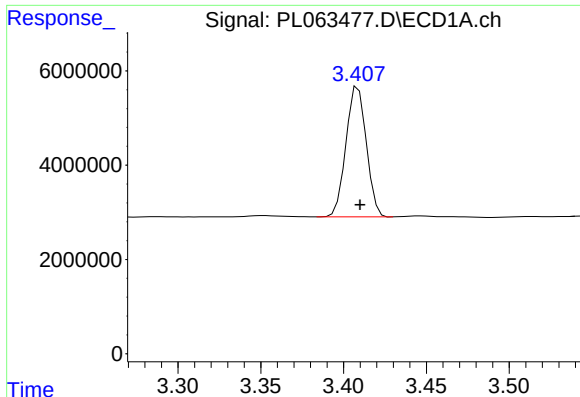

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: -0.001 min
Response: 23650287
Conc: 13.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
72-11976

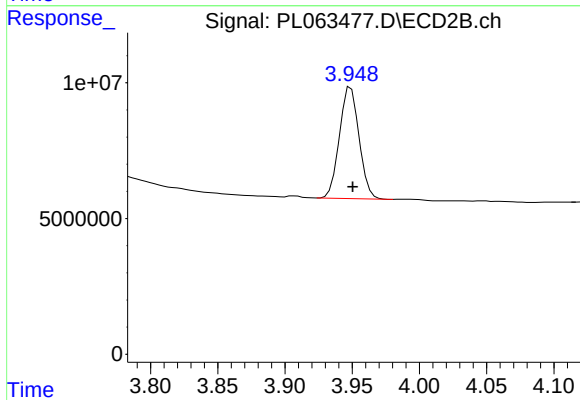


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 41605005
Conc: 13.27 ng/ml

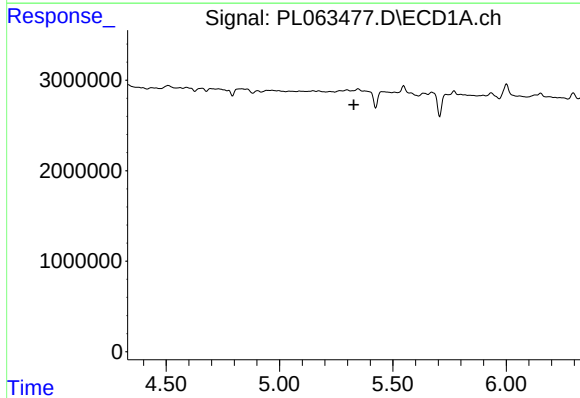


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

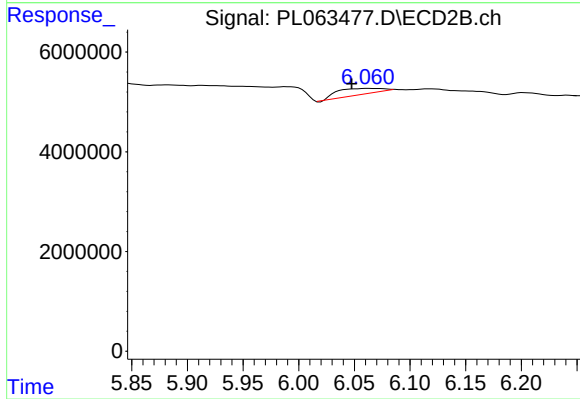

#10 gamma-Chlordane


R.T.: 6.062 min
Delta R.T.: 0.014 min
Response: 3735787
Conc: 1.05 ng/ml

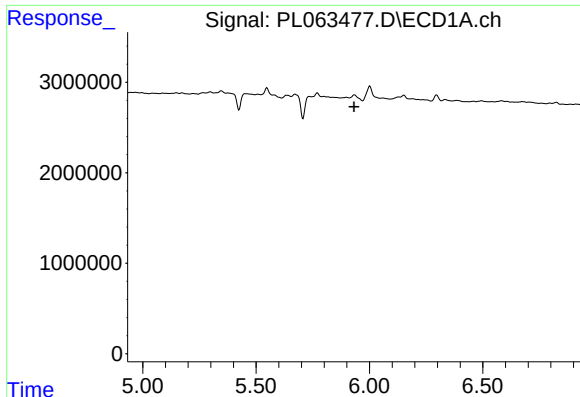

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
72-11976

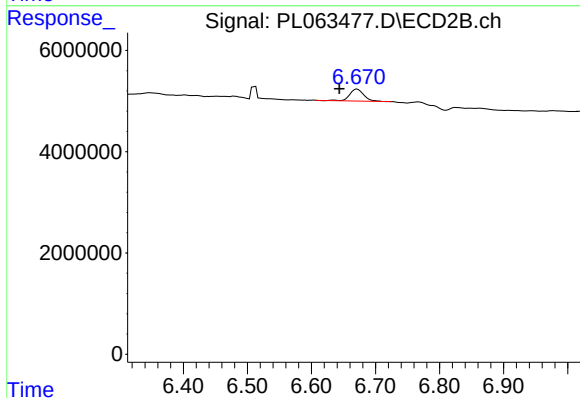


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.028 min
Response: 3546204
Conc: 1.21 ng/ml

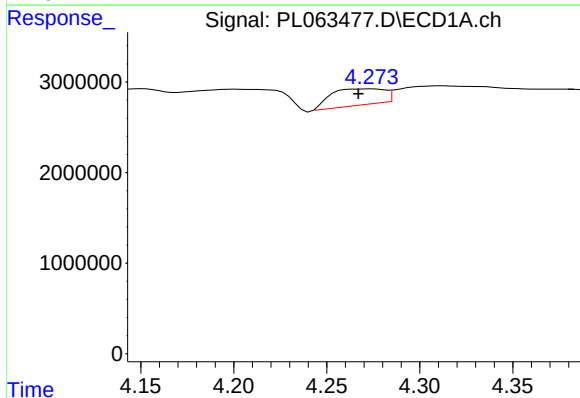


#23 Chlordane-1

R.T.: 4.274 min
Delta R.T.: 0.007 min
Response: 3579070
Conc: 65.47 ng/ml

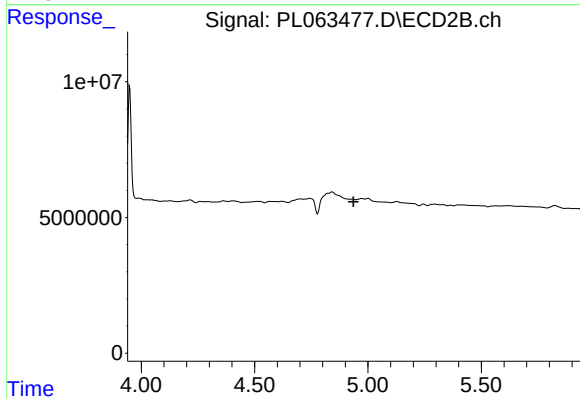

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.937 min
Response: 0
Conc: N.D.

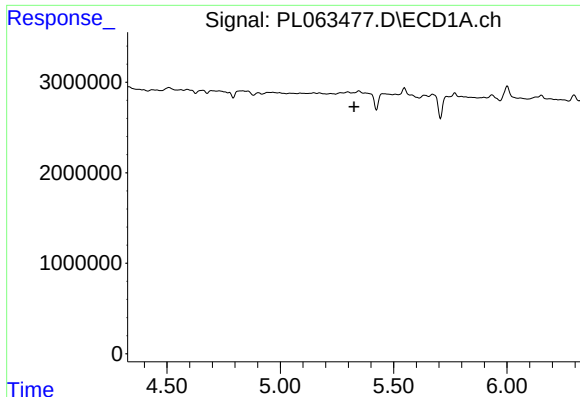

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.326 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
72-11976

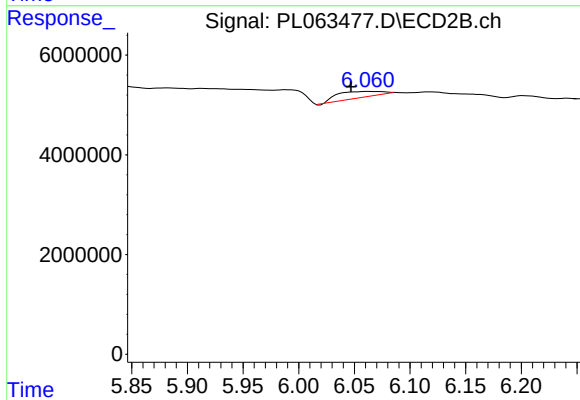


#25 Chlordane-3

R.T.: 6.062 min
Delta R.T.: 0.015 min
Response: 3735787
Conc: 8.11 ng/ml

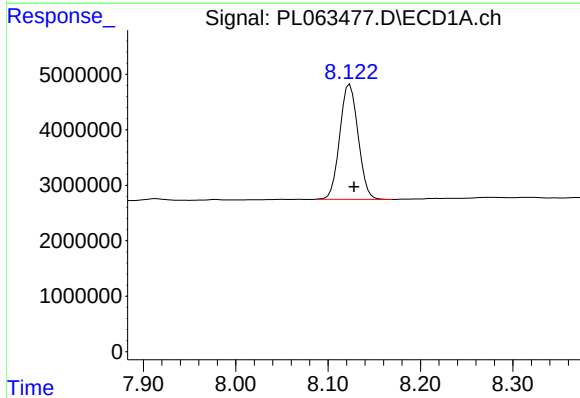

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.005 min
Response: 28627091
Conc: 14.22 ng/ml

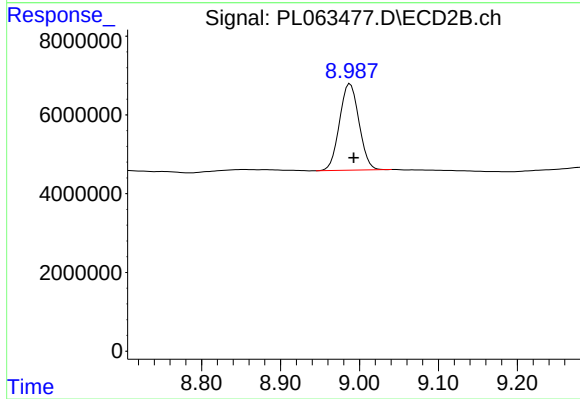

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 37717815
Conc: 14.98 ng/ml