

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
 Data File : PL063481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 18:37
 Operator : DD\AJ
 Sample : L4983-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR1-A-D-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:58:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.949	34001518	63797246	19.981	20.355
28)	SA Decachlor...	8.124	8.988	38475364	49424130	19.105	19.626
Target Compounds							
7)	B delta-BHC	0.000	5.002	0	4826429	N.D.	1.193 #
10)	B gamma-Chl...	0.000	6.040	0	5685969	N.D.	1.602 #
14)	MA Endrin	5.938	0.000	7211668	0	4.297	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	3056871	N.D.	0.960 #
19)	B Endosulfa...	6.600f	0.000	43691471	0	25.477	N.D. #
25)	Chlordane-3	0.000	6.040	0	5685969	N.D.	12.340 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
Data File : PL063481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 18:37
Operator : DD\AJ
Sample : L4983-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:58:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

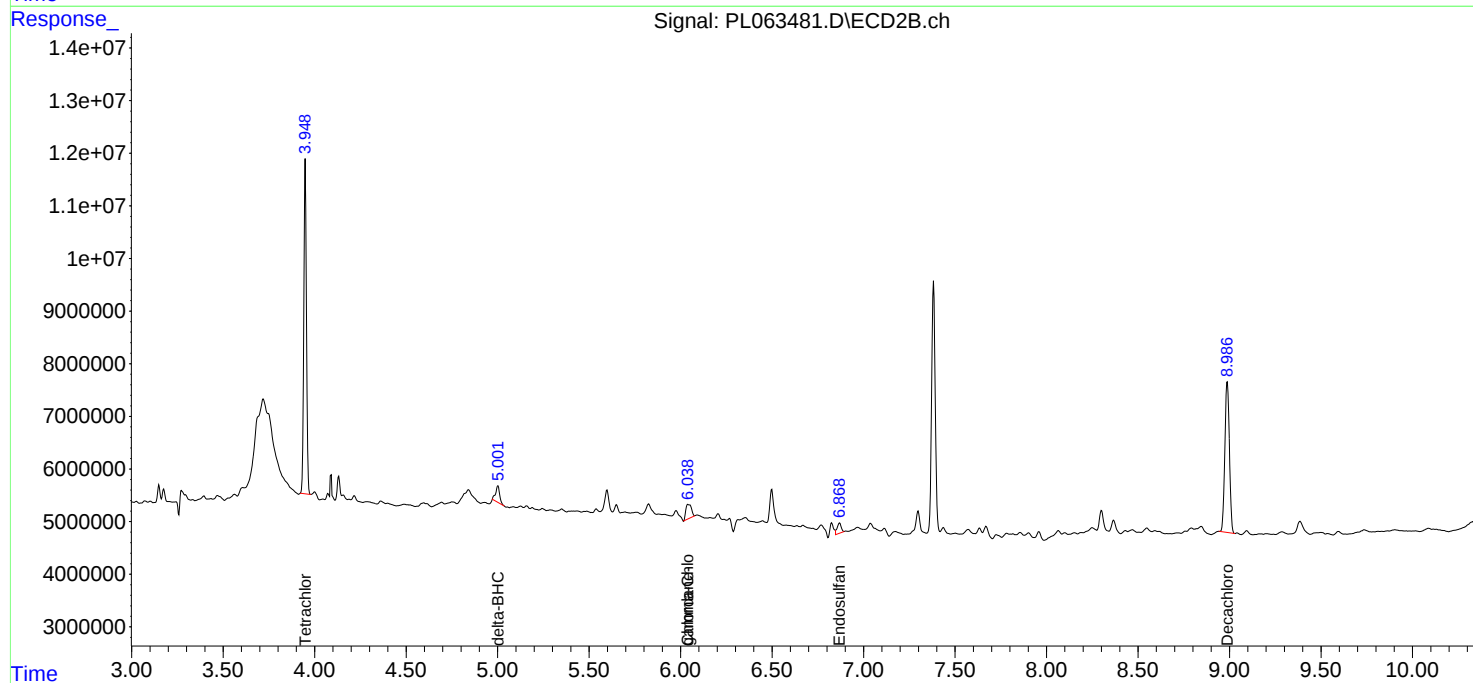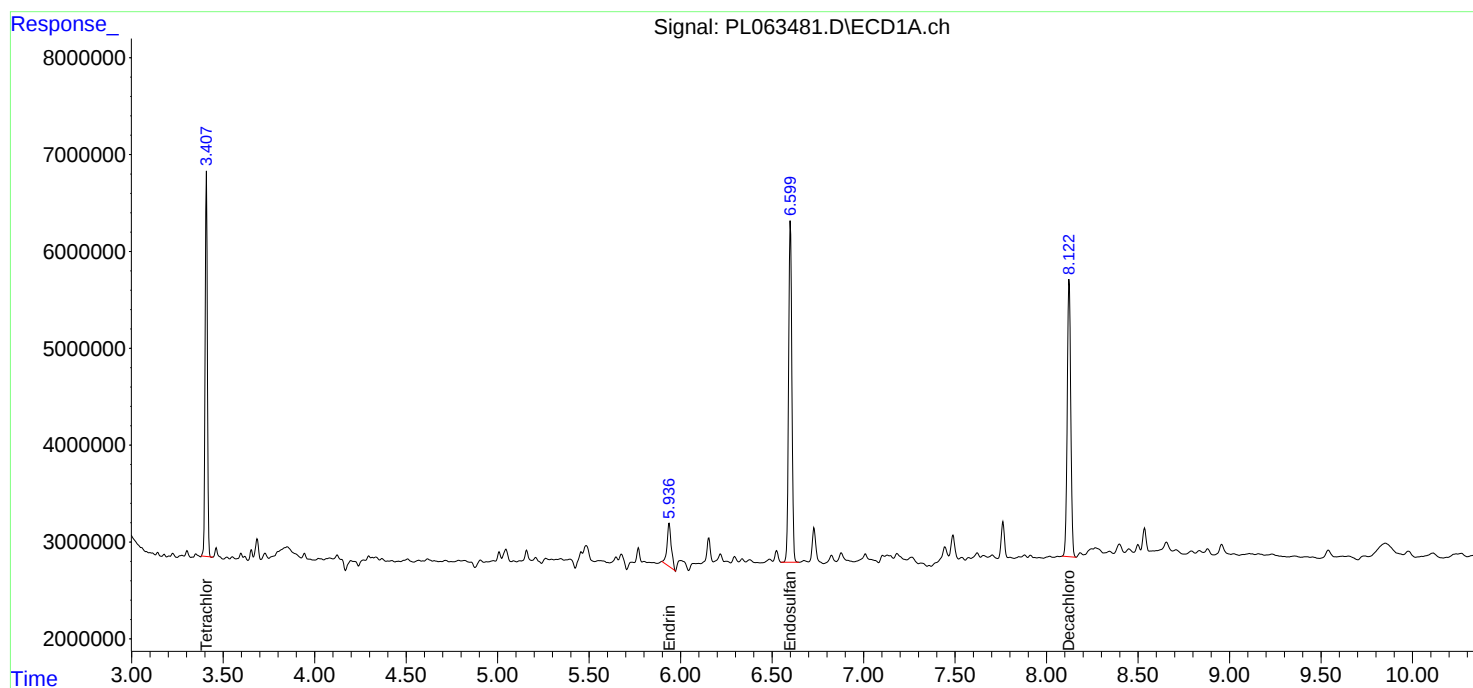


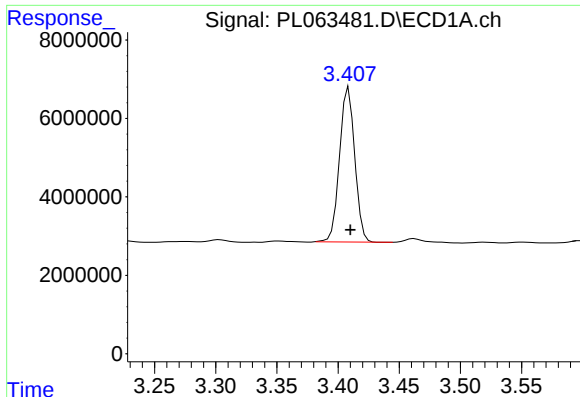

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: -0.001 min
Response: 34001518
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP

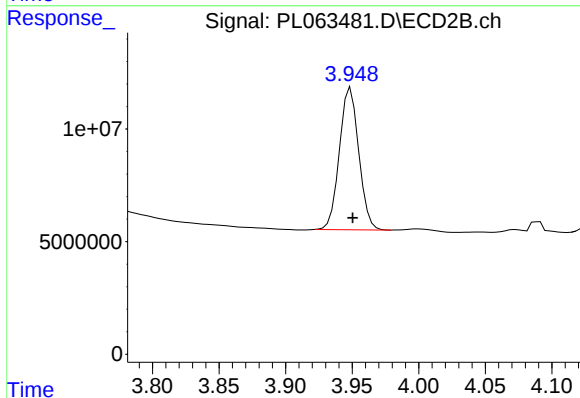


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 63797246
Conc: 20.36 ng/ml

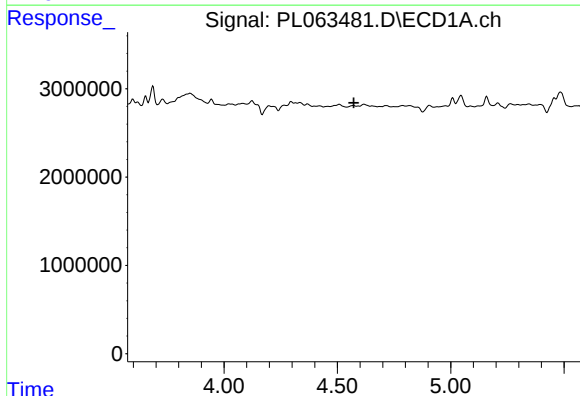


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

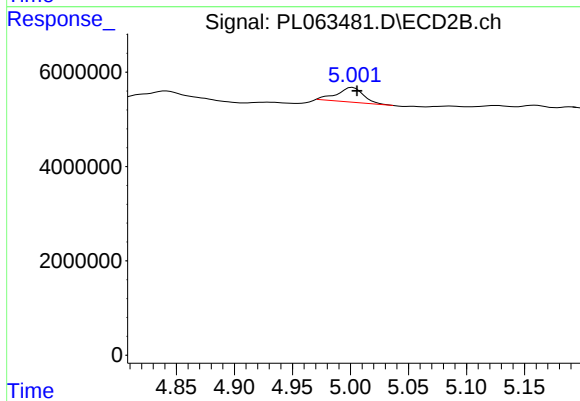

#7 delta-BHC


R.T.: 5.002 min
Delta R.T.: -0.004 min
Response: 4826429
Conc: 1.19 ng/ml

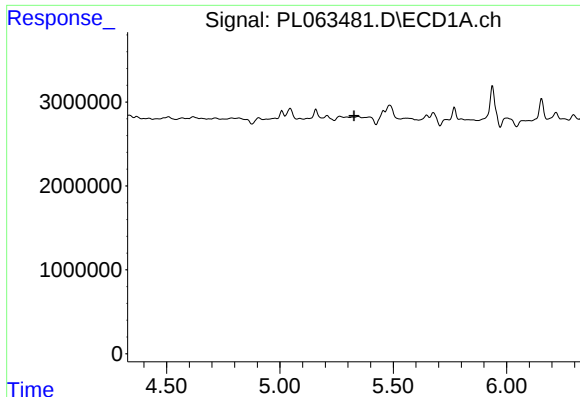

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP

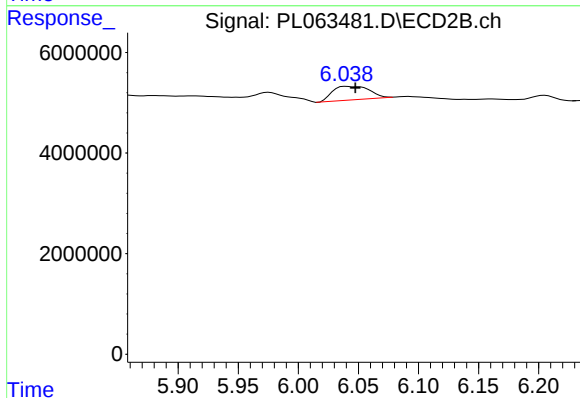


#10 gamma-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.008 min
Response: 5685969
Conc: 1.60 ng/ml

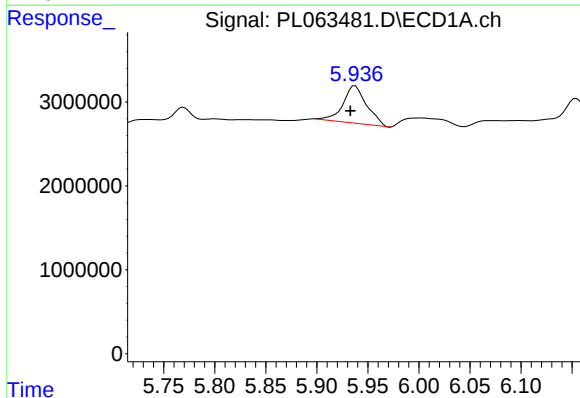


#14 Endrin

R.T.: 5.938 min
Delta R.T.: 0.005 min
Response: 7211668
Conc: 4.30 ng/ml

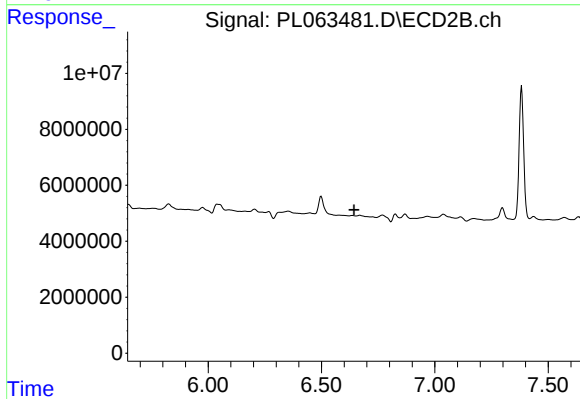

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.643 min
Response: 0
Conc: N.D.

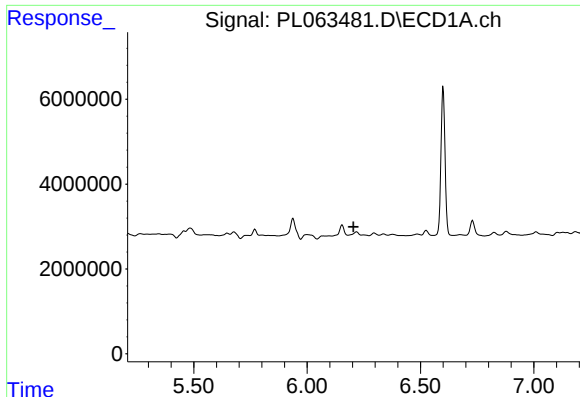

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP

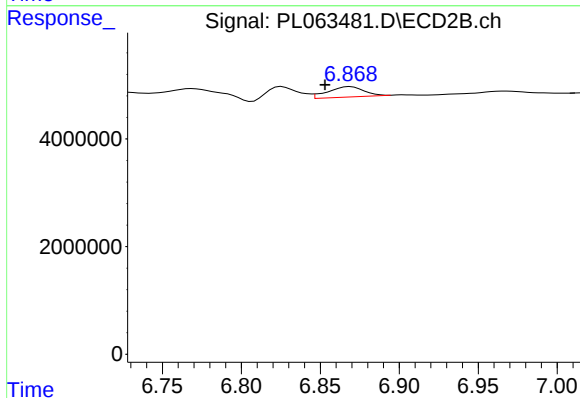


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 3056871
Conc: 0.96 ng/ml

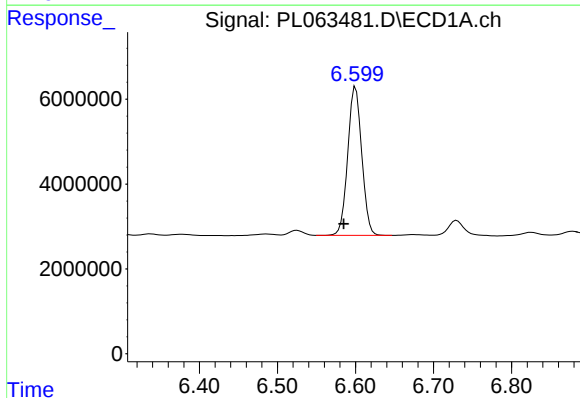


#19 Endosulfan Sulfate

R.T.: 6.600 min
Delta R.T.: 0.015 min
Response: 43691471
Conc: 25.48 ng/ml

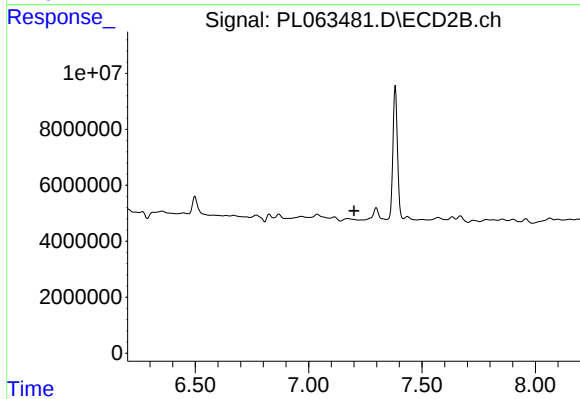

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.201 min
Response: 0
Conc: N.D.

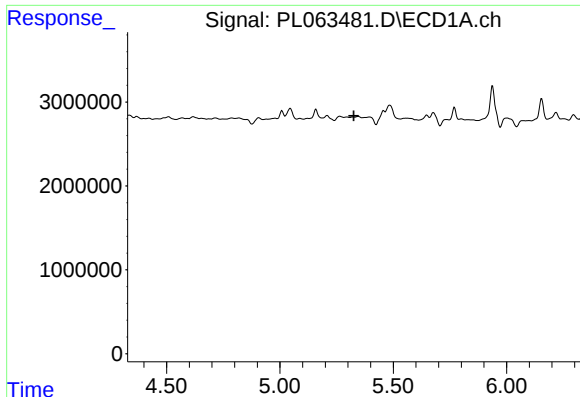

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.326 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP

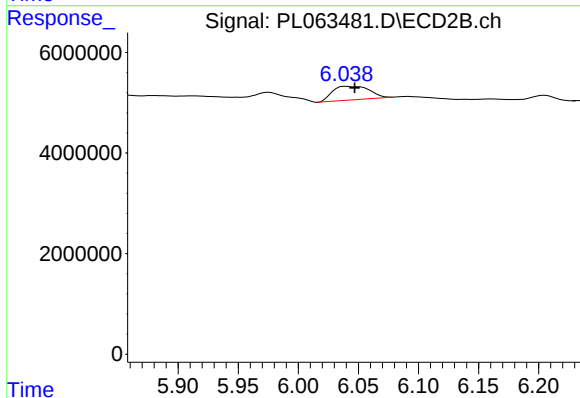


#25 Chlordane-3

R.T.: 6.040 min
Delta R.T.: -0.007 min
Response: 5685969
Conc: 12.34 ng/ml

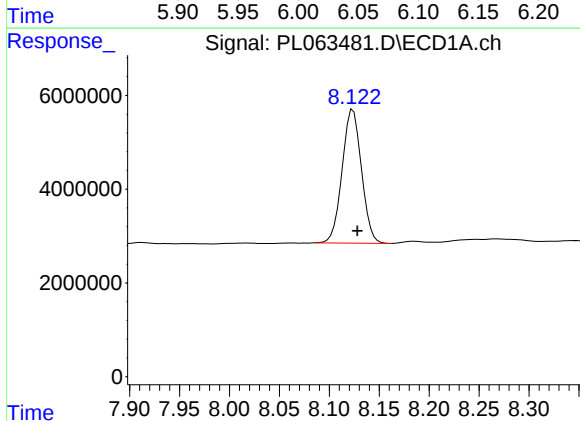

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 38475364
Conc: 19.11 ng/ml

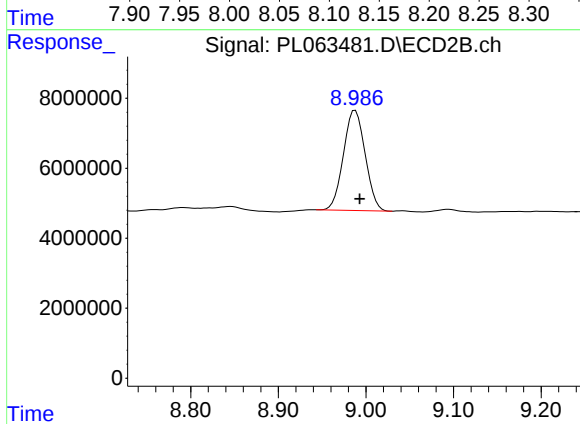

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 49424130
Conc: 19.63 ng/ml