

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
 Data File : PL063482.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 18:51
 Operator : DD\AJ
 Sample : L4283-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 L4283-12

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:58:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.949	35951083	66468620	21.126	21.208
28)	SA Decachlor...	8.124	8.988	39935437	51580235	19.830	20.482
Target Compounds							
12)	B 4,4'-DDE	5.547	6.275	2403977	5488508	1.415	1.567
15)	B Endosulfa...	0.000	6.869f	0	14786388	N.D.	4.642 #
17)	MA 4,4'-DDT	6.296	7.064	5503300	6343336	4.010	2.481 #
18)	B Endrin al...	0.000	6.949f	0	3456814	N.D.	1.355 #
19)	B Endosulfa...	6.601f	0.000	11326976	0	6.605	N.D. #
27)	Chlordane-5	0.000	6.949f	0	3456814	N.D.	38.091 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
Data File : PL063482.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 18:51
Operator : DD\AJ
Sample : L4283-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
L4283-12

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:58:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

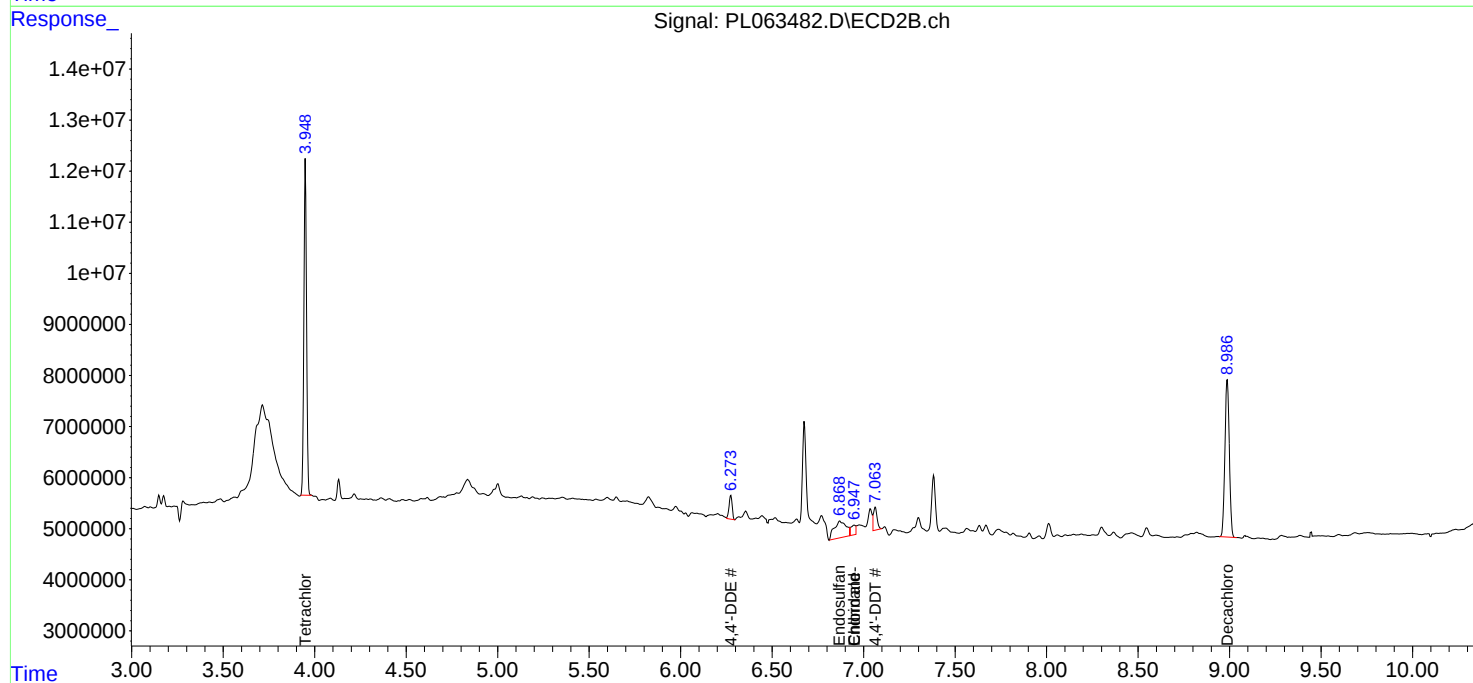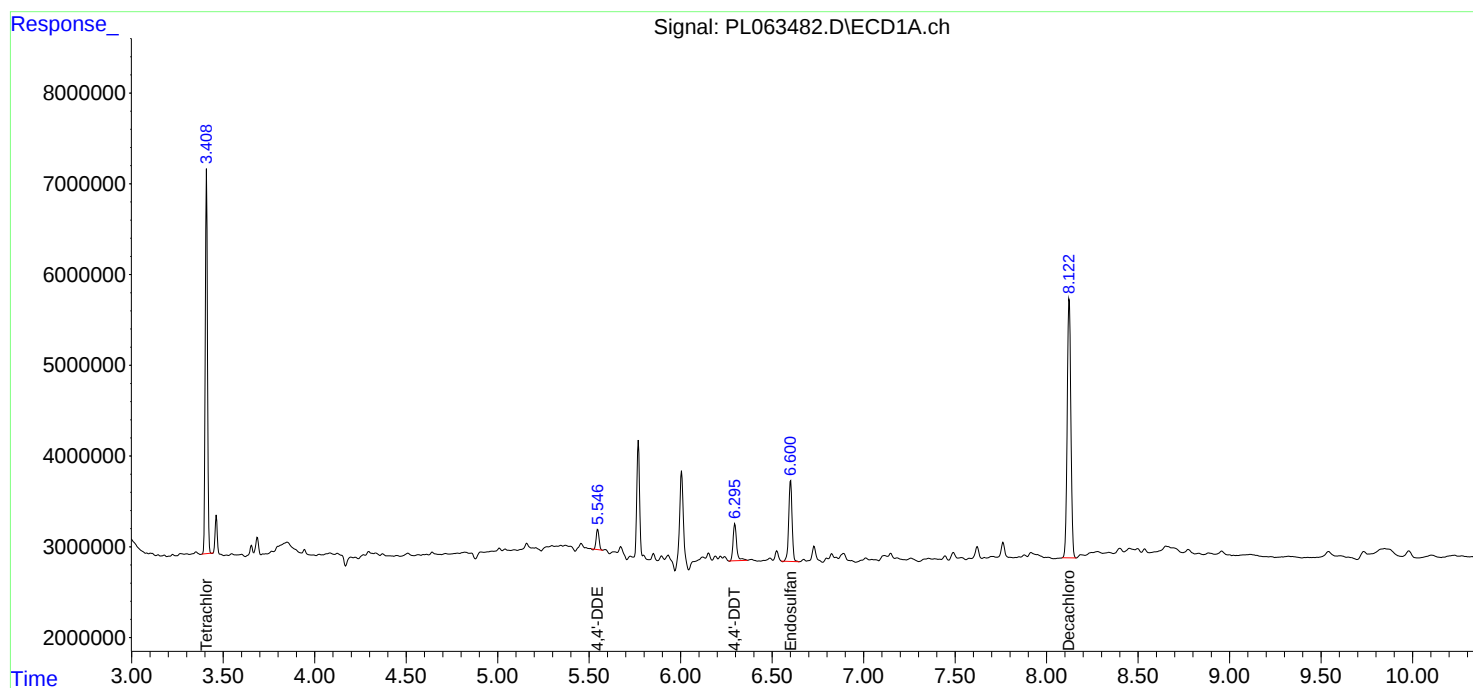


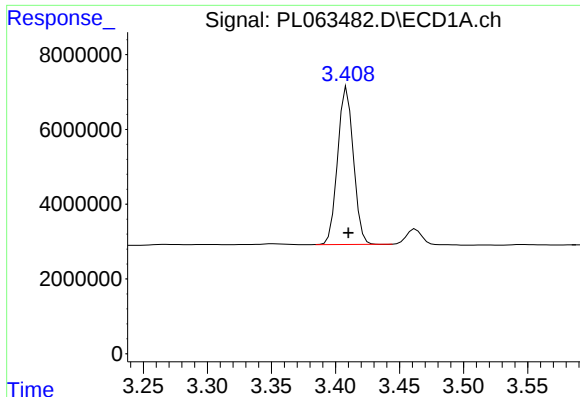

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 35951083
Conc: 21.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
L4283-12

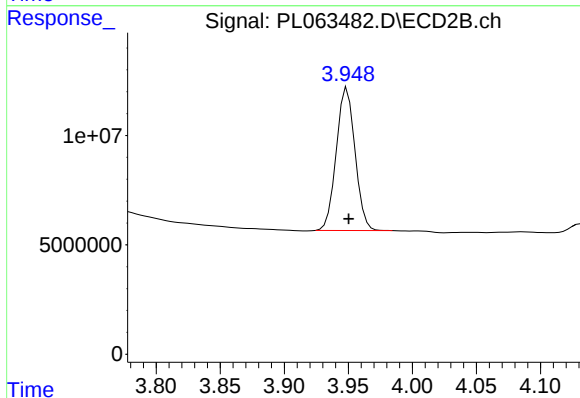


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 66468620
Conc: 21.21 ng/ml

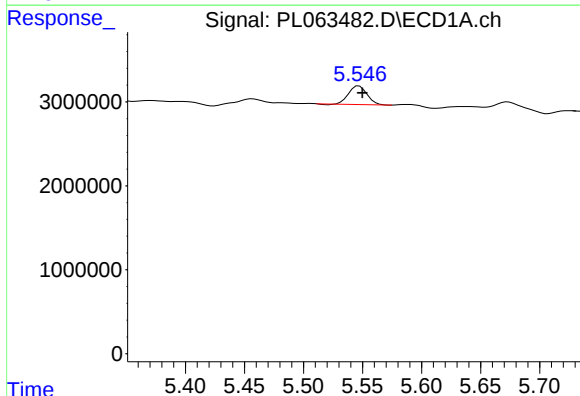


#12 4,4'-DDE

R.T.: 5.547 min
Delta R.T.: -0.003 min
Response: 2403977
Conc: 1.42 ng/ml

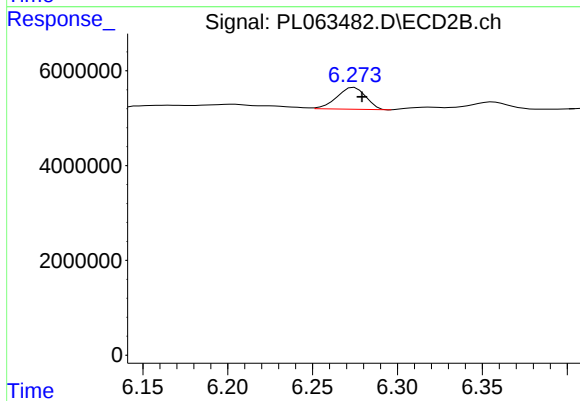

#12 4,4'-DDE


R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 5488508
Conc: 1.57 ng/ml

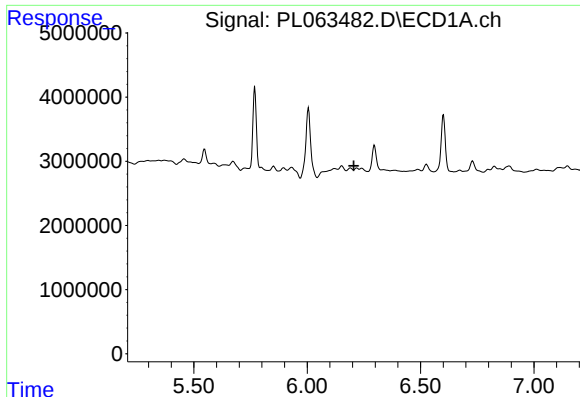

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L4283-12

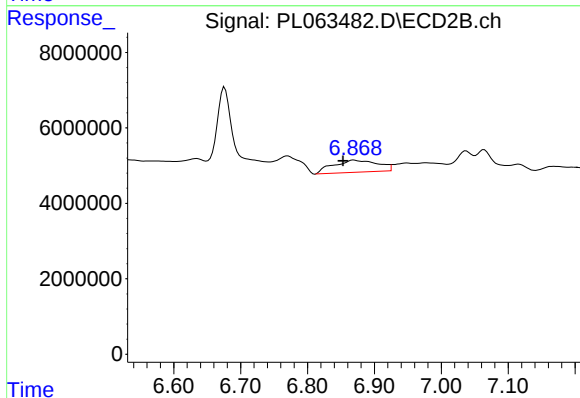


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 14786388
Conc: 4.64 ng/ml

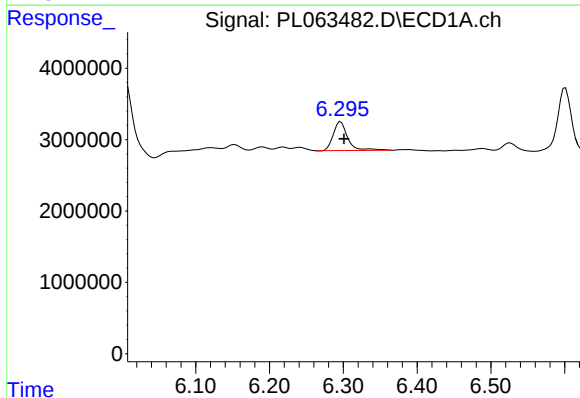


#17 4,4'-DDT

R.T.: 6.296 min
Delta R.T.: -0.005 min
Response: 5503300
Conc: 4.01 ng/ml

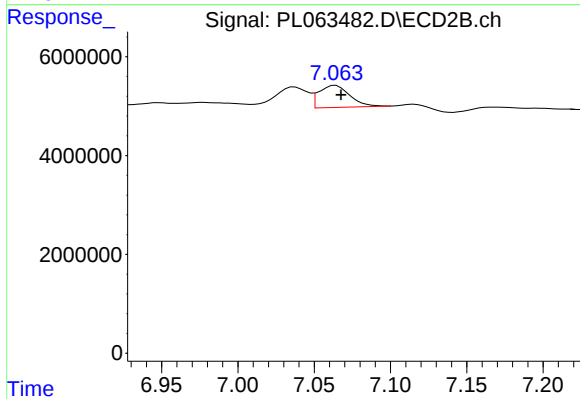

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: -0.004 min
Response: 6343336
Conc: 2.48 ng/ml

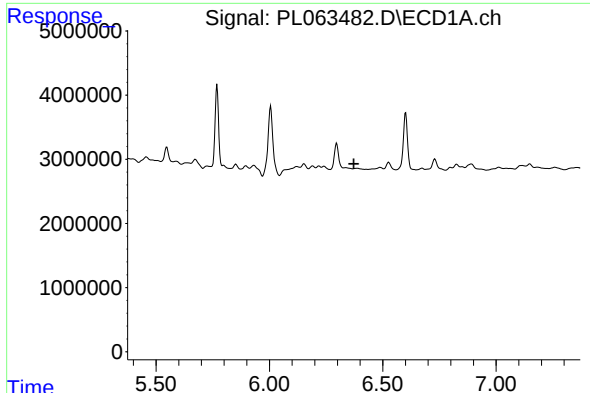

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L4283-12

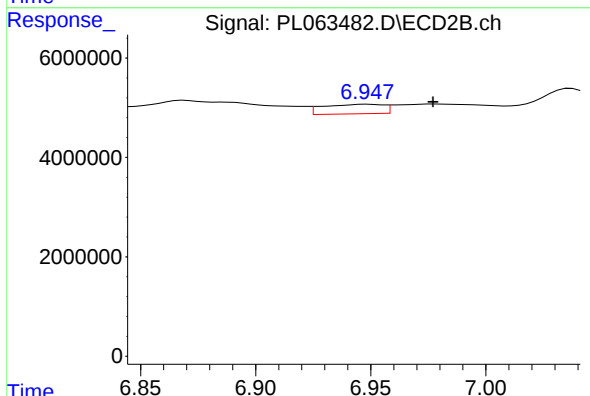


#18 Endrin aldehyde

R.T.: 6.949 min
Delta R.T.: -0.028 min
Response: 3456814
Conc: 1.35 ng/ml

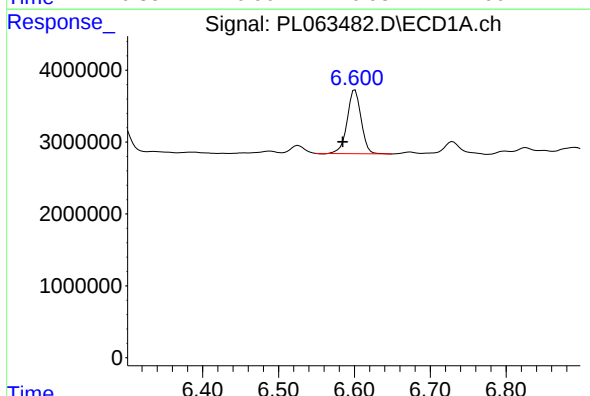


#19 Endosulfan Sulfate

R.T.: 6.601 min
Delta R.T.: 0.016 min
Response: 11326976
Conc: 6.60 ng/ml

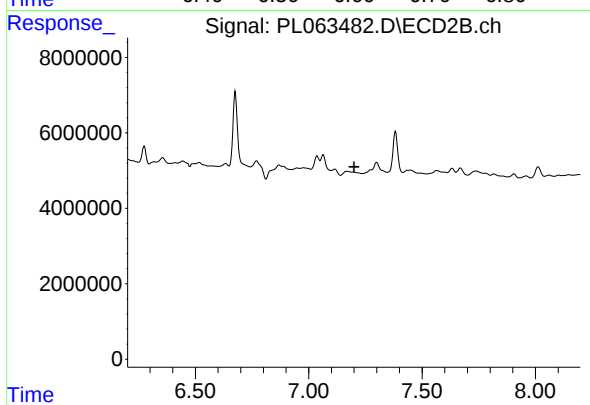

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.201 min
Response: 0
Conc: N.D.

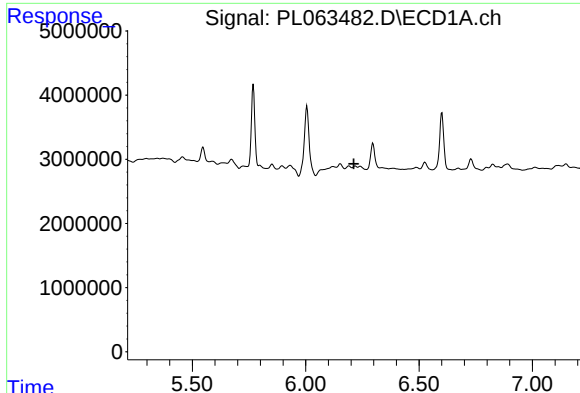

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
L4283-12

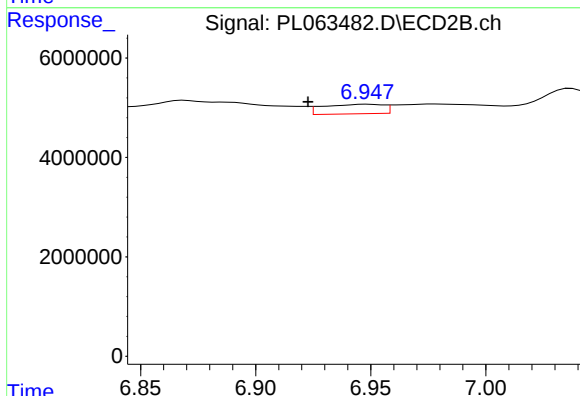


#27 Chlordane-5

R.T.: 6.949 min
Delta R.T.: 0.026 min
Response: 3456814
Conc: 38.09 ng/ml

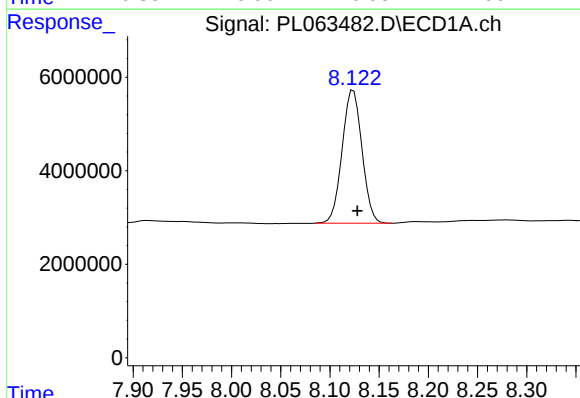

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 39935437
Conc: 19.83 ng/ml

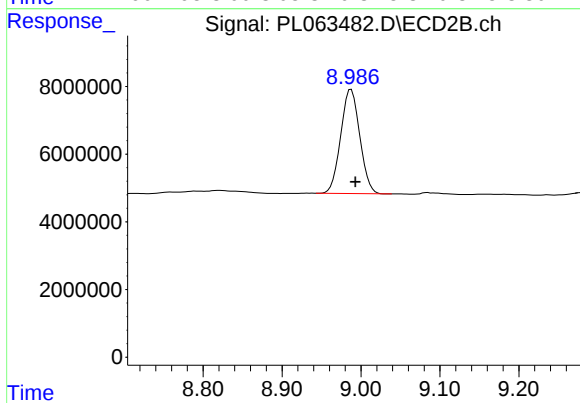

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 51580235
Conc: 20.48 ng/ml