

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
 Data File : PL063452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 11:42
 Operator : DD\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 12:14:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 10:28:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.408	3.949	94901732	157.0E6	55.768	50.104
28)	SA Decachlor...	8.124	8.989	96836396	124.2E6	48.085	49.325
Target Compounds							
23)	Chlordane-1	4.266	4.936	25775316	55217975	471.492	481.253
24)	Chlordane-2	4.763	5.402	28937625	68107539	460.844	539.660
25)	Chlordane-3	5.326	6.046	79313795	231.8E6	457.780	502.998
26)	Chlordane-4	5.383	6.120	66868681	269.1E6	457.146	490.781
27)	Chlordane-5	6.211	6.922	27845342	41905728	446.661	461.764



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121120\
Data File : PL063452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 11:42
Operator : DD\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 12:14:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 10:28:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

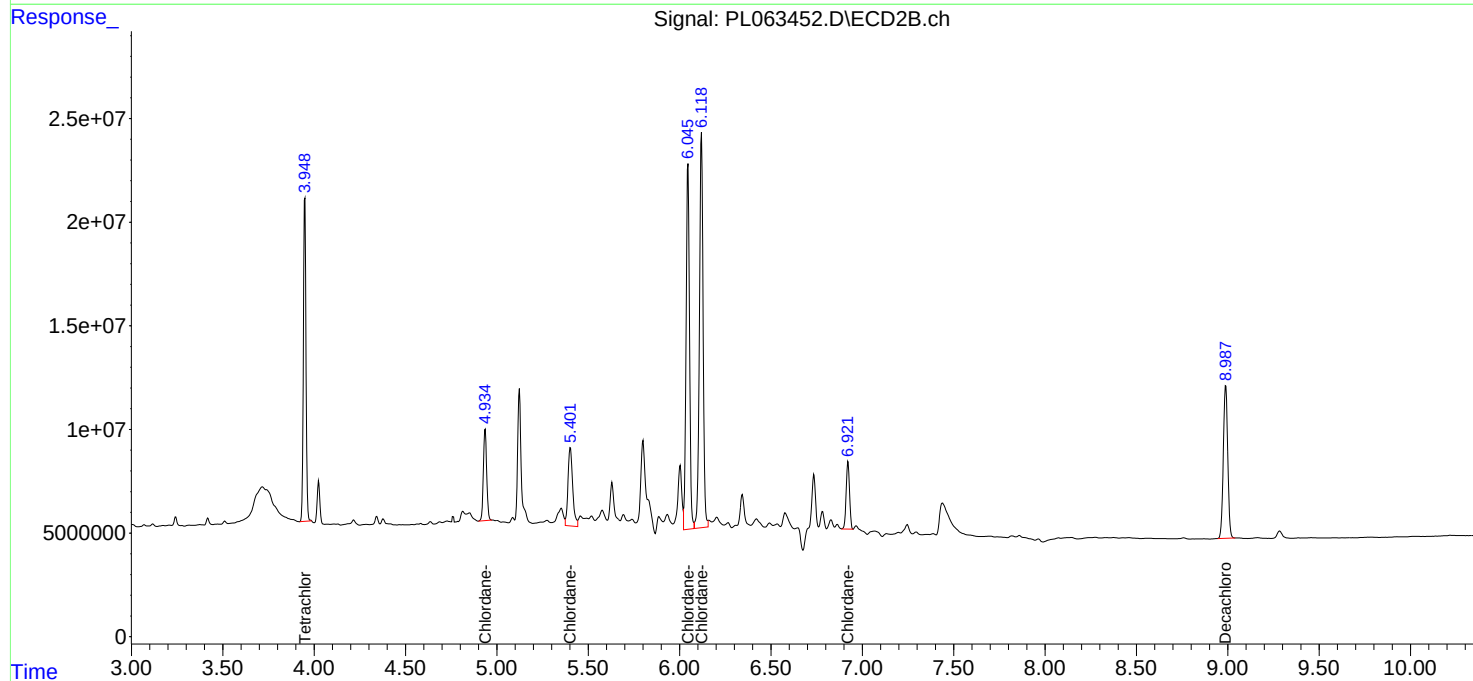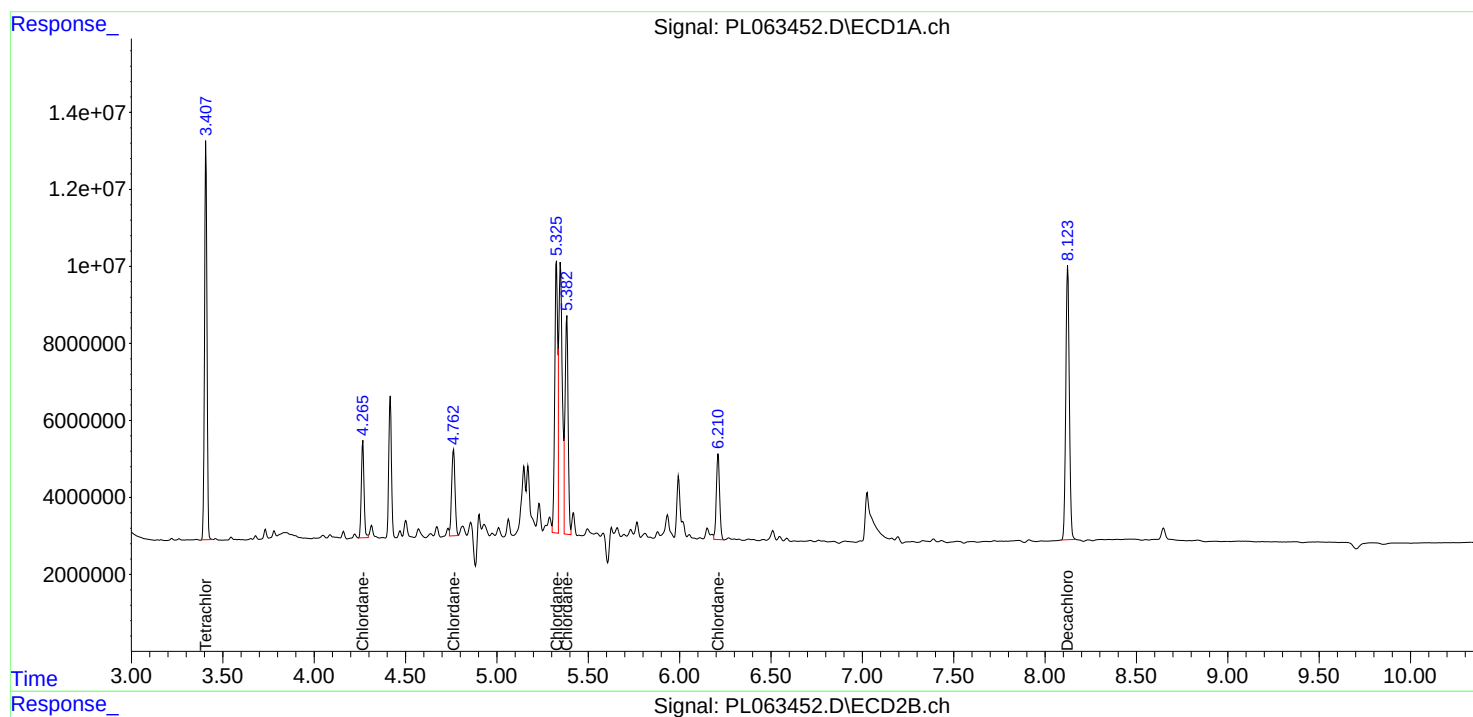


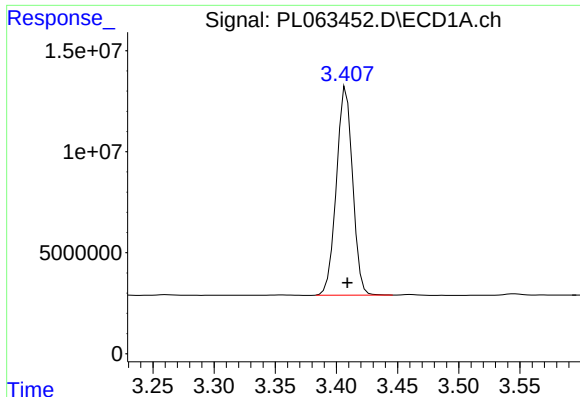

#1 Tetrachloro-m-xylene


R.T.: 3.408 min
Delta R.T.: 0.000 min
Response: 94901732
Conc: 55.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

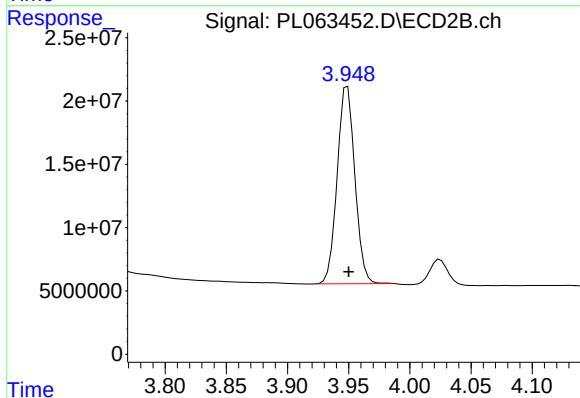


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 157036046
Conc: 50.10 ng/ml

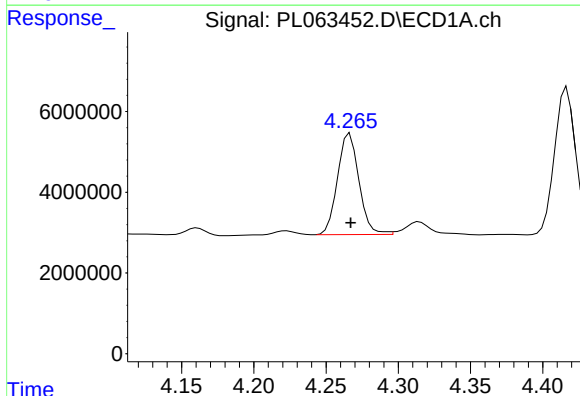


#23 Chlordane-1

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 25775316
Conc: 471.49 ng/ml

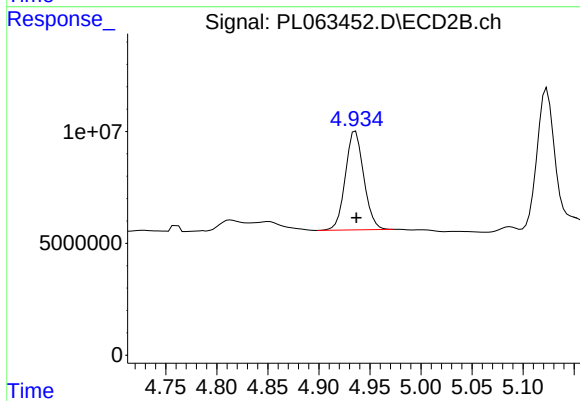

#23 Chlordane-1


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 55217975
Conc: 481.25 ng/ml

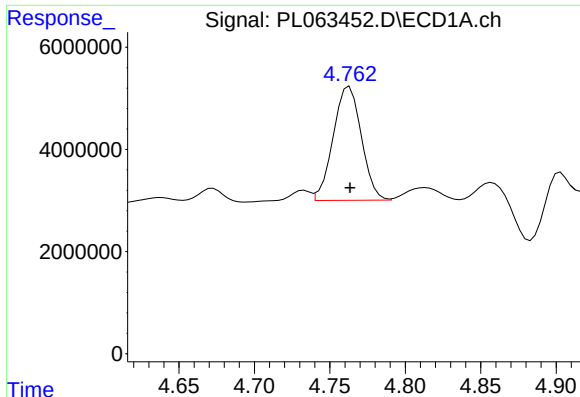

#24 Chlordane-2


R.T.: 4.763 min
Delta R.T.: 0.000 min
Response: 28937625
Conc: 460.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

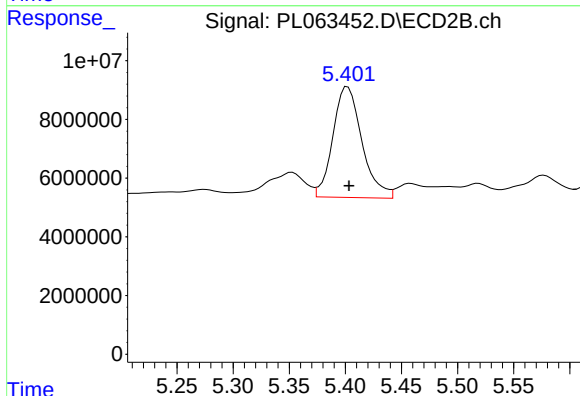


#24 Chlordane-2

R.T.: 5.402 min
Delta R.T.: -0.001 min
Response: 68107539
Conc: 539.66 ng/ml

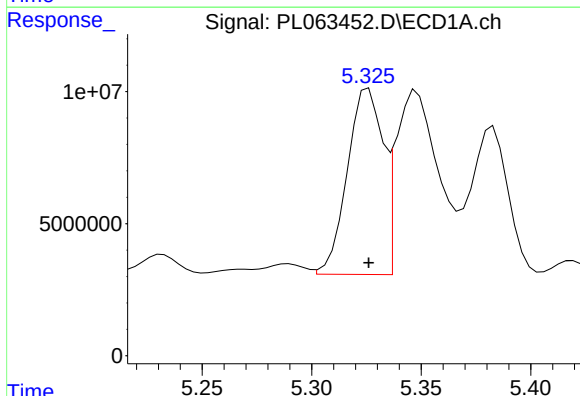


#25 Chlordane-3

R.T.: 5.326 min
Delta R.T.: 0.000 min
Response: 79313795
Conc: 457.78 ng/ml

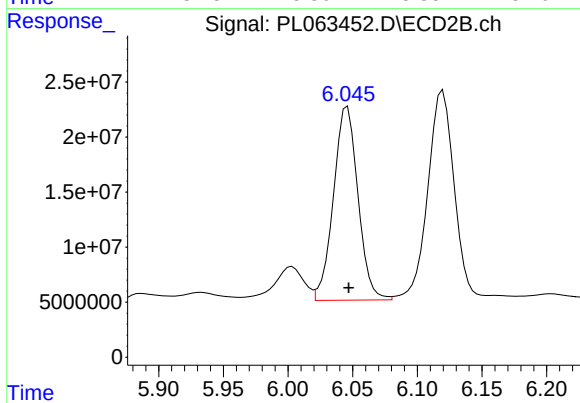

#25 Chlordane-3


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 231773082
Conc: 503.00 ng/ml

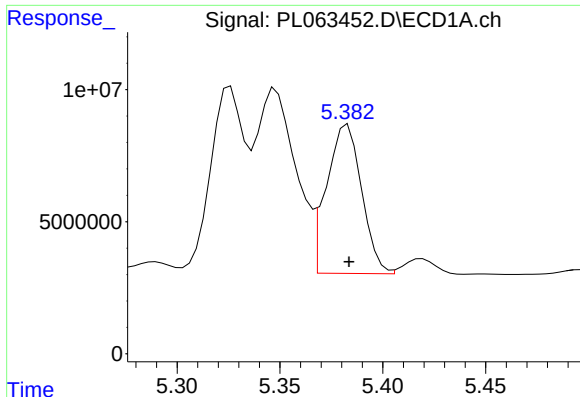

#26 Chlordane-4


R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 66868681
Conc: 457.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

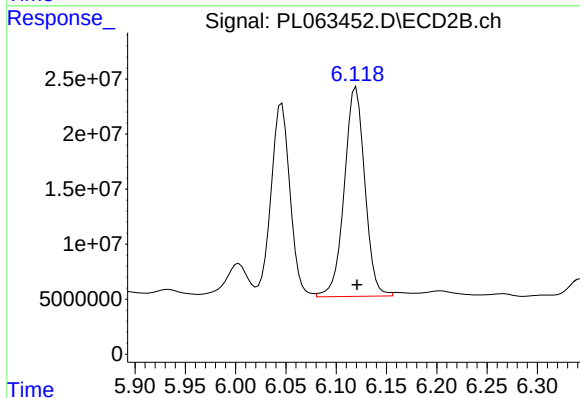


#26 Chlordane-4

R.T.: 6.120 min
Delta R.T.: -0.001 min
Response: 269080418
Conc: 490.78 ng/ml

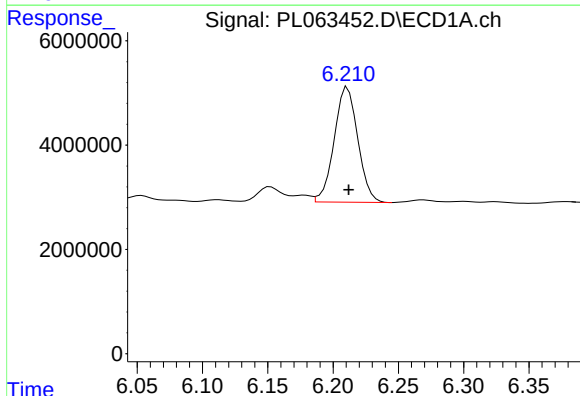


#27 Chlordane-5

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 27845342
Conc: 446.66 ng/ml

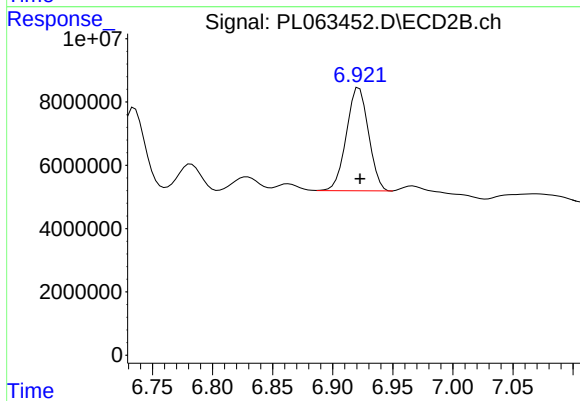

#27 Chlordane-5


R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 41905728
Conc: 461.76 ng/ml

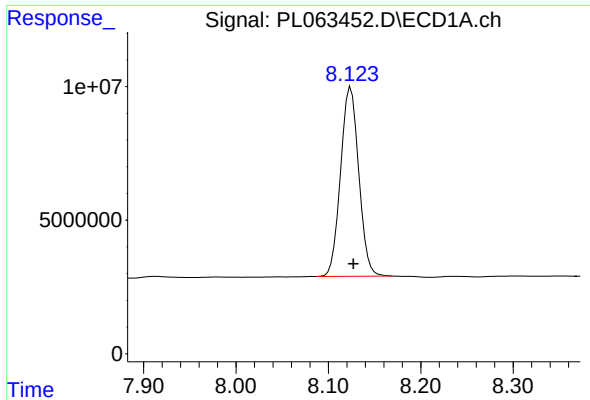

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.003 min
Response: 96836396
Conc: 48.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

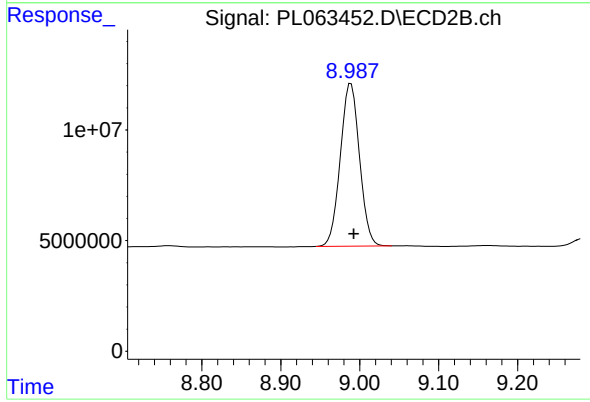

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 124216827
Conc: 49.32 ng/ml