

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121124\
 Data File : PL093375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2024 16:40
 Operator : AR\AJ
 Sample : P5220-03 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GAS-AUD-1610-1611-1612

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/12/2024
 Supervised By :Ankita Jodhani 12/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 02:06:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.531	2.773	11727434	6471587	4.512	2.244 #
28) SA Decachlor...	9.059	7.914	2285391	3039998	1.315m	1.064m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121124\
Data File : PL093375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2024 16:40
Operator : AR\AJ
Sample : P5220-03 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GAS-AUD-1610-1611-1612


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/12/2024
Supervised By : Ankita Jodhani 12/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 02:06:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

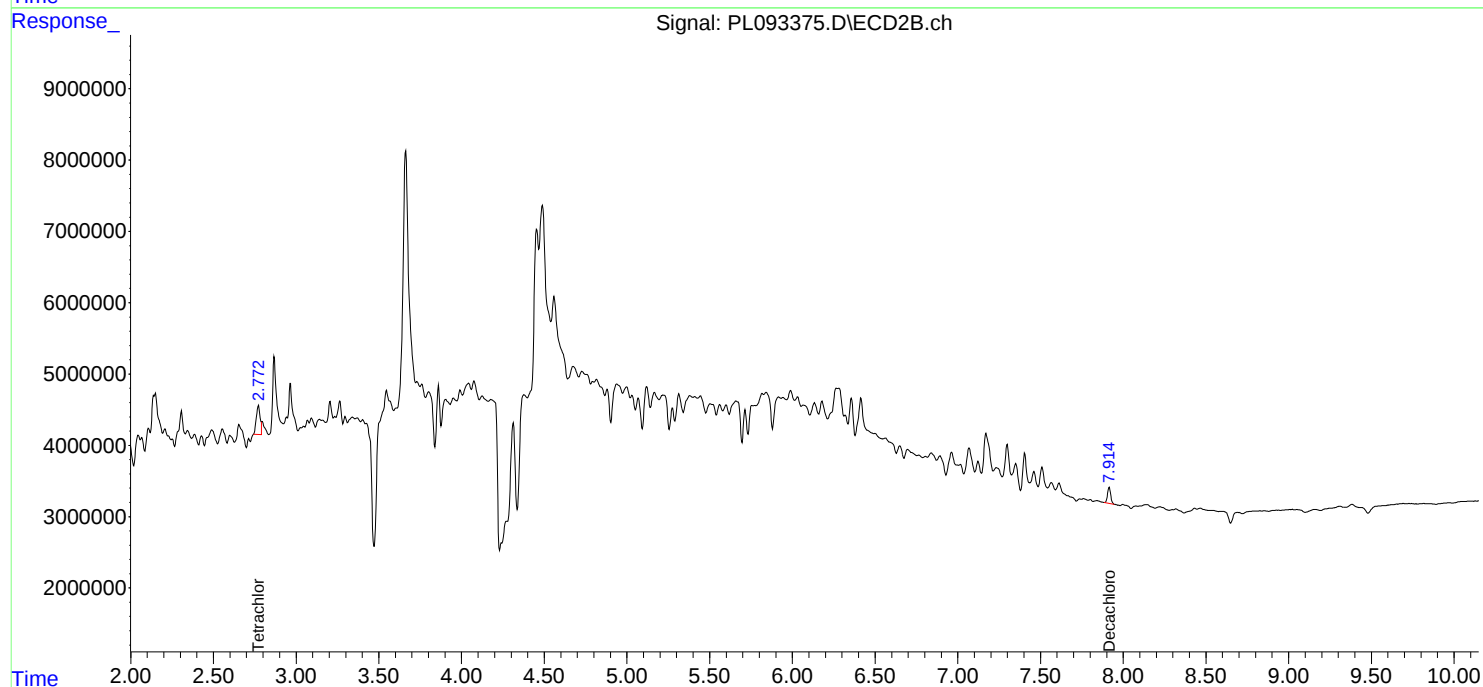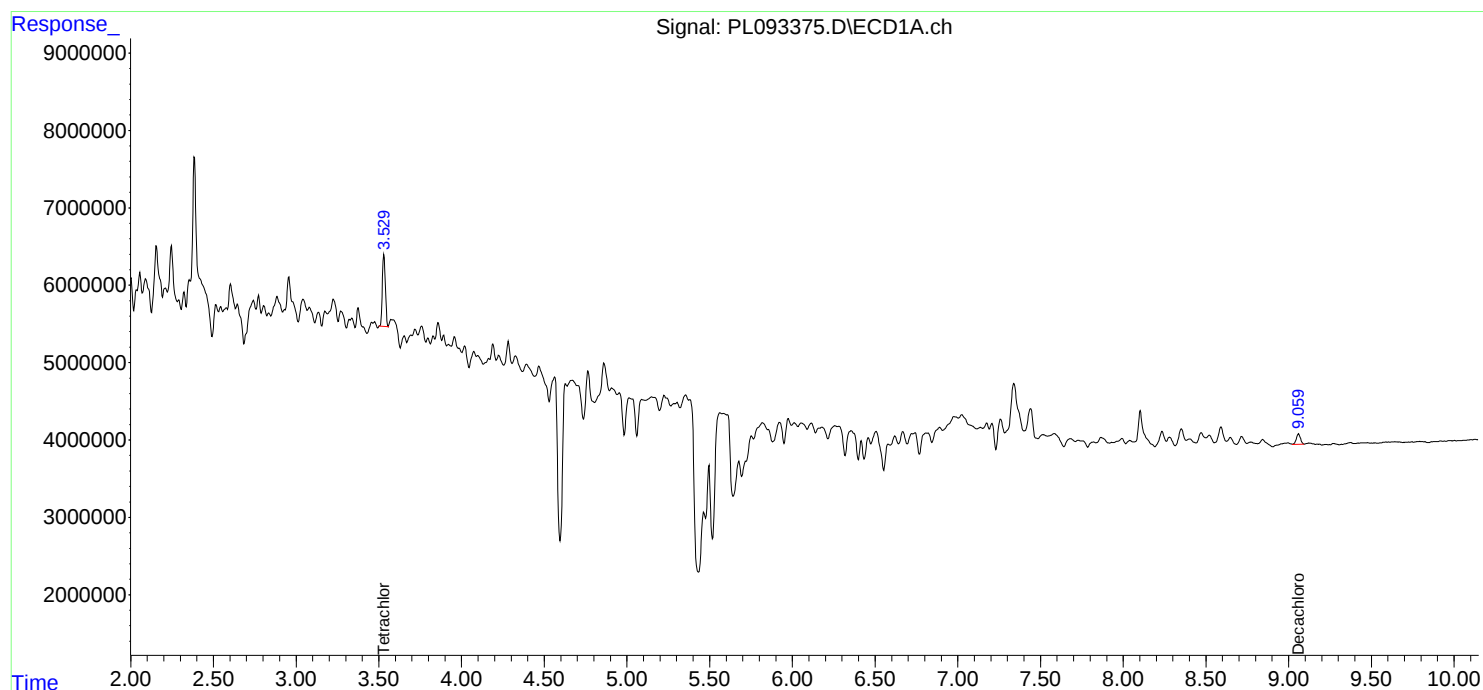

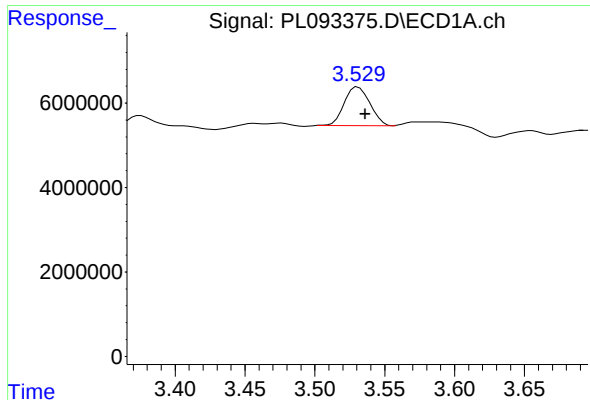


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: -0.005 min
Response: 11727434
Conc: 4.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
GAS-AUD-1610-1611-1612


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2024
Supervised By :Ankita Jodhani 12/12/2024

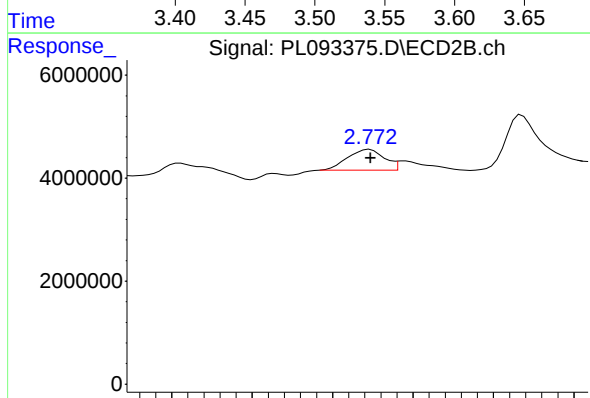


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 6471587
Conc: 2.24 ng/ml

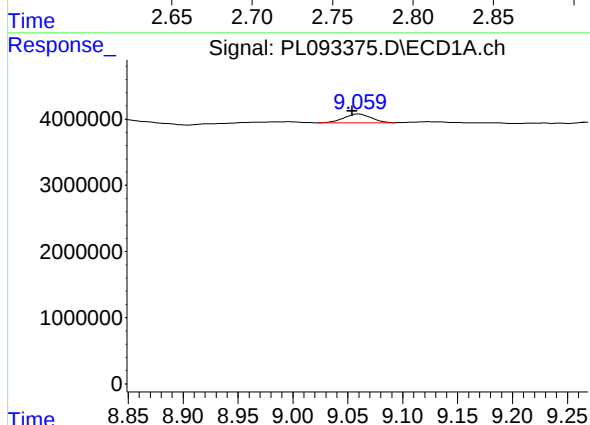

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.005 min
Response: 2285391
Conc: 1.31 ng/ml m

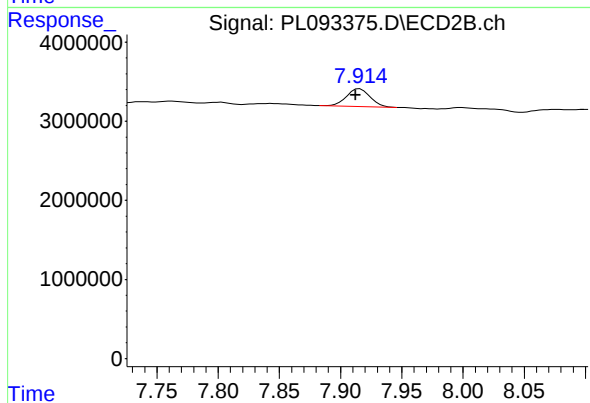

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.002 min
Response: 3039998
Conc: 1.06 ng/ml m