

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121125\
 Data File : PL097842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2025 17:24
 Operator : AR\AJ
 Sample : PB170835BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 03:10:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 14:16:16 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.499	2.796	100.1E6	153.4E6	19.825	21.960
28)	SA Decachlor...	8.966	7.951	81124807	146.1E6	21.352	22.213
Target Compounds							
23)	Chlordane-1	0.000	3.810	0	541573	N.D.	2.047 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121125\
Data File : PL097842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2025 17:24
Operator : AR\AJ
Sample : PB170835BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 03:10:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120925.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 14:16:16 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

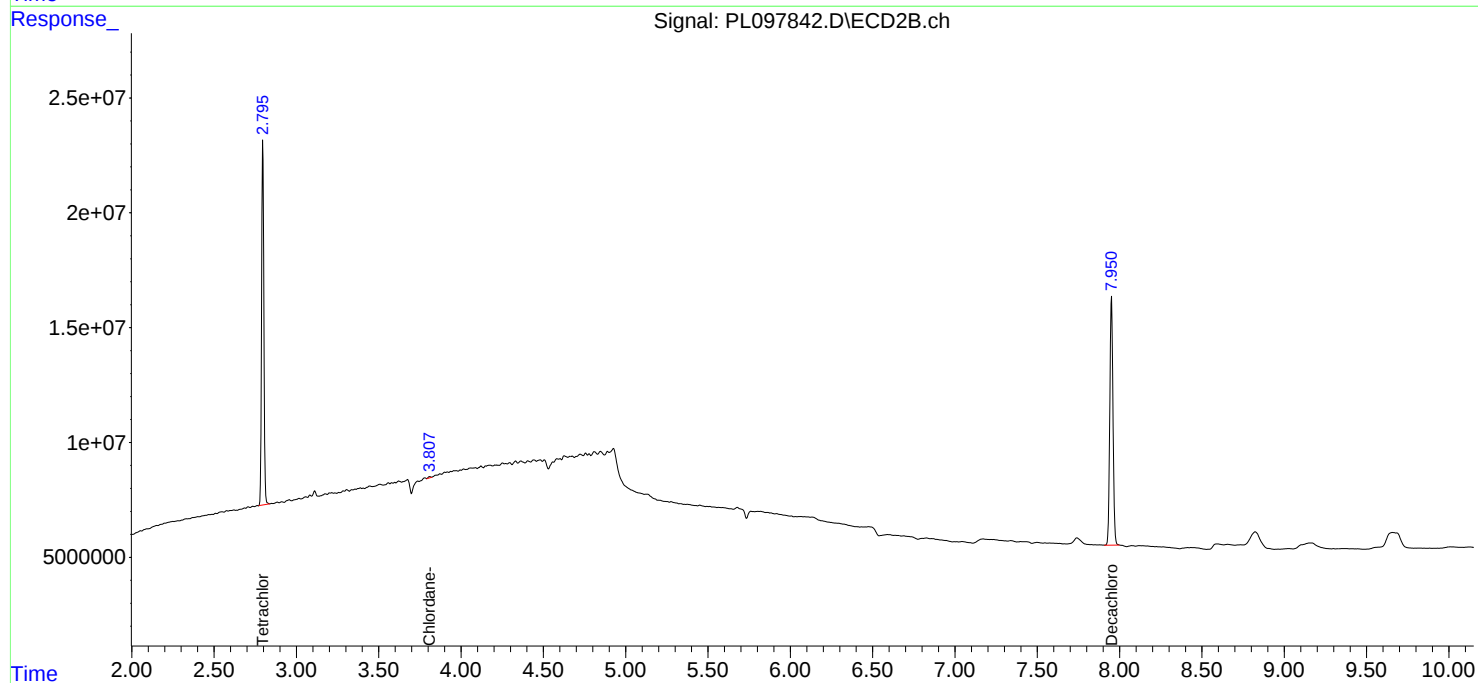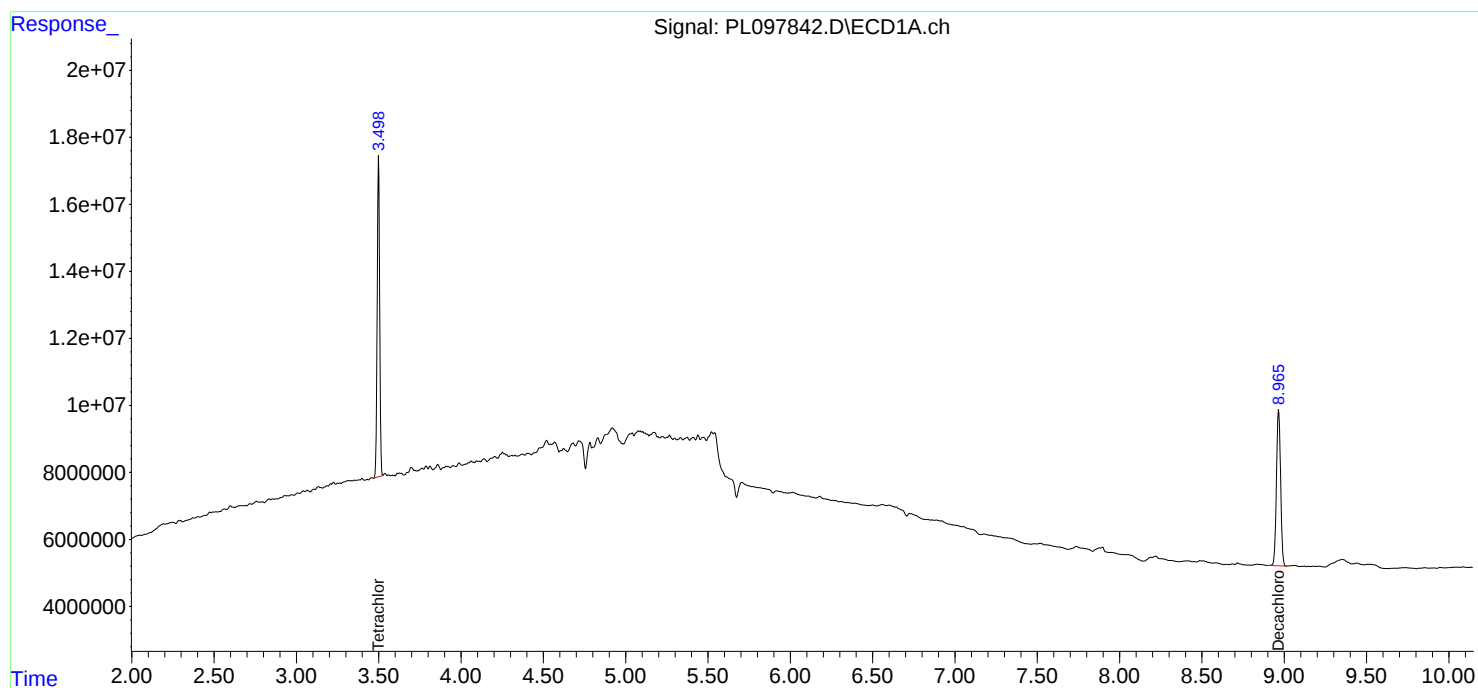


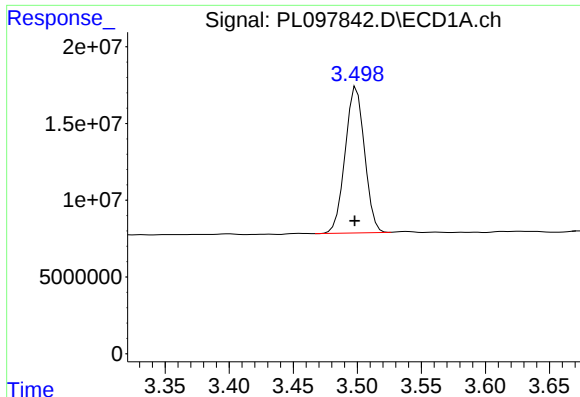

#1 Tetrachloro-m-xylene


R.T.: 3.499 min
Delta R.T.: 0.001 min
Response: 100057739
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

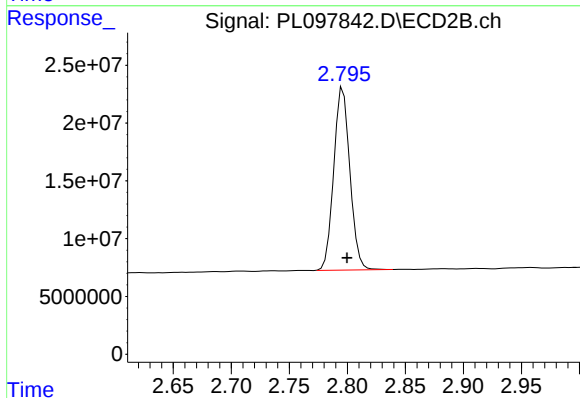


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: -0.003 min
Response: 153393955
Conc: 21.96 ng/ml

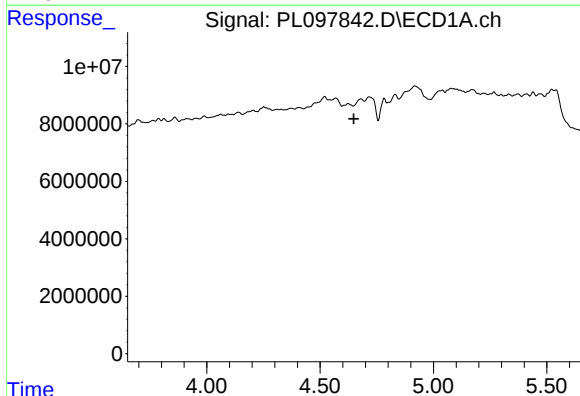


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

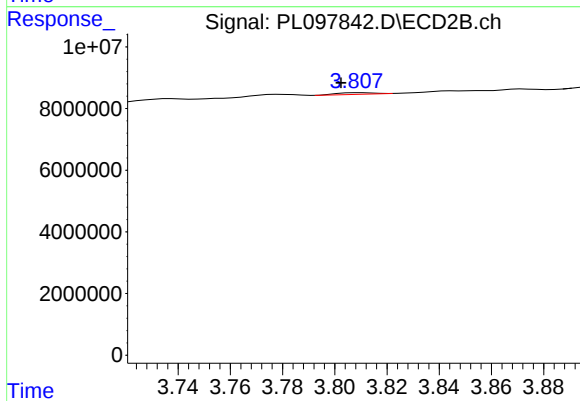

#23 Chlordane-1


R.T.: 3.810 min
Delta R.T.: 0.007 min
Response: 541573
Conc: 2.05 ng/ml

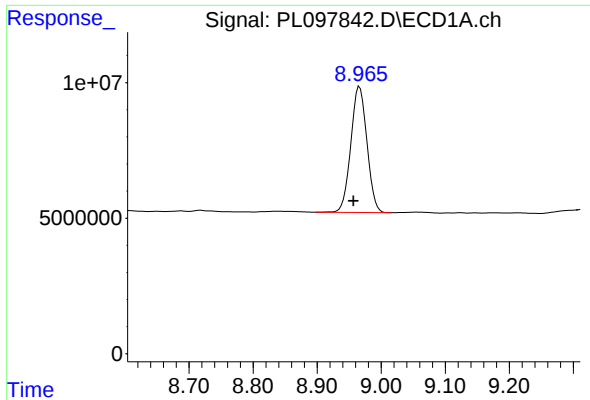

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: 0.009 min
Response: 81124807
Conc: 21.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

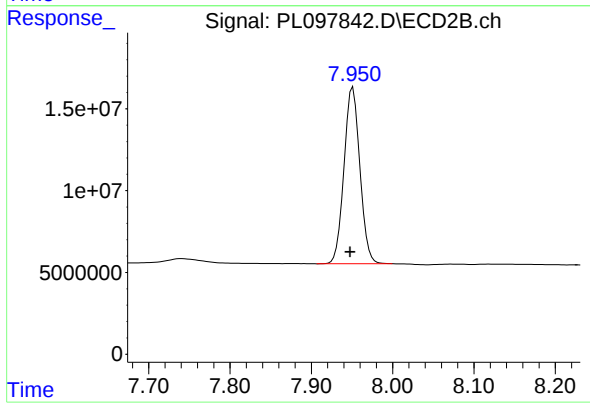

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.004 min
Response: 146072871
Conc: 22.21 ng/ml