

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
 Data File : PL042993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2018 08:51
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 11:21:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.099	128.7E6	61908959	20.984	20.888
28)	SA Decachlor...	8.203	9.228	137.4E6	53803307	21.042	20.626
Target Compounds							
2)	A alpha-BHC	3.898	4.444f	3531297	740218	0.374	0.164 #
6)	B beta-BHC	4.399f	0.000	3771122	0	1.022	N.D. #
7)	B delta-BHC	0.000	5.160	0	15104185	N.D.	3.515 #
8)	B Heptachlo...	0.000	5.993	0	7374769	N.D.	1.945 #
14)	MA Endrin	0.000	6.856	0	646121	N.D.	0.207 #
16)	A 4,4'-DDD	6.088f	0.000	1304928	0	0.230	N.D. #
17)	MA 4,4'-DDT	0.000	7.186f	0	1543688	N.D.	0.526 #
18)	B Endrin al...	0.000	7.186	0	1543688	N.D.	0.615 #
23)	Chlordane-1	4.363	5.160	1060347	15104185	3.946	106.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
Data File : PL042993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2018 08:51
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 11:21:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

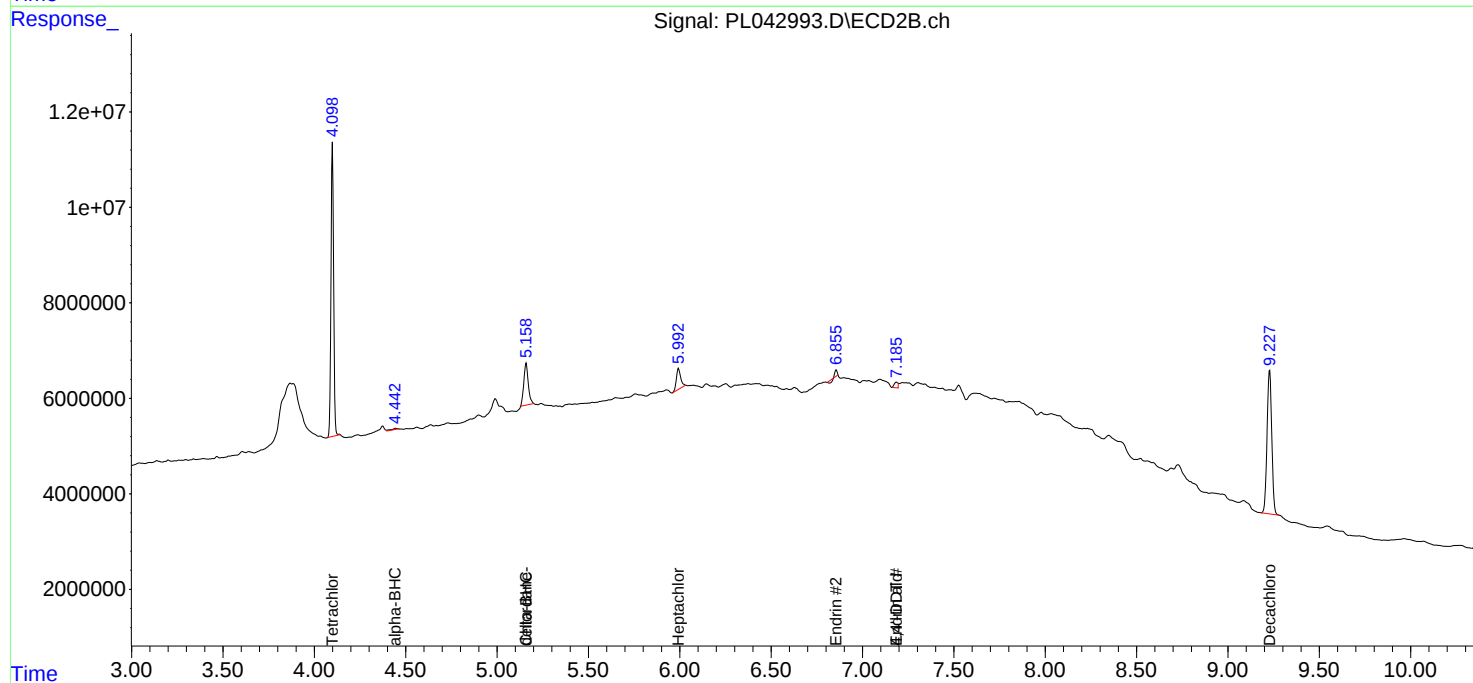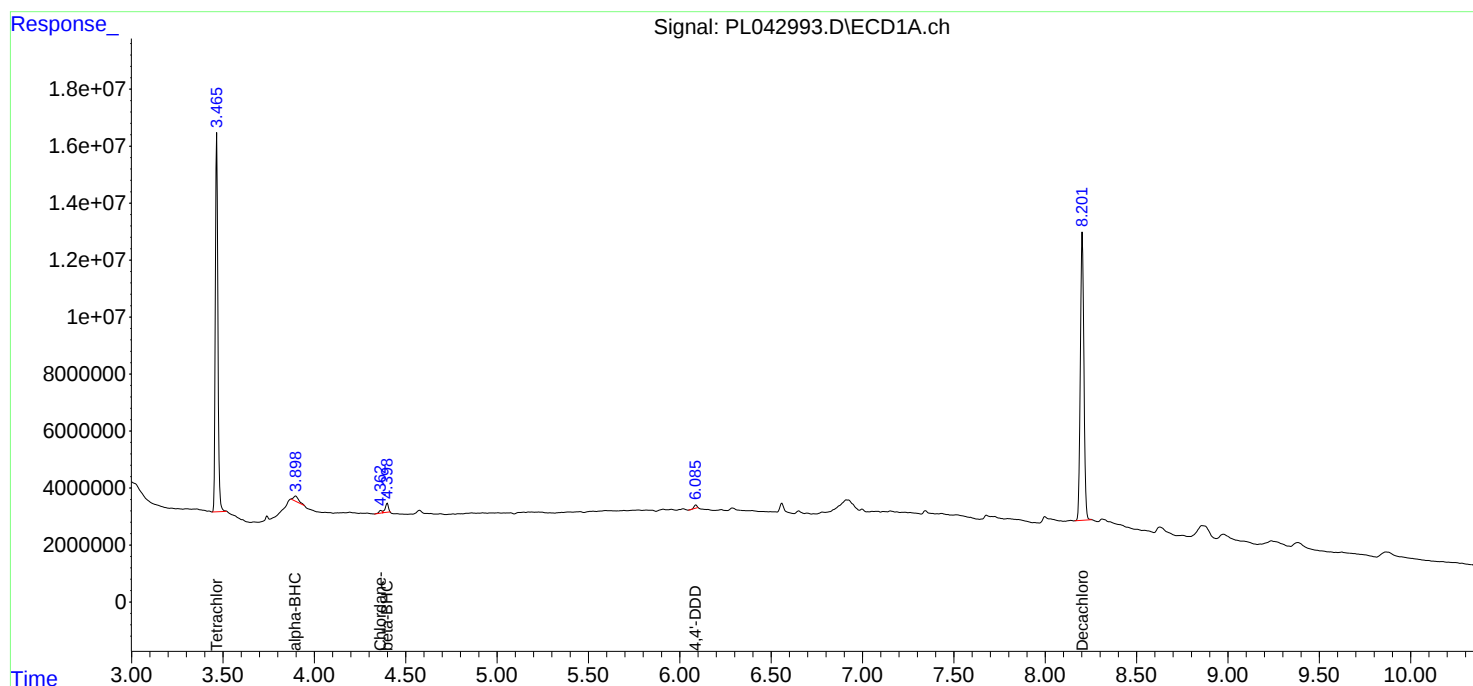


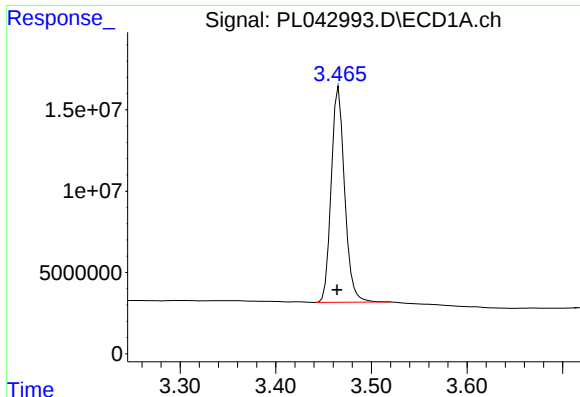

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.002 min
Response: 128692419
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

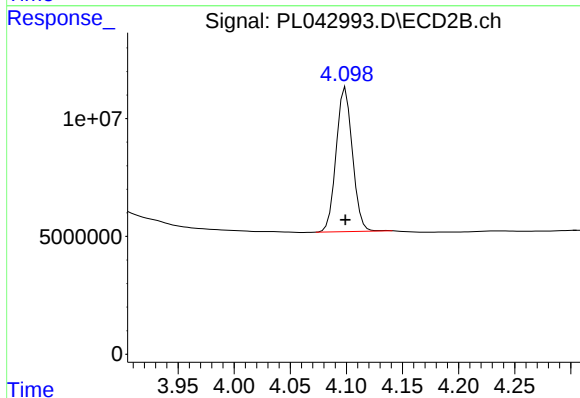


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 61908959
Conc: 20.89 ng/ml

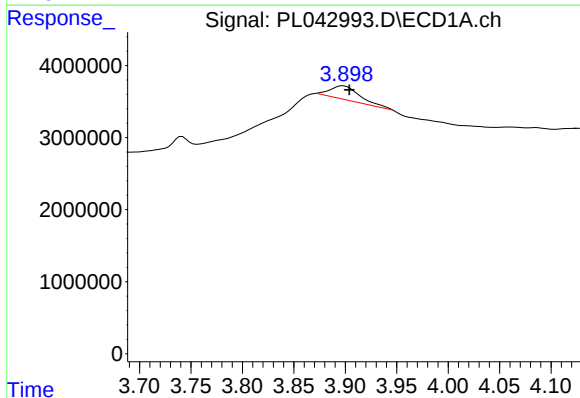


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: -0.006 min
Response: 3531297
Conc: 0.37 ng/ml

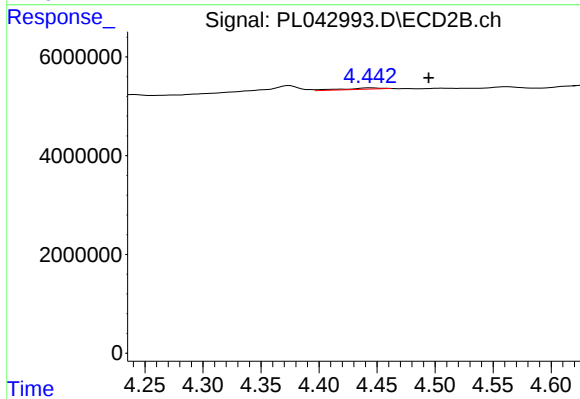

#2 alpha-BHC


R.T.: 4.444 min
Delta R.T.: -0.050 min
Response: 740218
Conc: 0.16 ng/ml

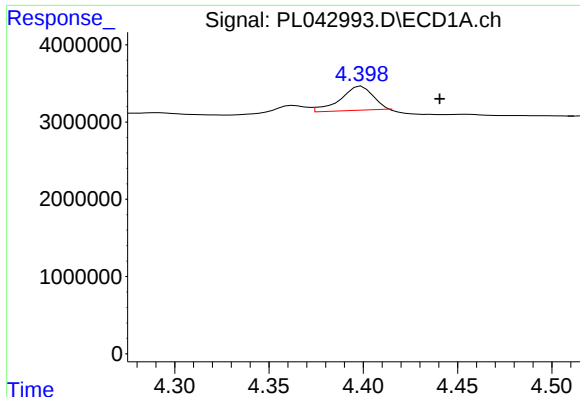

#6 beta-BHC


R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 3771122
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

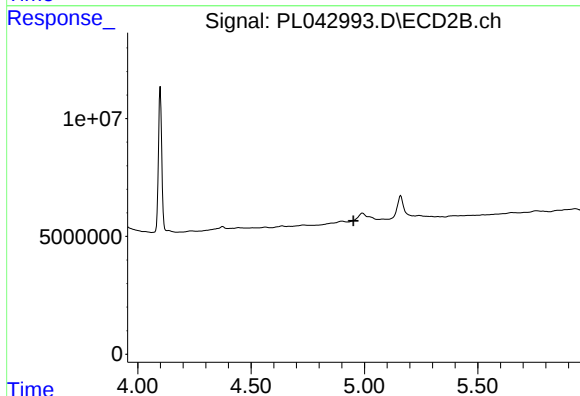


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

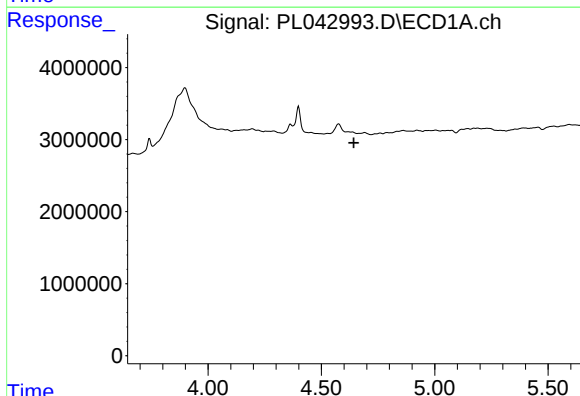


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

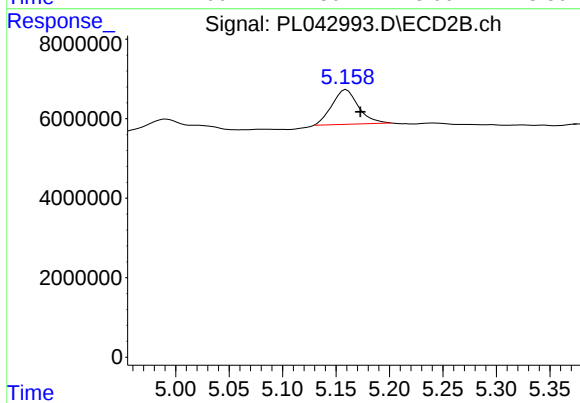

#7 delta-BHC


R.T.: 5.160 min
Delta R.T.: -0.013 min
Response: 15104185
Conc: 3.51 ng/ml

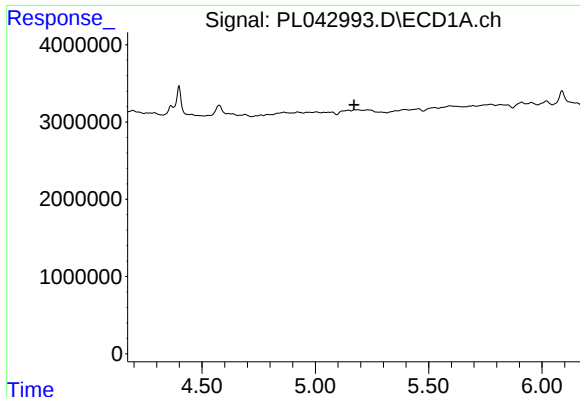

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

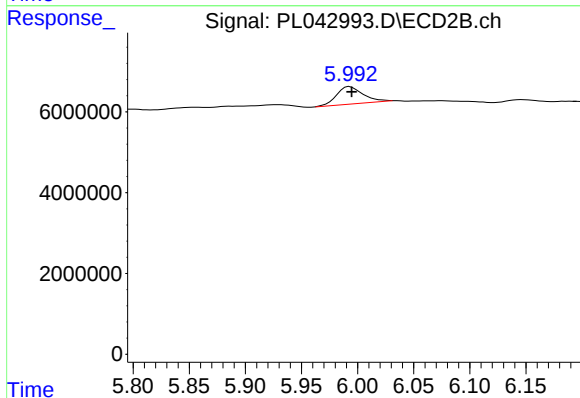


#8 Heptachlor epoxide

R.T.: 5.993 min
Delta R.T.: -0.002 min
Response: 7374769
Conc: 1.94 ng/ml

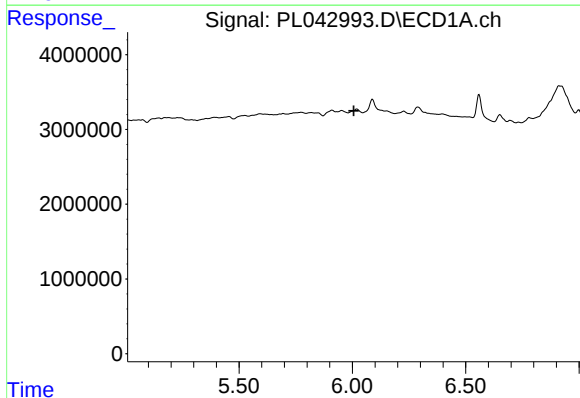


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.007 min
Response: 0
Conc: N.D.

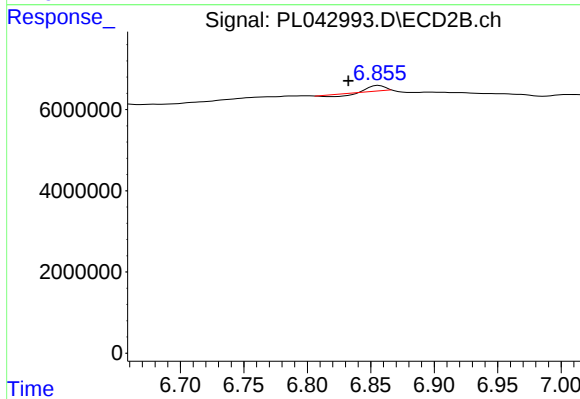

#14 Endrin


R.T.: 6.856 min
Delta R.T.: 0.024 min
Response: 646121
Conc: 0.21 ng/ml

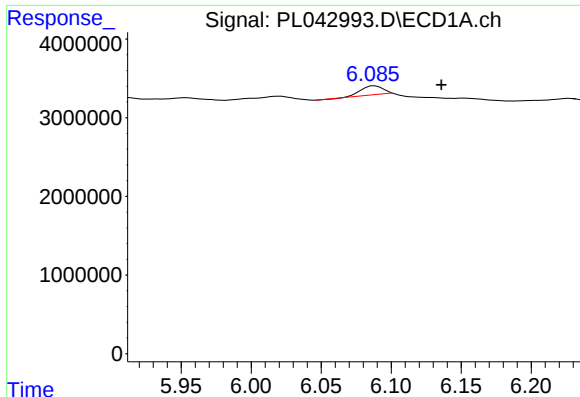

#16 4,4'-DDD


R.T.: 6.088 min
Delta R.T.: -0.048 min
Response: 1304928
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

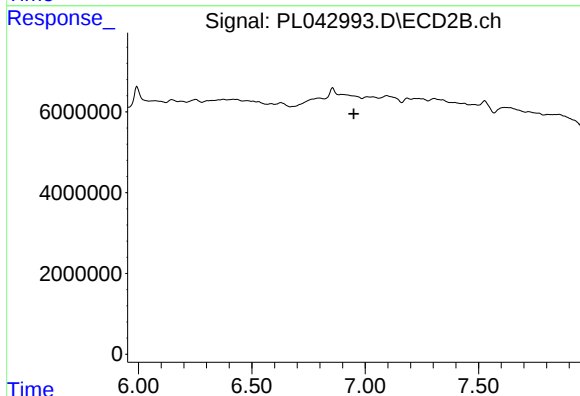


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

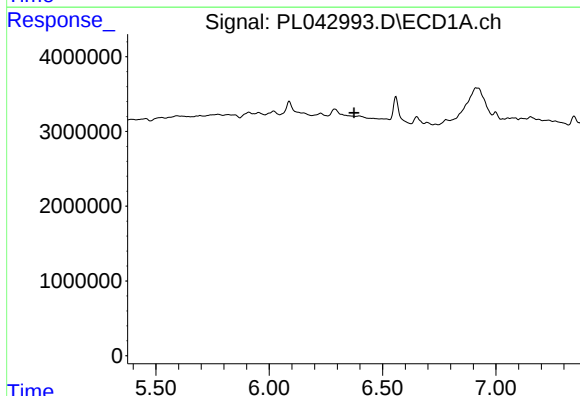


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.374 min
Response: 0
Conc: N.D.

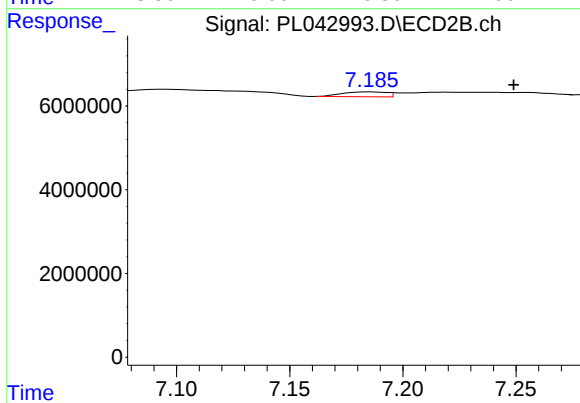

#17 4,4'-DDT


R.T.: 7.186 min
Delta R.T.: -0.063 min
Response: 1543688
Conc: 0.53 ng/ml

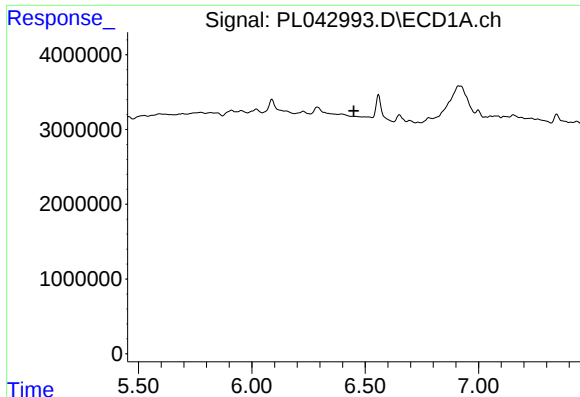

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.450 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

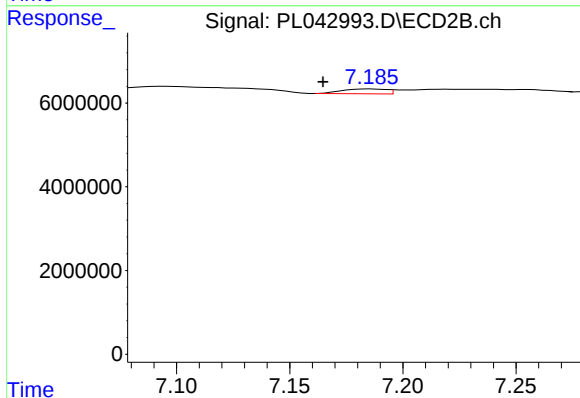


#18 Endrin aldehyde

R.T.: 7.186 min
Delta R.T.: 0.021 min
Response: 1543688
Conc: 0.62 ng/ml

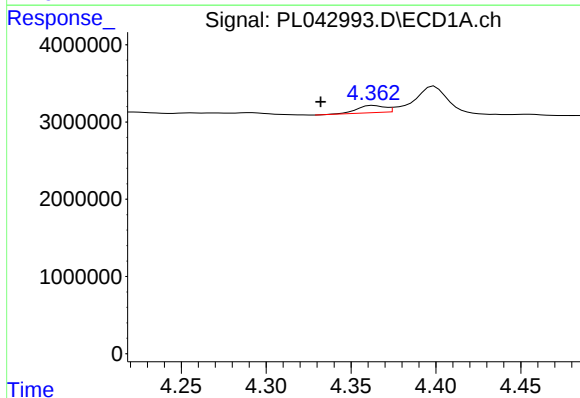


#23 Chlordane-1

R.T.: 4.363 min
Delta R.T.: 0.031 min
Response: 1060347
Conc: 3.95 ng/ml

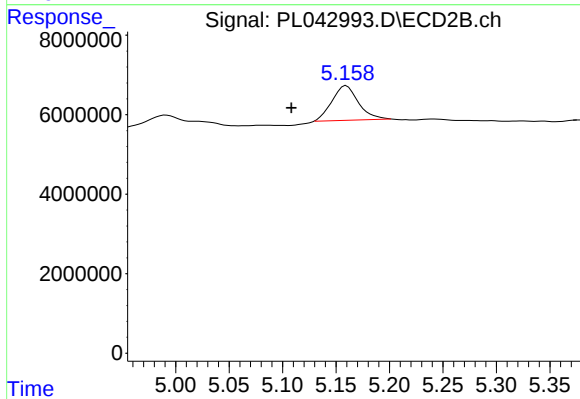

#23 Chlordane-1


R.T.: 5.160 min
Delta R.T.: 0.052 min
Response: 15104185
Conc: 106.87 ng/ml

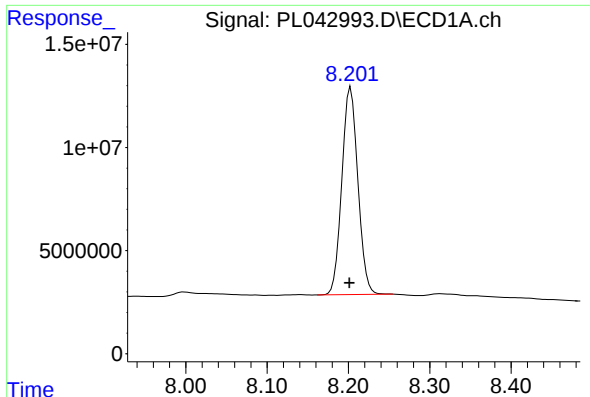

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.002 min
Response: 137402485
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

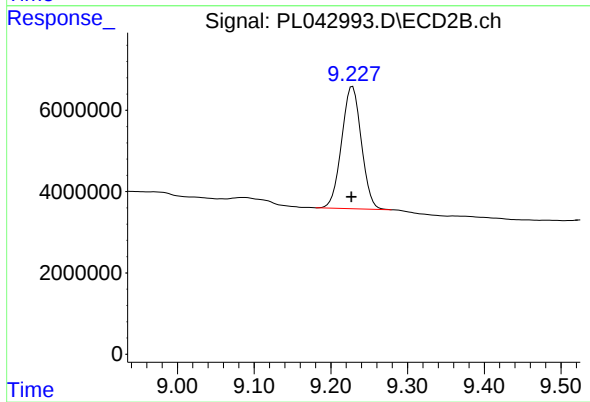

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.001 min
Response: 53803307
Conc: 20.63 ng/ml