

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
 Data File : PL043002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2018 11:15
 Operator : AJ\SJ
 Sample : J6234-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 11:29:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	120.6E6	61778986	19.663	20.844
28)	SA Decachlor...	8.201	9.227	121.4E6	50874243	18.596	19.503
Target Compounds							
2)	A alpha-BHC	3.863f	0.000	255375	0	0.027	N.D. #
6)	B beta-BHC	4.398f	0.000	14762051	0	4.002	N.D. #
7)	B delta-BHC	0.000	5.156	0	25747902	N.D.	5.991 #
8)	B Heptachlo...	0.000	5.991	0	14458388	N.D.	3.813 #
9)	A Endosulfan I	5.520	0.000	3810943	0	0.520	N.D. #
11)	B alpha-Chl...	5.520f	0.000	3810943	0	0.480	N.D. #
23)	Chlordane-1	4.398	5.156	14762051	25747902	54.938	182.179 #
26)	Chlordane-4	5.520	0.000	3810943	0	5.040	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
Data File : PL043002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2018 11:15
Operator : AJ\SJ
Sample : J6234-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 11:29:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

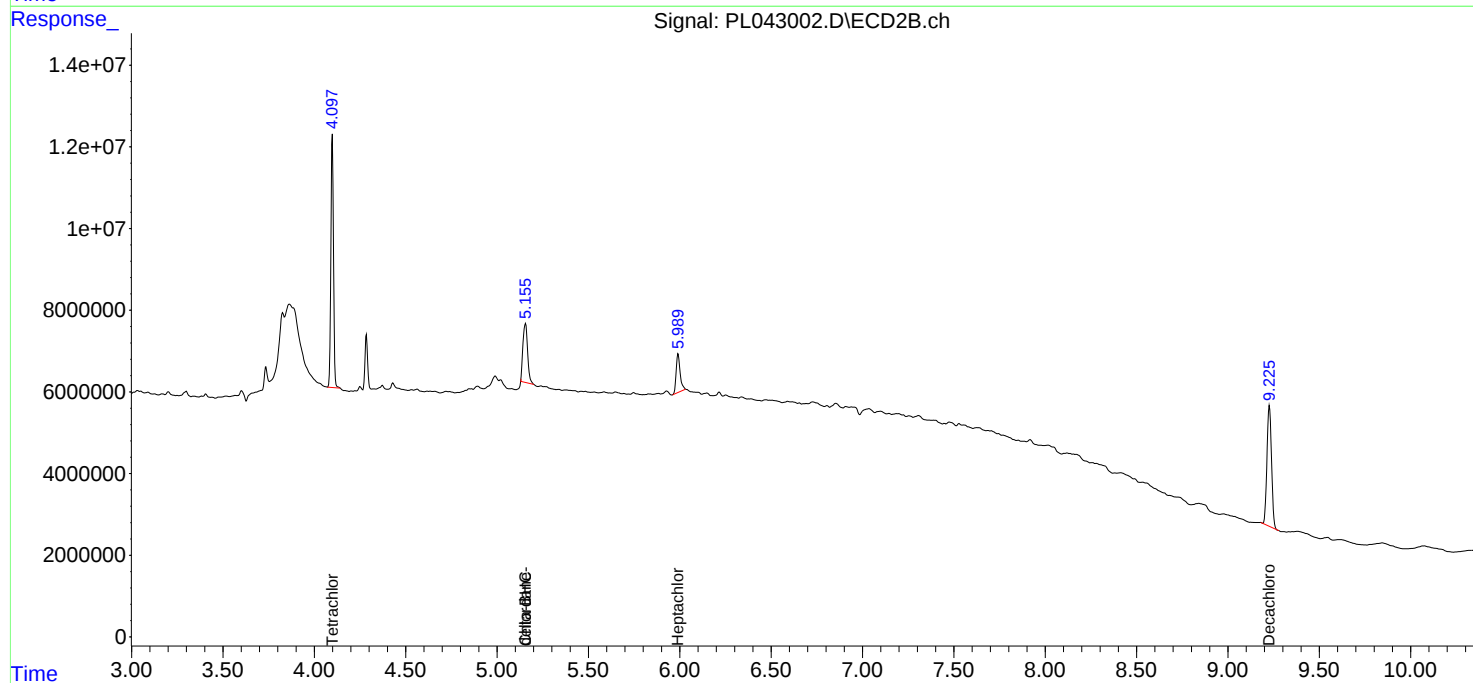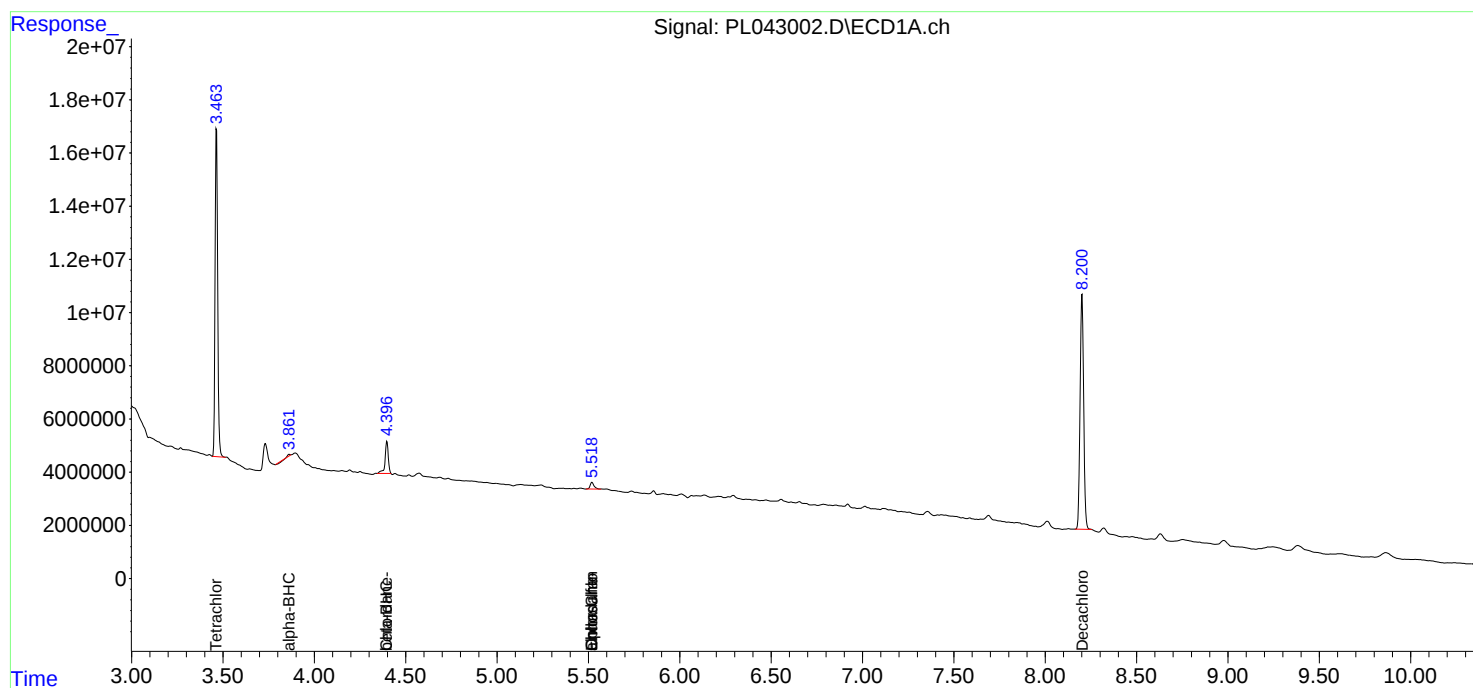


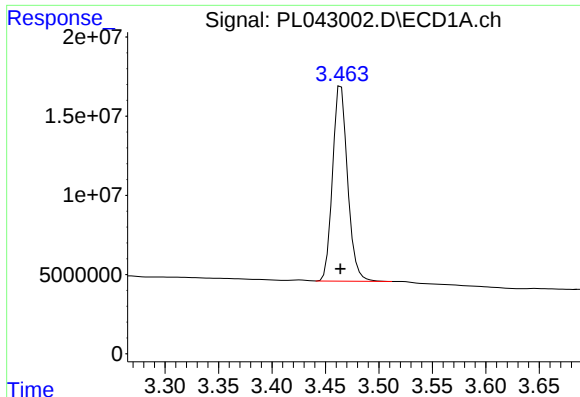

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 120590093
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

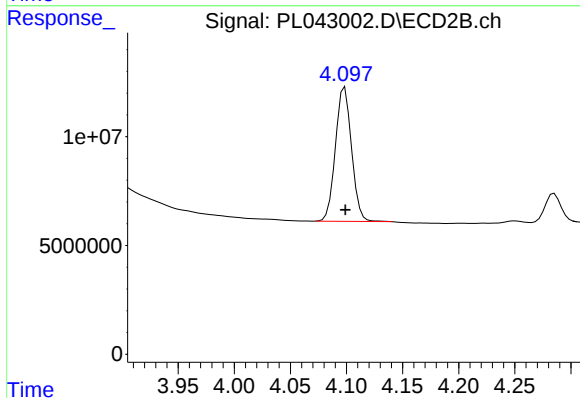


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 61778986
Conc: 20.84 ng/ml

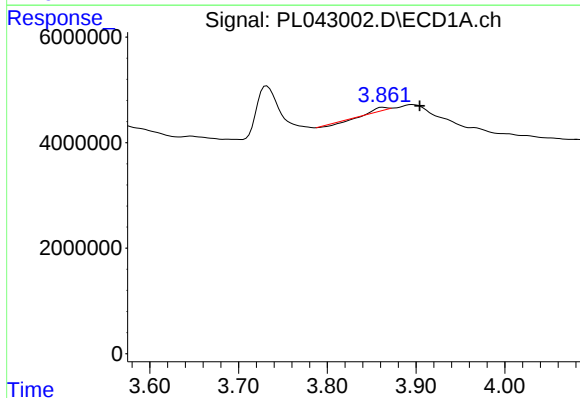


#2 alpha-BHC

R.T.: 3.863 min
Delta R.T.: -0.041 min
Response: 255375
Conc: 0.03 ng/ml

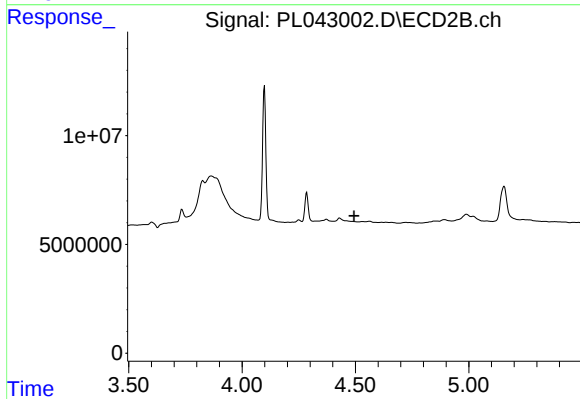

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

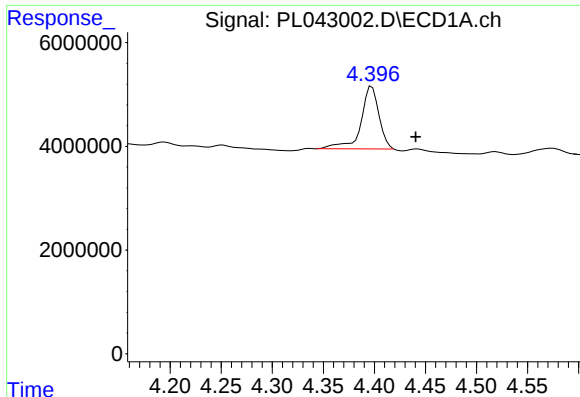

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 14762051
Conc: 4.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

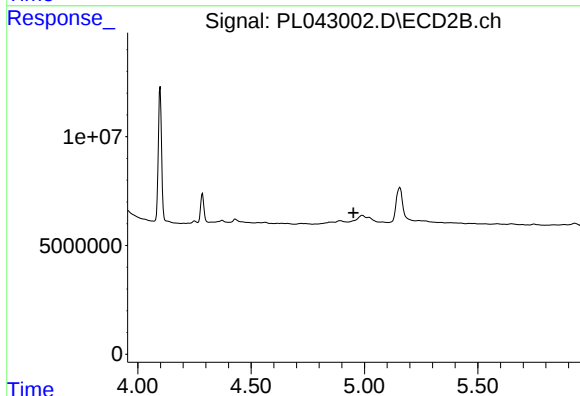


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

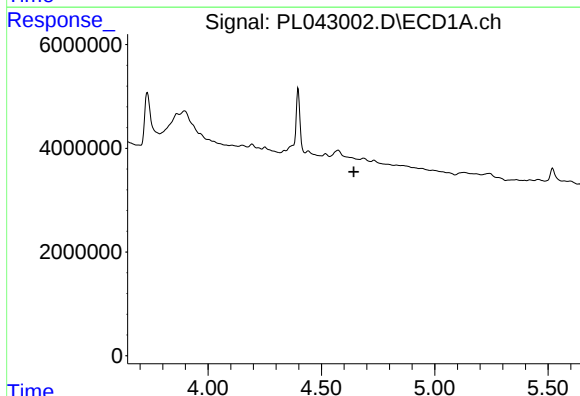


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

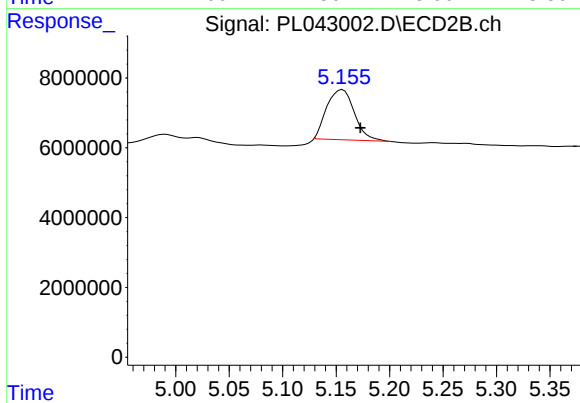

#7 delta-BHC


R.T.: 5.156 min
Delta R.T.: -0.017 min
Response: 25747902
Conc: 5.99 ng/ml

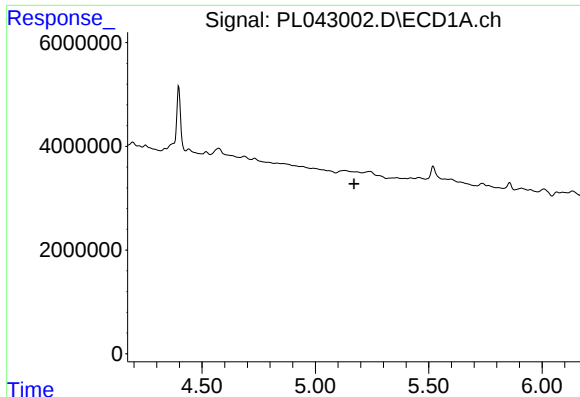

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

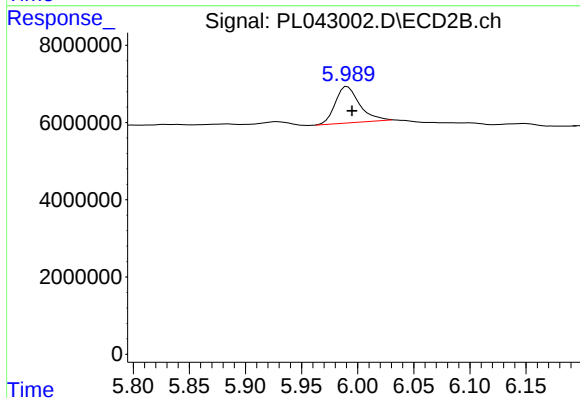


#8 Heptachlor epoxide

R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 14458388
Conc: 3.81 ng/ml

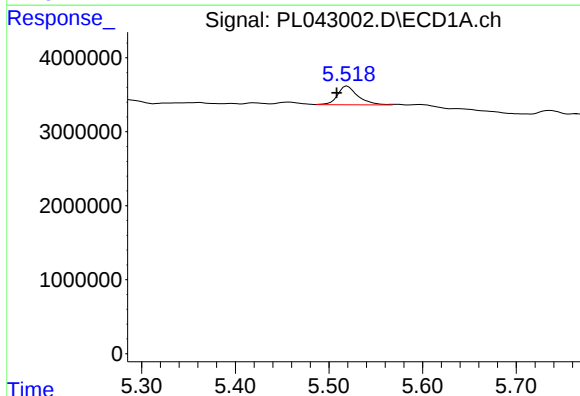


#9 Endosulfan I

R.T.: 5.520 min
Delta R.T.: 0.012 min
Response: 3810943
Conc: 0.52 ng/ml

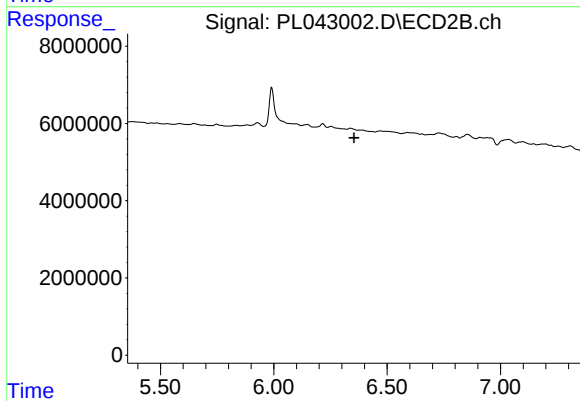

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.354 min
Response: 0
Conc: N.D.

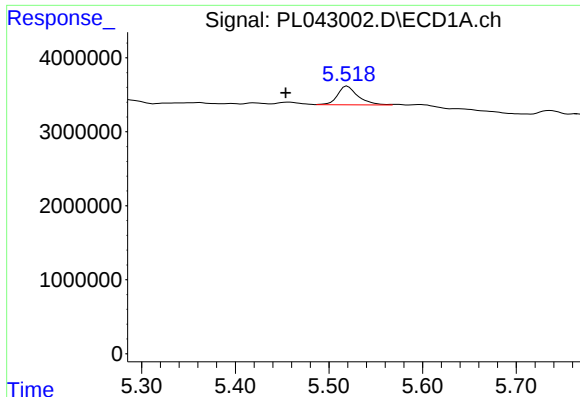

#11 alpha-Chlordane


R.T.: 5.520 min
Delta R.T.: 0.066 min
Response: 3810943
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

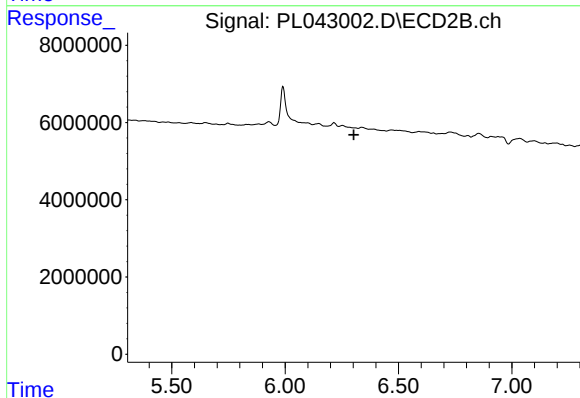


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.303 min
Response: 0
Conc: N.D.

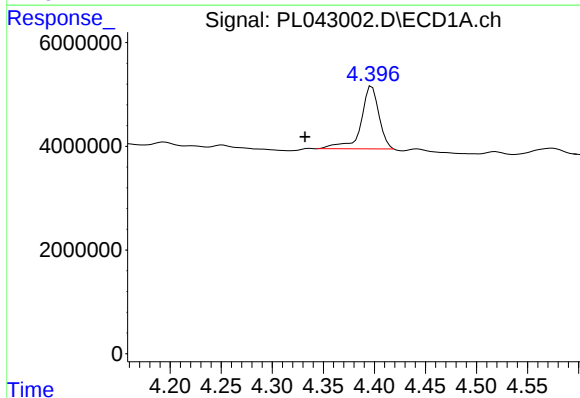


#23 Chlordane-1

R.T.: 4.398 min
Delta R.T.: 0.065 min
Response: 14762051
Conc: 54.94 ng/ml

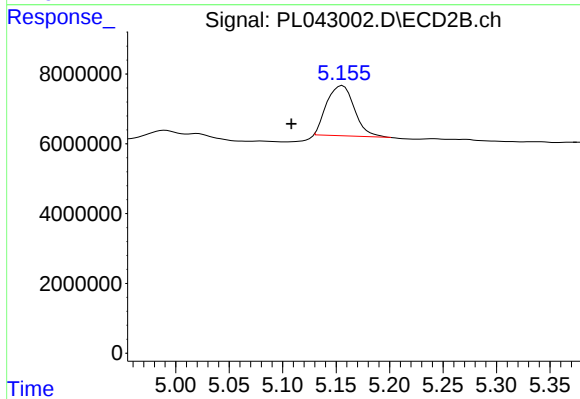

#23 Chlordane-1


R.T.: 5.156 min
Delta R.T.: 0.048 min
Response: 25747902
Conc: 182.18 ng/ml

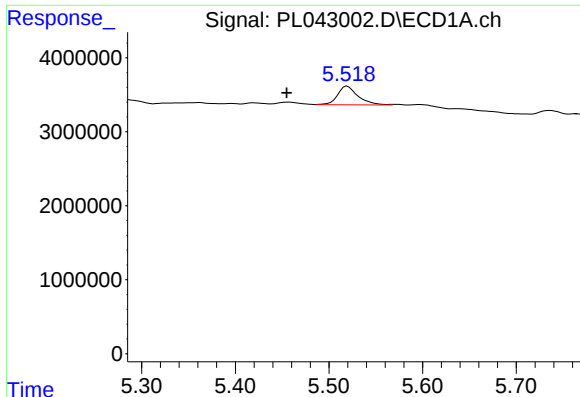

#26 Chlordane-4


R.T.: 5.520 min
Delta R.T.: 0.065 min
Response: 3810943
Conc: 5.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

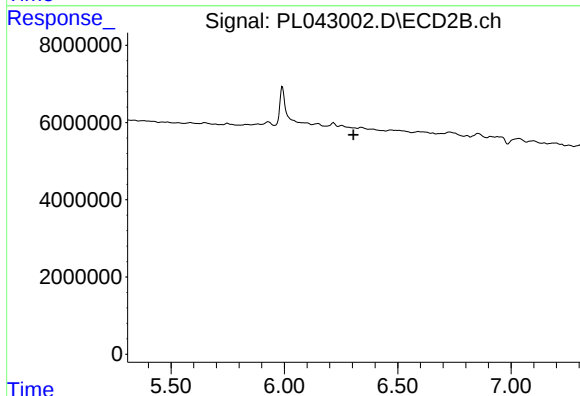


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.305 min
Response: 0
Conc: N.D.

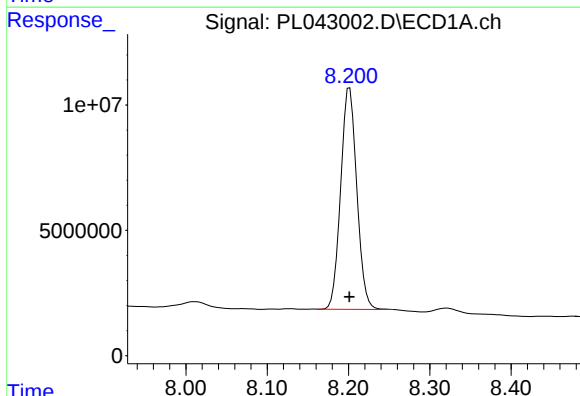

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 121433073
Conc: 18.60 ng/ml

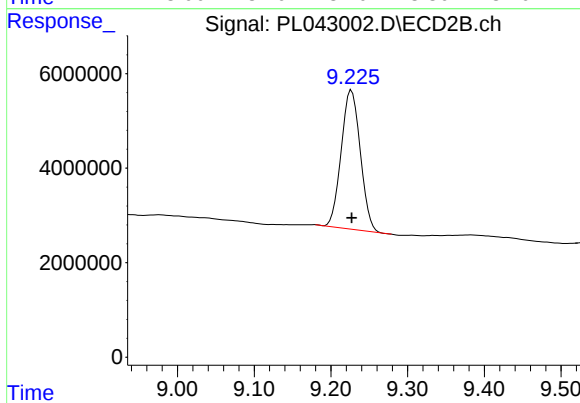

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 50874243
Conc: 19.50 ng/ml