

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
 Data File : PL043021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2018 15:47
 Operator : AJ\SJ
 Sample : J6316-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BORING-SAMPLE-SIGNAL-TOWER-

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 02:46:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	112.9E6	58627990	18.402	19.781
28)	SA Decachlor...	8.201	9.227	119.7E6	47727848	18.337	18.297
Target Compounds							
6)	B beta-BHC	4.397f	0.000	4365989	0	1.184	N.D. #
7)	B delta-BHC	0.000	5.157	0	10180813	N.D.	2.369 #
8)	B Heptachlo...	0.000	5.991	0	4711959	N.D.	1.243 #
10)	B gamma-Chl...	0.000	6.252	0	2231783	N.D.	0.608 #
11)	B alpha-Chl...	0.000	6.252f	0	2231783	N.D.	0.621 #
23)	Chlordane-1	4.362	5.157	1208572	10180813	4.498	72.034 #
25)	Chlordane-3	0.000	6.252	0	2231783	N.D.	4.545 #
26)	Chlordane-4	0.000	6.252	0	2231783	N.D.	3.910 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
Data File : PL043021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2018 15:47
Operator : AJ\SJ
Sample : J6316-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BORING-SAMPLE-SIGNAL-TOWER-

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 02:46:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

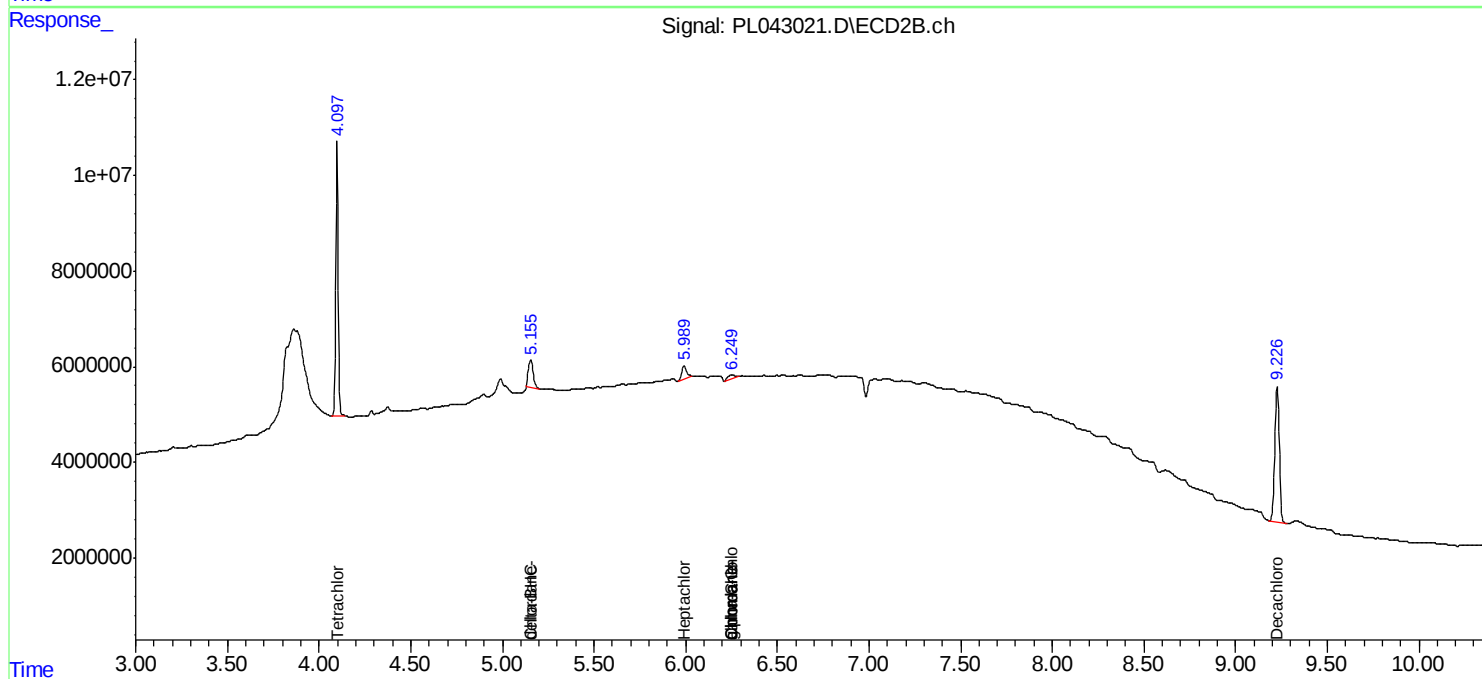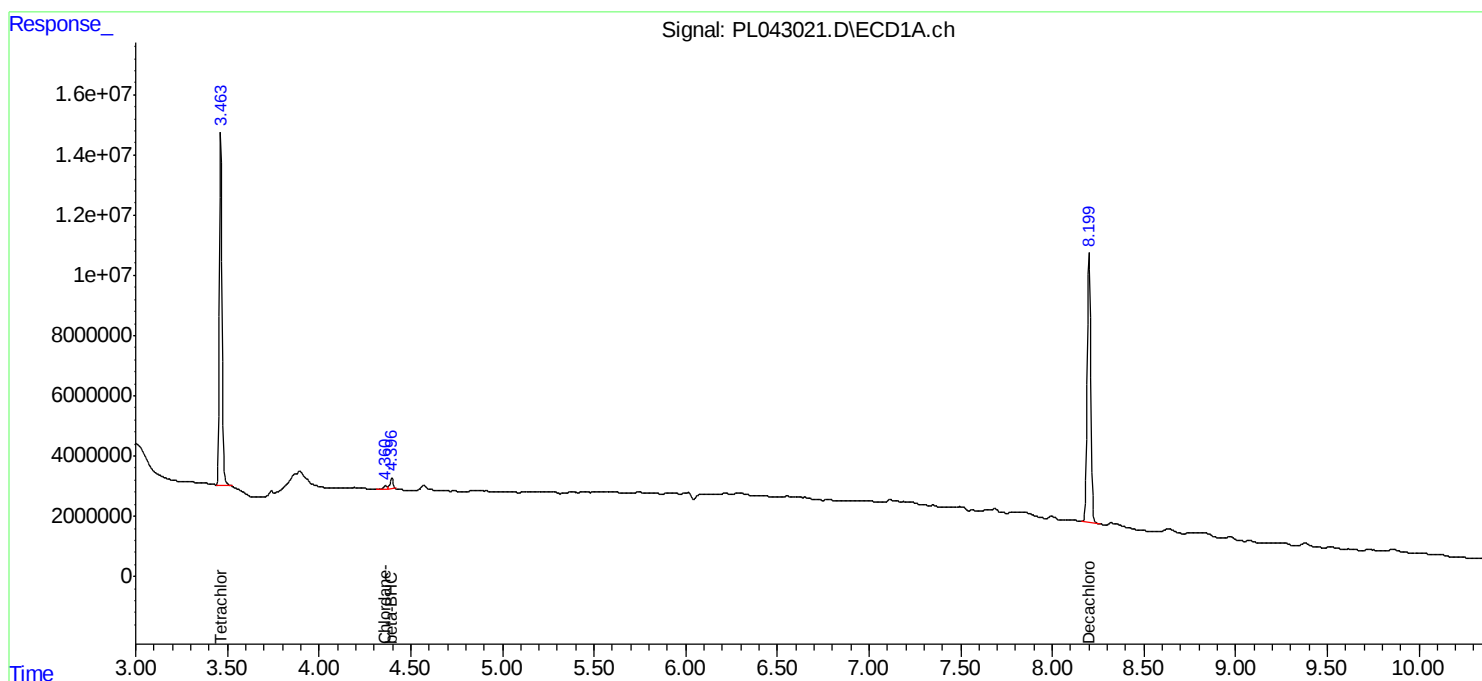


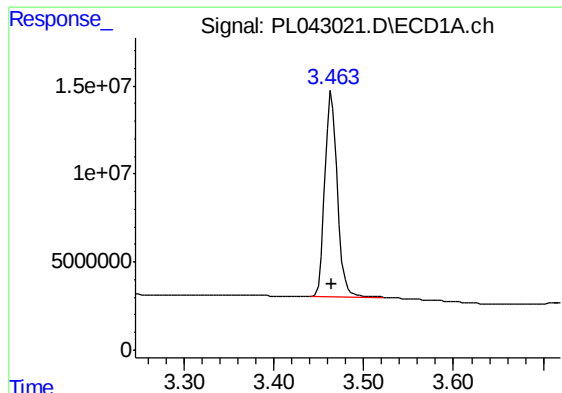

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 112859174
Conc: 18.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORING-SAMPLE-SIGNAL-TOWER-

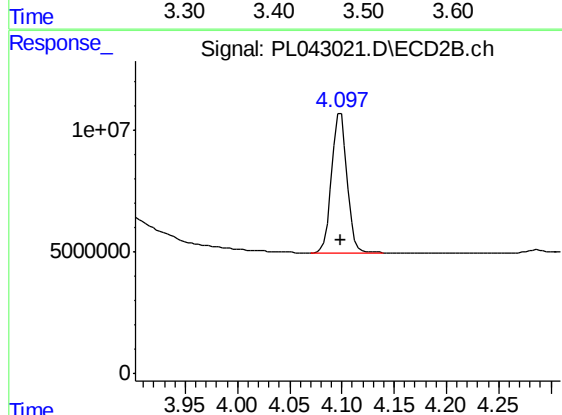


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 58627990
Conc: 19.78 ng/ml

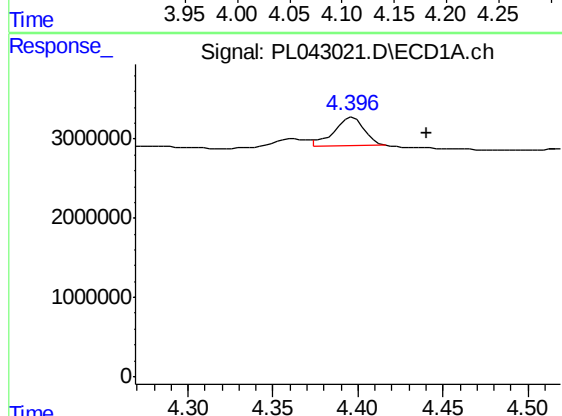


#6 beta-BHC

R.T.: 4.397 min
Delta R.T.: -0.044 min
Response: 4365989
Conc: 1.18 ng/ml

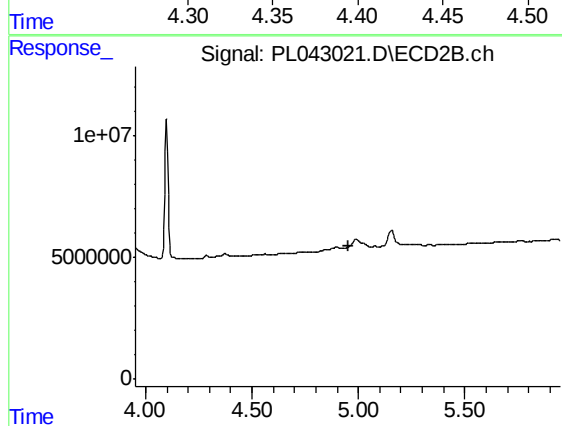

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

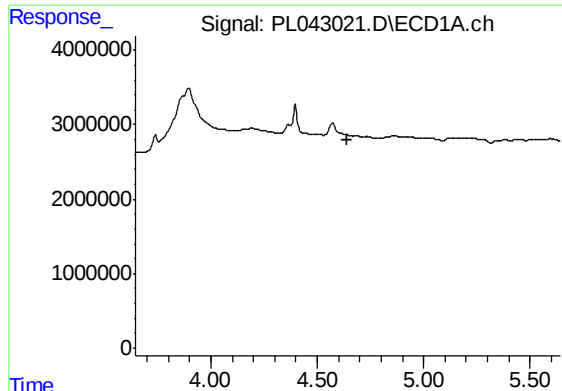

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BORING-SAMPLE-SIGNAL-TOWER-

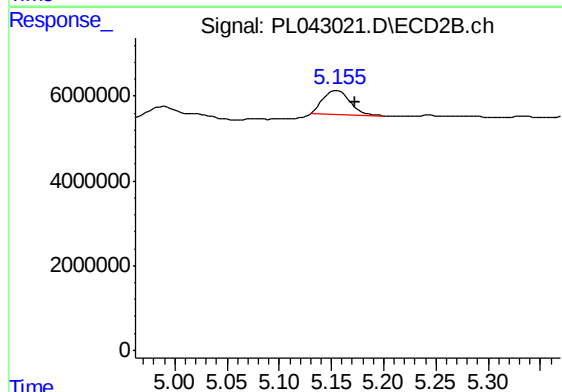


#7 delta-BHC

R.T.: 5.157 min
Delta R.T.: -0.016 min
Response: 10180813
Conc: 2.37 ng/ml

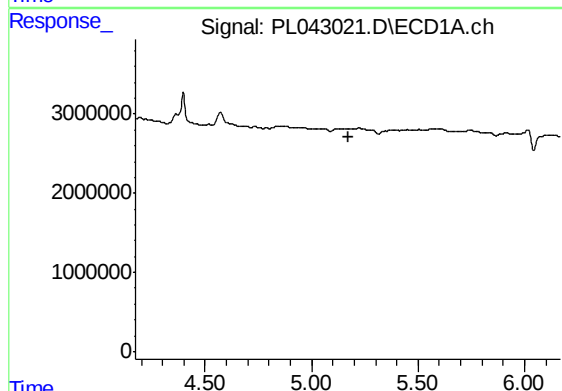


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

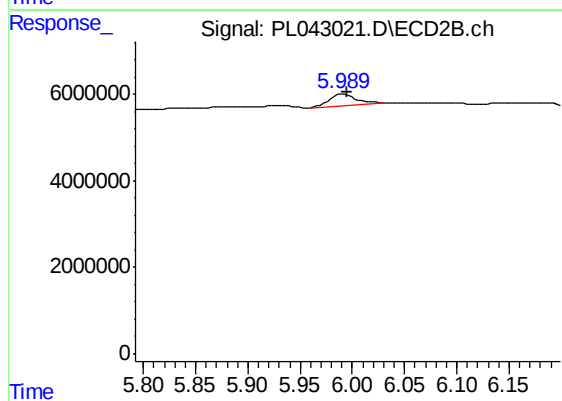

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.003 min
Response: 4711959
Conc: 1.24 ng/ml

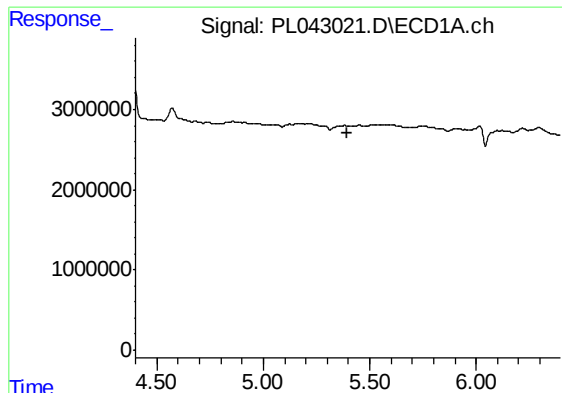

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BORING-SAMPLE-SIGNAL-TOWER-

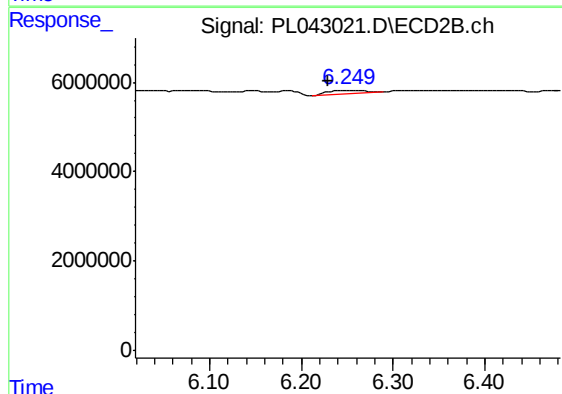


#10 gamma-Chlordane

R.T.: 6.252 min
Delta R.T.: 0.022 min
Response: 2231783
Conc: 0.61 ng/ml

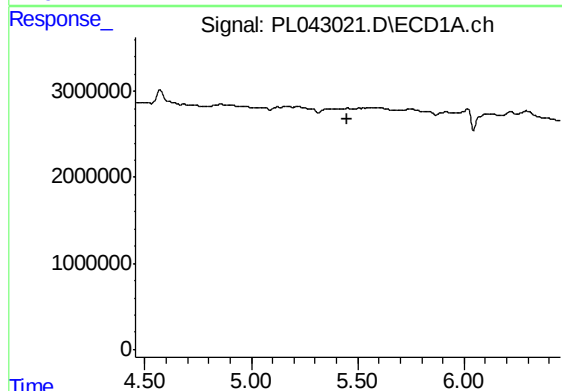


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

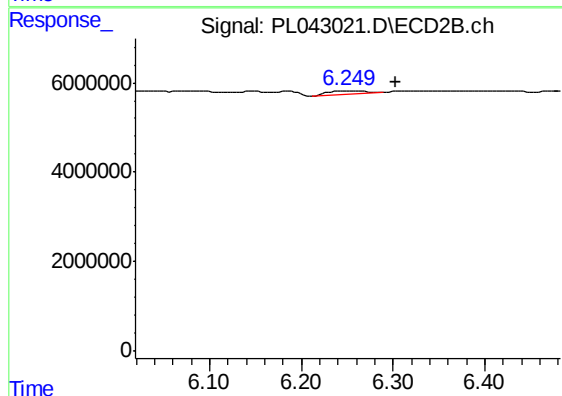

#11 alpha-Chlordane


R.T.: 6.252 min
Delta R.T.: -0.051 min
Response: 2231783
Conc: 0.62 ng/ml

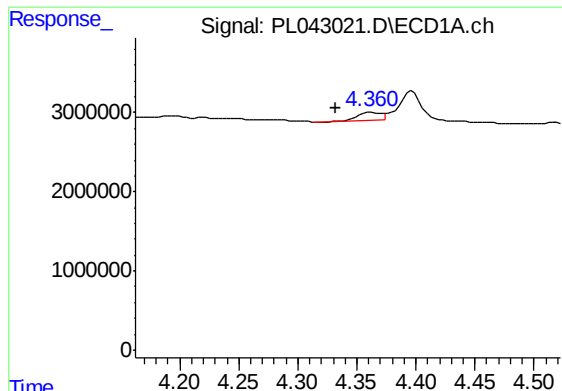

#23 Chlordane-1


R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 1208572
Conc: 4.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORING-SAMPLE-SIGNAL-TOWER-

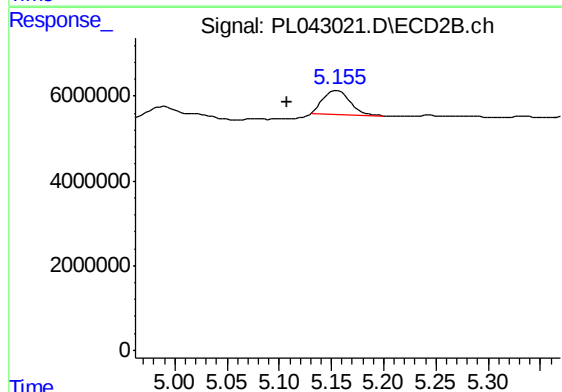


#23 Chlordane-1

R.T.: 5.157 min
Delta R.T.: 0.048 min
Response: 10180813
Conc: 72.03 ng/ml

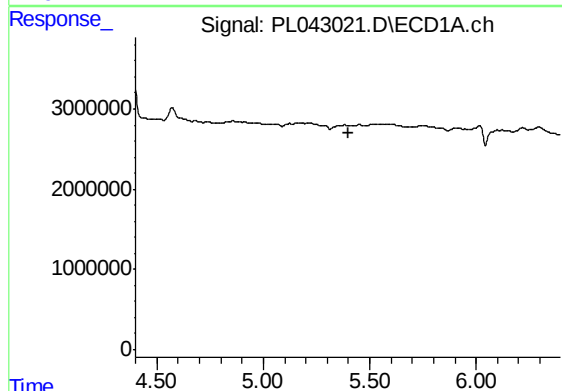


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

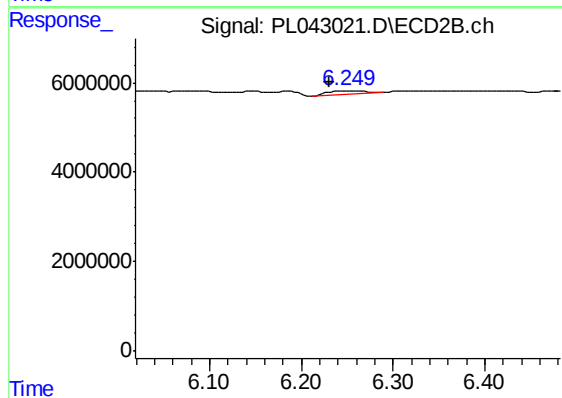

#25 Chlordane-3


R.T.: 6.252 min
Delta R.T.: 0.021 min
Response: 2231783
Conc: 4.54 ng/ml

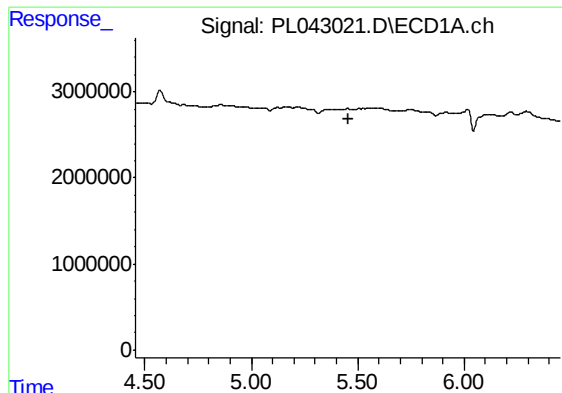

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BORING-SAMPLE-SIGNAL-TOWER-

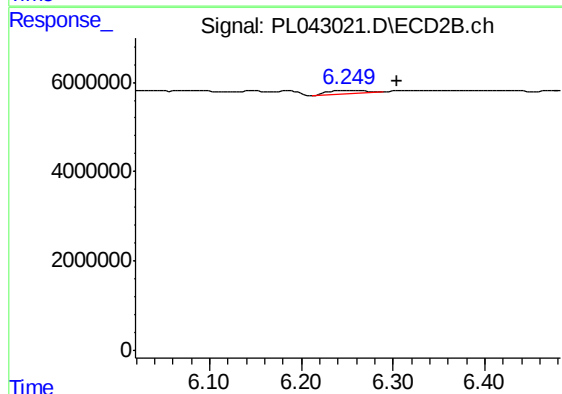


#26 Chlordane-4

R.T.: 6.252 min
Delta R.T.: -0.053 min
Response: 2231783
Conc: 3.91 ng/ml

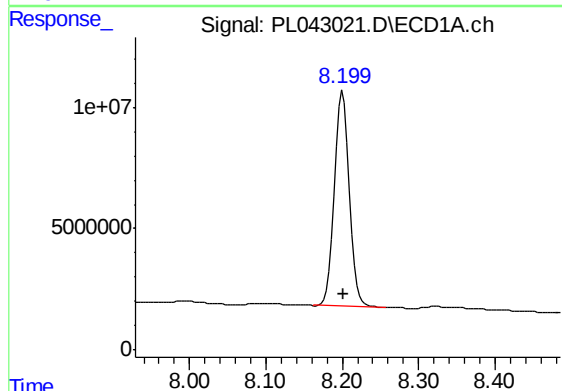

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 119737165
Conc: 18.34 ng/ml

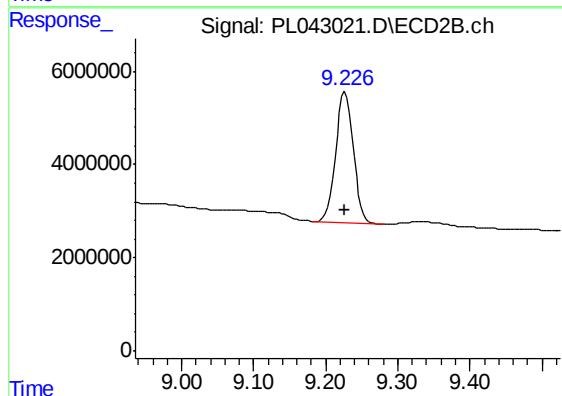

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 47727848
Conc: 18.30 ng/ml