

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
 Data File : PL043022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2018 16:01
 Operator : AJ\SJ
 Sample : PB115576BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB115576BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 02:46:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	111.5E6	57270699	18.184	19.323
28)	SA Decachlor...	8.201	9.227	121.5E6	49505625	18.606	18.979
Target Compounds							
6)	B beta-BHC	4.397f	0.000	4663230	0	1.264	N.D. #
7)	B delta-BHC	0.000	5.156	0	9559445	N.D.	2.224 #
8)	B Heptachlo...	0.000	5.991	0	4521910	N.D.	1.192 #
10)	B gamma-Chl...	0.000	6.255	0	448289	N.D.	0.122 #
11)	B alpha-Chl...	0.000	6.255f	0	448289	N.D.	0.125 #
23)	Chlordane-1	4.361	5.156	1157268	9559445	4.307	67.638 #
25)	Chlordane-3	0.000	6.255	0	448289	N.D.	0.913 #
26)	Chlordane-4	0.000	6.255	0	448289	N.D.	0.785 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
Data File : PL043022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2018 16:01
Operator : AJ\SJ
Sample : PB115576BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB115576BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 02:46:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

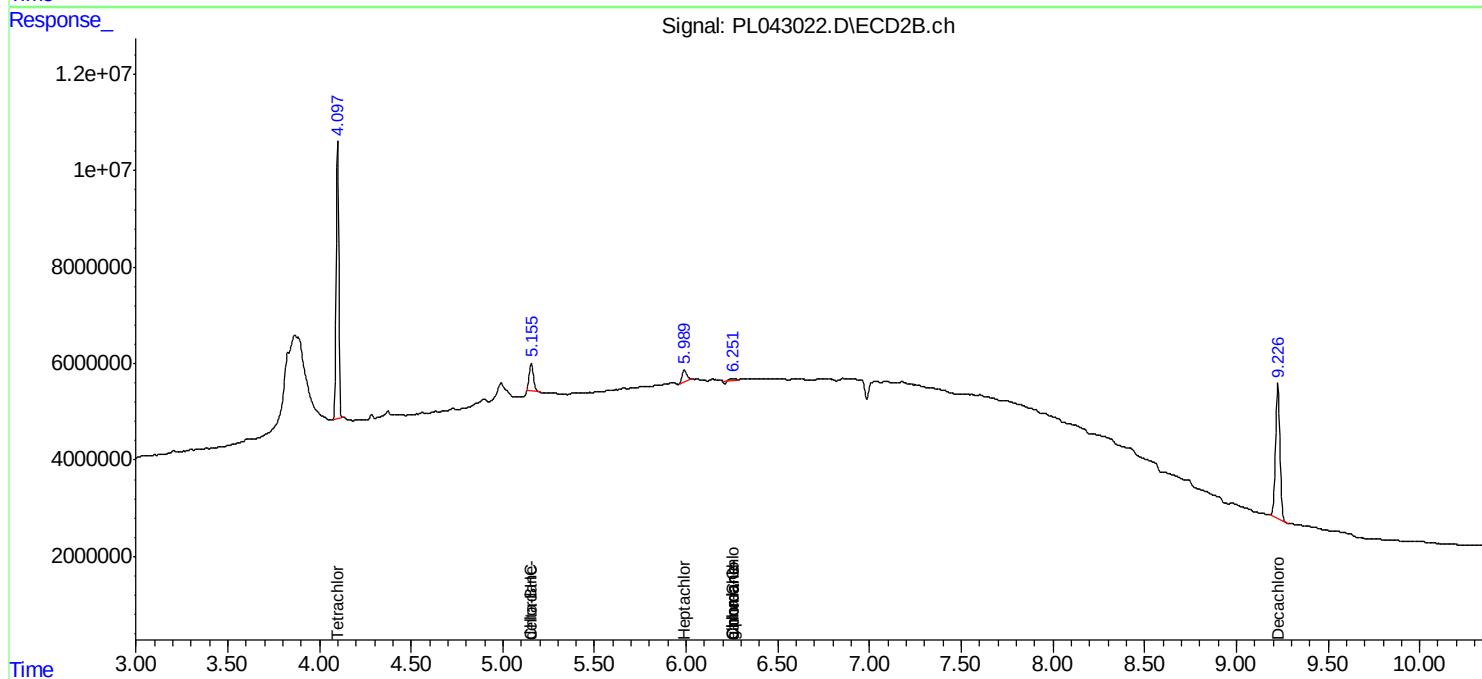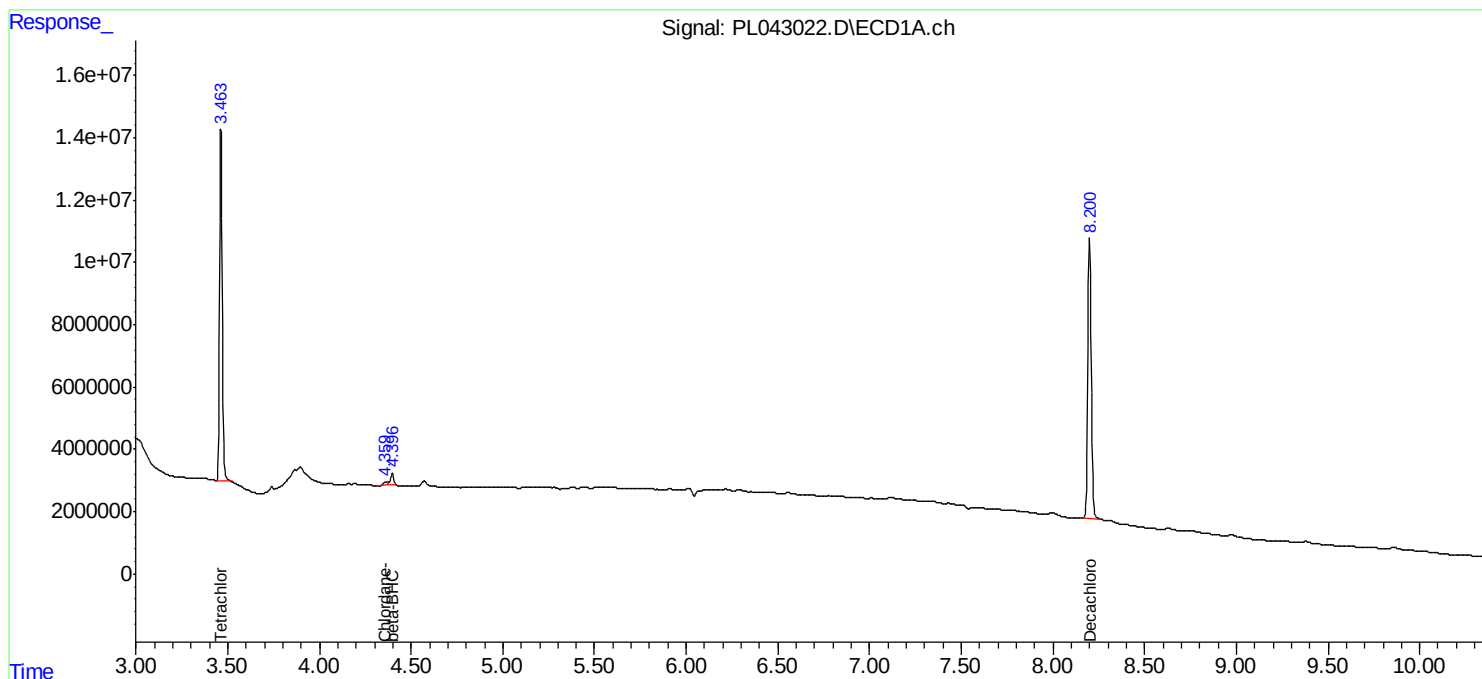


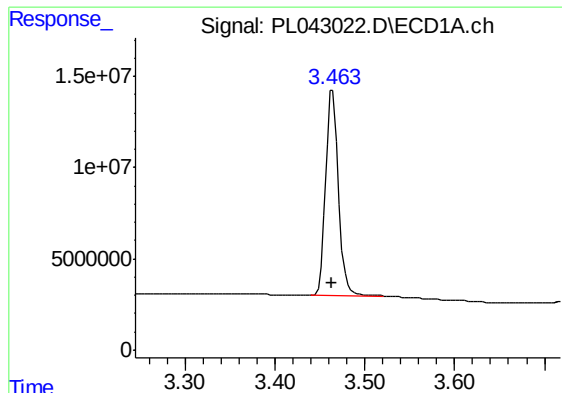

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 111521935
Conc: 18.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB115576BL

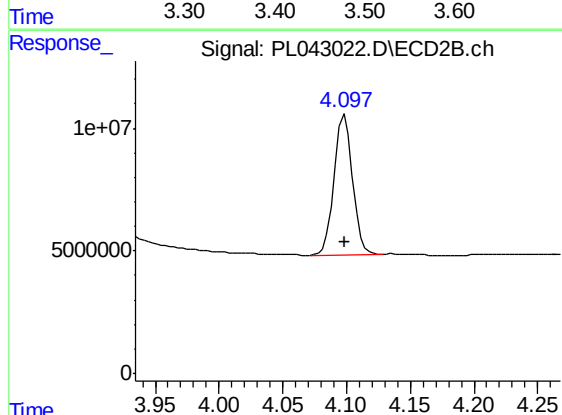


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 57270699
Conc: 19.32 ng/ml

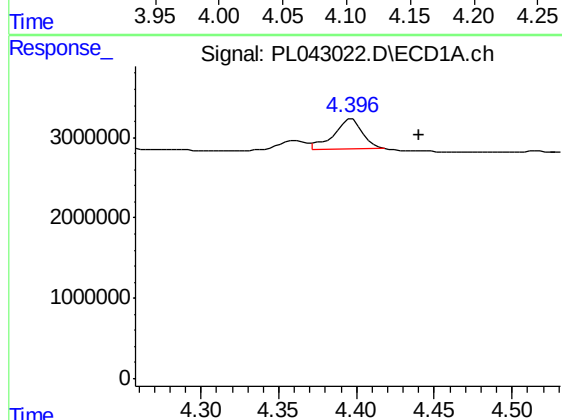


#6 beta-BHC

R.T.: 4.397 min
Delta R.T.: -0.044 min
Response: 4663230
Conc: 1.26 ng/ml

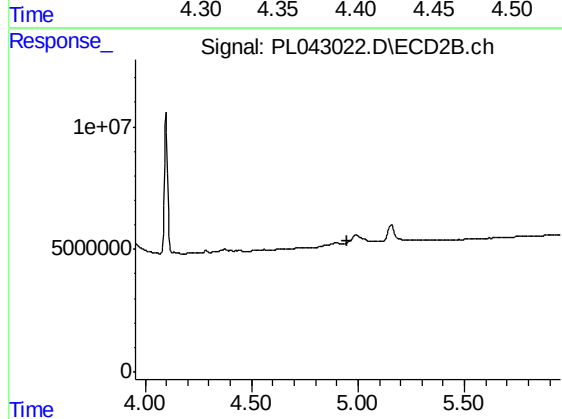

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

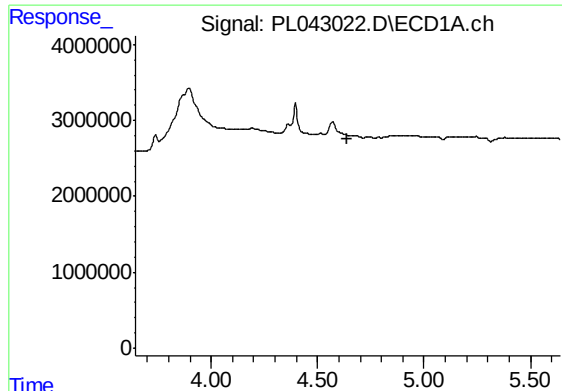

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB115576BL

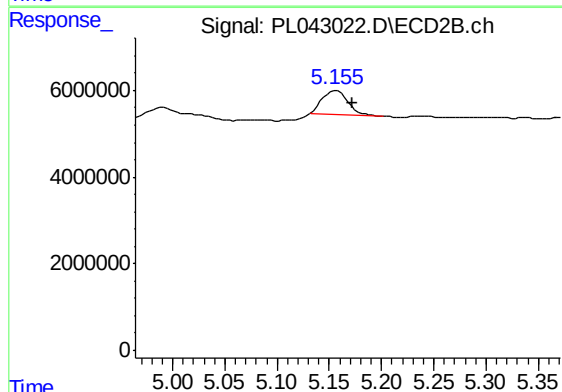


#7 delta-BHC

R.T.: 5.156 min
Delta R.T.: -0.016 min
Response: 9559445
Conc: 2.22 ng/ml

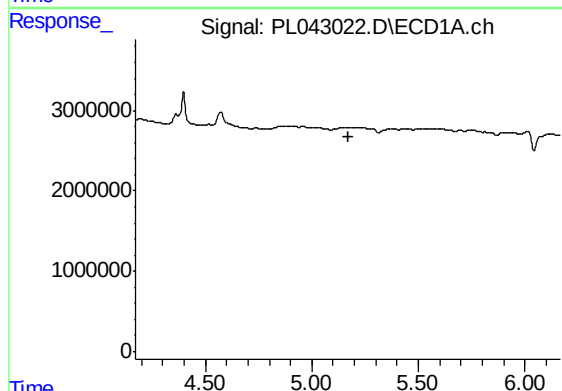


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

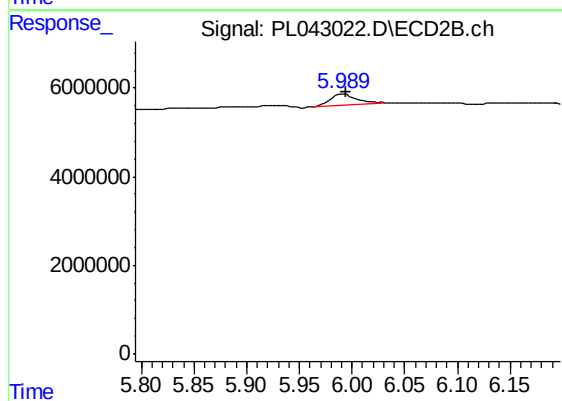

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 4521910
Conc: 1.19 ng/ml

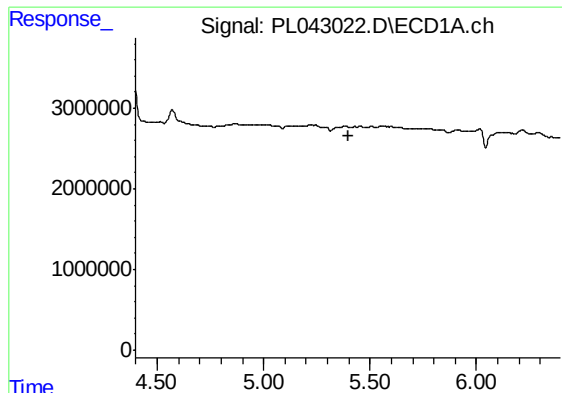

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB115576BL

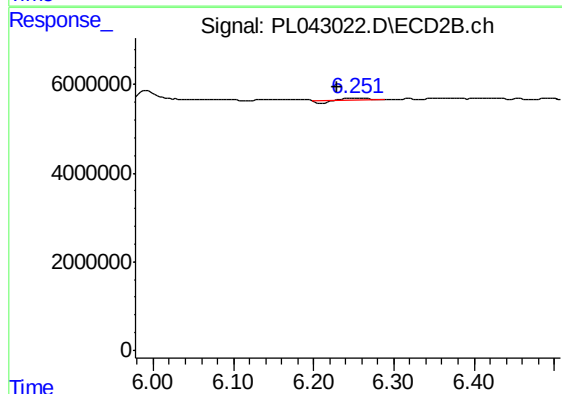


#10 gamma-Chlordane

R.T.: 6.255 min
Delta R.T.: 0.025 min
Response: 448289
Conc: 0.12 ng/ml

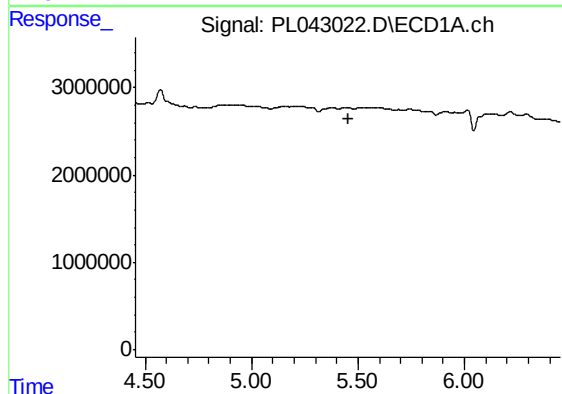


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

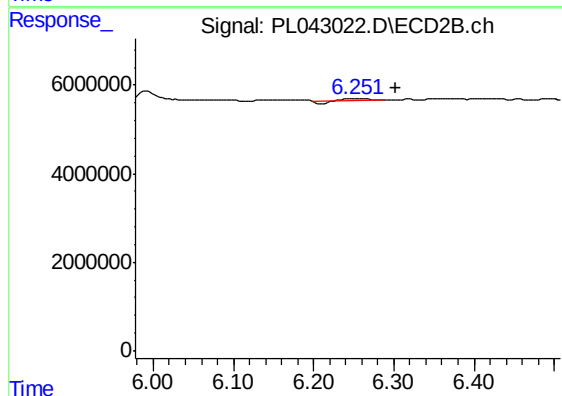

#11 alpha-Chlordane


R.T.: 6.255 min
Delta R.T.: -0.048 min
Response: 448289
Conc: 0.12 ng/ml

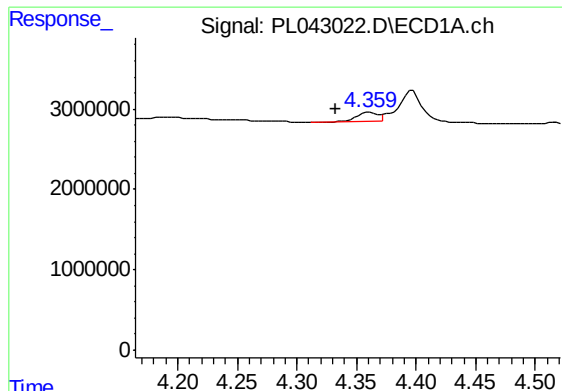

#23 Chlordane-1


R.T.: 4.361 min
Delta R.T.: 0.028 min
Response: 1157268
Conc: 4.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB115576BL

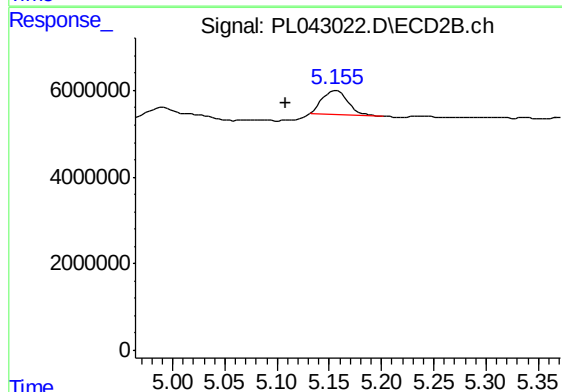


#23 Chlordane-1

R.T.: 5.156 min
Delta R.T.: 0.048 min
Response: 9559445
Conc: 67.64 ng/ml

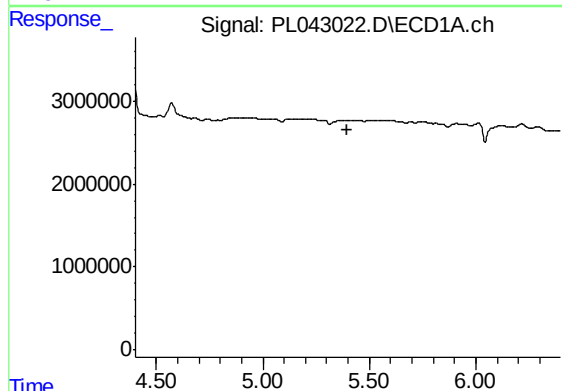


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

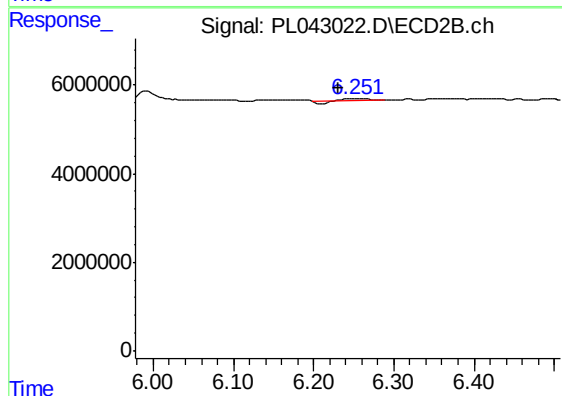

#25 Chlordane-3


R.T.: 6.255 min
Delta R.T.: 0.025 min
Response: 448289
Conc: 0.91 ng/ml

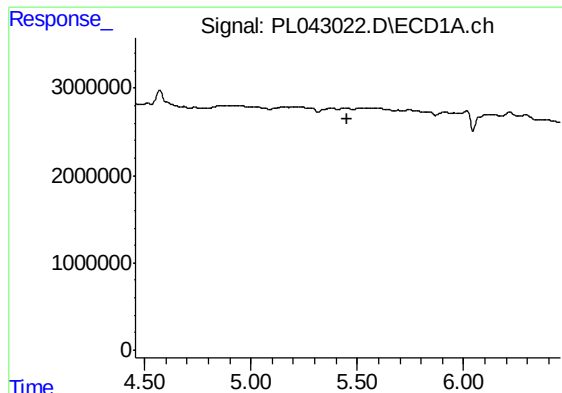

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB115576BL

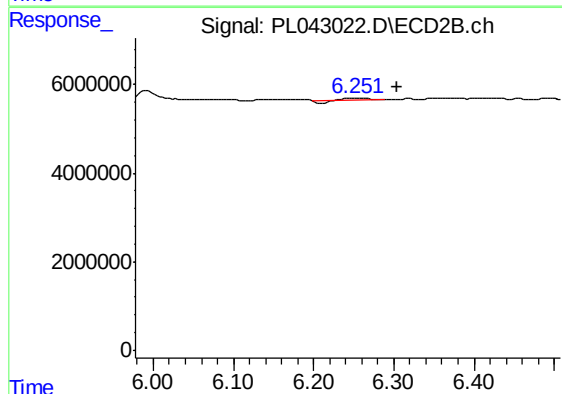


#26 Chlordane-4

R.T.: 6.255 min
Delta R.T.: -0.050 min
Response: 448289
Conc: 0.79 ng/ml

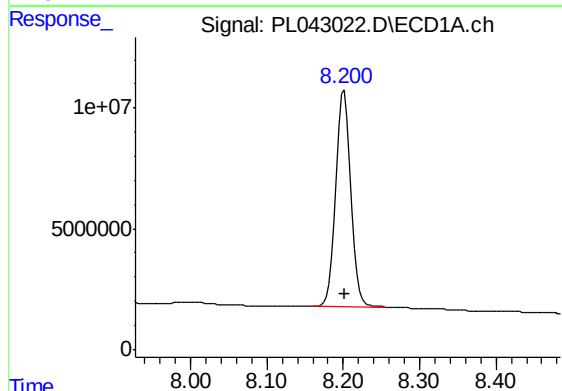

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 121499584
Conc: 18.61 ng/ml

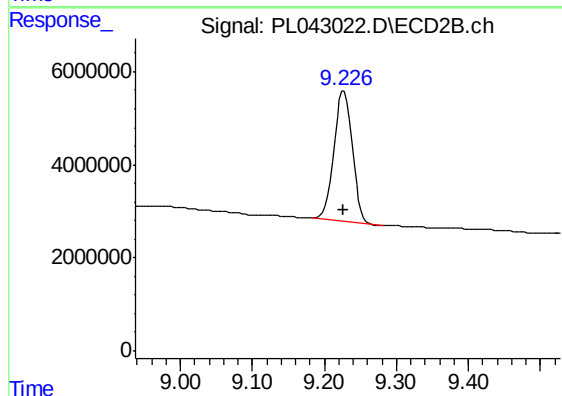

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 49505625
Conc: 18.98 ng/ml