

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
 Data File : PL043038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2018 19:47
 Operator : AJ\SJ
 Sample : J6340-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-02A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 02:52:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	120.7E6	60772562	19.687	20.504
28)	SA Decachlor...	8.201	9.229	108.6E6	43207930	16.628	16.564
Target Compounds							
2)	A alpha-BHC	3.858f	0.000	268493	0	0.028	N.D. #
3)	MA gamma-BHC...	4.196	0.000	4168185	0	0.483	N.D. #
6)	B beta-BHC	4.398f	4.903f	2986729	528971	0.810	0.312 #
7)	B delta-BHC	0.000	5.160	0	23428996	N.D.	5.452 #
8)	B Heptachlo...	5.241f	5.991	4531039	15142860	0.572	3.993 #
9)	A Endosulfan I	5.539	6.305f	3051649	3613400	0.417	1.064 #
10)	B gamma-Chl...	5.399	6.225	2222276	5065656	0.276	1.379 #
11)	B alpha-Chl...	5.454	6.305	4414093	3613400	0.556	1.005 #
13)	MA Dieldrin	5.742	0.000	10068448	0	1.295	N.D. #
14)	MA Endrin	6.005	0.000	3477019	0	0.483	N.D. #
16)	A 4,4'-DDD	6.093f	6.956	501743	8317147	0.088	2.836 #
17)	MA 4,4'-DDT	6.369	7.301f	6781051	3406245	1.140	1.160
19)	B Endosulfa...	6.655	0.000	5995176	0	0.895	N.D. #
20)	A Methoxychlor	6.901	0.000	6971514	0	2.078	N.D. #
21)	B Endrin ke...	7.174	7.822f	2441442	6459123	0.338	2.113 #
23)	Chlordane-1	4.338	5.160	565656	23428996	2.105	165.772 #
24)	Chlordane-2	0.000	5.521	0	3315668	N.D.	23.115 #
25)	Chlordane-3	5.399	6.225	2222276	5065656	2.674	10.315 #
26)	Chlordane-4	5.454	6.305	4414093	3613400	5.838	6.331


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
Data File : PL043038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2018 19:47
Operator : AJ\SJ
Sample : J6340-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SB-02A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 02:52:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

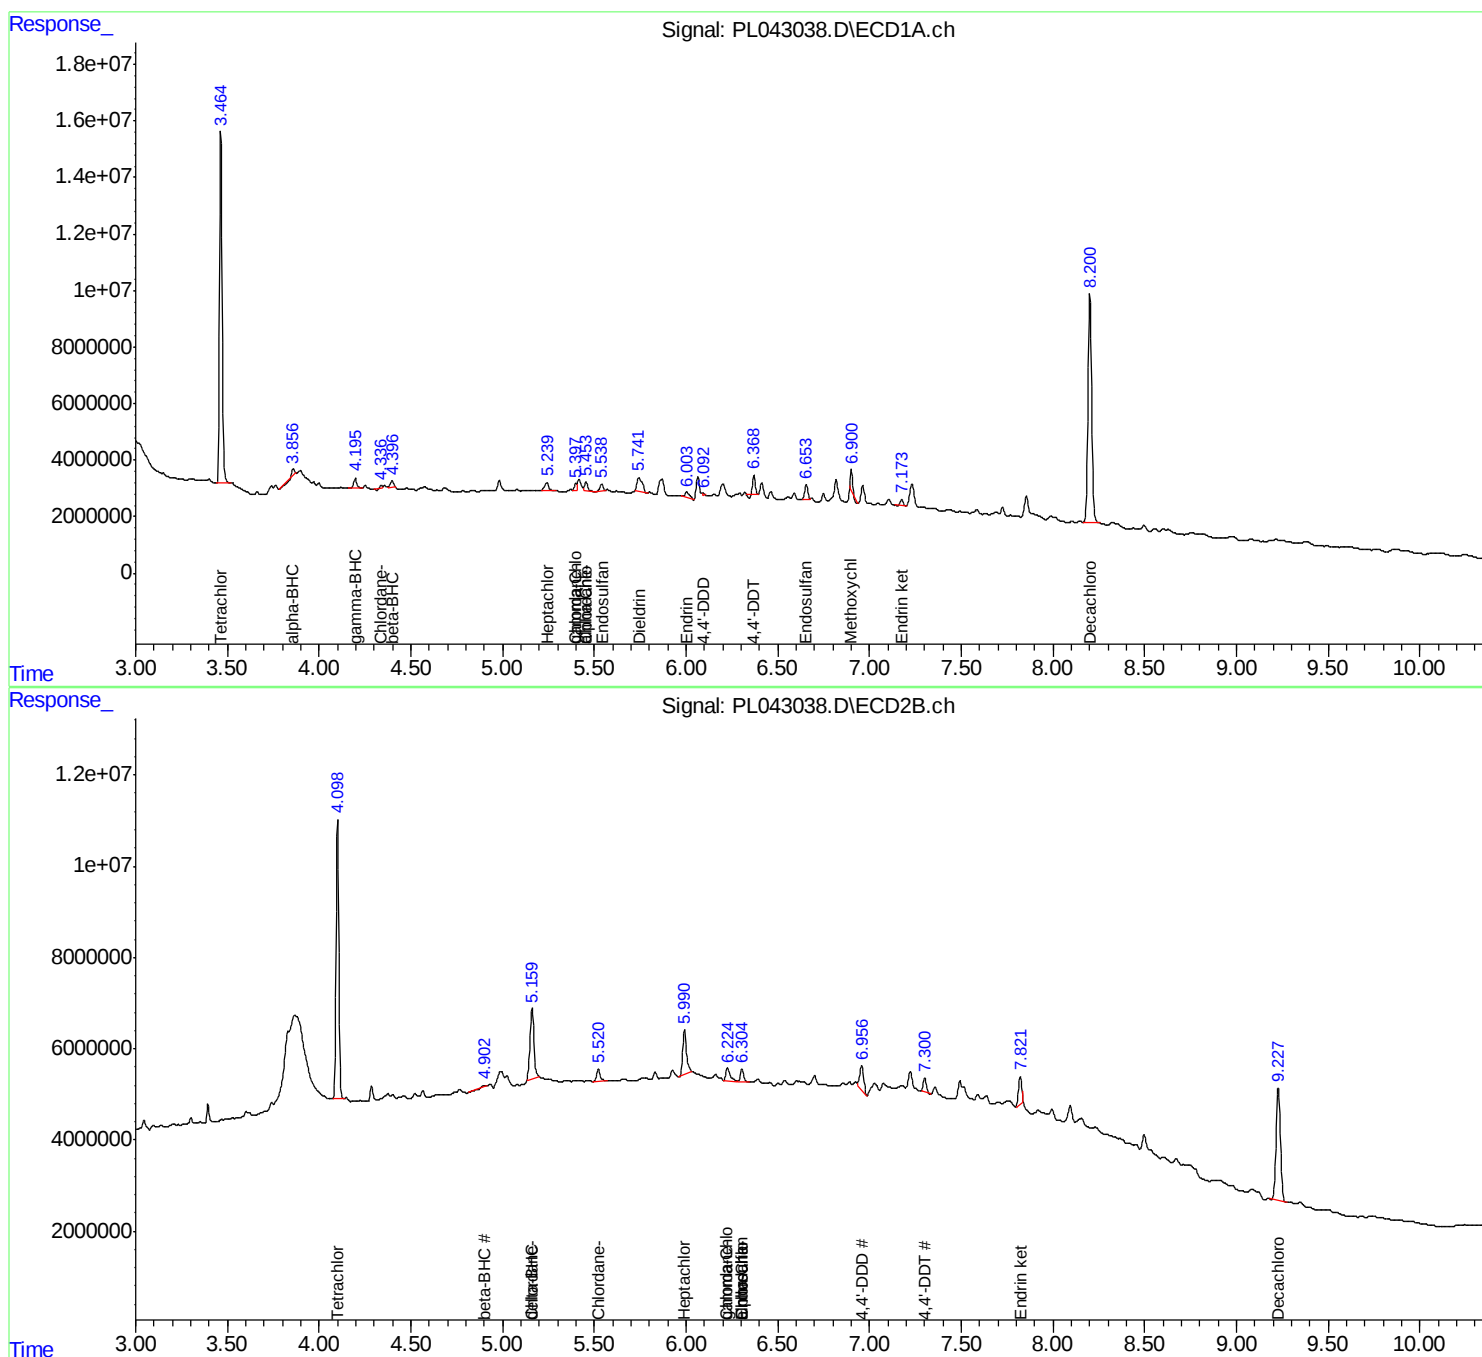


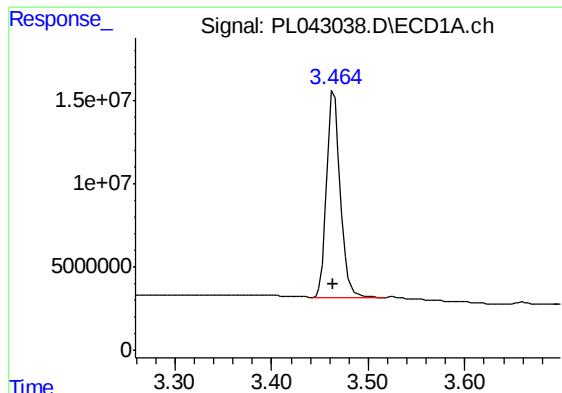

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 120736657
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-02A

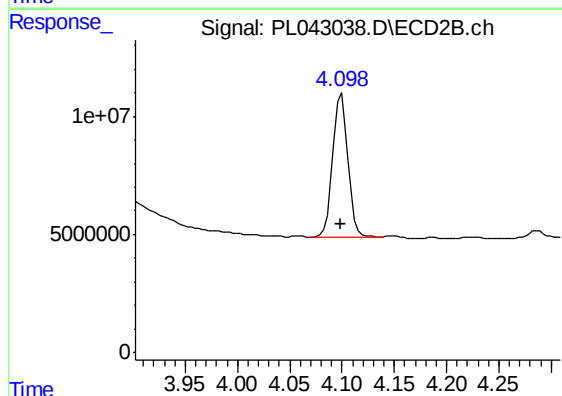


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 60772562
Conc: 20.50 ng/ml

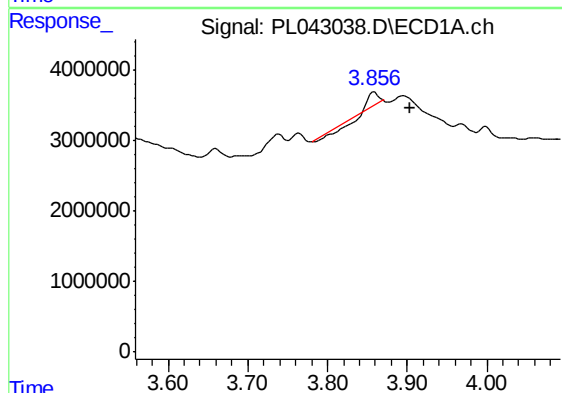


#2 alpha-BHC

R.T.: 3.858 min
Delta R.T.: -0.046 min
Response: 268493
Conc: 0.03 ng/ml

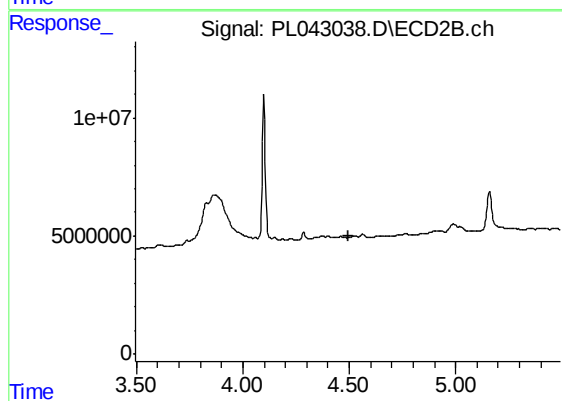

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

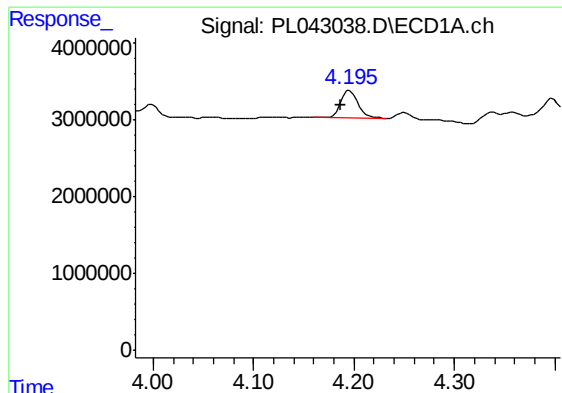

#3 gamma-BHC (Lindane)


R.T.: 4.196 min
Delta R.T.: 0.009 min
Response: 4168185
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-02A

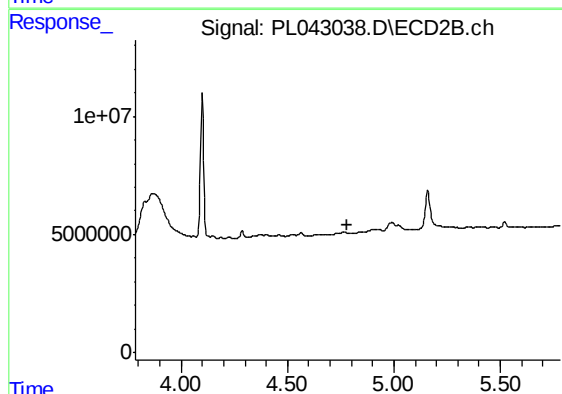


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

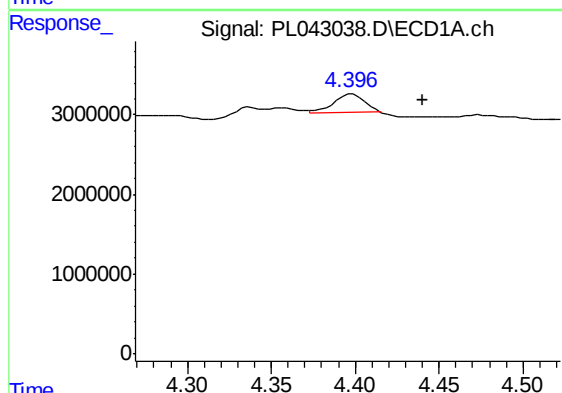

#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.043 min
Response: 2986729
Conc: 0.81 ng/ml

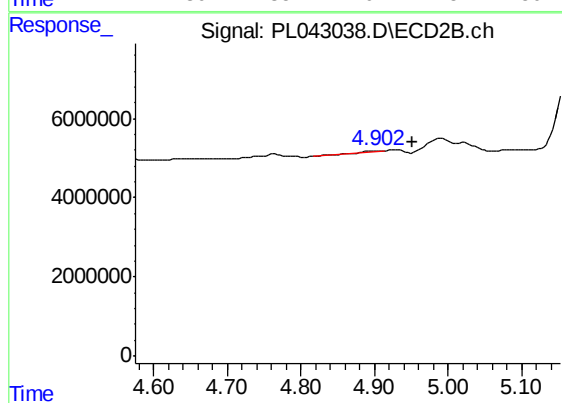

#6 beta-BHC

R.T.: 4.903 min
Delta R.T.: -0.048 min
Response: 528971
Conc: 0.31 ng/ml