

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
 Data File : PL043058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2018 00:30
 Operator : AJ\SJ
 Sample : J5193-08
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:25:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.099	126.2E6	63584137	20.579	21.453
28)	SA Decachlor...	8.200	9.227	124.1E6	51048457	19.009	19.570
Target Compounds							
6)	B beta-BHC	4.397f	0.000	2260065	0	0.613	N.D. #
7)	B delta-BHC	0.000	5.157	0	4937398	N.D.	1.149 #
8)	B Heptachlo...	0.000	5.991	0	4884394	N.D.	1.288 #
13)	MA Dieldrin	5.694f	0.000	474137	0	0.061	N.D. #
23)	Chlordane-1	4.361	5.157	2508649	4937398	9.336	34.935 #
24)	Chlordane-2	4.840	0.000	412011	0	1.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121218\
Data File : PL043058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2018 00:30
Operator : AJ\SJ
Sample : J5193-08
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:25:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

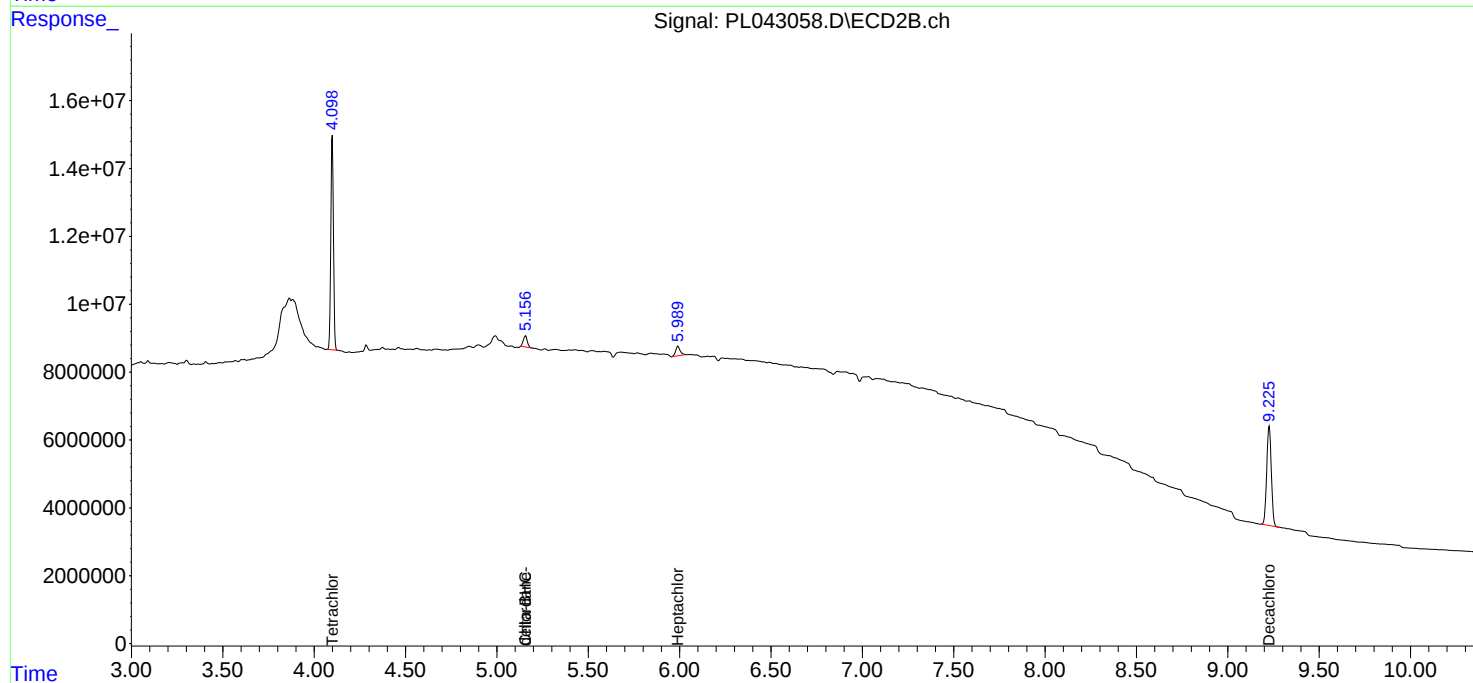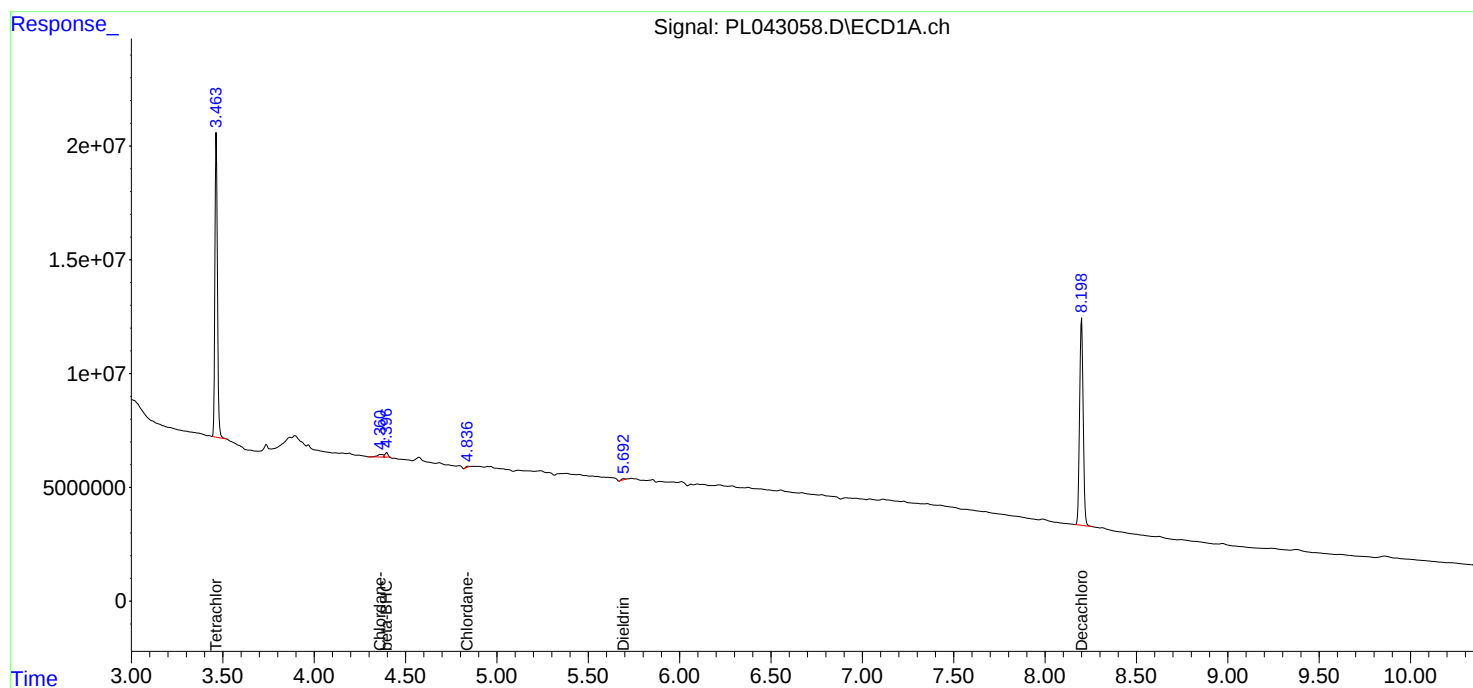


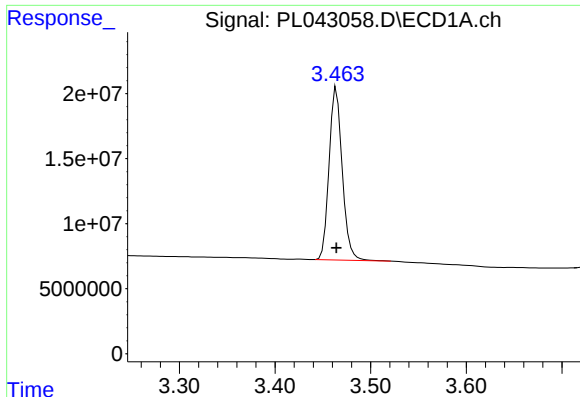

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 126208797
Conc: 20.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

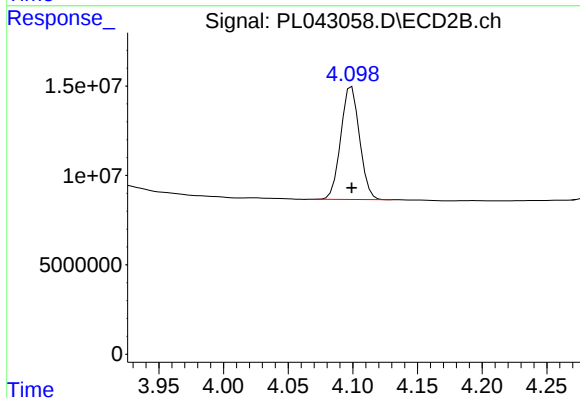


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 63584137
Conc: 21.45 ng/ml

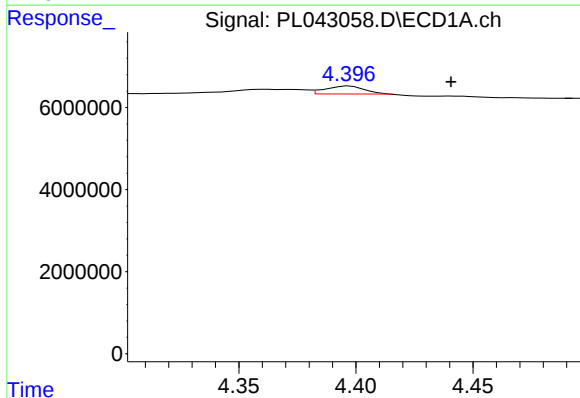


#6 beta-BHC

R.T.: 4.397 min
Delta R.T.: -0.043 min
Response: 2260065
Conc: 0.61 ng/ml

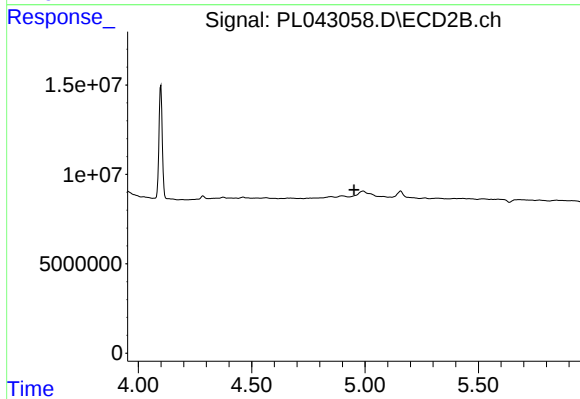

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

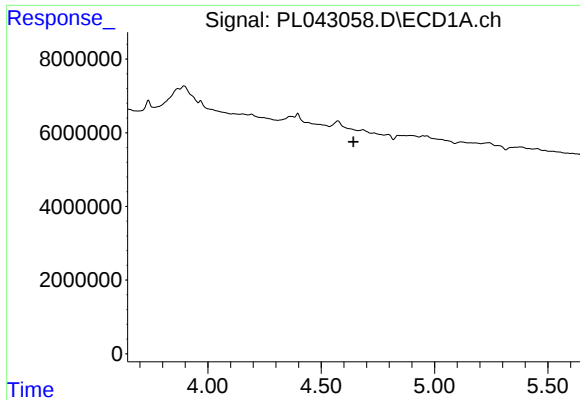

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

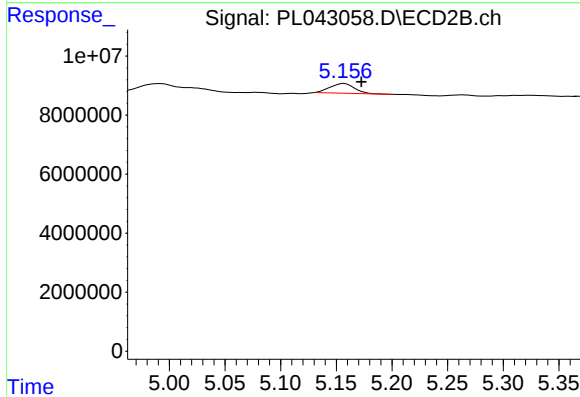


#7 delta-BHC

R.T.: 5.157 min
Delta R.T.: -0.016 min
Response: 4937398
Conc: 1.15 ng/ml

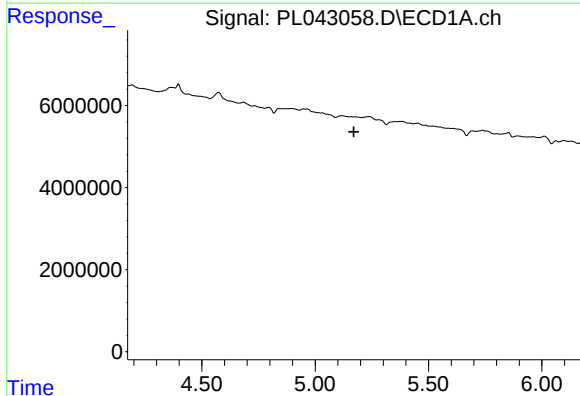


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

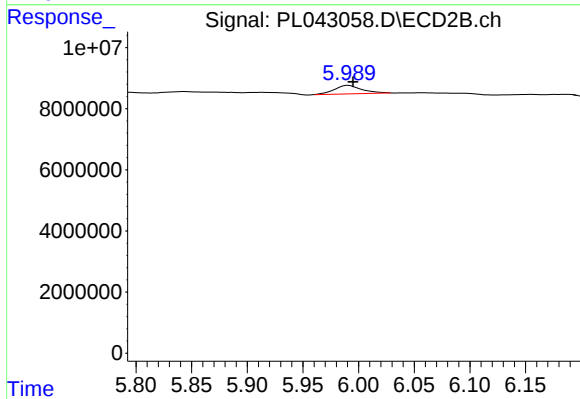

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.004 min
Response: 4884394
Conc: 1.29 ng/ml

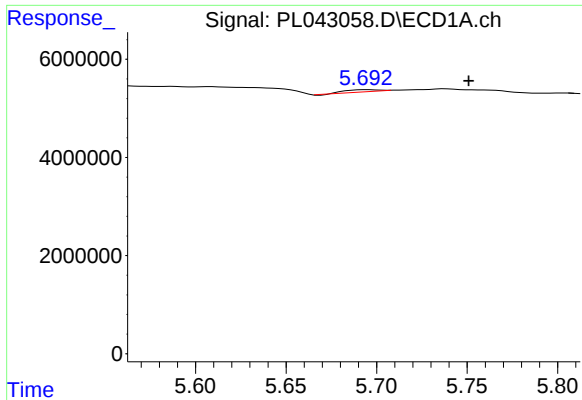

#13 Dieldrin


R.T.: 5.694 min
Delta R.T.: -0.057 min
Response: 474137
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

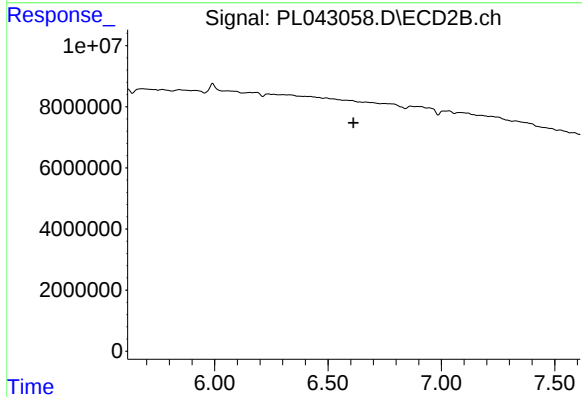


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

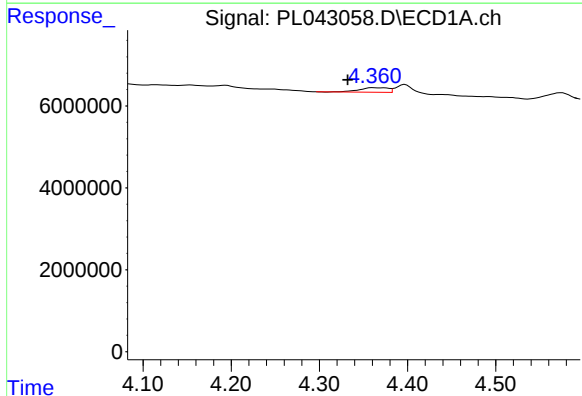


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.029 min
Response: 2508649
Conc: 9.34 ng/ml

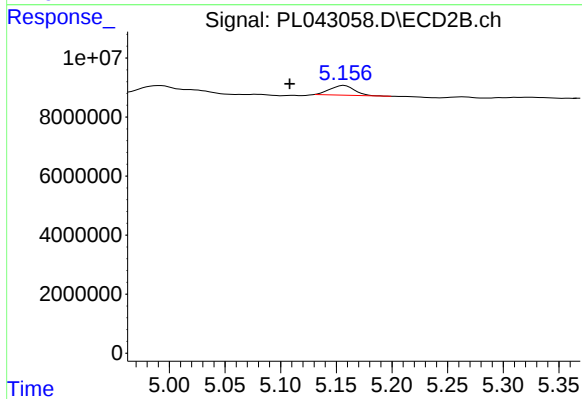

#23 Chlordane-1


R.T.: 5.157 min
Delta R.T.: 0.049 min
Response: 4937398
Conc: 34.93 ng/ml

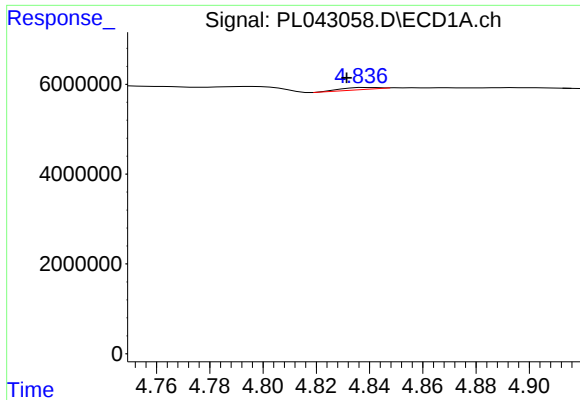

#24 Chlordane-2


R.T.: 4.840 min
Delta R.T.: 0.008 min
Response: 412011
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

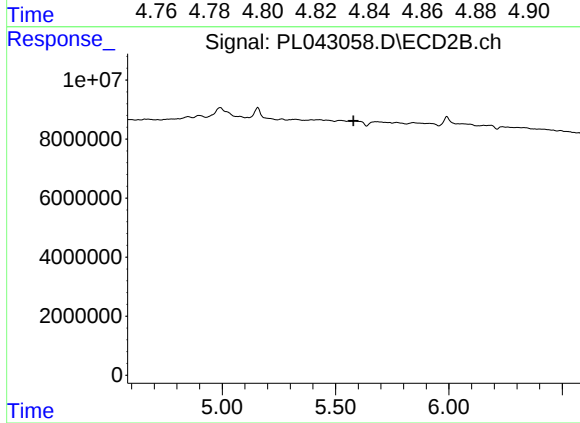


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.579 min
Response: 0
Conc: N.D.

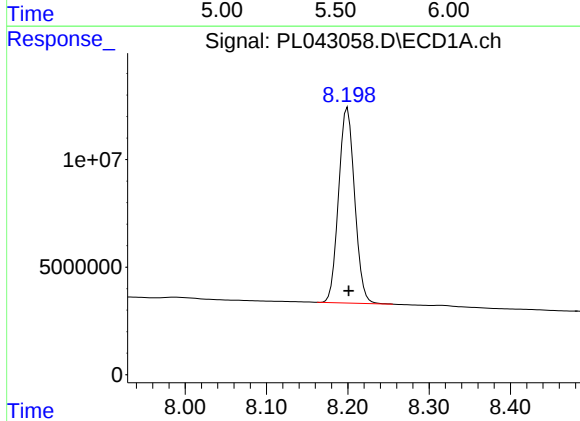

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.001 min
Response: 124130310
Conc: 19.01 ng/ml

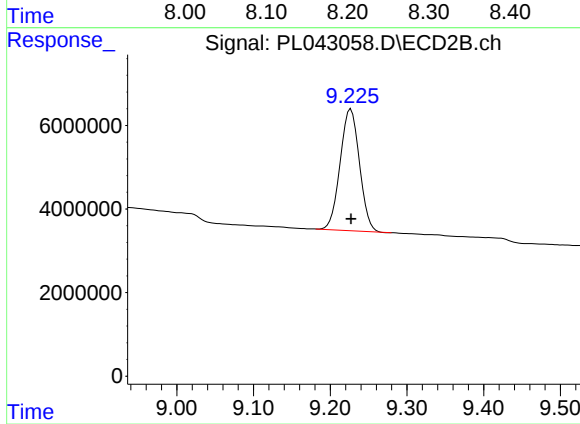

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 51048457
Conc: 19.57 ng/ml