

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121219\
 Data File : PL054954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2019 09:23
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:29:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
6) B	beta-BHC	4.509	0.000	3649415	0	0.492	N.D. #
8) B	Heptachlo...	5.267	5.918	18157068	48905684	1.200	19.576 #
9) A	Endosulfan I	5.606	6.276	66508907	21099112	4.877	8.530 #
10) B	gamma-Chl...	0.000	6.177	0	18546961	N.D.	7.040 #
12) B	4,4'-DDE	5.735f	0.000	29949372	0	2.251	N.D. #
14) MA	Endrin	6.107	6.749f	11206678	7994476	0.880	3.609 #
15) B	Endosulfa...	6.408f	0.000	11156959	0	0.922	N.D. #
24)	Chlordane-2	4.939f	0.000	54224672	0	124.868	N.D. #
25)	Chlordane-3	0.000	6.177	0	18546961	N.D.	59.752 #
27)	Chlordane-5	6.408	0.000	11156959	0	29.633	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121219\
Data File : PL054954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2019 09:23
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:29:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

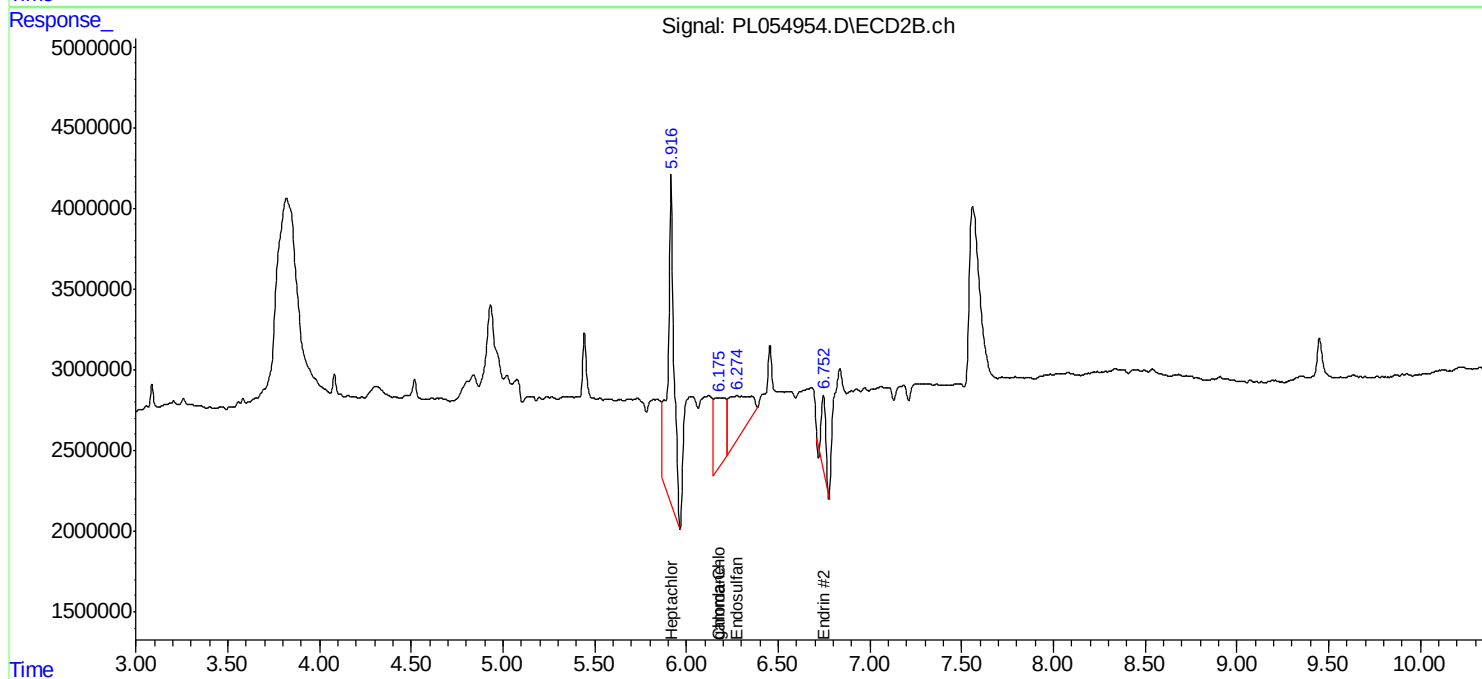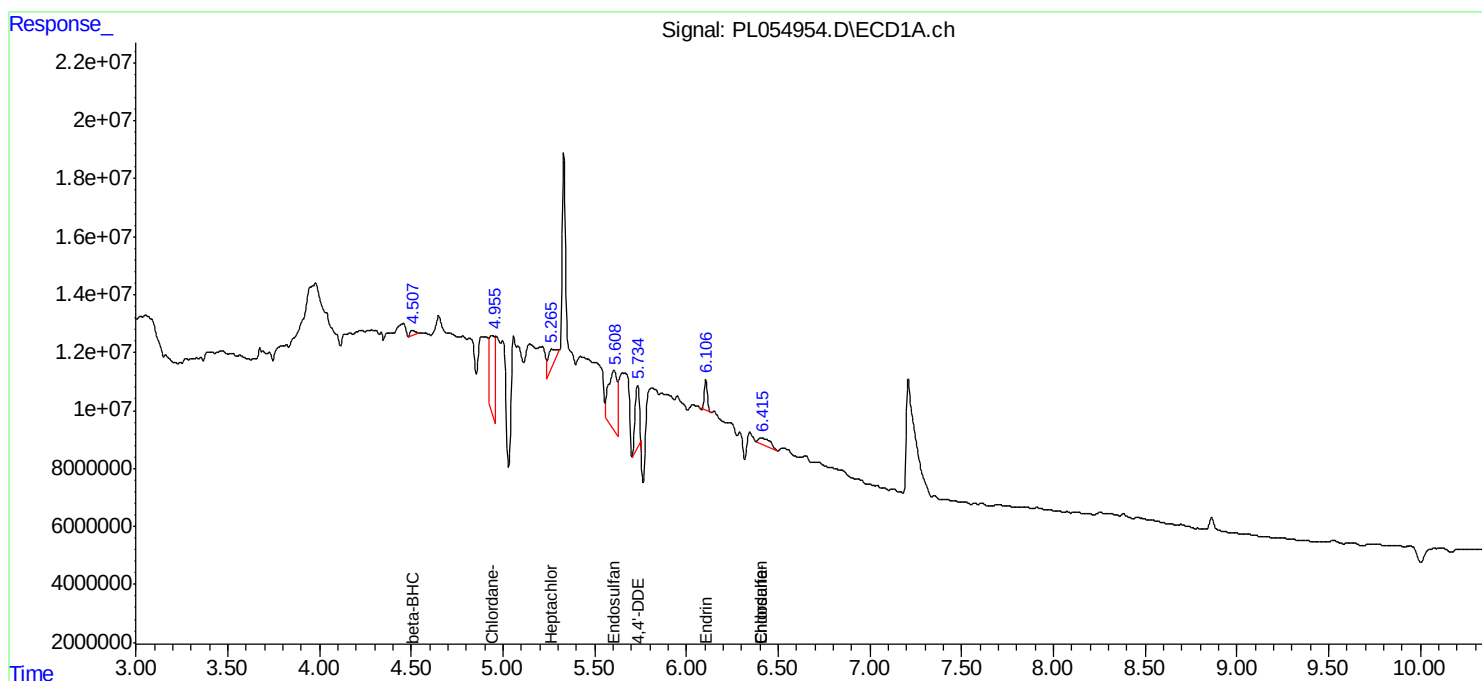


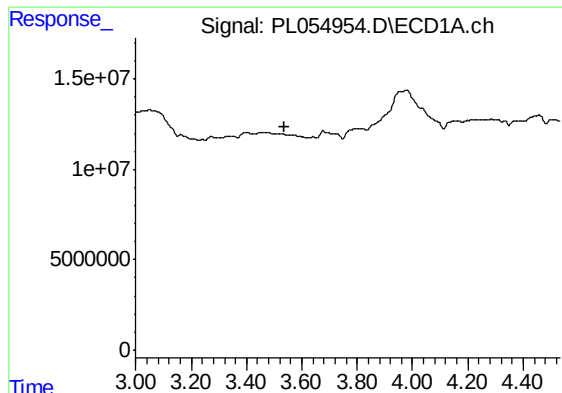

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

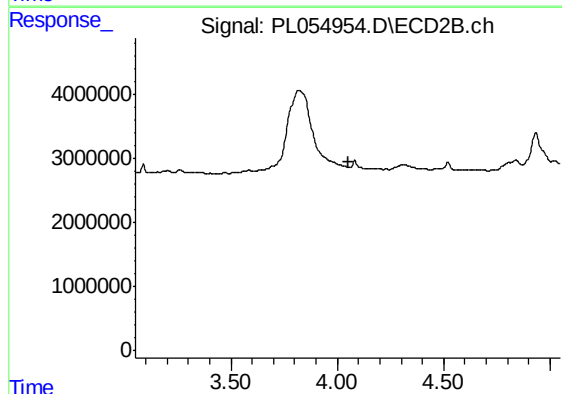


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.052 min
Response: 0
Conc: N.D.

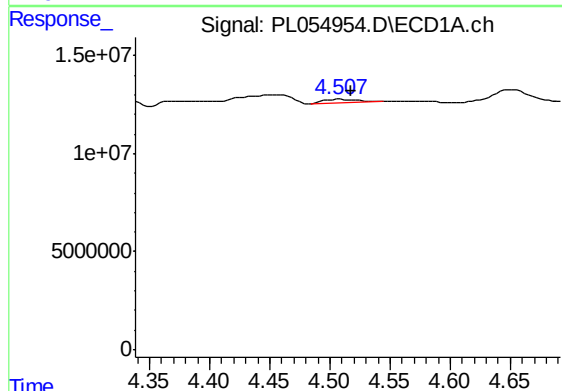


#6 beta-BHC

R.T.: 4.509 min
Delta R.T.: -0.009 min
Response: 3649415
Conc: 0.49 ng/ml

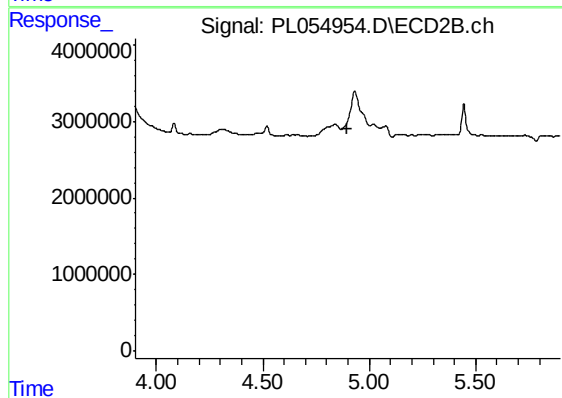

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.899 min
Response: 0
Conc: N.D.

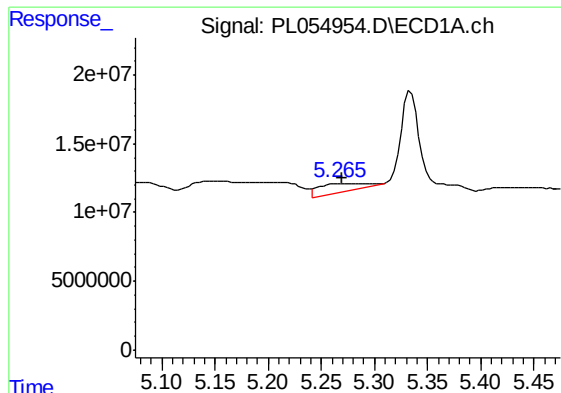

#8 Heptachlor epoxide


R.T.: 5.267 min
Delta R.T.: -0.002 min
Response: 18157068
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

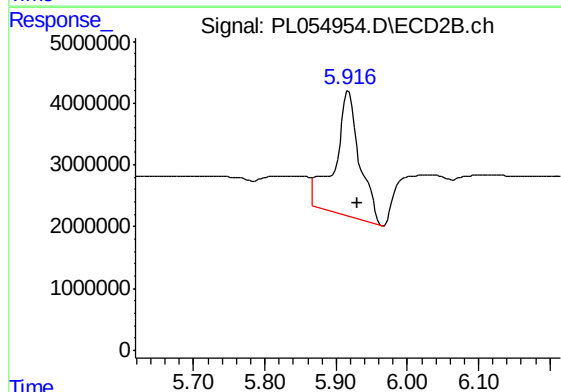


#8 Heptachlor epoxide

R.T.: 5.918 min
Delta R.T.: -0.013 min
Response: 48905684
Conc: 19.58 ng/ml

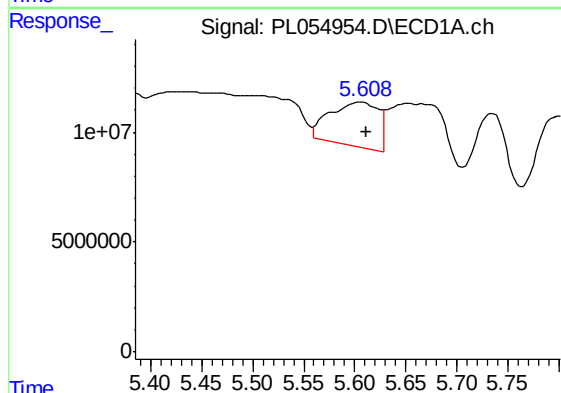


#9 Endosulfan I

R.T.: 5.606 min
Delta R.T.: -0.006 min
Response: 66508907
Conc: 4.88 ng/ml

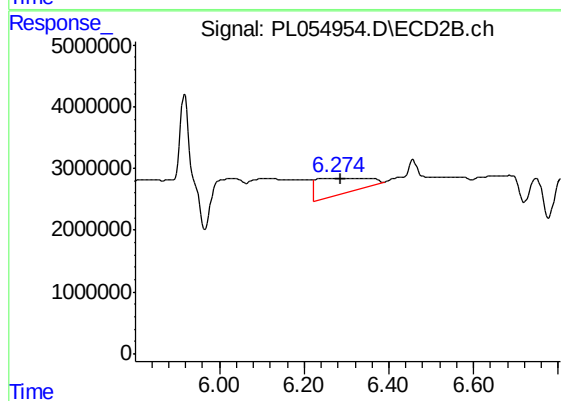

#9 Endosulfan I


R.T.: 6.276 min
Delta R.T.: -0.012 min
Response: 21099112
Conc: 8.53 ng/ml

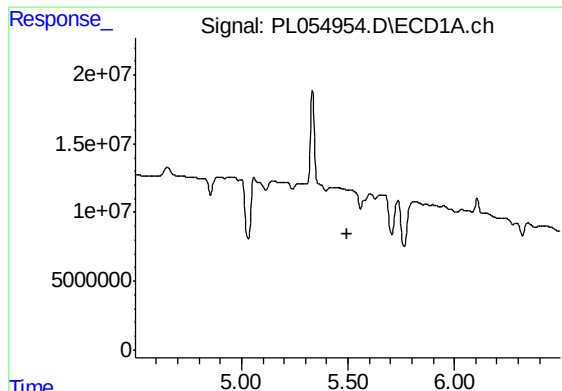

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

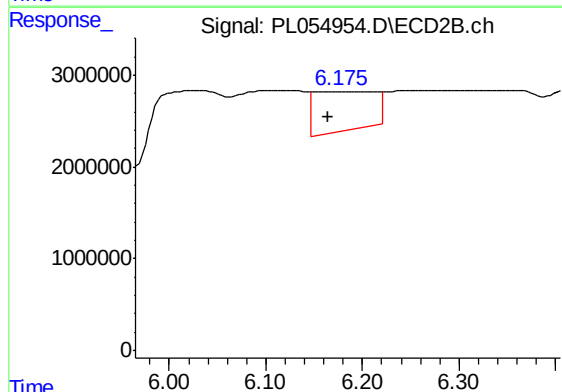


#10 gamma-Chlordane

R.T.: 6.177 min
Delta R.T.: 0.013 min
Response: 18546961
Conc: 7.04 ng/ml

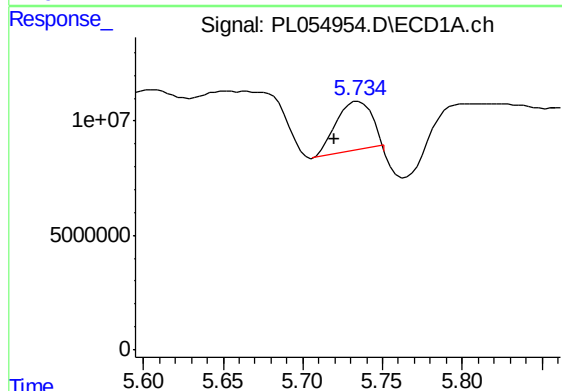


#12 4,4'-DDE

R.T.: 5.735 min
Delta R.T.: 0.015 min
Response: 29949372
Conc: 2.25 ng/ml

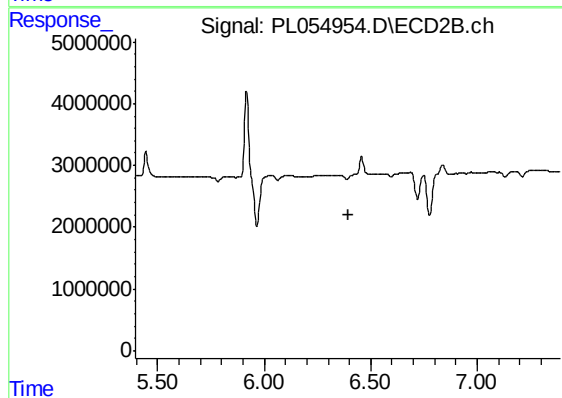

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

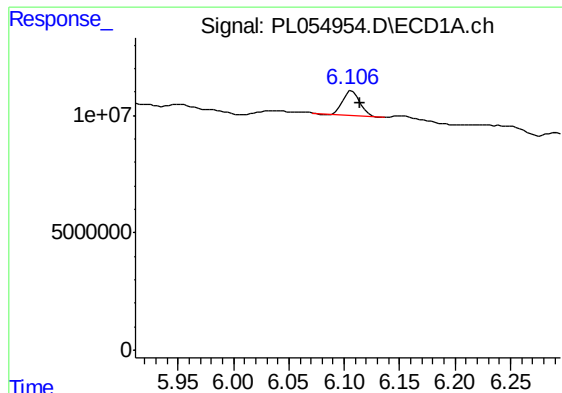

#14 Endrin


R.T.: 6.107 min
Delta R.T.: -0.007 min
Response: 11206678
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

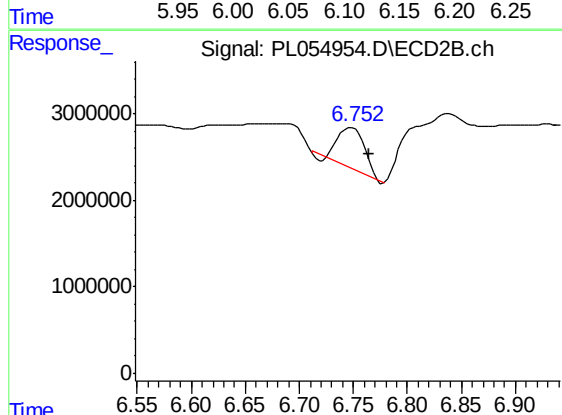


#14 Endrin

R.T.: 6.749 min
Delta R.T.: -0.015 min
Response: 7994476
Conc: 3.61 ng/ml

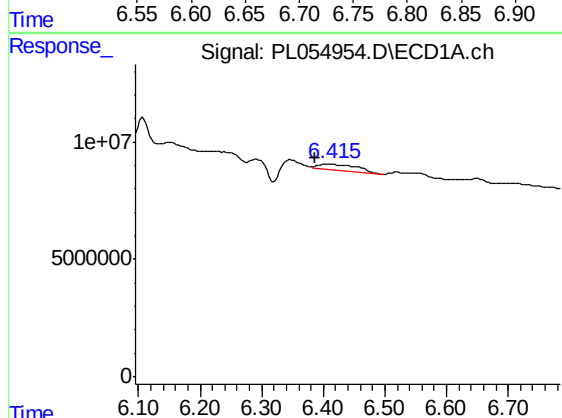


#15 Endosulfan II

R.T.: 6.408 min
Delta R.T.: 0.021 min
Response: 11156959
Conc: 0.92 ng/ml

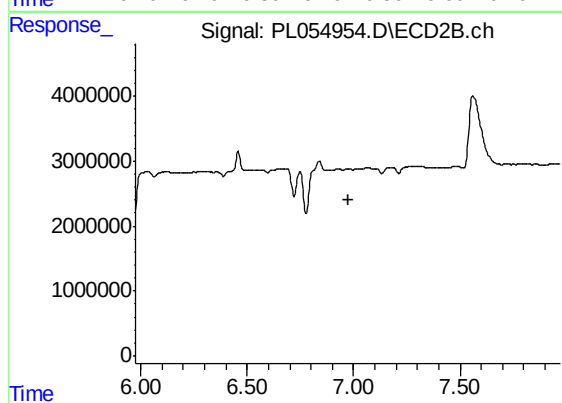

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.974 min
Response: 0
Conc: N.D.

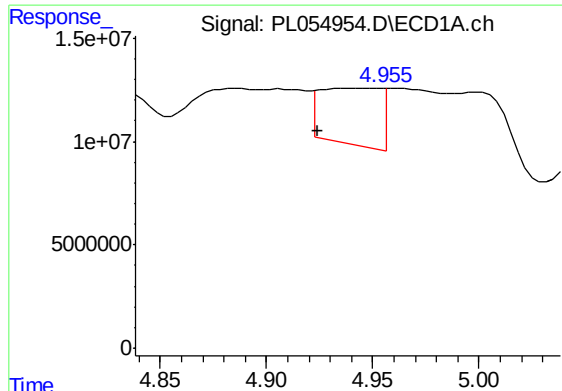

#24 Chlordane-2


R.T.: 4.939 min
Delta R.T.: 0.015 min
Response: 54224672
Conc: 124.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

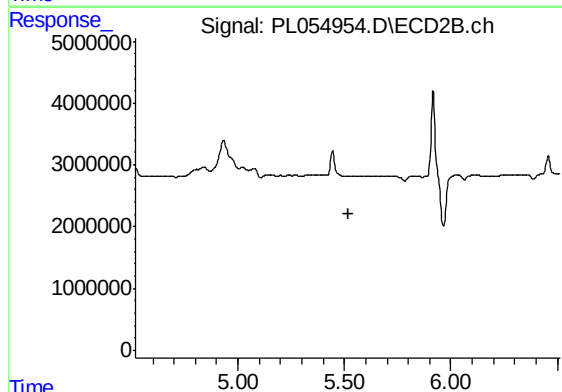


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.517 min
Response: 0
Conc: N.D.

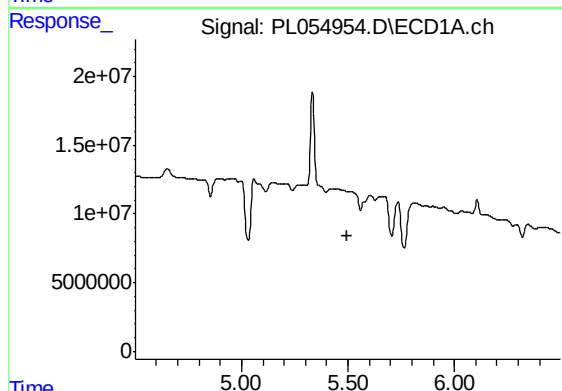


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

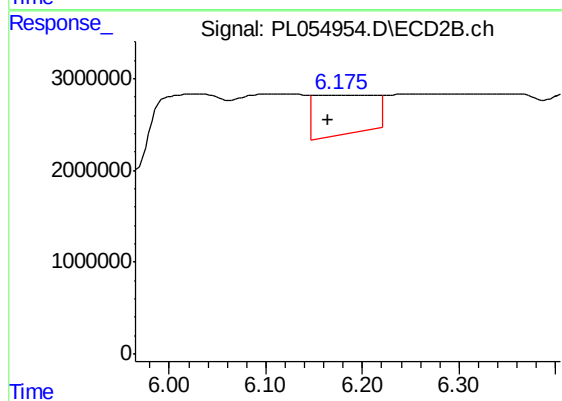

#25 Chlordane-3


R.T.: 6.177 min
Delta R.T.: 0.013 min
Response: 18546961
Conc: 59.75 ng/ml

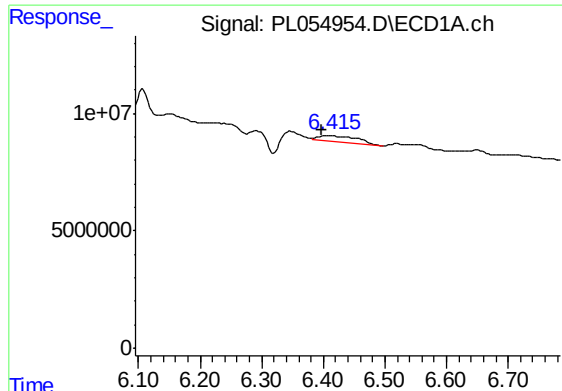

#27 Chlordane-5


R.T.: 6.408 min
Delta R.T.: 0.011 min
Response: 11156959
Conc: 29.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

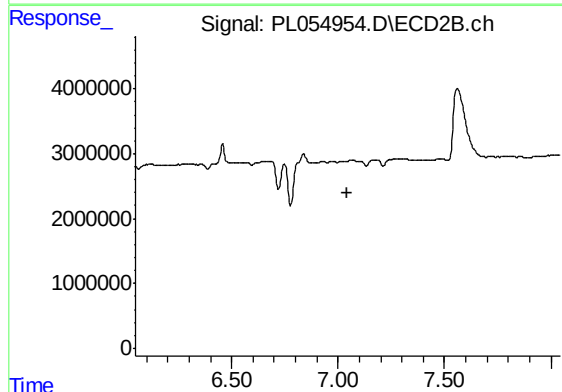


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

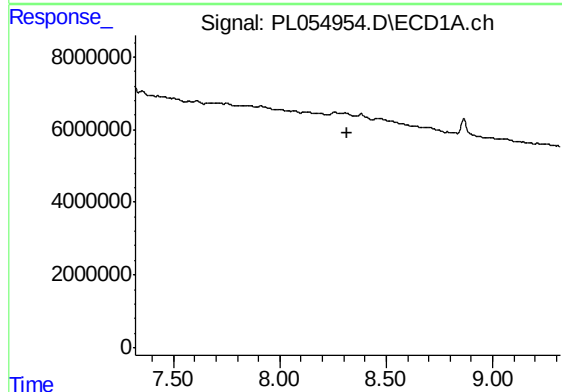

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.320 min
Response: 0
Conc: N.D.

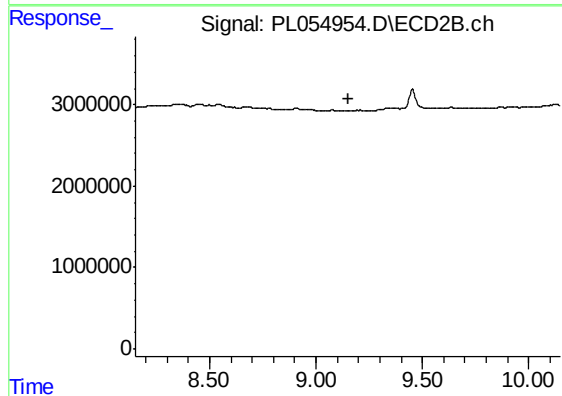

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.152 min
Response: 0
Conc: N.D.