

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 10:25
 Operator : DD\AJ
 Sample : L4977-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 12:09:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.408	3.949	24050111	42469248	14.133	13.550
28)	SA Decachlor...	8.123	8.988	29497105	40127086	14.647	15.934
Target Compounds							
6)	B beta-BHC	0.000	4.819f	0	230595	N.D.	0.116 #
8)	B Heptachlo...	0.000	5.807	0	9784749	N.D.	2.702 #
10)	B gamma-Chl...	0.000	6.061	0	12985438	N.D.	3.659 #
13)	MA Dieldrin	5.670	0.000	6035158	0	3.315	N.D. #
23)	Chlordane-1	0.000	4.942	0	171830	N.D.	1.498 #
25)	Chlordane-3	0.000	6.061	0	12985438	N.D.	28.181 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 10:25
Operator : DD\AJ
Sample : L4977-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 12:09:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

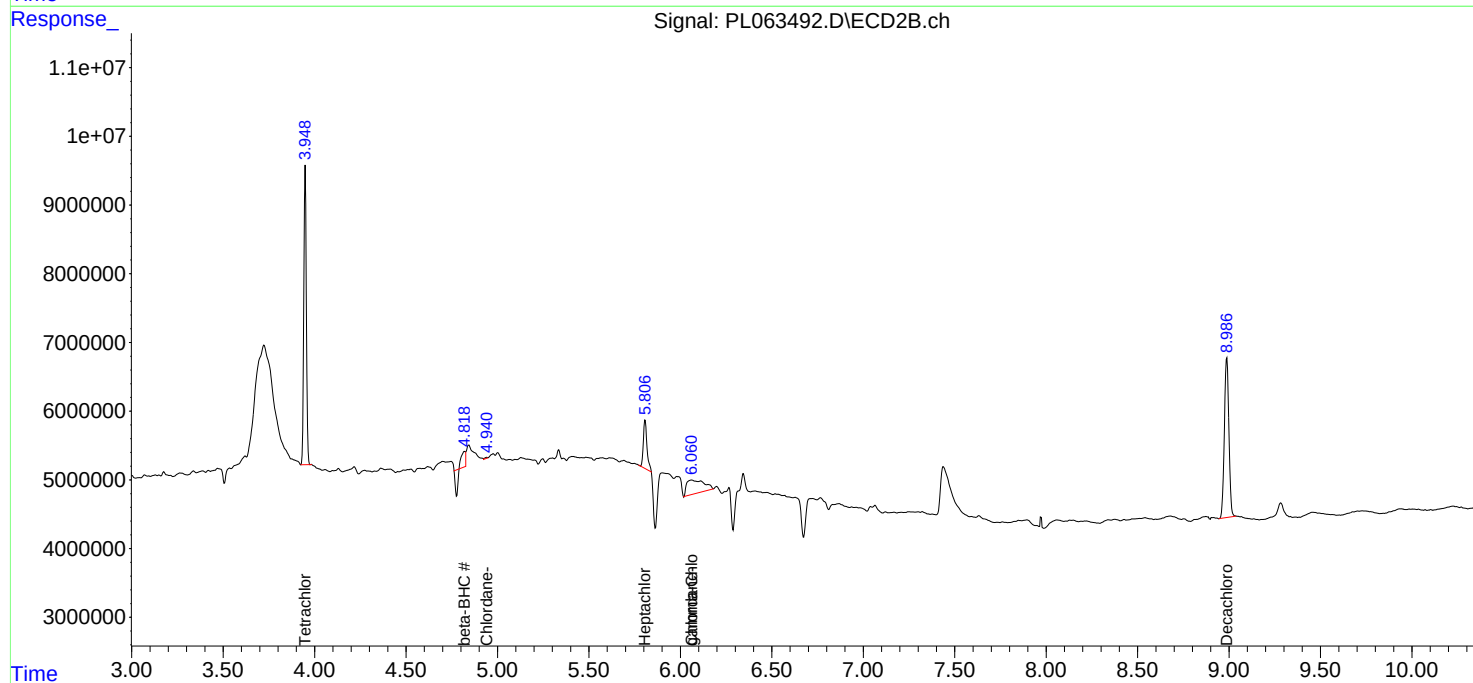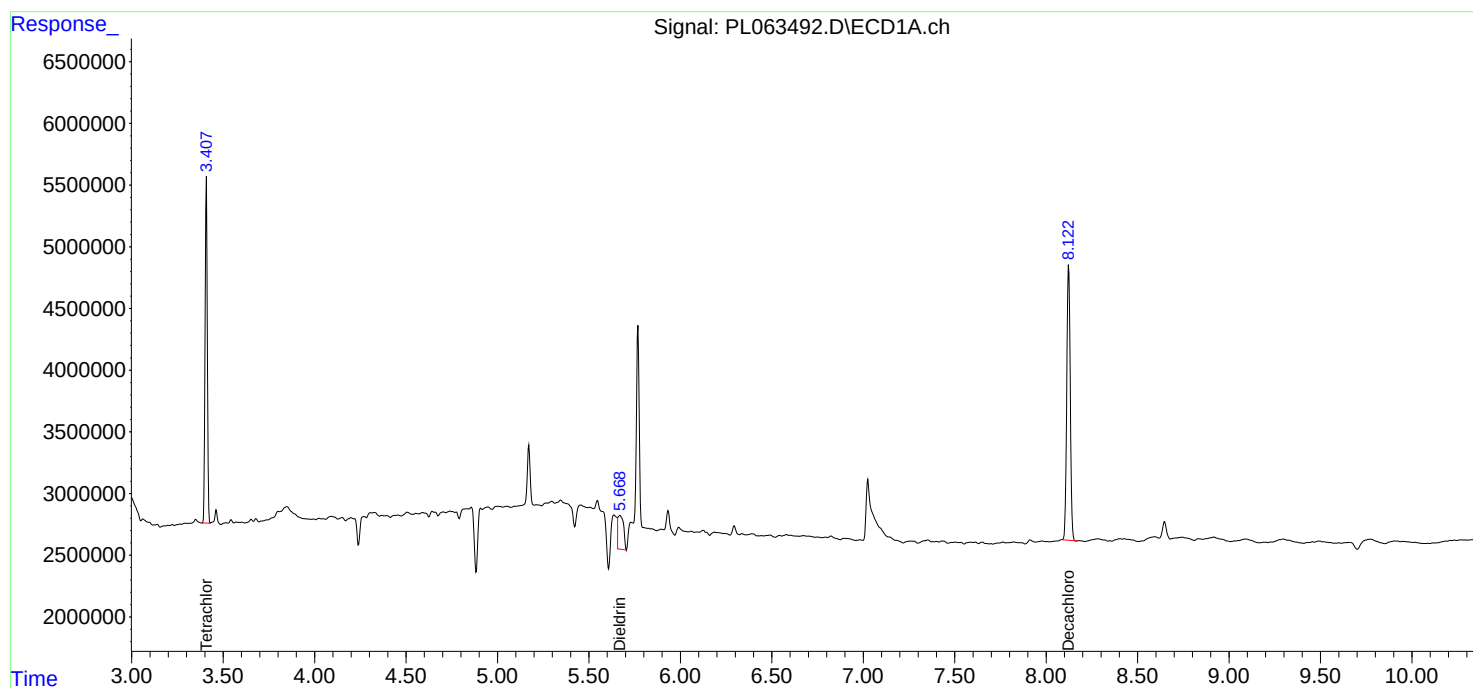


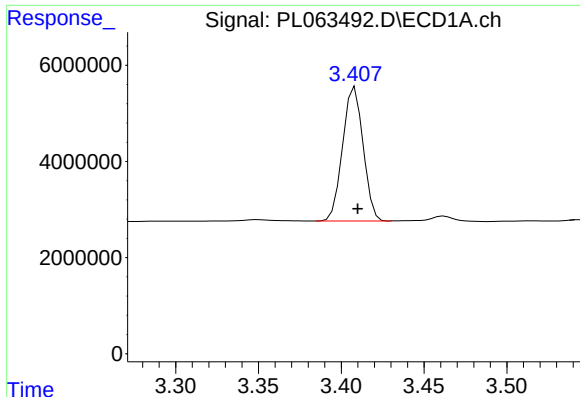

#1 Tetrachloro-m-xylene


R.T.: 3.408 min
Delta R.T.: -0.002 min
Response: 24050111
Conc: 14.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

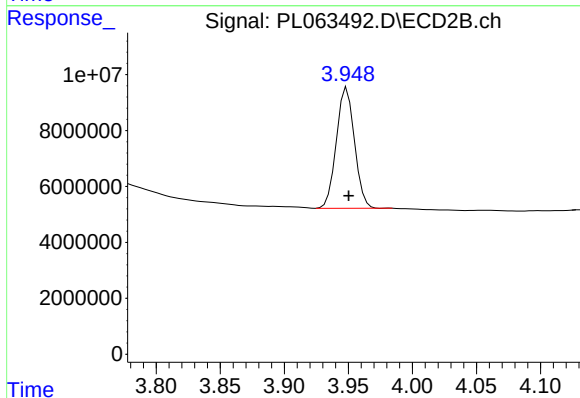


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 42469248
Conc: 13.55 ng/ml

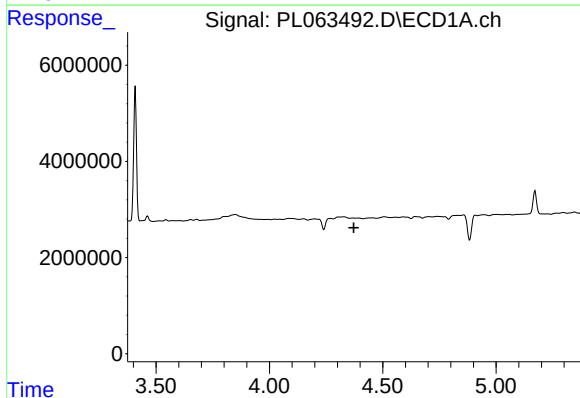


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

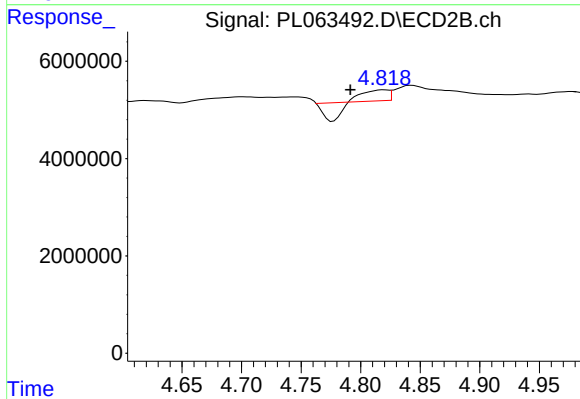

#6 beta-BHC


R.T.: 4.819 min
Delta R.T.: 0.028 min
Response: 230595
Conc: 0.12 ng/ml

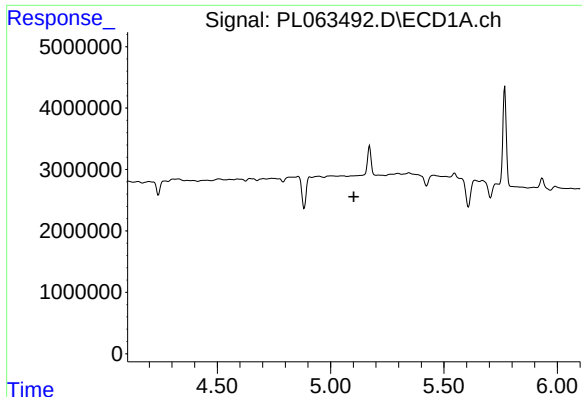

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

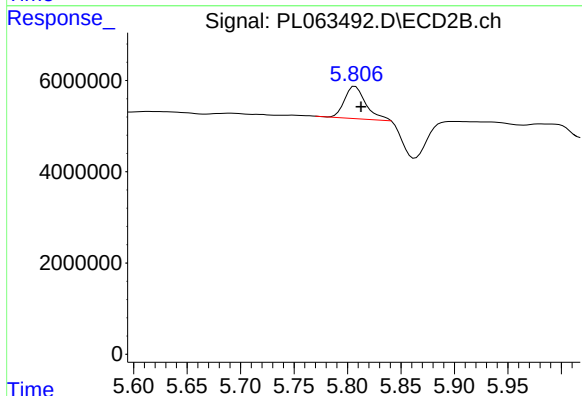


#8 Heptachlor epoxide

R.T.: 5.807 min
Delta R.T.: -0.005 min
Response: 9784749
Conc: 2.70 ng/ml

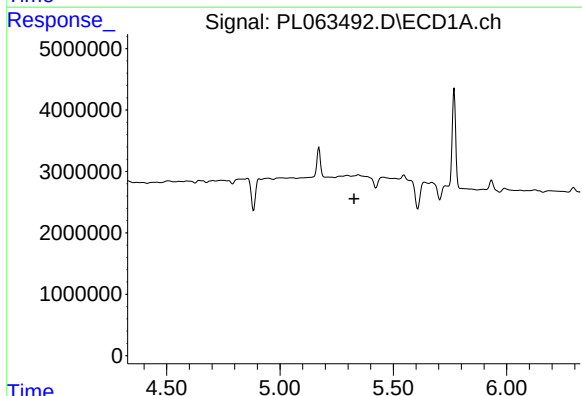


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

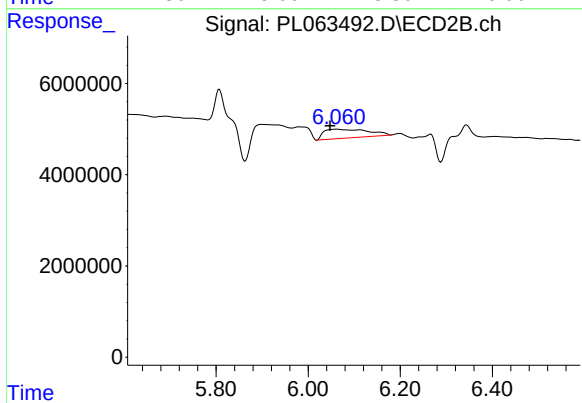

#10 gamma-Chlordane


R.T.: 6.061 min
Delta R.T.: 0.013 min
Response: 12985438
Conc: 3.66 ng/ml

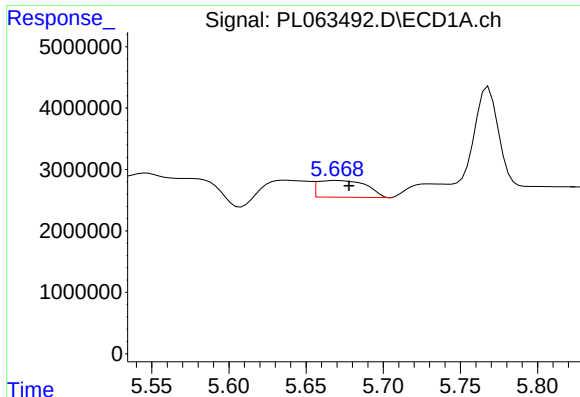

#13 Dieldrin


R.T.: 5.670 min
Delta R.T.: -0.008 min
Response: 6035158
Conc: 3.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

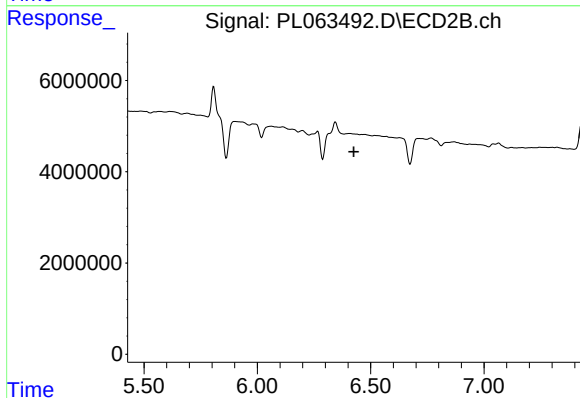


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.426 min
Response: 0
Conc: N.D.

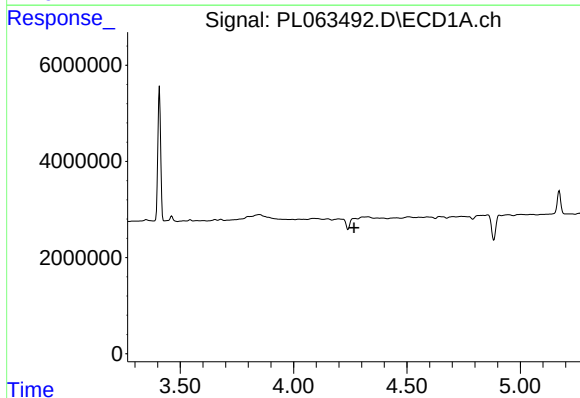


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.267 min
Response: 0
Conc: N.D.

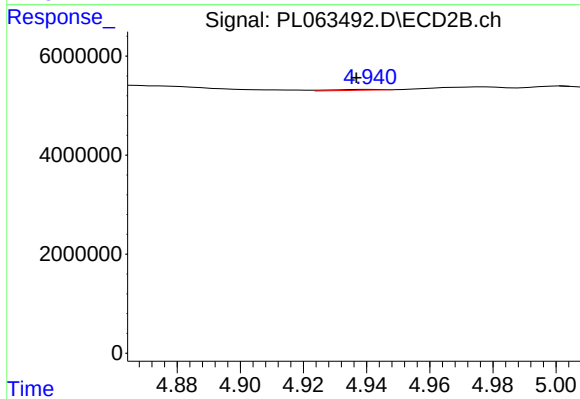

#23 Chlordane-1


R.T.: 4.942 min
Delta R.T.: 0.005 min
Response: 171830
Conc: 1.50 ng/ml

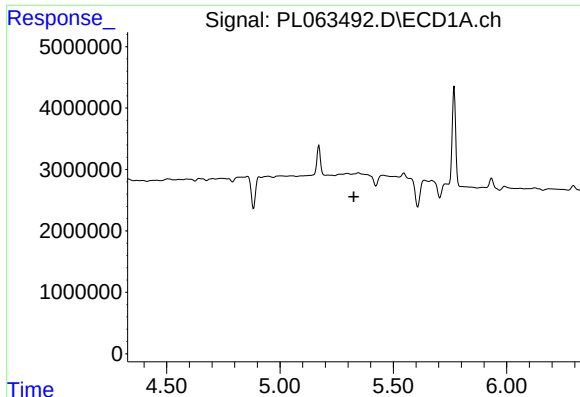

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.326 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

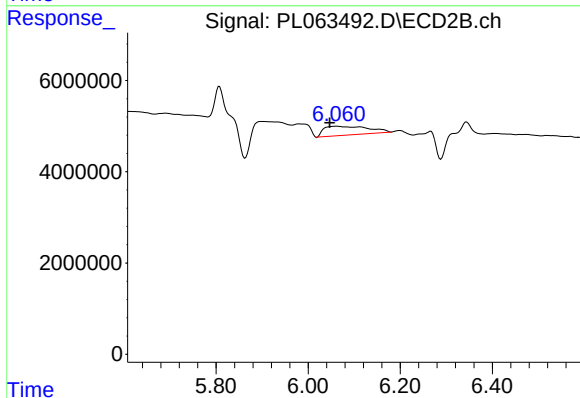


#25 Chlordane-3

R.T.: 6.061 min
Delta R.T.: 0.014 min
Response: 12985438
Conc: 28.18 ng/ml

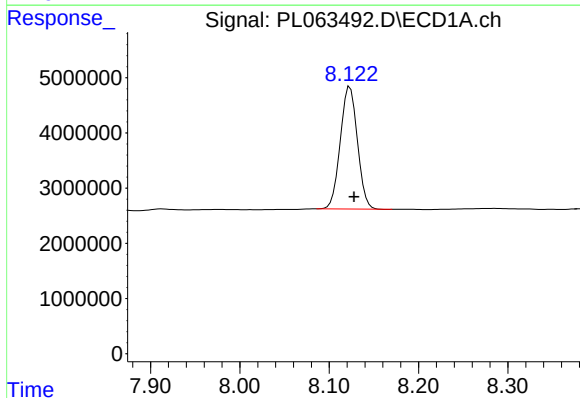

#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: -0.005 min
Response: 29497105
Conc: 14.65 ng/ml

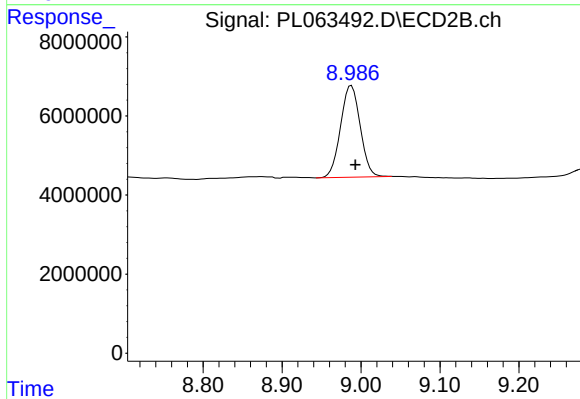

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 40127086
Conc: 15.93 ng/ml