

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 11:22
 Operator : DD\AJ
 Sample : L4983-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 12:10:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.949	34304967	63466978	20.159	20.250
28)	SA Decachlor...	8.124	8.988	39037718	50984729	19.385	20.245
Target Compounds							
7)	B delta-BHC	0.000	5.002	0	5014875	N.D.	1.239 #
8)	B Heptachlo...	0.000	5.808	0	12063234	N.D.	3.331 #
10)	B gamma-Chl...	0.000	6.039	0	5996461	N.D.	1.690 #
13)	MA Dieldrin	5.676	0.000	4040198	0	2.219	N.D. #
14)	MA Endrin	5.937	0.000	8690733	0	5.178	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	3622625	N.D.	1.137 #
19)	B Endosulfa...	6.600f	0.000	44269537	0	25.814	N.D. #
25)	Chlordane-3	0.000	6.039	0	5996461	N.D.	13.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 11:22
Operator : DD\AJ
Sample : L4983-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 12:10:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

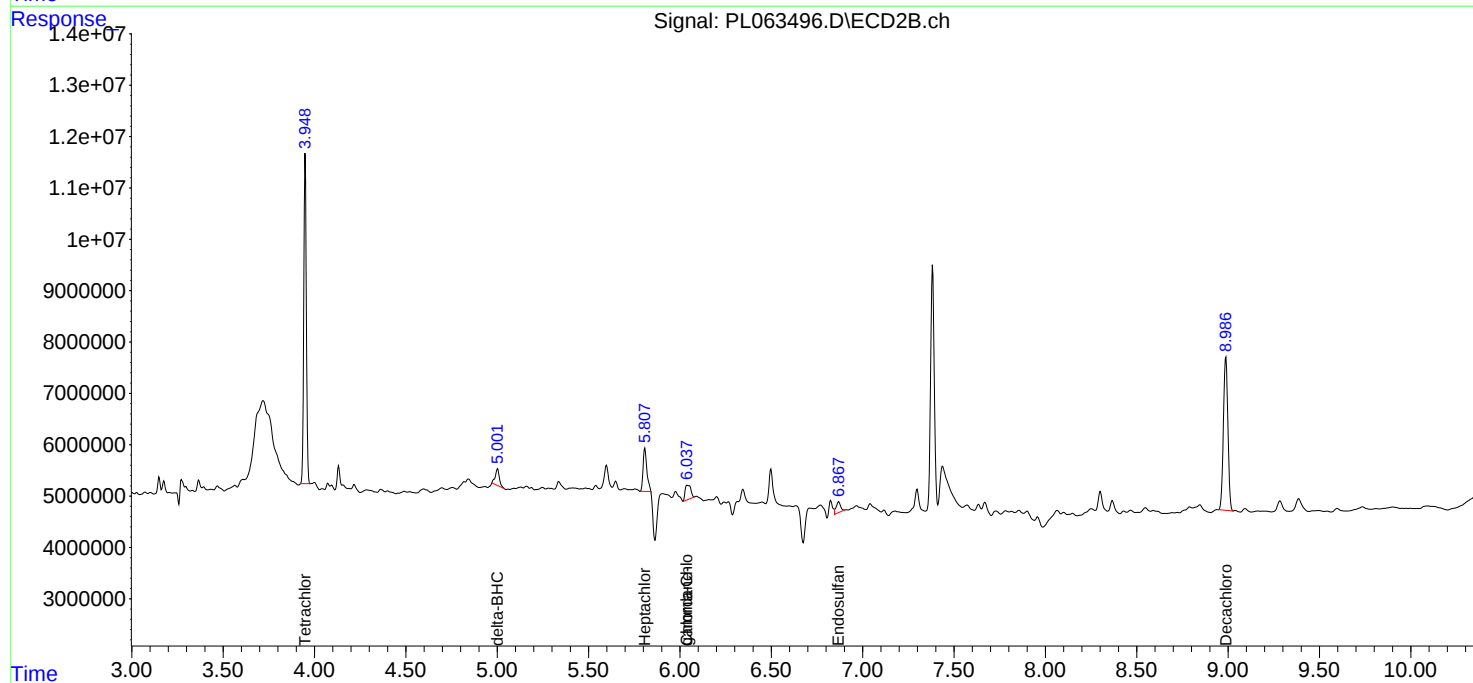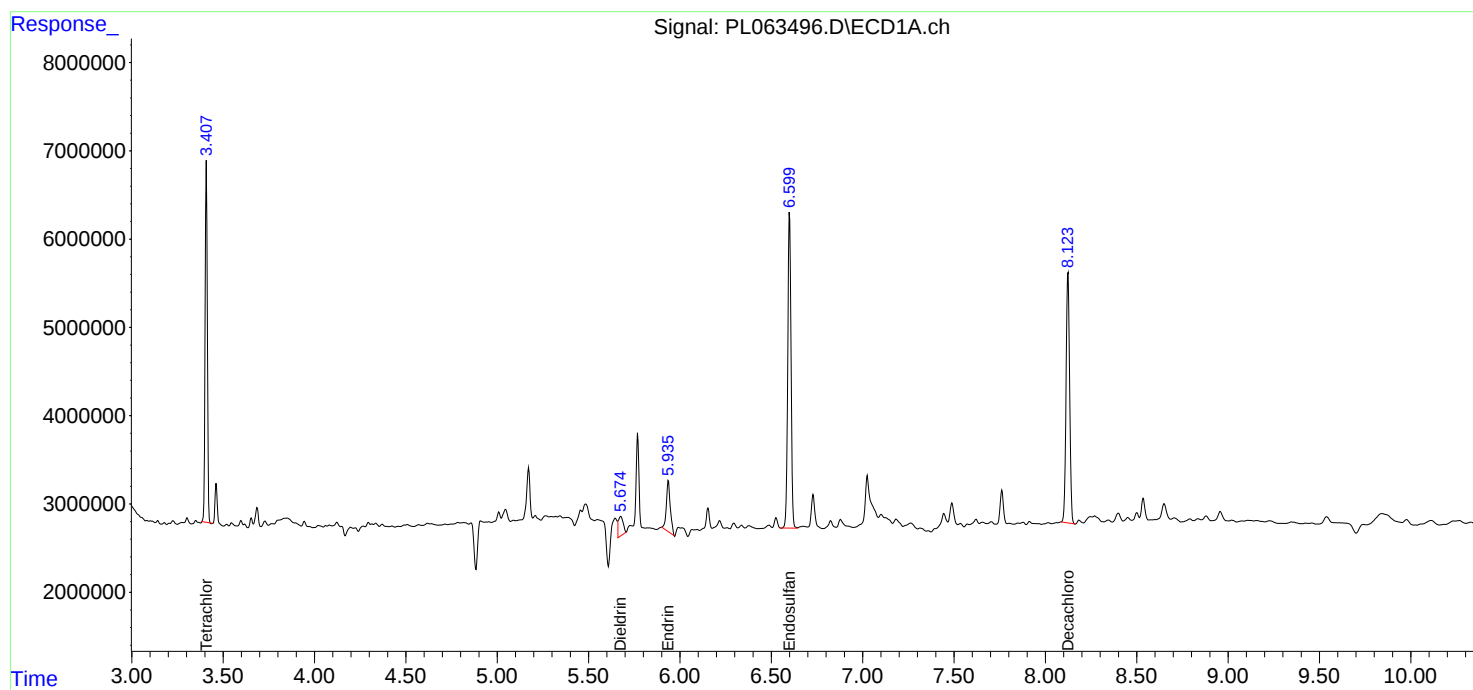


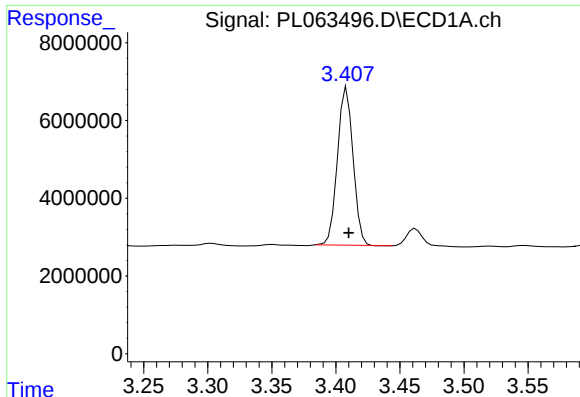

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: -0.001 min
Response: 34304967
Conc: 20.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

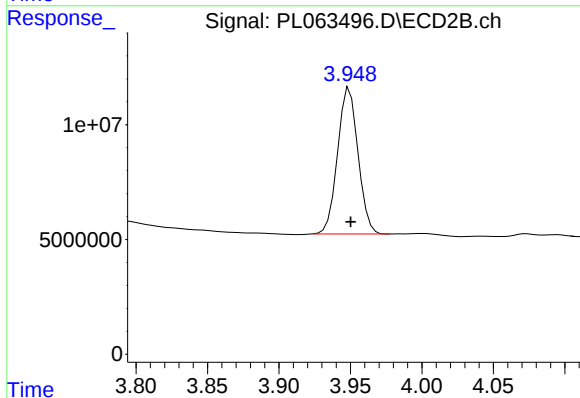


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 63466978
Conc: 20.25 ng/ml

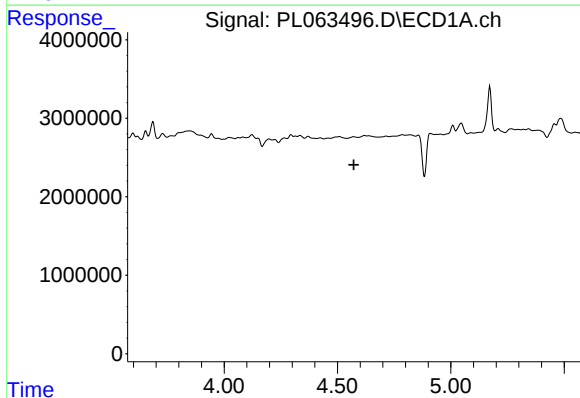


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

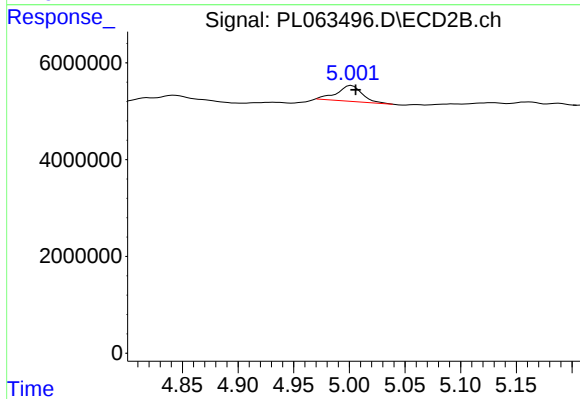

#7 delta-BHC


R.T.: 5.002 min
Delta R.T.: -0.004 min
Response: 5014875
Conc: 1.24 ng/ml

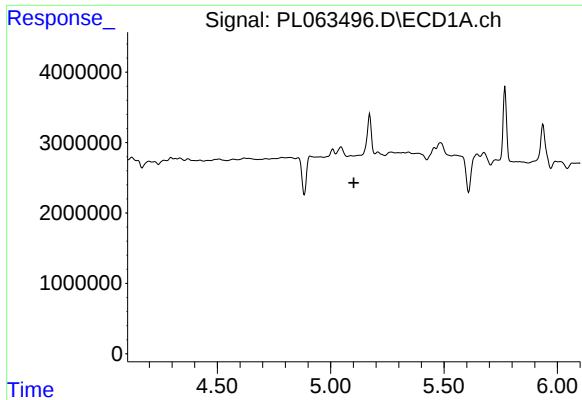

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

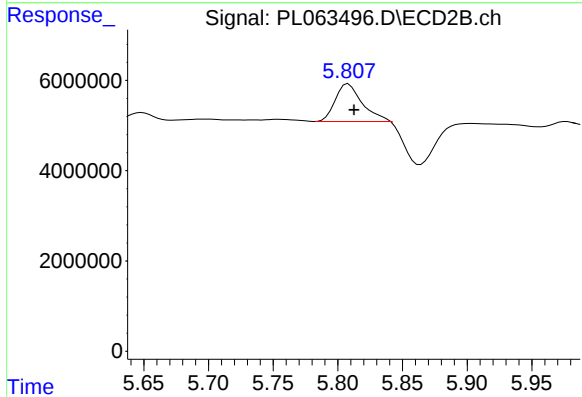


#8 Heptachlor epoxide

R.T.: 5.808 min
Delta R.T.: -0.005 min
Response: 12063234
Conc: 3.33 ng/ml

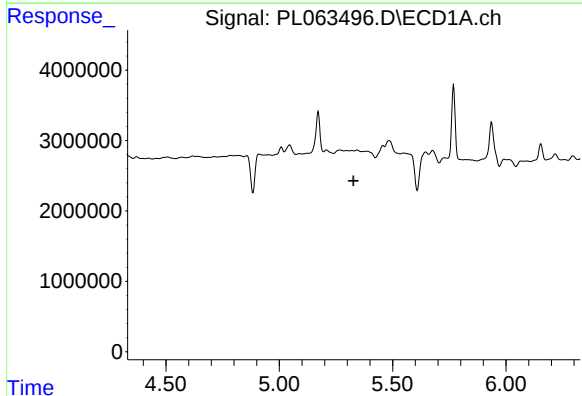


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

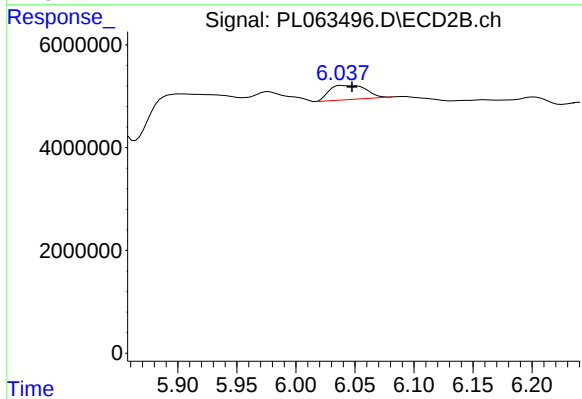

#10 gamma-Chlordane


R.T.: 6.039 min
Delta R.T.: -0.009 min
Response: 5996461
Conc: 1.69 ng/ml

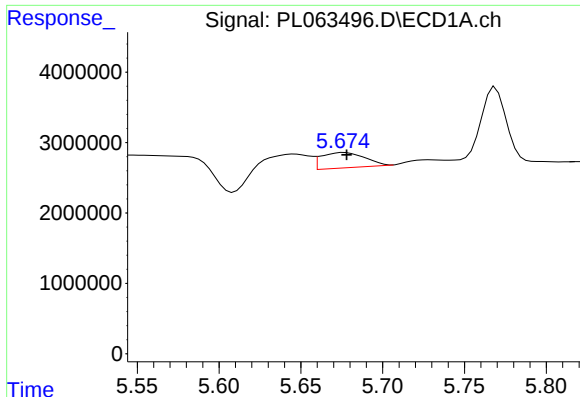

#13 Dieldrin


R.T.: 5.676 min
Delta R.T.: -0.002 min
Response: 4040198
Conc: 2.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

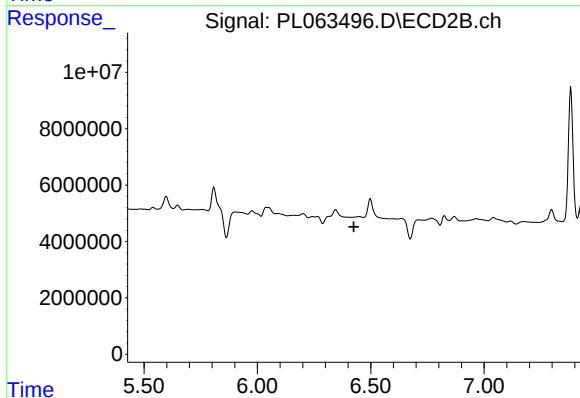


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.426 min
Response: 0
Conc: N.D.

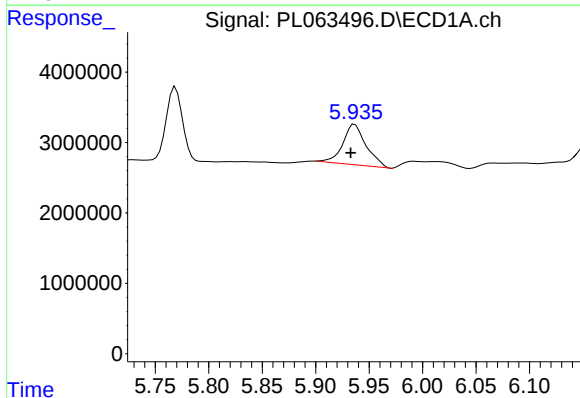


#14 Endrin

R.T.: 5.937 min
Delta R.T.: 0.004 min
Response: 8690733
Conc: 5.18 ng/ml

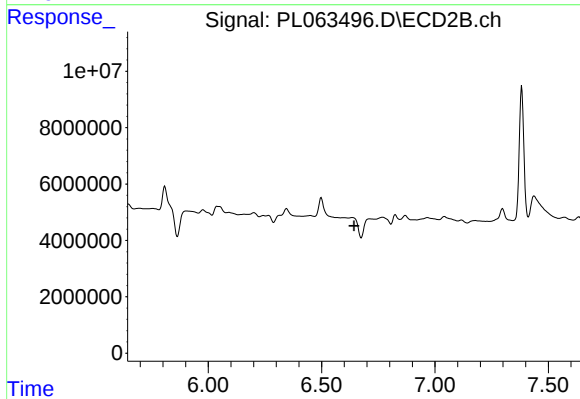

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

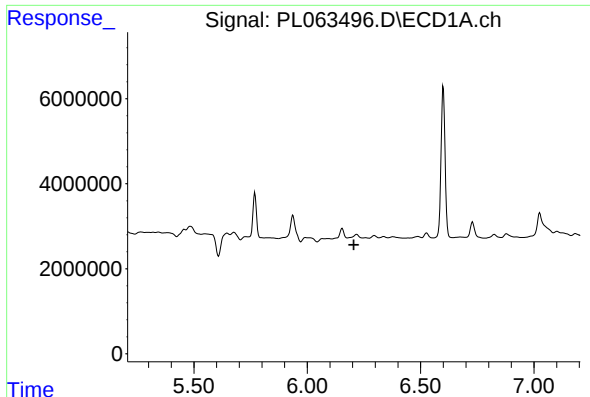

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

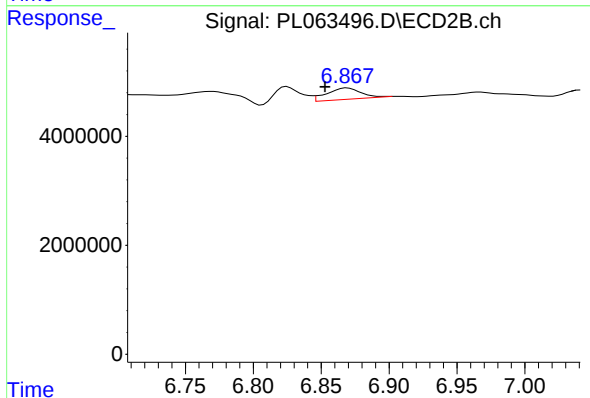


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 3622625
Conc: 1.14 ng/ml

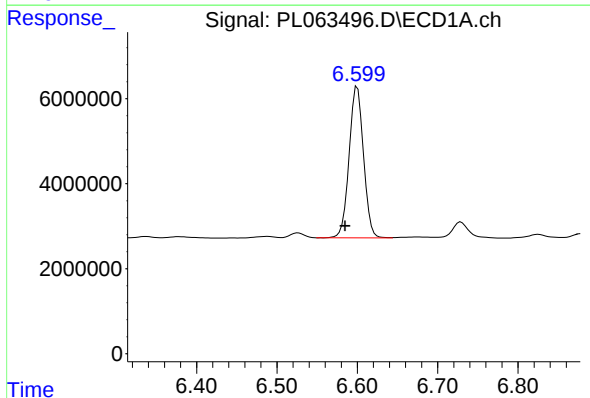


#19 Endosulfan Sulfate

R.T.: 6.600 min
Delta R.T.: 0.015 min
Response: 44269537
Conc: 25.81 ng/ml

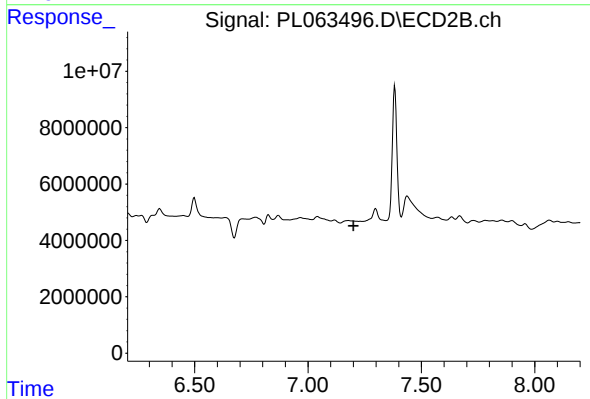

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.201 min
Response: 0
Conc: N.D.

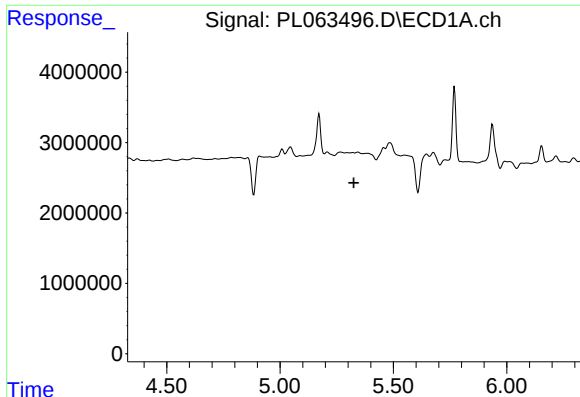

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.326 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

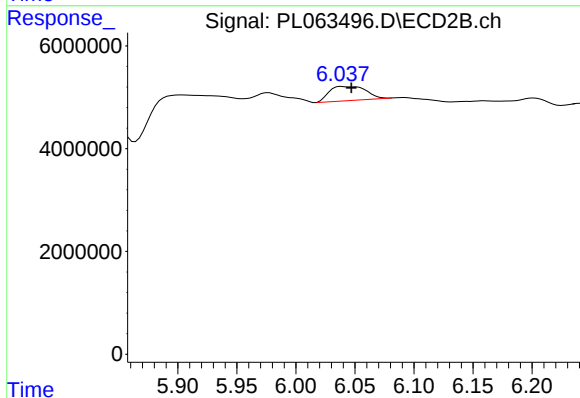


#25 Chlordane-3

R.T.: 6.039 min
Delta R.T.: -0.008 min
Response: 5996461
Conc: 13.01 ng/ml

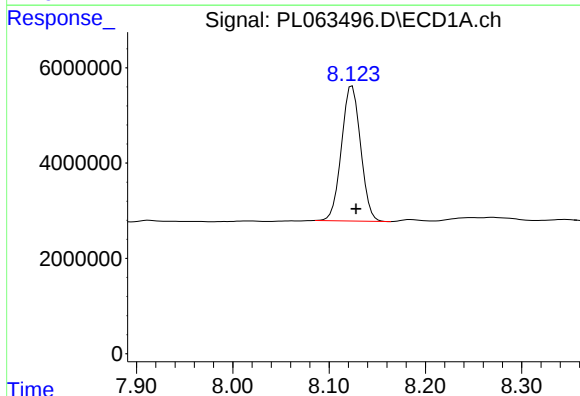

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 39037718
Conc: 19.38 ng/ml

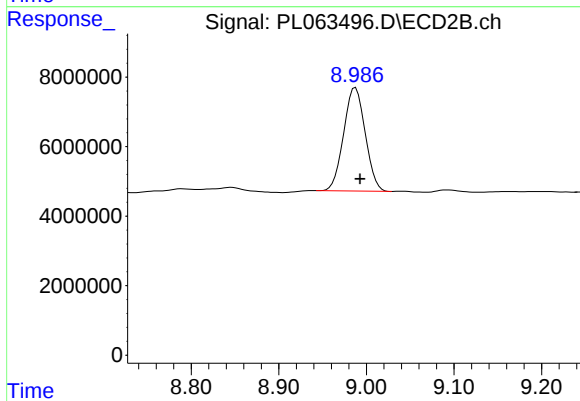

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 50984729
Conc: 20.25 ng/ml