

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 16:37
 Operator : DD\AJ
 Sample : L5033-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-48

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:42:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.409	3.949	26914708	41553615	15.816	13.258
28) SA	Decachlor...	8.124	8.988	27886411	37868471	13.847	15.037
Target Compounds							
8) B	Heptachlo...	0.000	5.826	0	2636897	N.D.	0.728 #
15) B	Endosulfa...	0.000	6.865	0	4608962	N.D.	1.447 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 16:37
Operator : DD\AJ
Sample : L5033-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-48

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:42:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

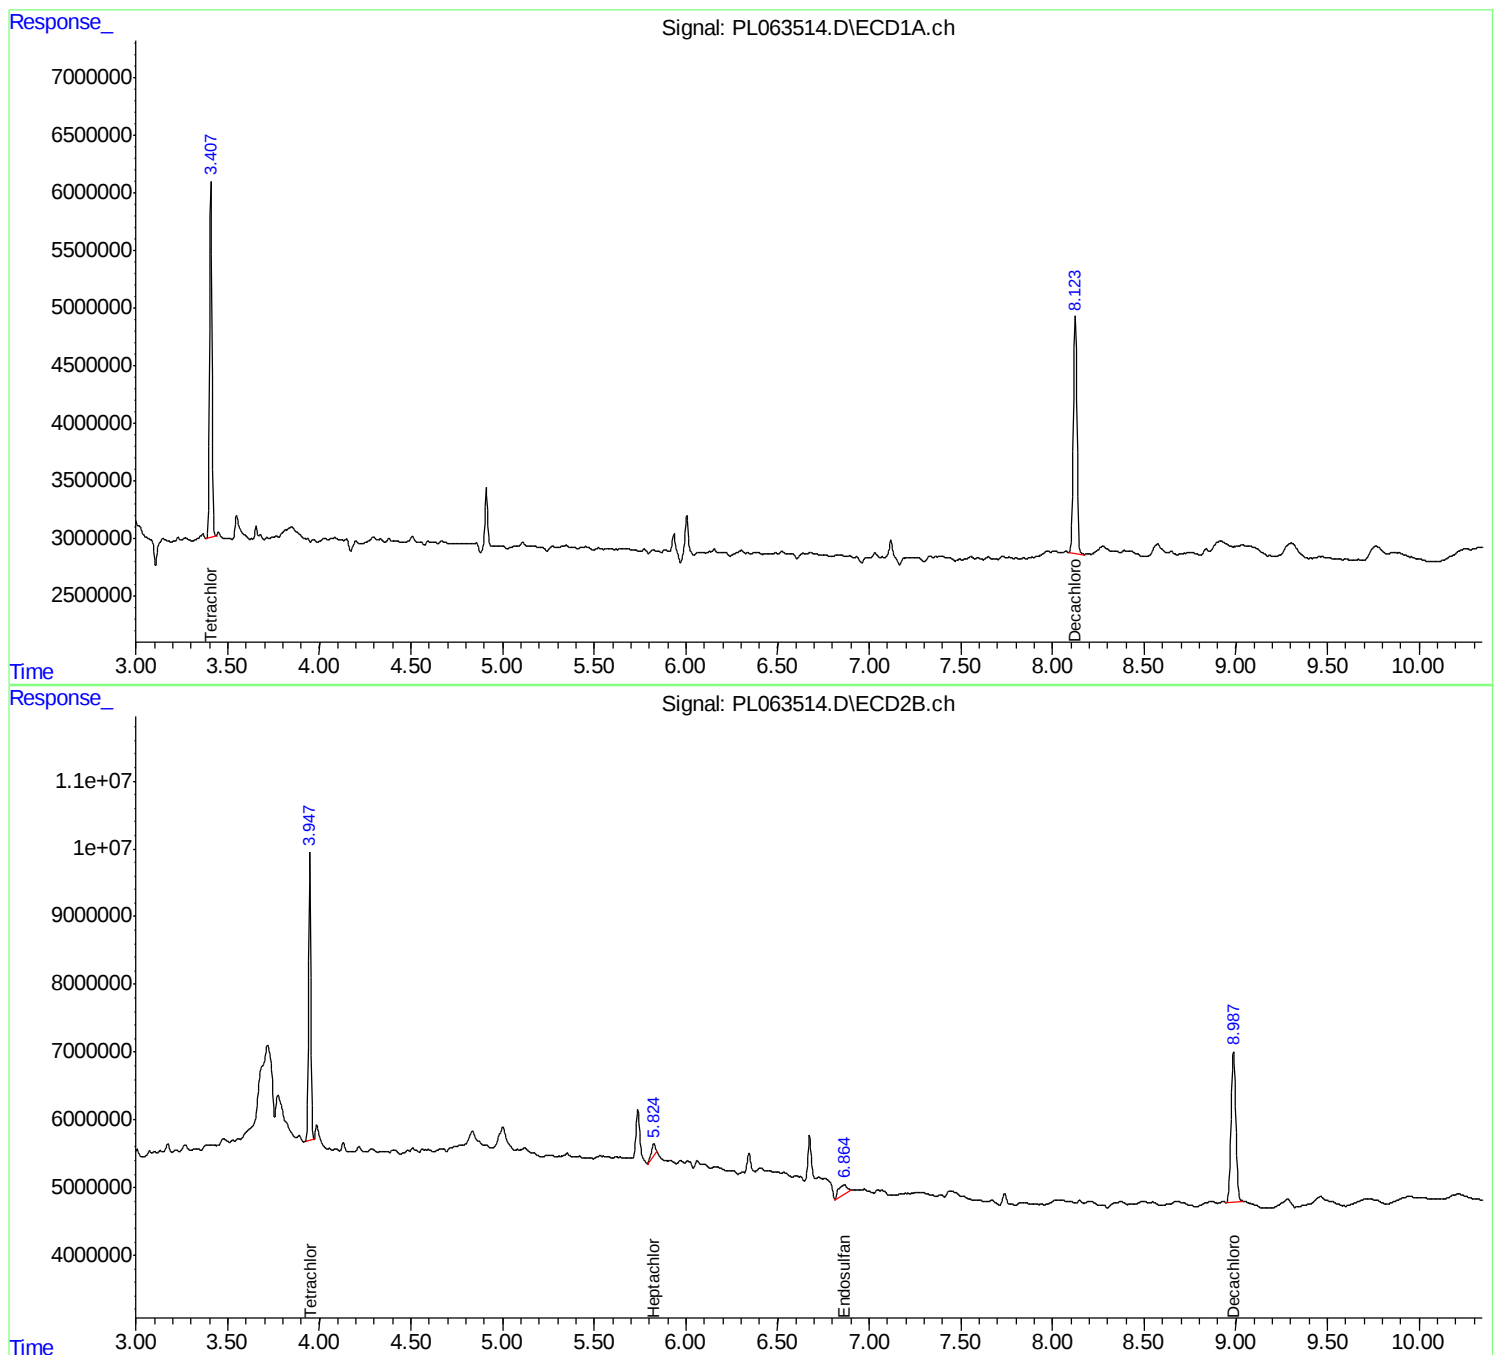


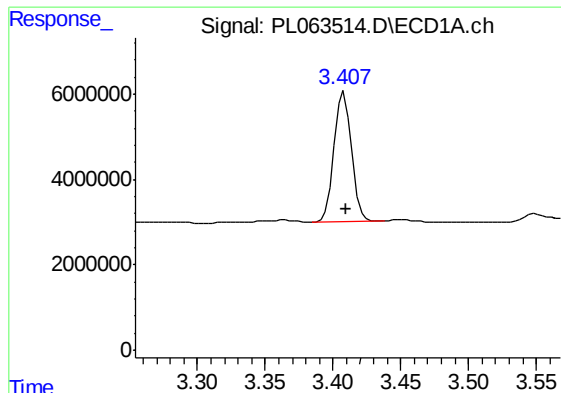

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: -0.001 min
Response: 26914708
Conc: 15.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-48

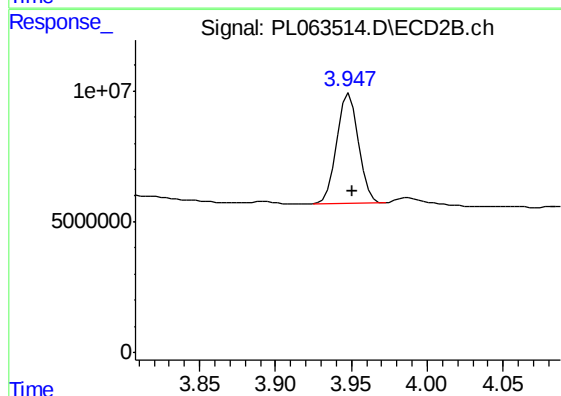


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 41553615
Conc: 13.26 ng/ml

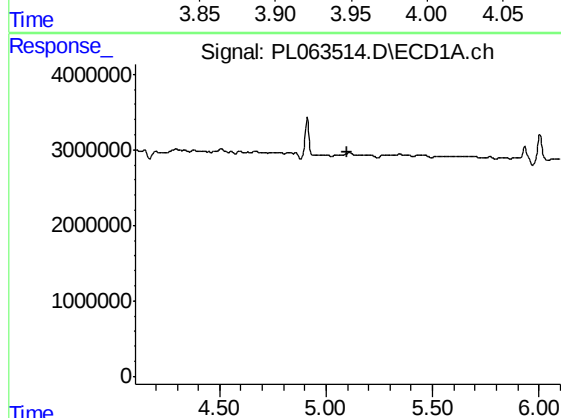


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

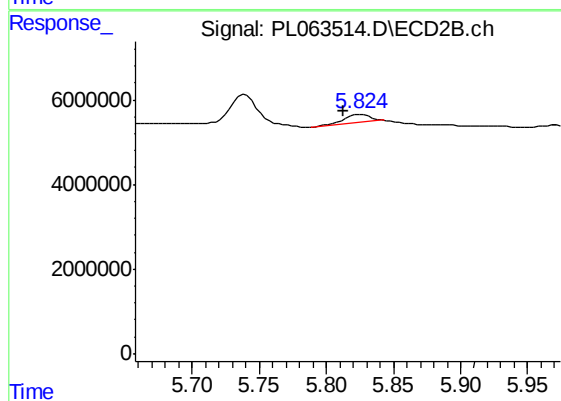

#8 Heptachlor epoxide


R.T.: 5.826 min
Delta R.T.: 0.013 min
Response: 2636897
Conc: 0.73 ng/ml

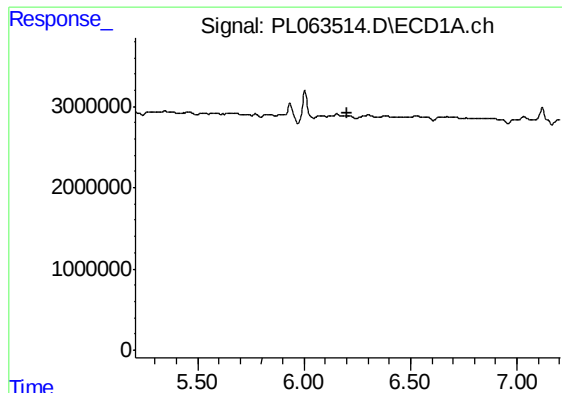

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-48

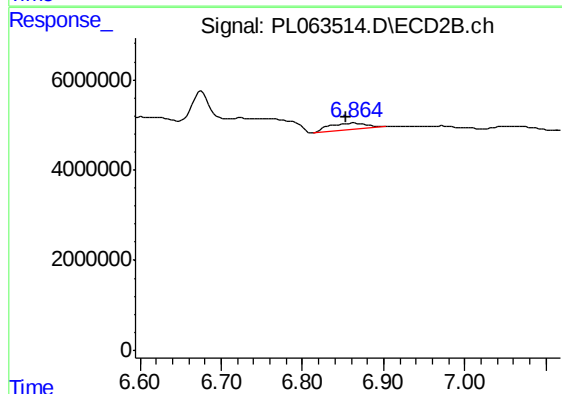


#15 Endosulfan II

R.T.: 6.865 min
Delta R.T.: 0.012 min
Response: 4608962
Conc: 1.45 ng/ml

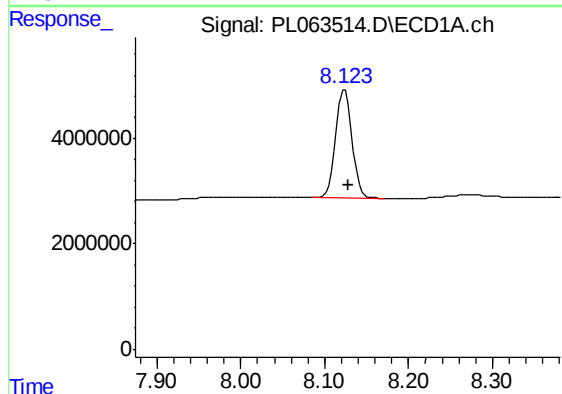

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 27886411
Conc: 13.85 ng/ml

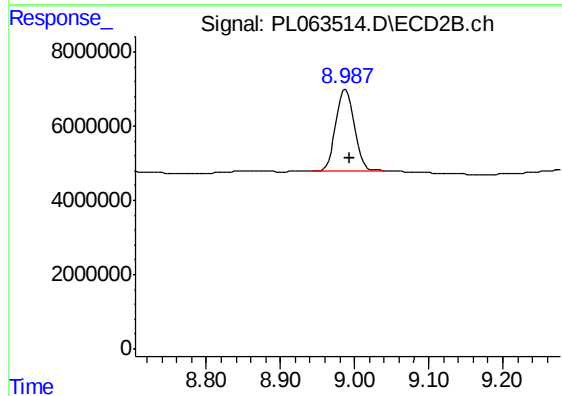

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 37868471
Conc: 15.04 ng/ml