

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 16:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:42:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	3.949	44223671	72394411	25.988	23.098
28) SA Decachlor...	8.125	8.989	41340377	57165786	20.528	22.700
Target Compounds						
8) B Heptachlo...	0.000	5.810	0	4921832	N.D.	1.359 #
14) MA Endrin	5.935	0.000	4907590	0	2.924	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 16:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:42:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

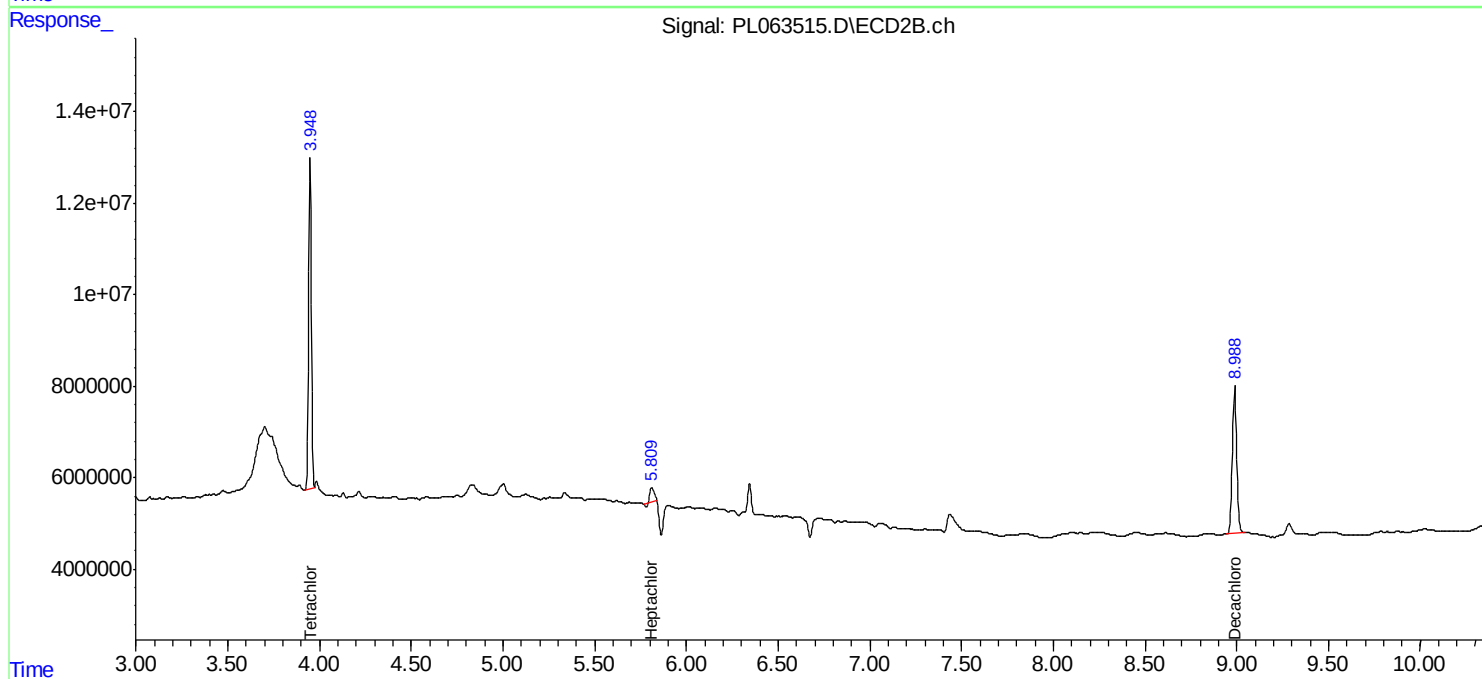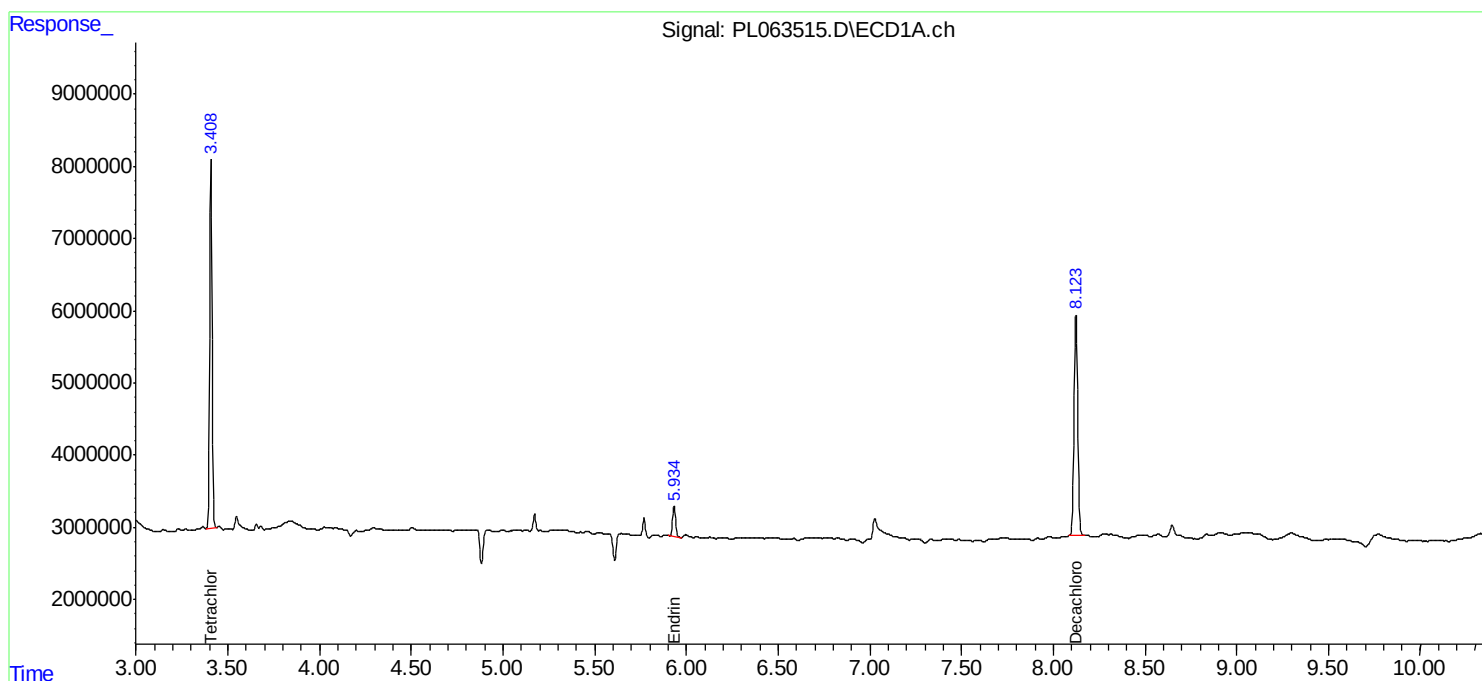


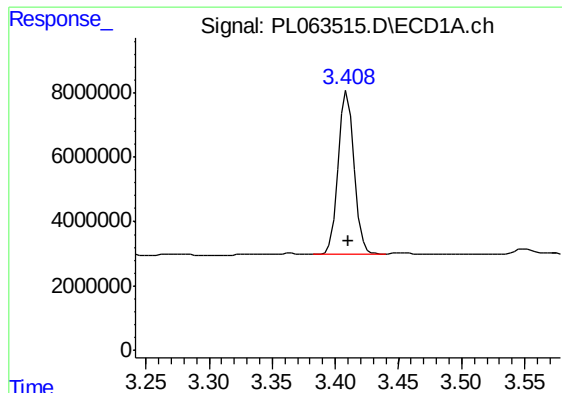

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 44223671
Conc: 25.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

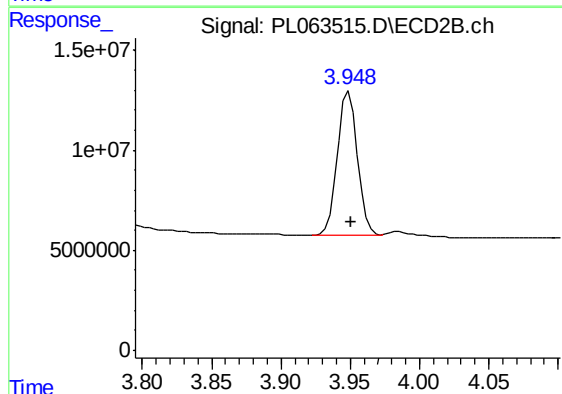


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 72394411
Conc: 23.10 ng/ml

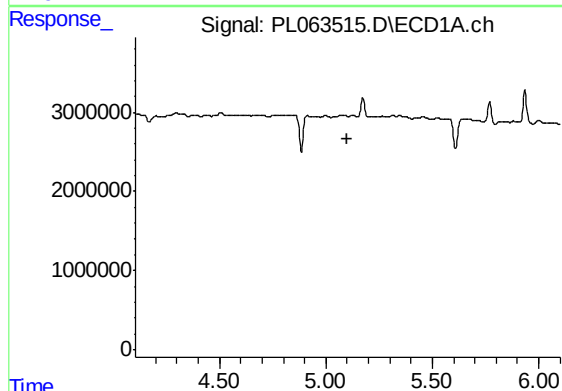


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

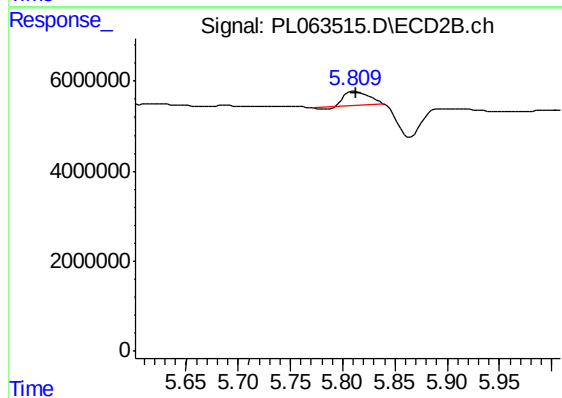

#8 Heptachlor epoxide


R.T.: 5.810 min
Delta R.T.: -0.002 min
Response: 4921832
Conc: 1.36 ng/ml

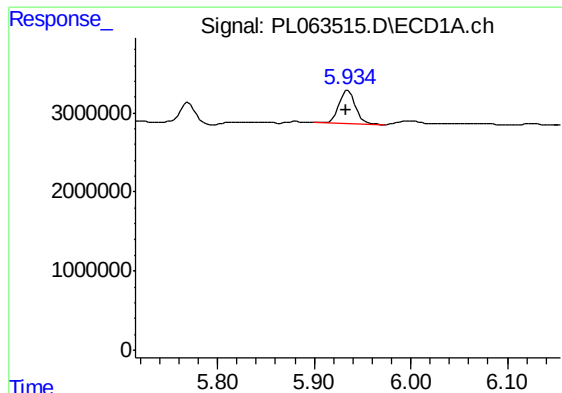

#14 Endrin


R.T.: 5.935 min
Delta R.T.: 0.002 min
Response: 4907590
Conc: 2.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

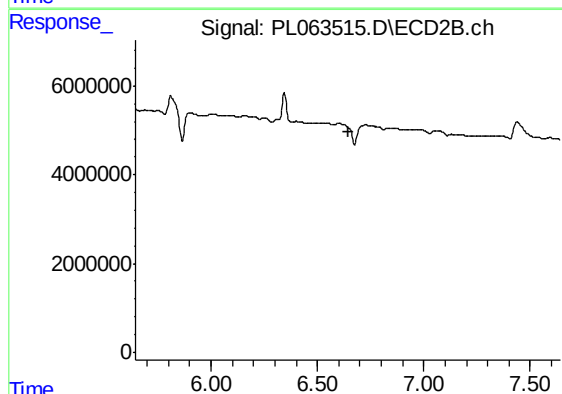


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

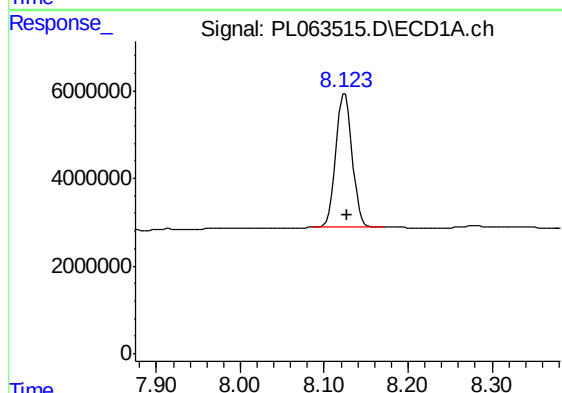

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 41340377
Conc: 20.53 ng/ml

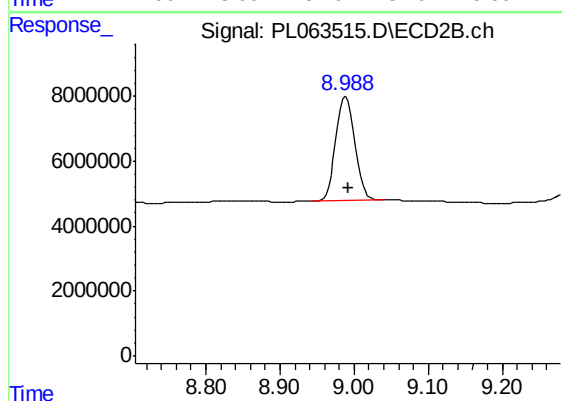

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 57165786
Conc: 22.70 ng/ml