

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 10:11
 Operator : DD\AJ
 Sample : L4973-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-120820

Manual Integrations
 APPROVED

Ankita
 12/14/2020 4:21:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 12:09:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.408	3.949	23020785	39446318	13.528	12.586
28)	SA Decachlor...	8.123	8.988	24885612	33068782	12.357	13.131
Target Compounds							
17)	MA 4,4'-DDT	6.295	7.064	2258377	5260226	1.646m	2.057 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 10:11
Operator : DD\AJ
Sample : L4973-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-01-120820


Manual Integrations
APPROVED

Ankita
12/14/2020 4:21:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 12:09:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

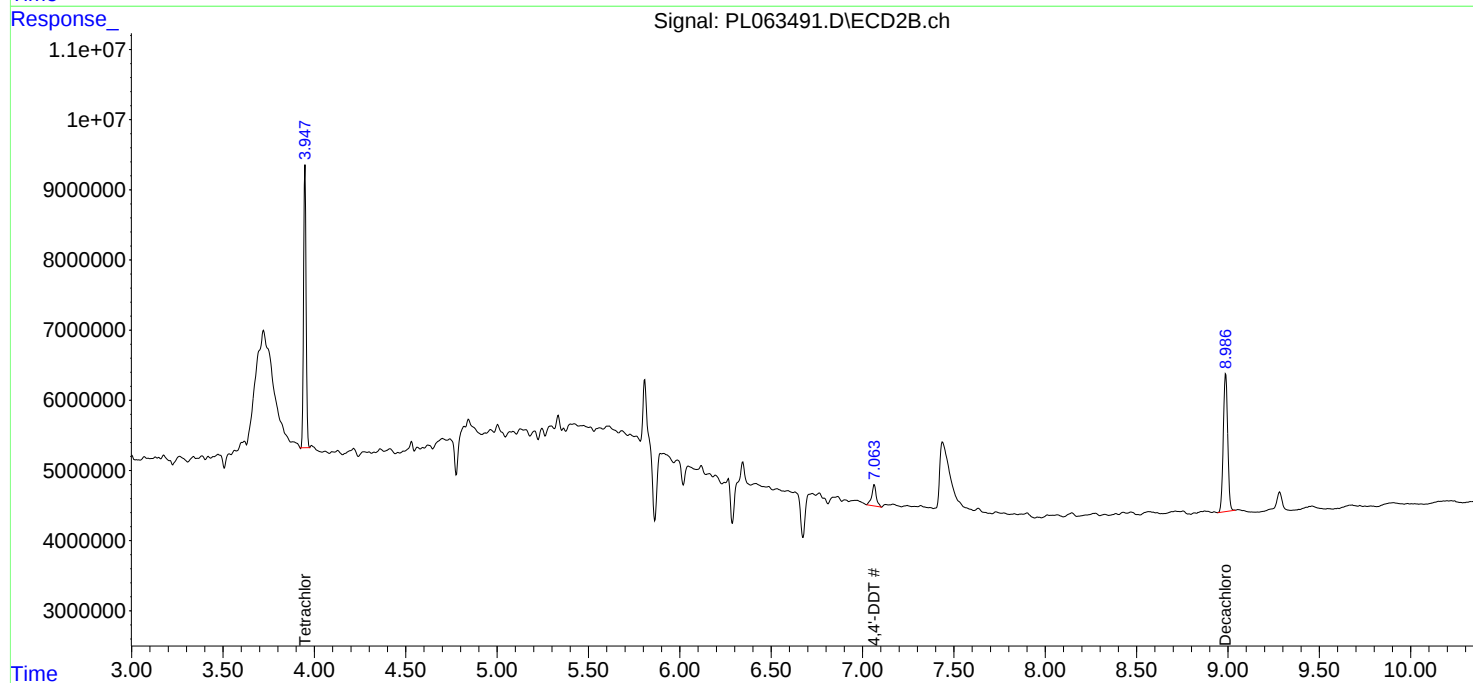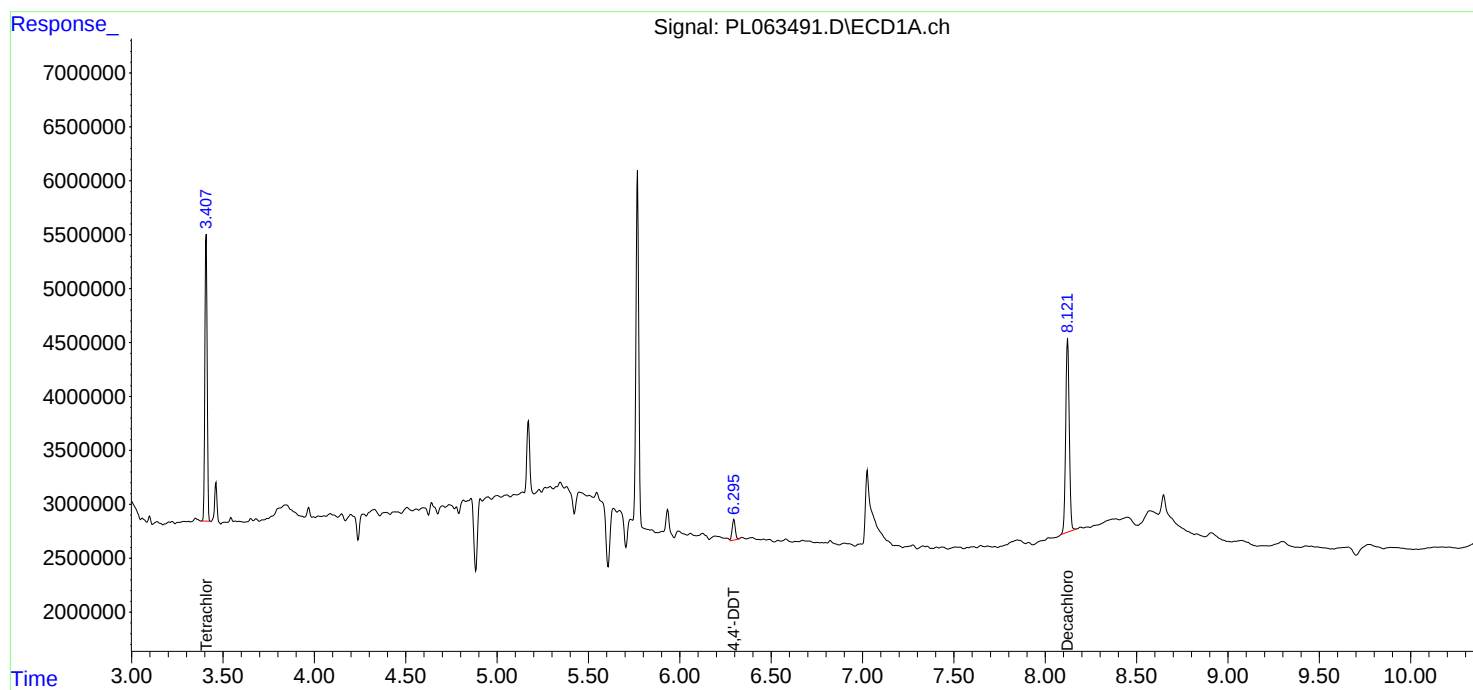

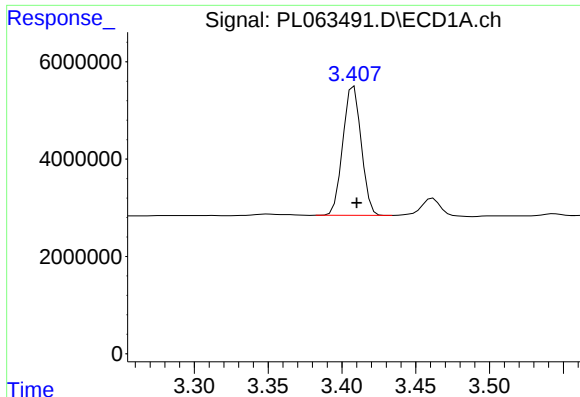


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: -0.002 min
Response: 23020785
Conc: 13.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-120820


Manual Integrations
APPROVED

Ankita
12/14/2020 4:21:57 PM

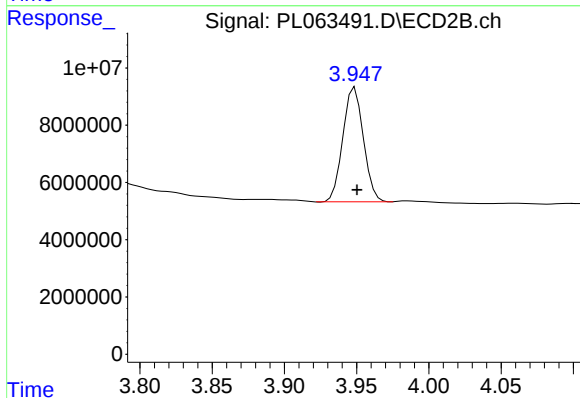


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 39446318
Conc: 12.59 ng/ml

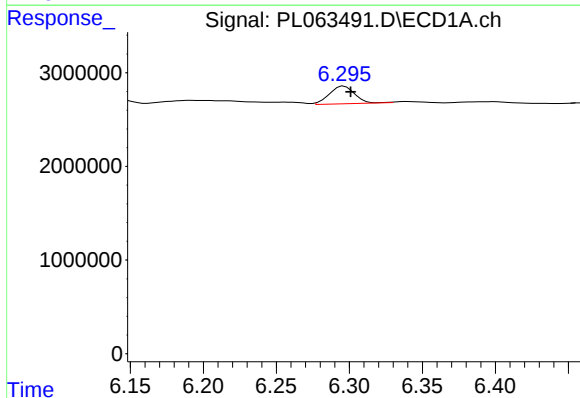


#17 4,4'-DDT

R.T.: 6.295 min
Delta R.T.: -0.006 min
Response: 2258377
Conc: 1.65 ng/ml m

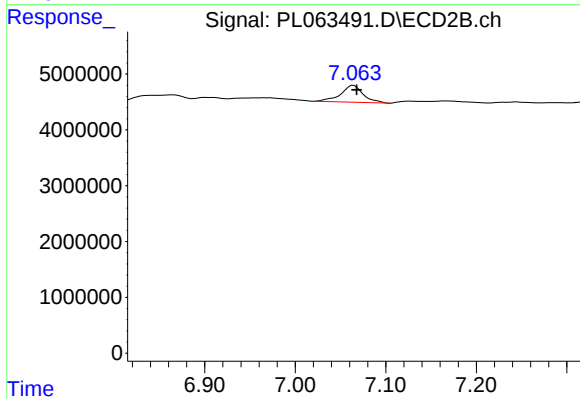

#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: -0.003 min
Response: 5260226
Conc: 2.06 ng/ml

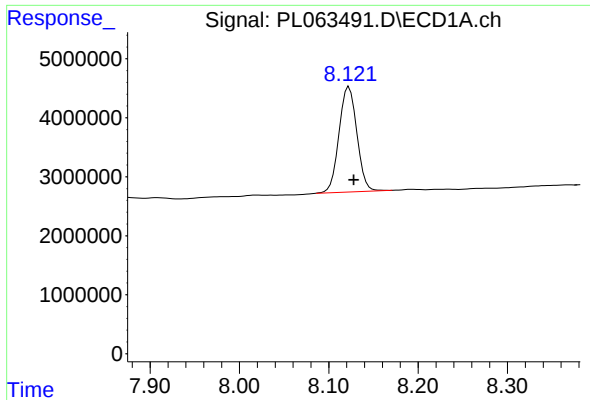


#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: -0.005 min
Response: 24885612
Conc: 12.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-120820

Manual Integrations
APPROVED

Ankita
12/14/2020 4:21:57 PM

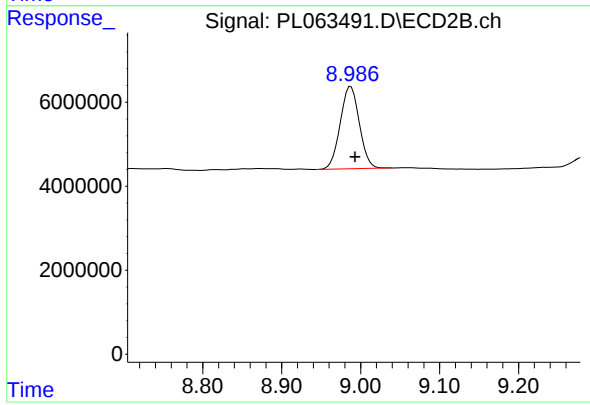

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.005 min
Response: 33068782
Conc: 13.13 ng/ml