

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 11:37
 Operator : DD\AJ
 Sample : L4983-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR2-A-D-COMP

Manual Integrations
 APPROVED

Ankita
 12/14/2020 4:22:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:04:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.408	3.949	37627223	67435352	22.111	21.516
28) SA Decachlor...	8.124	8.987	41422828	54602383	20.569	21.682
Target Compounds						
12) B 4,4'-DDE	5.546	6.275	2664208	5725234	1.569m	1.635
17) MA 4,4'-DDT	6.297	7.063	5444445	7094601	3.968	2.775 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 11:37
Operator : DD\AJ
Sample : L4983-12
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/14/2020 4:22:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:04:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

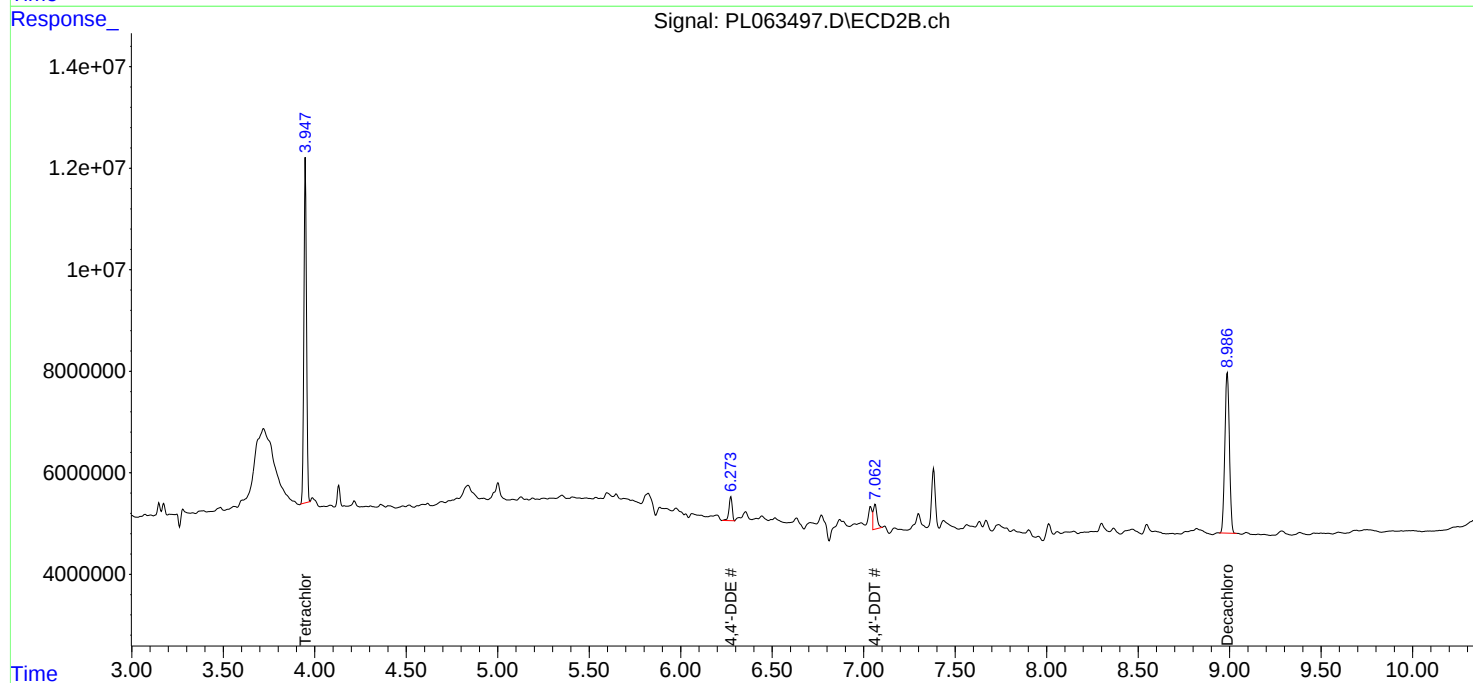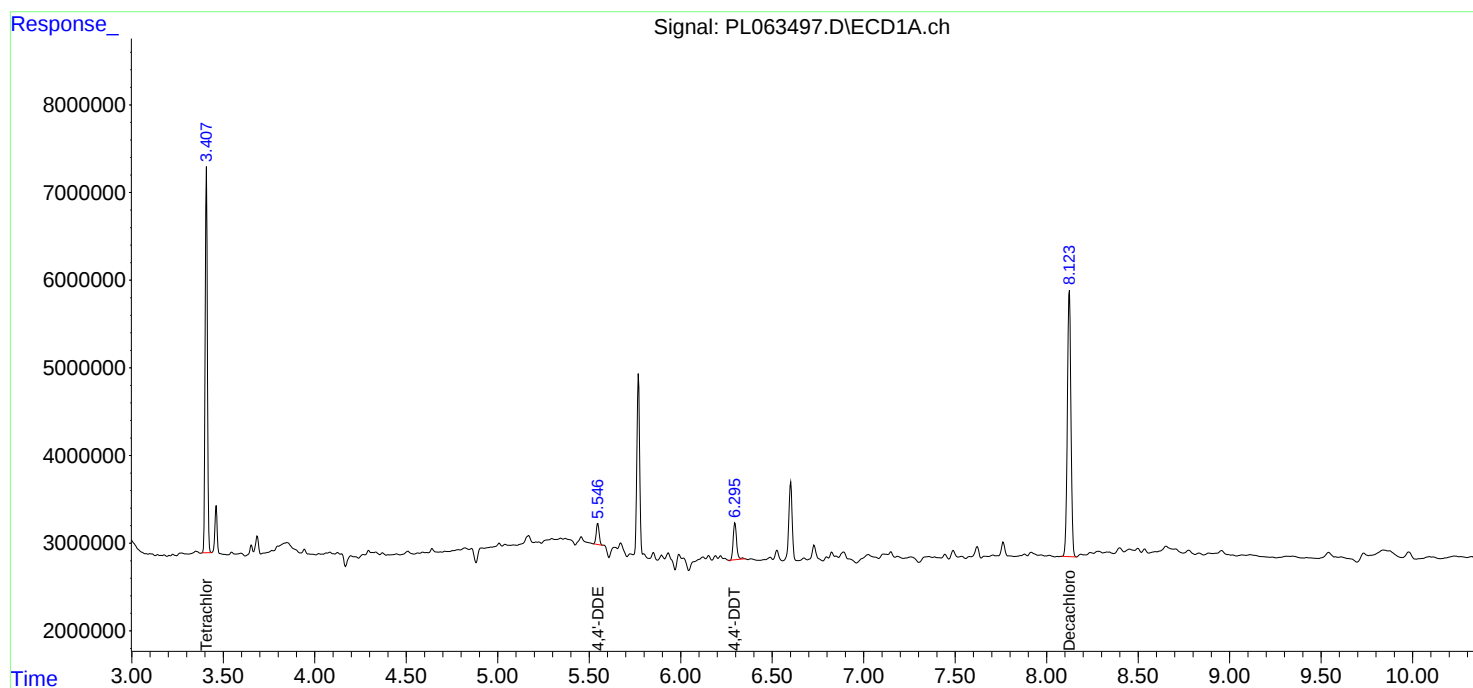

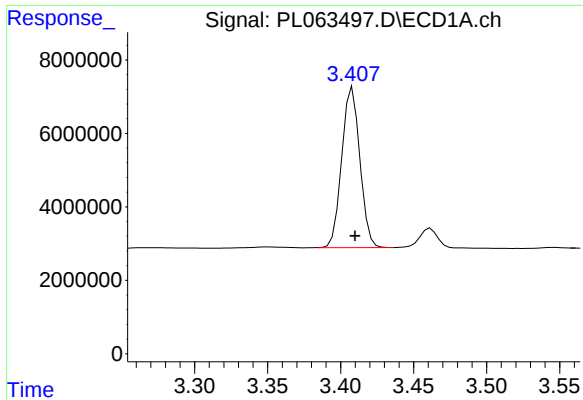


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: -0.002 min
Response: 37627223
Conc: 22.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/14/2020 4:22:05 PM

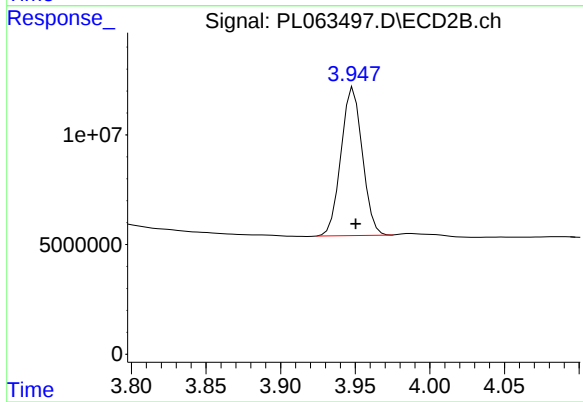


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 67435352
Conc: 21.52 ng/ml

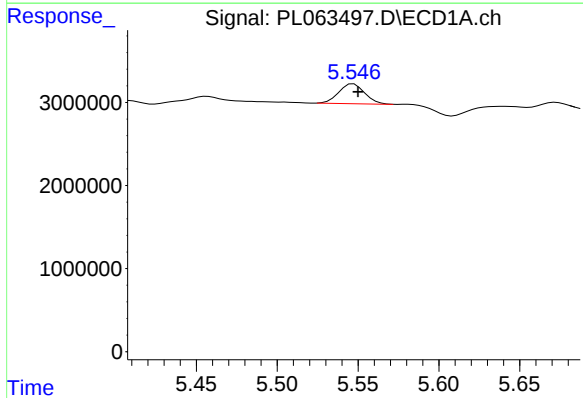


#12 4,4'-DDE

R.T.: 5.546 min
Delta R.T.: -0.004 min
Response: 2664208
Conc: 1.57 ng/ml m

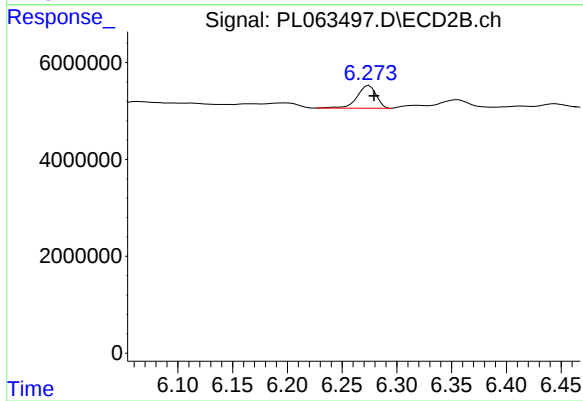

#12 4,4'-DDE

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 5725234
Conc: 1.63 ng/ml

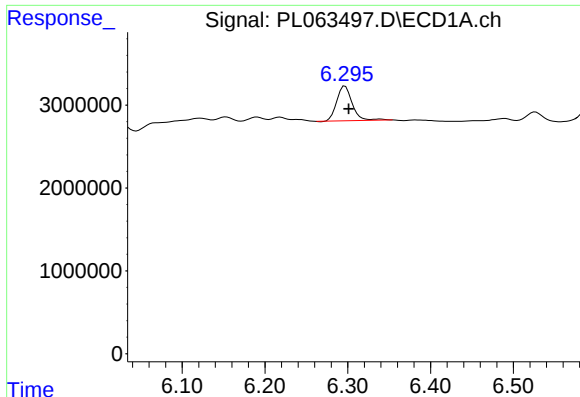


#17 4,4'-DDT

R.T.: 6.297 min
Delta R.T.: -0.004 min
Response: 5444445
Conc: 3.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/14/2020 4:22:05 PM

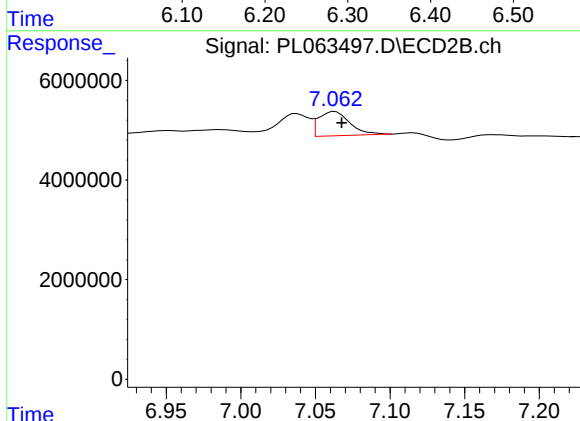


#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: -0.005 min
Response: 7094601
Conc: 2.77 ng/ml

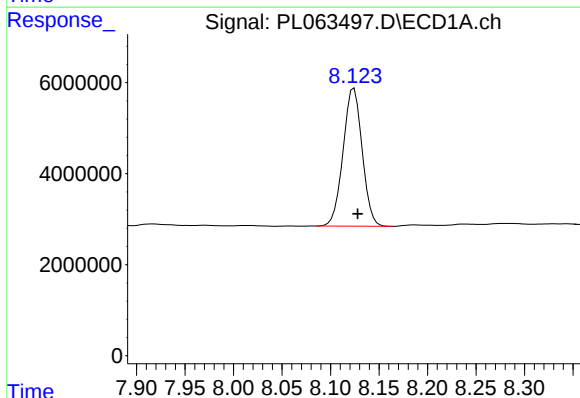

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.004 min
Response: 41422828
Conc: 20.57 ng/ml

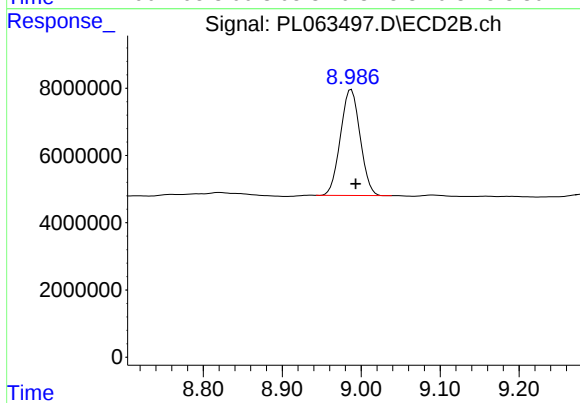

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: -0.005 min
Response: 54602383
Conc: 21.68 ng/ml