

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
 Data File : PL063512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2020 16:09
 Operator : DD\AJ
 Sample : L5015-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-121020

Manual Integrations
 APPROVED

Ankita
 12/14/2020 4:22:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 16:35:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 15:57:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.949	21547250	32987886	12.662	10.525
28)	SA Decachlor...	8.125	8.989	24007433	34246922	11.921	13.599
Target Compounds							
12)	B 4,4'-DDE	5.548	6.275	5754621	12515936	3.388	3.574
17)	MA 4,4'-DDT	6.297	7.064	2111311	3651164	1.539m	1.428m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121220\
Data File : PL063512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2020 16:09
Operator : DD\AJ
Sample : L5015-02
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-05-121020


Manual Integrations
APPROVED

Ankita
12/14/2020 4:22:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 16:35:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 15:57:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

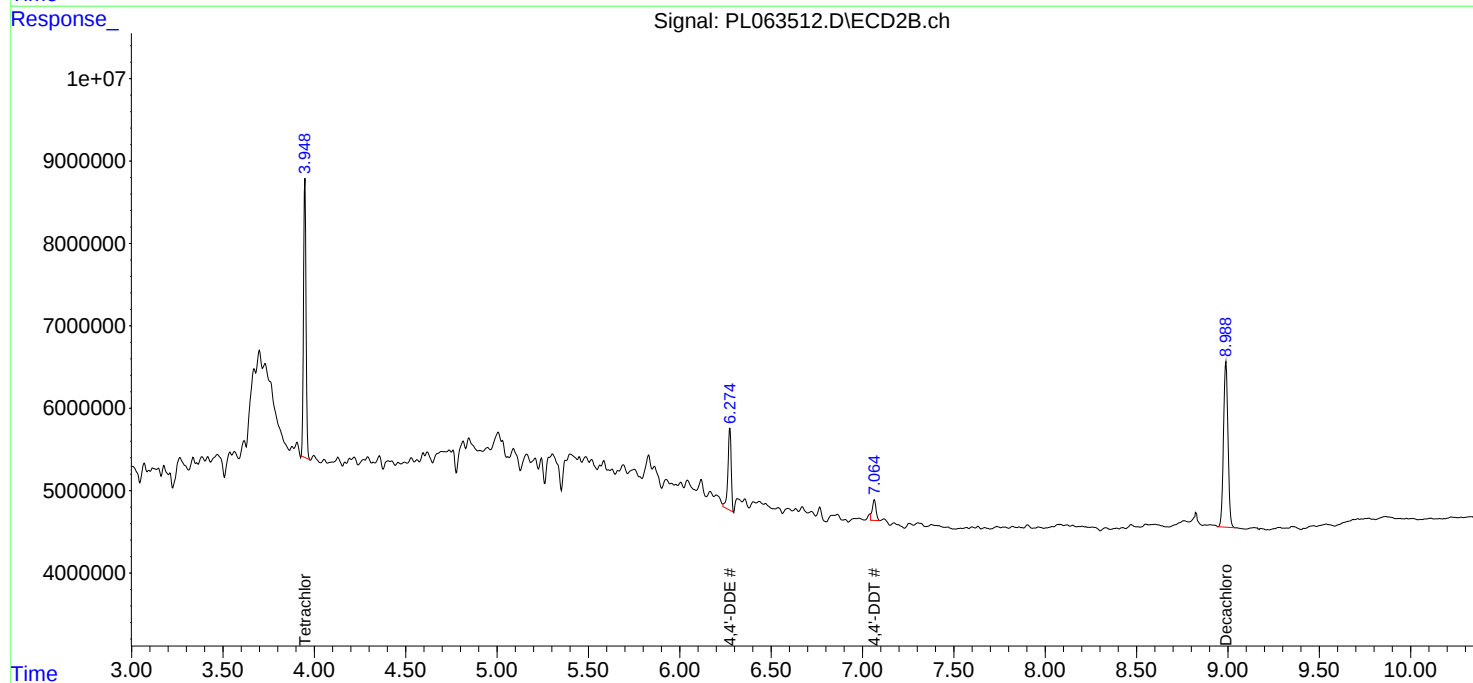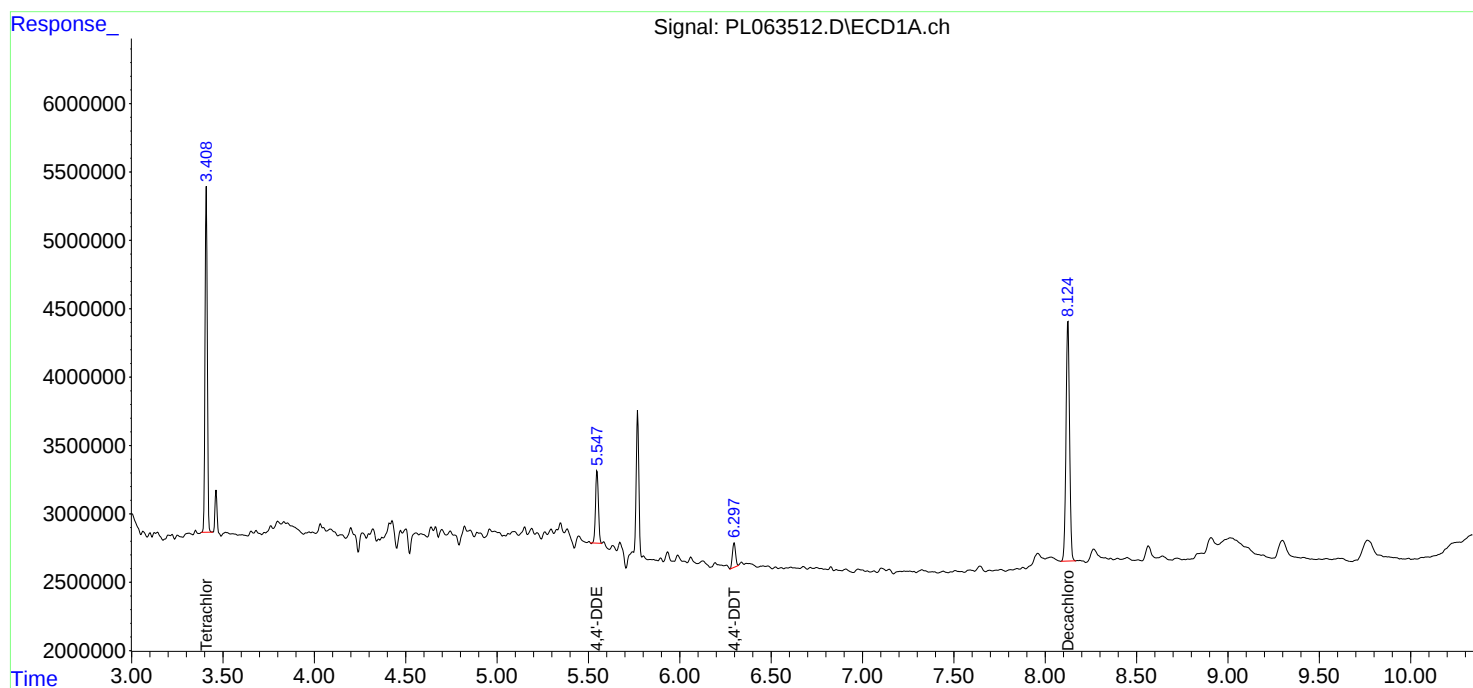

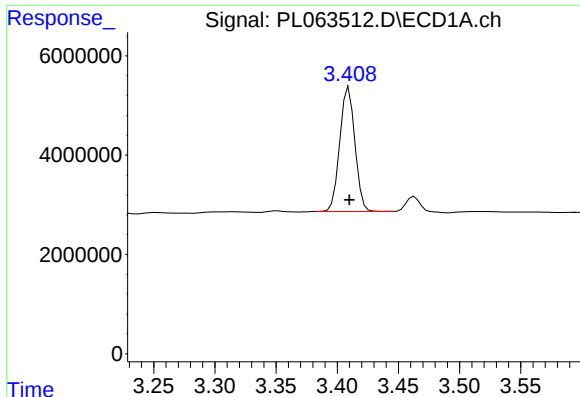


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 21547250
Conc: 12.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-121020


Manual Integrations
APPROVED

Ankita
12/14/2020 4:22:11 PM

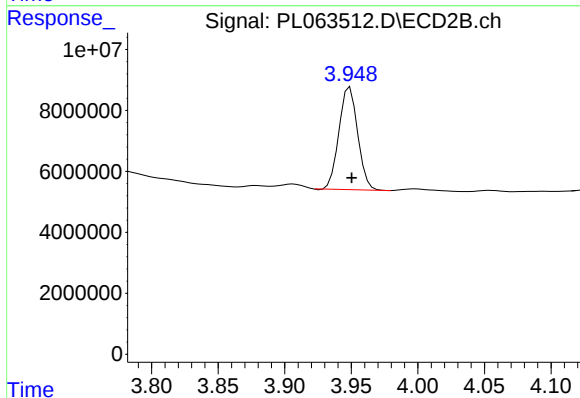


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 32987886
Conc: 10.53 ng/ml

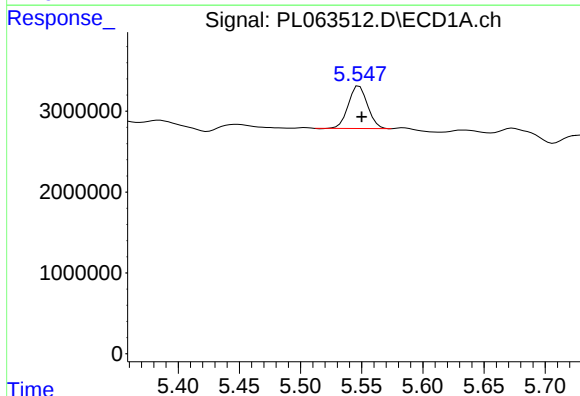


#12 4,4'-DDE

R.T.: 5.548 min
Delta R.T.: -0.002 min
Response: 5754621
Conc: 3.39 ng/ml

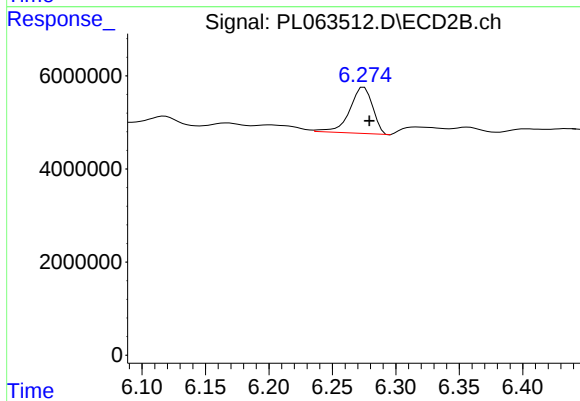

#12 4,4'-DDE

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 12515936
Conc: 3.57 ng/ml

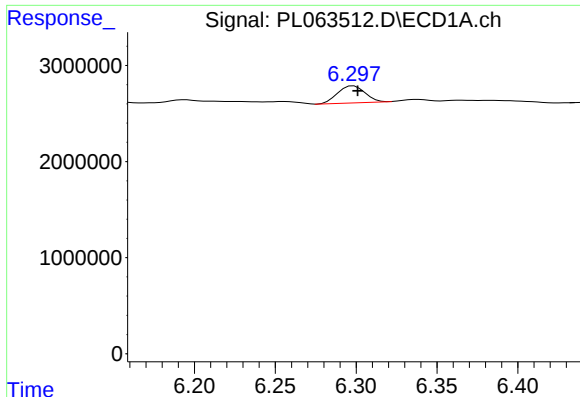


#17 4,4'-DDT

R.T.: 6.297 min
Delta R.T.: -0.004 min
Response: 2111311
Conc: 1.54 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-05-121020


Manual Integrations
APPROVED

Ankita
12/14/2020 4:22:11 PM

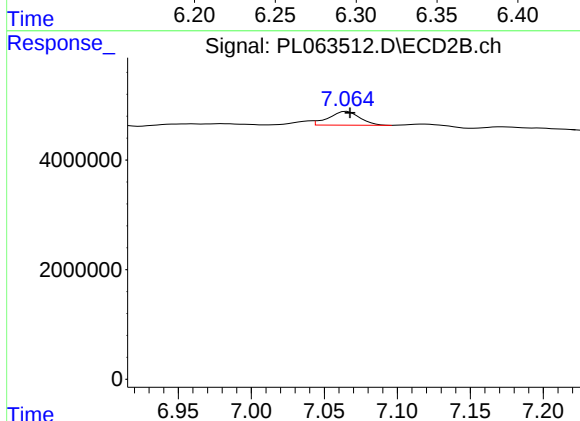


#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: -0.004 min
Response: 3651164
Conc: 1.43 ng/ml m

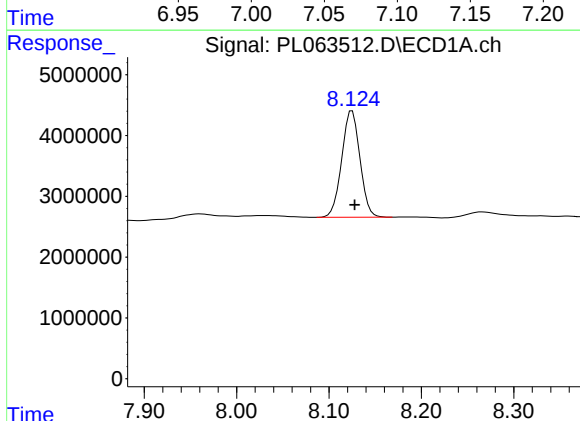

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 24007433
Conc: 11.92 ng/ml

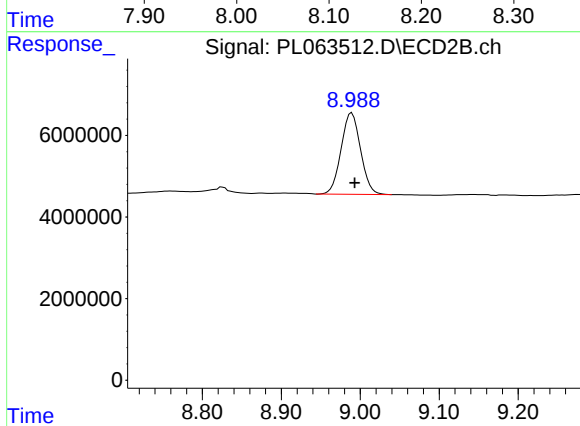

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.004 min
Response: 34246922
Conc: 13.60 ng/ml